

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072920\
 Data File : PP030728.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jul 2020 8:42
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 12:14:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072820.M
 Quant Title : 8080.M
 QLast Update : Wed Jul 29 01:54:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
5) T	DICAMBA	0.000	11.288	0	3919210	N.D. 2.278 #
7) T	MCPA	0.000	11.758	0	51951166	N.D. 25.501 #
15) T	Picloram	16.123	0.000	3163690	0	0.862 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072920\
Data File : PP030728.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jul 2020 8:42
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 12:14:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072820.M
Quant Title : 8080.M
QLast Update : Wed Jul 29 01:54:31 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

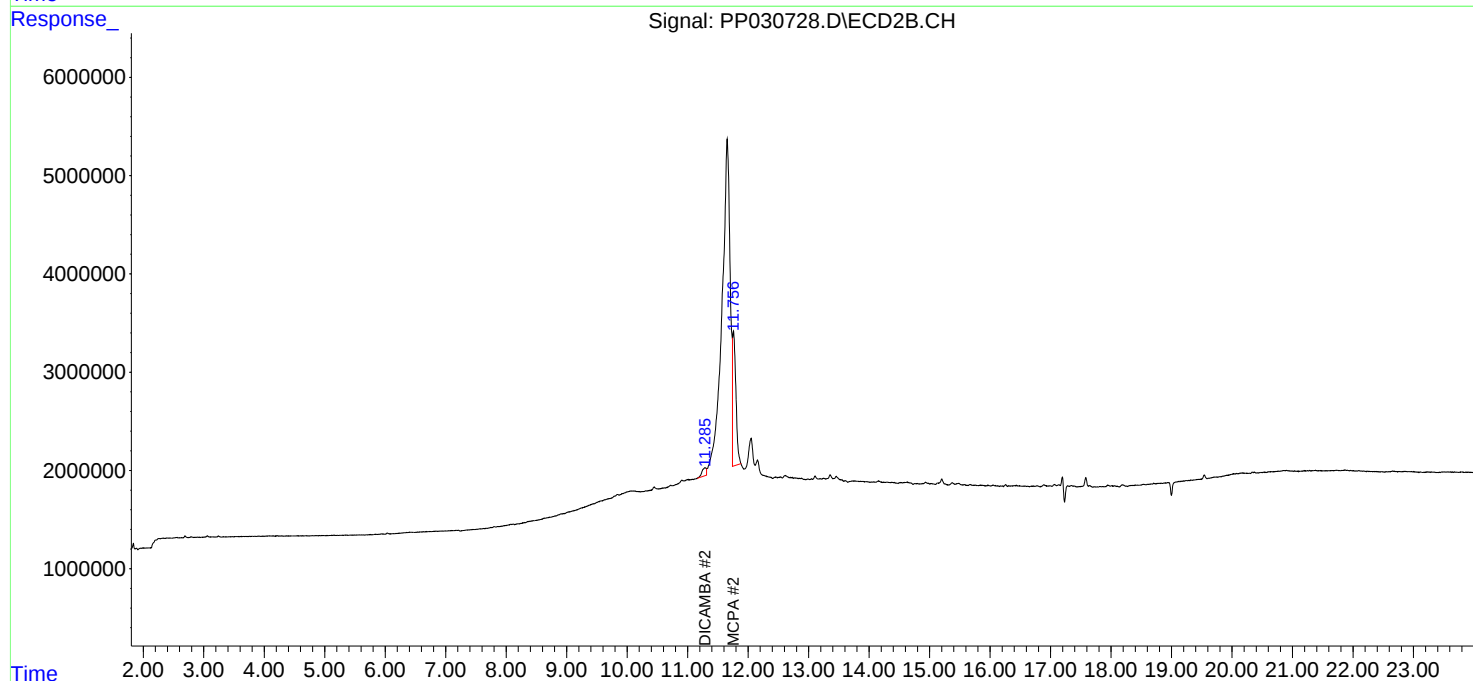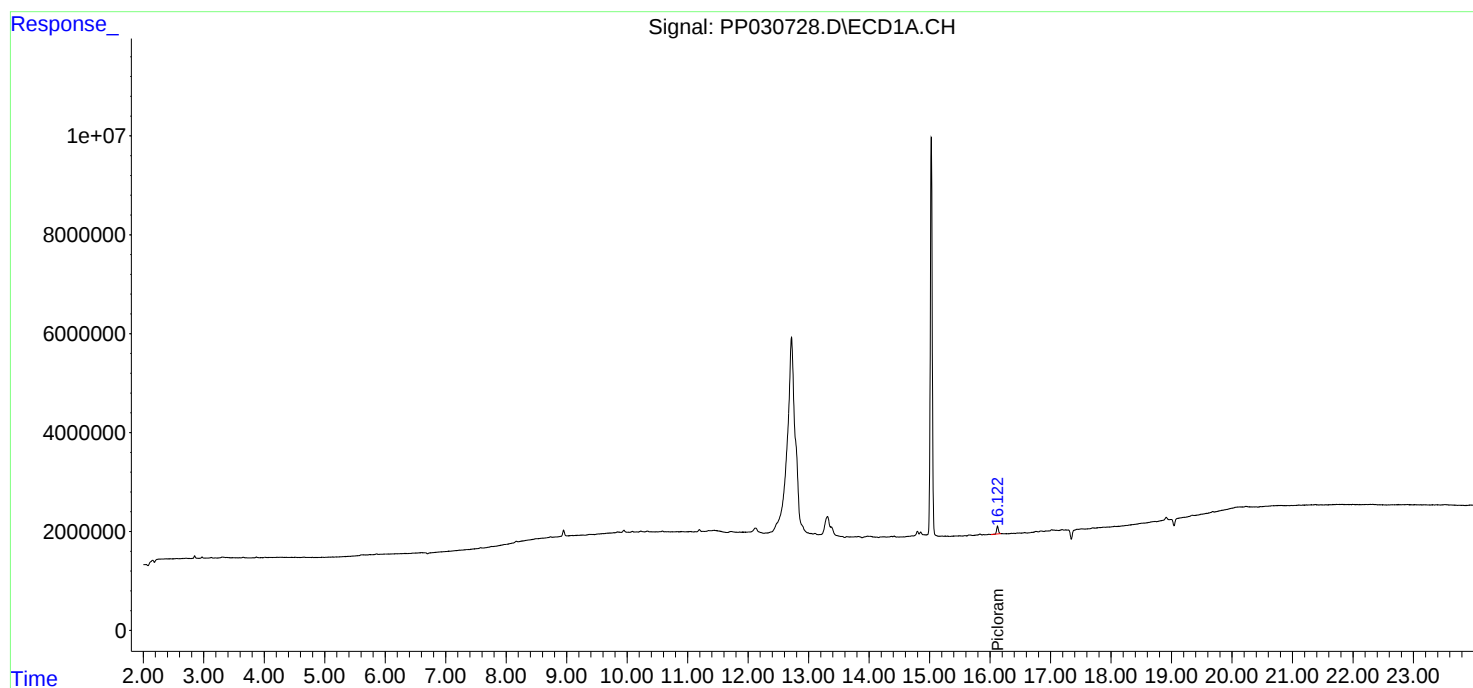


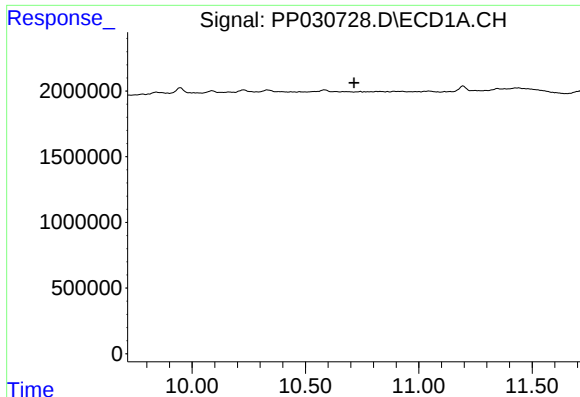

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 10.715 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

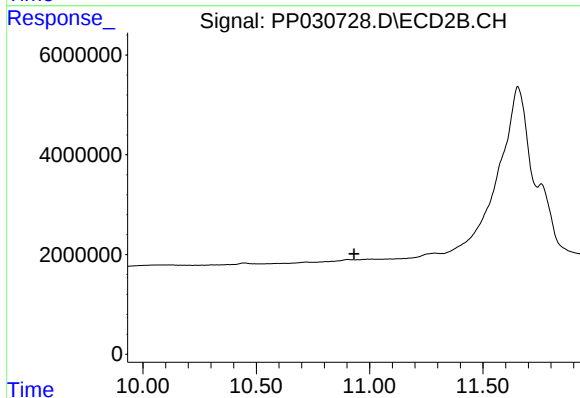


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 10.931 min
Response: 0
Conc: N.D.

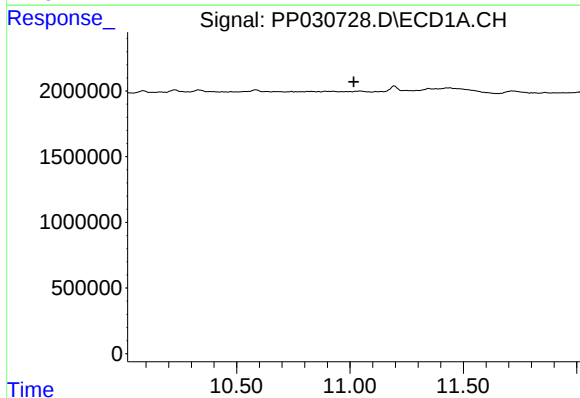


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.017 min
Response: 0
Conc: N.D.

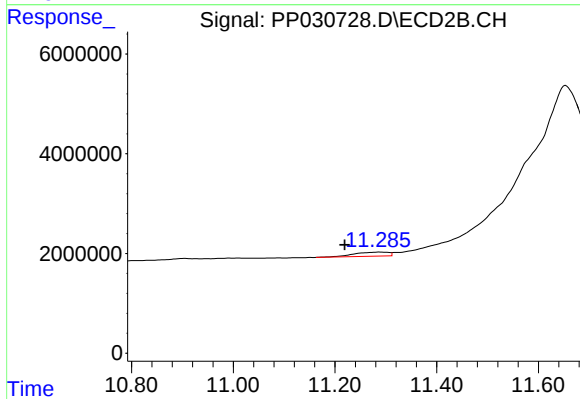

#5 DICAMBA


R.T.: 11.288 min
Delta R.T.: 0.068 min
Response: 3919210
Conc: 2.28 ng/ml

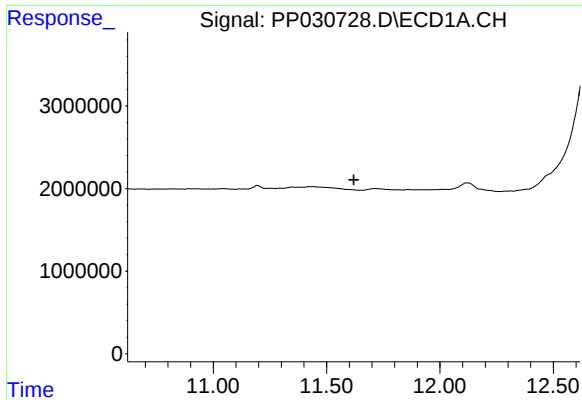

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.620 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

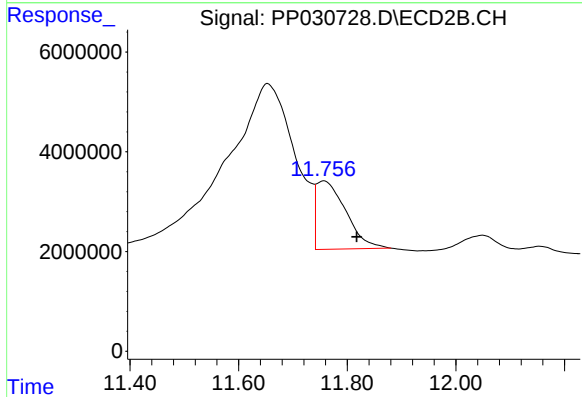


#7 MCPA

R.T.: 11.758 min
Delta R.T.: -0.060 min
Response: 51951166
Conc: 25.50 ug/ml

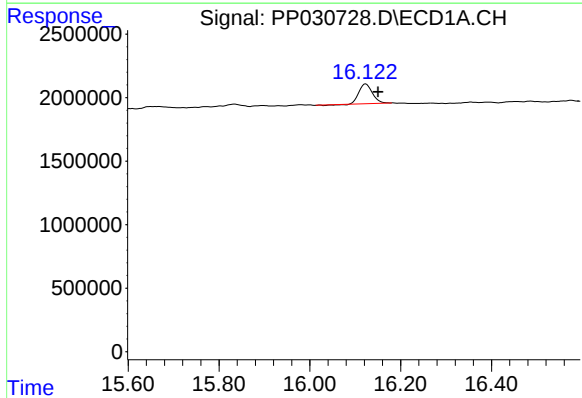

#15 Picloram

R.T.: 16.123 min
Delta R.T.: -0.027 min
Response: 3163690
Conc: 0.86 ng/ml

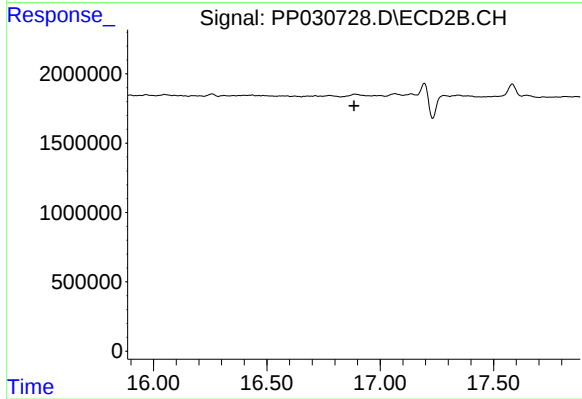

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.885 min
Response: 0
Conc: N.D.