

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072920\
 Data File : PP030731.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jul 2020 10:08
 Operator : DD\AJ
 Sample : PB130011BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 12:17:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072820.M
 Quant Title : 8080.M
 QLast Update : Wed Jul 29 01:54:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	10.715	10.933	135.7E6	127.9E6	304.896	285.607
Target Compounds							
1) T	Dalapon	0.000	2.331	0	50146801	N.D.	91.746 #
2) T	3,5-DICHL...	0.000	9.057	0	1915719	N.D.	3.020 #
3) T	4-Nitroph...	0.000	10.086	0	4184671	N.D.	15.754 #
6) T	MCP	11.378	0.000	6740260	0	5.529	N.D. #
7) T	MCPA	0.000	11.761	0	40126522	N.D.	19.697 #
8) T	DICHLORPROP	0.000	12.272	0	2512041	N.D.	6.031 #
11) T	2,4,5-TP ...	0.000	13.925	0	2723059	N.D.	1.246 #
15) T	Picloram	16.137	16.894	4842160	6447172	1.319	2.212 #
16) T	DCPA	0.000	16.784	0	6533251	N.D.	2.399 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072920\
Data File : PP030731.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jul 2020 10:08
Operator : DD\AJ
Sample : PB130011BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 12:17:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072820.M
Quant Title : 8080.M
QLast Update : Wed Jul 29 01:54:31 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

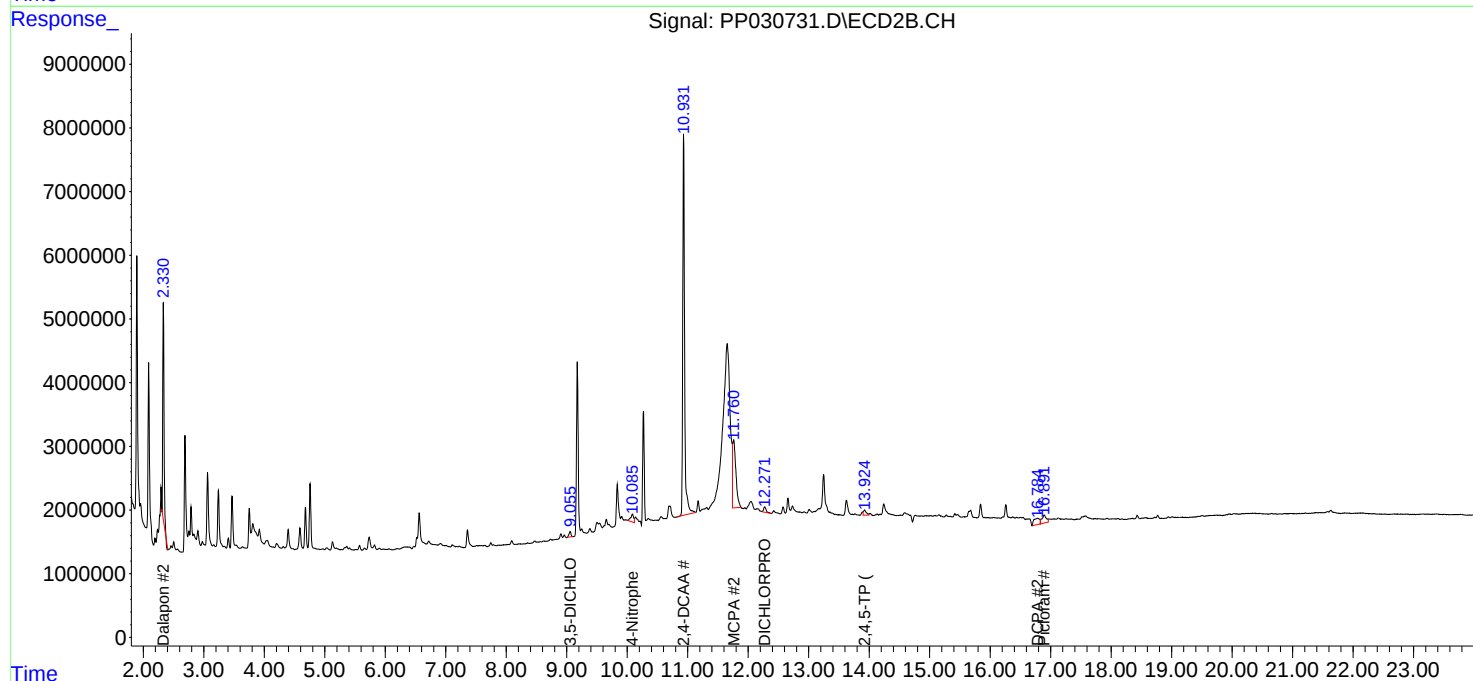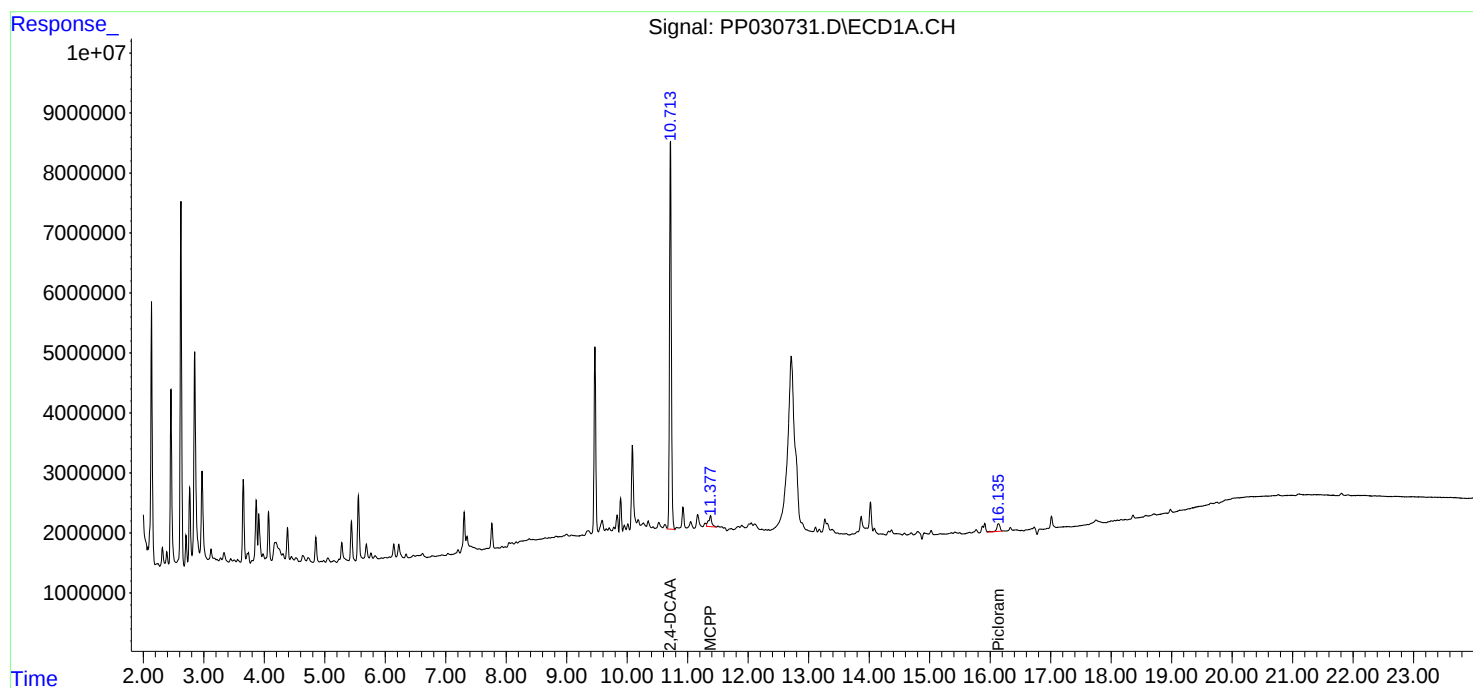


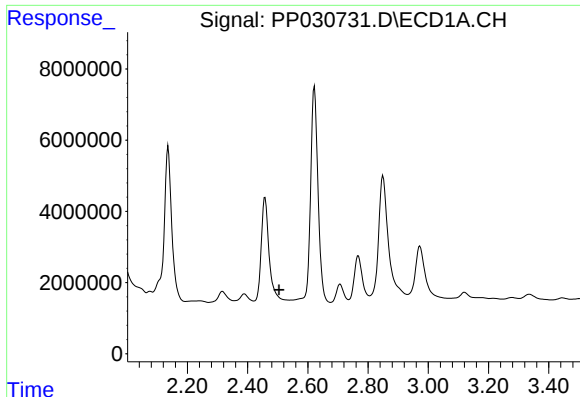

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.505 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

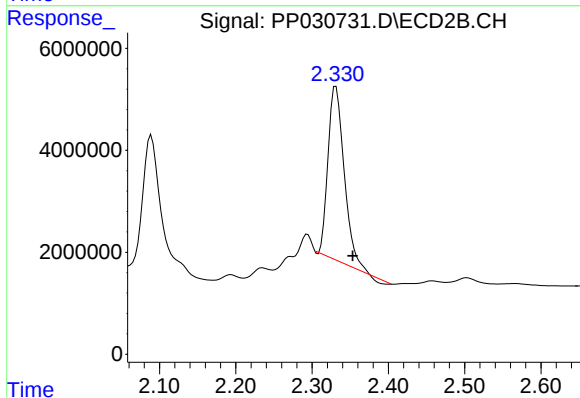


#1 Dalapon

R.T.: 2.331 min
Delta R.T.: -0.022 min
Response: 50146801
Conc: 91.75 ng/ml

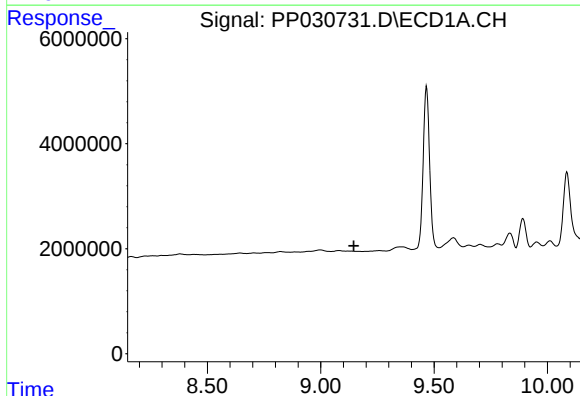


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.145 min
Response: 0
Conc: N.D.

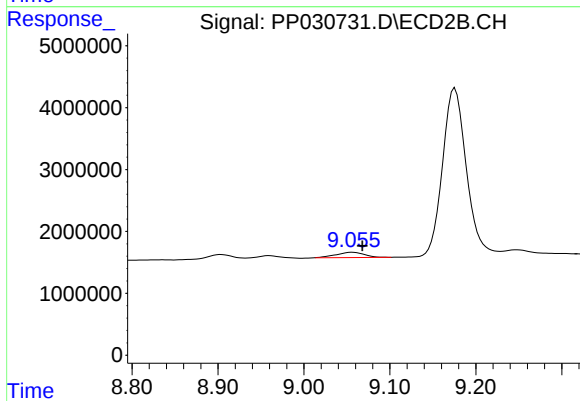

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.057 min
Delta R.T.: -0.012 min
Response: 1915719
Conc: 3.02 ng/ml

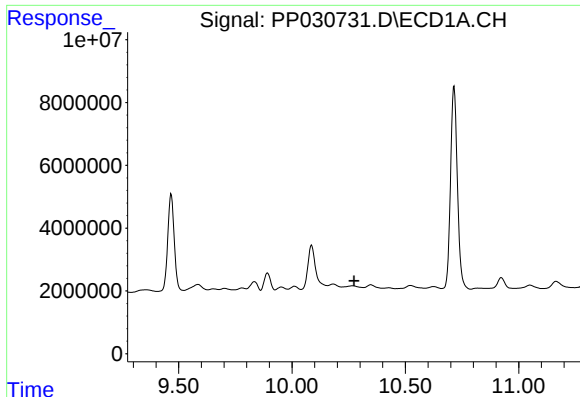

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

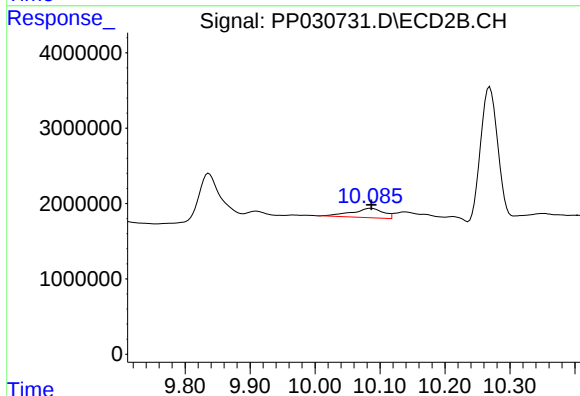


#3 4-Nitrophenol

R.T.: 10.086 min
Delta R.T.: 0.000 min
Response: 4184671
Conc: 15.75 ng/ml

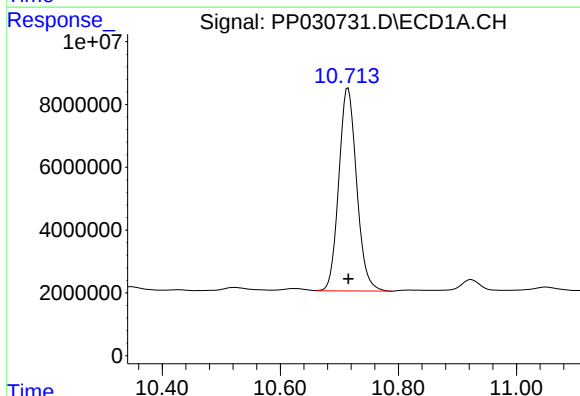


#4 2,4-DCAA

R.T.: 10.715 min
Delta R.T.: 0.000 min
Response: 135676446
Conc: 304.90 ng/ml

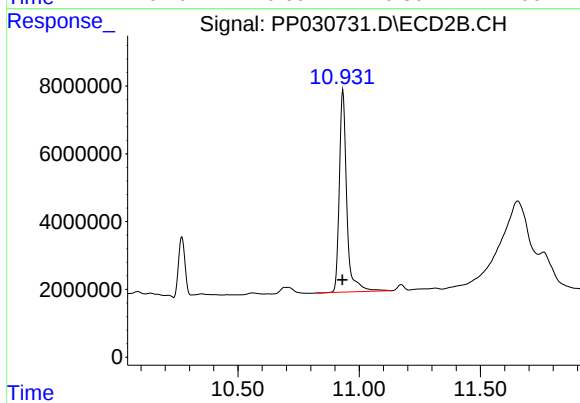

#4 2,4-DCAA


R.T.: 10.933 min
Delta R.T.: 0.002 min
Response: 127872645
Conc: 285.61 ng/ml

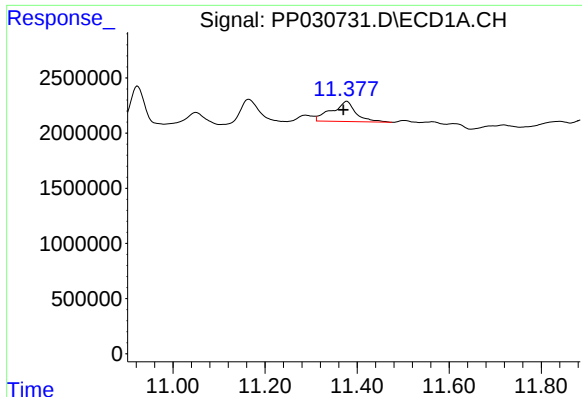

#6 MCPP


R.T.: 11.378 min
Delta R.T.: 0.008 min
Response: 6740260
Conc: 5.53 ug/ml

Instrument :
ECD_P
ClientSampleId :

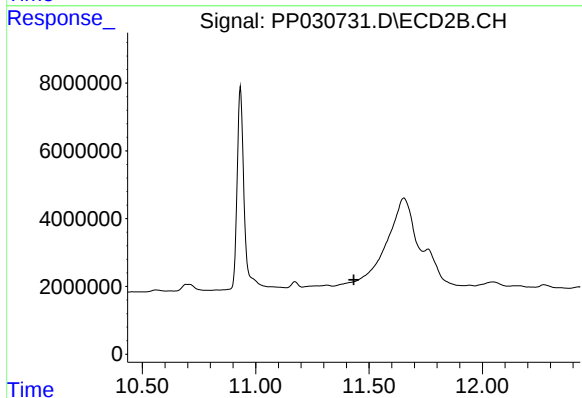


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.433 min
Response: 0
Conc: N.D.

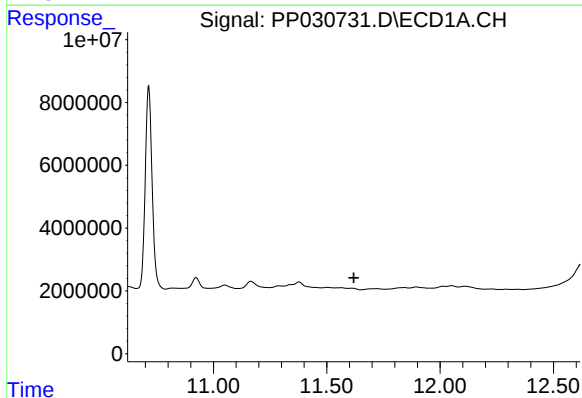


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.620 min
Response: 0
Conc: N.D.

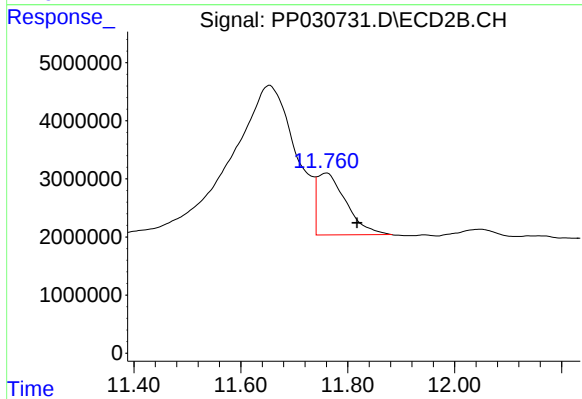

#7 MCPA


R.T.: 11.761 min
Delta R.T.: -0.057 min
Response: 40126522
Conc: 19.70 ug/ml

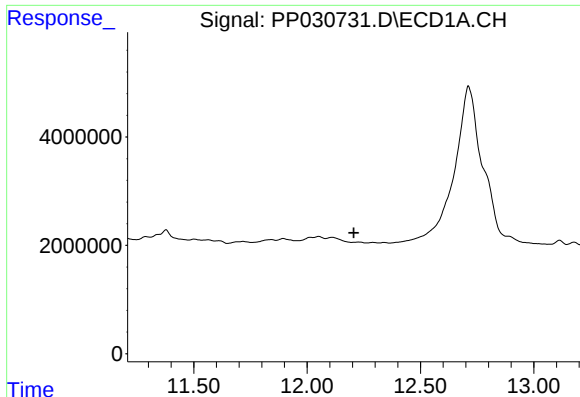

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.206 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

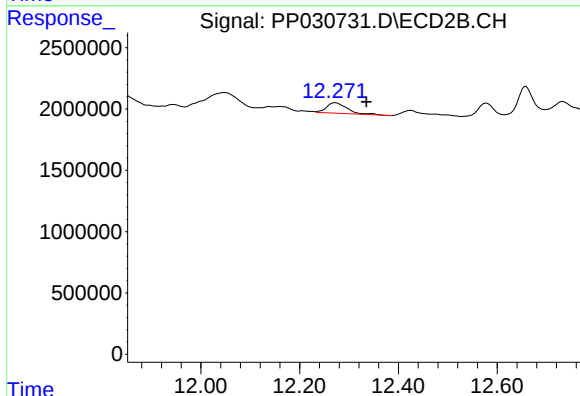


#8 DICHLORPROP

R.T.: 12.272 min
Delta R.T.: -0.063 min
Response: 2512041
Conc: 6.03 ng/ml

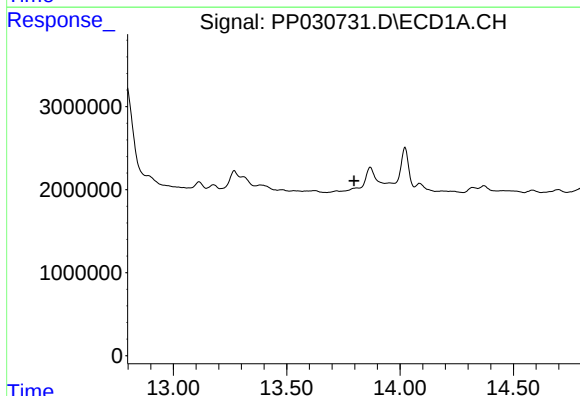


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 13.797 min
Response: 0
Conc: N.D.

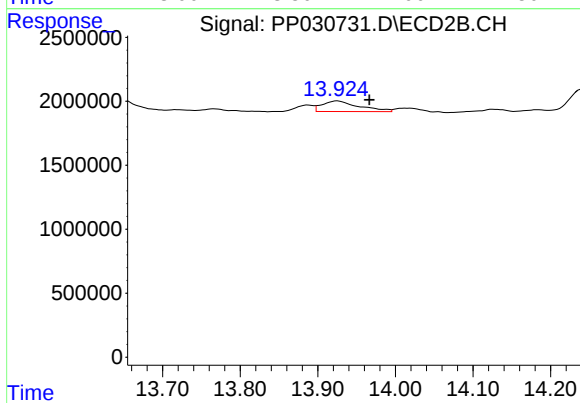

#11 2,4,5-TP (SILVEX)


R.T.: 13.925 min
Delta R.T.: -0.041 min
Response: 2723059
Conc: 1.25 ng/ml

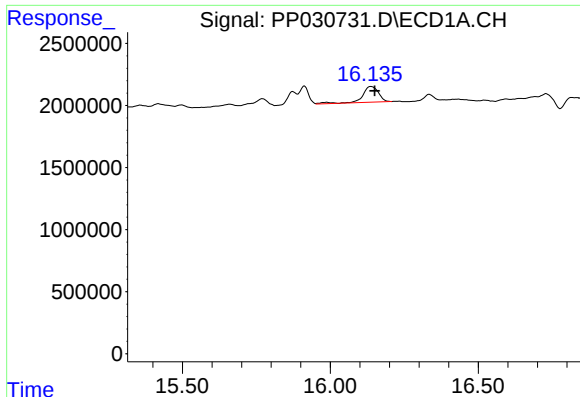

#15 Picloram


R.T.: 16.137 min
Delta R.T.: -0.014 min
Response: 4842160
Conc: 1.32 ng/ml

Instrument :
ECD_P
ClientSampleId :

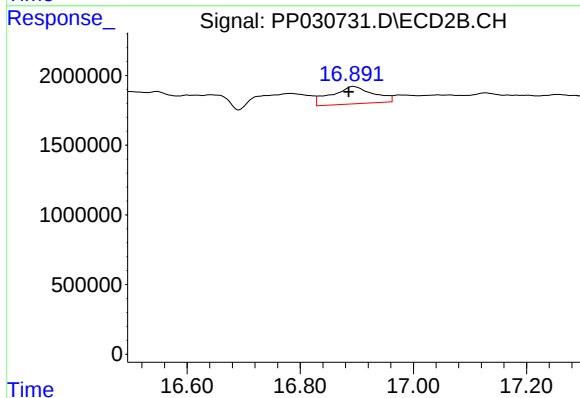


#15 Picloram

R.T.: 16.894 min
Delta R.T.: 0.008 min
Response: 6447172
Conc: 2.21 ng/ml

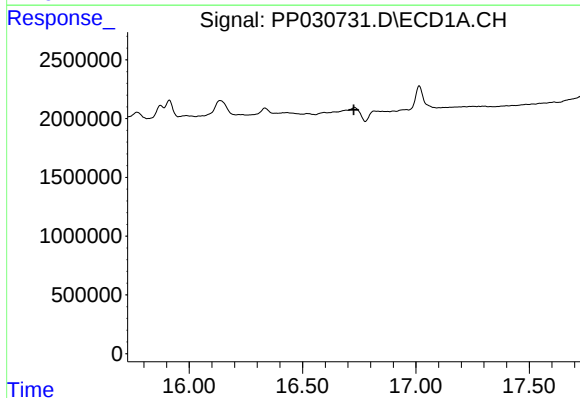

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.726 min
Response: 0
Conc: N.D.

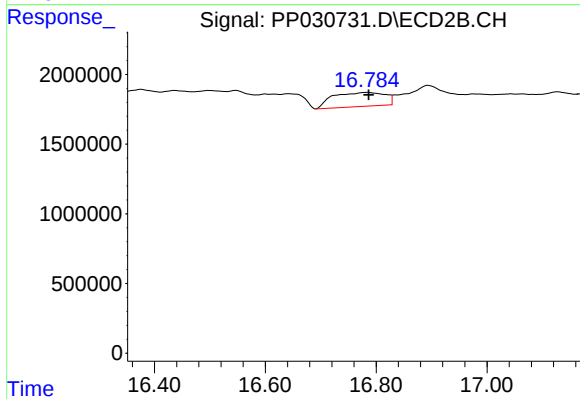

#16 DCPA

R.T.: 16.784 min
Delta R.T.: -0.002 min
Response: 6533251
Conc: 2.40 ng/ml