

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072921\
 Data File : P0079976.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2021 1:20
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 03:08:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.001	4.119	1307397	516882	21.697	22.570
2)	SA Decachlor...	11.114	9.530	1014838	458166	21.634	22.047
Target Compounds							
8)	L2 AR-1221-1	5.253	0.000	41802	0	64.872	N.D. #
20)	L4 AR-1242-5	0.000	6.310f	0	36724	N.D.	56.439 #
24)	L5 AR-1248-4	7.253f	0.000	155094	0	66.254	N.D. #
25)	L5 AR-1248-5	0.000	6.310	0	36724	N.D.	40.053 #
26)	L6 AR-1254-1	7.253	6.310f	155094	36724	71.001	27.081 #
28)	L6 AR-1254-3	7.878f	0.000	52877	0	15.357	N.D. #
29)	L6 AR-1254-4	8.186f	0.000	108233	0	42.555	N.D. #
32)	L7 AR-1260-2	0.000	7.217	0	28373	N.D.	18.547 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072921\
Data File : P0079976.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2021 1:20
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 03:08:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

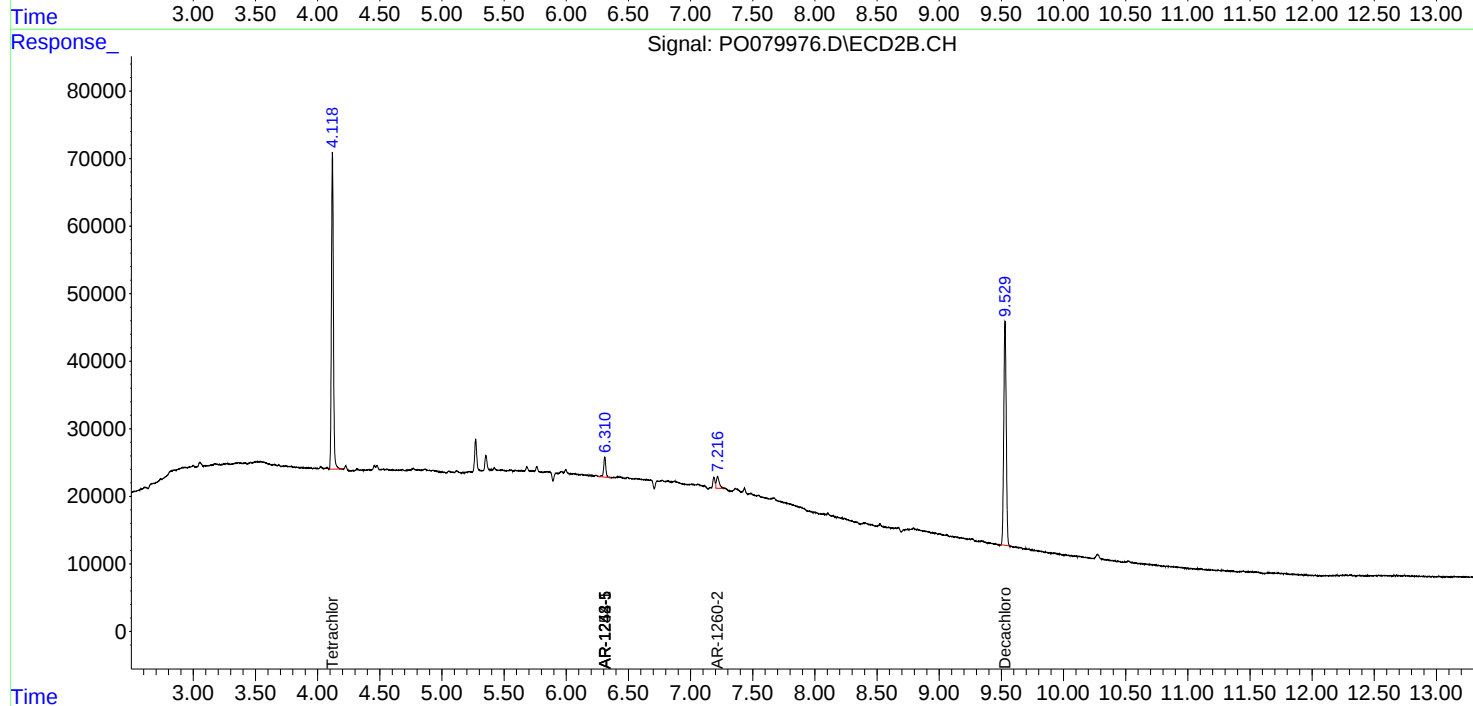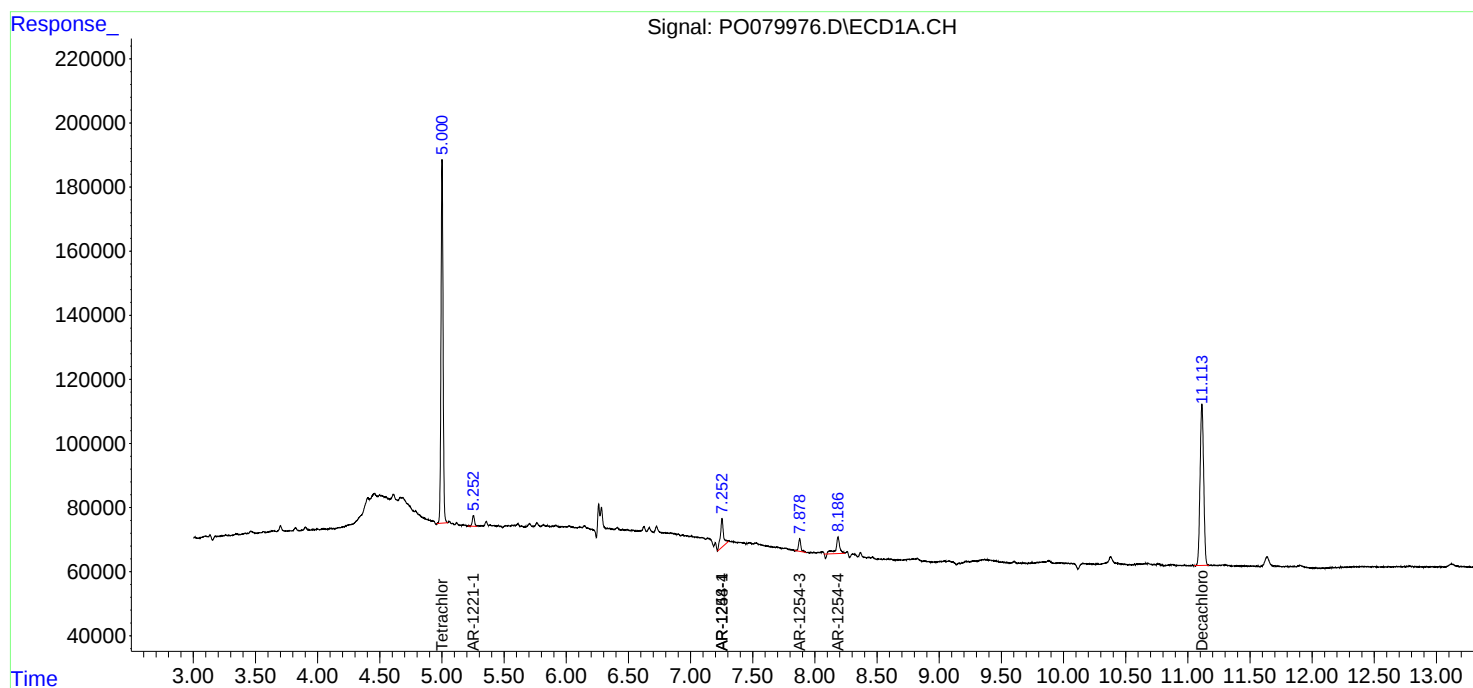


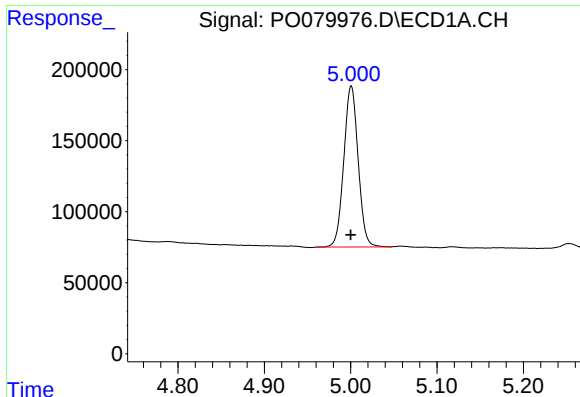

#1 Tetrachloro-m-xylene


R.T.: 5.001 min
Delta R.T.: 0.000 min
Response: 1307397
Conc: 21.70 ng/ml

Instrument :
ECD_P
ClientSampleId :

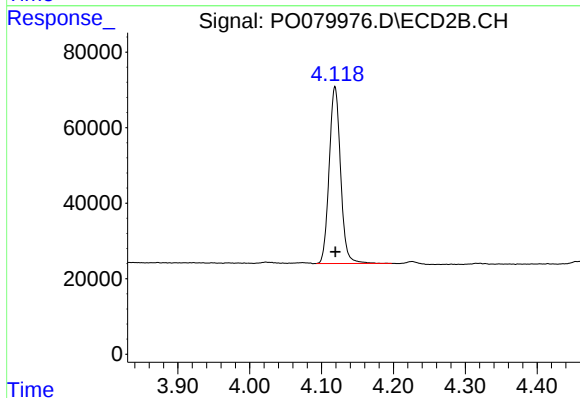


#1 Tetrachloro-m-xylene

R.T.: 4.119 min
Delta R.T.: 0.000 min
Response: 516882
Conc: 22.57 ng/ml

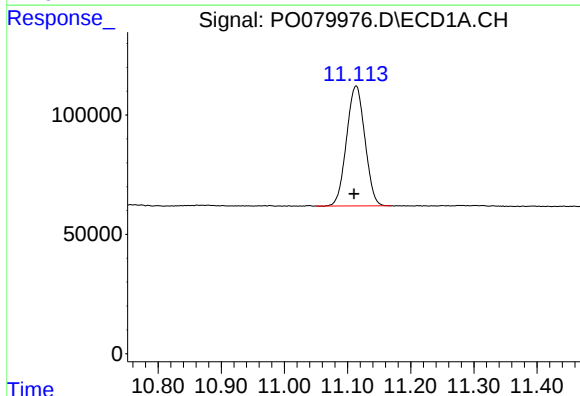


#2 Decachlorobiphenyl

R.T.: 11.114 min
Delta R.T.: 0.003 min
Response: 1014838
Conc: 21.63 ng/ml

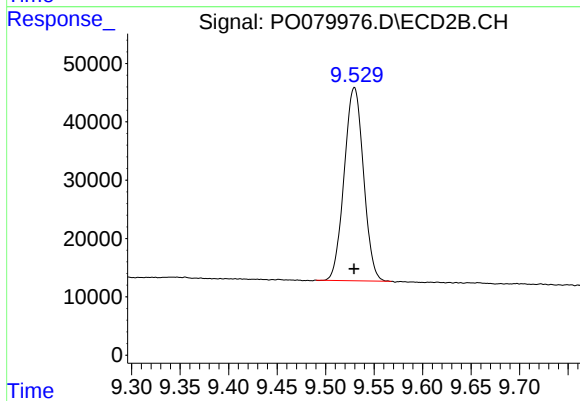

#2 Decachlorobiphenyl


R.T.: 9.530 min
Delta R.T.: 0.000 min
Response: 458166
Conc: 22.05 ng/ml

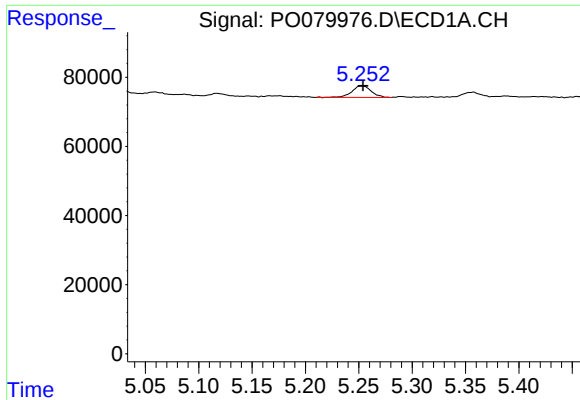

#8 AR-1221-1


R.T.: 5.253 min
Delta R.T.: -0.001 min
Response: 41802
Conc: 64.87 ng/ml

Instrument :
ECD_P
ClientSampleId :

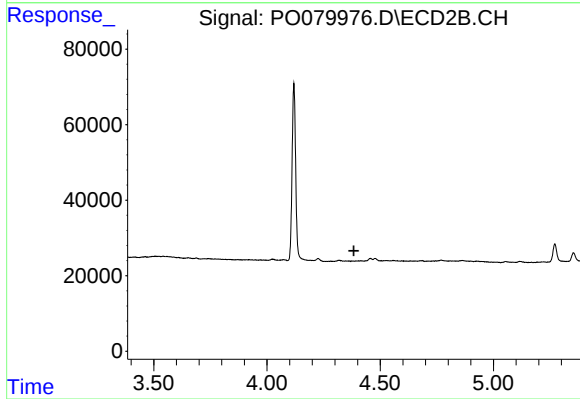


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.384 min
Response: 0
Conc: N.D.

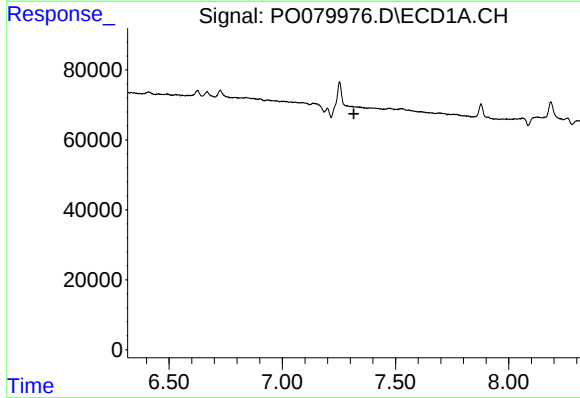


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 7.316 min
Response: 0
Conc: N.D.

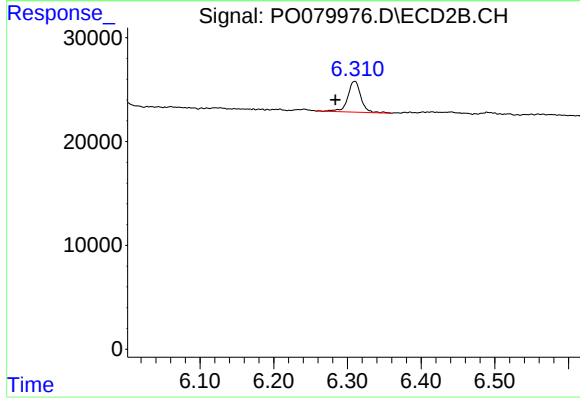

#20 AR-1242-5


R.T.: 6.310 min
Delta R.T.: 0.026 min
Response: 36724
Conc: 56.44 ng/ml

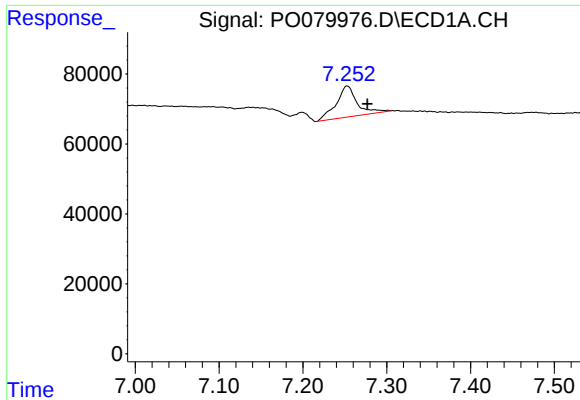

#24 AR-1248-4


R.T.: 7.253 min
Delta R.T.: -0.024 min
Response: 155094
Conc: 66.25 ng/ml

Instrument :
ECD_P
ClientSampleId :

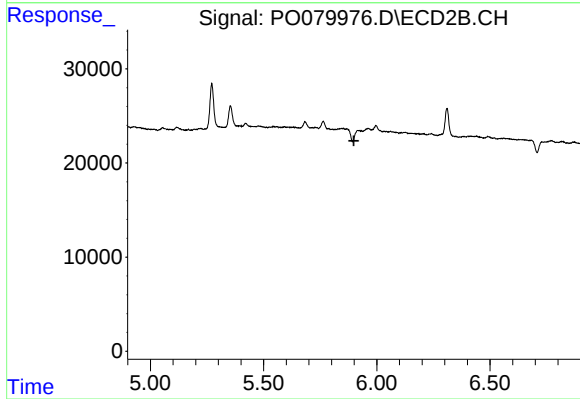


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.899 min
Response: 0
Conc: N.D.

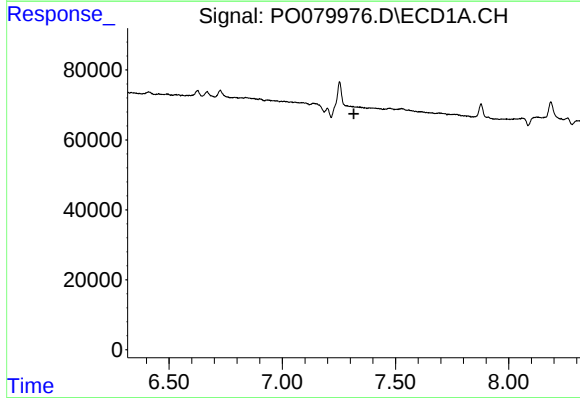


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 7.316 min
Response: 0
Conc: N.D.

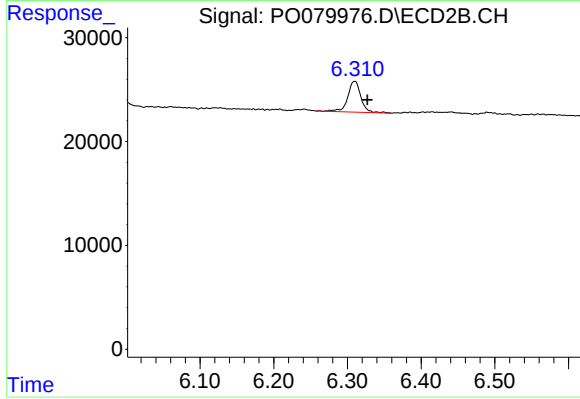

#25 AR-1248-5


R.T.: 6.310 min
Delta R.T.: -0.017 min
Response: 36724
Conc: 40.05 ng/ml

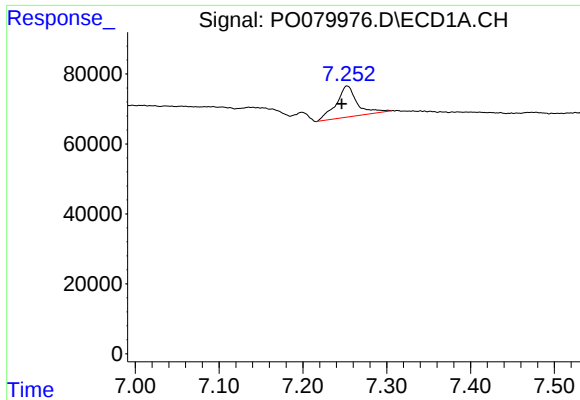

#26 AR-1254-1


R.T.: 7.253 min
Delta R.T.: 0.006 min
Response: 155094
Conc: 71.00 ng/ml

Instrument :
ECD_P
ClientSampleId :

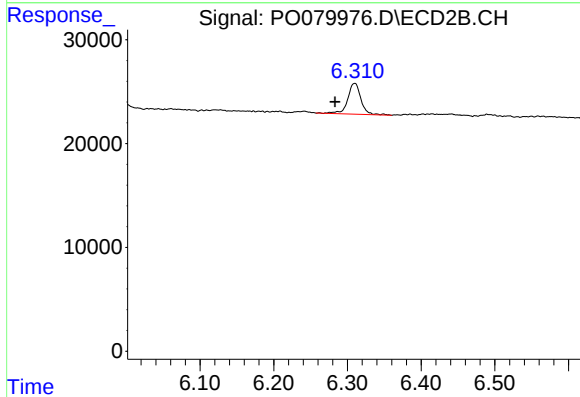


#26 AR-1254-1

R.T.: 6.310 min
Delta R.T.: 0.027 min
Response: 36724
Conc: 27.08 ng/ml

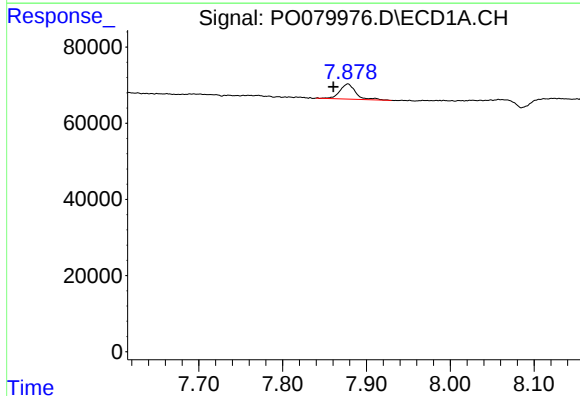


#28 AR-1254-3

R.T.: 7.878 min
Delta R.T.: 0.017 min
Response: 52877
Conc: 15.36 ng/ml

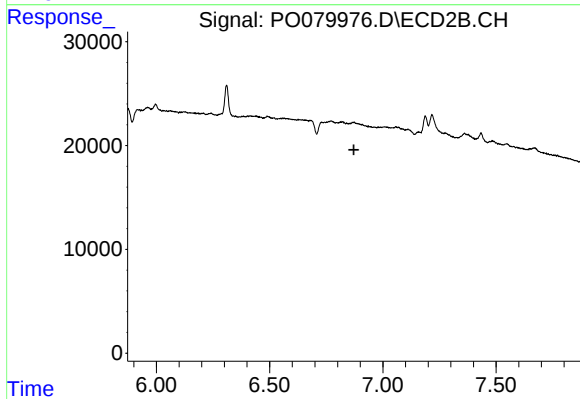

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.872 min
Response: 0
Conc: N.D.

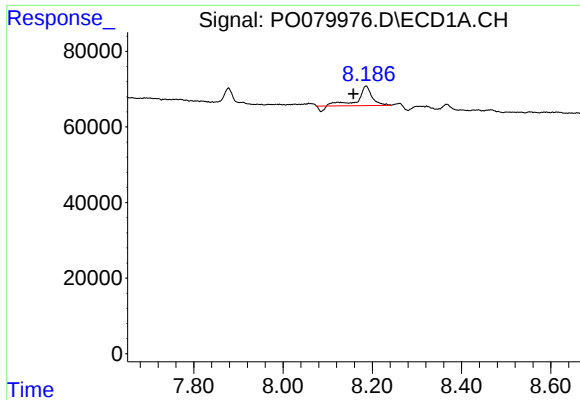

#29 AR-1254-4


R.T.: 8.186 min
Delta R.T.: 0.028 min
Response: 108233
Conc: 42.55 ng/ml

Instrument :
ECD_P
ClientSampleId :

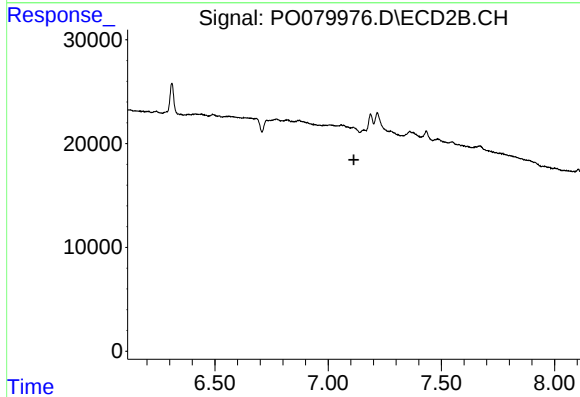


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.114 min
Response: 0
Conc: N.D.

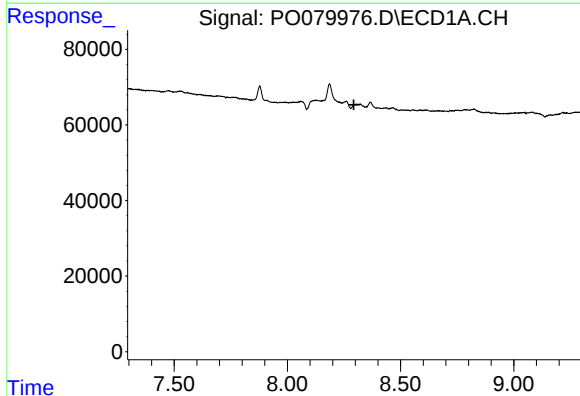

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.294 min
Response: 0
Conc: N.D.

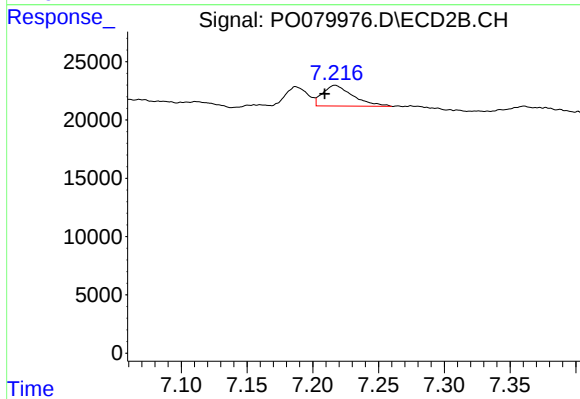

#32 AR-1260-2

R.T.: 7.217 min
Delta R.T.: 0.008 min
Response: 28373
Conc: 18.55 ng/ml