

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072921\
 Data File : PP037858.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2021 9:18
 Operator : DD\AJ
 Sample : M2940-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 16:34:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.953	3.944	947602	533205	20.850	19.485
2) SA Decachlor...	10.982	9.234	979390	535550	21.275	19.240
Target Compounds						
8) L2 AR-1221-1	5.195f	4.198	23509	7808	44.326m	25.563m#
9) L2 AR-1221-2	5.305	4.296	16460	11073	40.629m	47.035m
10) L2 AR-1221-3	5.388	4.385	35988	20015	29.536m	26.910m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072921\
Data File : PP037858.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2021 9:18
Operator : DD\AJ
Sample : M2940-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 71 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 16:34:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

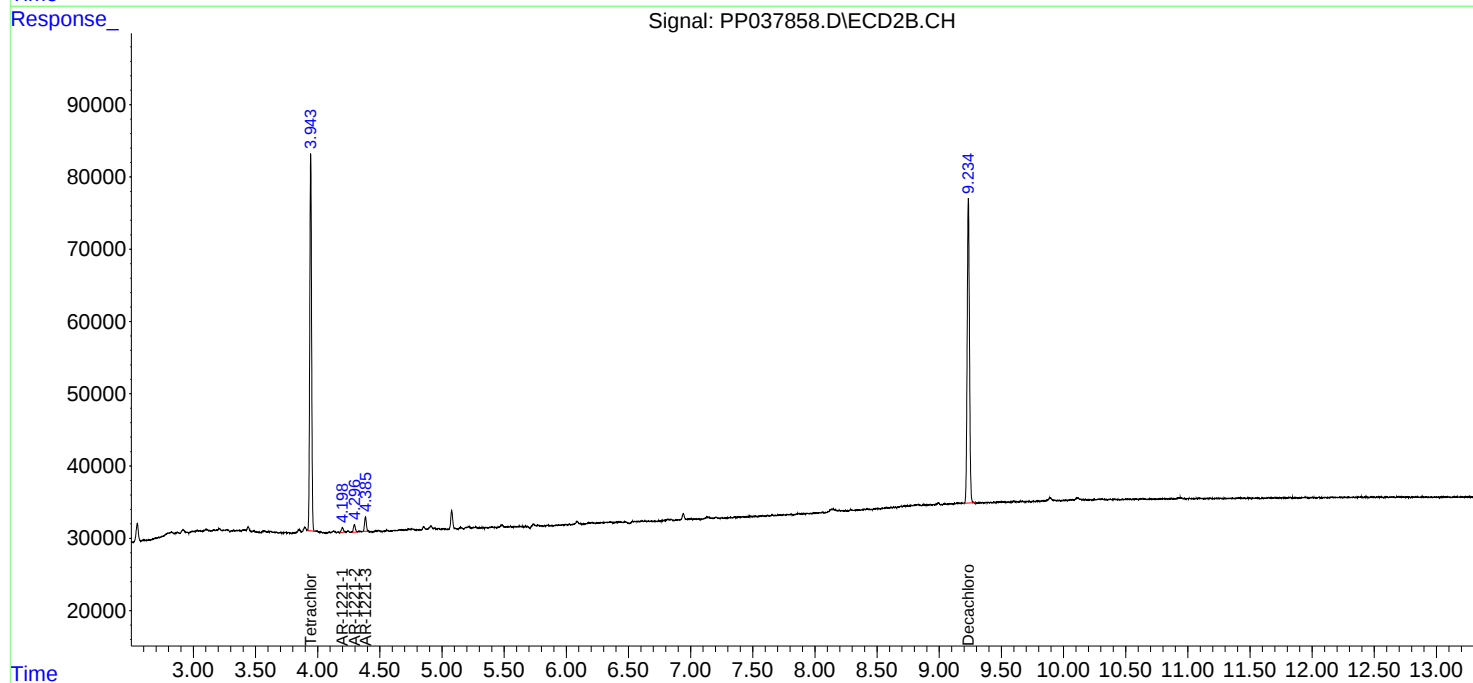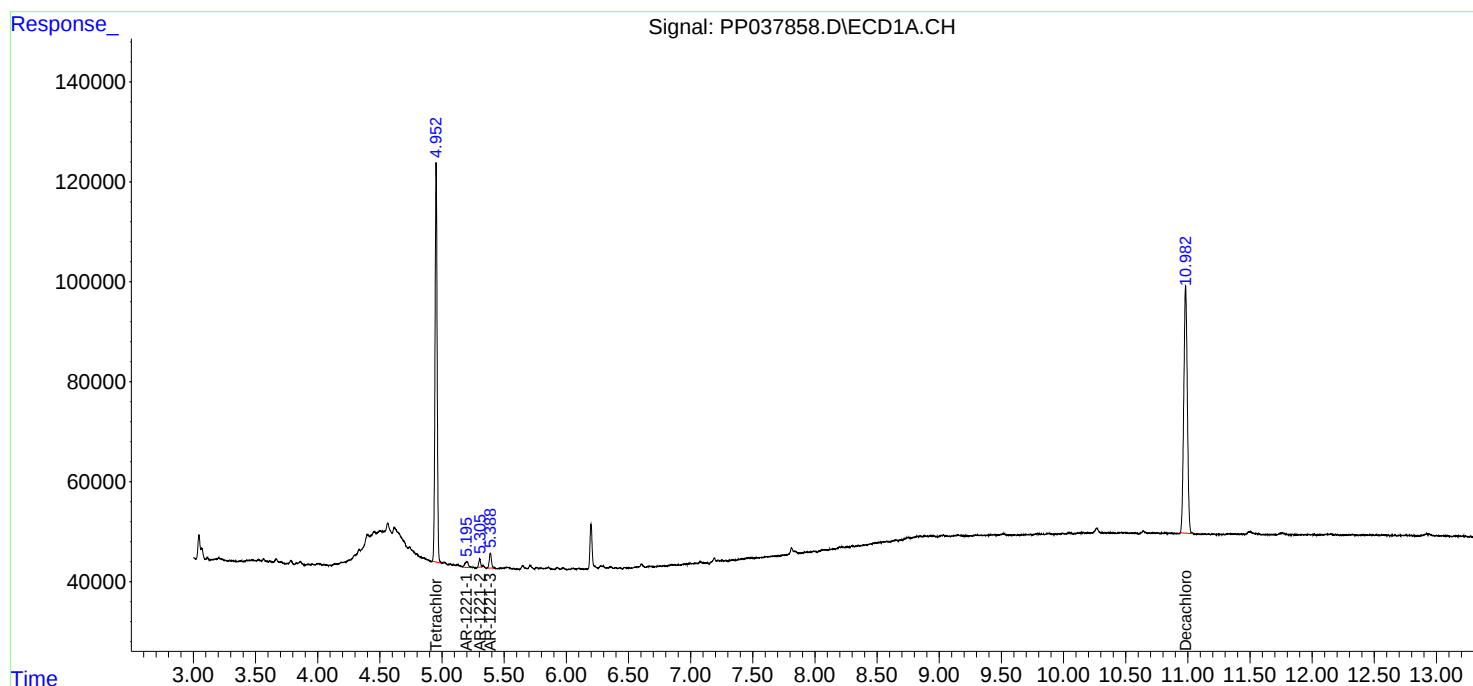


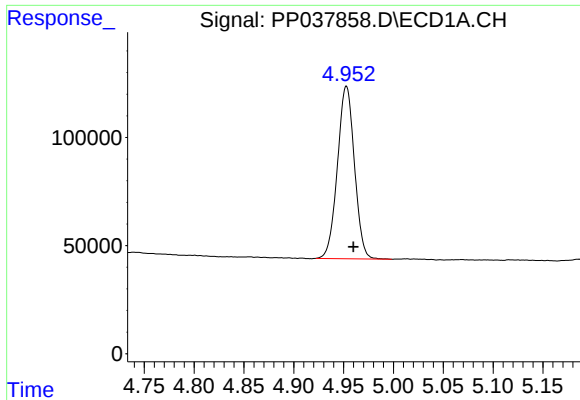

#1 Tetrachloro-m-xylene


R.T.: 4.953 min
Delta R.T.: -0.007 min
Response: 947602
Conc: 20.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

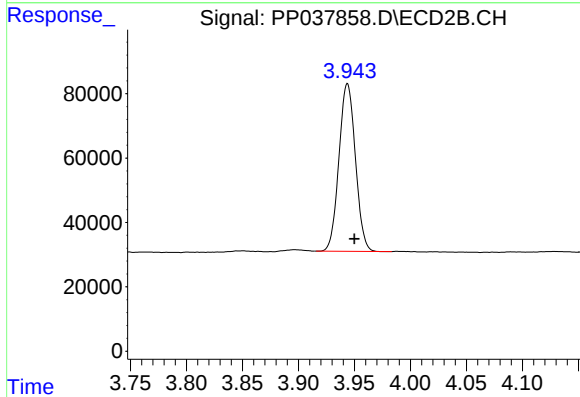


#1 Tetrachloro-m-xylene

R.T.: 3.944 min
Delta R.T.: -0.006 min
Response: 533205
Conc: 19.49 ng/ml

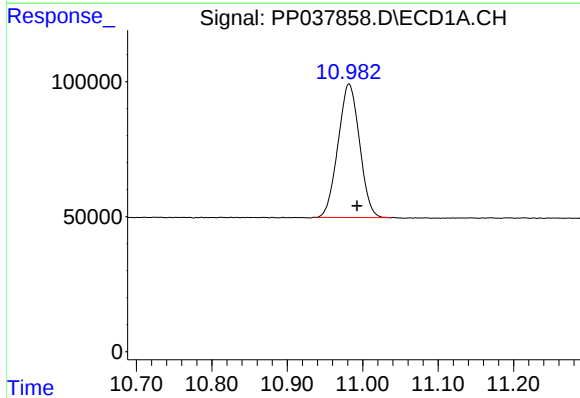


#2 Decachlorobiphenyl

R.T.: 10.982 min
Delta R.T.: -0.010 min
Response: 979390
Conc: 21.27 ng/ml

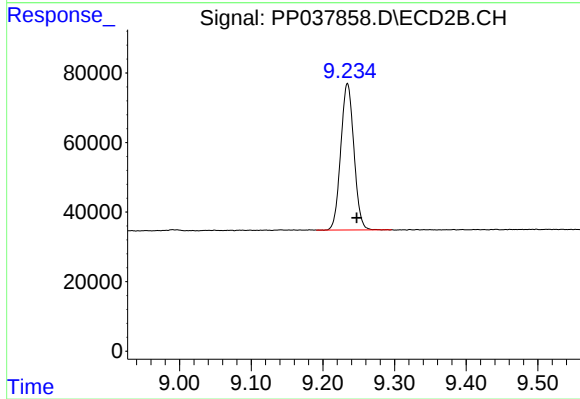

#2 Decachlorobiphenyl


R.T.: 9.234 min
Delta R.T.: -0.013 min
Response: 535550
Conc: 19.24 ng/ml

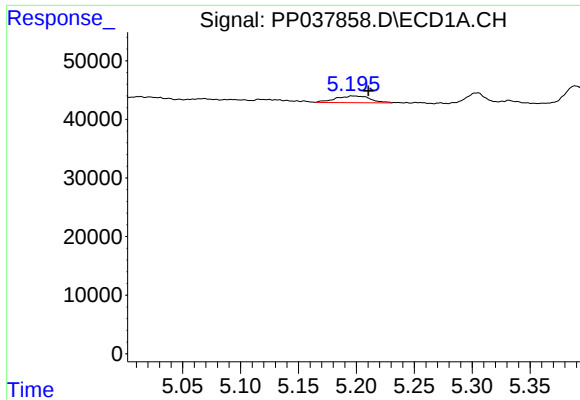

#8 AR-1221-1


R.T.: 5.195 min
Delta R.T.: -0.015 min
Response: 23509
Conc: 44.33 ng/ml m

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

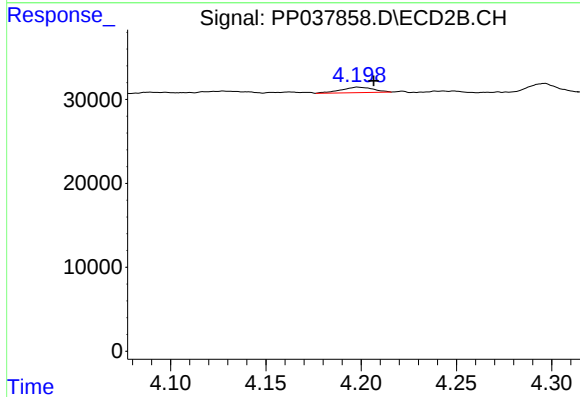


#8 AR-1221-1

R.T.: 4.198 min
Delta R.T.: -0.009 min
Response: 7808
Conc: 25.56 ng/ml m

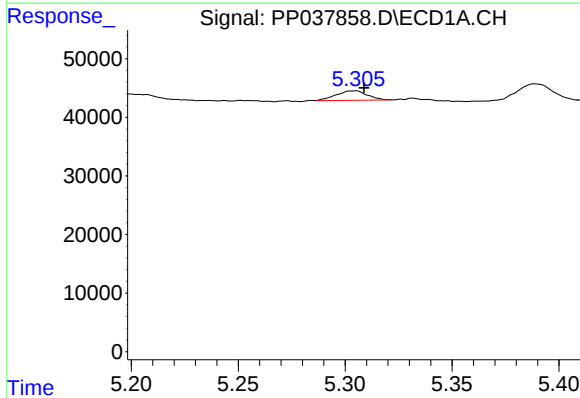


#9 AR-1221-2

R.T.: 5.305 min
Delta R.T.: -0.004 min
Response: 16460
Conc: 40.63 ng/ml m

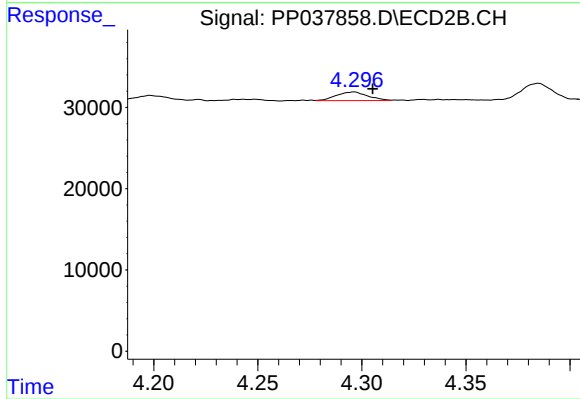

#9 AR-1221-2


R.T.: 4.296 min
Delta R.T.: -0.009 min
Response: 11073
Conc: 47.04 ng/ml m

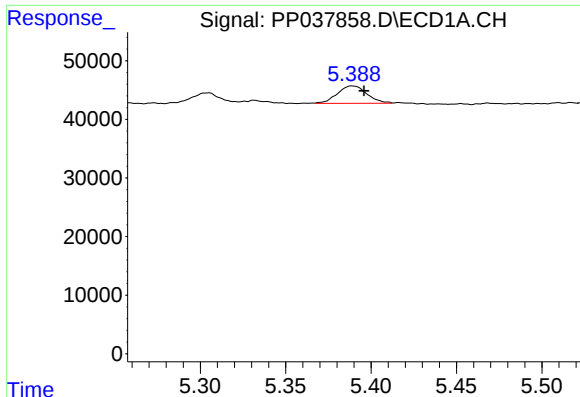

#10 AR-1221-3

R.T.: 5.388 min
Delta R.T.: -0.008 min
Response: 35988
Conc: 29.54 ng/ml m

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

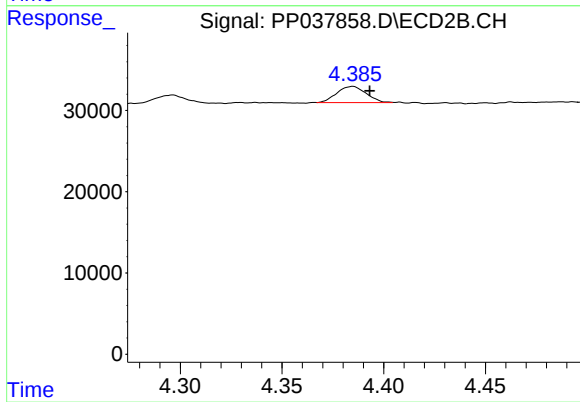

#10 AR-1221-3

R.T.: 4.385 min
Delta R.T.: -0.009 min
Response: 20015
Conc: 26.91 ng/ml m