

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072921\
 Data File : PP037859.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2021 9:35
 Operator : DD\AJ
 Sample : M2940-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 16:34:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.953	3.944	930299	528380	20.469	19.309
2) SA Decachlor...	10.981	9.234	972308	531942	21.121	19.111
Target Compounds						
11) L3 AR-1232-1	5.390	4.385	32557	20117	29.301	29.628
12) L3 AR-1232-2	5.975	5.212	18391	15635	30.843m	24.979
13) L3 AR-1232-3	6.297	5.402	33915	9336	30.993	28.118m
14) L3 AR-1232-4	6.471	5.498	17549	5076	30.227	18.412m#
15) L3 AR-1232-5	6.568	5.683	10838	9136	28.180	30.731m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072921\
Data File : PP037859.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2021 9:35
Operator : DD\AJ
Sample : M2940-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 72 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 16:34:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

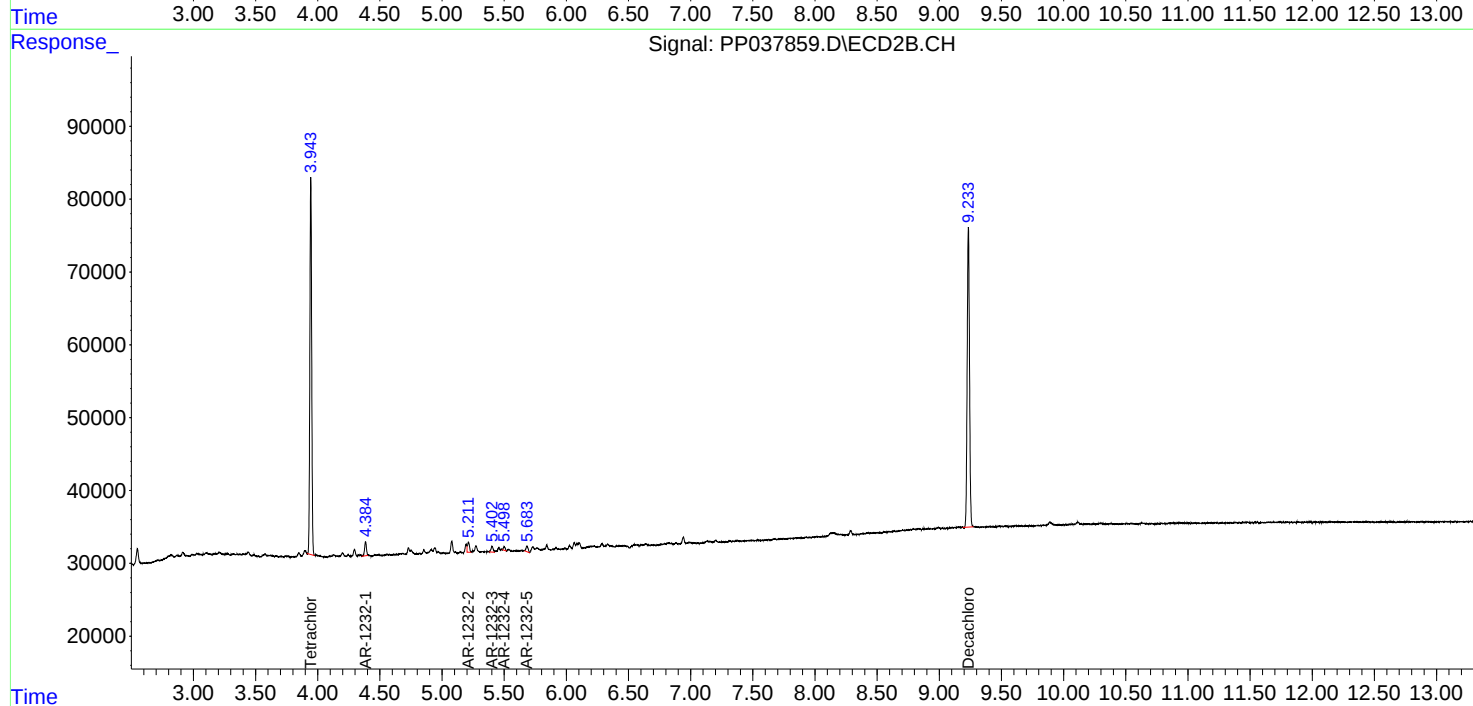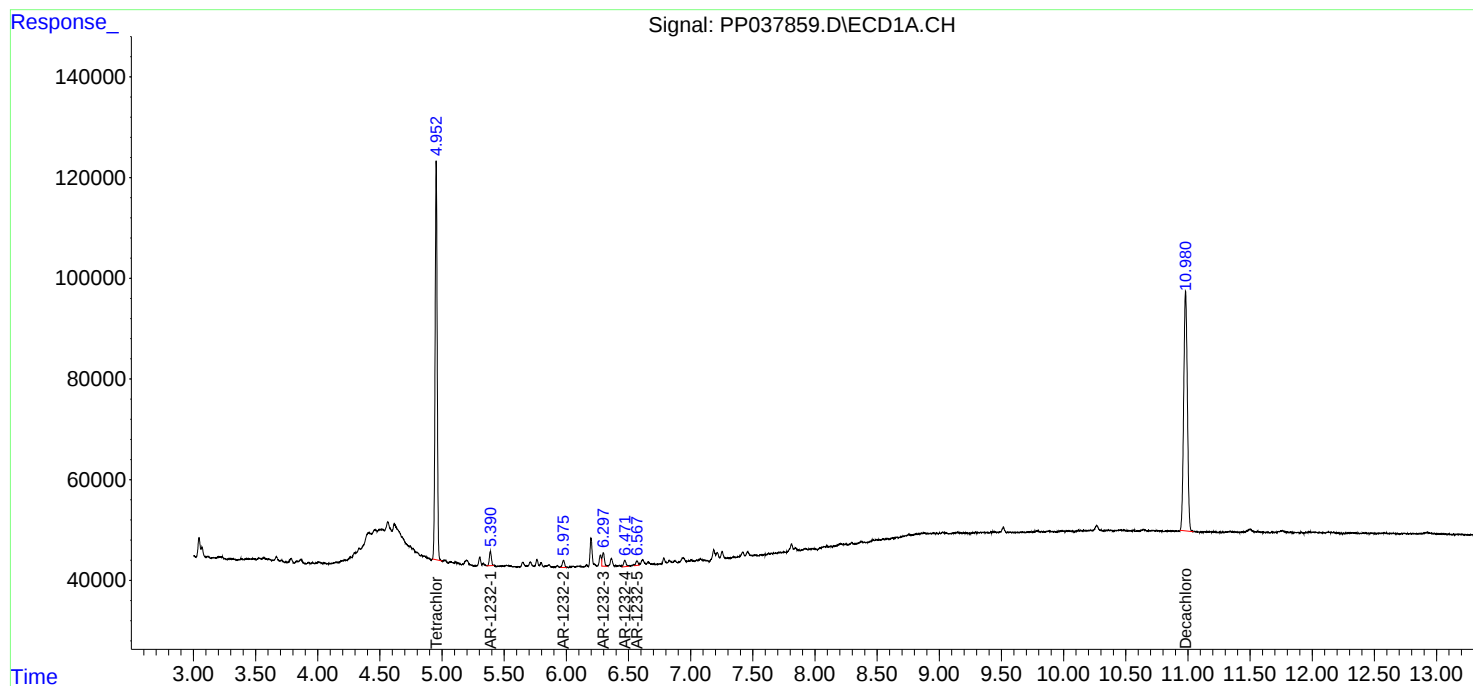


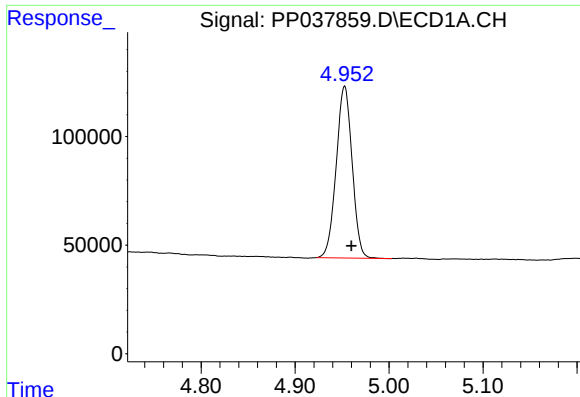

#1 Tetrachloro-m-xylene


R.T.: 4.953 min
Delta R.T.: -0.007 min
Response: 930299
Conc: 20.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

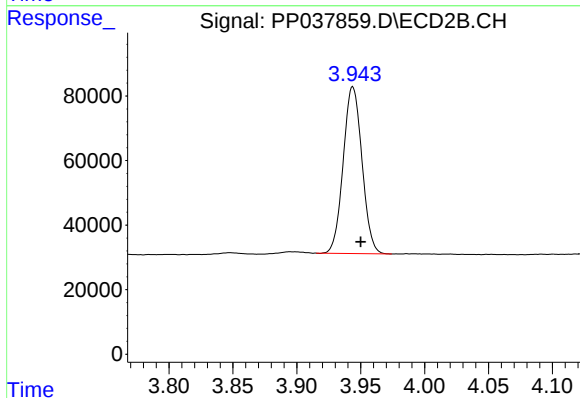


#1 Tetrachloro-m-xylene

R.T.: 3.944 min
Delta R.T.: -0.006 min
Response: 528380
Conc: 19.31 ng/ml

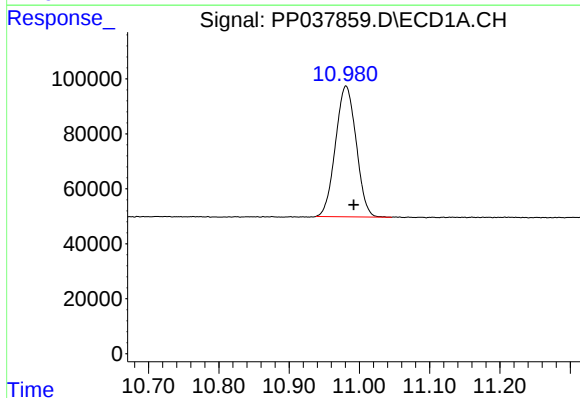


#2 Decachlorobiphenyl

R.T.: 10.981 min
Delta R.T.: -0.011 min
Response: 972308
Conc: 21.12 ng/ml

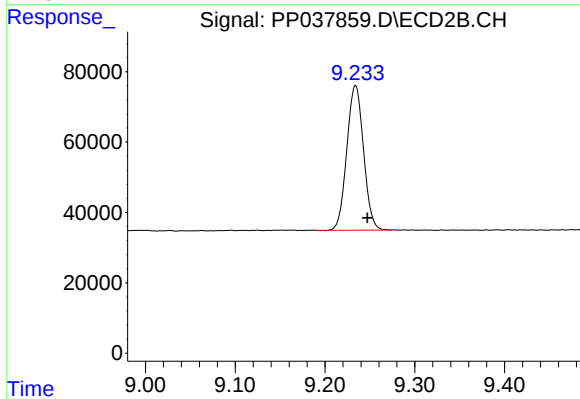

#2 Decachlorobiphenyl


R.T.: 9.234 min
Delta R.T.: -0.013 min
Response: 531942
Conc: 19.11 ng/ml

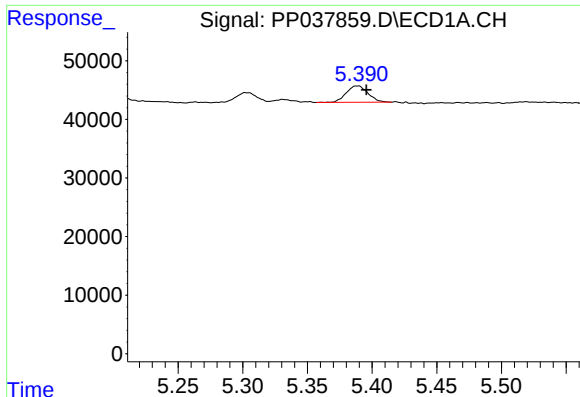

#11 AR-1232-1


R.T.: 5.390 min
Delta R.T.: -0.006 min
Response: 32557
Conc: 29.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

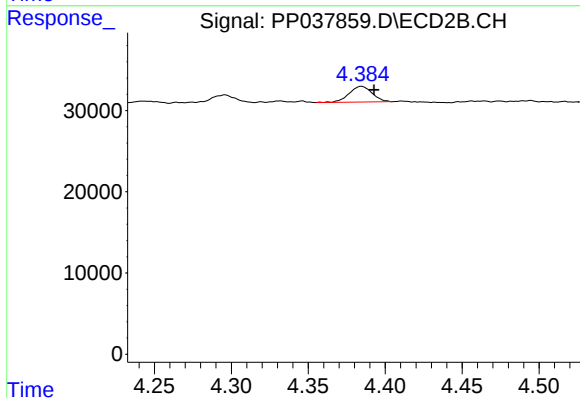


#11 AR-1232-1

R.T.: 4.385 min
Delta R.T.: -0.008 min
Response: 20117
Conc: 29.63 ng/ml

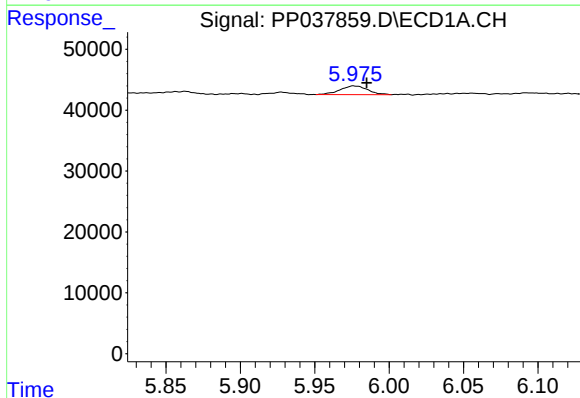


#12 AR-1232-2

R.T.: 5.975 min
Delta R.T.: -0.010 min
Response: 18391
Conc: 30.84 ng/ml m

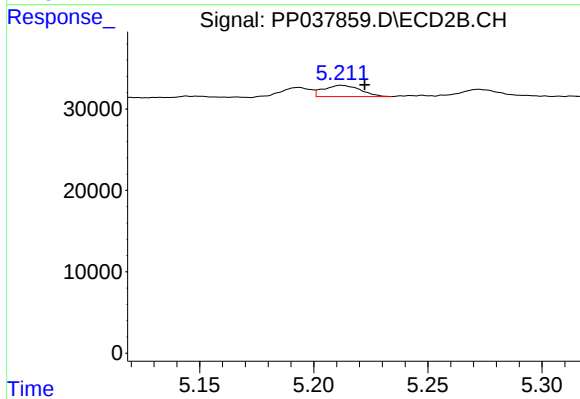

#12 AR-1232-2


R.T.: 5.212 min
Delta R.T.: -0.010 min
Response: 15635
Conc: 24.98 ng/ml

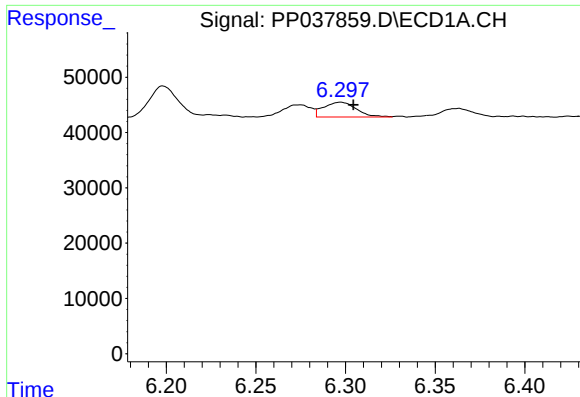

#13 AR-1232-3


R.T.: 6.297 min
Delta R.T.: -0.007 min
Response: 33915
Conc: 30.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

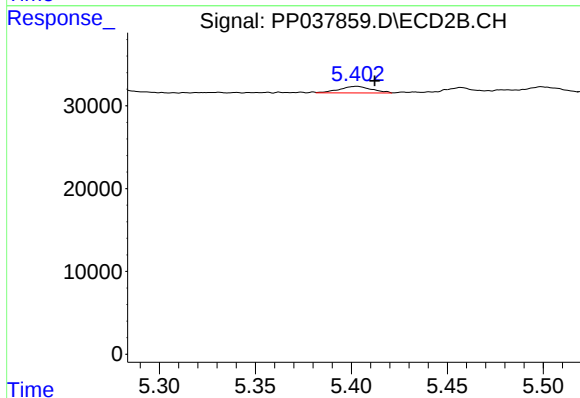


#13 AR-1232-3

R.T.: 5.402 min
Delta R.T.: -0.010 min
Response: 9336
Conc: 28.12 ng/ml m

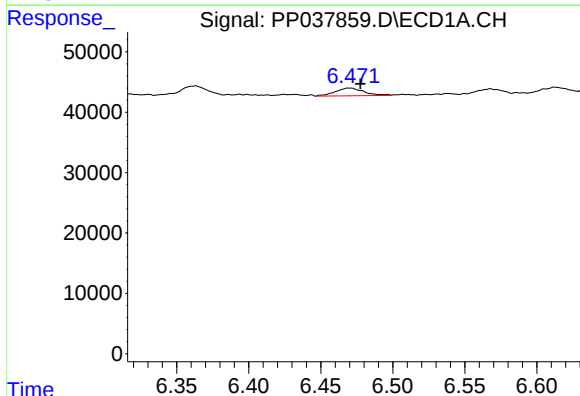


#14 AR-1232-4

R.T.: 6.471 min
Delta R.T.: -0.007 min
Response: 17549
Conc: 30.23 ng/ml

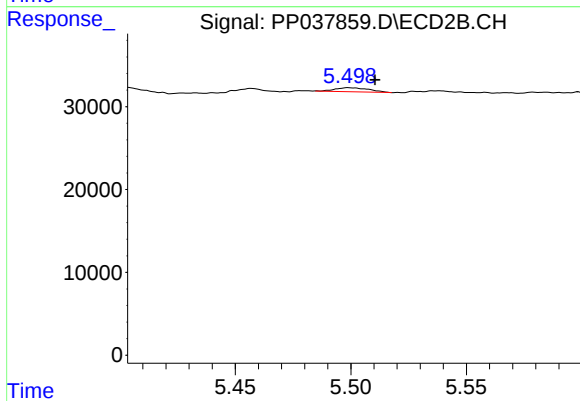

#14 AR-1232-4


R.T.: 5.498 min
Delta R.T.: -0.012 min
Response: 5076
Conc: 18.41 ng/ml m

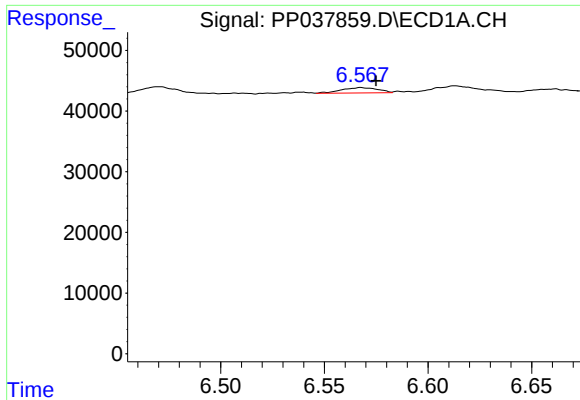

#15 AR-1232-5

R.T.: 6.568 min
Delta R.T.: -0.007 min
Response: 10838
Conc: 28.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

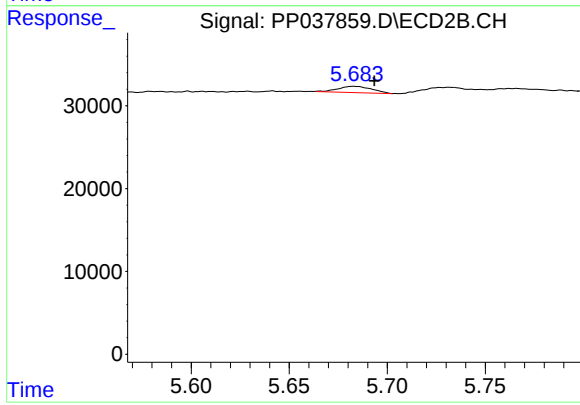

#15 AR-1232-5

R.T.: 5.683 min
Delta R.T.: -0.010 min
Response: 9136
Conc: 30.73 ng/ml m