

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072921\
 Data File : PP037862.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2021 10:26
 Operator : DD\AJ
 Sample : M2940-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 16:35:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.953	3.944	917914	521468	20.196	19.057
2) SA Decachlor...	10.982	9.234	947026	518944	20.572	18.644
Target Compounds						
26) L6 AR-1254-1	7.184	6.063	56007	31771	31.175	21.401 #
27) L6 AR-1254-2	7.412	6.224	78176	33249	28.104	25.596
28) L6 AR-1254-3	7.794	6.642	87015	47883	28.224	22.438
29) L6 AR-1254-4	8.090	6.882	63831	29784	28.101	21.953
30) L6 AR-1254-5	8.518	7.312	51081	28756	20.413	15.340



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072921\
Data File : PP037862.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2021 10:26
Operator : DD\AJ
Sample : M2940-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 75 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 16:35:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

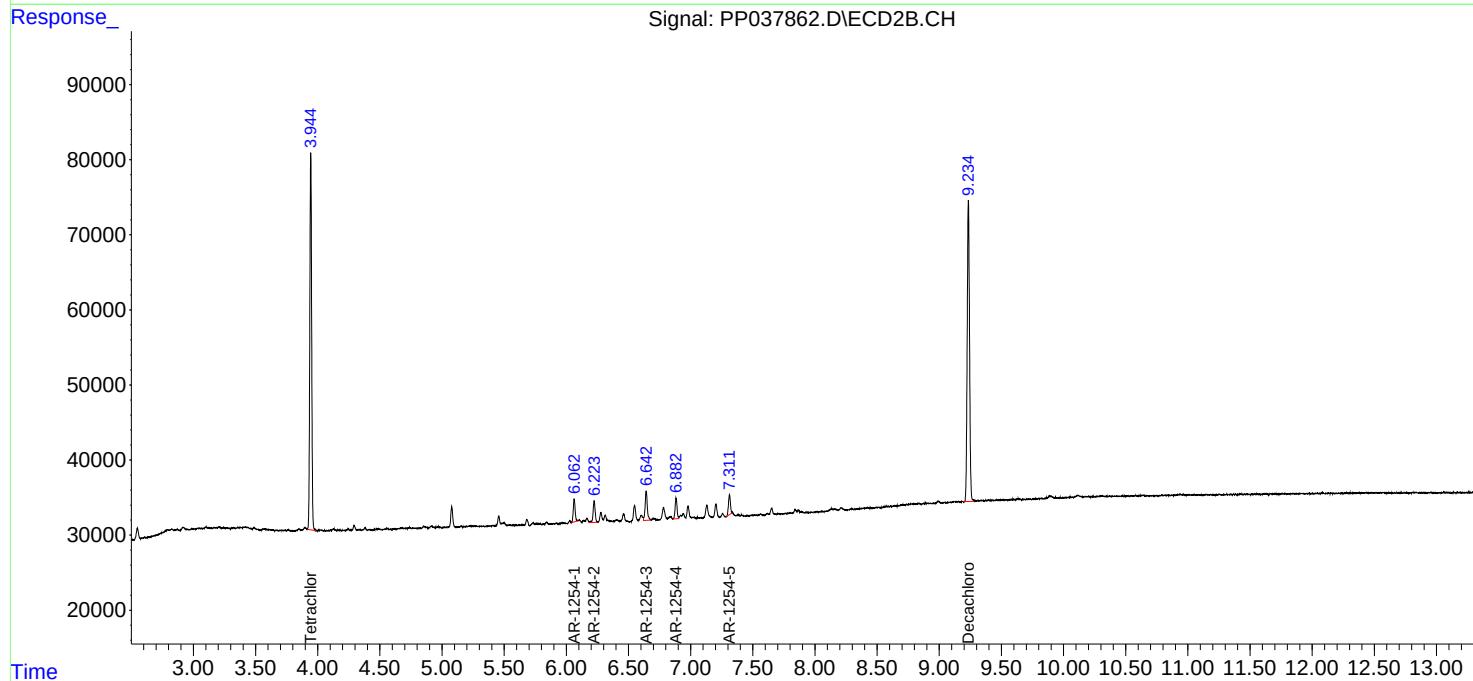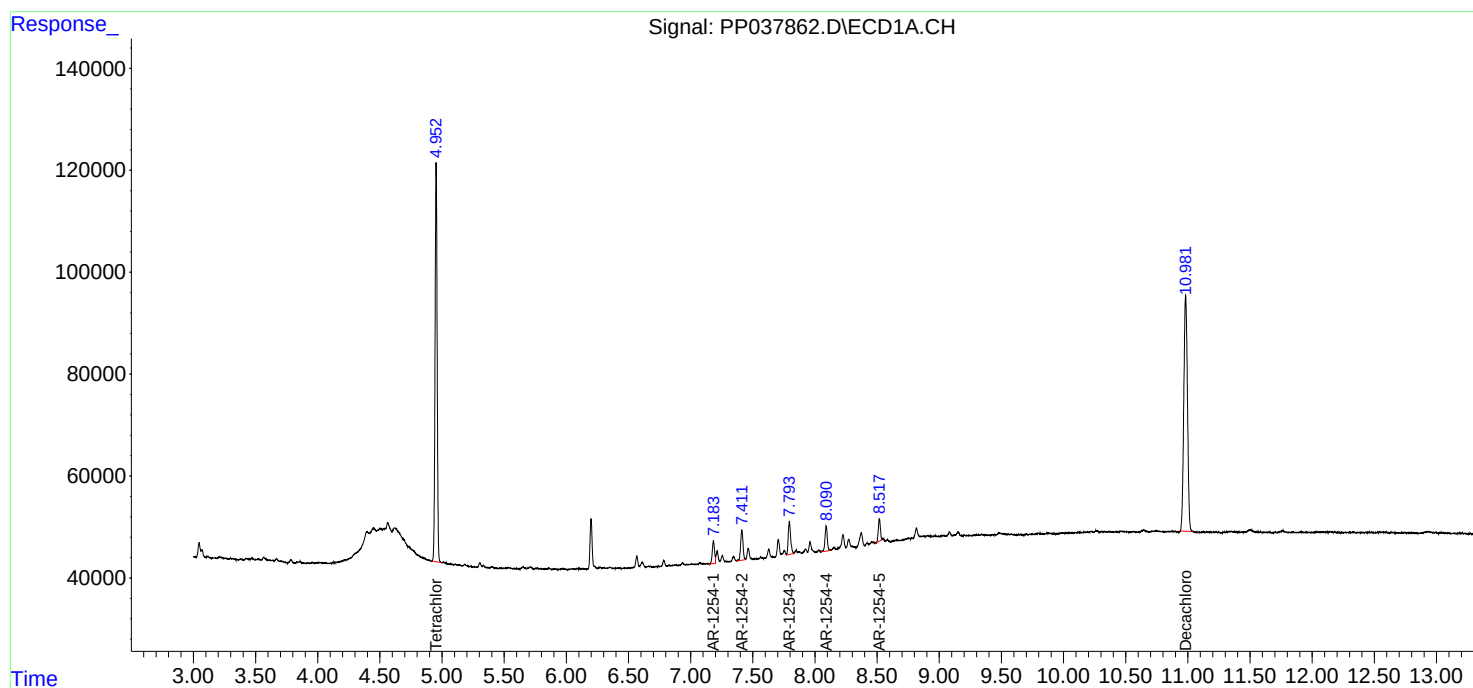


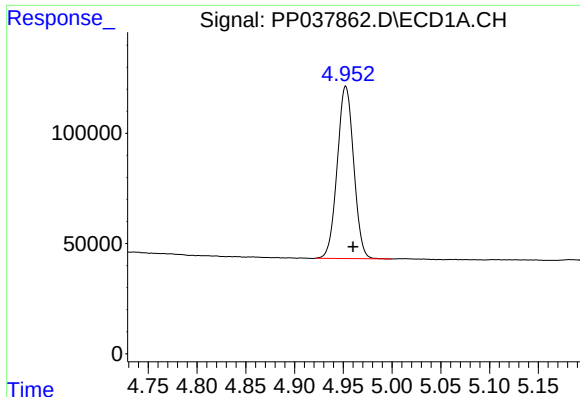

#1 Tetrachloro-m-xylene


R.T.: 4.953 min
Delta R.T.: -0.007 min
Response: 917914
Conc: 20.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

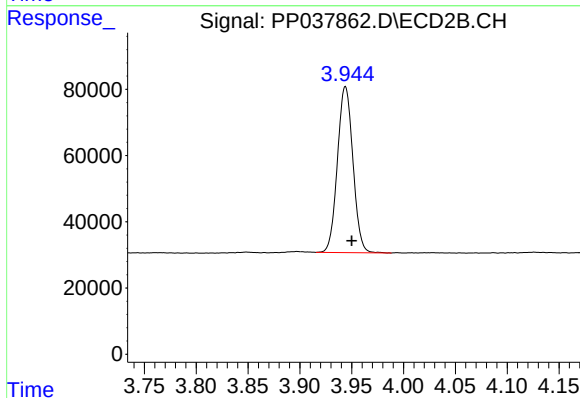


#1 Tetrachloro-m-xylene

R.T.: 3.944 min
Delta R.T.: -0.006 min
Response: 521468
Conc: 19.06 ng/ml

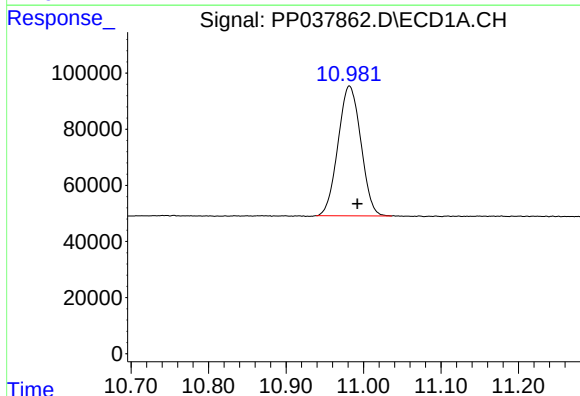


#2 Decachlorobiphenyl

R.T.: 10.982 min
Delta R.T.: -0.010 min
Response: 947026
Conc: 20.57 ng/ml

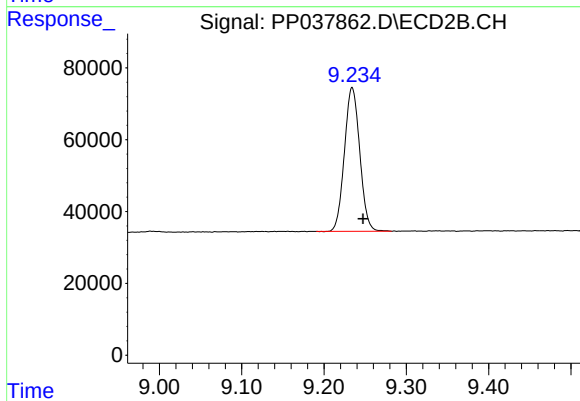

#2 Decachlorobiphenyl


R.T.: 9.234 min
Delta R.T.: -0.013 min
Response: 518944
Conc: 18.64 ng/ml

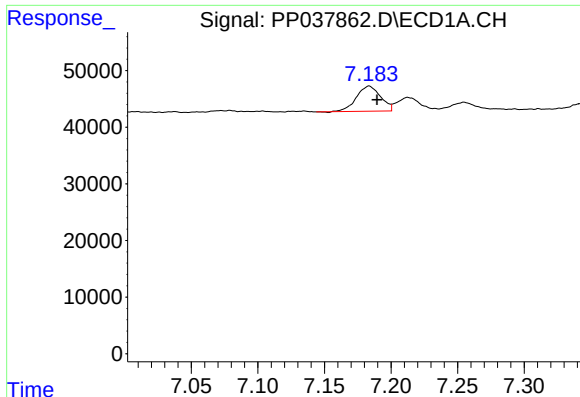

#26 AR-1254-1


R.T.: 7.184 min
Delta R.T.: -0.006 min
Response: 56007
Conc: 31.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

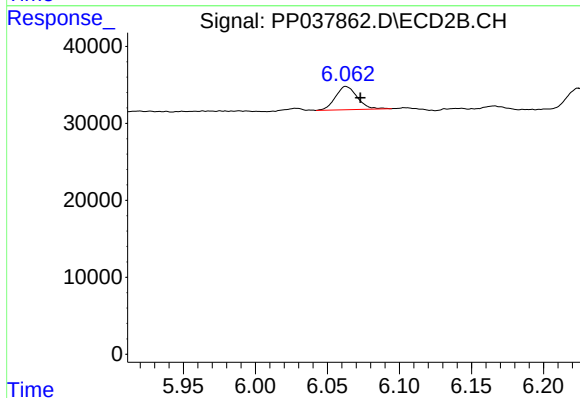


#26 AR-1254-1

R.T.: 6.063 min
Delta R.T.: -0.010 min
Response: 31771
Conc: 21.40 ng/ml

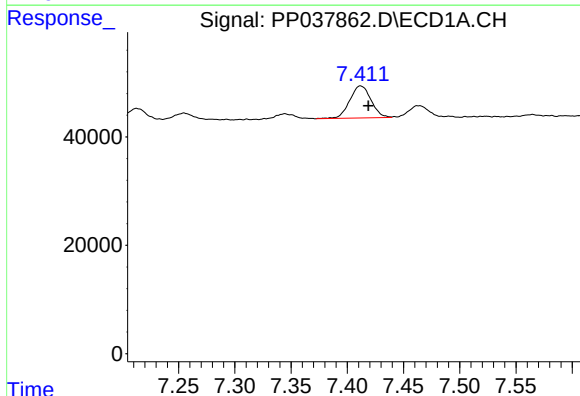


#27 AR-1254-2

R.T.: 7.412 min
Delta R.T.: -0.007 min
Response: 78176
Conc: 28.10 ng/ml

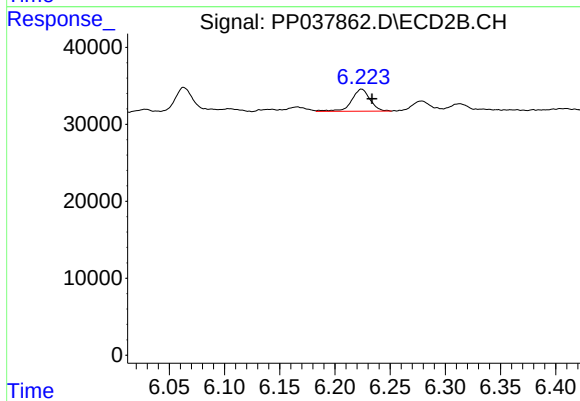

#27 AR-1254-2


R.T.: 6.224 min
Delta R.T.: -0.009 min
Response: 33249
Conc: 25.60 ng/ml

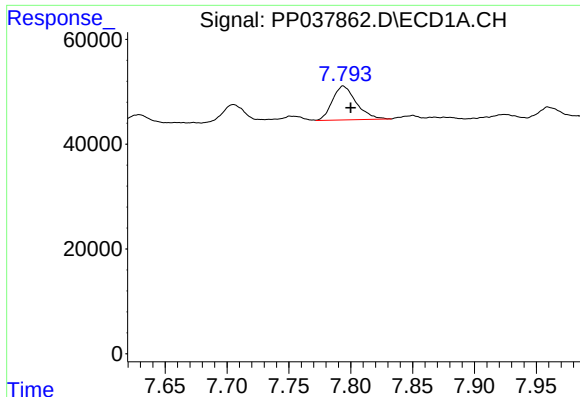

#28 AR-1254-3


R.T.: 7.794 min
Delta R.T.: -0.006 min
Response: 87015
Conc: 28.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

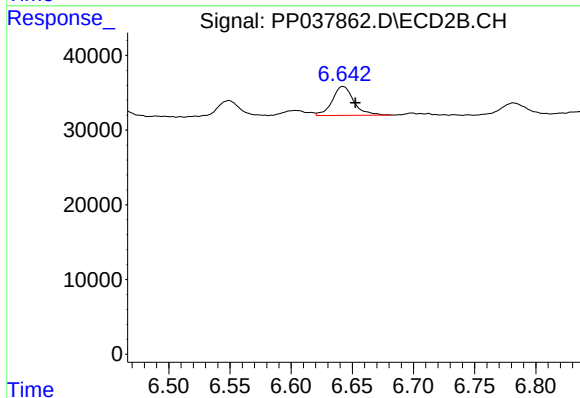


#28 AR-1254-3

R.T.: 6.642 min
Delta R.T.: -0.010 min
Response: 47883
Conc: 22.44 ng/ml

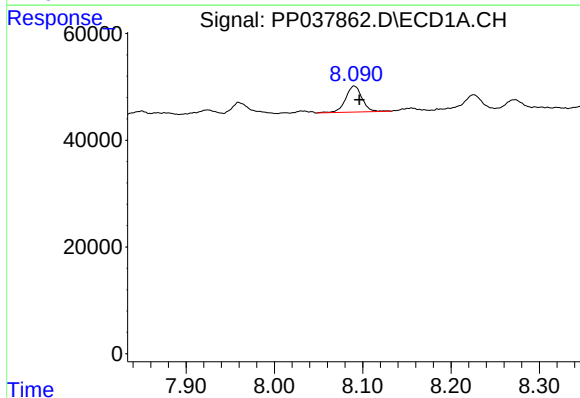


#29 AR-1254-4

R.T.: 8.090 min
Delta R.T.: -0.006 min
Response: 63831
Conc: 28.10 ng/ml

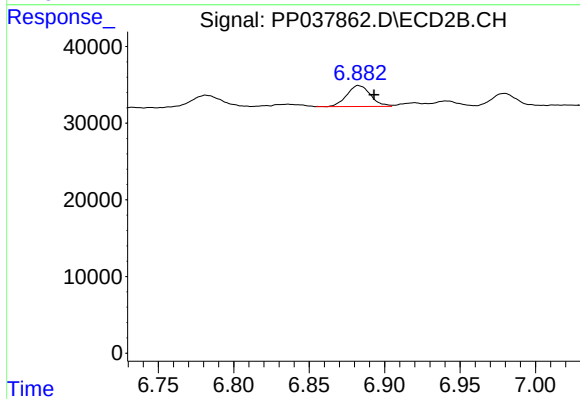

#29 AR-1254-4


R.T.: 6.882 min
Delta R.T.: -0.011 min
Response: 29784
Conc: 21.95 ng/ml

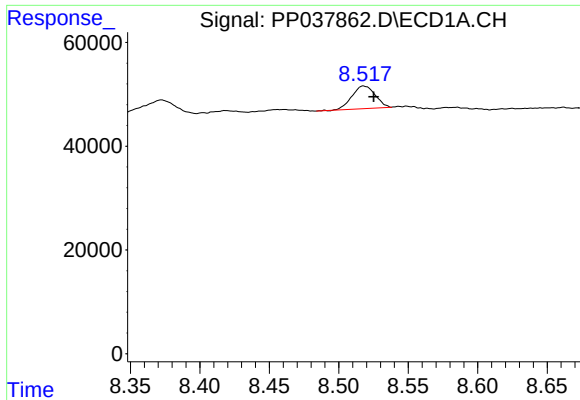

#30 AR-1254-5

R.T.: 8.518 min
Delta R.T.: -0.007 min
Response: 51081
Conc: 20.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

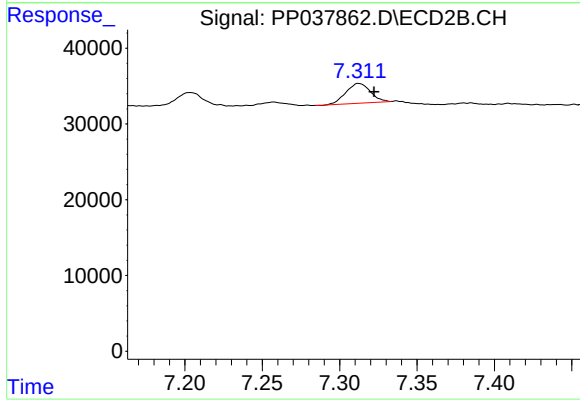

#30 AR-1254-5

R.T.: 7.312 min
Delta R.T.: -0.010 min
Response: 28756
Conc: 15.34 ng/ml