

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072921\
 Data File : PP037863.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2021 10:43
 Operator : DD\AJ
 Sample : M2940-09
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 16:35:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.953	3.944	911333	519148	20.052	18.972
2) SA Decachlor...	10.982	9.234	953689	519198	20.716	18.653
Target Compounds						
36) L8 AR-1262-1	8.592	7.310	78743	24014	27.036	23.126
37) L8 AR-1262-2	9.150	7.866	143874	75395	27.395	21.674
38) L8 AR-1262-3	9.463	8.153	71830	31003	18.747	22.020m
39) L8 AR-1262-4	9.557	8.216	49127	62308	16.719	23.398 #
40) L8 AR-1262-5	10.227	8.715	53804	27420	25.304	21.693



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072921\
Data File : PP037863.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2021 10:43
Operator : DD\AJ
Sample : M2940-09
Misc : AR1262 MDL 25 PPB
ALS Vial : 76 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 16:35:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

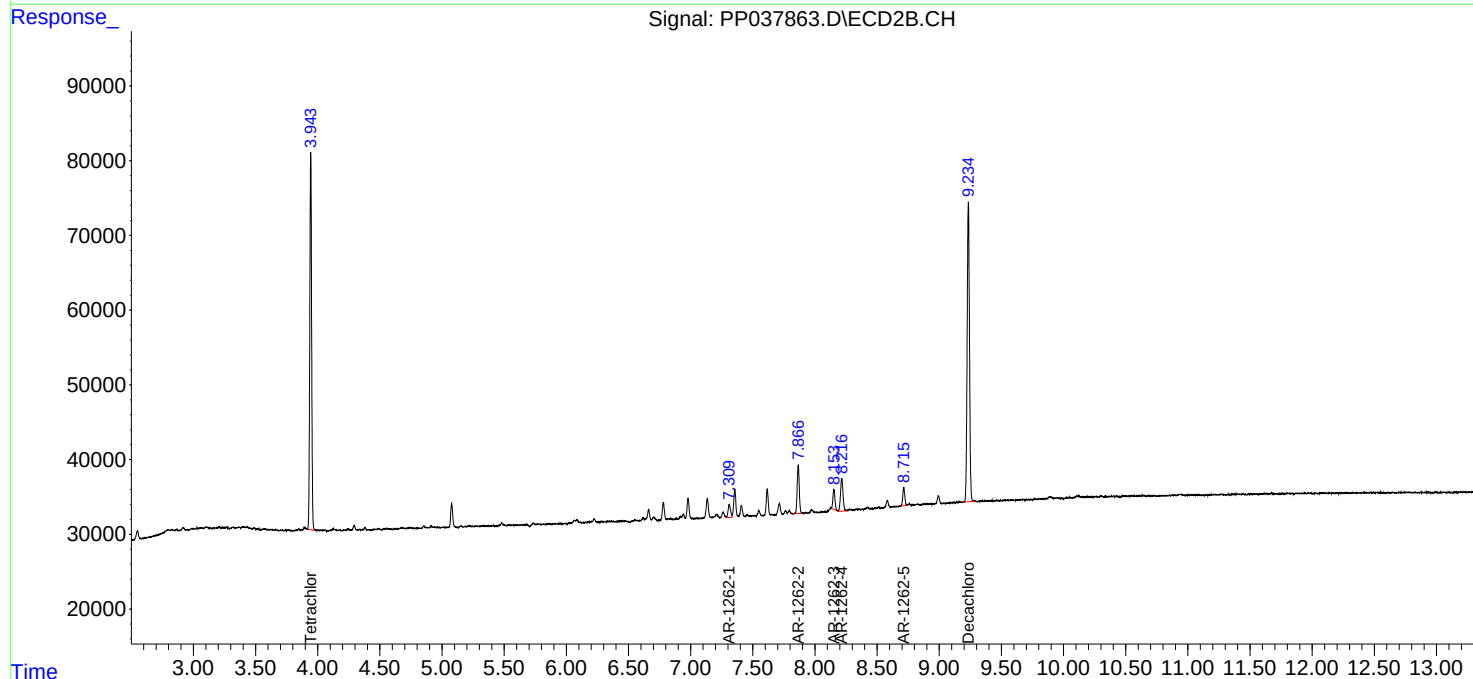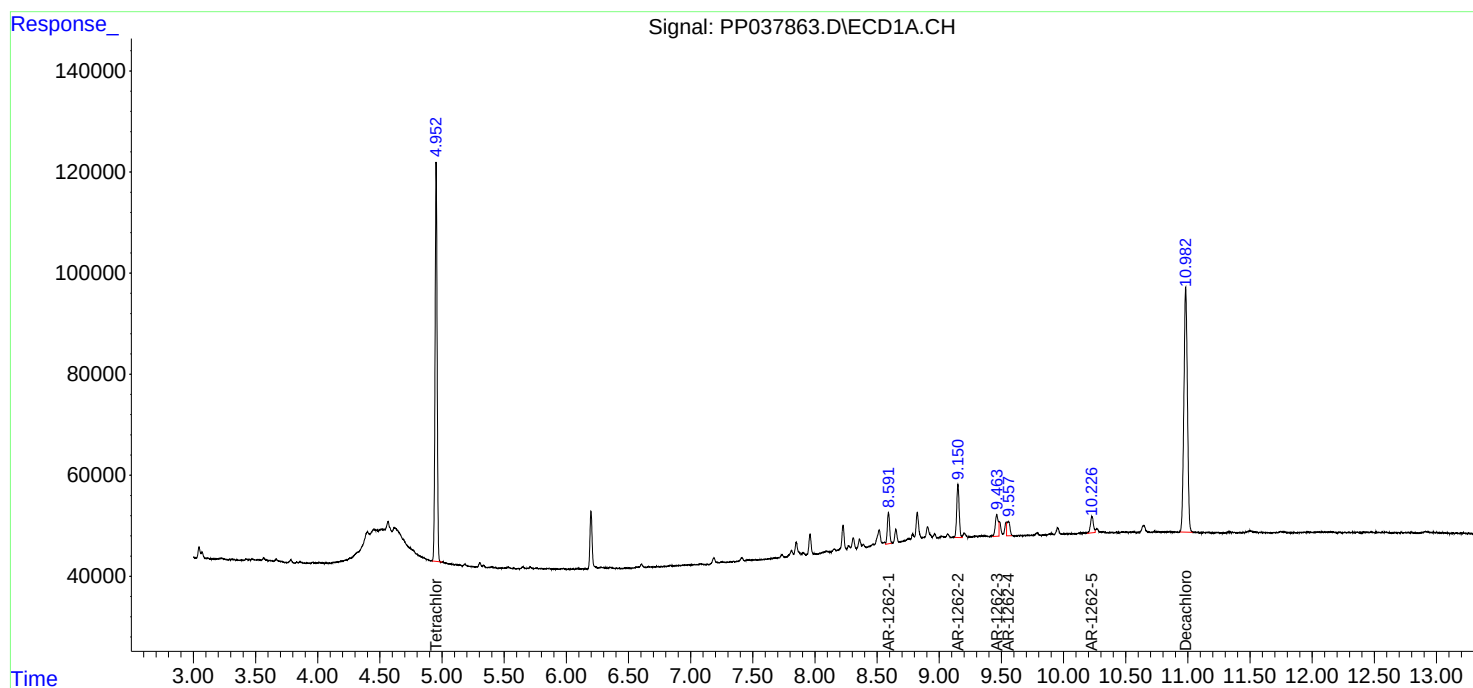


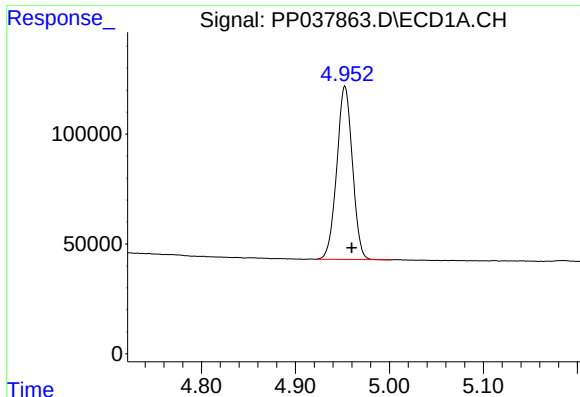

#1 Tetrachloro-m-xylene


R.T.: 4.953 min
Delta R.T.: -0.007 min
Response: 911333
Conc: 20.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

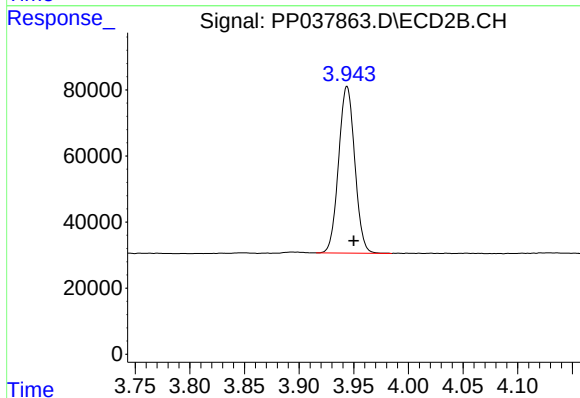


#1 Tetrachloro-m-xylene

R.T.: 3.944 min
Delta R.T.: -0.006 min
Response: 519148
Conc: 18.97 ng/ml

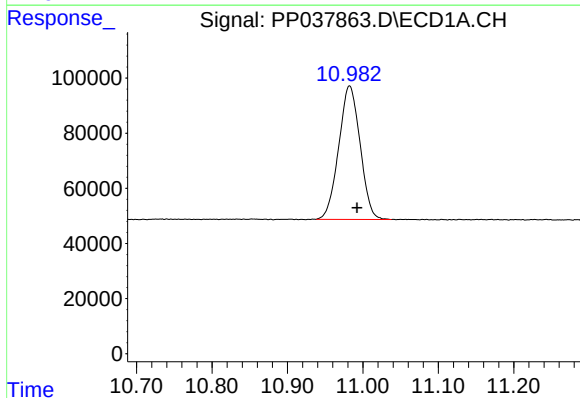


#2 Decachlorobiphenyl

R.T.: 10.982 min
Delta R.T.: -0.010 min
Response: 953689
Conc: 20.72 ng/ml

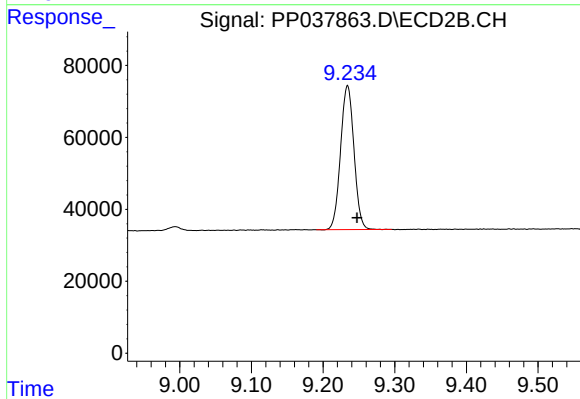

#2 Decachlorobiphenyl


R.T.: 9.234 min
Delta R.T.: -0.013 min
Response: 519198
Conc: 18.65 ng/ml

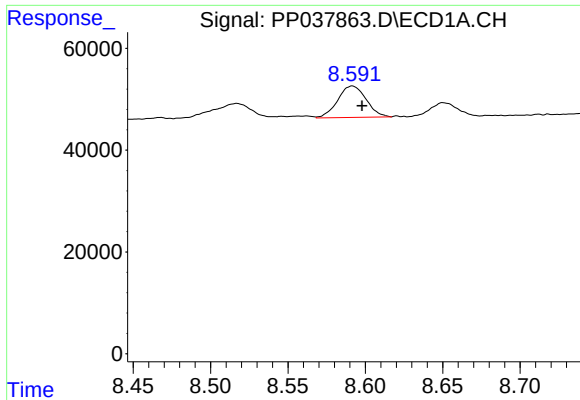

#36 AR-1262-1


R.T.: 8.592 min
Delta R.T.: -0.006 min
Response: 78743
Conc: 27.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

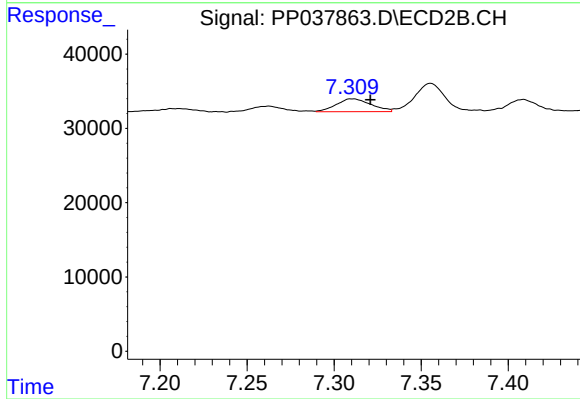


#36 AR-1262-1

R.T.: 7.310 min
Delta R.T.: -0.010 min
Response: 24014
Conc: 23.13 ng/ml

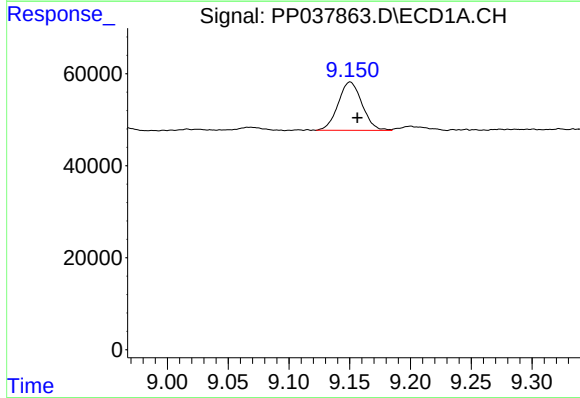


#37 AR-1262-2

R.T.: 9.150 min
Delta R.T.: -0.006 min
Response: 143874
Conc: 27.40 ng/ml

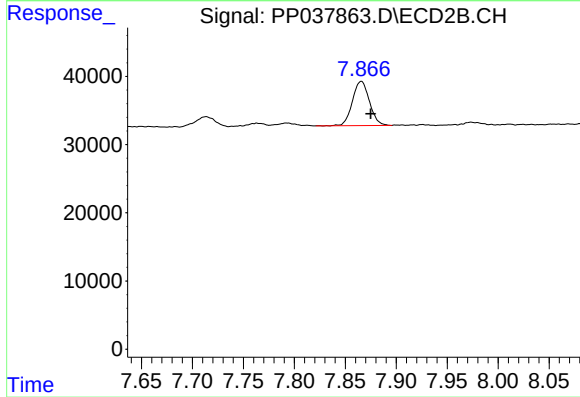

#37 AR-1262-2


R.T.: 7.866 min
Delta R.T.: -0.009 min
Response: 75395
Conc: 21.67 ng/ml

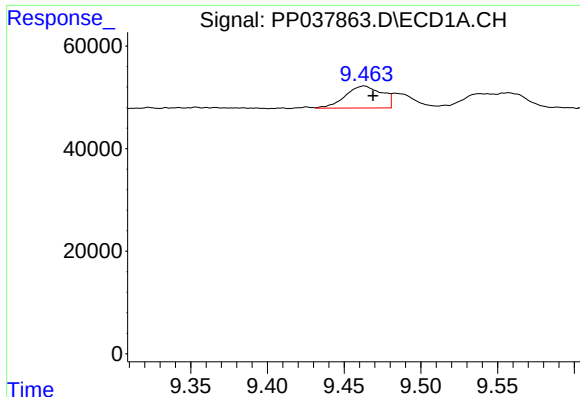

#38 AR-1262-3


R.T.: 9.463 min
Delta R.T.: -0.006 min
Response: 71830
Conc: 18.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

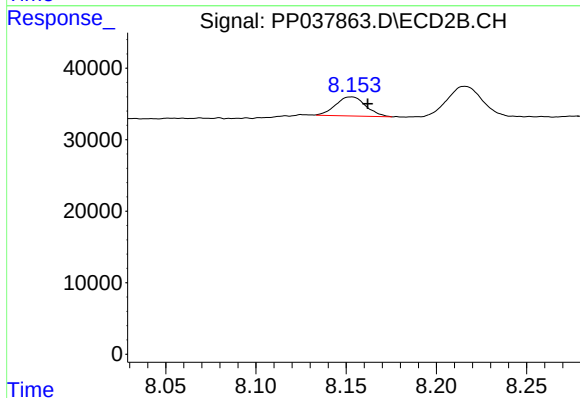


#38 AR-1262-3

R.T.: 8.153 min
Delta R.T.: -0.009 min
Response: 31003
Conc: 22.02 ng/ml m

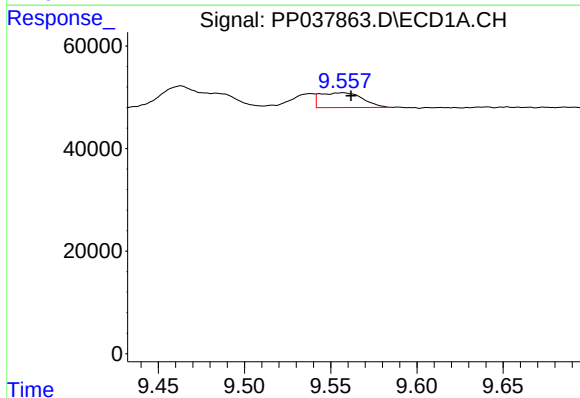


#39 AR-1262-4

R.T.: 9.557 min
Delta R.T.: -0.005 min
Response: 49127
Conc: 16.72 ng/ml

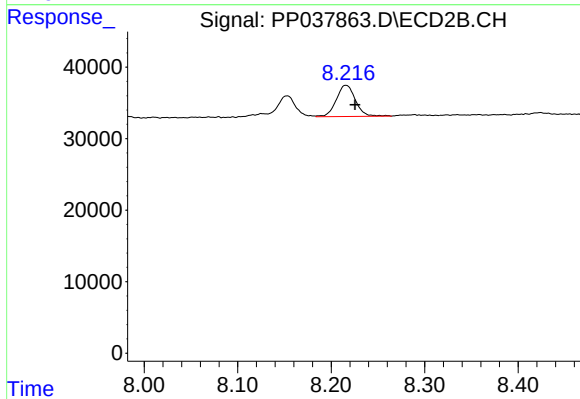

#39 AR-1262-4


R.T.: 8.216 min
Delta R.T.: -0.010 min
Response: 62308
Conc: 23.40 ng/ml

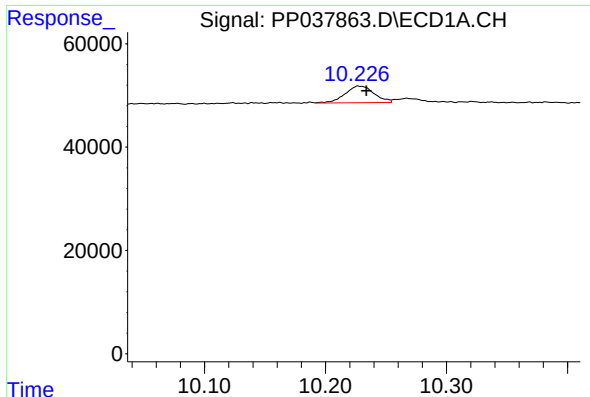

#40 AR-1262-5

R.T.: 10.227 min
Delta R.T.: -0.007 min
Response: 53804
Conc: 25.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2021

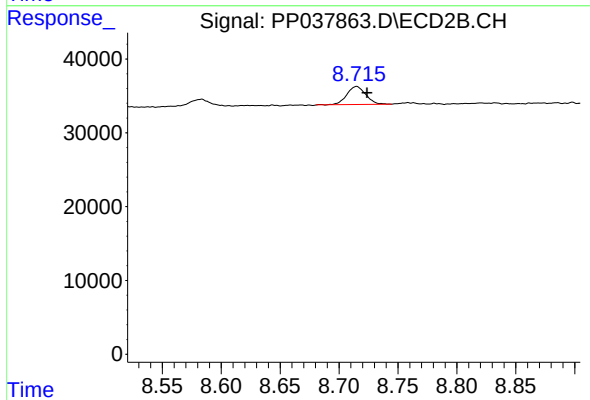

#40 AR-1262-5

R.T.: 8.715 min
Delta R.T.: -0.009 min
Response: 27420
Conc: 21.69 ng/ml