

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072922\
 Data File : PP049960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2022 09:48
 Operator : YP\AJ
 Sample : N3945-02DL 2X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S4-01-SDL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/01/2022
 Supervised By :Ankita Jodhani 08/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 13:09:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 14 06:08:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.350	3.598	22428504	42432006	15.456	17.359
2) SA Decachlor...	10.103	8.564	22085988	19610299	15.615	16.839
Target Compounds						
26) L6 AR-1254-1	6.383	5.465	7085628	12556675	112.504	99.003
27) L6 AR-1254-2	6.601	5.611	16176379	22754825	166.044	205.868
28) L6 AR-1254-3	6.974	6.013	25782906	43601723	249.536	267.866
29) L6 AR-1254-4	7.260	6.241	19432624	19999936	242.744	206.703
30) L6 AR-1254-5	7.683	6.656	46728171	216.8E6	525.732m	1636.092 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072922\
Data File : PP049960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2022 09:48
Operator : YP\AJ
Sample : N3945-02DL 2X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
S4-01-SDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2022
Supervised By :Ankita Jodhani 08/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 13:09:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 14 06:08:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

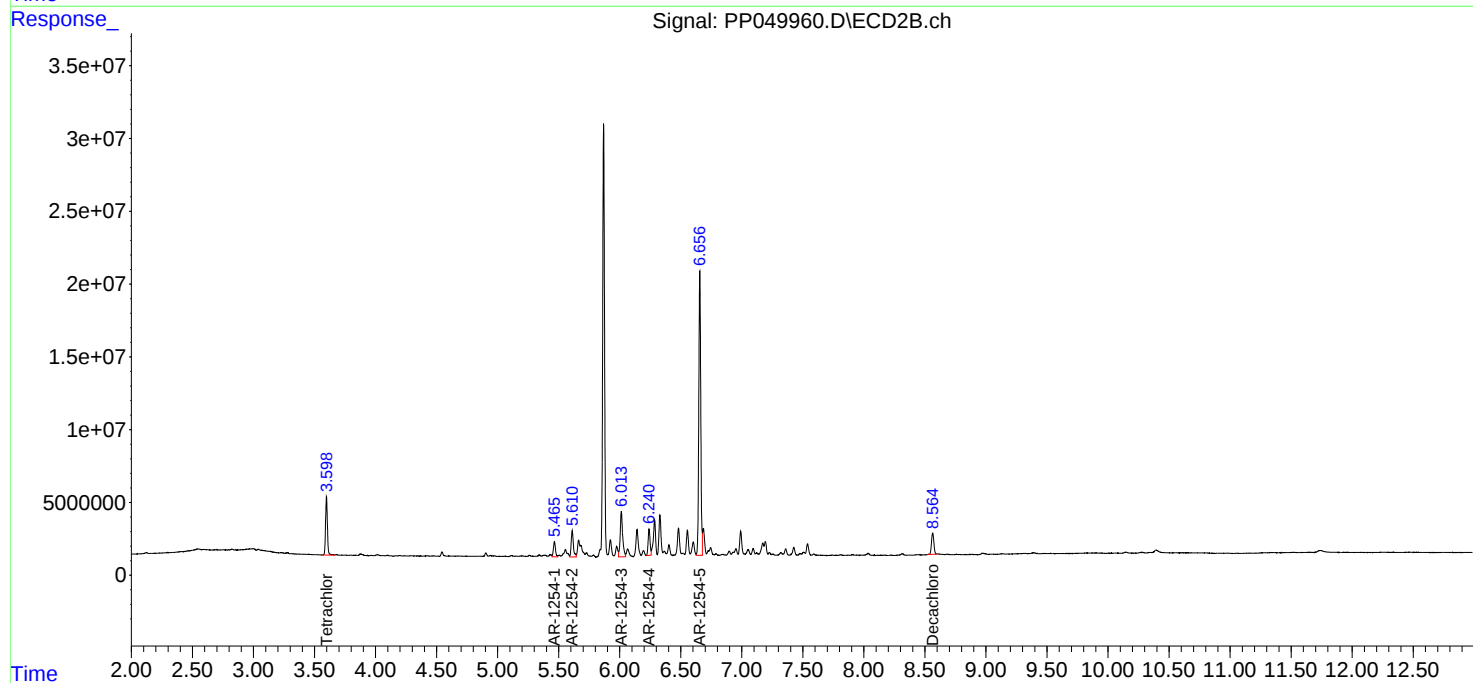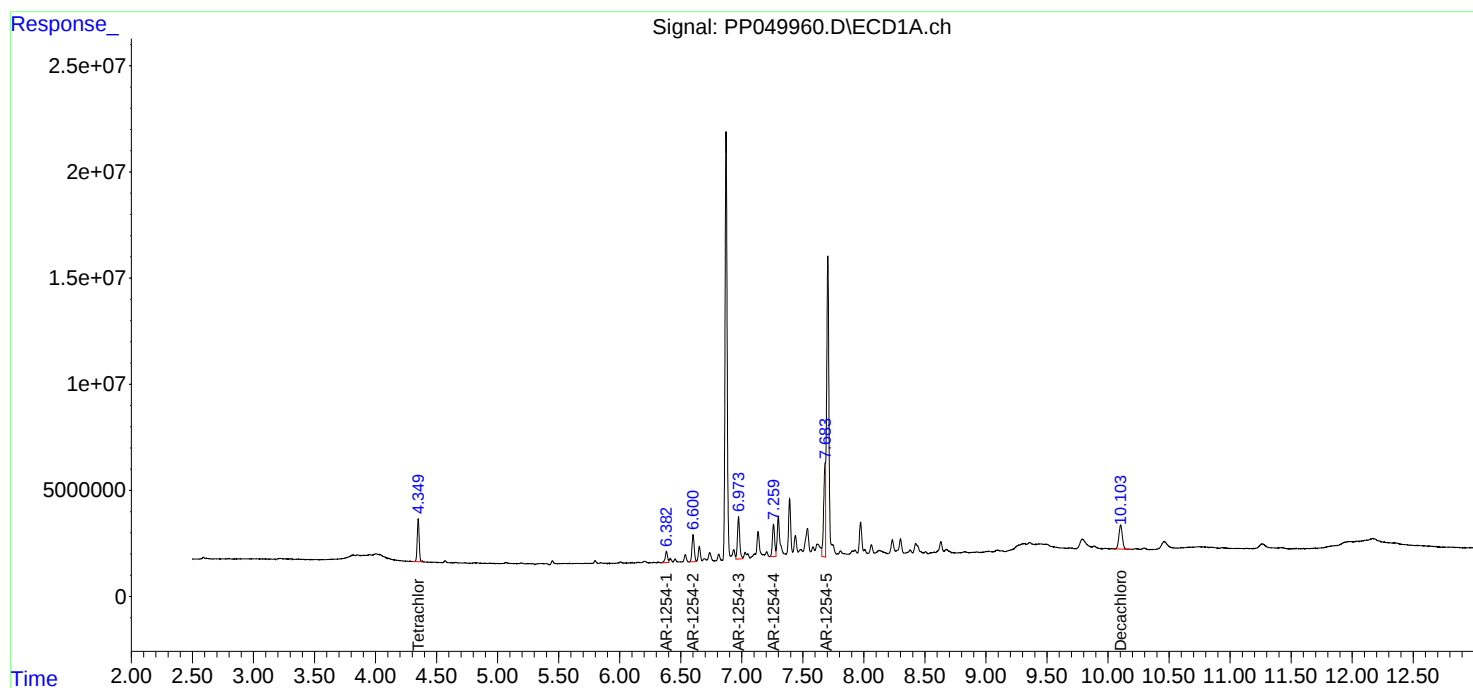

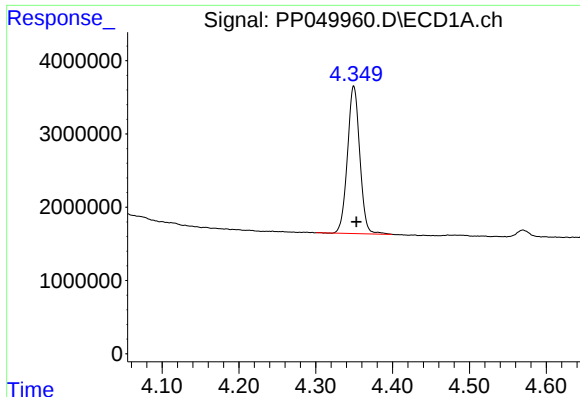


#1 Tetrachloro-m-xylene

R.T.: 4.350 min
Delta R.T.: -0.003 min
Response: 22428504
Conc: 15.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
S4-01-SDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2022
Supervised By :Ankita Jodhani 08/01/2022

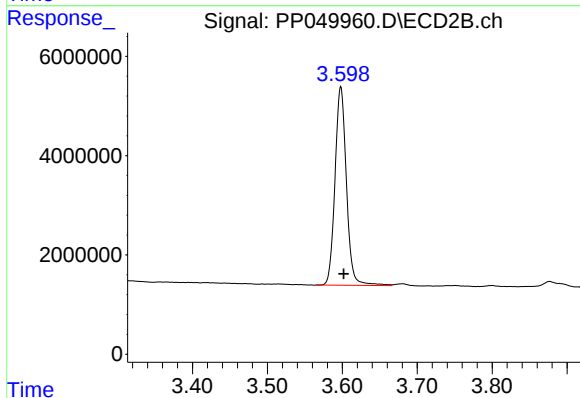


#1 Tetrachloro-m-xylene

R.T.: 3.598 min
Delta R.T.: -0.004 min
Response: 42432006
Conc: 17.36 ng/ml

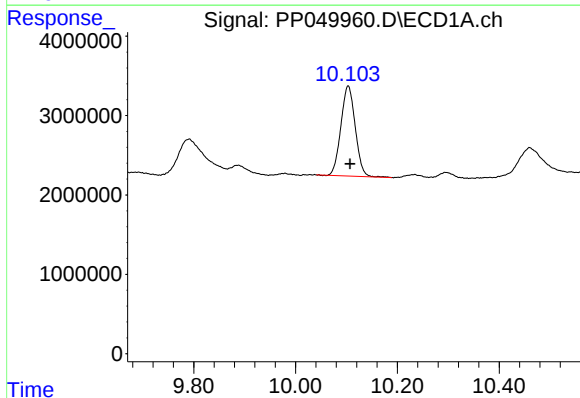


#2 Decachlorobiphenyl

R.T.: 10.103 min
Delta R.T.: -0.004 min
Response: 22085988
Conc: 15.61 ng/ml

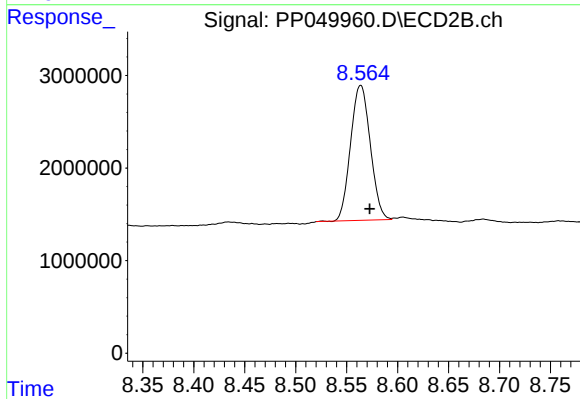

#2 Decachlorobiphenyl

R.T.: 8.564 min
Delta R.T.: -0.009 min
Response: 19610299
Conc: 16.84 ng/ml

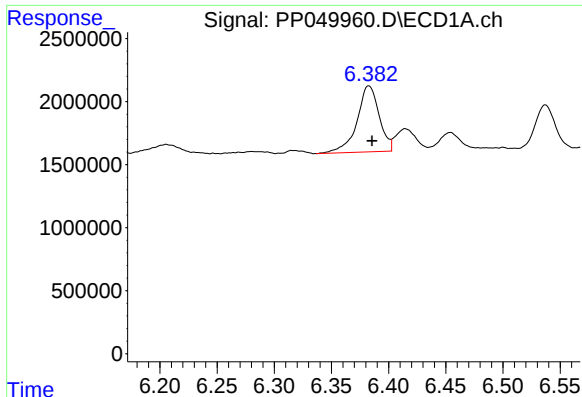


#26 AR-1254-1

R.T.: 6.383 min
Delta R.T.: -0.003 min
Response: 7085628
Conc: 112.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
S4-01-SDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2022
Supervised By :Ankita Jodhani 08/01/2022

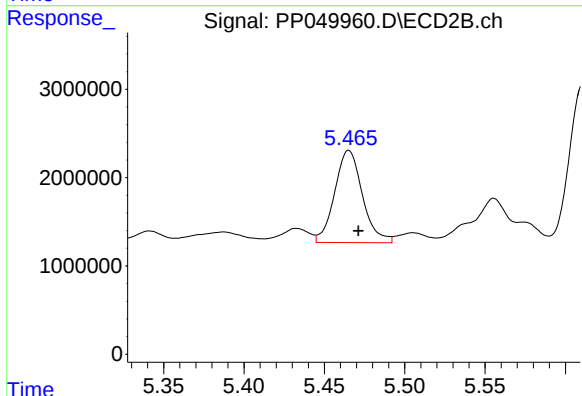


#26 AR-1254-1

R.T.: 5.465 min
Delta R.T.: -0.006 min
Response: 12556675
Conc: 99.00 ng/ml

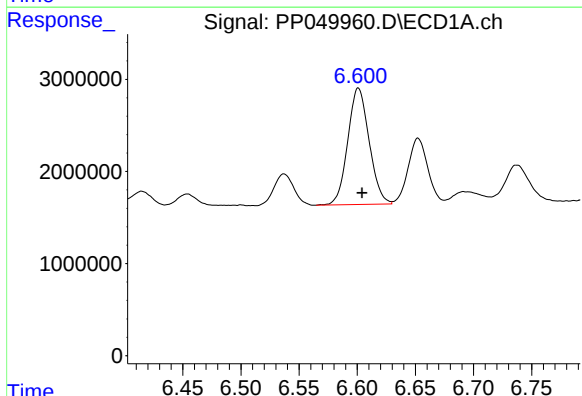


#27 AR-1254-2

R.T.: 6.601 min
Delta R.T.: -0.003 min
Response: 16176379
Conc: 166.04 ng/ml

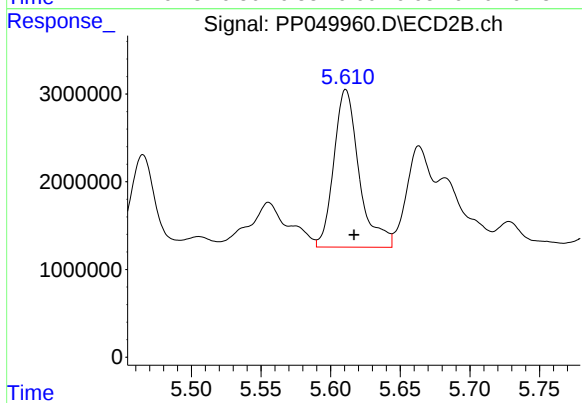

#27 AR-1254-2

R.T.: 5.611 min
Delta R.T.: -0.006 min
Response: 22754825
Conc: 205.87 ng/ml

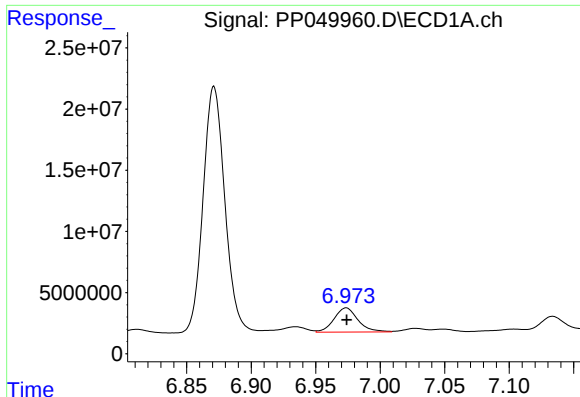


#28 AR-1254-3

R.T.: 6.974 min
Delta R.T.: 0.000 min
Response: 25782906
Conc: 249.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
S4-01-SDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2022
Supervised By :Ankita Jodhani 08/01/2022

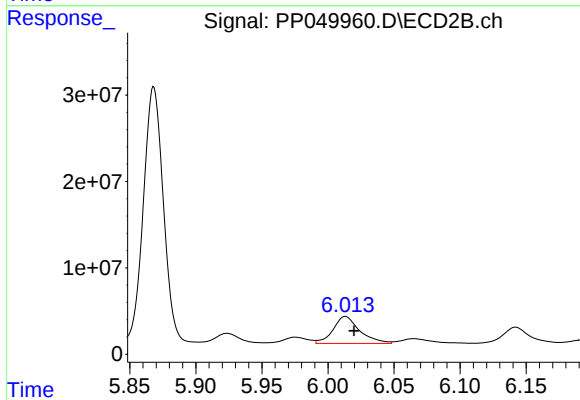


#28 AR-1254-3

R.T.: 6.013 min
Delta R.T.: -0.006 min
Response: 43601723
Conc: 267.87 ng/ml

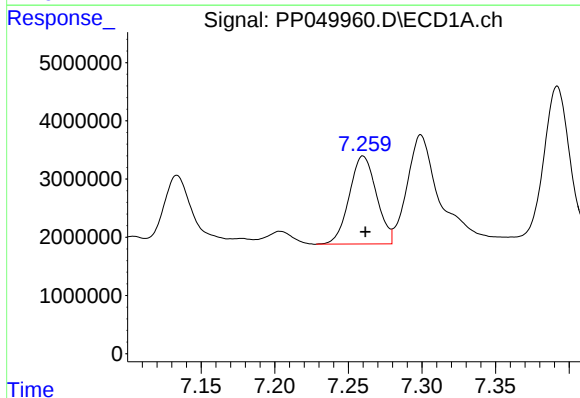


#29 AR-1254-4

R.T.: 7.260 min
Delta R.T.: -0.001 min
Response: 19432624
Conc: 242.74 ng/ml

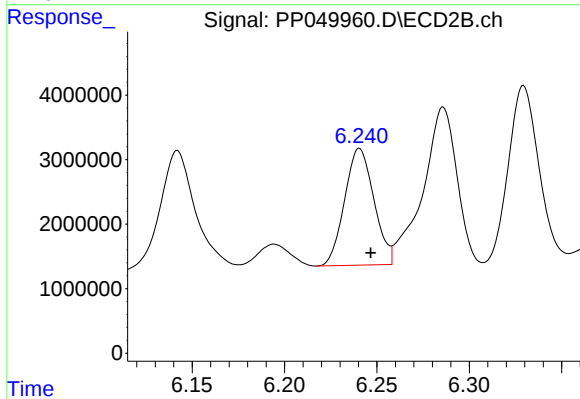

#29 AR-1254-4

R.T.: 6.241 min
Delta R.T.: -0.006 min
Response: 19999936
Conc: 206.70 ng/ml

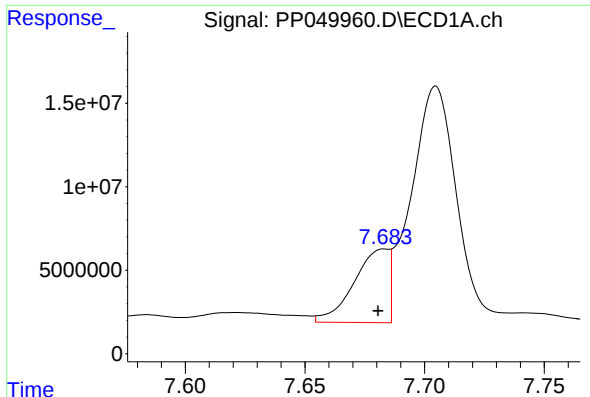


#30 AR-1254-5

R.T.: 7.683 min
Delta R.T.: 0.002 min
Response: 46728171
Conc: 525.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
S4-01-SDL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2022
Supervised By :Ankita Jodhani 08/01/2022

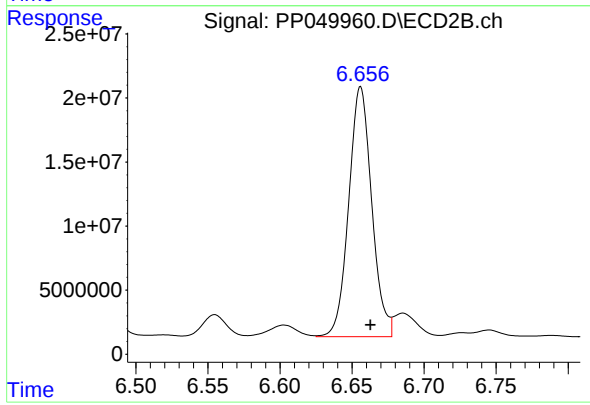

#30 AR-1254-5

R.T.: 6.656 min
Delta R.T.: -0.007 min
Response: 216807658
Conc: 1636.09 ng/ml