

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072922\
 Data File : PP049970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2022 14:55
 Operator : YP\AJ
 Sample : N3969-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CHAMBERS-STREET-A3-9065X-MH

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/01/2022
 Supervised By :Ankita Jodhani 08/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 16:27:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 14 06:08:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.351	3.601	20571868	41470427	14.176m	16.966
2) SA Decachlor...	10.103	8.566	14895899	15614012	10.532m	13.407 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072922\
Data File : PP049970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2022 14:55
Operator : YP\AJ
Sample : N3969-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CHAMBERS-STREET-A3-9065X-MH


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2022
Supervised By :Ankita Jodhani 08/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 16:27:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 14 06:08:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

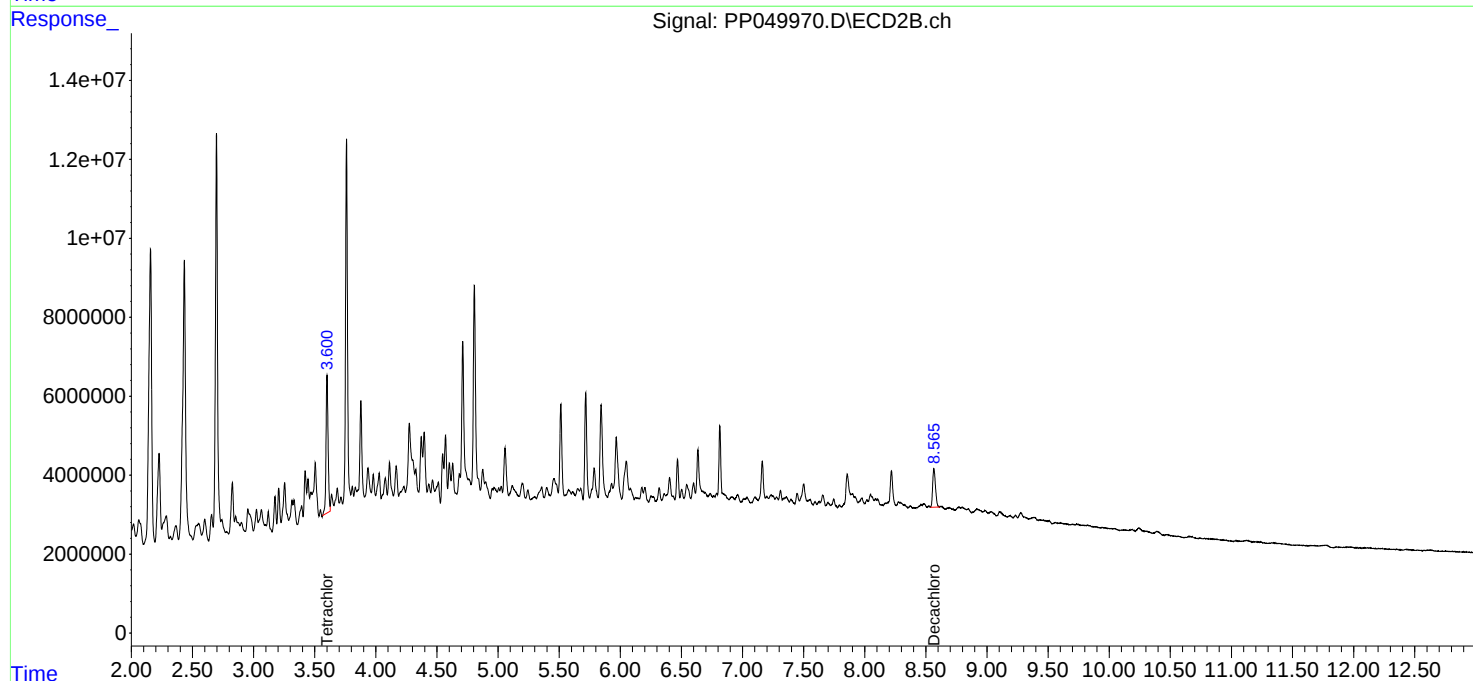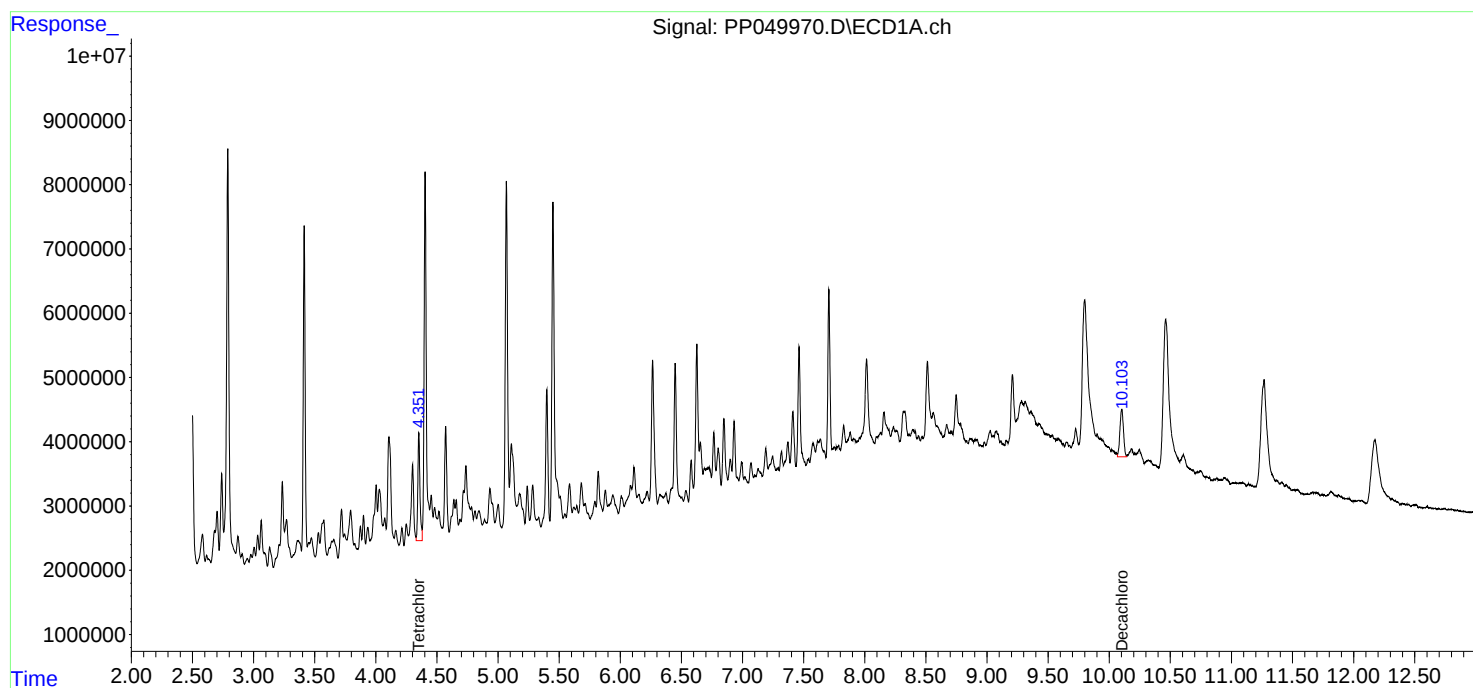

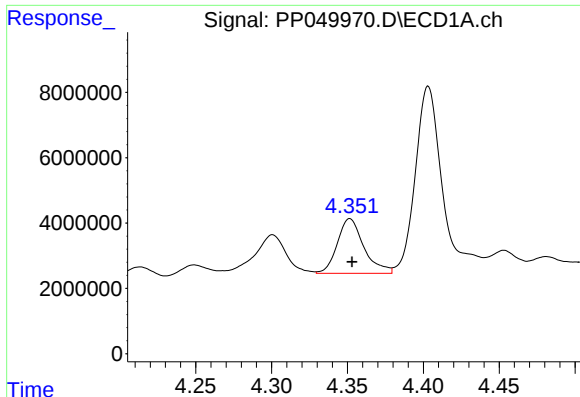


#1 Tetrachloro-m-xylene

R.T.: 4.351 min
Delta R.T.: -0.002 min
Response: 20571868
Conc: 14.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHAMBERS-STREET-A3-9065X-MH


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2022
Supervised By :Ankita Jodhani 08/01/2022

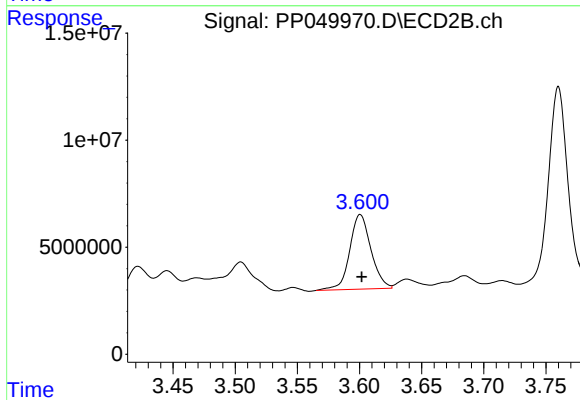


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: -0.001 min
Response: 41470427
Conc: 16.97 ng/ml

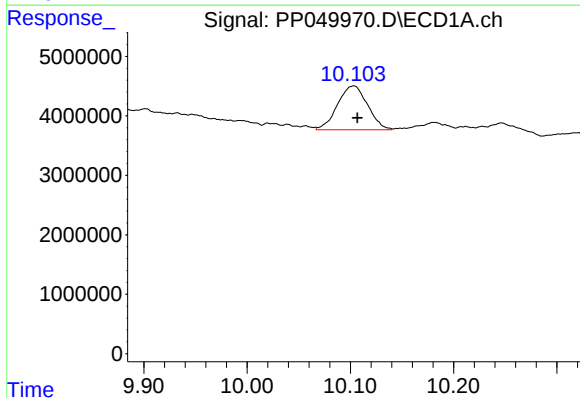

#2 Decachlorobiphenyl

R.T.: 10.103 min
Delta R.T.: -0.004 min
Response: 14895899
Conc: 10.53 ng/ml m

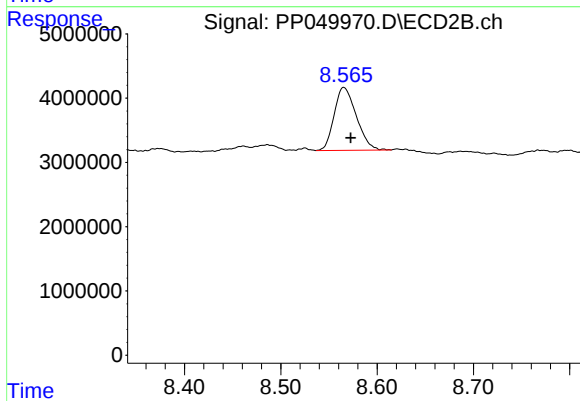

#2 Decachlorobiphenyl

R.T.: 8.566 min
Delta R.T.: -0.007 min
Response: 15614012
Conc: 13.41 ng/ml