

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072922\
 Data File : PP049983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2022 19:00
 Operator : YP\AJ
 Sample : N3935-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RVE-132

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/01/2022
 Supervised By :Ankita Jodhani 08/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:47:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 14 06:08:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.352	3.601	29764626	56817059	20.511	23.244
2) SA Decachlor...	10.102	8.565	27147775	23550528	19.194m	20.222

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072922\
Data File : PP049983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2022 19:00
Operator : YP\AJ
Sample : N3935-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
RVE-132


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2022
Supervised By :Ankita Jodhani 08/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 01:47:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 14 06:08:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

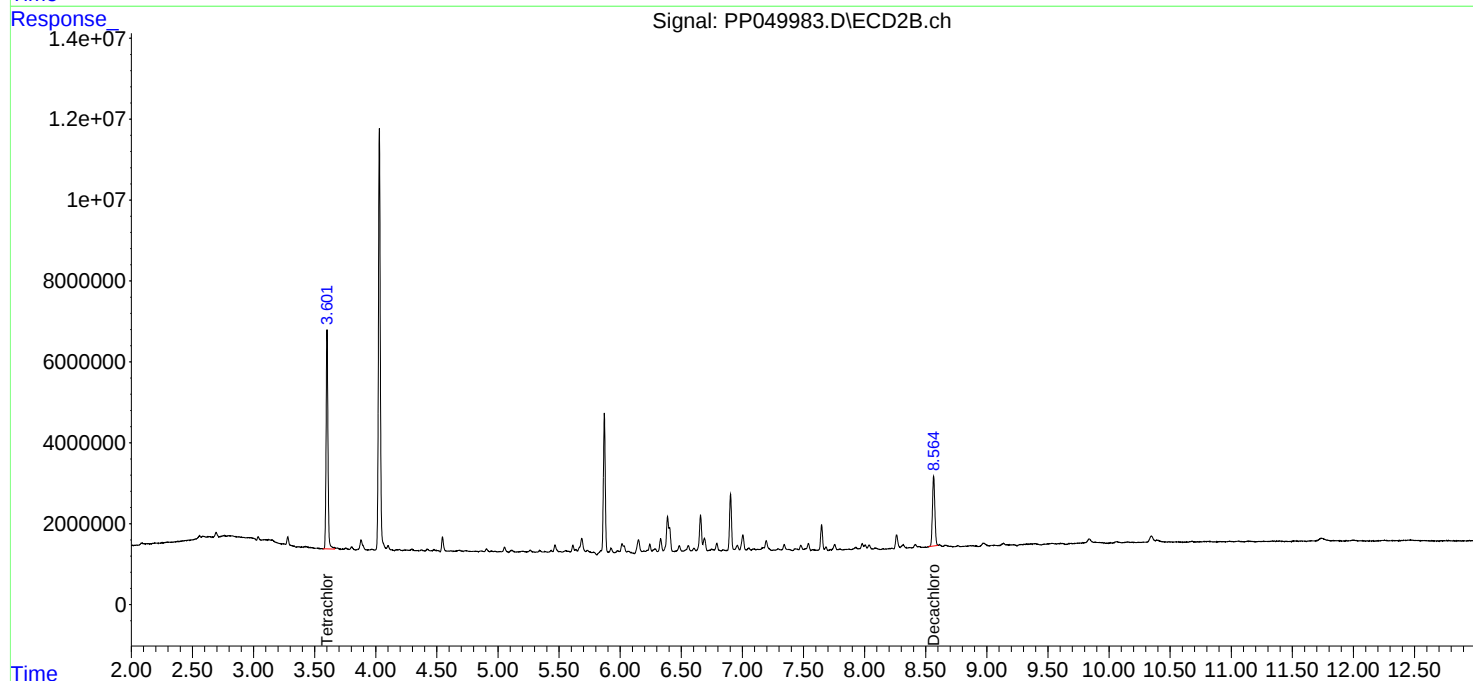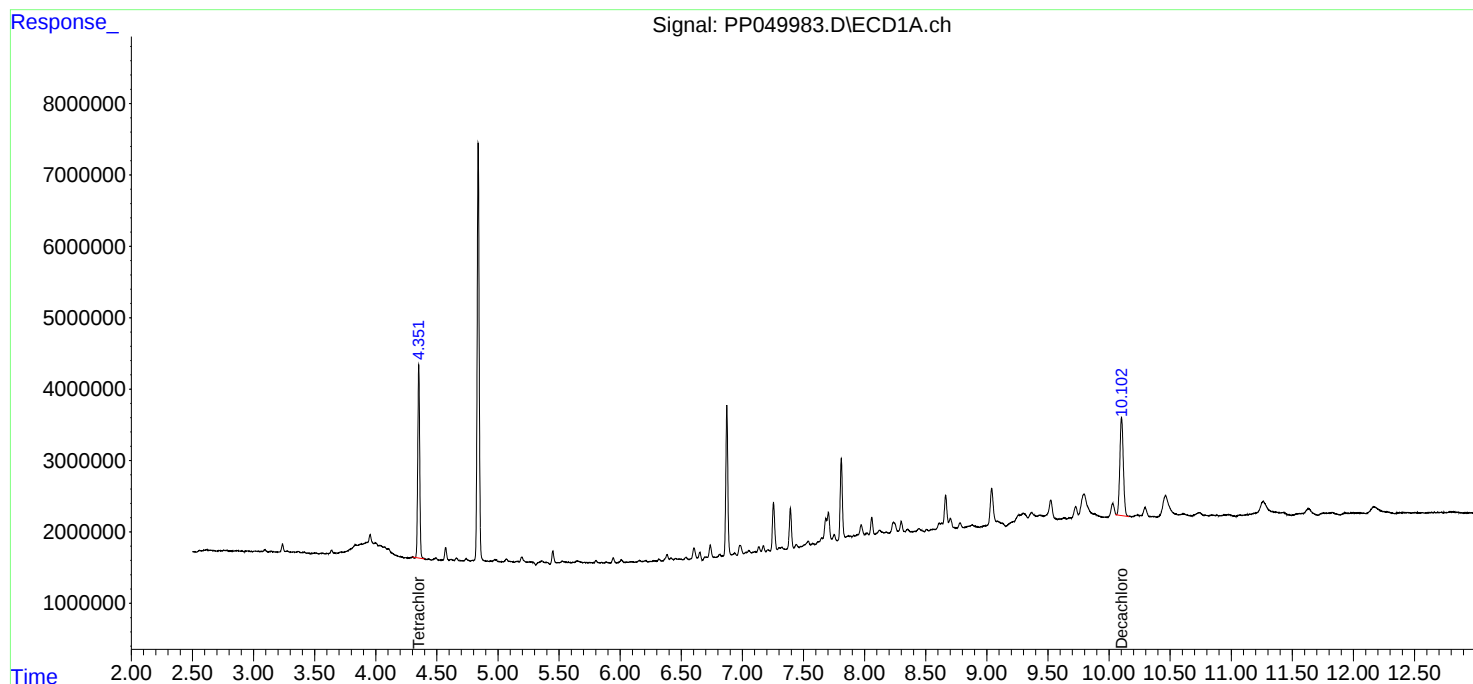

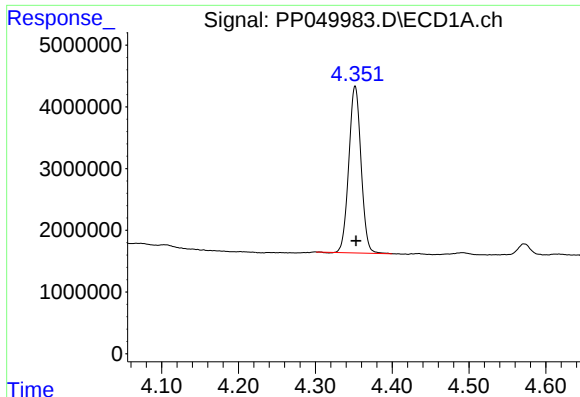


#1 Tetrachloro-m-xylene

R.T.: 4.352 min
Delta R.T.: -0.001 min
Response: 29764626
Conc: 20.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
RVE-132


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2022
Supervised By :Ankita Jodhani 08/01/2022

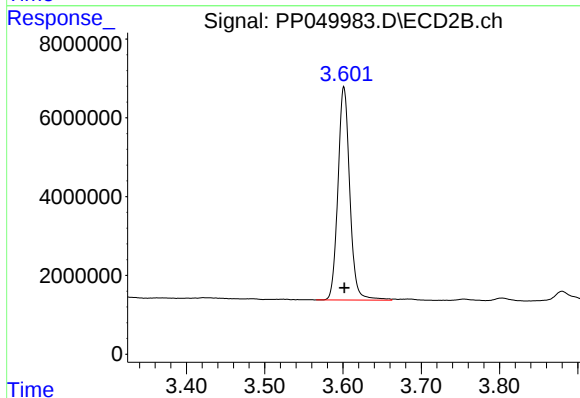


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: 0.000 min
Response: 56817059
Conc: 23.24 ng/ml

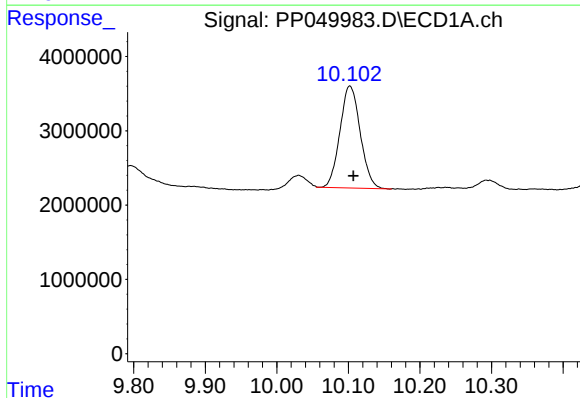

#2 Decachlorobiphenyl

R.T.: 10.102 min
Delta R.T.: -0.005 min
Response: 27147775
Conc: 19.19 ng/ml m

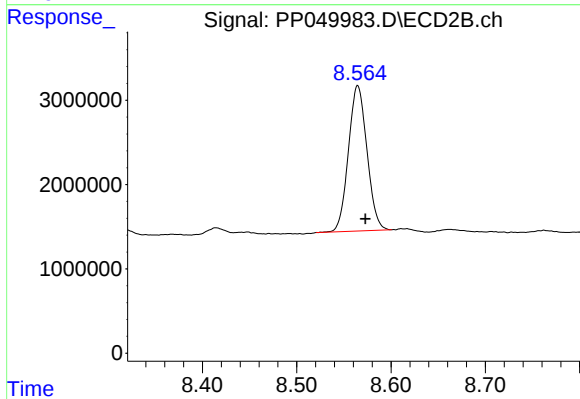

#2 Decachlorobiphenyl

R.T.: 8.565 min
Delta R.T.: -0.008 min
Response: 23550528
Conc: 20.22 ng/ml