

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072925\
 Data File : PP074093.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2025 10:11
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:45:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 28 18:16:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.896	0	104517	N.D.	0.011 #
2)	SA Decachlor...	10.587	9.026	96154	982565	0.143	0.086 #
Target Compounds							
3)	L1 AR-1016-1	5.857	5.021	79218	481884	2.155	0.567 #
4)	L1 AR-1016-2	5.891	5.075	63626	581787	1.167	1.551 #
5)	L1 AR-1016-3	5.947	5.194	72545	142511	2.092	0.647 #
6)	L1 AR-1016-4	6.047	5.242	34269	557986	1.237	2.669 #
7)	L1 AR-1016-5	6.316	5.456	42418	933896	1.577	4.050 #
8)	L2 AR-1221-1	0.000	4.120	0	531320	N.D.	4.745 #
9)	L2 AR-1221-2	0.000	4.192	0	336618	N.D.	4.396 #
10)	L2 AR-1221-3	0.000	4.271	0	207727	N.D.	0.722 #
11)	L3 AR-1232-1	0.000	4.271	0	207727	N.D.	0.914 #
12)	L3 AR-1232-2	5.593	5.021	100233	481884	7.210	1.585 #
13)	L3 AR-1232-3	5.891	5.194	63626	142511	2.341	1.387 #
14)	L3 AR-1232-4	6.047	5.279	34269	754888	2.467	7.155 #
15)	L3 AR-1232-5	6.103	5.456	38557	933896	3.946	9.674 #
16)	L4 AR-1242-1	5.857	5.006	79218	198785	2.400	0.248 #
17)	L4 AR-1242-2	5.891	5.060	63626	1509419	1.316	4.410 #
18)	L4 AR-1242-3	5.947	5.189	72545	230621	2.381	1.168 #
19)	L4 AR-1242-4	6.047	5.279	34269	754888	1.416	3.136 #
20)	L4 AR-1242-5	6.821f	5.804	2411423	316252	78.863	1.107 #
21)	L5 AR-1248-1	5.857	5.006	79218	198785	2.941	0.397 #
22)	L5 AR-1248-2	6.103f	5.224	38557	142766	1.035	0.459 #
23)	L5 AR-1248-3	6.368	5.279	150599	754888	3.662	2.179 #
24)	L5 AR-1248-4	6.707f	5.456	1111738	933896	23.755	2.603 #
25)	L5 AR-1248-5	6.821	5.848	2411423	398144	44.922	0.665 #
26)	L6 AR-1254-1	6.707	5.809	1111738	198796	22.133	0.283 #
27)	L6 AR-1254-2	6.944	5.976	2888248	22998834	41.211	42.936
28)	L6 AR-1254-3	7.313	6.371	2908312	36508648	39.807	41.715
29)	L6 AR-1254-4	7.606	6.596	746738	122794	14.304	0.181 #
30)	L6 AR-1254-5	8.031f	7.009	416.2E6	6341.4E6	6888.559	7918.197
31)	L7 AR-1260-1	7.481	6.683	146810	6942734	3.415	8.857 #
32)	L7 AR-1260-2	7.716	6.886f	512.3E6	19388572	9358.960	25.523 #
33)	L7 AR-1260-3	8.031f	7.009f	416.2E6	6341.4E6	10966.040	7980.959 #
34)	L7 AR-1260-4	8.328	7.318	140518	283702	2.938	0.494 #
35)	L7 AR-1260-5	8.625	7.561	86599	566554	1.015	0.364 #
36)	L8 AR-1262-1	8.328	7.009f	140518	6341.4E6	2.265	5358.760 #
37)	L8 AR-1262-2	8.625	7.318	86599	283702	0.783	0.338 #
38)	L8 AR-1262-3	9.001	7.838	100443	977172	1.306	1.266
39)	L8 AR-1262-4	9.065	7.902	18760	1499122	0.327	1.064 #
40)	L8 AR-1262-5	9.789	8.410	33523	702370	0.861	1.117 #
41)	L9 AR-1268-1	9.001	7.838	100443	977172	0.785	0.437 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072925\
 Data File : PP074093.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2025 10:11
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:45:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 28 18:16:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	9.081	7.902	13427	1499122	0.115	0.693 #
43) L9	AR-1268-3	9.349	8.122	286601	954495	2.962	0.595 #
44) L9	AR-1268-4	9.789	8.410	33523	702370	0.772	1.059 #
45) L9	AR-1268-5	10.226	8.730	145412	932249	0.506	0.185 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072925\
Data File : PP074093.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2025 10:11
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 01:45:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 28 18:16:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

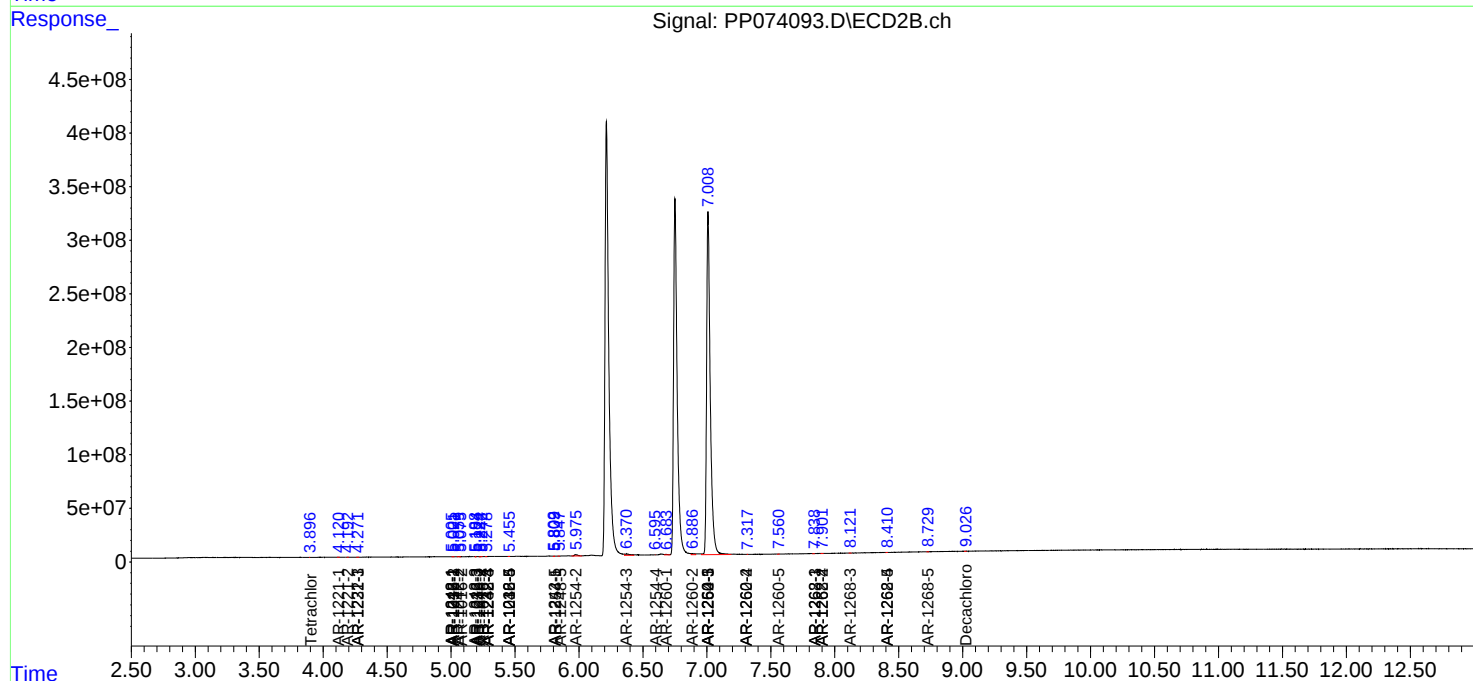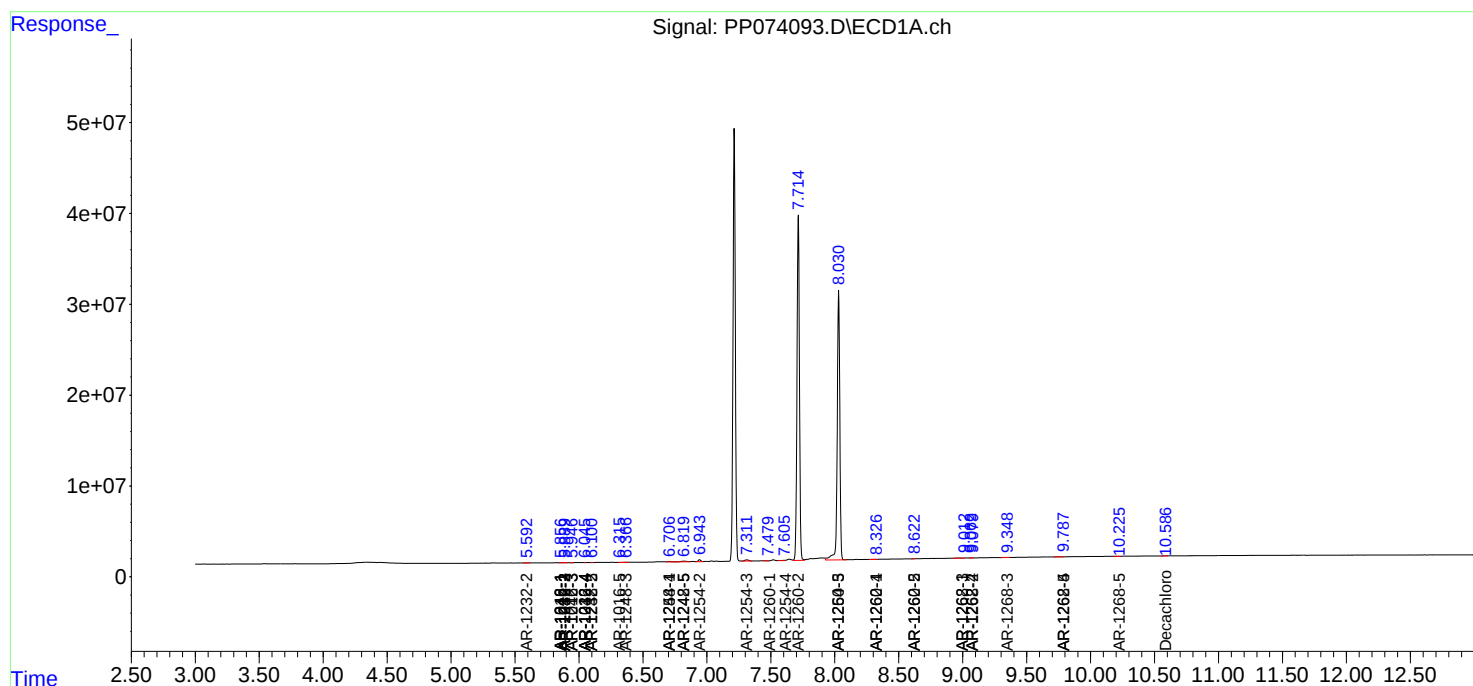


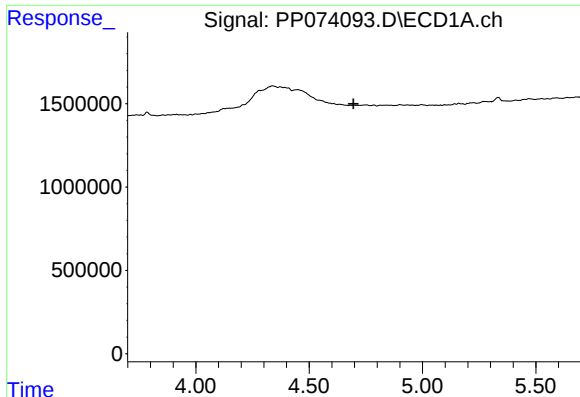

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 4.696 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

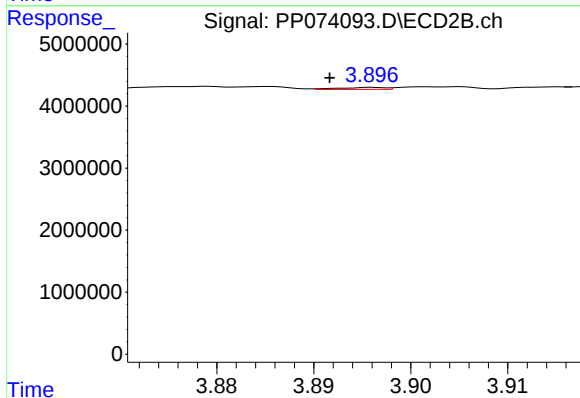


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.005 min
Response: 104517
Conc: 0.01 ng/ml

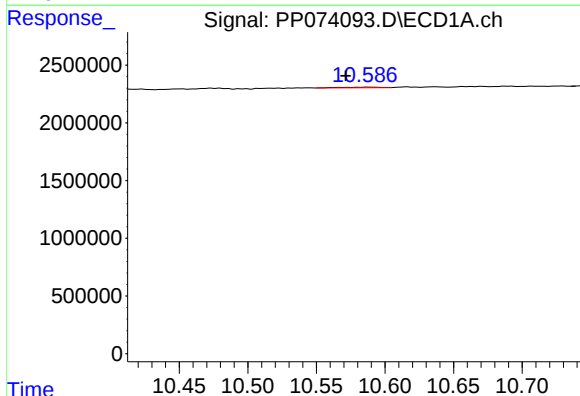


#2 Decachlorobiphenyl

R.T.: 10.587 min
Delta R.T.: 0.016 min
Response: 96154
Conc: 0.14 ng/ml

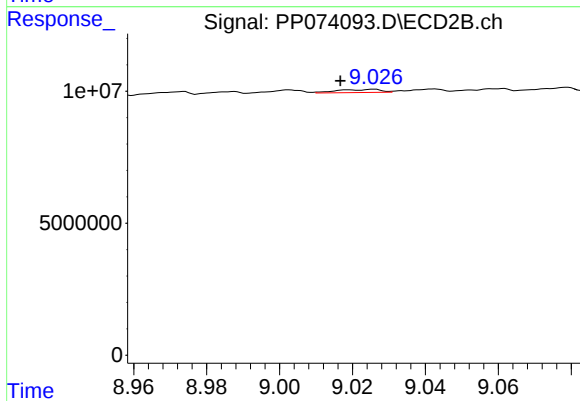

#2 Decachlorobiphenyl


R.T.: 9.026 min
Delta R.T.: 0.009 min
Response: 982565
Conc: 0.09 ng/ml

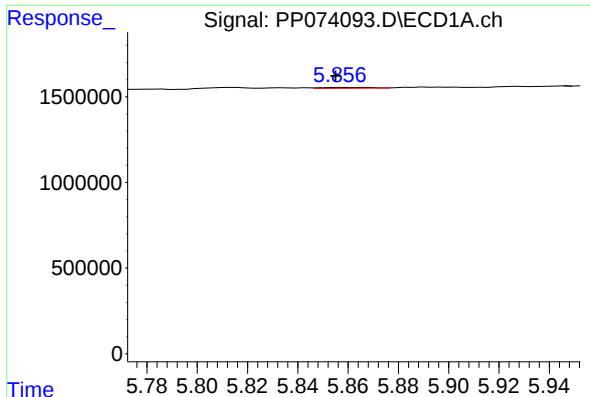

#3 AR-1016-1


R.T.: 5.857 min
Delta R.T.: 0.002 min
Response: 79218
Conc: 2.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

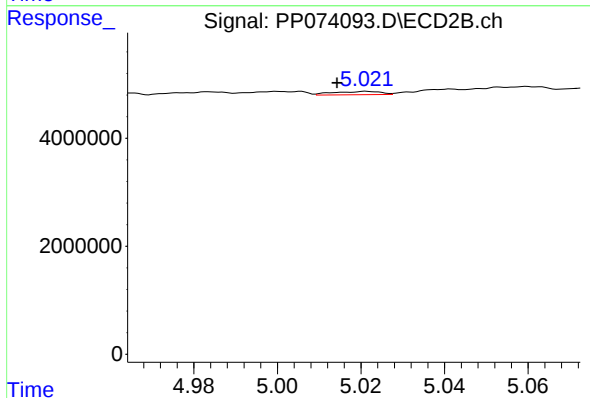


#3 AR-1016-1

R.T.: 5.021 min
Delta R.T.: 0.007 min
Response: 481884
Conc: 0.57 ng/ml

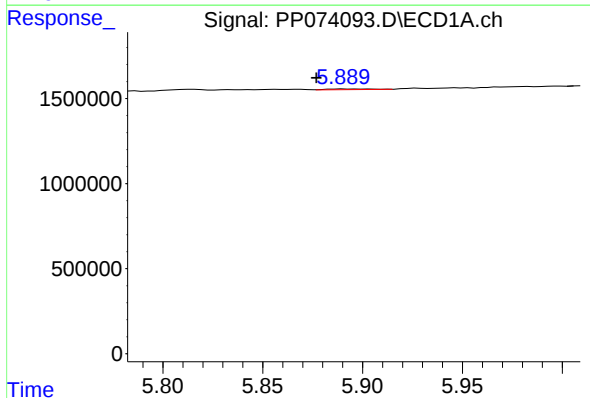


#4 AR-1016-2

R.T.: 5.891 min
Delta R.T.: 0.014 min
Response: 63626
Conc: 1.17 ng/ml

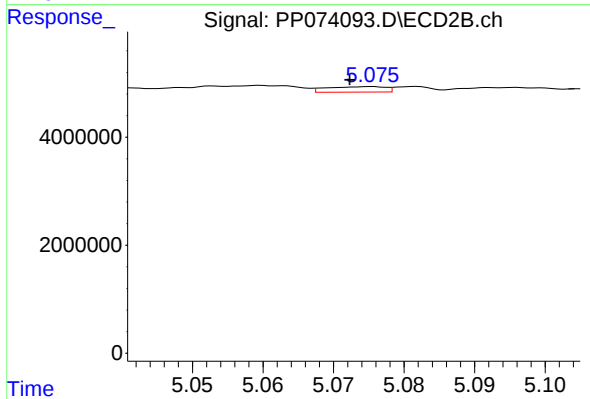

#4 AR-1016-2


R.T.: 5.075 min
Delta R.T.: 0.003 min
Response: 581787
Conc: 1.55 ng/ml

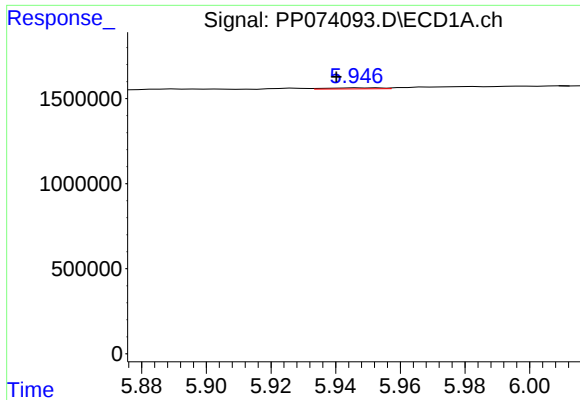

#5 AR-1016-3


R.T.: 5.947 min
Delta R.T.: 0.007 min
Response: 72545
Conc: 2.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

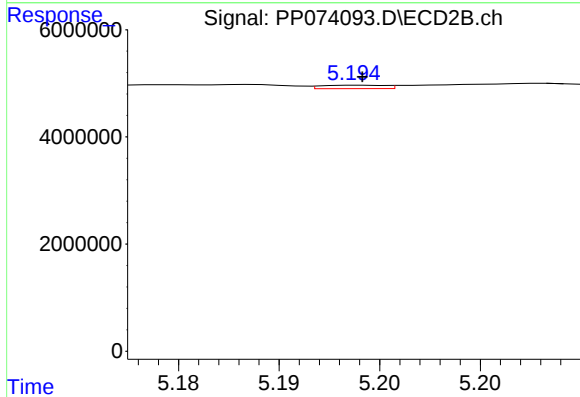


#5 AR-1016-3

R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 142511
Conc: 0.65 ng/ml

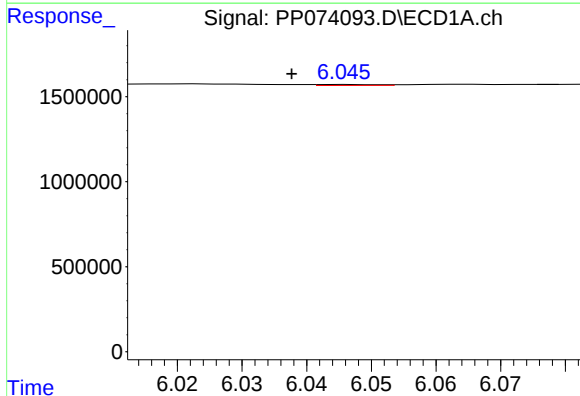


#6 AR-1016-4

R.T.: 6.047 min
Delta R.T.: 0.009 min
Response: 34269
Conc: 1.24 ng/ml

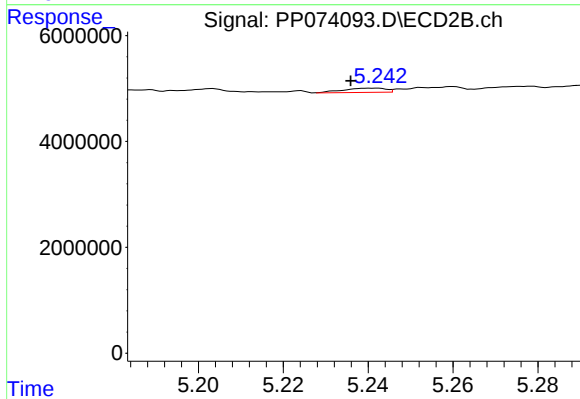

#6 AR-1016-4


R.T.: 5.242 min
Delta R.T.: 0.006 min
Response: 557986
Conc: 2.67 ng/ml

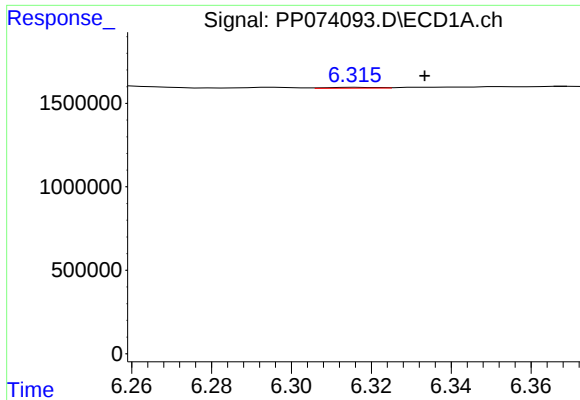

#7 AR-1016-5


R.T.: 6.316 min
Delta R.T.: -0.017 min
Response: 42418
Conc: 1.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

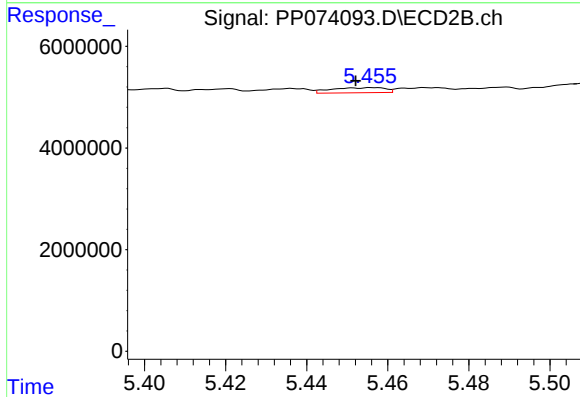


#7 AR-1016-5

R.T.: 5.456 min
Delta R.T.: 0.004 min
Response: 933896
Conc: 4.05 ng/ml

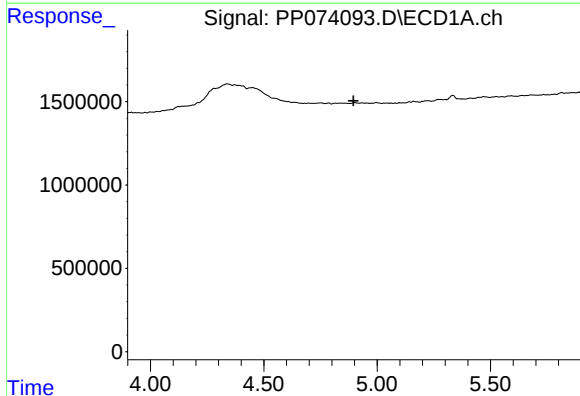


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.896 min
Response: 0
Conc: N.D.

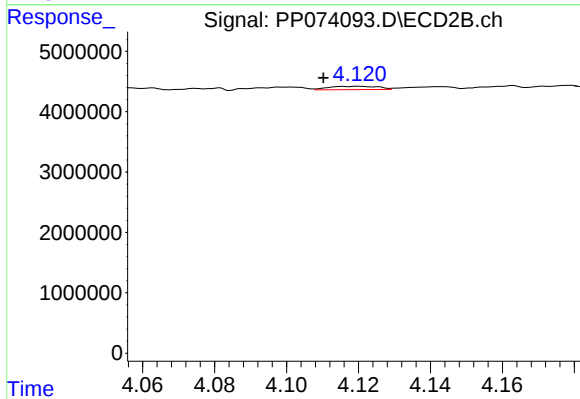

#8 AR-1221-1


R.T.: 4.120 min
Delta R.T.: 0.010 min
Response: 531320
Conc: 4.74 ng/ml

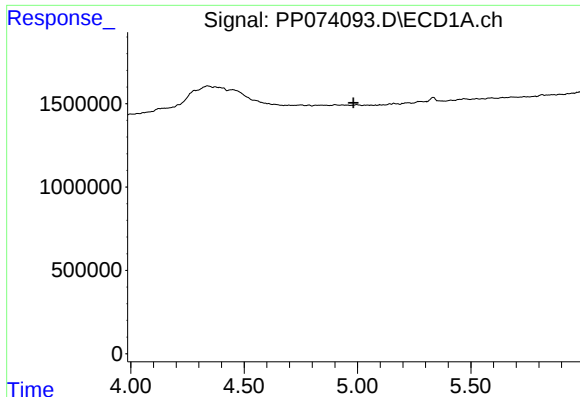

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.982 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

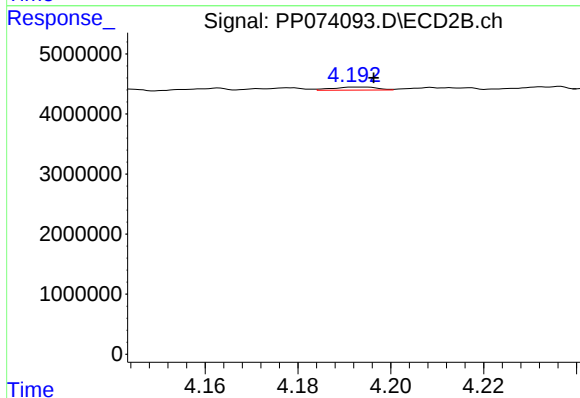


#9 AR-1221-2

R.T.: 4.192 min
Delta R.T.: -0.004 min
Response: 336618
Conc: 4.40 ng/ml

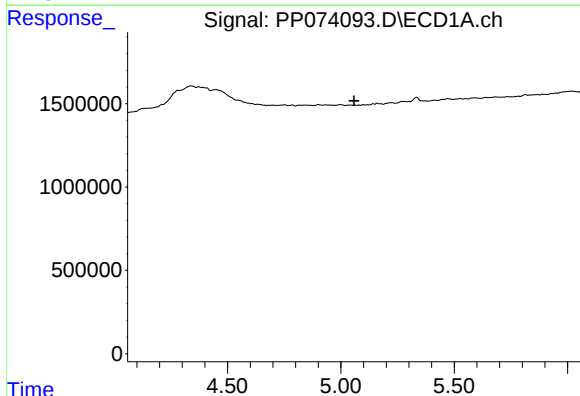


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T.: 5.058 min
Response: 0
Conc: N.D.

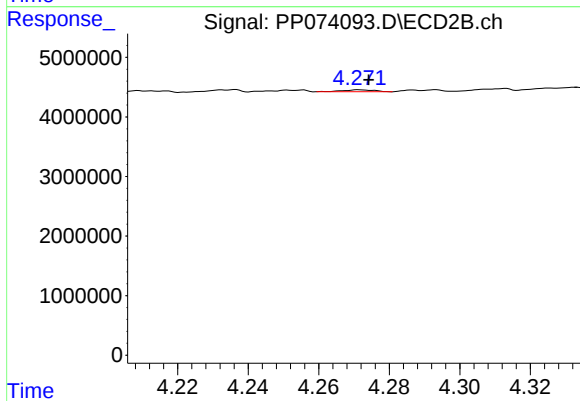

#10 AR-1221-3


R.T.: 4.271 min
Delta R.T.: -0.003 min
Response: 207727
Conc: 0.72 ng/ml

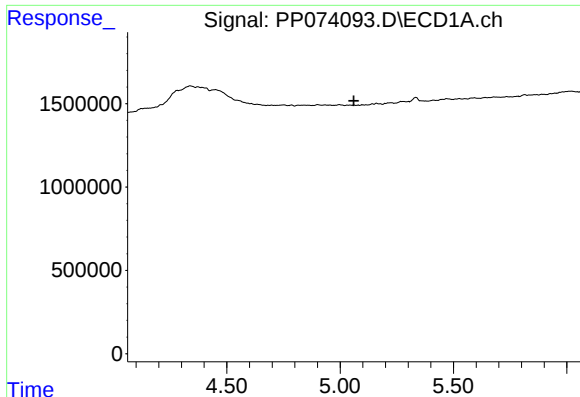

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 5.061 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

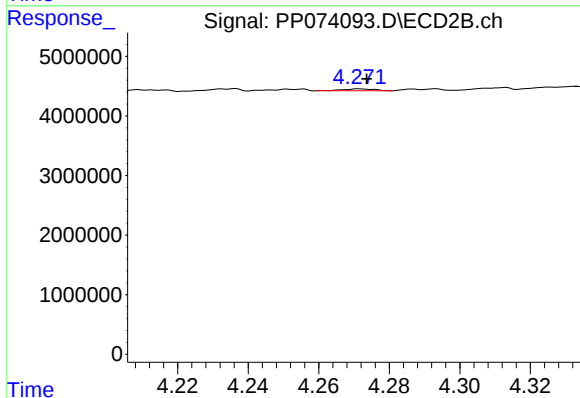


#11 AR-1232-1

R.T.: 4.271 min
Delta R.T.: -0.002 min
Response: 207727
Conc: 0.91 ng/ml

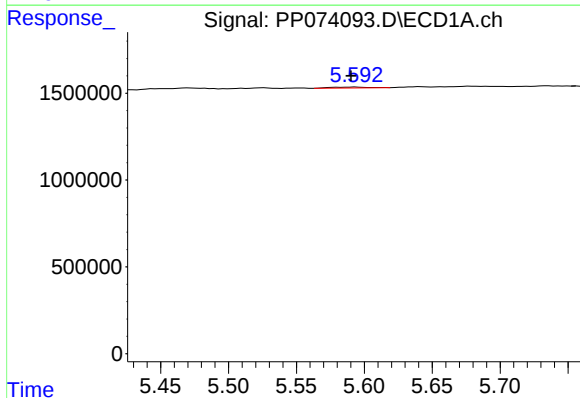


#12 AR-1232-2

R.T.: 5.593 min
Delta R.T.: 0.003 min
Response: 100233
Conc: 7.21 ng/ml

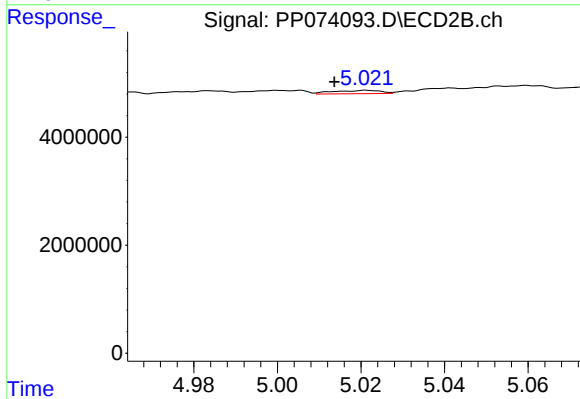

#12 AR-1232-2


R.T.: 5.021 min
Delta R.T.: 0.008 min
Response: 481884
Conc: 1.59 ng/ml

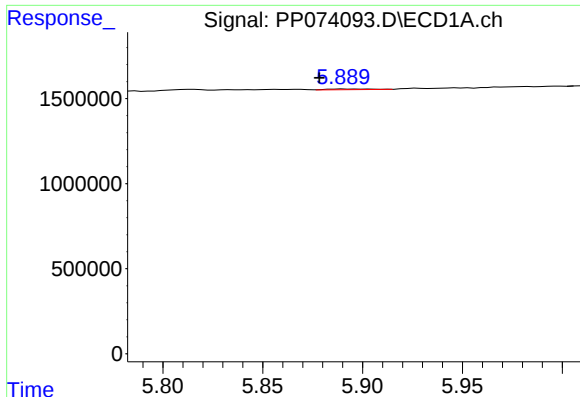

#13 AR-1232-3


R.T.: 5.891 min
Delta R.T.: 0.012 min
Response: 63626
Conc: 2.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

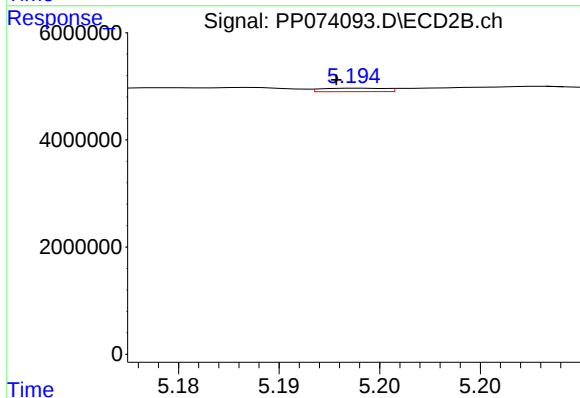


#13 AR-1232-3

R.T.: 5.194 min
Delta R.T.: 0.002 min
Response: 142511
Conc: 1.39 ng/ml

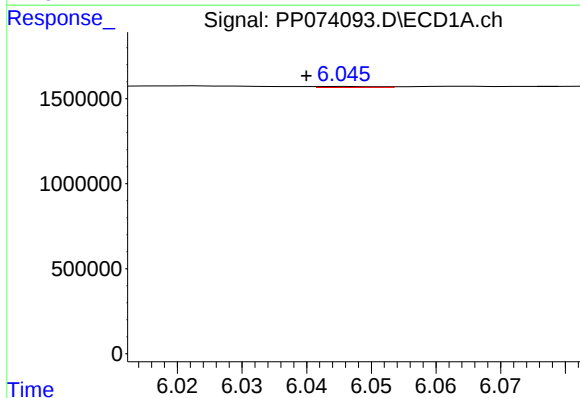


#14 AR-1232-4

R.T.: 6.047 min
Delta R.T.: 0.007 min
Response: 34269
Conc: 2.47 ng/ml

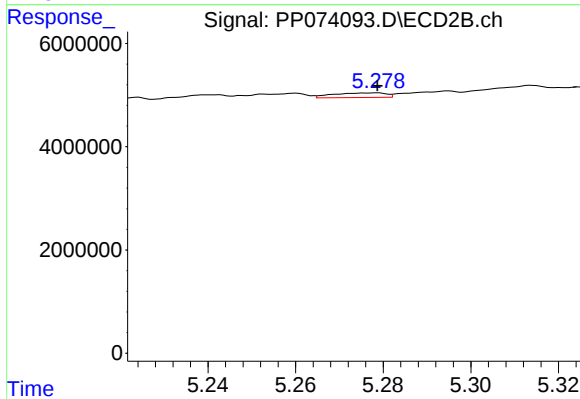

#14 AR-1232-4


R.T.: 5.279 min
Delta R.T.: 0.000 min
Response: 754888
Conc: 7.15 ng/ml

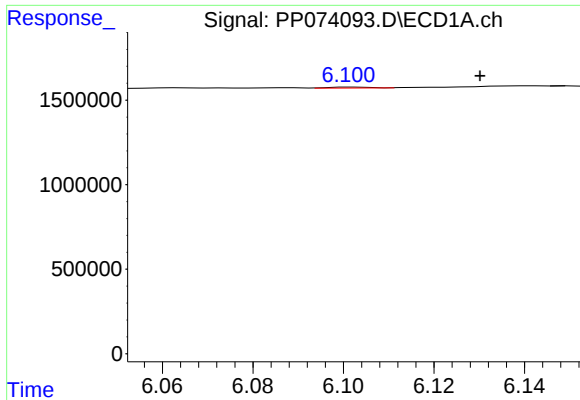

#15 AR-1232-5


R.T.: 6.103 min
Delta R.T.: -0.028 min
Response: 38557
Conc: 3.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

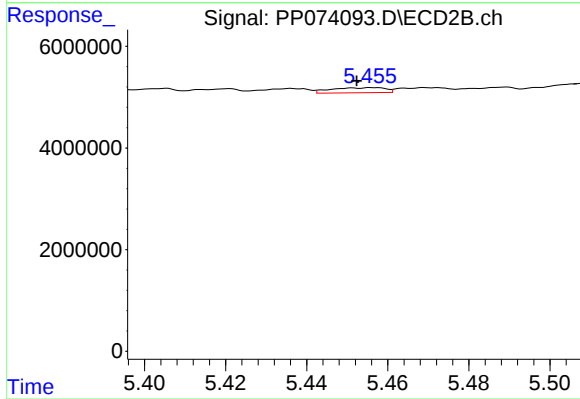


#15 AR-1232-5

R.T.: 5.456 min
Delta R.T.: 0.004 min
Response: 933896
Conc: 9.67 ng/ml

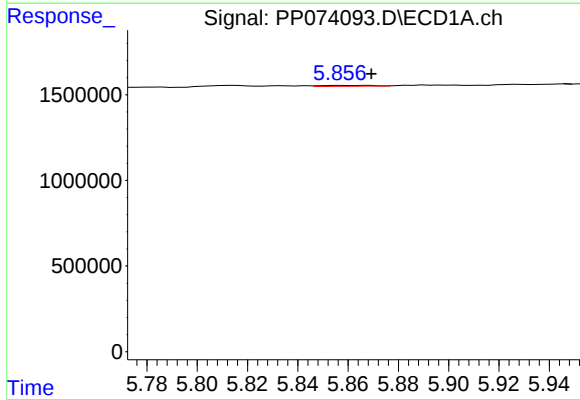


#16 AR-1242-1

R.T.: 5.857 min
Delta R.T.: -0.012 min
Response: 79218
Conc: 2.40 ng/ml

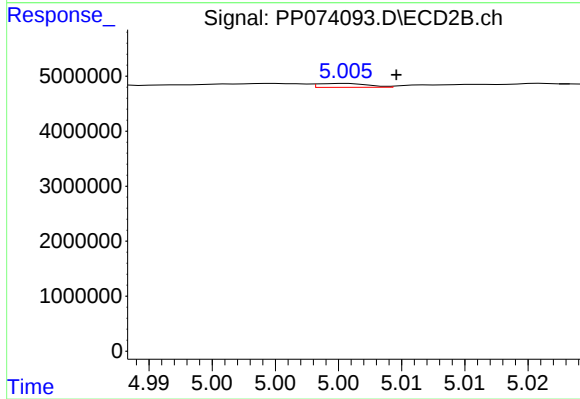

#16 AR-1242-1


R.T.: 5.006 min
Delta R.T.: -0.004 min
Response: 198785
Conc: 0.25 ng/ml

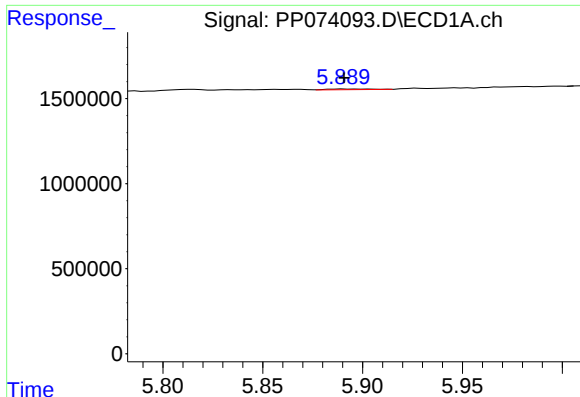

#17 AR-1242-2


R.T.: 5.891 min
Delta R.T.: 0.000 min
Response: 63626
Conc: 1.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

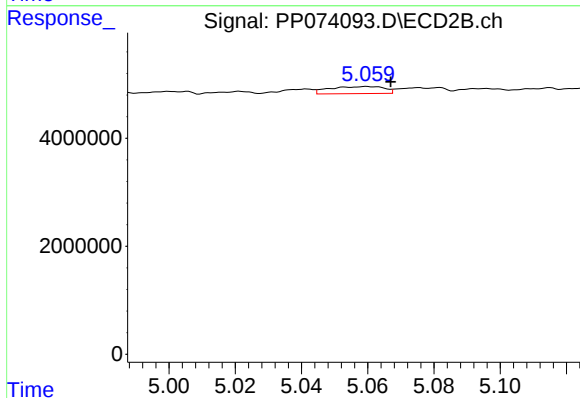


#17 AR-1242-2

R.T.: 5.060 min
Delta R.T.: -0.007 min
Response: 1509419
Conc: 4.41 ng/ml

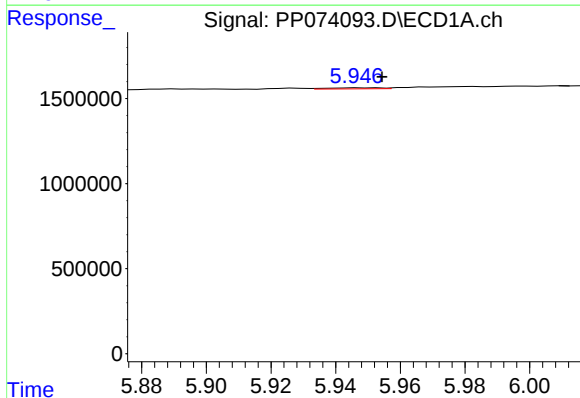


#18 AR-1242-3

R.T.: 5.947 min
Delta R.T.: -0.007 min
Response: 72545
Conc: 2.38 ng/ml

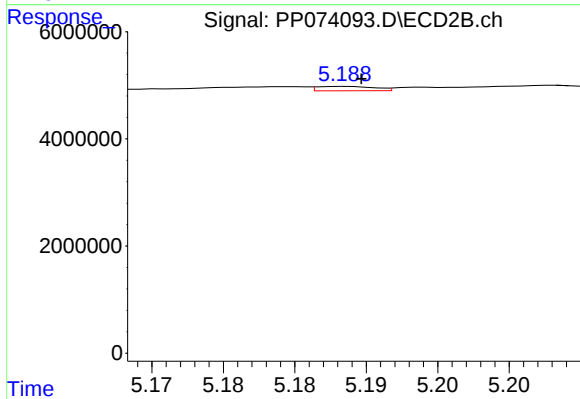

#18 AR-1242-3


R.T.: 5.189 min
Delta R.T.: -0.001 min
Response: 230621
Conc: 1.17 ng/ml

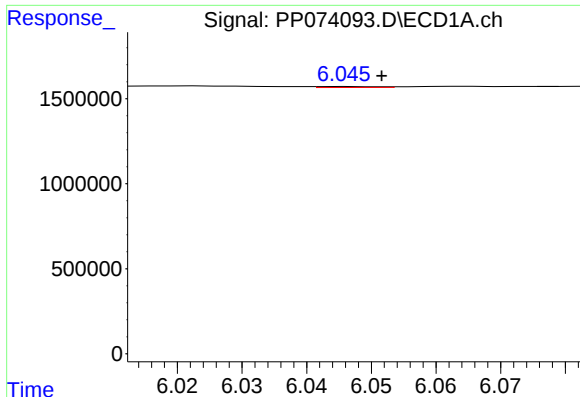

#19 AR-1242-4


R.T.: 6.047 min
Delta R.T.: -0.005 min
Response: 34269
Conc: 1.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

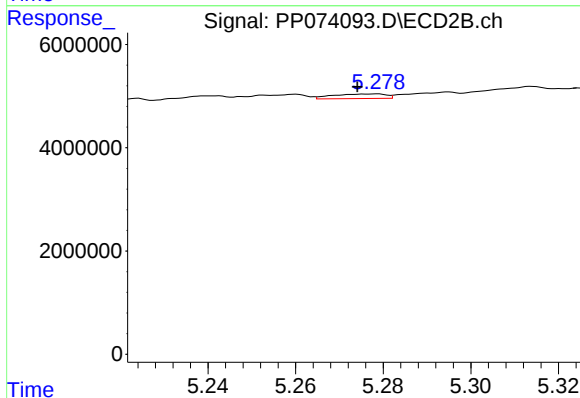


#19 AR-1242-4

R.T.: 5.279 min
Delta R.T.: 0.004 min
Response: 754888
Conc: 3.14 ng/ml

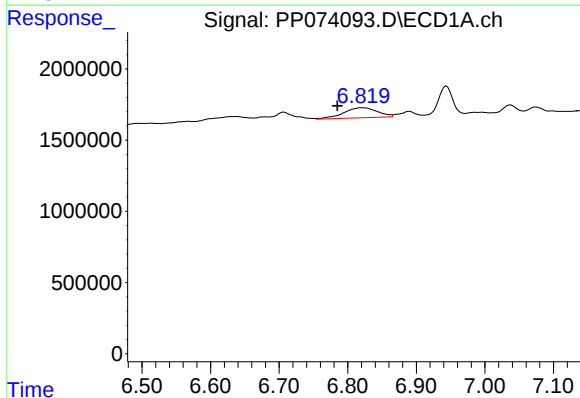


#20 AR-1242-5

R.T.: 6.821 min
Delta R.T.: 0.036 min
Response: 2411423
Conc: 78.86 ng/ml

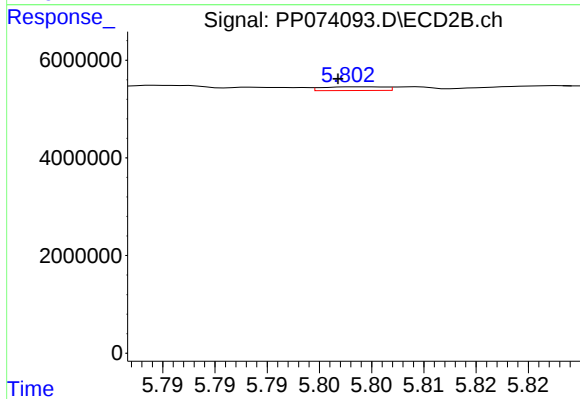

#20 AR-1242-5


R.T.: 5.804 min
Delta R.T.: 0.002 min
Response: 316252
Conc: 1.11 ng/ml

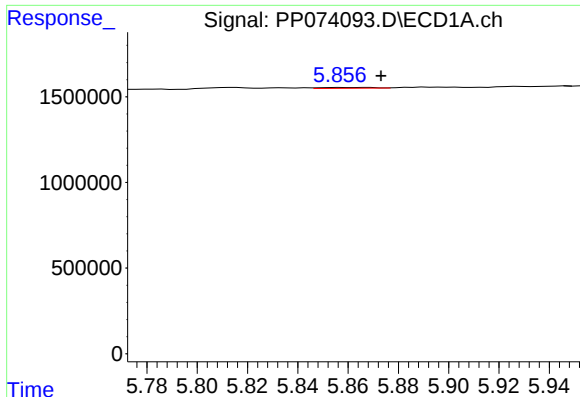

#21 AR-1248-1


R.T.: 5.857 min
Delta R.T.: -0.016 min
Response: 79218
Conc: 2.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

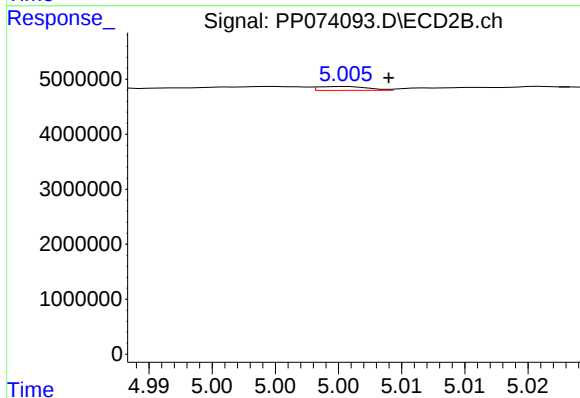


#21 AR-1248-1

R.T.: 5.006 min
Delta R.T.: -0.003 min
Response: 198785
Conc: 0.40 ng/ml

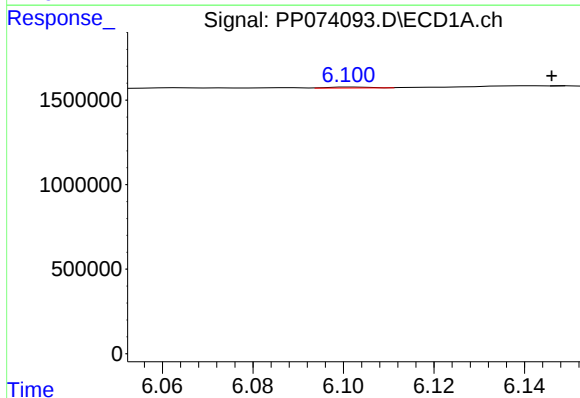


#22 AR-1248-2

R.T.: 6.103 min
Delta R.T.: -0.043 min
Response: 38557
Conc: 1.04 ng/ml

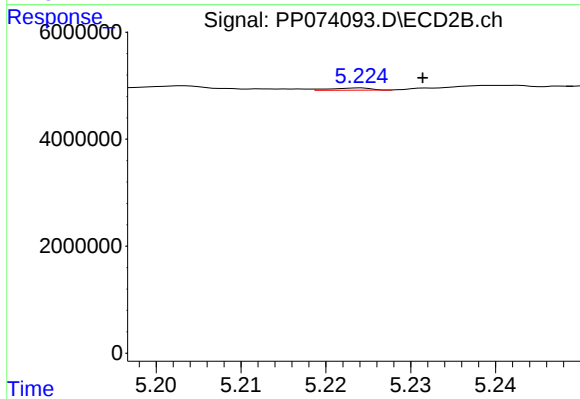

#22 AR-1248-2


R.T.: 5.224 min
Delta R.T.: -0.007 min
Response: 142766
Conc: 0.46 ng/ml

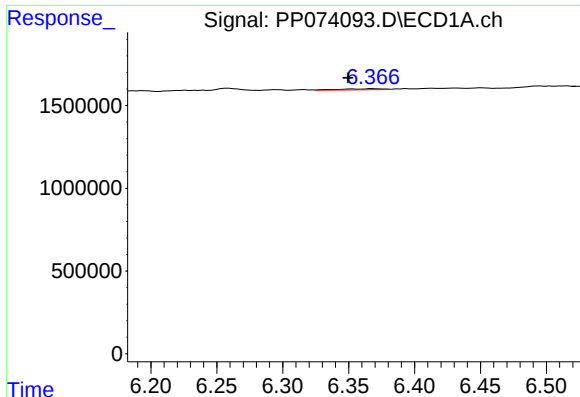

#23 AR-1248-3


R.T.: 6.368 min
Delta R.T.: 0.018 min
Response: 150599
Conc: 3.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

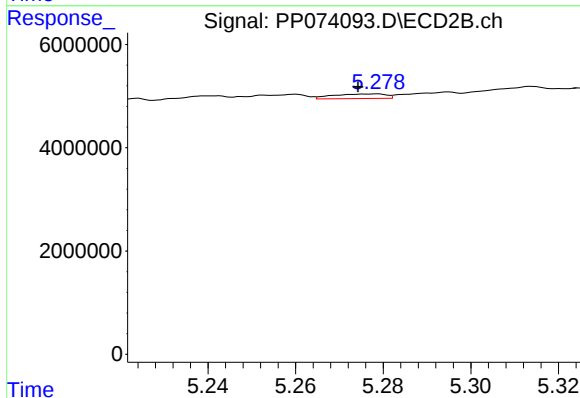


#23 AR-1248-3

R.T.: 5.279 min
Delta R.T.: 0.004 min
Response: 754888
Conc: 2.18 ng/ml

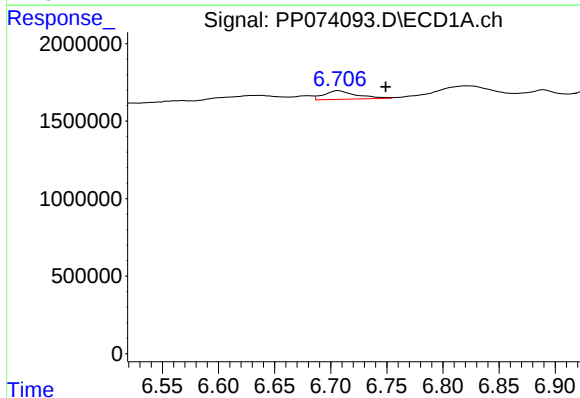


#24 AR-1248-4

R.T.: 6.707 min
Delta R.T.: -0.042 min
Response: 1111738
Conc: 23.76 ng/ml

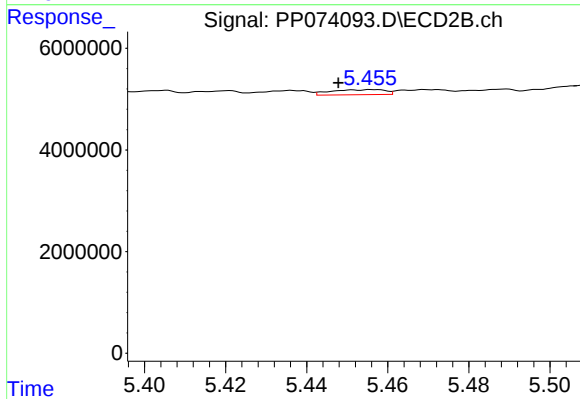

#24 AR-1248-4


R.T.: 5.456 min
Delta R.T.: 0.008 min
Response: 933896
Conc: 2.60 ng/ml

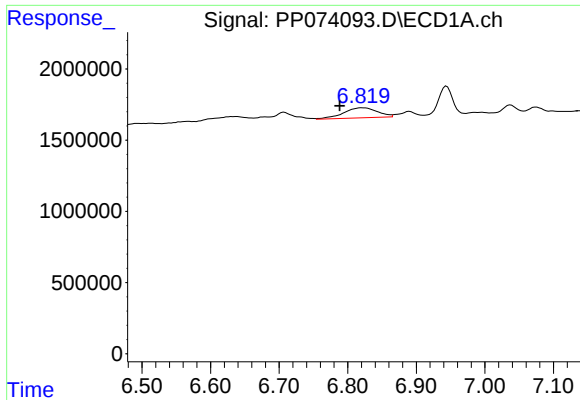

#25 AR-1248-5


R.T.: 6.821 min
Delta R.T.: 0.033 min
Response: 2411423
Conc: 44.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

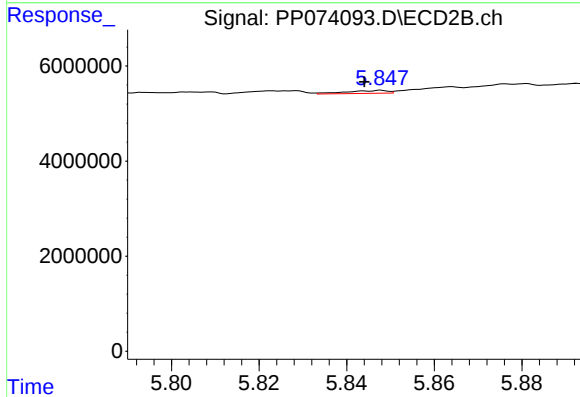


#25 AR-1248-5

R.T.: 5.848 min
Delta R.T.: 0.004 min
Response: 398144
Conc: 0.67 ng/ml

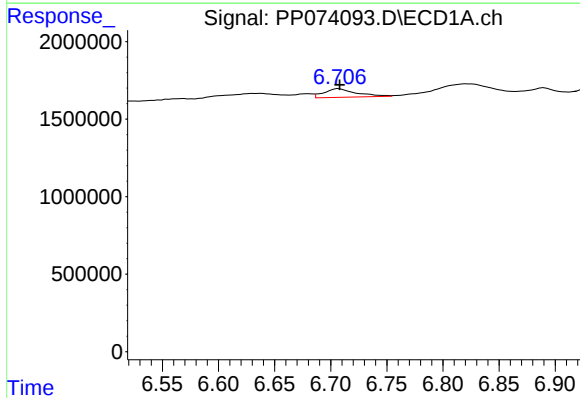


#26 AR-1254-1

R.T.: 6.707 min
Delta R.T.: 0.000 min
Response: 1111738
Conc: 22.13 ng/ml

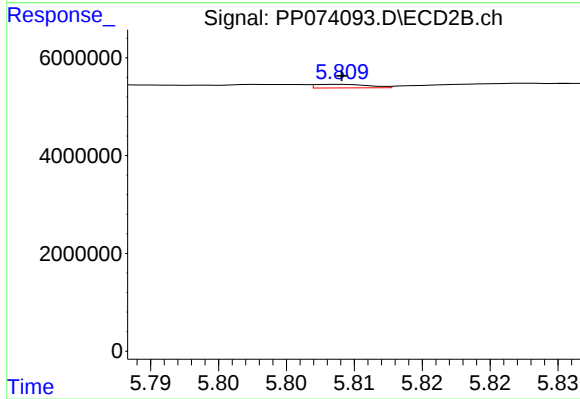

#26 AR-1254-1


R.T.: 5.809 min
Delta R.T.: 0.000 min
Response: 198796
Conc: 0.28 ng/ml

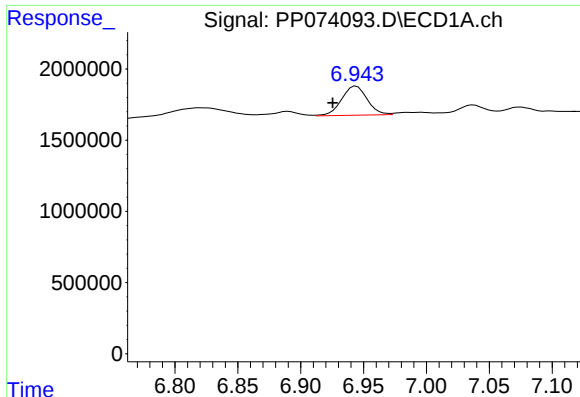

#27 AR-1254-2


R.T.: 6.944 min
Delta R.T.: 0.019 min
Response: 2888248
Conc: 41.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

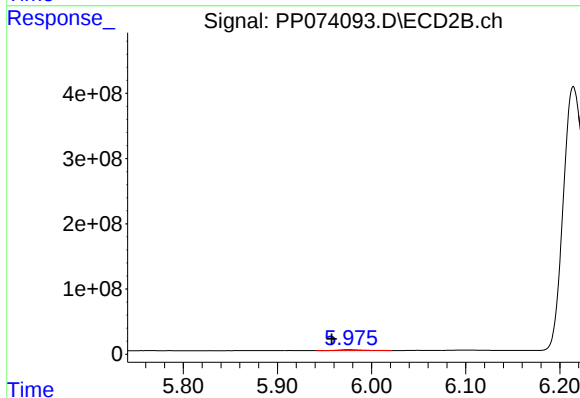


#27 AR-1254-2

R.T.: 5.976 min
Delta R.T.: 0.018 min
Response: 22998834
Conc: 42.94 ng/ml

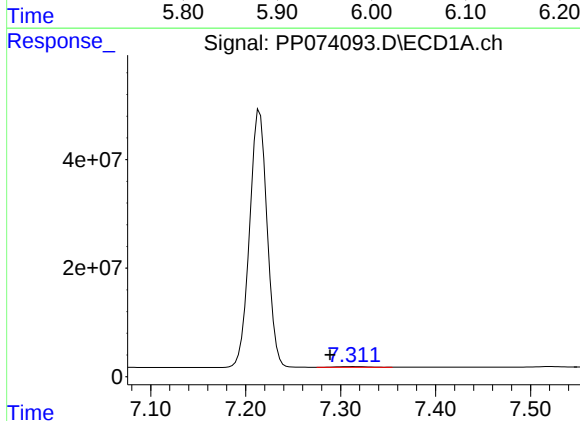


#28 AR-1254-3

R.T.: 7.313 min
Delta R.T.: 0.024 min
Response: 2908312
Conc: 39.81 ng/ml

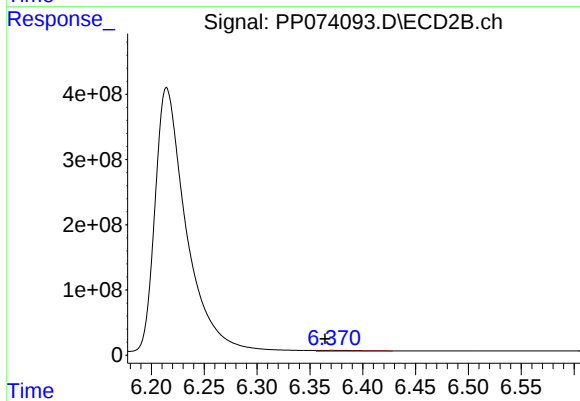

#28 AR-1254-3


R.T.: 6.371 min
Delta R.T.: 0.006 min
Response: 36508648
Conc: 41.72 ng/ml

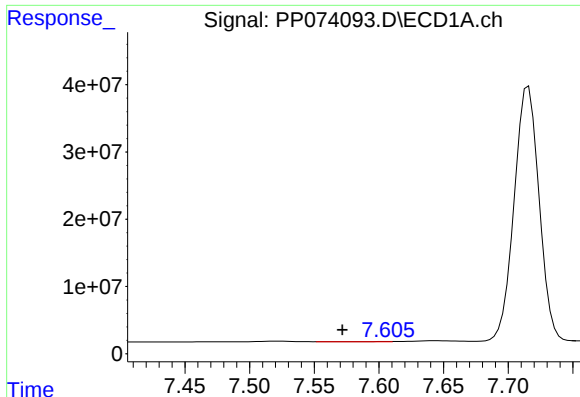

#29 AR-1254-4


R.T.: 7.606 min
Delta R.T.: 0.034 min
Response: 746738
Conc: 14.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

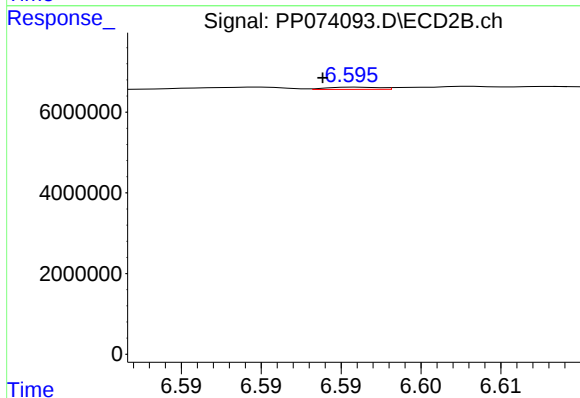


#29 AR-1254-4

R.T.: 6.596 min
Delta R.T.: 0.002 min
Response: 122794
Conc: 0.18 ng/ml

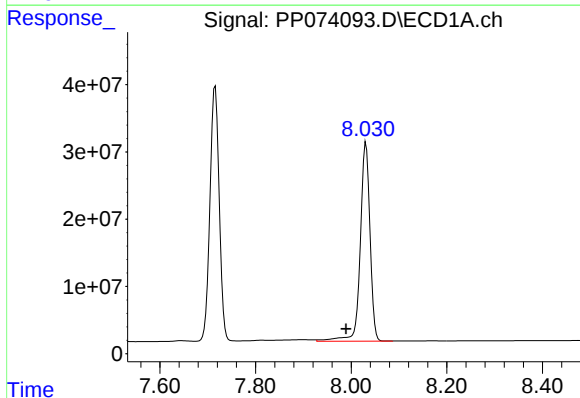


#30 AR-1254-5

R.T.: 8.031 min
Delta R.T.: 0.042 min
Response: 416215353
Conc: 6888.56 ng/ml

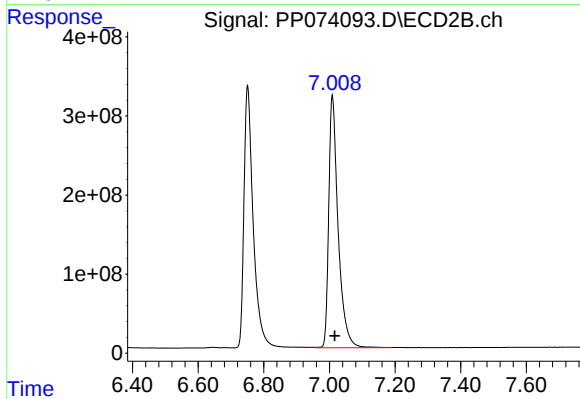

#30 AR-1254-5


R.T.: 7.009 min
Delta R.T.: -0.007 min
Response: 6341367921
Conc: 7918.20 ng/ml

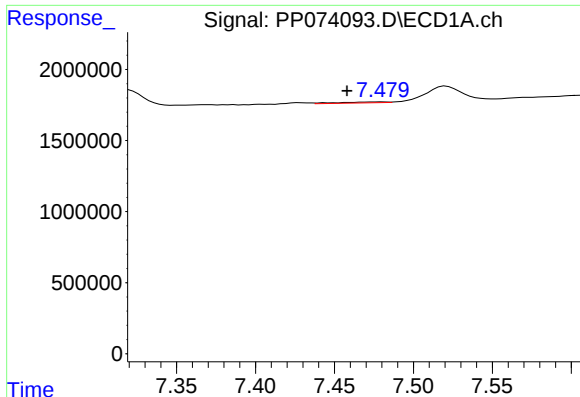

#31 AR-1260-1

R.T.: 7.481 min
Delta R.T.: 0.023 min
Response: 146810
Conc: 3.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

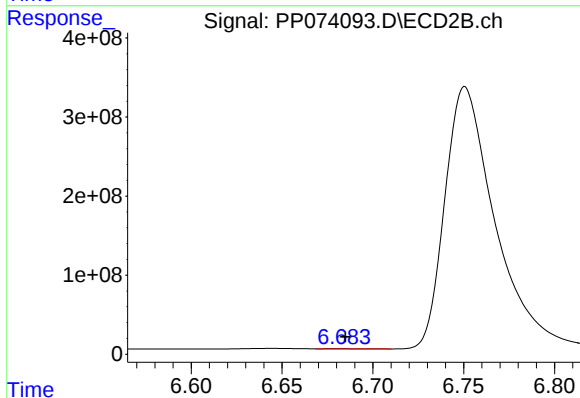

#31 AR-1260-1


R.T.: 6.683 min
Delta R.T.: -0.002 min
Response: 6942734
Conc: 8.86 ng/ml

#32 AR-1260-2

R.T.: 7.716 min
Delta R.T.: 0.004 min
Response: 512349634
Conc: 9358.96 ng/ml

#32 AR-1260-2


R.T.: 6.886 min
Delta R.T.: 0.044 min
Response: 19388572
Conc: 25.52 ng/ml

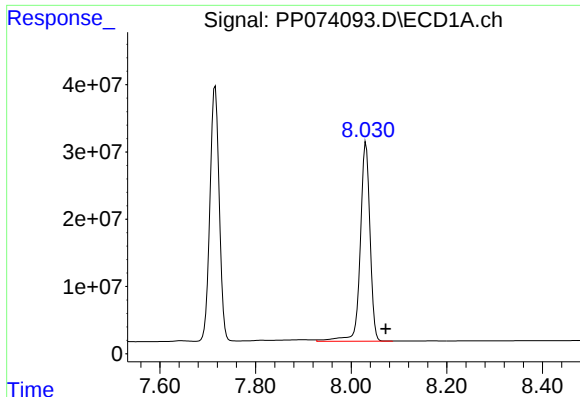

#33 AR-1260-3


R.T.: 8.031 min
Delta R.T.: -0.041 min
Response: 416215353
Conc: 10966.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

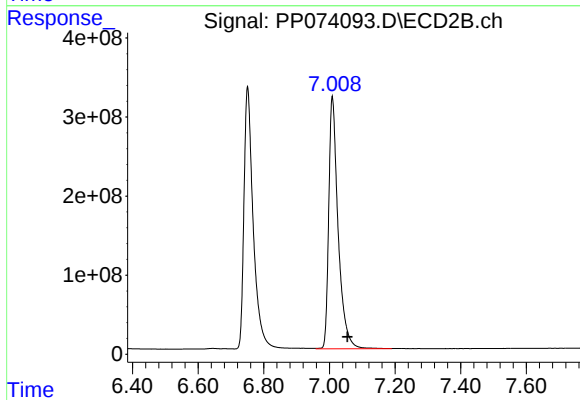


#33 AR-1260-3

R.T.: 7.009 min
Delta R.T.: -0.046 min
Response: 6341367921
Conc: 7980.96 ng/ml

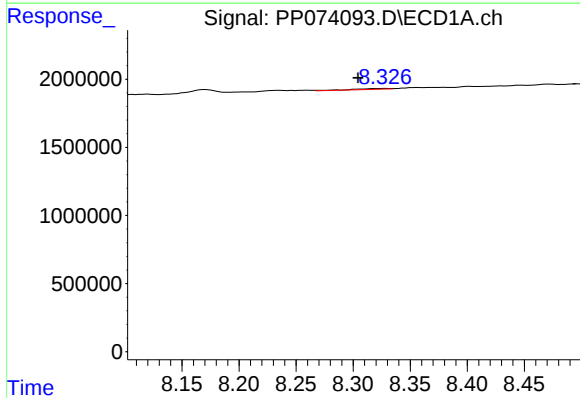


#34 AR-1260-4

R.T.: 8.328 min
Delta R.T.: 0.024 min
Response: 140518
Conc: 2.94 ng/ml

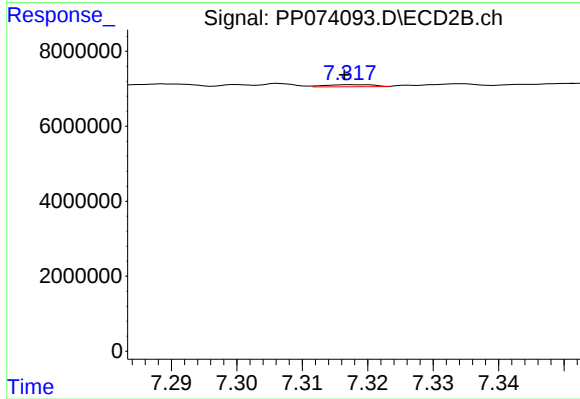

#34 AR-1260-4


R.T.: 7.318 min
Delta R.T.: 0.002 min
Response: 283702
Conc: 0.49 ng/ml

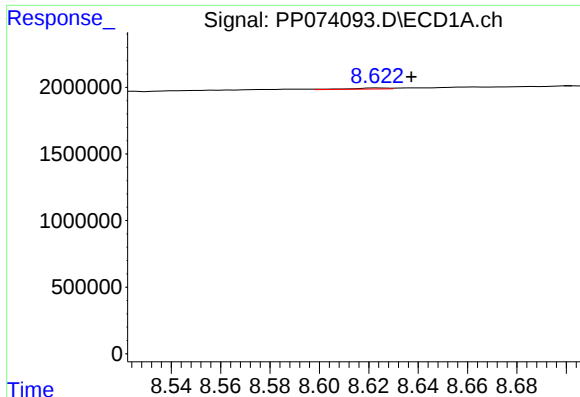

#35 AR-1260-5


R.T.: 8.625 min
Delta R.T.: -0.013 min
Response: 86599
Conc: 1.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

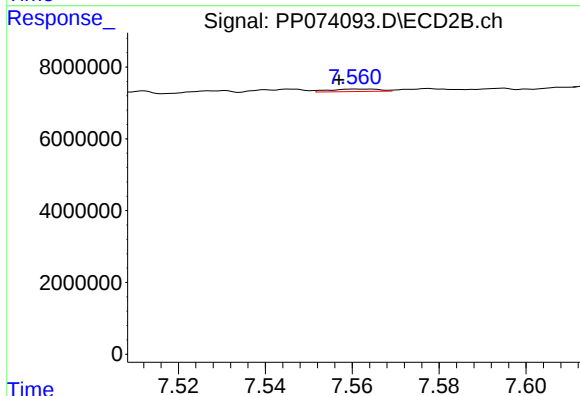


#35 AR-1260-5

R.T.: 7.561 min
Delta R.T.: 0.004 min
Response: 566554
Conc: 0.36 ng/ml

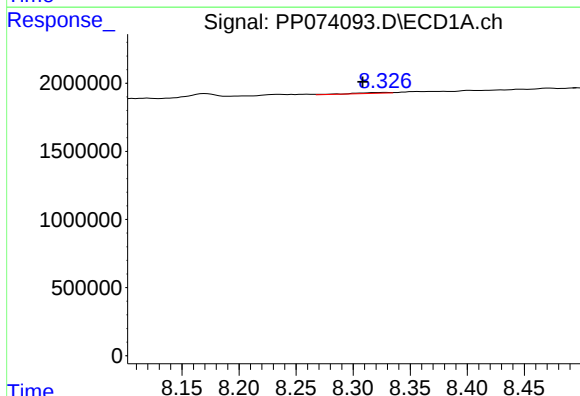


#36 AR-1262-1

R.T.: 8.328 min
Delta R.T.: 0.020 min
Response: 140518
Conc: 2.27 ng/ml

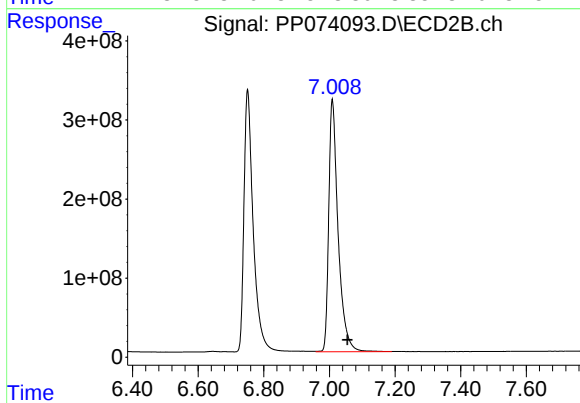

#36 AR-1262-1


R.T.: 7.009 min
Delta R.T.: -0.046 min
Response: 6341367921
Conc: 5358.76 ng/ml

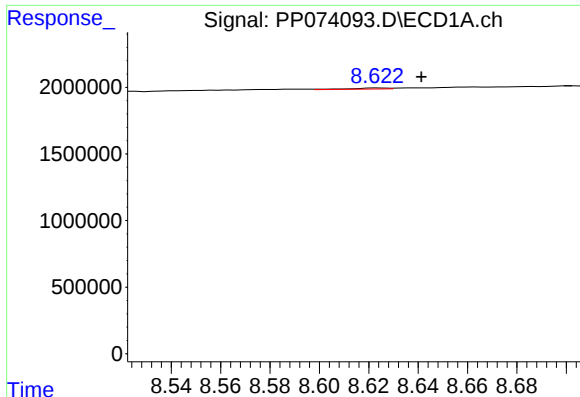

#37 AR-1262-2


R.T.: 8.625 min
Delta R.T.: -0.017 min
Response: 86599
Conc: 0.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

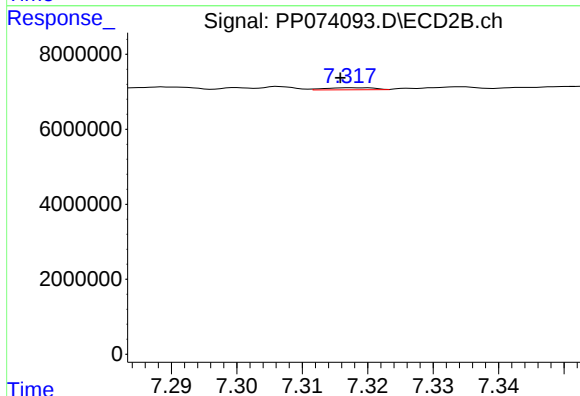


#37 AR-1262-2

R.T.: 7.318 min
Delta R.T.: 0.002 min
Response: 283702
Conc: 0.34 ng/ml

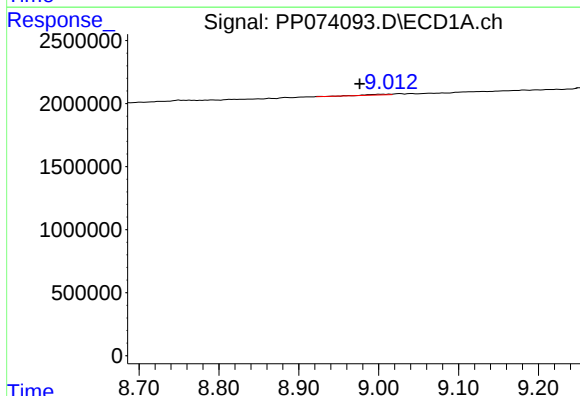


#38 AR-1262-3

R.T.: 9.001 min
Delta R.T.: 0.025 min
Response: 100443
Conc: 1.31 ng/ml

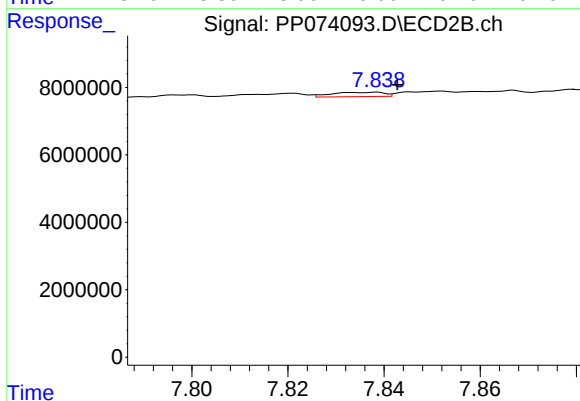

#38 AR-1262-3


R.T.: 7.838 min
Delta R.T.: -0.005 min
Response: 977172
Conc: 1.27 ng/ml

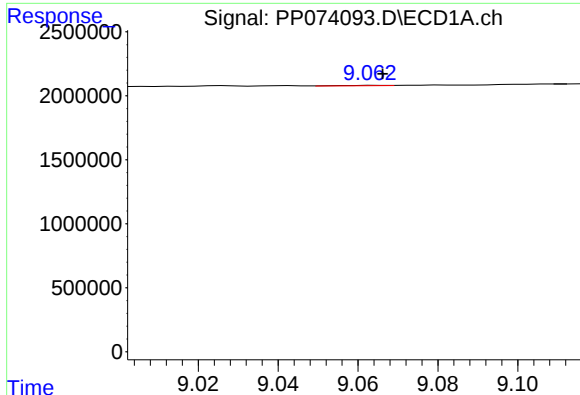

#39 AR-1262-4


R.T.: 9.065 min
Delta R.T.: -0.002 min
Response: 18760
Conc: 0.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

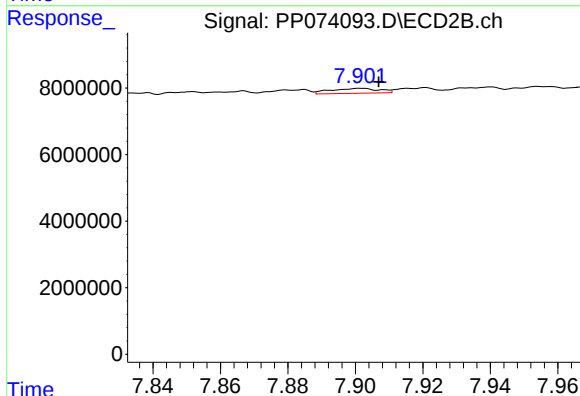


#39 AR-1262-4

R.T.: 7.902 min
Delta R.T.: -0.005 min
Response: 1499122
Conc: 1.06 ng/ml

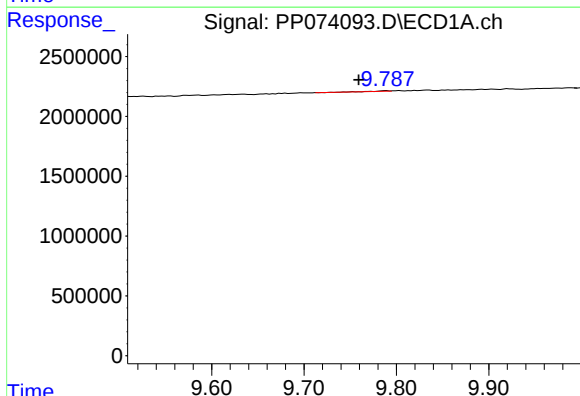


#40 AR-1262-5

R.T.: 9.789 min
Delta R.T.: 0.030 min
Response: 33523
Conc: 0.86 ng/ml

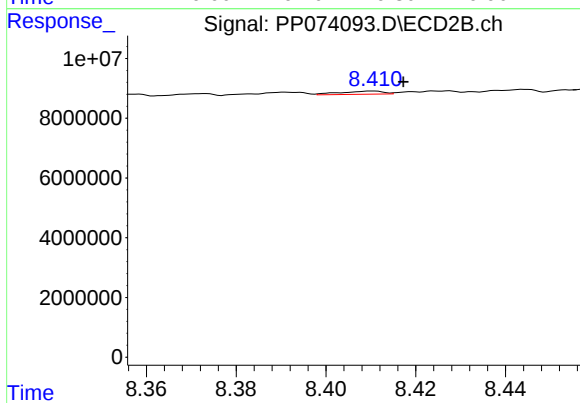

#40 AR-1262-5


R.T.: 8.410 min
Delta R.T.: -0.007 min
Response: 702370
Conc: 1.12 ng/ml

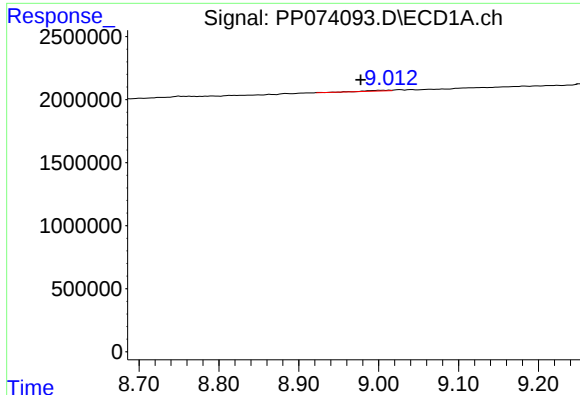

#41 AR-1268-1


R.T.: 9.001 min
Delta R.T.: 0.024 min
Response: 100443
Conc: 0.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

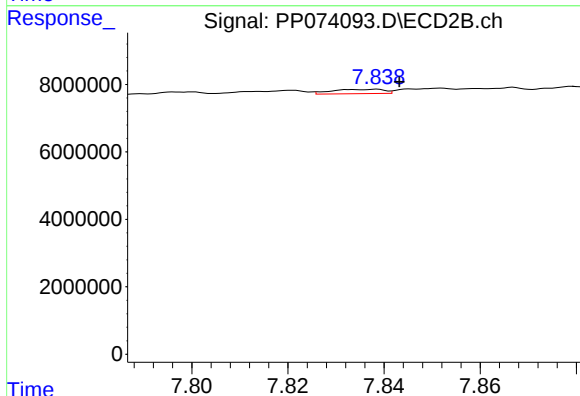


#41 AR-1268-1

R.T.: 7.838 min
Delta R.T.: -0.005 min
Response: 977172
Conc: 0.44 ng/ml

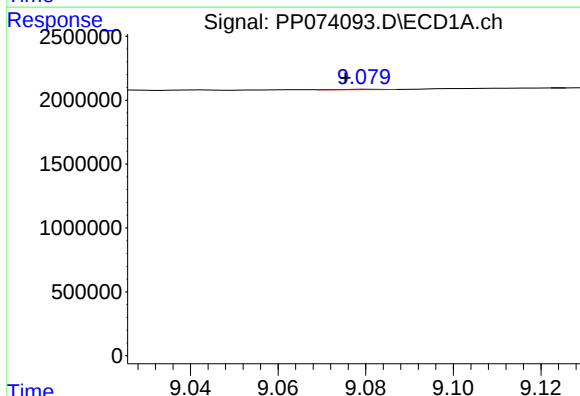


#42 AR-1268-2

R.T.: 9.081 min
Delta R.T.: 0.006 min
Response: 13427
Conc: 0.11 ng/ml

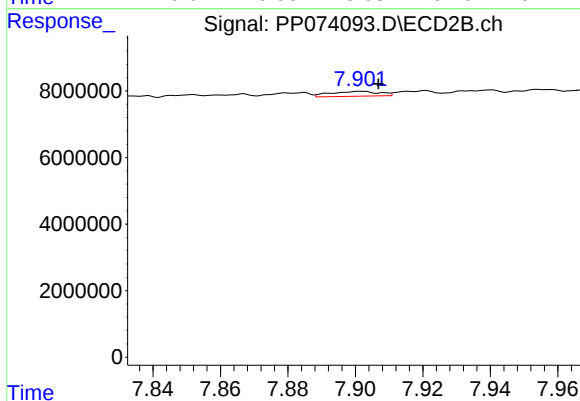

#42 AR-1268-2


R.T.: 7.902 min
Delta R.T.: -0.005 min
Response: 1499122
Conc: 0.69 ng/ml

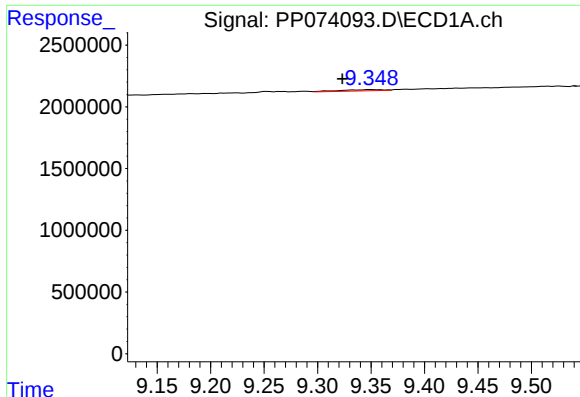

#43 AR-1268-3


R.T.: 9.349 min
Delta R.T.: 0.026 min
Response: 286601
Conc: 2.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

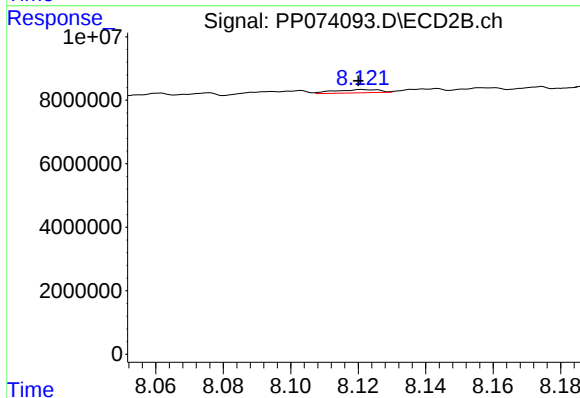


#43 AR-1268-3

R.T.: 8.122 min
Delta R.T.: 0.002 min
Response: 954495
Conc: 0.59 ng/ml

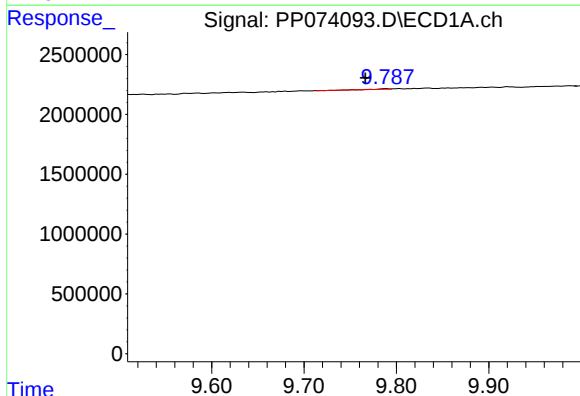


#44 AR-1268-4

R.T.: 9.789 min
Delta R.T.: 0.023 min
Response: 33523
Conc: 0.77 ng/ml

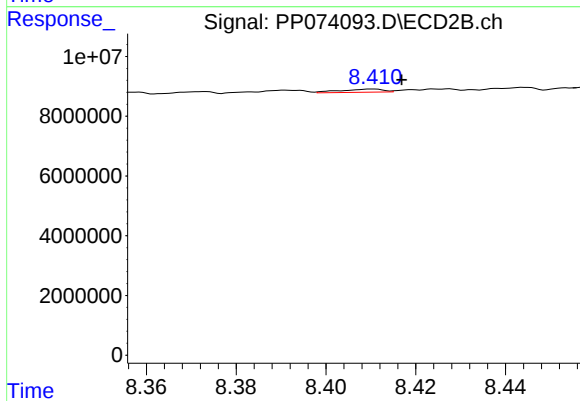

#44 AR-1268-4


R.T.: 8.410 min
Delta R.T.: -0.007 min
Response: 702370
Conc: 1.06 ng/ml

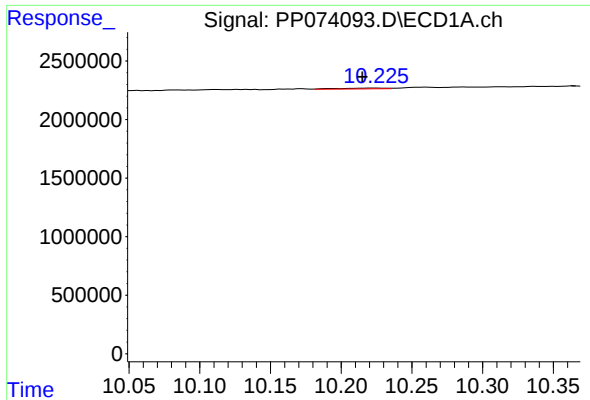

#45 AR-1268-5

R.T.: 10.226 min
Delta R.T.: 0.011 min
Response: 145412
Conc: 0.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

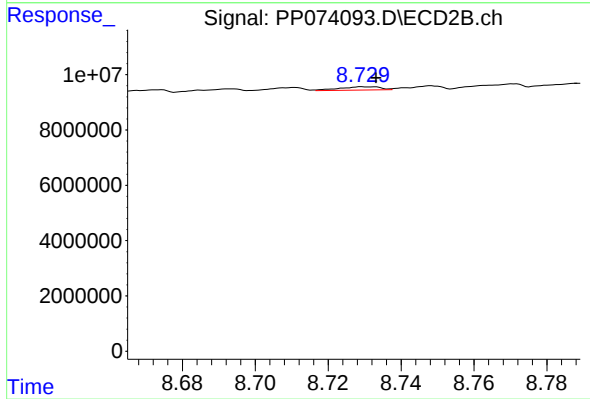

#45 AR-1268-5

R.T.: 8.730 min
Delta R.T.: -0.003 min
Response: 932249
Conc: 0.18 ng/ml