

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072925\
 Data File : PP074097.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2025 12:45
 Operator : YP\AJ
 Sample : Q2686-01 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 Y2310-0410-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/30/2025
 Supervised By :mohammad ahmed 07/31/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:46:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 28 18:16:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.716	3.886	1506894	8764182	1.443m	0.952 #
2) SA Decachlor...	10.596	9.007	1132456	10712525	1.686	0.942 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072925\
Data File : PP074097.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2025 12:45
Operator : YP\AJ
Sample : Q2686-01 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
Y2310-0410-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/30/2025
Supervised By :mohammad ahmed 07/31/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 01:46:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 28 18:16:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

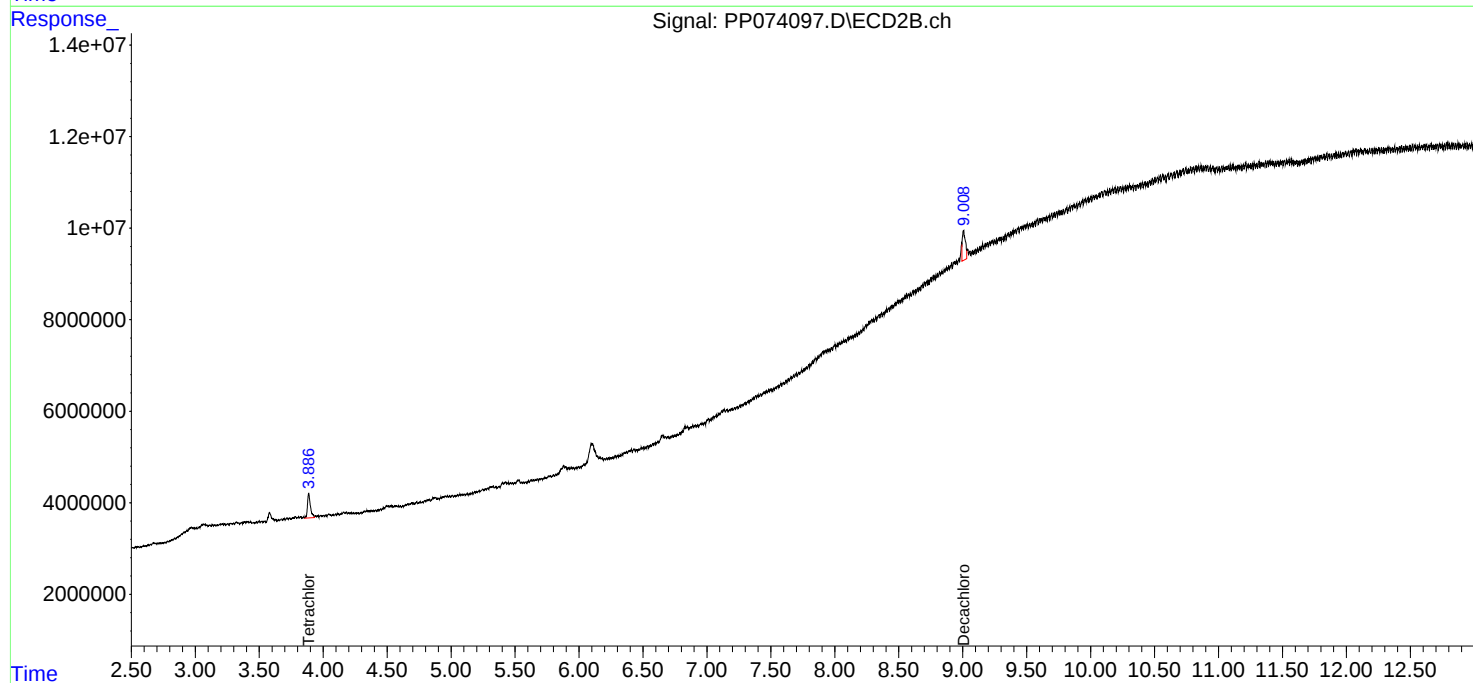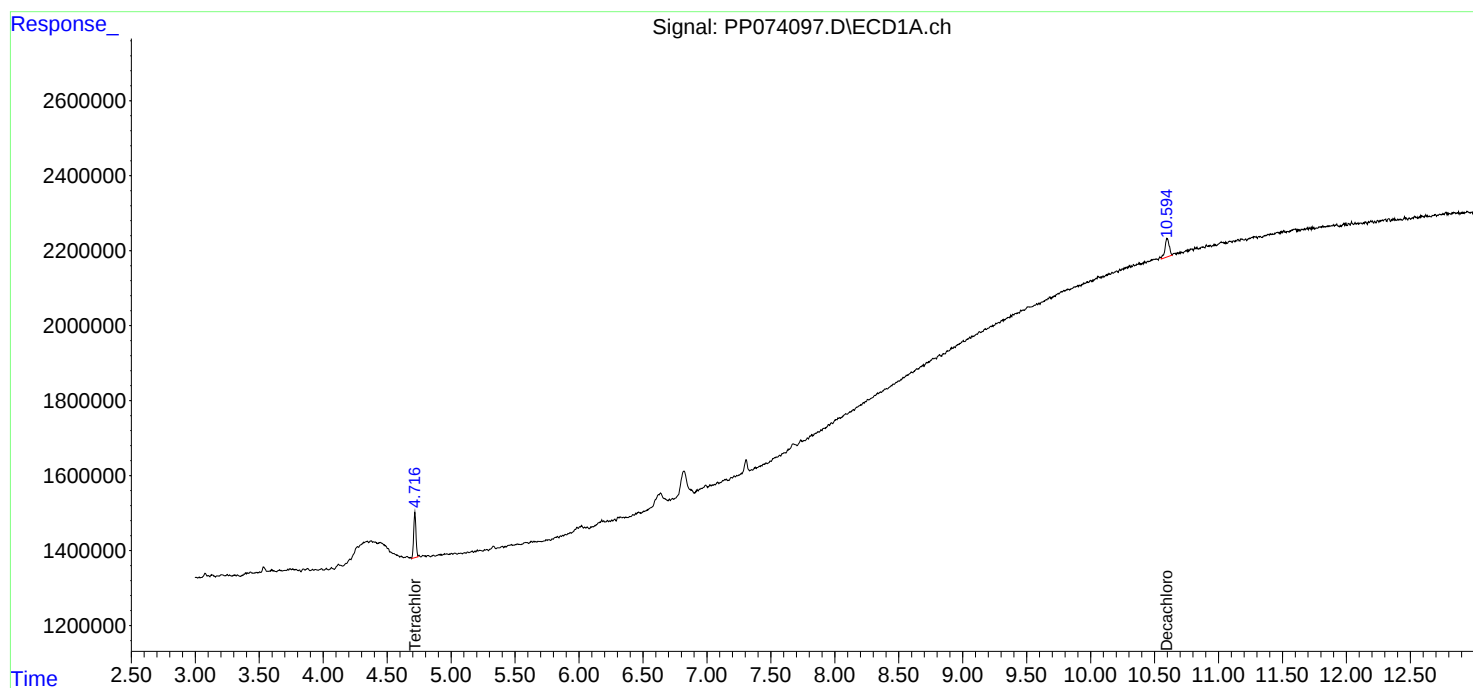

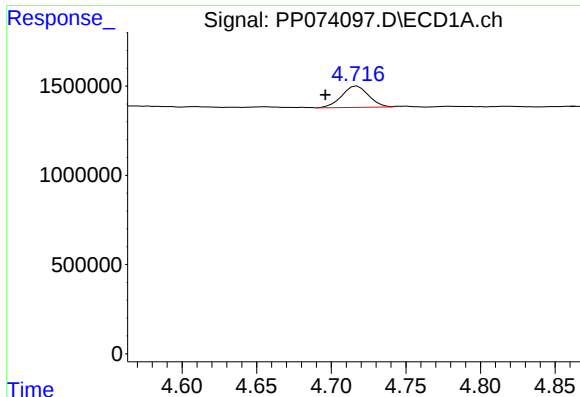


#1 Tetrachloro-m-xylene

R.T.: 4.716 min
Delta R.T.: 0.020 min
Response: 1506894
Conc: 1.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
Y2310-0410-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/30/2025
Supervised By :mohammad ahmed 07/31/2025

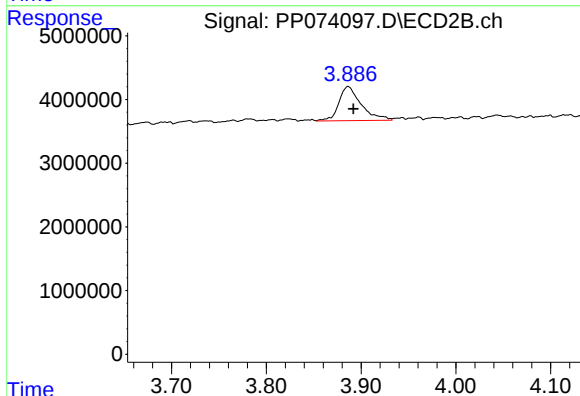


#1 Tetrachloro-m-xylene

R.T.: 3.886 min
Delta R.T.: -0.005 min
Response: 8764182
Conc: 0.95 ng/ml

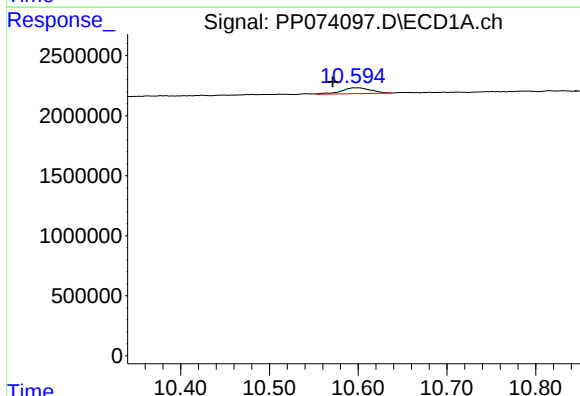

#2 Decachlorobiphenyl

R.T.: 10.596 min
Delta R.T.: 0.025 min
Response: 1132456
Conc: 1.69 ng/ml

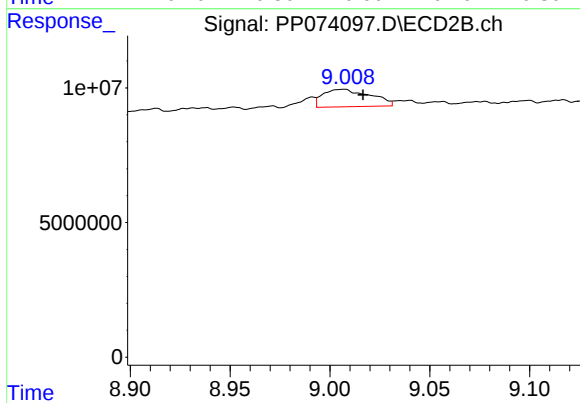

#2 Decachlorobiphenyl

R.T.: 9.007 min
Delta R.T.: -0.009 min
Response: 10712525
Conc: 0.94 ng/ml