

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072925\
 Data File : PP074115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2025 18:28
 Operator : YP\AJ
 Sample : Q2701-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PIPE-4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/30/2025
 Supervised By :mohammad ahmed 07/31/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 08:46:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 28 18:16:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.725	3.890	25504360	225.3E6	24.416	24.471
2) SA Decachlor...	10.606	9.007	18673546	268.5E6	27.806m	23.611

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072925\
Data File : PP074115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2025 18:28
Operator : YP\AJ
Sample : Q2701-04
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PIPE-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/30/2025
Supervised By :mohammad ahmed 07/31/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 08:46:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072525.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 28 18:16:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

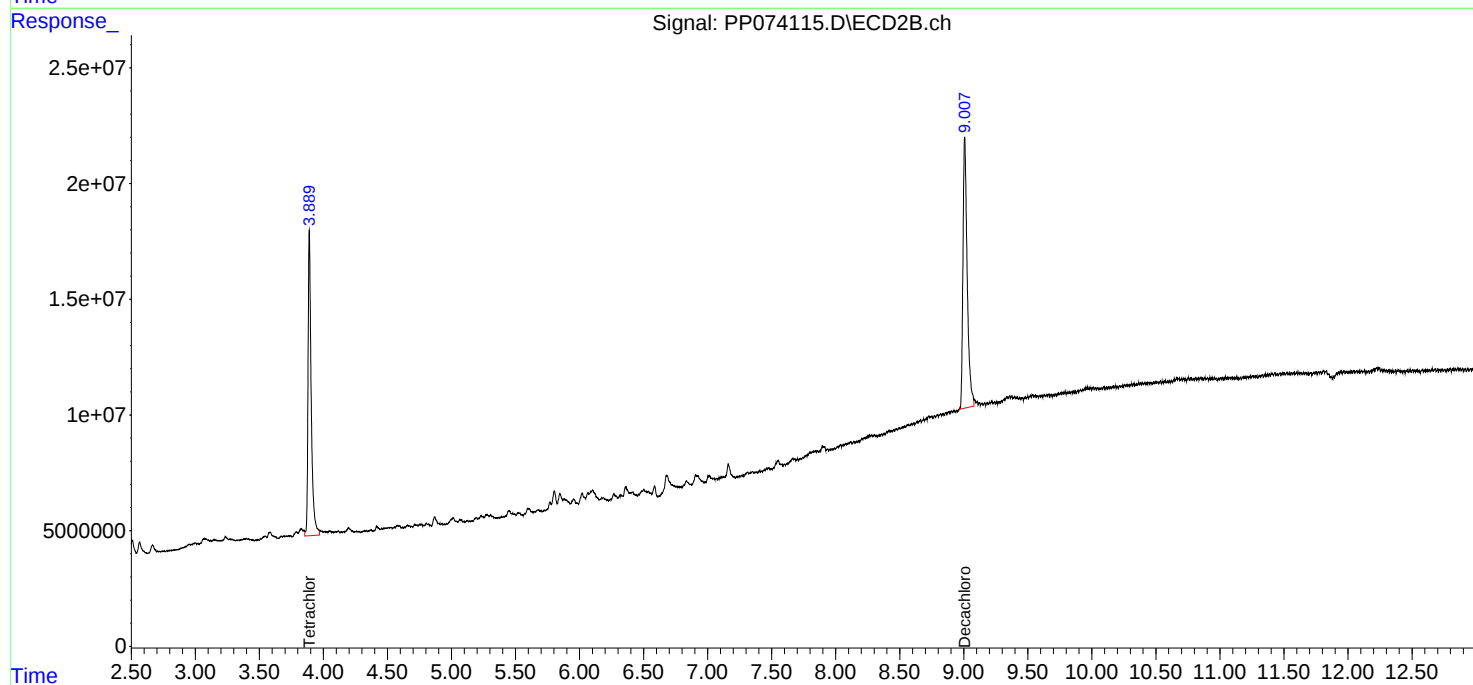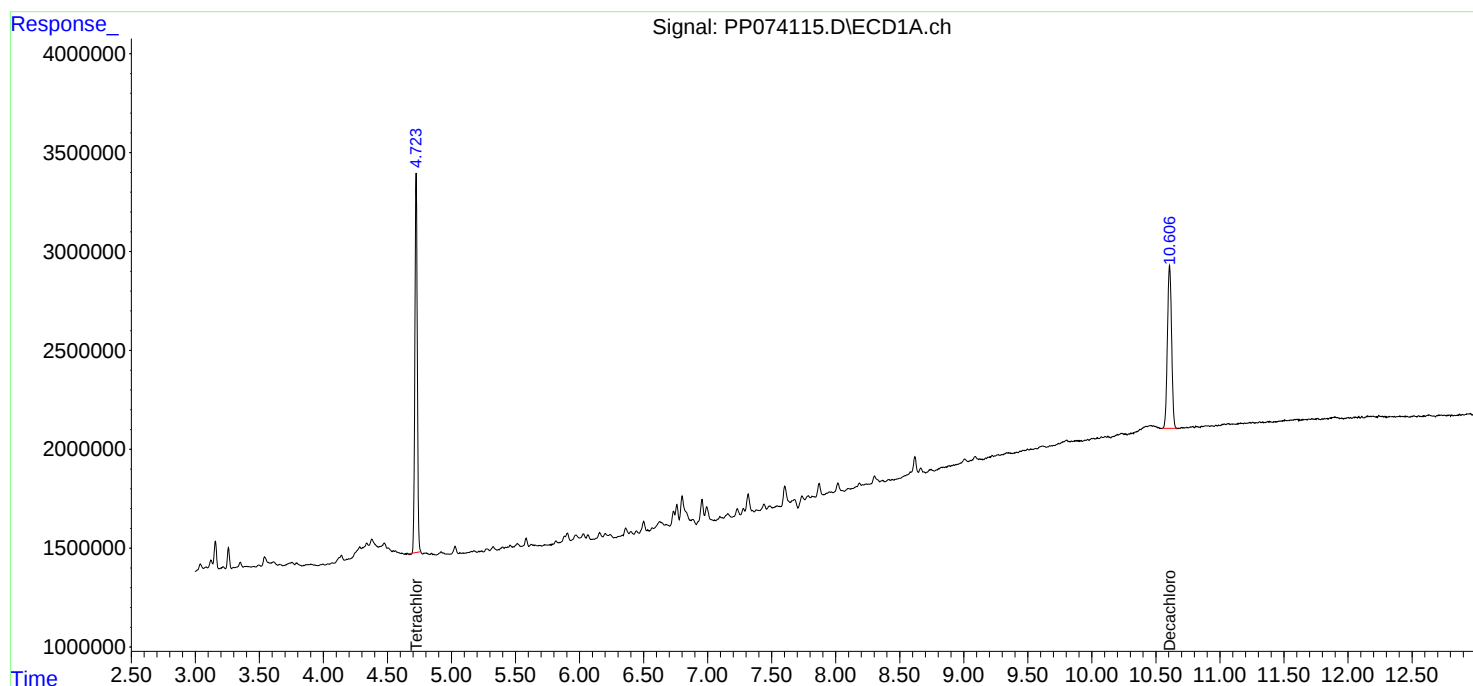

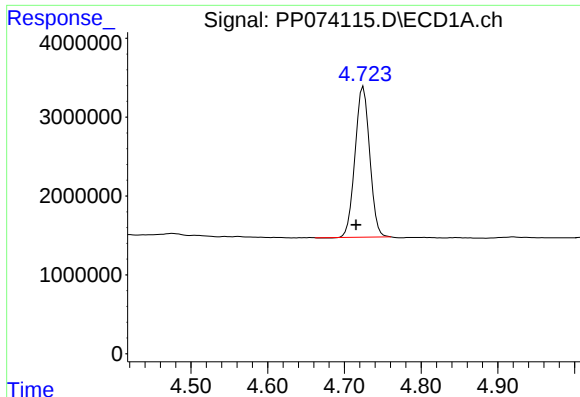


#1 Tetrachloro-m-xylene

R.T.: 4.725 min
Delta R.T.: 0.010 min
Response: 25504360
Conc: 24.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
PIPE-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/30/2025
Supervised By :mohammad ahmed 07/31/2025

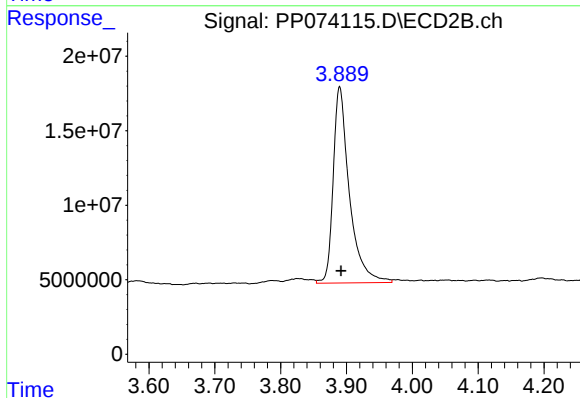


#1 Tetrachloro-m-xylene

R.T.: 3.890 min
Delta R.T.: -0.002 min
Response: 225339776
Conc: 24.47 ng/ml

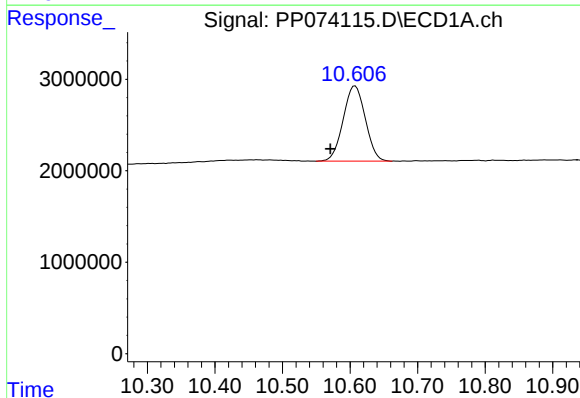

#2 Decachlorobiphenyl

R.T.: 10.606 min
Delta R.T.: 0.035 min
Response: 18673546
Conc: 27.81 ng/ml m

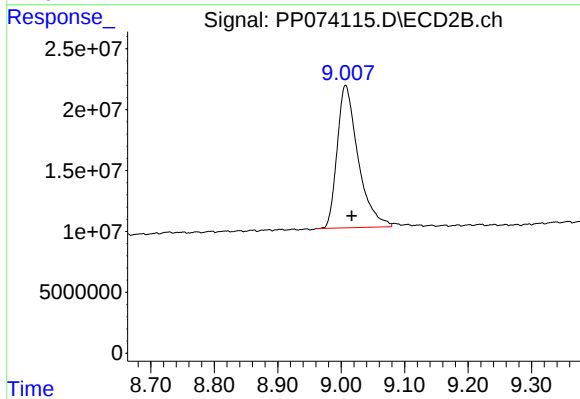

#2 Decachlorobiphenyl

R.T.: 9.007 min
Delta R.T.: -0.010 min
Response: 268462571
Conc: 23.61 ng/ml