

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP073018\
 Data File : PP026918.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2018 19:00
 Operator : EI\MA
 Sample : J4176-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PLASTIC-COAT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 05:03:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP073018.M
 Quant Title : 8080.M
 QLast Update : Tue Jul 31 01:31:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.049	12.156	82715804	139.5E6	346.348	344.460
Target Compounds							
1) T	Dalapon	3.276	0.000	21056819	0	35.841	N.D. #
3) T	4-Nitroph...	11.588	11.296	29601078	57805598	64.536	238.625 #
5) T	DICAMBA	12.410	0.000	12323537	0	8.724	N.D. #
6) T	MCPD	12.719	12.715	18180570	7426164	46.861	8.617 #
7) T	MCPA	12.963	0.000	315.7E6	0	470.492	N.D. #
8) T	DICHLORPROP	0.000	13.585	0	90913299	N.D.	234.237 #
10) T	Pentachlo...	14.288	14.714	281.0E6	8952993	36.925	1.342 #
12) T	2,4,5-T	15.579	15.933	106.6E6	19322887	41.778	8.869 #
13) T	2,4-DB	16.355	16.472	61413995	66704994	280.857	234.087
14) T	DINOSEB	17.833	16.863	22963807	118.8E6	11.355	65.838 #
15) T	Picloram	0.000	18.250	0	1189.3E6	N.D.	344.831 #
16) T	DCPA	18.163	18.164	25142735	10145699	6.268	3.152 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP073018\
Data File : PP026918.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2018 19:00
Operator : EI\MA
Sample : J4176-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PLASTIC-COAT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 05:03:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP073018.M
Quant Title : 8080.M
QLast Update : Tue Jul 31 01:31:14 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

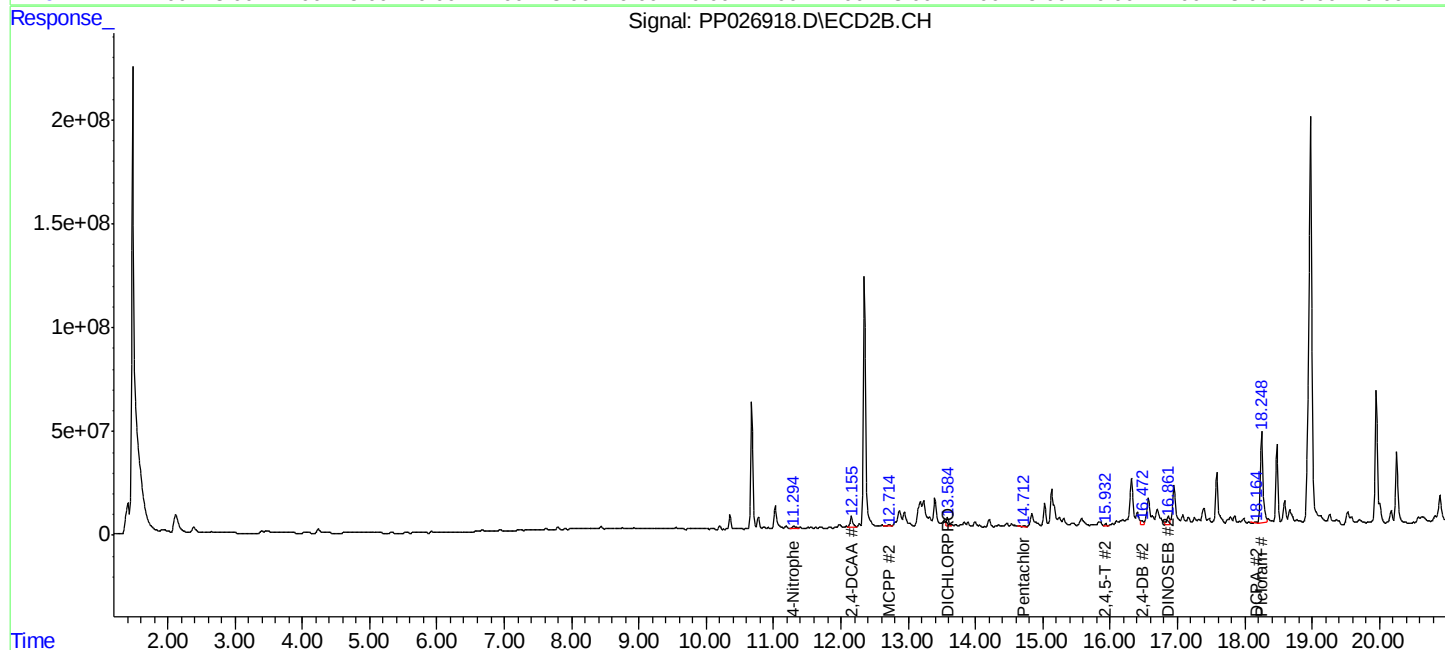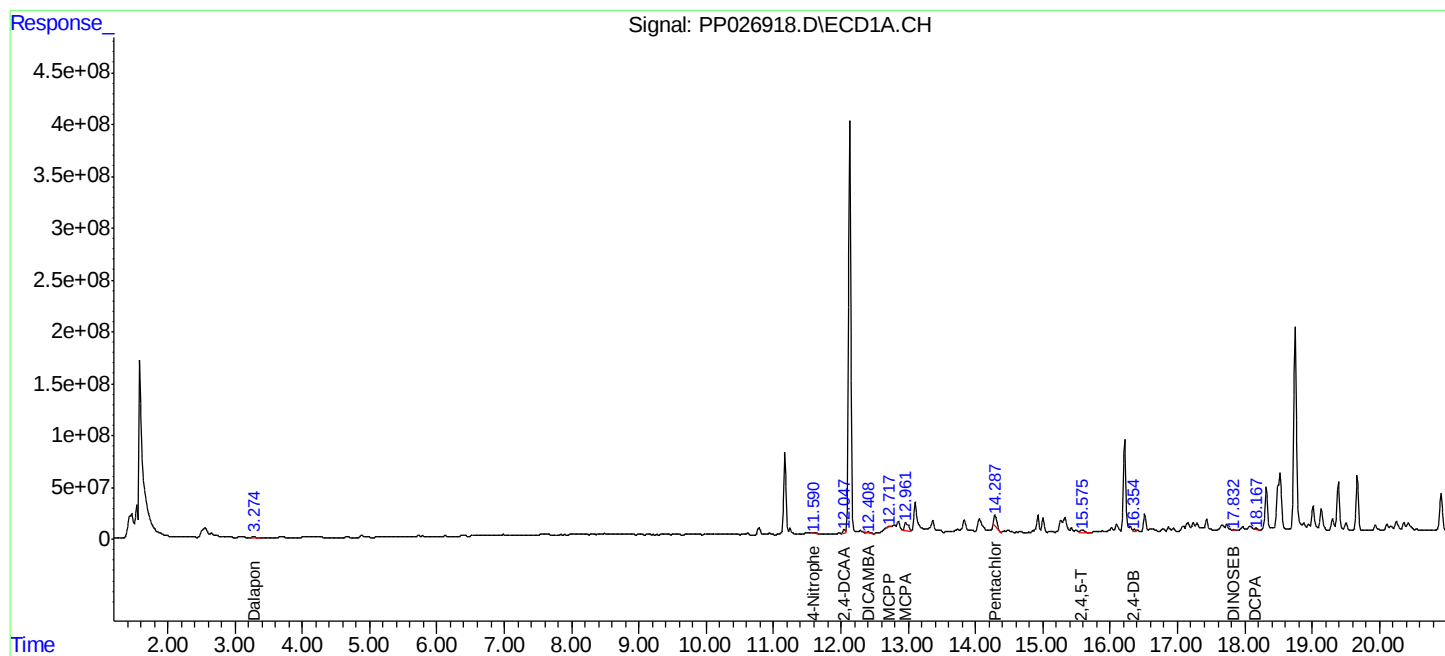


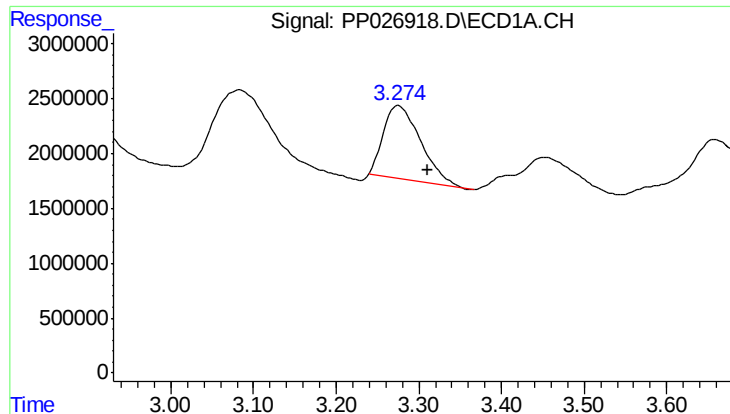

#1 Dalapon


R.T.: 3.276 min
Delta R.T.: -0.035 min
Response: 21056819
Conc: 35.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
PLASTIC-COAT

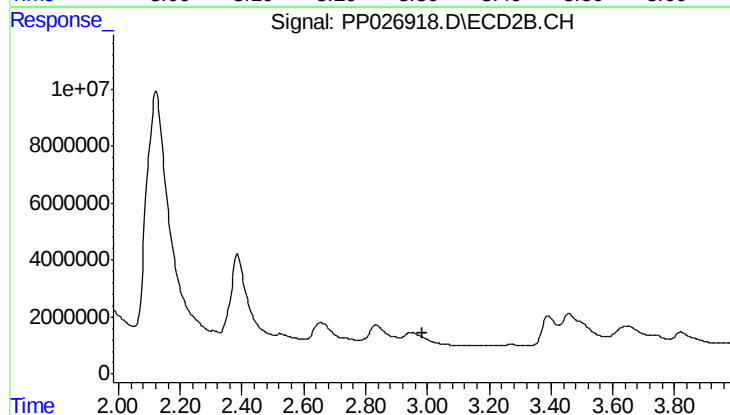


#1 Dalapon

R.T.: 0.000 min
Exp R.T.: 2.982 min
Response: 0
Conc: N.D.

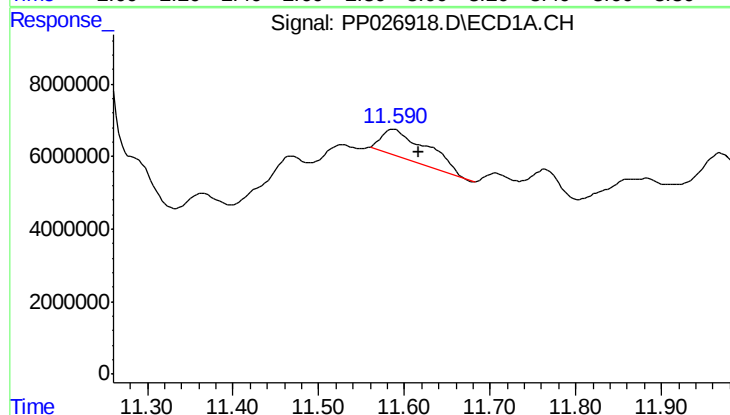


#3 4-Nitrophenol

R.T.: 11.588 min
Delta R.T.: -0.028 min
Response: 29601078
Conc: 64.54 ng/ml

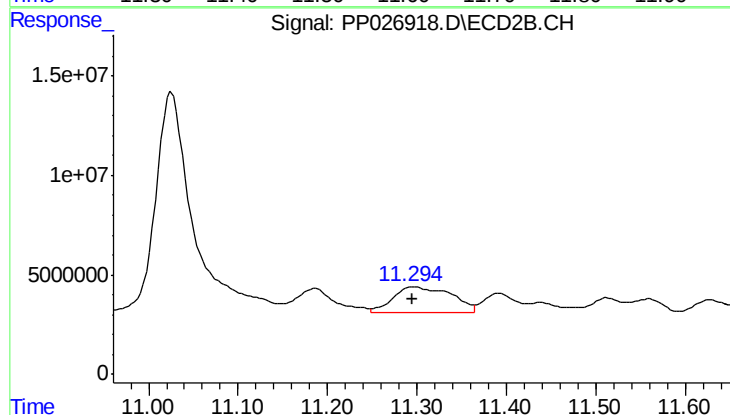

#3 4-Nitrophenol


R.T.: 11.296 min
Delta R.T.: 0.001 min
Response: 57805598
Conc: 238.63 ng/ml

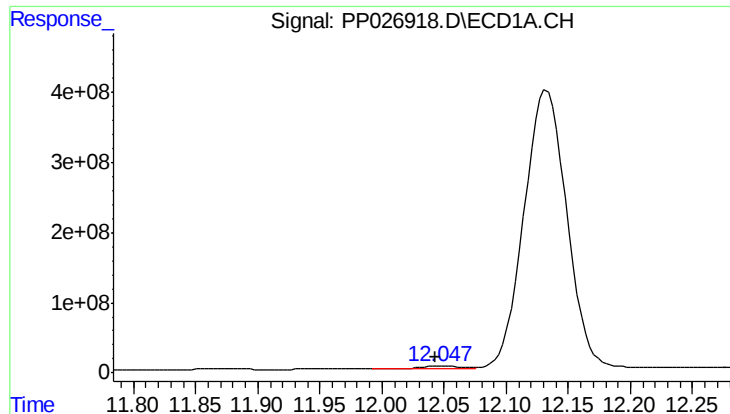

#4 2,4-DCAA


R.T.: 12.049 min
Delta R.T.: 0.006 min
Response: 82715804
Conc: 346.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
PLASTIC-COAT

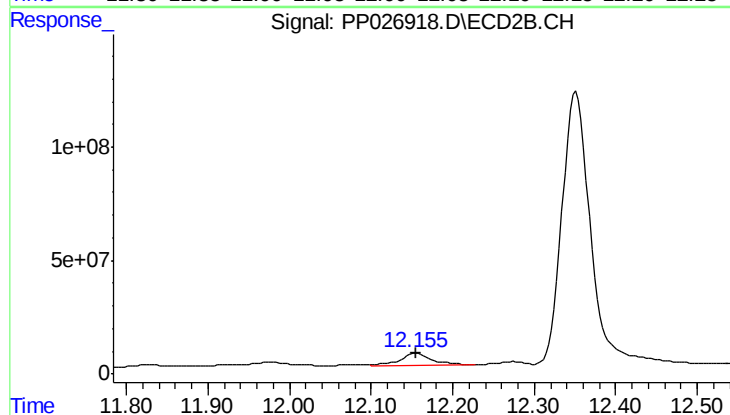


#4 2,4-DCAA

R.T.: 12.156 min
Delta R.T.: 0.000 min
Response: 139482905
Conc: 344.46 ng/ml

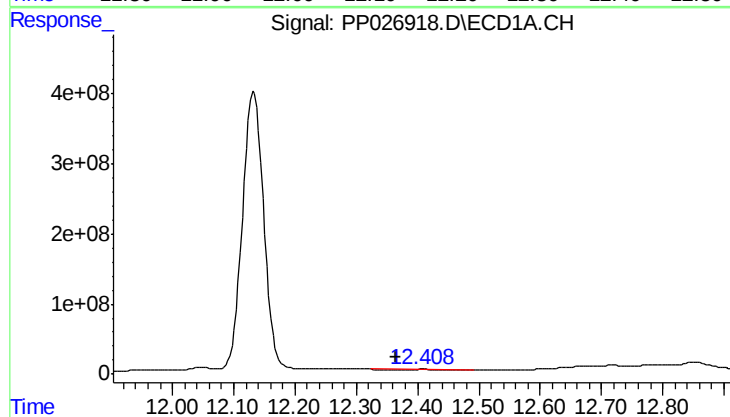


#5 DICAMBA

R.T.: 12.410 min
Delta R.T.: 0.044 min
Response: 12323537
Conc: 8.72 ng/ml

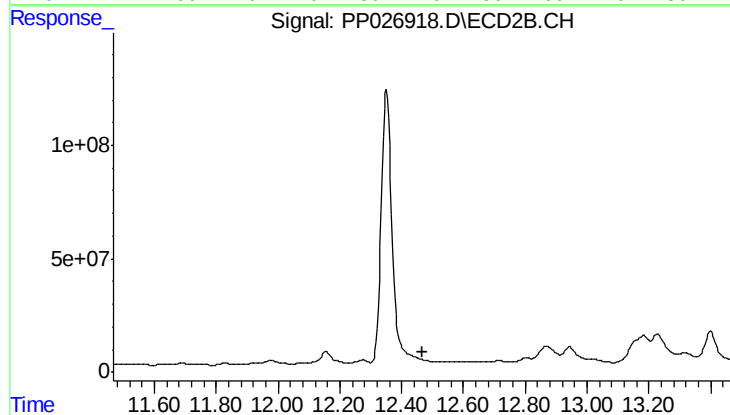

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 12.467 min
Response: 0
Conc: N.D.

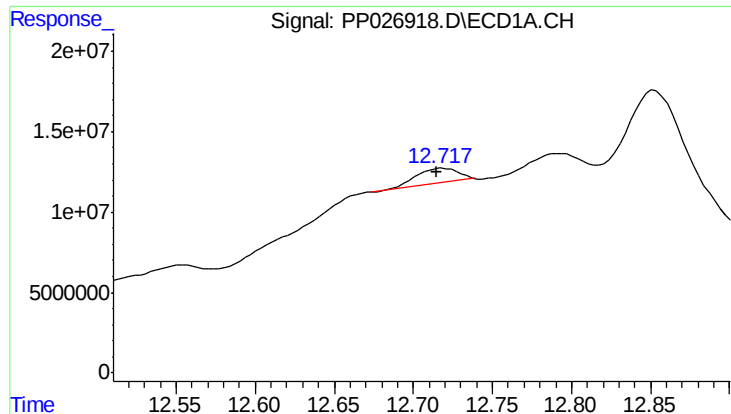

#6 MCPP


R.T.: 12.719 min
Delta R.T.: 0.004 min
Response: 18180570
Conc: 46.86 ug/ml

Instrument :
ECD_P
ClientSampleId :
PLASTIC-COAT

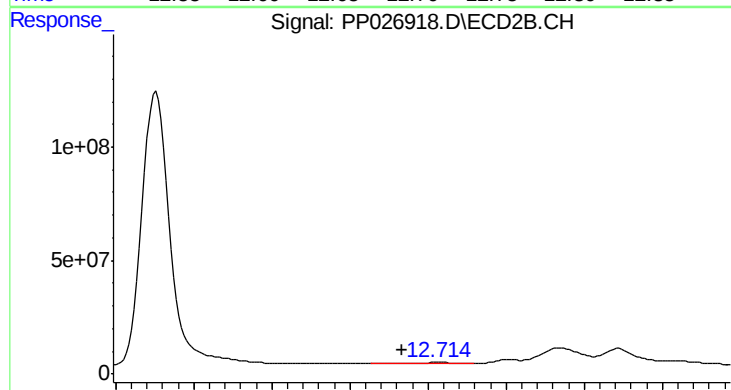


#6 MCPP

R.T.: 12.715 min
Delta R.T.: 0.048 min
Response: 7426164
Conc: 8.62 ug/ml

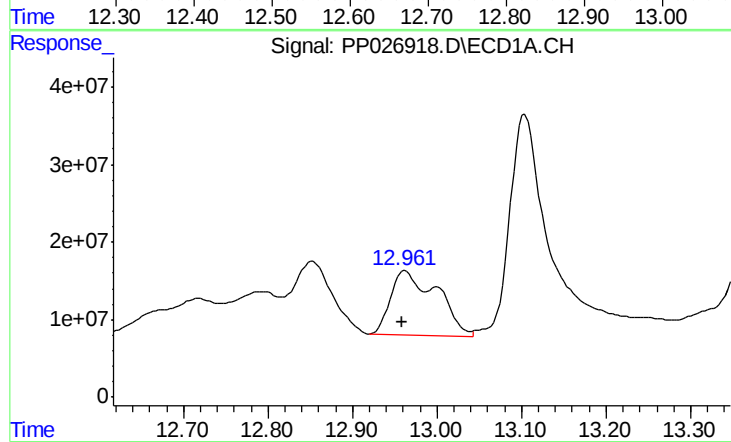


#7 MCPA

R.T.: 12.963 min
Delta R.T.: 0.004 min
Response: 315718679
Conc: 470.49 ug/ml

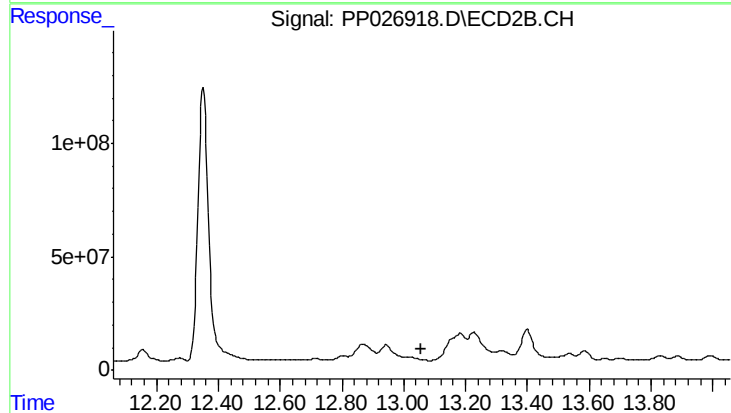

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 13.057 min
Response: 0
Conc: N.D.

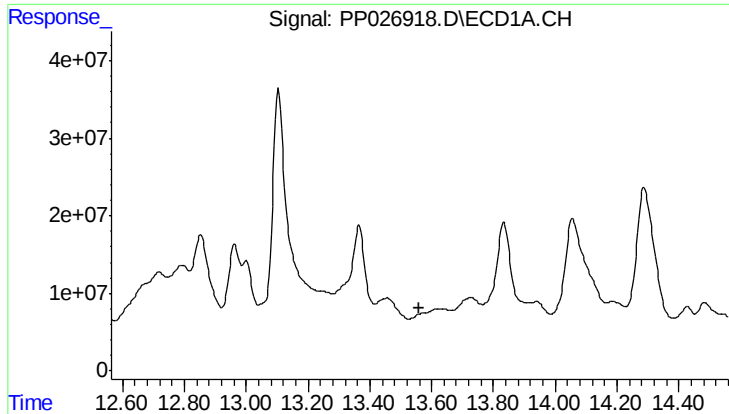

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.562 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PLASTIC-COAT

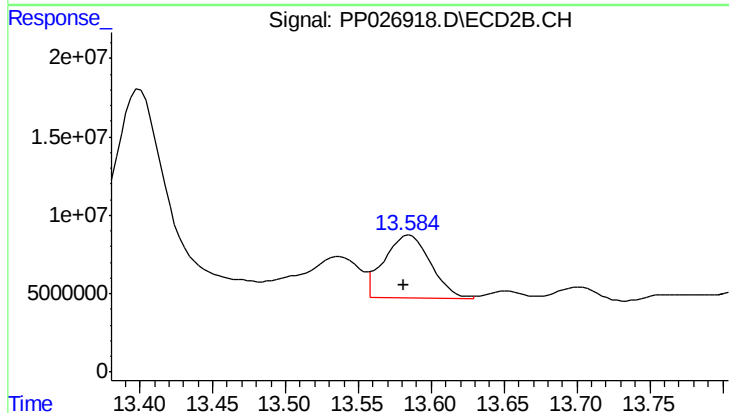


#8 DICHLORPROP

R.T.: 13.585 min
Delta R.T.: 0.004 min
Response: 90913299
Conc: 234.24 ng/ml

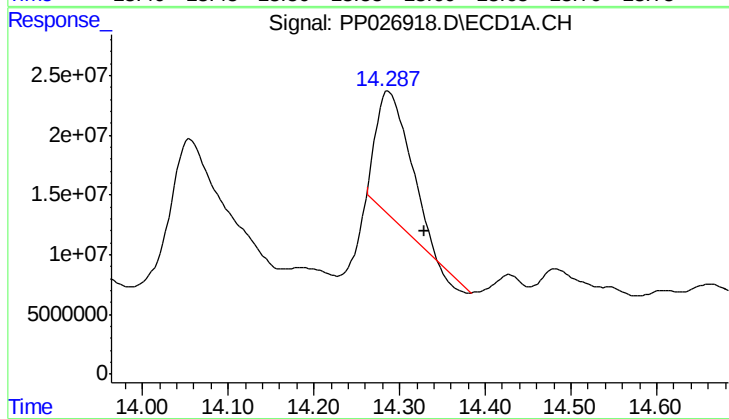


#10 Pentachlorophenol

R.T.: 14.288 min
Delta R.T.: -0.041 min
Response: 281030378
Conc: 36.92 ng/ml

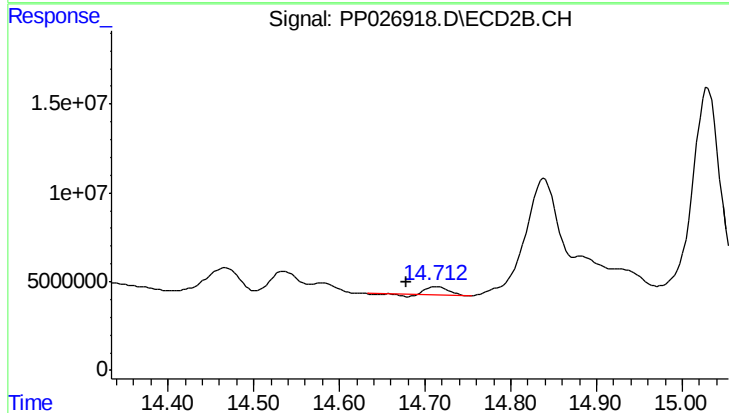

#10 Pentachlorophenol


R.T.: 14.714 min
Delta R.T.: 0.035 min
Response: 8952993
Conc: 1.34 ng/ml

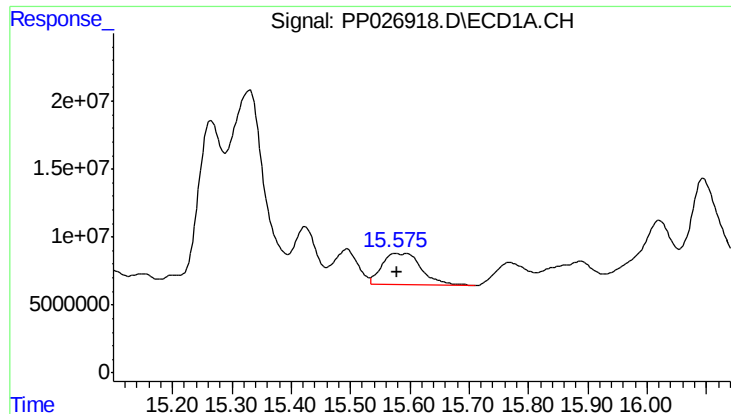

#12 2,4,5-T


R.T.: 15.579 min
Delta R.T.: 0.000 min
Response: 106606029
Conc: 41.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
PLASTIC-COAT

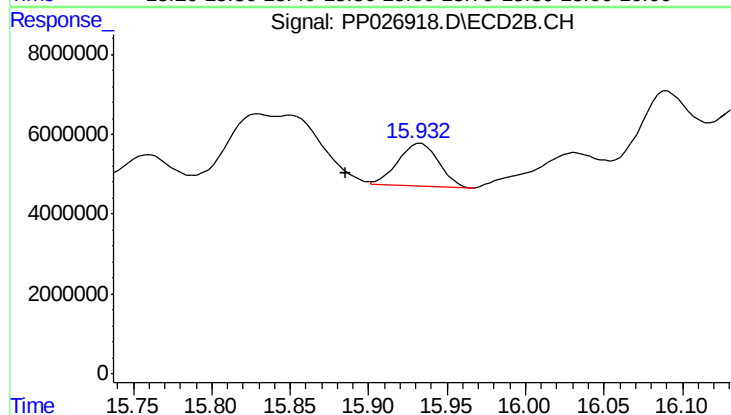


#12 2,4,5-T

R.T.: 15.933 min
Delta R.T.: 0.047 min
Response: 19322887
Conc: 8.87 ng/ml

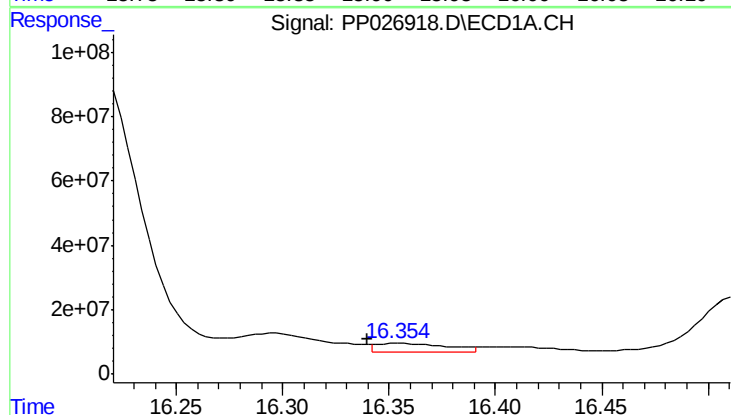


#13 2,4-DB

R.T.: 16.355 min
Delta R.T.: 0.015 min
Response: 61413995
Conc: 280.86 ng/ml

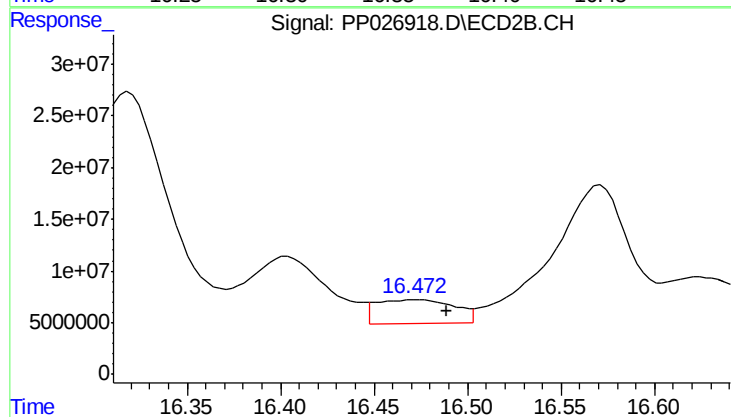

#13 2,4-DB


R.T.: 16.472 min
Delta R.T.: -0.017 min
Response: 66704994
Conc: 234.09 ng/ml

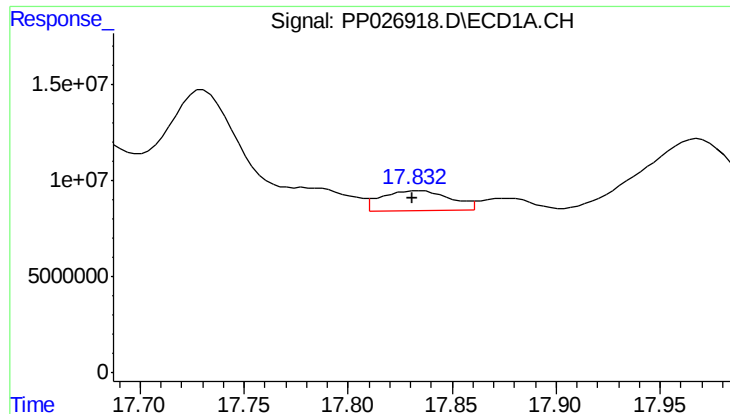

#14 DINOSEB


R.T.: 17.833 min
Delta R.T.: 0.002 min
Response: 22963807
Conc: 11.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
PLASTIC-COAT

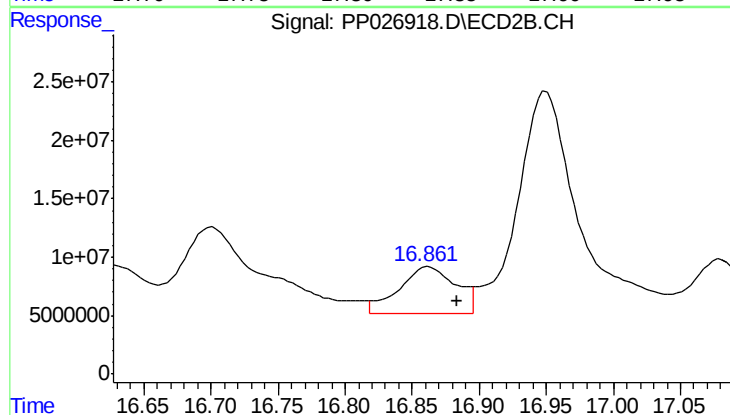


#14 DINOSEB

R.T.: 16.863 min
Delta R.T.: -0.021 min
Response: 118824685
Conc: 65.84 ng/ml

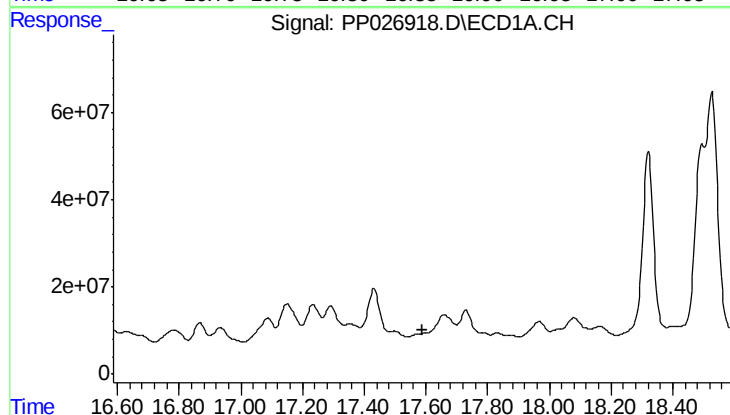


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.587 min
Response: 0
Conc: N.D.

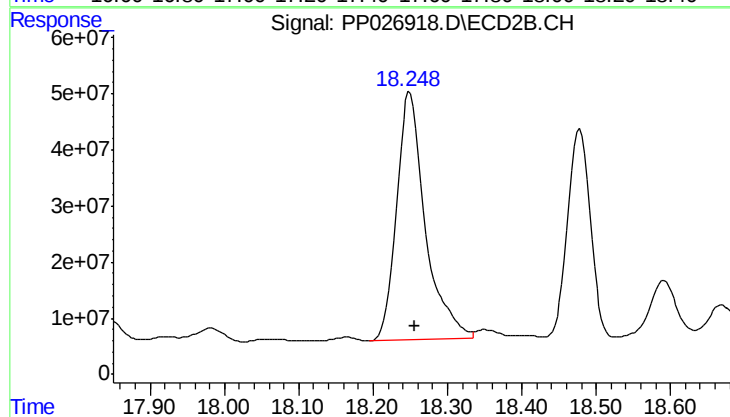

#15 Picloram


R.T.: 18.250 min
Delta R.T.: -0.006 min
Response: 1189305995
Conc: 344.83 ng/ml

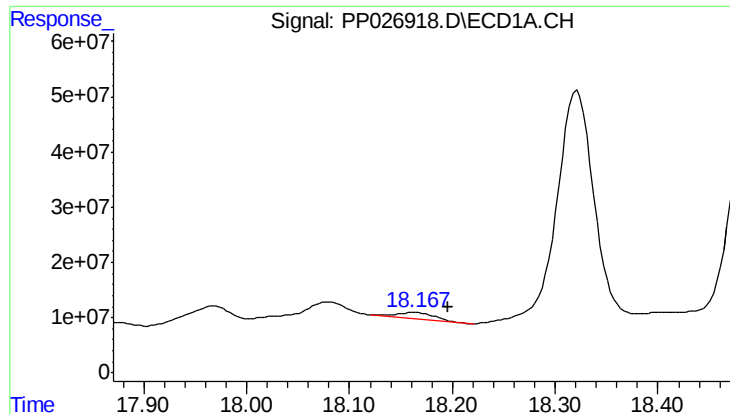

#16 DCPA

R.T.: 18.163 min
Delta R.T.: -0.032 min
Response: 25142735
Conc: 6.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
PLASTIC-COAT

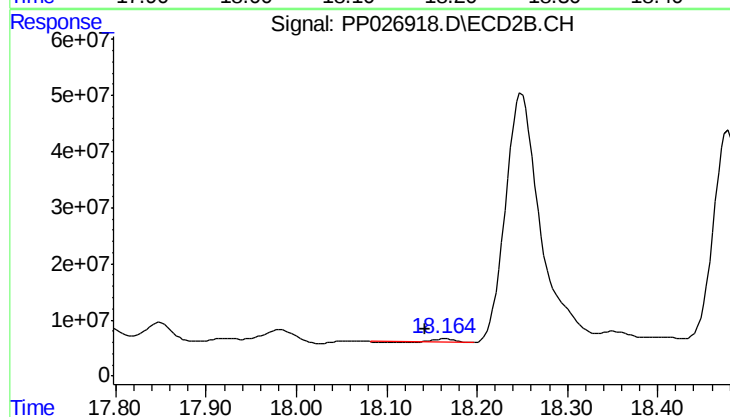

#16 DCPA

R.T.: 18.164 min
Delta R.T.: 0.021 min
Response: 10145699
Conc: 3.15 ng/ml