

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP073020\
 Data File : PP030741.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jul 2020 8:30
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 17:24:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072820.M
 Quant Title : 8080.M
 QLast Update : Wed Jul 29 01:54:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
5) T	DICAMBA	0.000	11.289	0	4318929	N.D. 2.510 #
7) T	MCPA	0.000	11.763	0	48695549	N.D. 23.903 #
13) T	2,4-DB	0.000	15.201	0	1379658	N.D. 4.722 #
15) T	Picloram	16.124	0.000	29067691	0	7.921 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP073020\
Data File : PP030741.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jul 2020 8:30
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 17:24:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP072820.M
Quant Title : 8080.M
QLast Update : Wed Jul 29 01:54:31 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

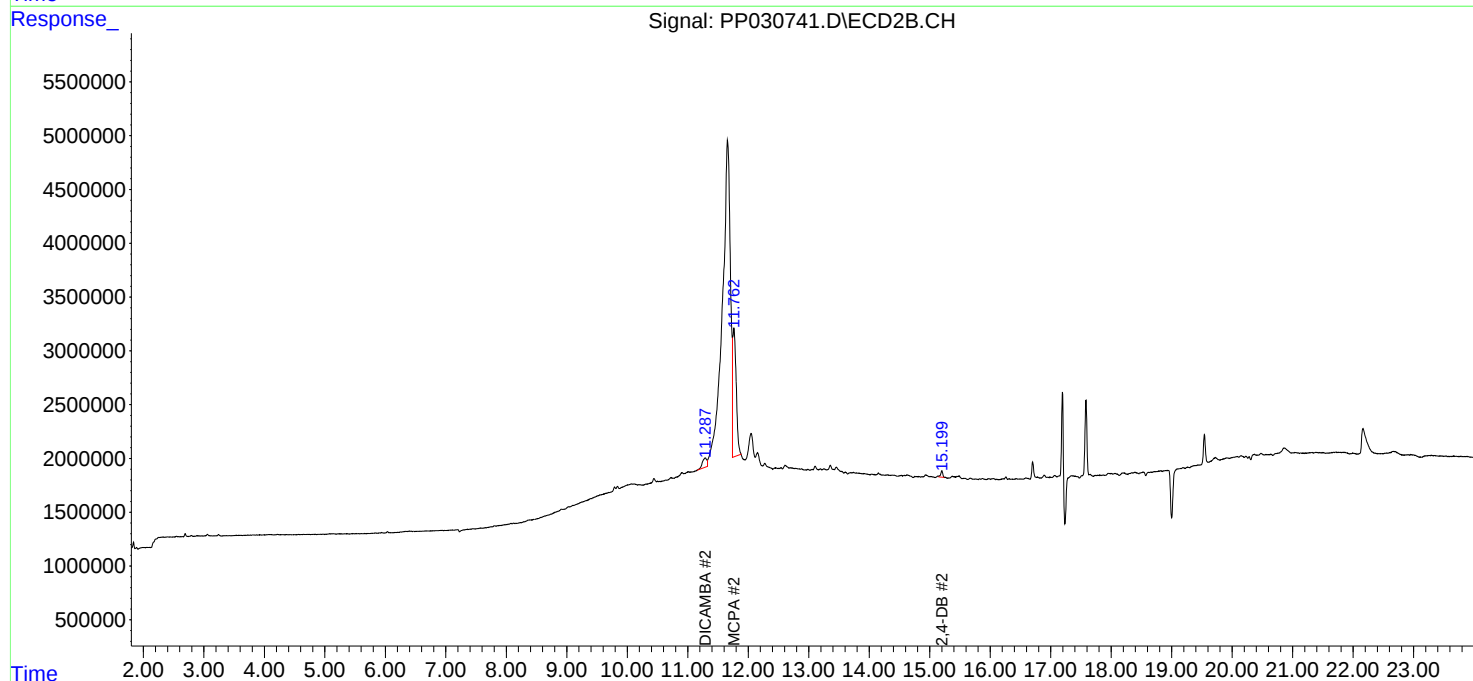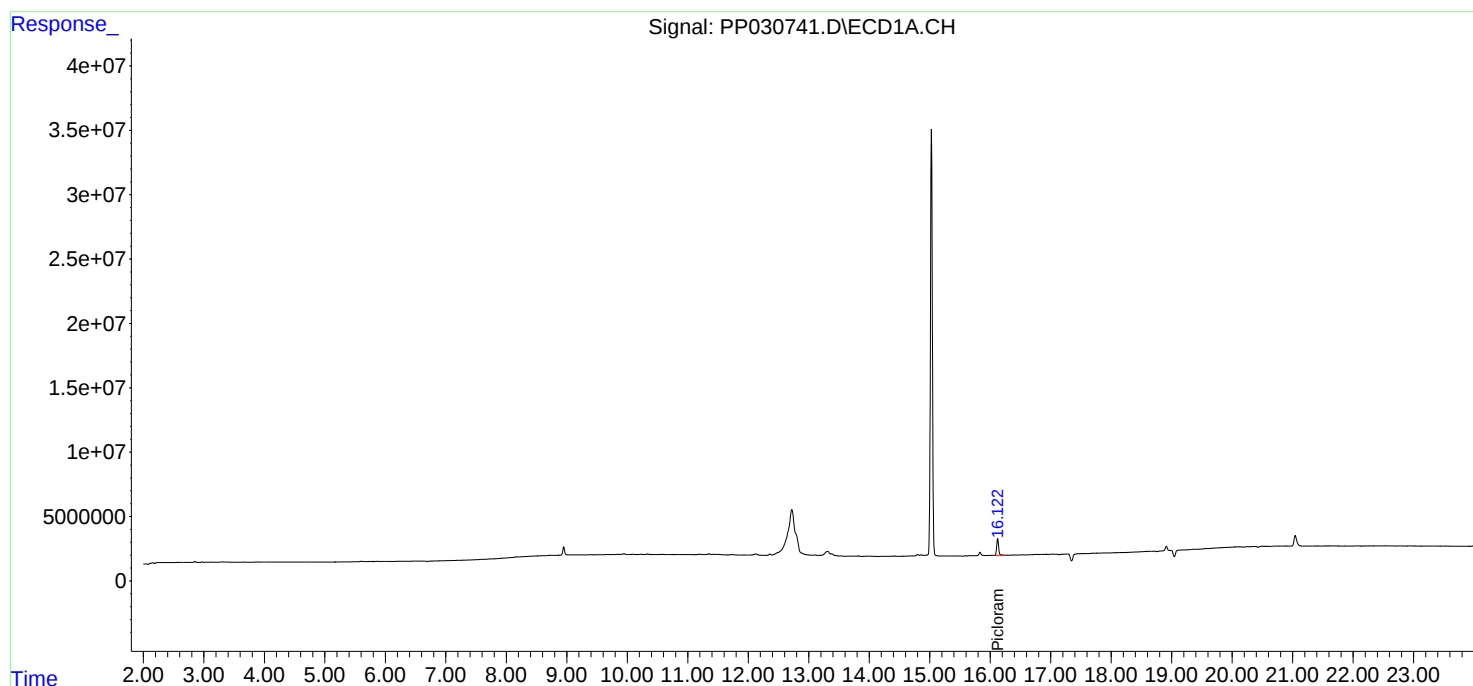


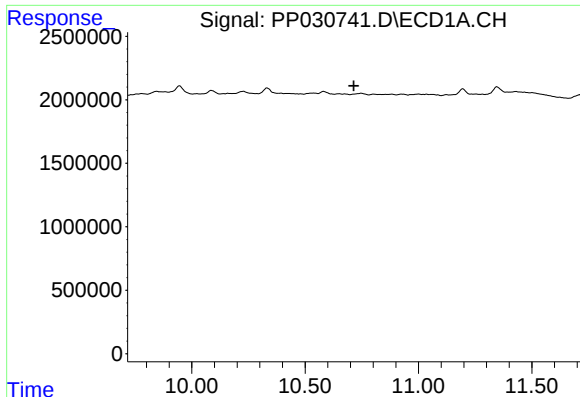

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 10.715 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

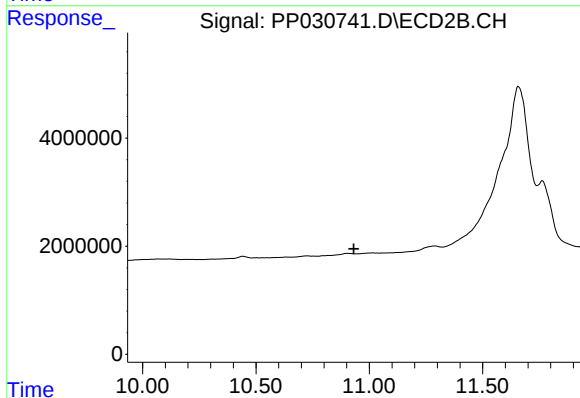


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 10.931 min
Response: 0
Conc: N.D.

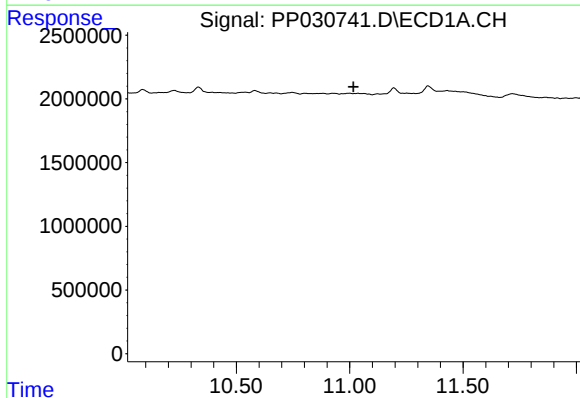


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.017 min
Response: 0
Conc: N.D.

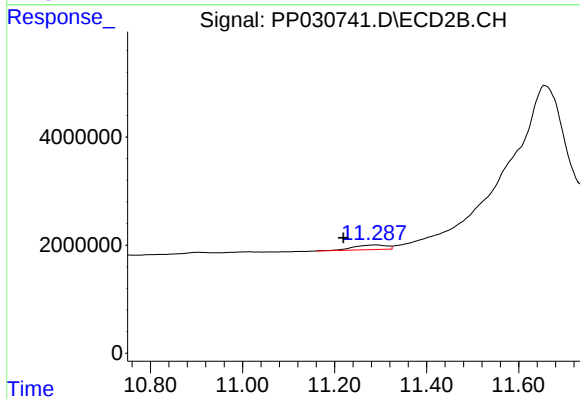

#5 DICAMBA


R.T.: 11.289 min
Delta R.T.: 0.070 min
Response: 4318929
Conc: 2.51 ng/ml

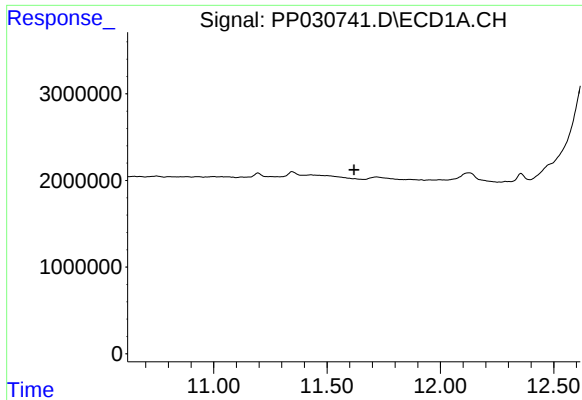

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.620 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

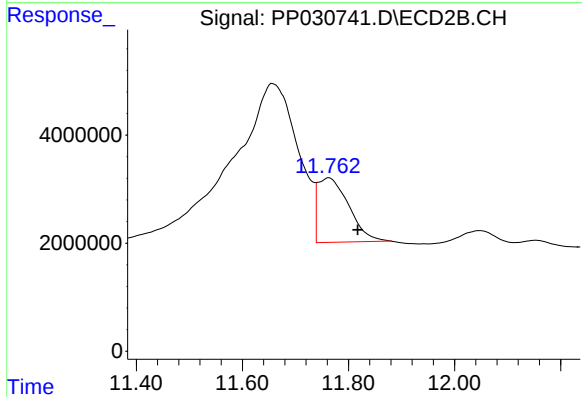


#7 MCPA

R.T.: 11.763 min
Delta R.T.: -0.054 min
Response: 48695549
Conc: 23.90 ug/ml

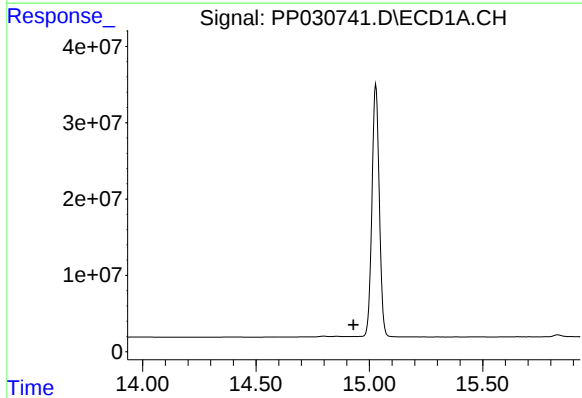


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 14.930 min
Response: 0
Conc: N.D.

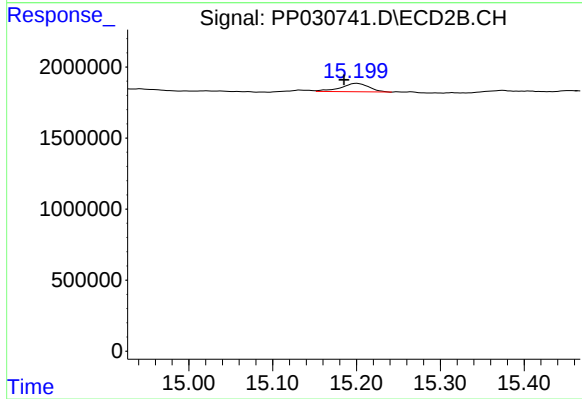

#13 2,4-DB


R.T.: 15.201 min
Delta R.T.: 0.016 min
Response: 1379658
Conc: 4.72 ng/ml

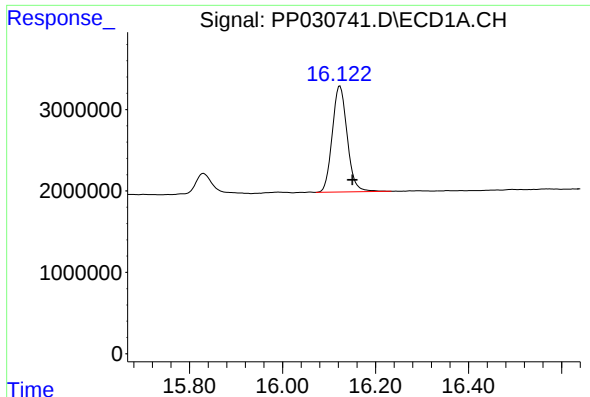

#15 Picloram

R.T.: 16.124 min
Delta R.T.: -0.027 min
Response: 29067691
Conc: 7.92 ng/ml

Instrument :
ECD_P
ClientSampleId :

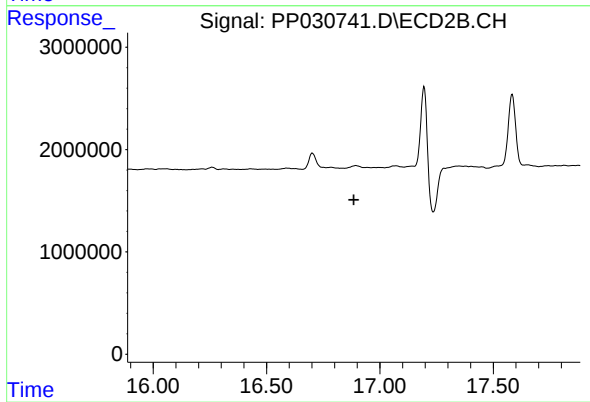

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.885 min
Response: 0
Conc: N.D.