

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080122\
 Data File : PP050024.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2022 17:26
 Operator : YP\AJ
 Sample : N3978-02 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KMH5050-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/02/2022
 Supervised By :Ankita Jodhani 08/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:54:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 14 06:08:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.349	3.599	1434406	1918379	0.988m	0.785m
2) SA Decachlor...	10.099	8.564	2044554	1571923	1.446m	1.350

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080122\
Data File : PP050024.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2022 17:26
Operator : YP\AJ
Sample : N3978-02 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KMH5050-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/02/2022
Supervised By :Ankita Jodhani 08/02/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:54:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 14 06:08:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

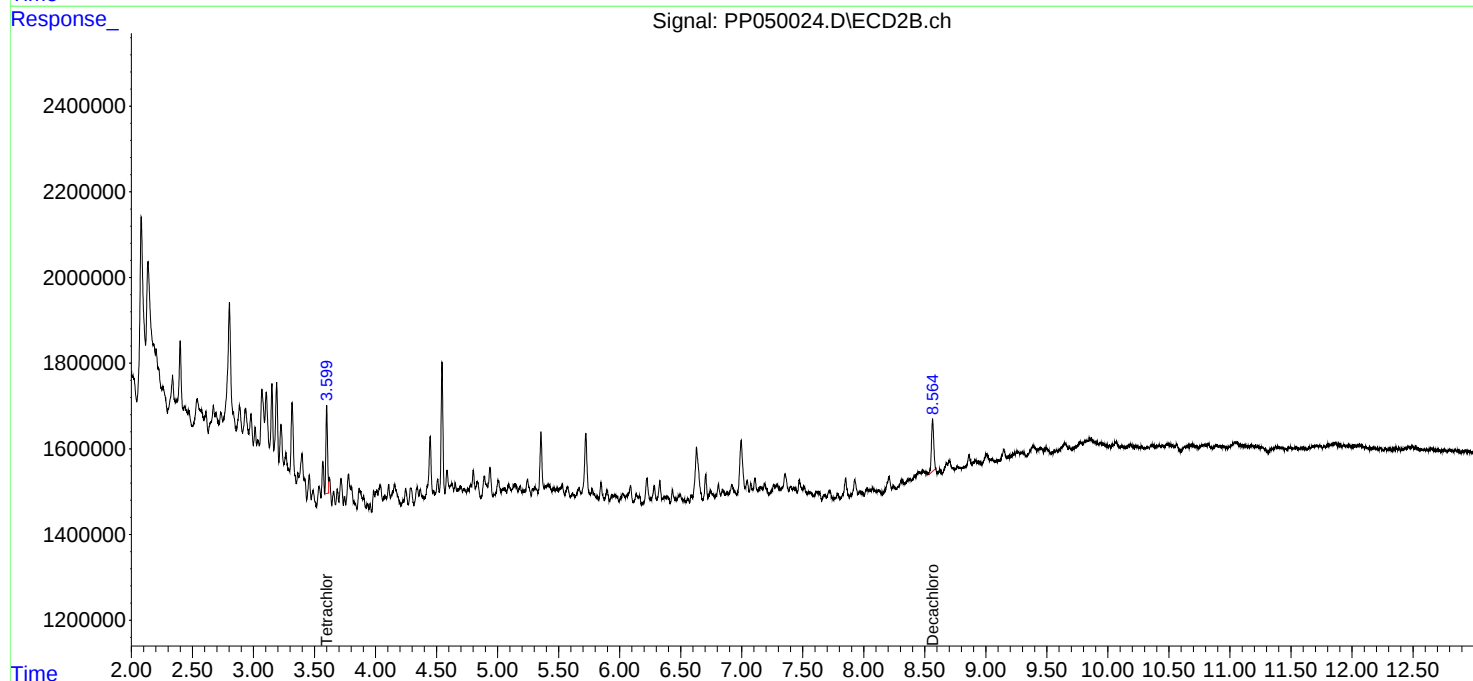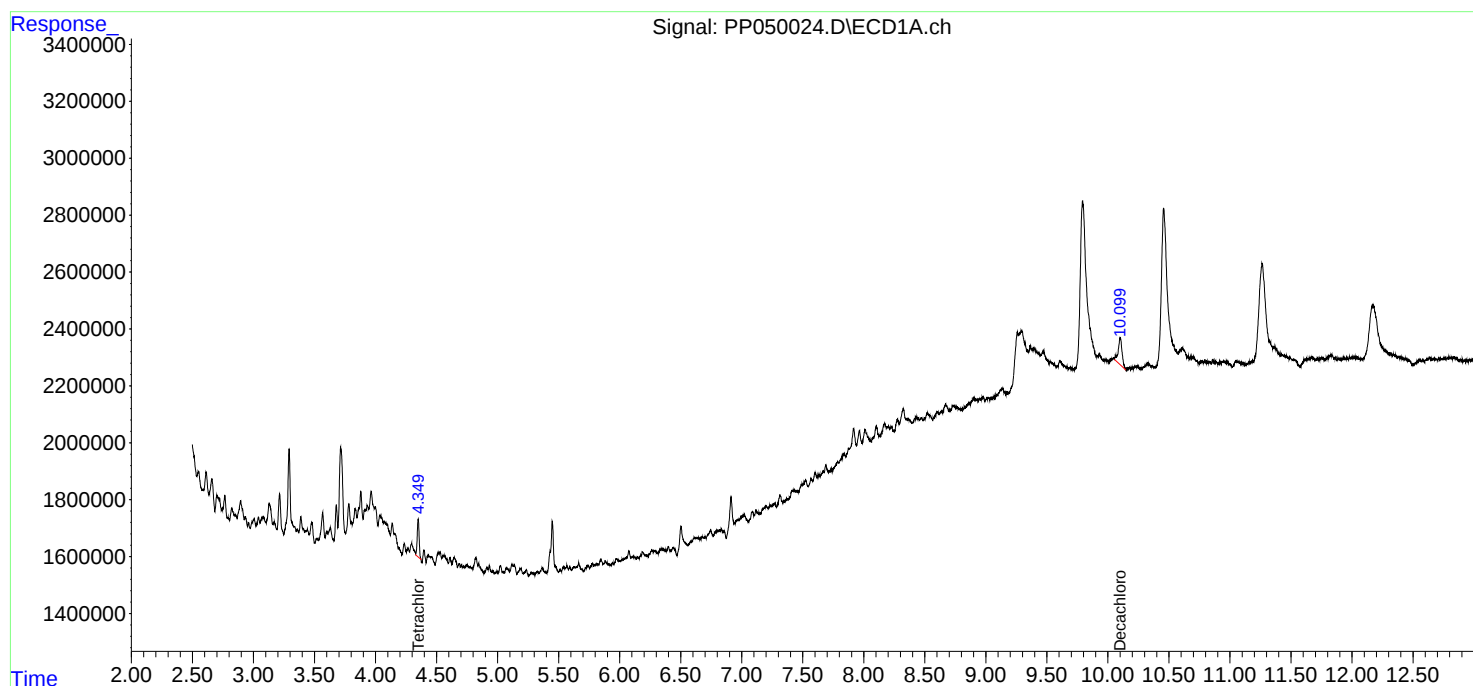

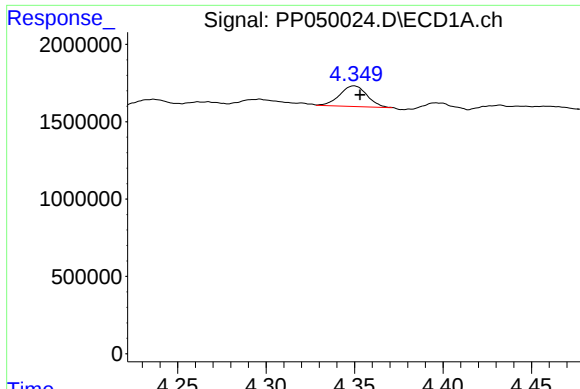


#1 Tetrachloro-m-xylene

R.T.: 4.349 min
Delta R.T.: -0.004 min
Response: 1434406
Conc: 0.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
KMH5050-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/02/2022
Supervised By :Ankita Jodhani 08/02/2022

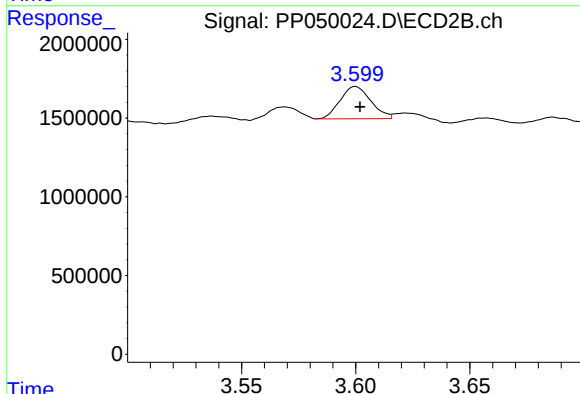


#1 Tetrachloro-m-xylene

R.T.: 3.599 min
Delta R.T.: -0.003 min
Response: 1918379
Conc: 0.78 ng/ml m

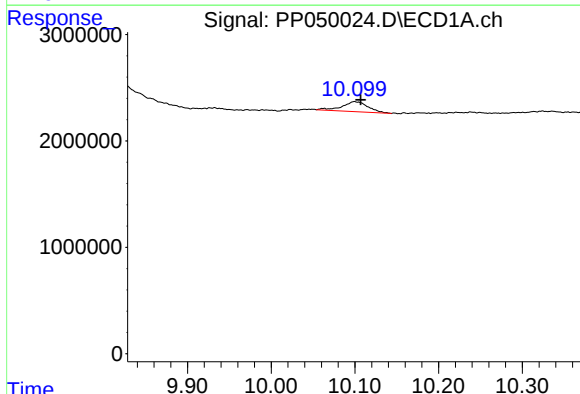

#2 Decachlorobiphenyl

R.T.: 10.099 min
Delta R.T.: -0.008 min
Response: 2044554
Conc: 1.45 ng/ml m

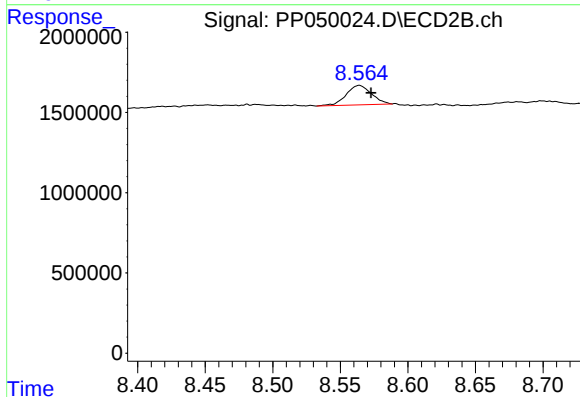

#2 Decachlorobiphenyl

R.T.: 8.564 min
Delta R.T.: -0.009 min
Response: 1571923
Conc: 1.35 ng/ml