

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080122\
 Data File : PP050026.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2022 18:00
 Operator : YP\AJ
 Sample : N3978-04 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JEH75651-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/02/2022
 Supervised By :Ankita Jodhani 08/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:55:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 14 06:08:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.350	3.599	2364636	4023382	1.630m	1.646
2) SA Decachlor...	10.104	8.565	2265432	1815588	1.602	1.559m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080122\
Data File : PP050026.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2022 18:00
Operator : YP\AJ
Sample : N3978-04 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
JEH75651-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/02/2022
Supervised By :Ankita Jodhani 08/02/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:55:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 14 06:08:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

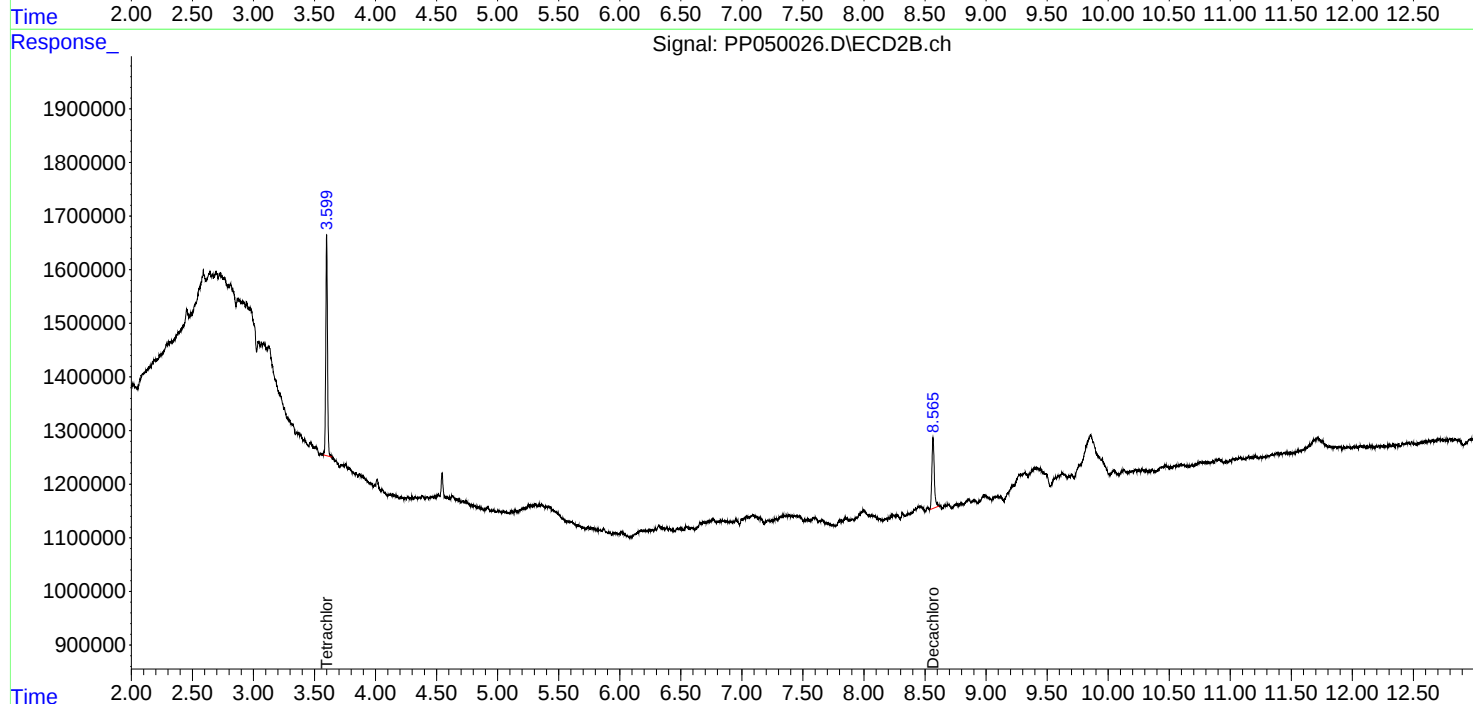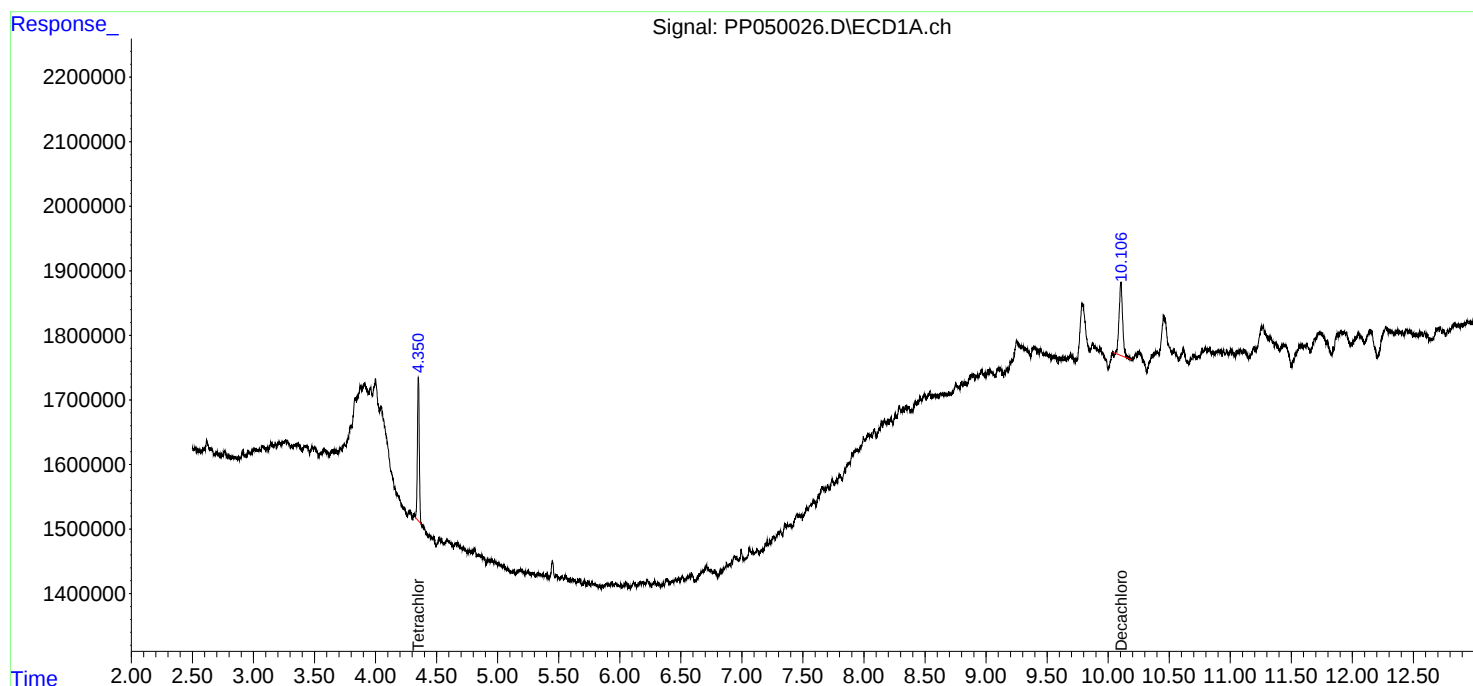

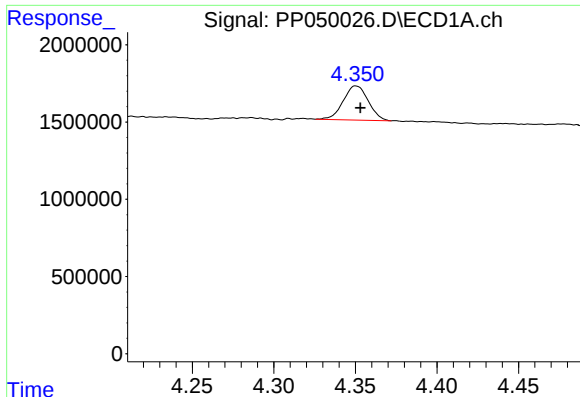


#1 Tetrachloro-m-xylene

R.T.: 4.350 min
Delta R.T.: -0.003 min
Response: 2364636
Conc: 1.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
JEH75651-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/02/2022
Supervised By :Ankita Jodhani 08/02/2022

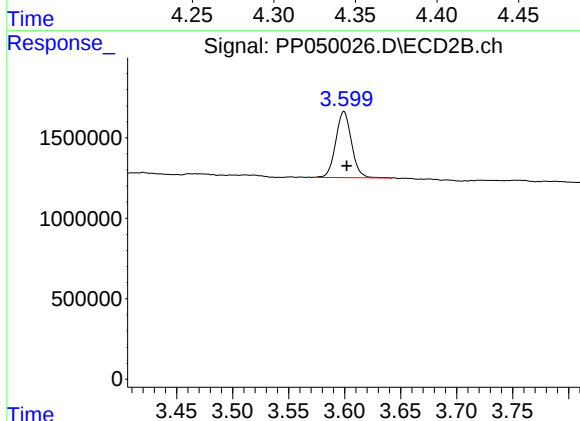


#1 Tetrachloro-m-xylene

R.T.: 3.599 min
Delta R.T.: -0.003 min
Response: 4023382
Conc: 1.65 ng/ml

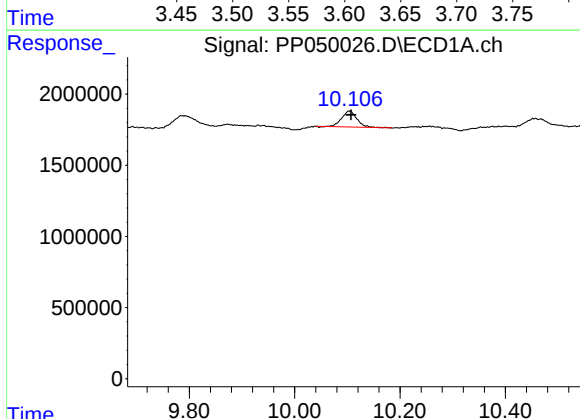

#2 Decachlorobiphenyl

R.T.: 10.104 min
Delta R.T.: -0.003 min
Response: 2265432
Conc: 1.60 ng/ml

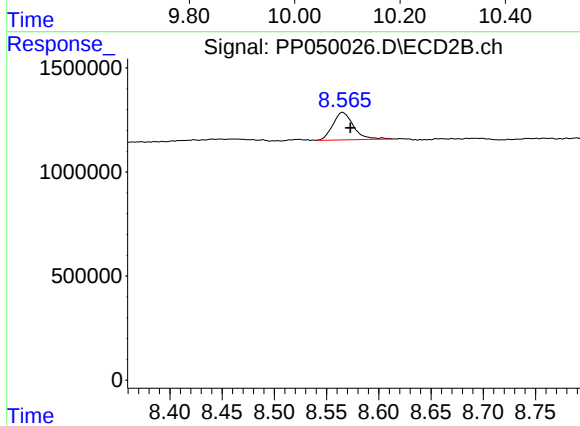

#2 Decachlorobiphenyl

R.T.: 8.565 min
Delta R.T.: -0.008 min
Response: 1815588
Conc: 1.56 ng/ml m