

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2025 00:15
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:37:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:33:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.686f	3.799	7999033	48858	7.153	0.013 #
2)	SA Decachlor...	10.440	8.798	119003	5121819	0.123	0.852 #
Target Compounds							
3)	L1 AR-1016-1	5.831	4.908	2208830	3086177	53.539	7.737 #
4)	L1 AR-1016-2	5.831	4.966	2208830	4476264	36.364	23.834 #
5)	L1 AR-1016-3	5.854f	5.077	7507165	9252788	189.286	87.233 #
6)	L1 AR-1016-4	0.000	5.131	0	4049980	N.D.	37.081 #
7)	L1 AR-1016-5	6.299	5.318	8162337	5512063	251.396	47.126 #
8)	L2 AR-1221-1	4.834	4.013	175950	3015870	10.496	61.442 #
9)	L2 AR-1221-2	4.966	4.095	228856	2236587	18.162	62.319 #
10)	L2 AR-1221-3	5.015	4.178	463155	2437386	12.642	18.025 #
11)	L3 AR-1232-1	5.015	4.178	463155	2437386	15.950	24.046 #
12)	L3 AR-1232-2	5.559	4.908	868399	3086177	57.729	17.710 #
13)	L3 AR-1232-3	5.831	5.077	2208830	9252788	76.162	201.953 #
14)	L3 AR-1232-4	0.000	5.165	0	2977301	N.D.	51.323 #
15)	L3 AR-1232-5	6.106	5.318	2329803	5512063	198.856	117.329 #
16)	L4 AR-1242-1	5.831	4.908	2208830	3086177	59.272	8.942 #
17)	L4 AR-1242-2	5.831	4.966	2208830	4476264	40.597	27.398 #
18)	L4 AR-1242-3	5.854f	5.077	7507165	9252788	210.074	100.303 #
19)	L4 AR-1242-4	0.000	5.165	0	2977301	N.D.	24.931 #
20)	L4 AR-1242-5	6.707	5.709	17788794	250.5E6	500.275	1675.013 #
21)	L5 AR-1248-1	5.831	4.908	2208830	3086177	78.846	14.426 #
22)	L5 AR-1248-2	6.106	5.131	2329803	4049980	57.867	27.680 #
23)	L5 AR-1248-3	6.299	5.165	8162337	2977301	183.121	17.364 #
24)	L5 AR-1248-4	6.707	5.318	17788794	5512063	341.848	33.131 #
25)	L5 AR-1248-5	6.707	5.709	17788794	250.5E6	312.395	860.977 #
26)	L6 AR-1254-1	6.651	5.709	49861768	250.5E6	947.203	684.127 #
27)	L6 AR-1254-2	6.863	5.850	11259682	10112293	141.623	36.347 #
28)	L6 AR-1254-3	7.224	6.247	152.8E6	26486054	1749.945	54.140 #
29)	L6 AR-1254-4	7.514	6.463	3160179	1559977	49.525	4.244 #
30)	L6 AR-1254-5	7.946	6.877	598.1E6	3623.7E6	7370.719	9218.418 #
31)	L7 AR-1260-1	7.395	6.525	10721881	516.5E6	190.252	1278.583 #
32)	L7 AR-1260-2	7.632	6.729	754.7E6	-4980182	11074.335	N.D. #
33)	L7 AR-1260-3	8.008	6.877f	3485848	3623.7E6	65.406	9194.476 #
34)	L7 AR-1260-4	8.224	7.183	3901854	230876	62.315	0.793 #
35)	L7 AR-1260-5	0.000	7.381f	0	1172412	N.D.	1.548 #
36)	L8 AR-1262-1	8.224	6.877f	3901854	3623.7E6	51.483	6434.803 #
37)	L8 AR-1262-2	0.000	7.183	0	230876	N.D.	0.576 #
38)	L8 AR-1262-3	8.887	7.722	83728	2108.9E6	0.890	5866.612 #
39)	L8 AR-1262-4	9.002	7.722f	138174	2108.9E6	1.897	3162.095 #
40)	L8 AR-1262-5	9.654	8.252	457241	372041	8.979	1.313 #
41)	L9 AR-1268-1	8.887	7.722	83728	2108.9E6	0.538	1934.274 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
Data File : PP074201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2025 00:15
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 01:37:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 02 01:33:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	9.002	7.722f	138174	2108.9E6	0.963	1987.013 #
43)	L9 AR-1268-3	0.000	7.954	0	2259280	N.D.	2.716 #
44)	L9 AR-1268-4	9.654	8.252	457241	372041	7.775	1.208 #
45)	L9 AR-1268-5	10.093	8.570	227469	445426	0.647	0.175 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
Data File : PP074201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2025 00:15
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 01:37:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 02 01:33:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

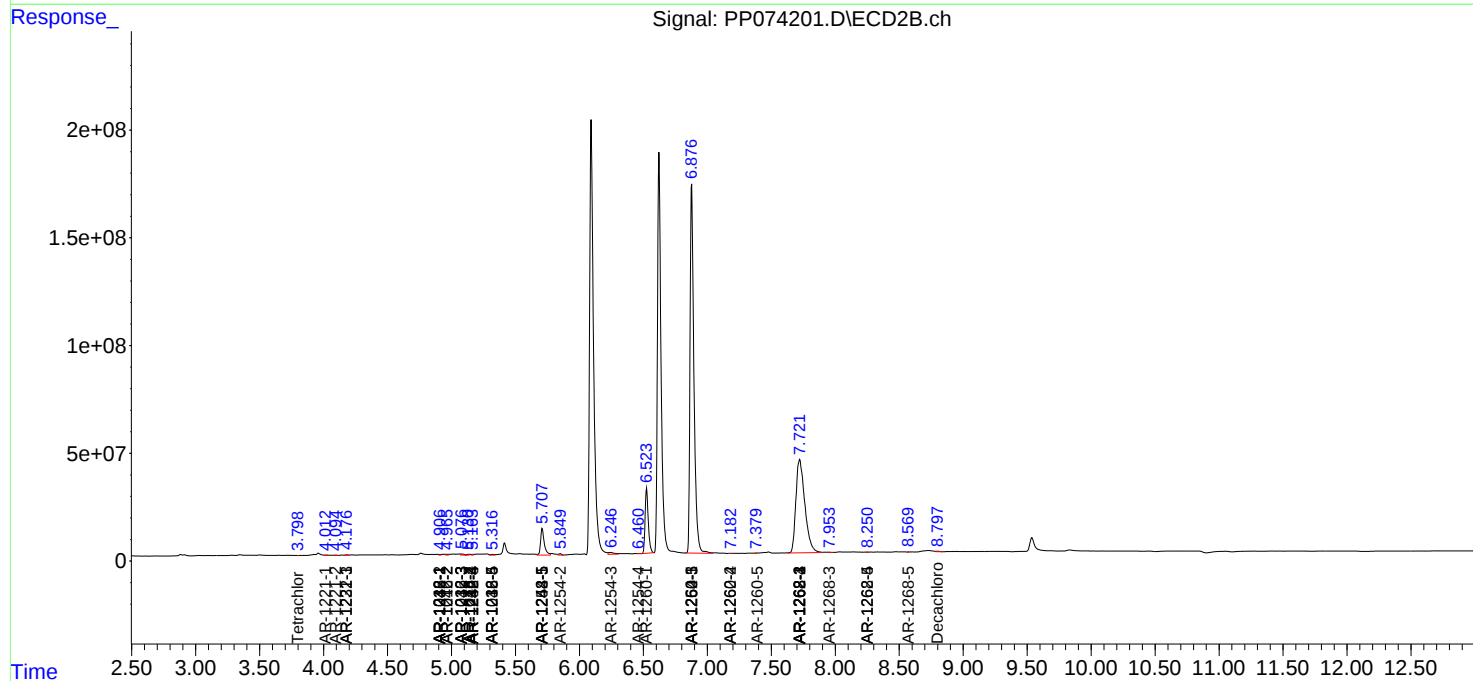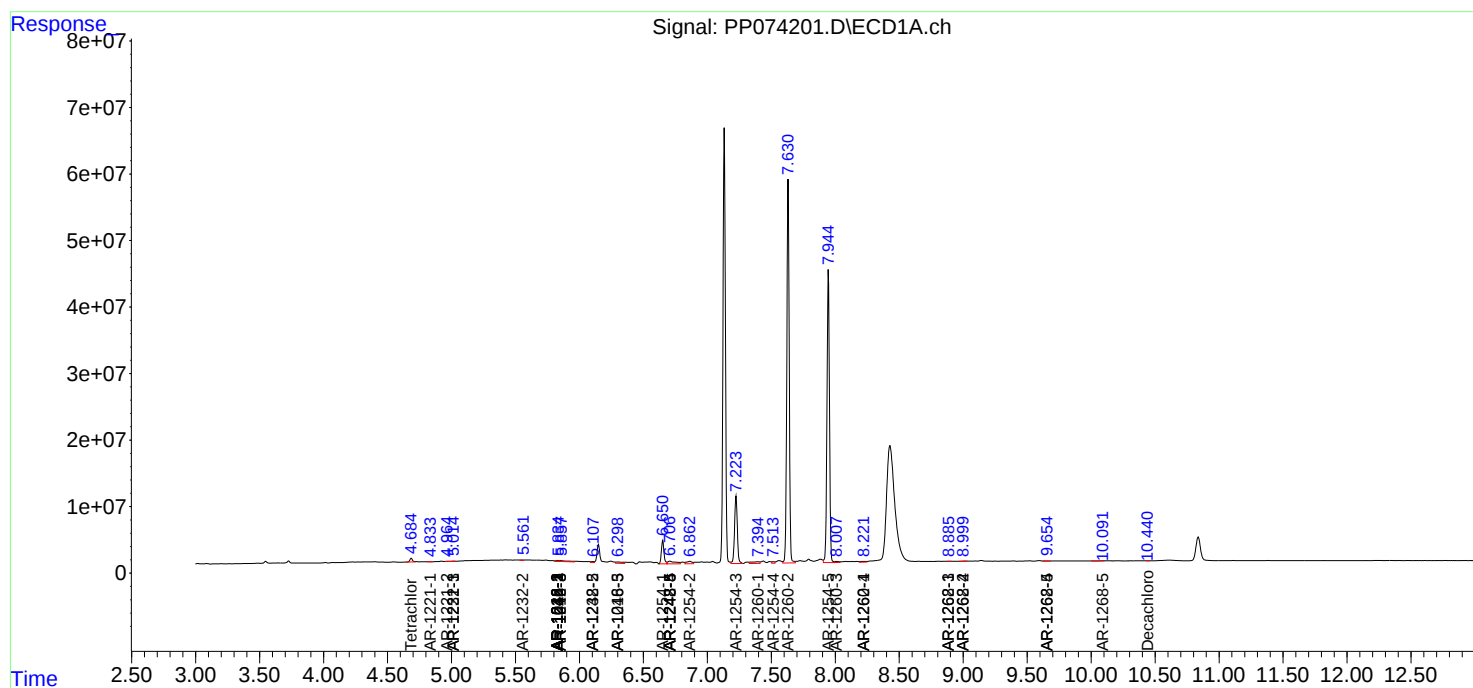


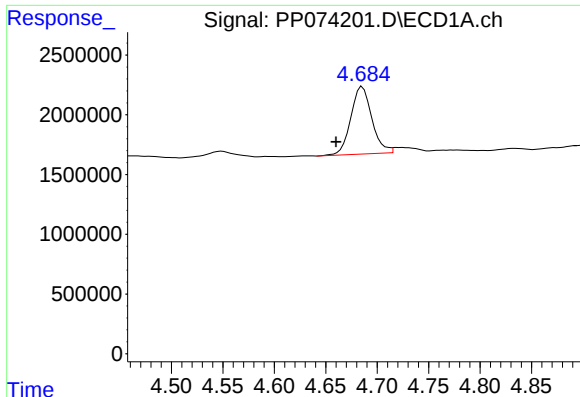

#1 Tetrachloro-m-xylene


R.T.: 4.686 min
Delta R.T.: 0.026 min
Response: 7999033
Conc: 7.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

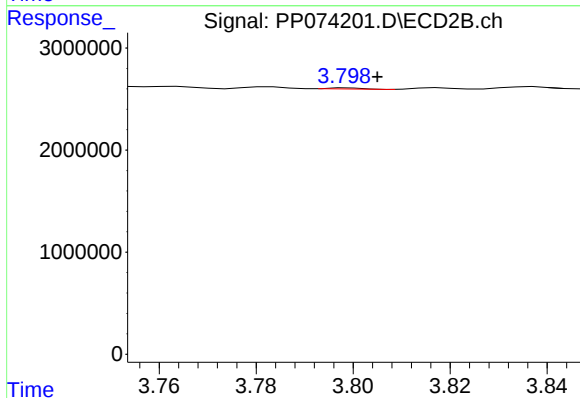


#1 Tetrachloro-m-xylene

R.T.: 3.799 min
Delta R.T.: -0.006 min
Response: 48858
Conc: 0.01 ng/ml

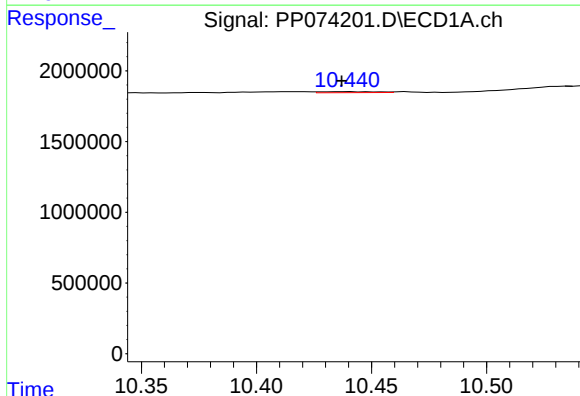


#2 Decachlorobiphenyl

R.T.: 10.440 min
Delta R.T.: 0.002 min
Response: 119003
Conc: 0.12 ng/ml

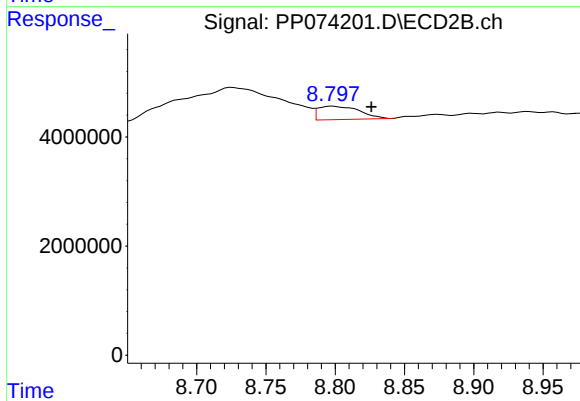

#2 Decachlorobiphenyl


R.T.: 8.798 min
Delta R.T.: -0.028 min
Response: 5121819
Conc: 0.85 ng/ml

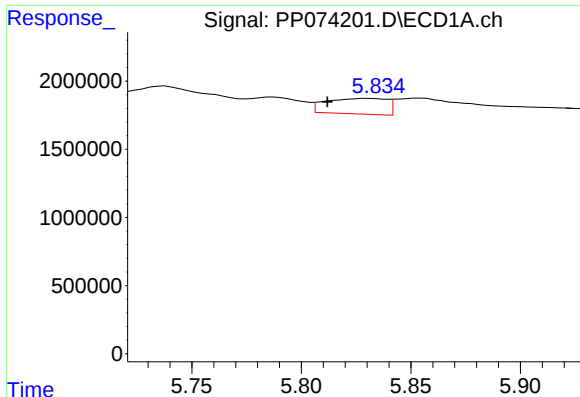

#3 AR-1016-1


R.T.: 5.831 min
Delta R.T.: 0.019 min
Response: 2208830
Conc: 53.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

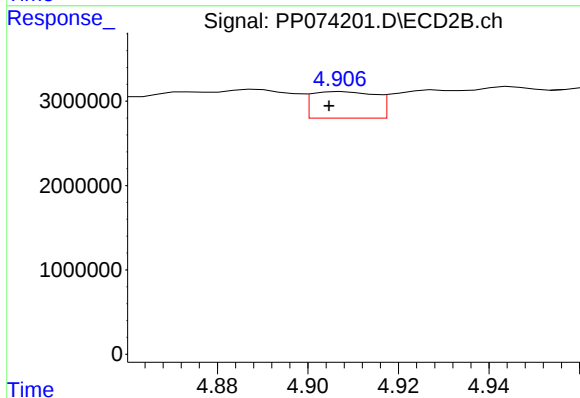


#3 AR-1016-1

R.T.: 4.908 min
Delta R.T.: 0.003 min
Response: 3086177
Conc: 7.74 ng/ml

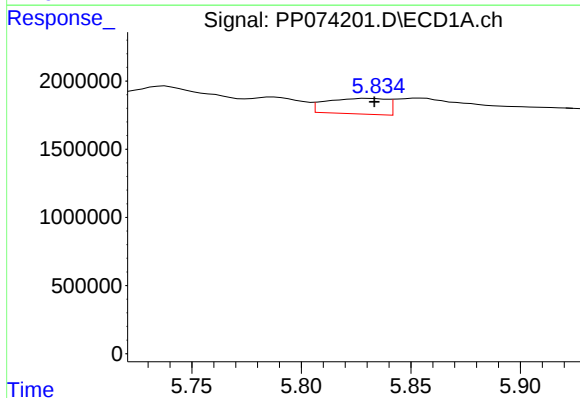


#4 AR-1016-2

R.T.: 5.831 min
Delta R.T.: -0.003 min
Response: 2208830
Conc: 36.36 ng/ml

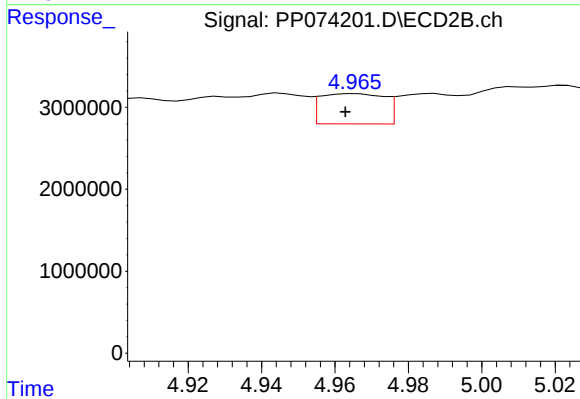

#4 AR-1016-2


R.T.: 4.966 min
Delta R.T.: 0.003 min
Response: 4476264
Conc: 23.83 ng/ml

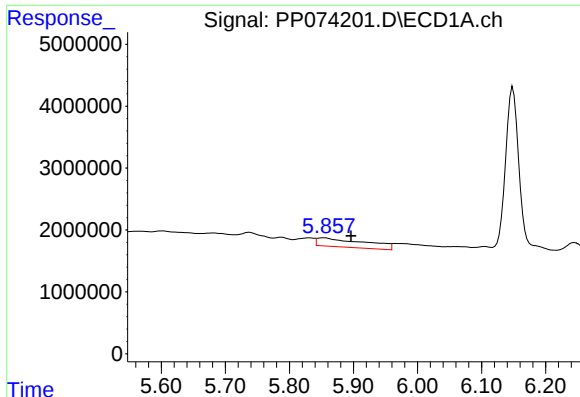

#5 AR-1016-3


R.T.: 5.854 min
Delta R.T.: -0.042 min
Response: 7507165
Conc: 189.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

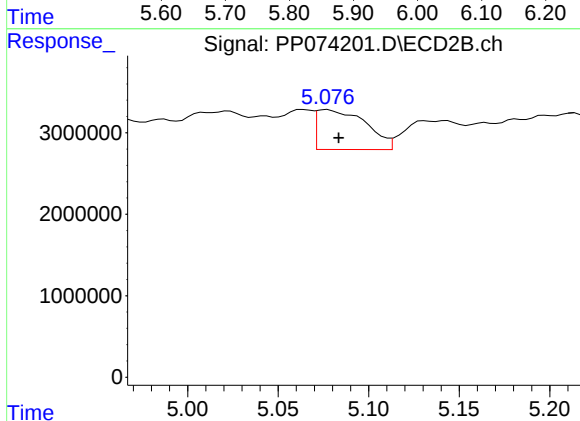


#5 AR-1016-3

R.T.: 5.077 min
Delta R.T.: -0.007 min
Response: 9252788
Conc: 87.23 ng/ml

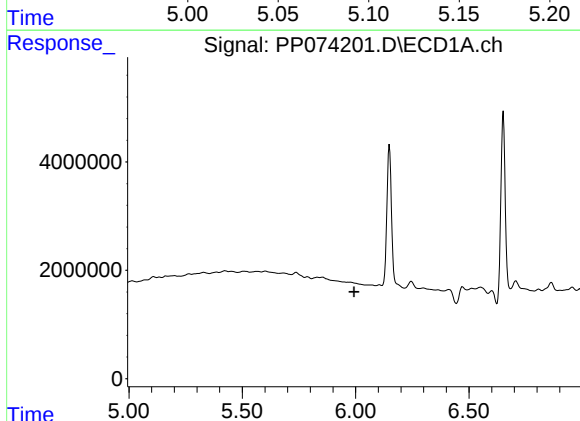


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.993 min
Response: 0
Conc: N.D.

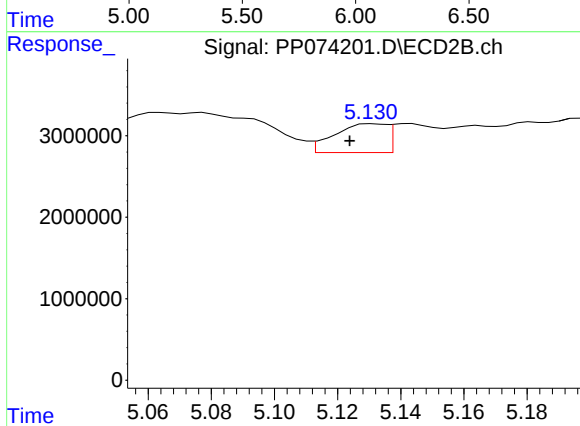

#6 AR-1016-4


R.T.: 5.131 min
Delta R.T.: 0.007 min
Response: 4049980
Conc: 37.08 ng/ml

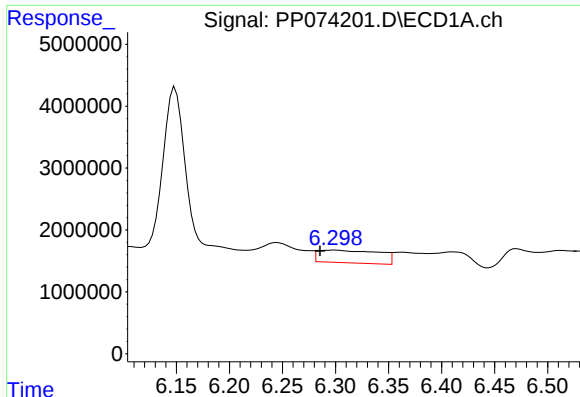

#7 AR-1016-5


R.T.: 6.299 min
Delta R.T.: 0.013 min
Response: 8162337
Conc: 251.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

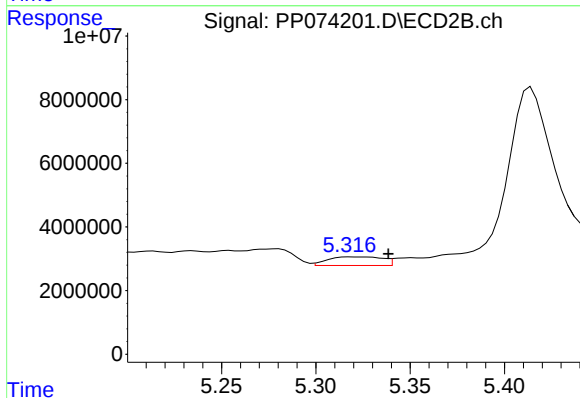


#7 AR-1016-5

R.T.: 5.318 min
Delta R.T.: -0.021 min
Response: 5512063
Conc: 47.13 ng/ml

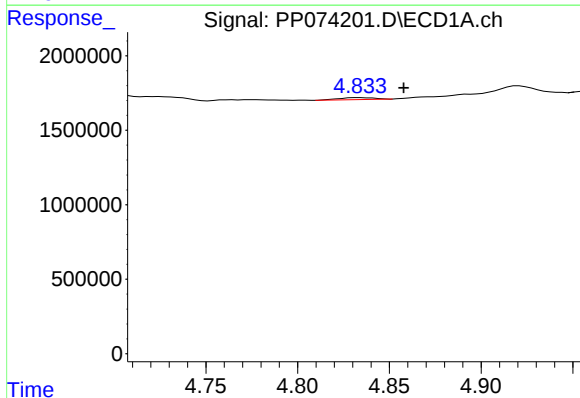


#8 AR-1221-1

R.T.: 4.834 min
Delta R.T.: -0.024 min
Response: 175950
Conc: 10.50 ng/ml

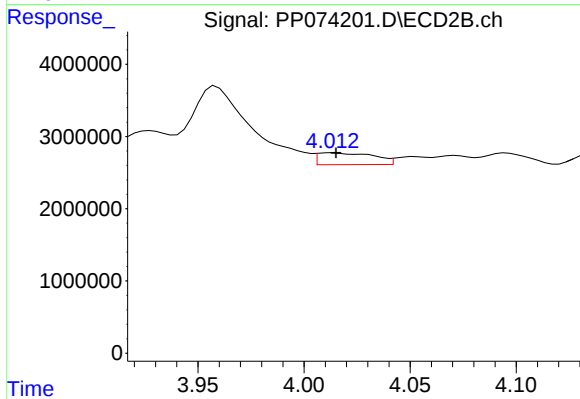

#8 AR-1221-1


R.T.: 4.013 min
Delta R.T.: -0.002 min
Response: 3015870
Conc: 61.44 ng/ml

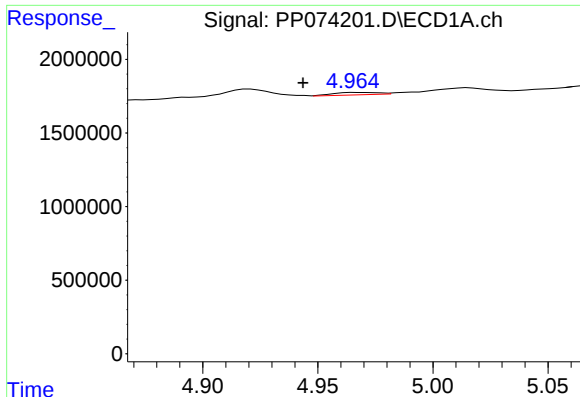

#9 AR-1221-2


R.T.: 4.966 min
Delta R.T.: 0.023 min
Response: 228856
Conc: 18.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

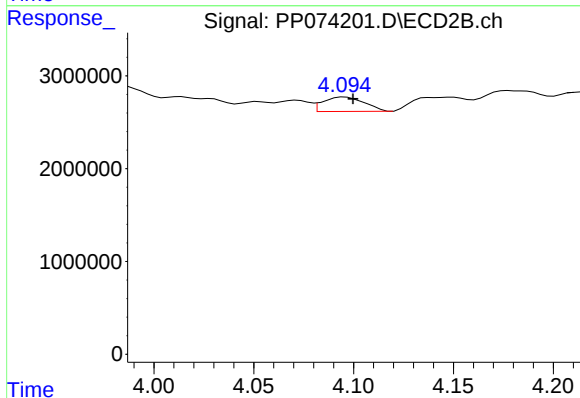


#9 AR-1221-2

R.T.: 4.095 min
Delta R.T.: -0.004 min
Response: 2236587
Conc: 62.32 ng/ml

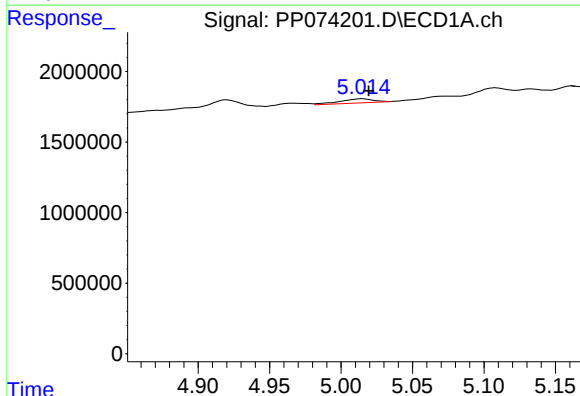


#10 AR-1221-3

R.T.: 5.015 min
Delta R.T.: -0.004 min
Response: 463155
Conc: 12.64 ng/ml

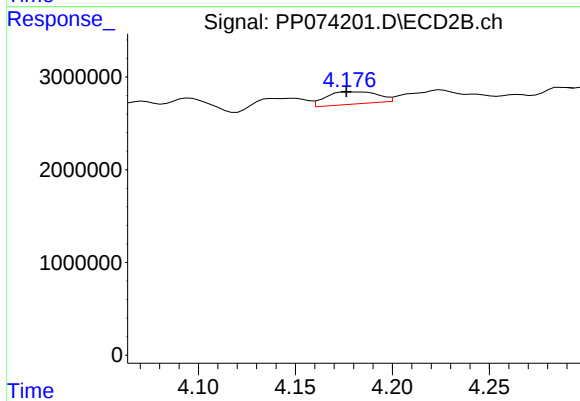

#10 AR-1221-3


R.T.: 4.178 min
Delta R.T.: 0.002 min
Response: 2437386
Conc: 18.02 ng/ml

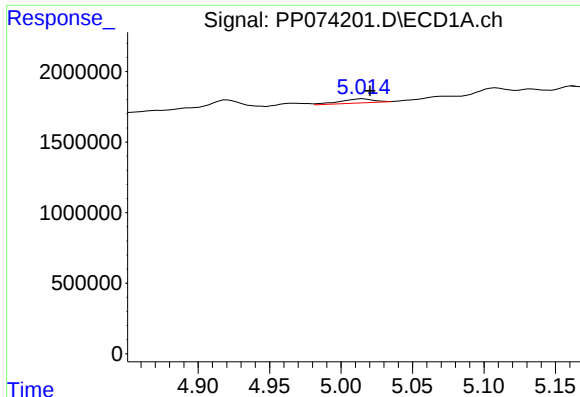

#11 AR-1232-1


R.T.: 5.015 min
Delta R.T.: -0.005 min
Response: 463155
Conc: 15.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

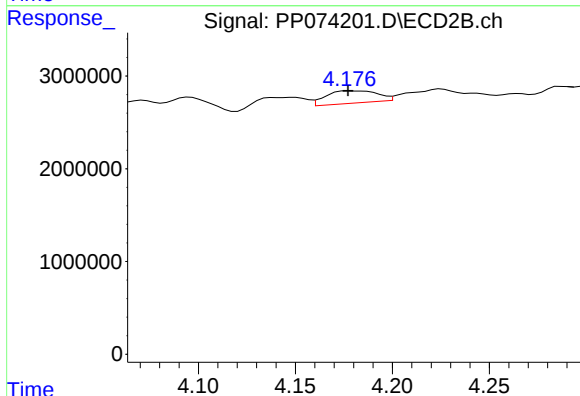


#11 AR-1232-1

R.T.: 4.178 min
Delta R.T.: 0.000 min
Response: 2437386
Conc: 24.05 ng/ml

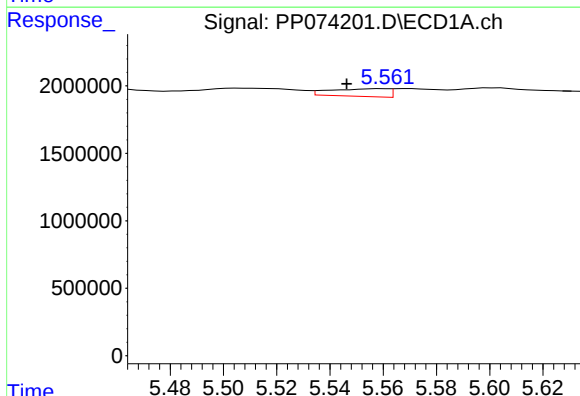


#12 AR-1232-2

R.T.: 5.559 min
Delta R.T.: 0.013 min
Response: 868399
Conc: 57.73 ng/ml

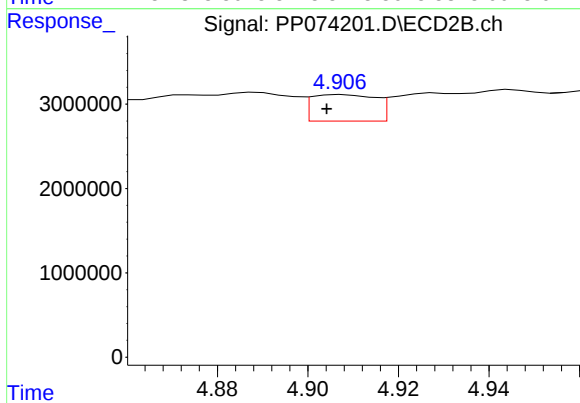

#12 AR-1232-2


R.T.: 4.908 min
Delta R.T.: 0.004 min
Response: 3086177
Conc: 17.71 ng/ml

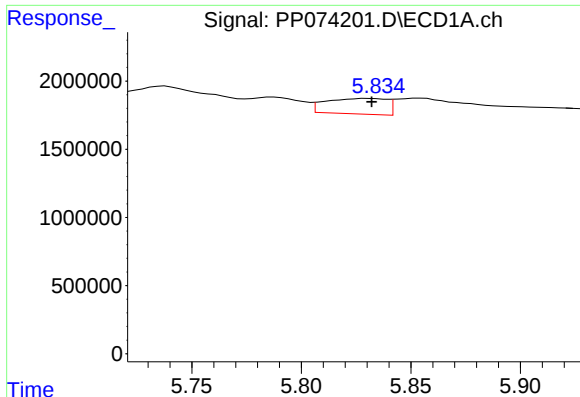

#13 AR-1232-3


R.T.: 5.831 min
Delta R.T.: -0.001 min
Response: 2208830
Conc: 76.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

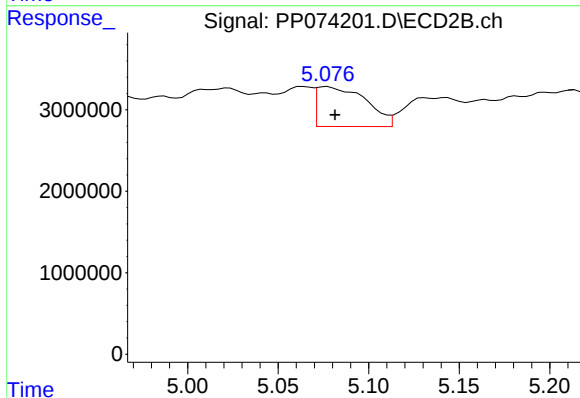


#13 AR-1232-3

R.T.: 5.077 min
Delta R.T.: -0.004 min
Response: 9252788
Conc: 201.95 ng/ml

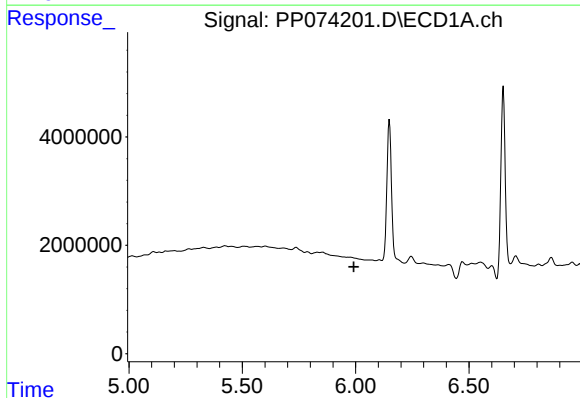


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.993 min
Response: 0
Conc: N.D.

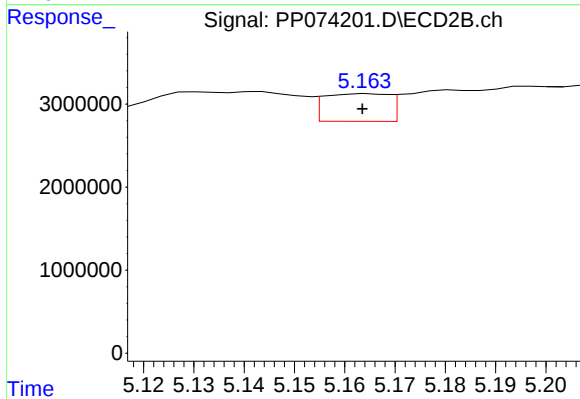

#14 AR-1232-4


R.T.: 5.165 min
Delta R.T.: 0.001 min
Response: 2977301
Conc: 51.32 ng/ml

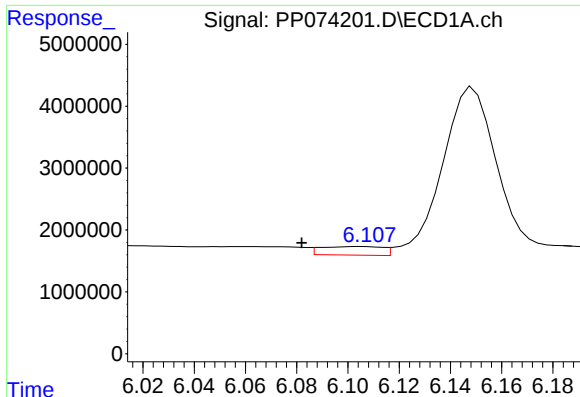

#15 AR-1232-5


R.T.: 6.106 min
Delta R.T.: 0.024 min
Response: 2329803
Conc: 198.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

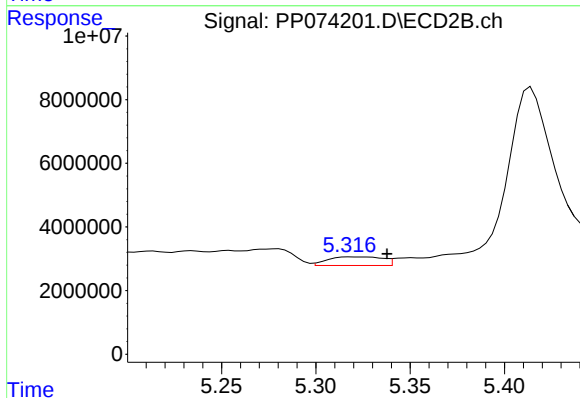


#15 AR-1232-5

R.T.: 5.318 min
Delta R.T.: -0.020 min
Response: 5512063
Conc: 117.33 ng/ml

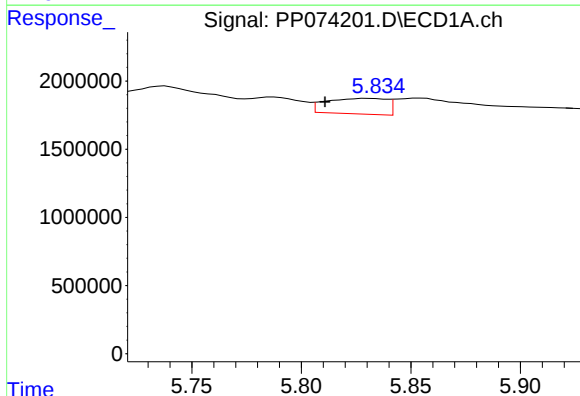


#16 AR-1242-1

R.T.: 5.831 min
Delta R.T.: 0.020 min
Response: 2208830
Conc: 59.27 ng/ml

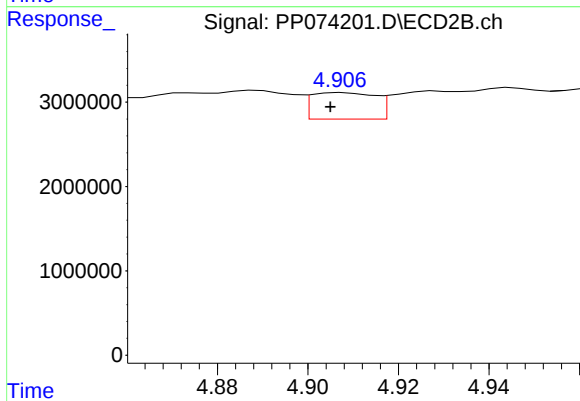

#16 AR-1242-1


R.T.: 4.908 min
Delta R.T.: 0.003 min
Response: 3086177
Conc: 8.94 ng/ml

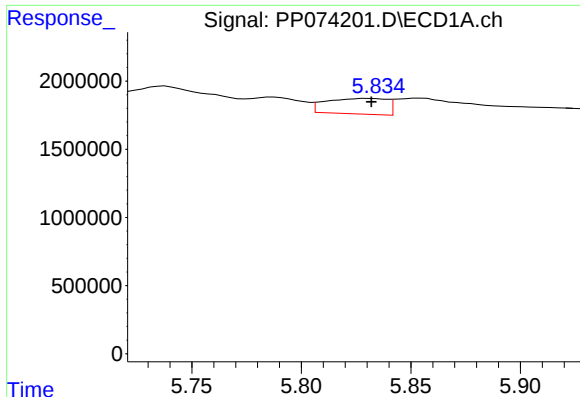

#17 AR-1242-2


R.T.: 5.831 min
Delta R.T.: -0.001 min
Response: 2208830
Conc: 40.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

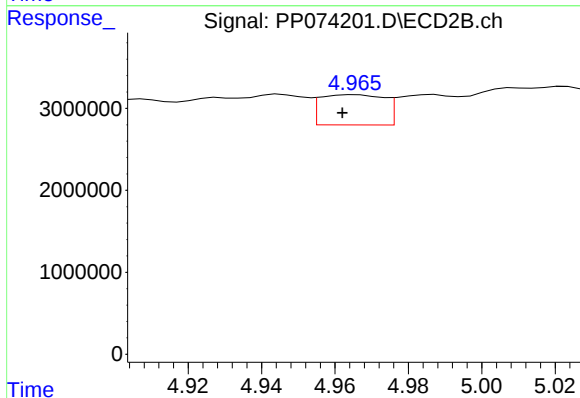


#17 AR-1242-2

R.T.: 4.966 min
Delta R.T.: 0.004 min
Response: 4476264
Conc: 27.40 ng/ml

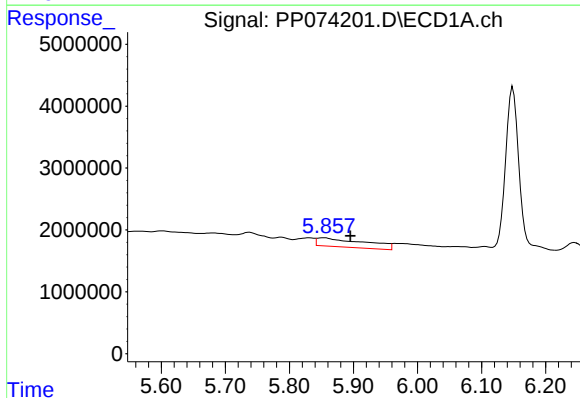


#18 AR-1242-3

R.T.: 5.854 min
Delta R.T.: -0.041 min
Response: 7507165
Conc: 210.07 ng/ml

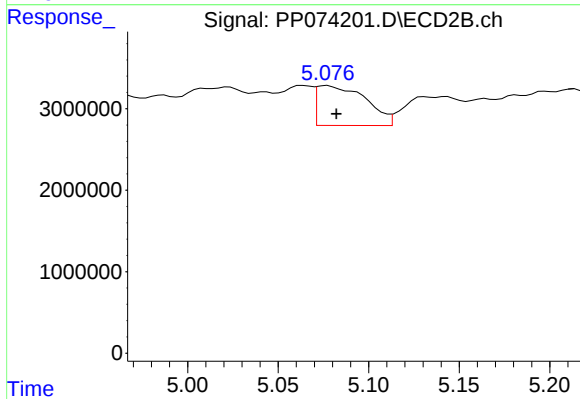

#18 AR-1242-3


R.T.: 5.077 min
Delta R.T.: -0.005 min
Response: 9252788
Conc: 100.30 ng/ml

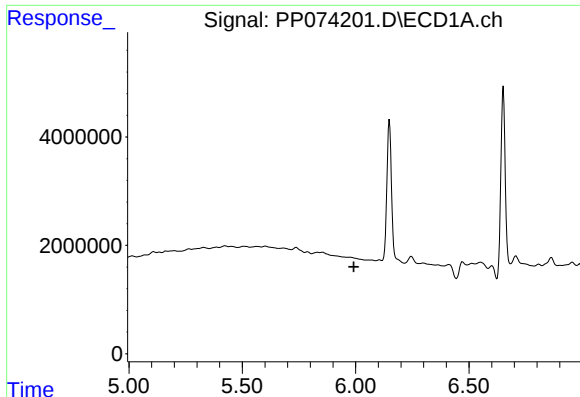

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

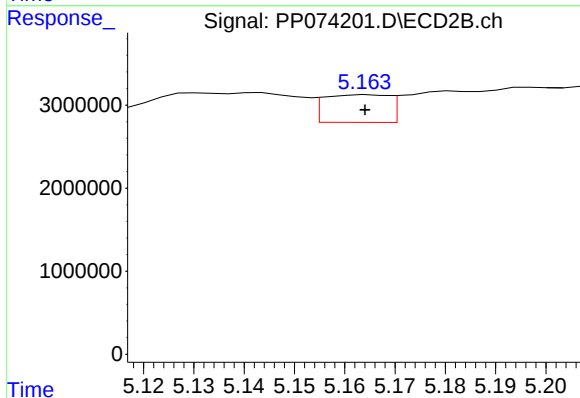


#19 AR-1242-4

R.T.: 5.165 min
Delta R.T.: 0.000 min
Response: 2977301
Conc: 24.93 ng/ml

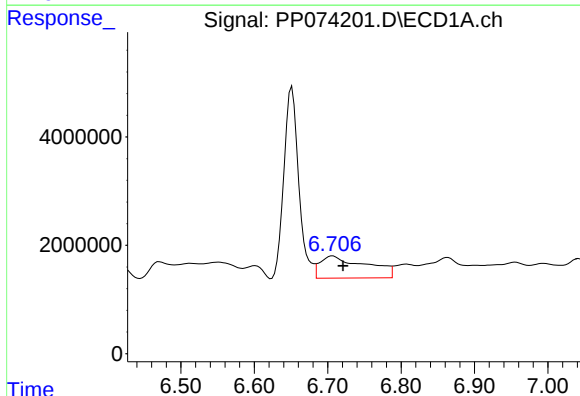


#20 AR-1242-5

R.T.: 6.707 min
Delta R.T.: -0.014 min
Response: 17788794
Conc: 500.28 ng/ml

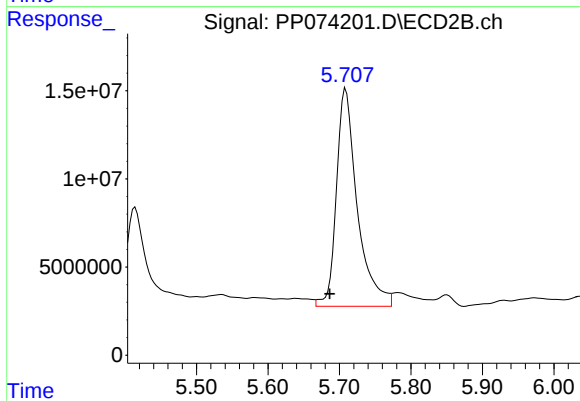

#20 AR-1242-5


R.T.: 5.709 min
Delta R.T.: 0.023 min
Response: 250514901
Conc: 1675.01 ng/ml

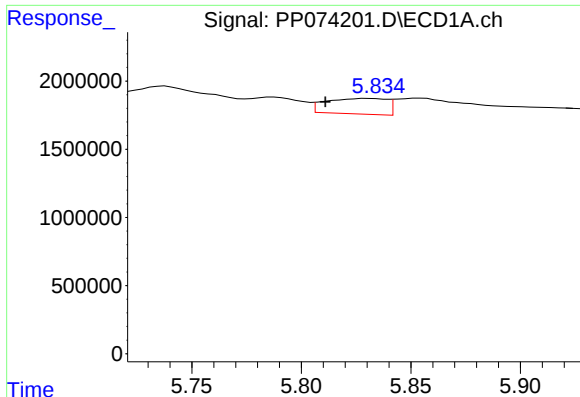

#21 AR-1248-1


R.T.: 5.831 min
Delta R.T.: 0.020 min
Response: 2208830
Conc: 78.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

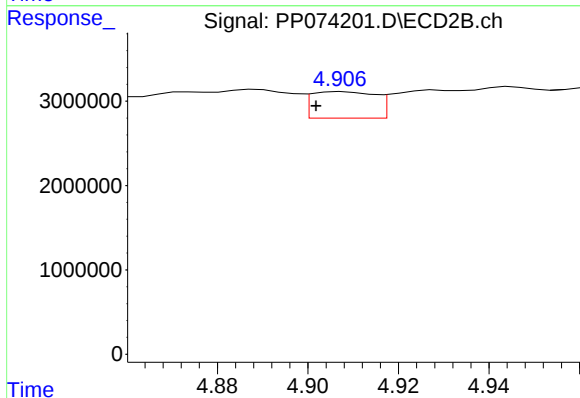


#21 AR-1248-1

R.T.: 4.908 min
Delta R.T.: 0.006 min
Response: 3086177
Conc: 14.43 ng/ml

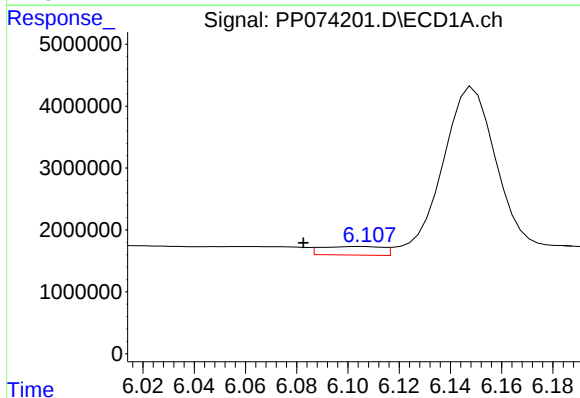


#22 AR-1248-2

R.T.: 6.106 min
Delta R.T.: 0.023 min
Response: 2329803
Conc: 57.87 ng/ml

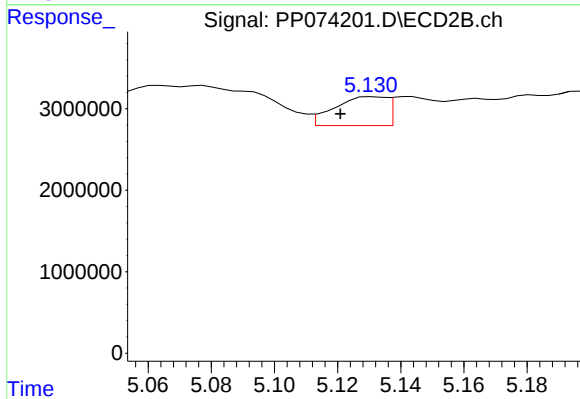

#22 AR-1248-2


R.T.: 5.131 min
Delta R.T.: 0.010 min
Response: 4049980
Conc: 27.68 ng/ml

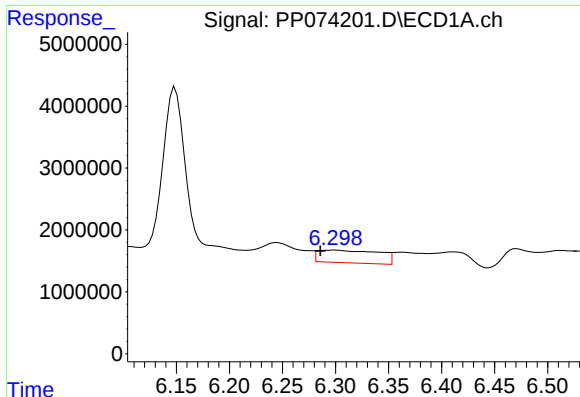

#23 AR-1248-3


R.T.: 6.299 min
Delta R.T.: 0.013 min
Response: 8162337
Conc: 183.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

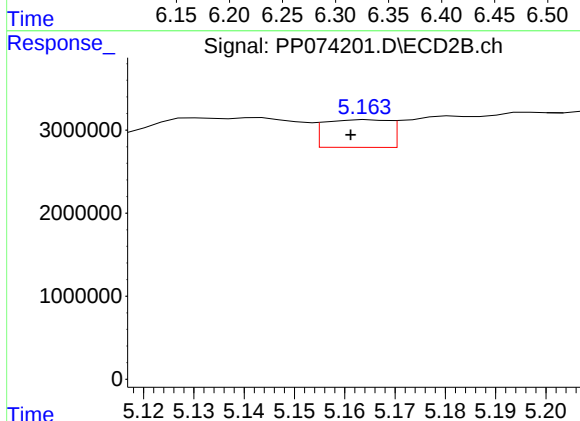


#23 AR-1248-3

R.T.: 5.165 min
Delta R.T.: 0.004 min
Response: 2977301
Conc: 17.36 ng/ml

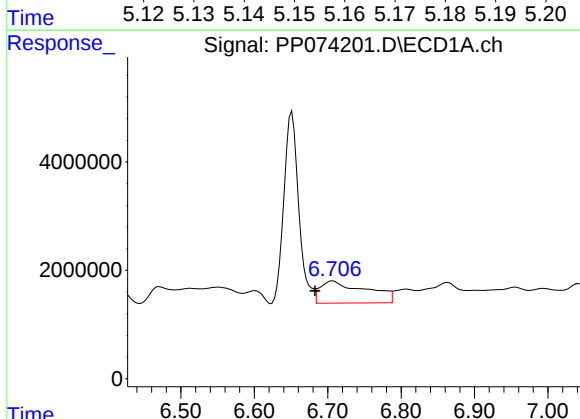


#24 AR-1248-4

R.T.: 6.707 min
Delta R.T.: 0.024 min
Response: 17788794
Conc: 341.85 ng/ml

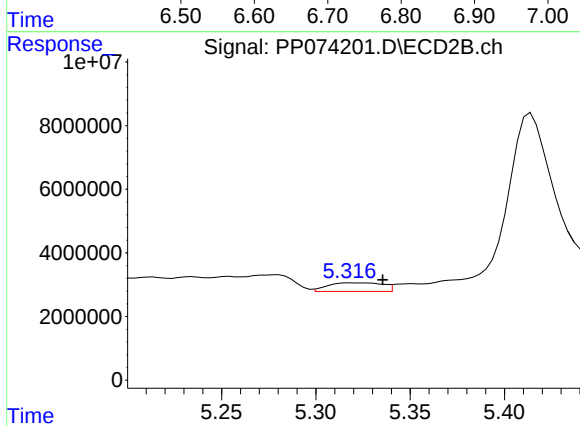

#24 AR-1248-4


R.T.: 5.318 min
Delta R.T.: -0.018 min
Response: 5512063
Conc: 33.13 ng/ml

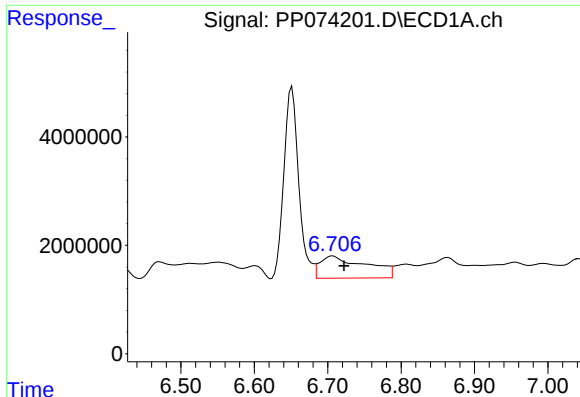

#25 AR-1248-5


R.T.: 6.707 min
Delta R.T.: -0.016 min
Response: 17788794
Conc: 312.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

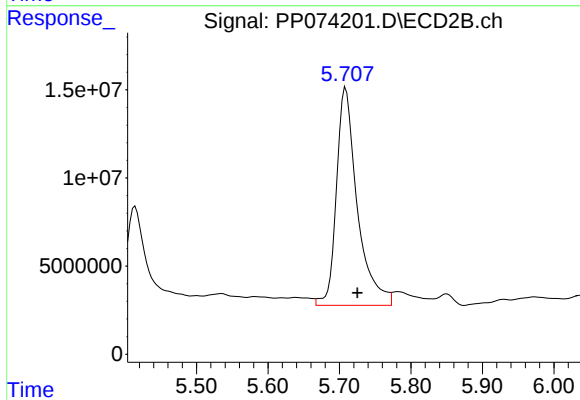


#25 AR-1248-5

R.T.: 5.709 min
Delta R.T.: -0.016 min
Response: 250514901
Conc: 860.98 ng/ml

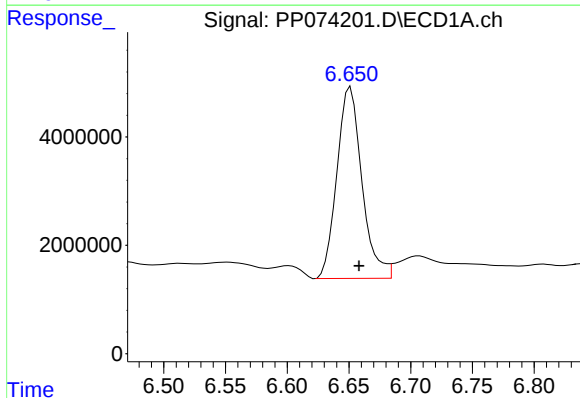


#26 AR-1254-1

R.T.: 6.651 min
Delta R.T.: -0.007 min
Response: 49861768
Conc: 947.20 ng/ml

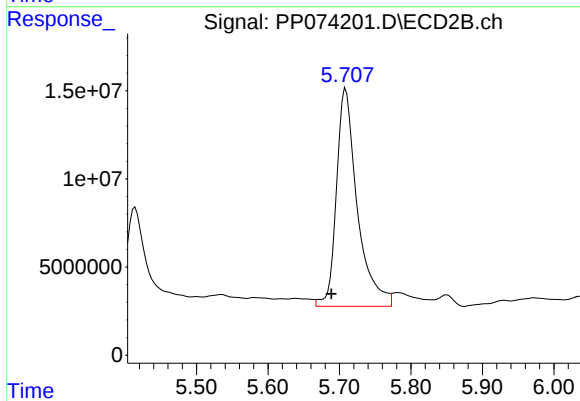

#26 AR-1254-1


R.T.: 5.709 min
Delta R.T.: 0.020 min
Response: 250514901
Conc: 684.13 ng/ml

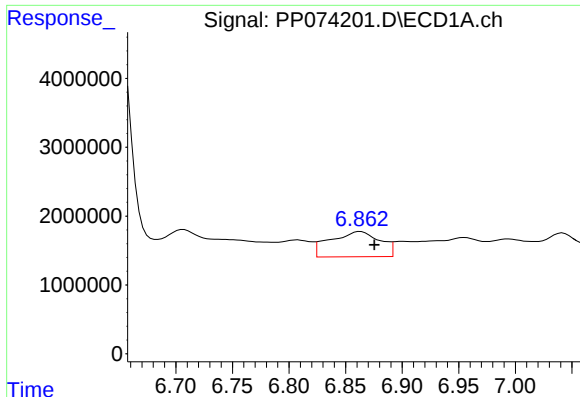

#27 AR-1254-2


R.T.: 6.863 min
Delta R.T.: -0.012 min
Response: 11259682
Conc: 141.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

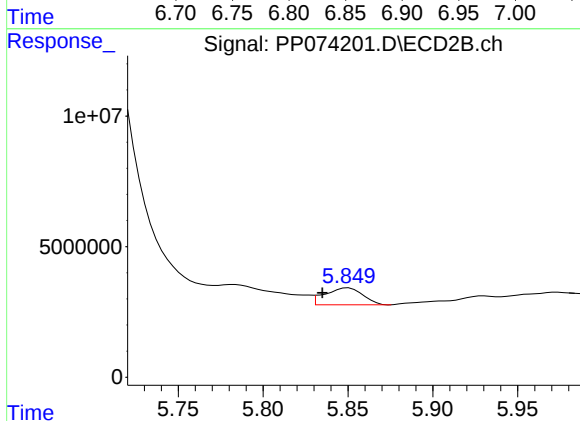


#27 AR-1254-2

R.T.: 5.850 min
Delta R.T.: 0.015 min
Response: 10112293
Conc: 36.35 ng/ml

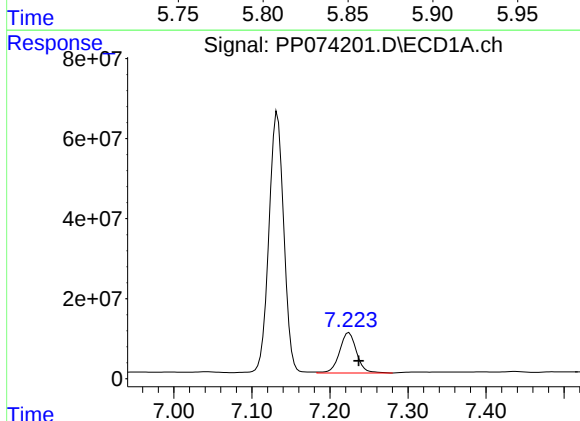


#28 AR-1254-3

R.T.: 7.224 min
Delta R.T.: -0.013 min
Response: 152798548
Conc: 1749.94 ng/ml

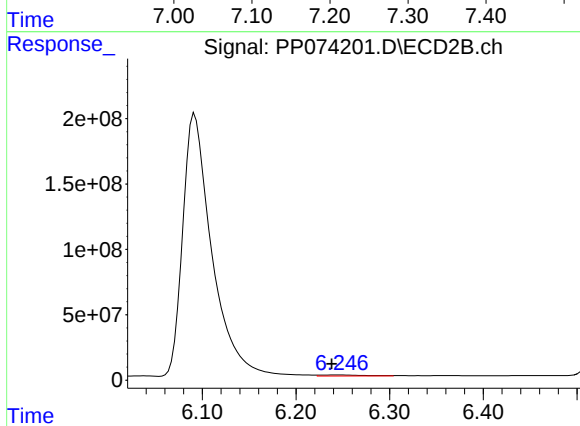

#28 AR-1254-3


R.T.: 6.247 min
Delta R.T.: 0.009 min
Response: 26486054
Conc: 54.14 ng/ml

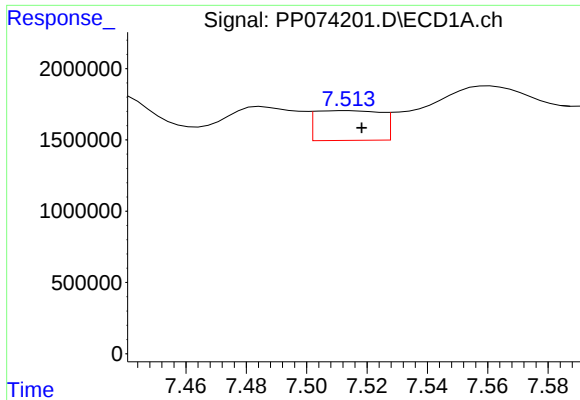

#29 AR-1254-4


R.T.: 7.514 min
Delta R.T.: -0.005 min
Response: 3160179
Conc: 49.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

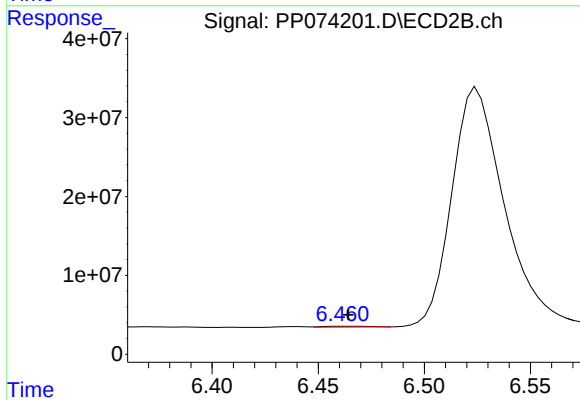


#29 AR-1254-4

R.T.: 6.463 min
Delta R.T.: -0.002 min
Response: 1559977
Conc: 4.24 ng/ml

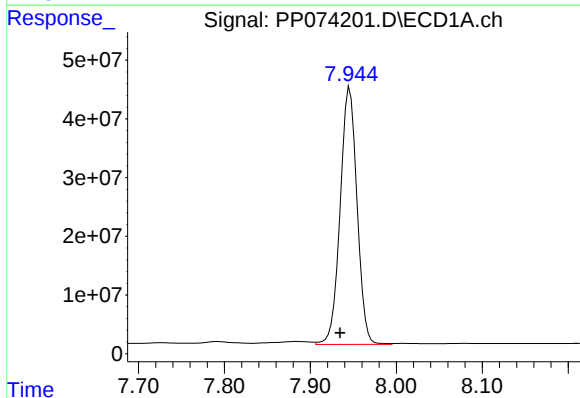


#30 AR-1254-5

R.T.: 7.946 min
Delta R.T.: 0.011 min
Response: 598095196
Conc: 7370.72 ng/ml

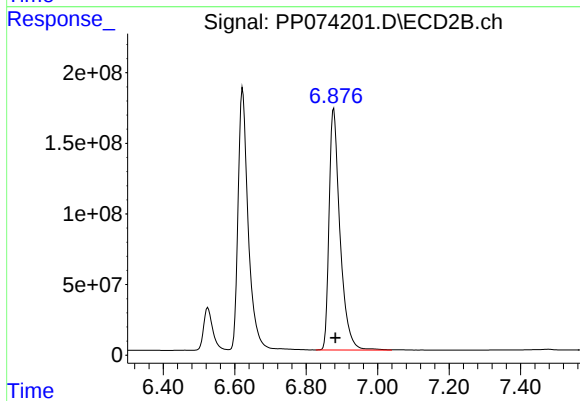

#30 AR-1254-5


R.T.: 6.877 min
Delta R.T.: -0.004 min
Response: 3623711238
Conc: 9218.42 ng/ml

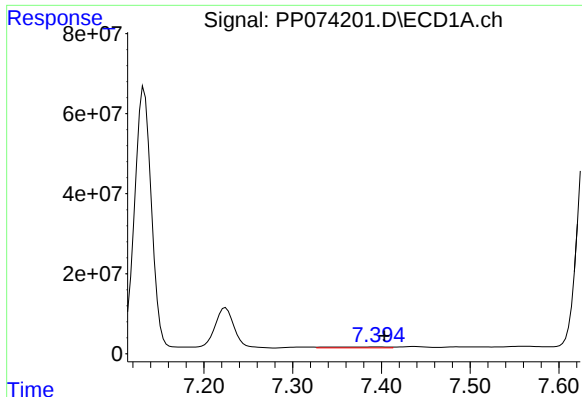

#31 AR-1260-1


R.T.: 7.395 min
Delta R.T.: -0.008 min
Response: 10721881
Conc: 190.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

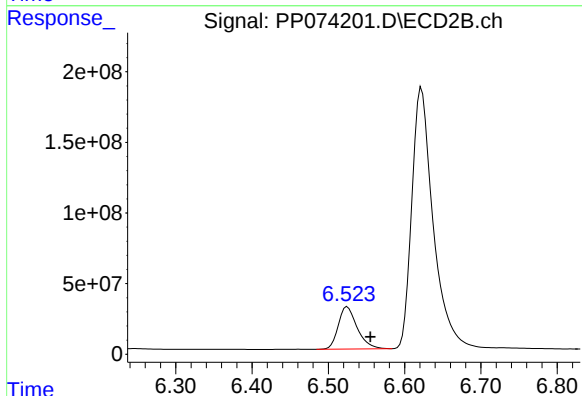


#31 AR-1260-1

R.T.: 6.525 min
Delta R.T.: -0.030 min
Response: 516492718
Conc: 1278.58 ng/ml

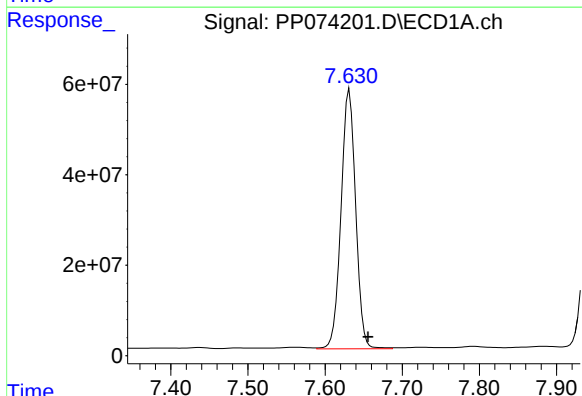


#32 AR-1260-2

R.T.: 7.632 min
Delta R.T.: -0.024 min
Response: 754742142
Conc: 11074.34 ng/ml

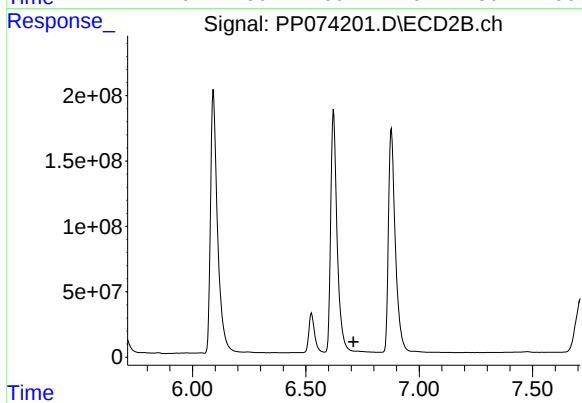

#32 AR-1260-2


R.T.: 6.729 min
Delta R.T.: 0.019 min
Response: -4980182
Conc: N.D.

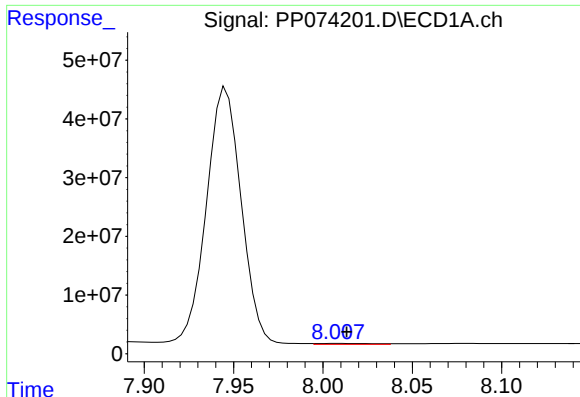

#33 AR-1260-3


R.T.: 8.008 min
Delta R.T.: -0.005 min
Response: 3485848
Conc: 65.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

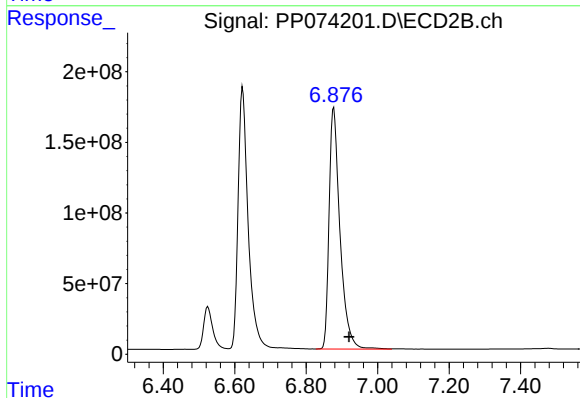


#33 AR-1260-3

R.T.: 6.877 min
Delta R.T.: -0.043 min
Response: 3623711238
Conc: 9194.48 ng/ml

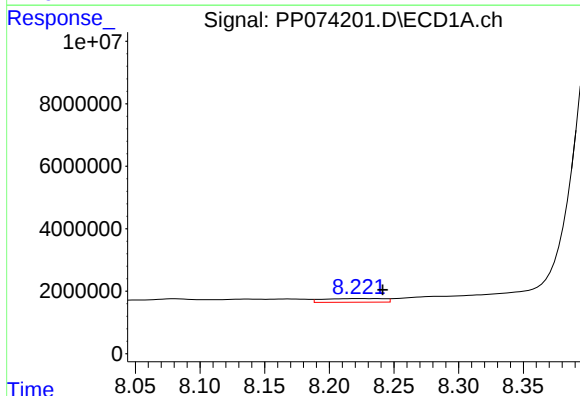


#34 AR-1260-4

R.T.: 8.224 min
Delta R.T.: -0.018 min
Response: 3901854
Conc: 62.32 ng/ml

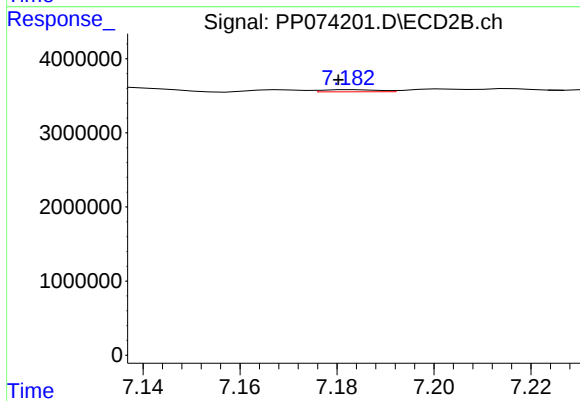

#34 AR-1260-4


R.T.: 7.183 min
Delta R.T.: 0.003 min
Response: 230876
Conc: 0.79 ng/ml

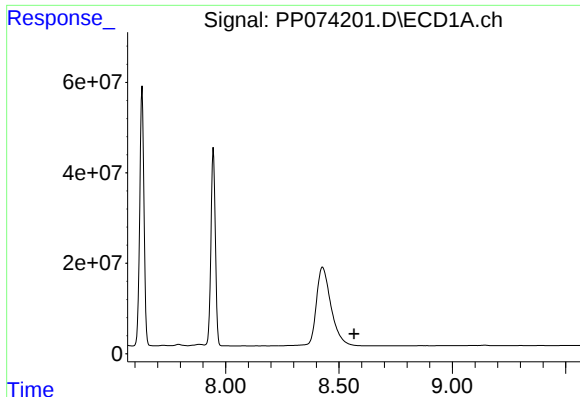

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.567 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

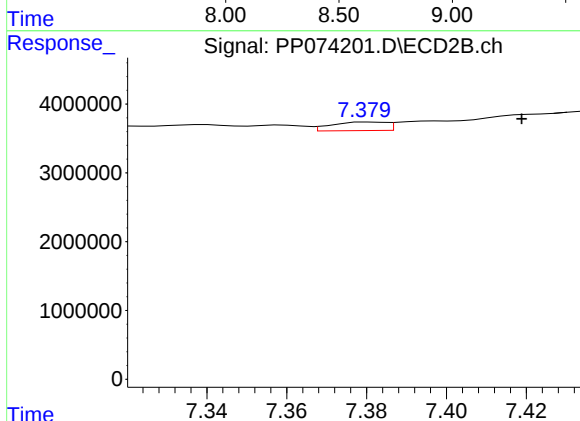


#35 AR-1260-5

R.T.: 7.381 min
Delta R.T.: -0.038 min
Response: 1172412
Conc: 1.55 ng/ml

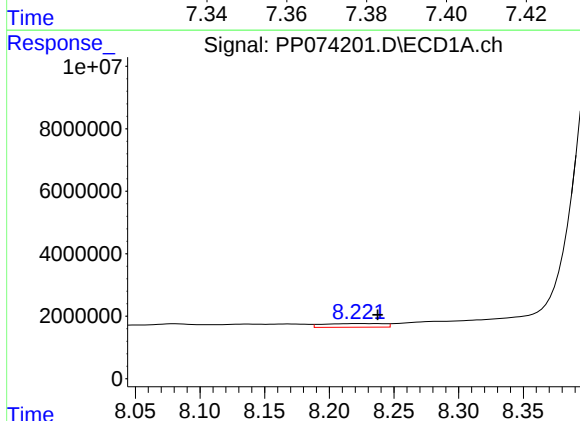


#36 AR-1262-1

R.T.: 8.224 min
Delta R.T.: -0.014 min
Response: 3901854
Conc: 51.48 ng/ml

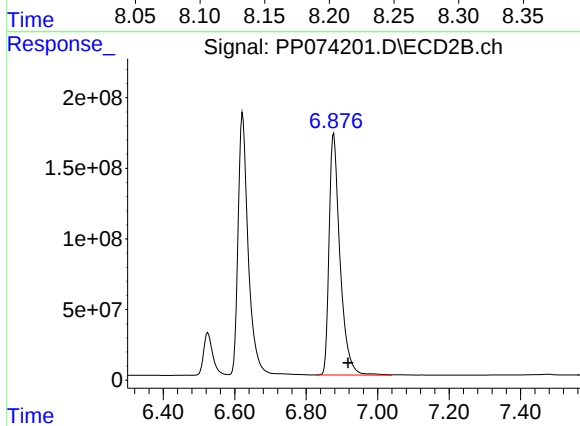

#36 AR-1262-1


R.T.: 6.877 min
Delta R.T.: -0.040 min
Response: 3623711238
Conc: 6434.80 ng/ml

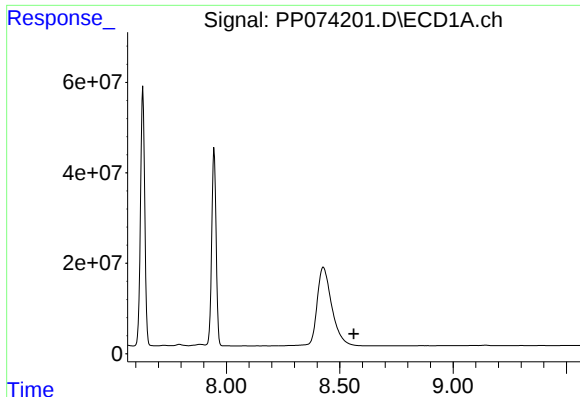

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.562 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

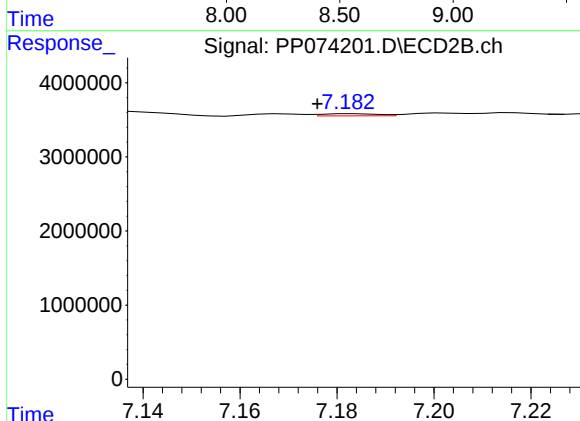


#37 AR-1262-2

R.T.: 7.183 min
Delta R.T.: 0.007 min
Response: 230876
Conc: 0.58 ng/ml

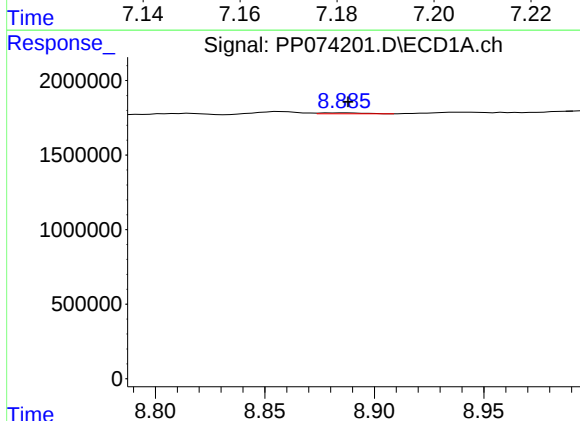


#38 AR-1262-3

R.T.: 8.887 min
Delta R.T.: -0.001 min
Response: 83728
Conc: 0.89 ng/ml

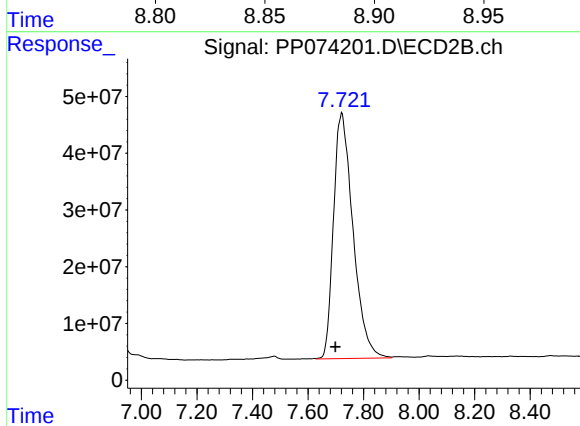

#38 AR-1262-3


R.T.: 7.722 min
Delta R.T.: 0.024 min
Response: 2108870155
Conc: 5866.61 ng/ml

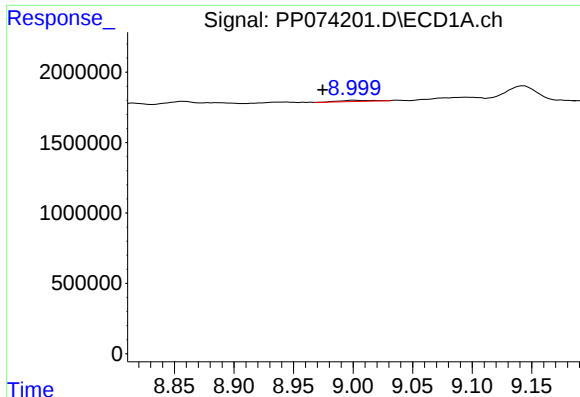

#39 AR-1262-4


R.T.: 9.002 min
Delta R.T.: 0.027 min
Response: 138174
Conc: 1.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

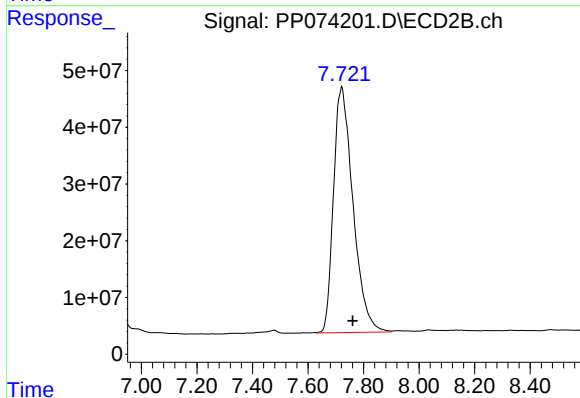


#39 AR-1262-4

R.T.: 7.722 min
Delta R.T.: -0.039 min
Response: 2108870155
Conc: 3162.10 ng/ml

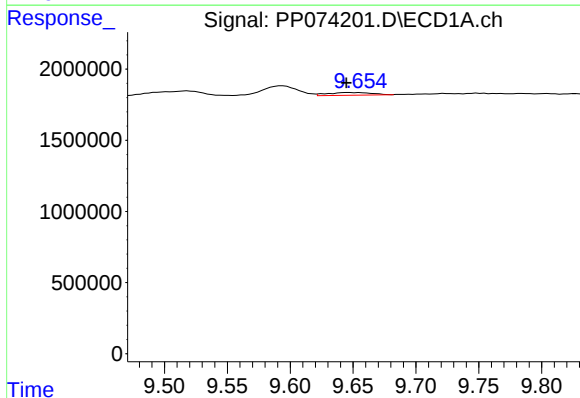


#40 AR-1262-5

R.T.: 9.654 min
Delta R.T.: 0.009 min
Response: 457241
Conc: 8.98 ng/ml

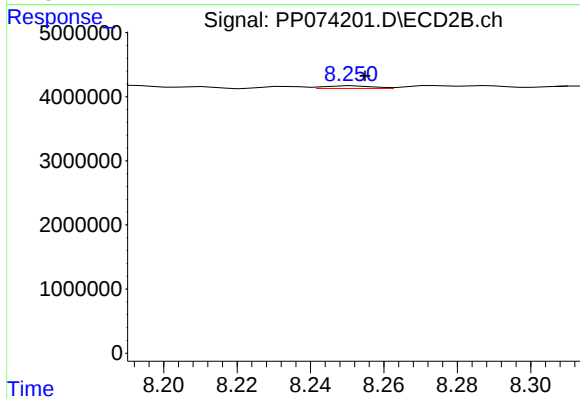

#40 AR-1262-5


R.T.: 8.252 min
Delta R.T.: -0.003 min
Response: 372041
Conc: 1.31 ng/ml

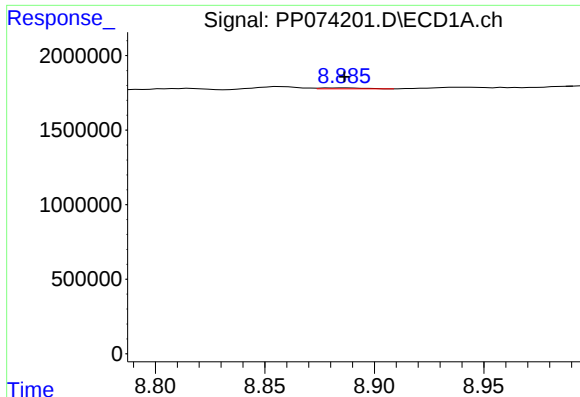

#41 AR-1268-1


R.T.: 8.887 min
Delta R.T.: 0.000 min
Response: 83728
Conc: 0.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

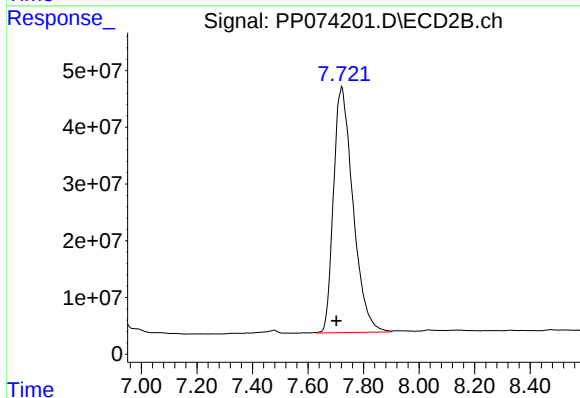


#41 AR-1268-1

R.T.: 7.722 min
Delta R.T.: 0.020 min
Response: 2108870155
Conc: 1934.27 ng/ml

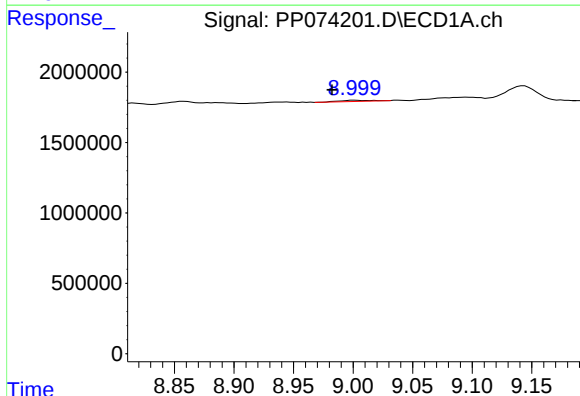


#42 AR-1268-2

R.T.: 9.002 min
Delta R.T.: 0.019 min
Response: 138174
Conc: 0.96 ng/ml

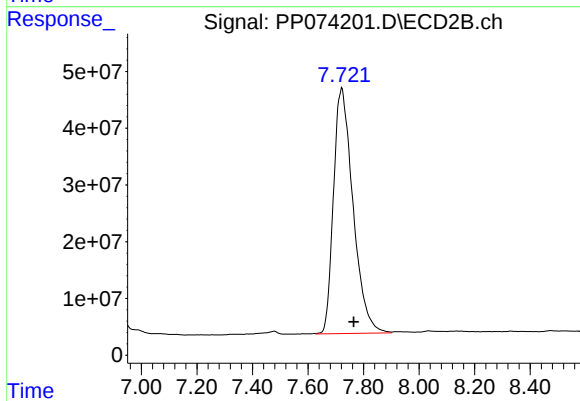

#42 AR-1268-2


R.T.: 7.722 min
Delta R.T.: -0.043 min
Response: 2108870155
Conc: 1987.01 ng/ml

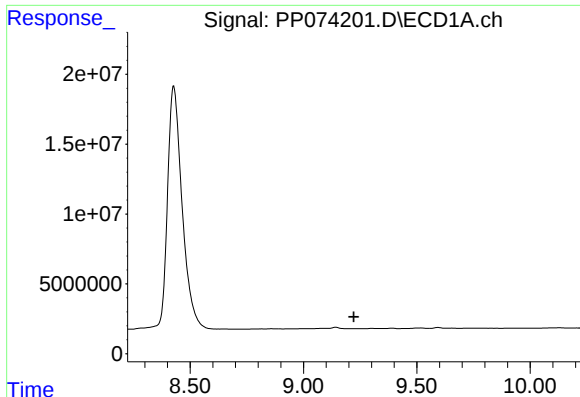

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.222 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

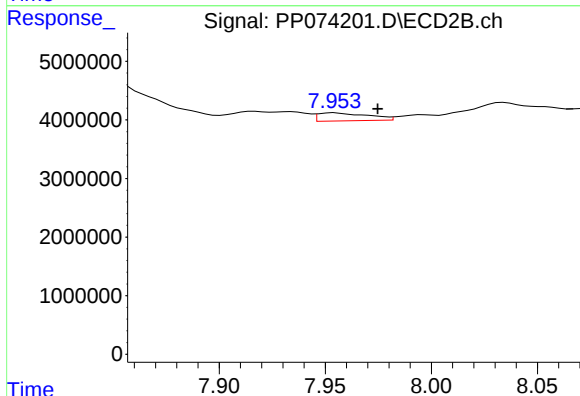


#43 AR-1268-3

R.T.: 7.954 min
Delta R.T.: -0.020 min
Response: 2259280
Conc: 2.72 ng/ml

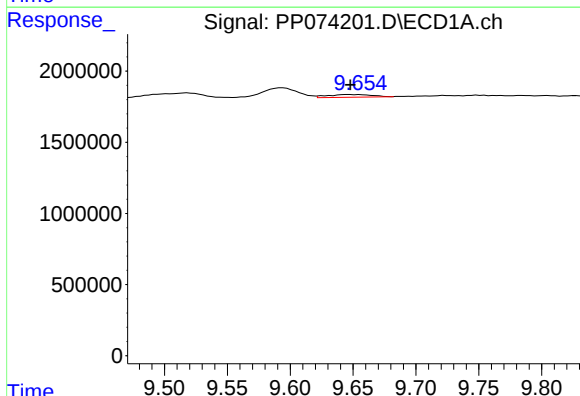


#44 AR-1268-4

R.T.: 9.654 min
Delta R.T.: 0.006 min
Response: 457241
Conc: 7.77 ng/ml

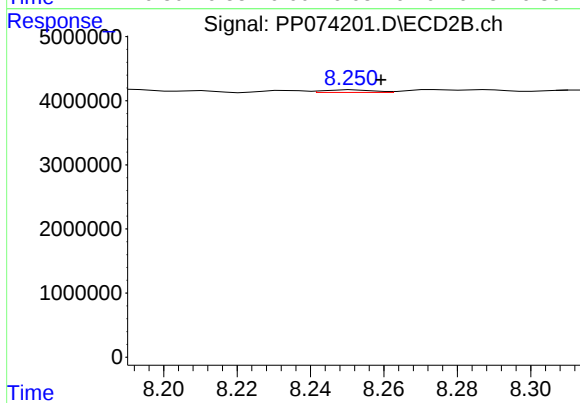

#44 AR-1268-4


R.T.: 8.252 min
Delta R.T.: -0.007 min
Response: 372041
Conc: 1.21 ng/ml

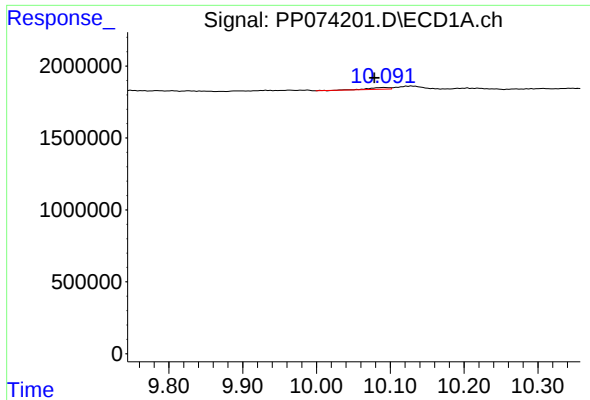

#45 AR-1268-5

R.T.: 10.093 min
Delta R.T.: 0.014 min
Response: 227469
Conc: 0.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

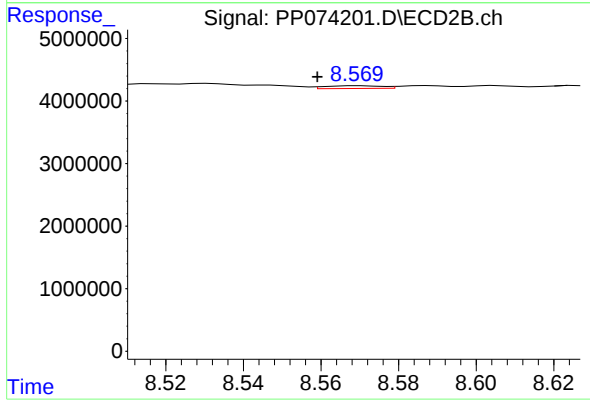

#45 AR-1268-5

R.T.: 8.570 min
Delta R.T.: 0.011 min
Response: 445426
Conc: 0.17 ng/ml