

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080222\
 Data File : PP050099.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2022 18:32
 Operator : YP\AJ
 Sample : N3993-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PLA-155

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/03/2022
 Supervised By :Ankita Jodhani 08/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 23:52:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 14 06:08:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.354	3.607	38487414	45419482	26.522m	18.582m#
2) SA Decachlor...	10.106	8.567	21884543	18697370	15.473m	16.055m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080222\
Data File : PP050099.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2022 18:32
Operator : YP\AJ
Sample : N3993-02
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PLA-155


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/03/2022
Supervised By :Ankita Jodhani 08/03/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 23:52:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 14 06:08:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

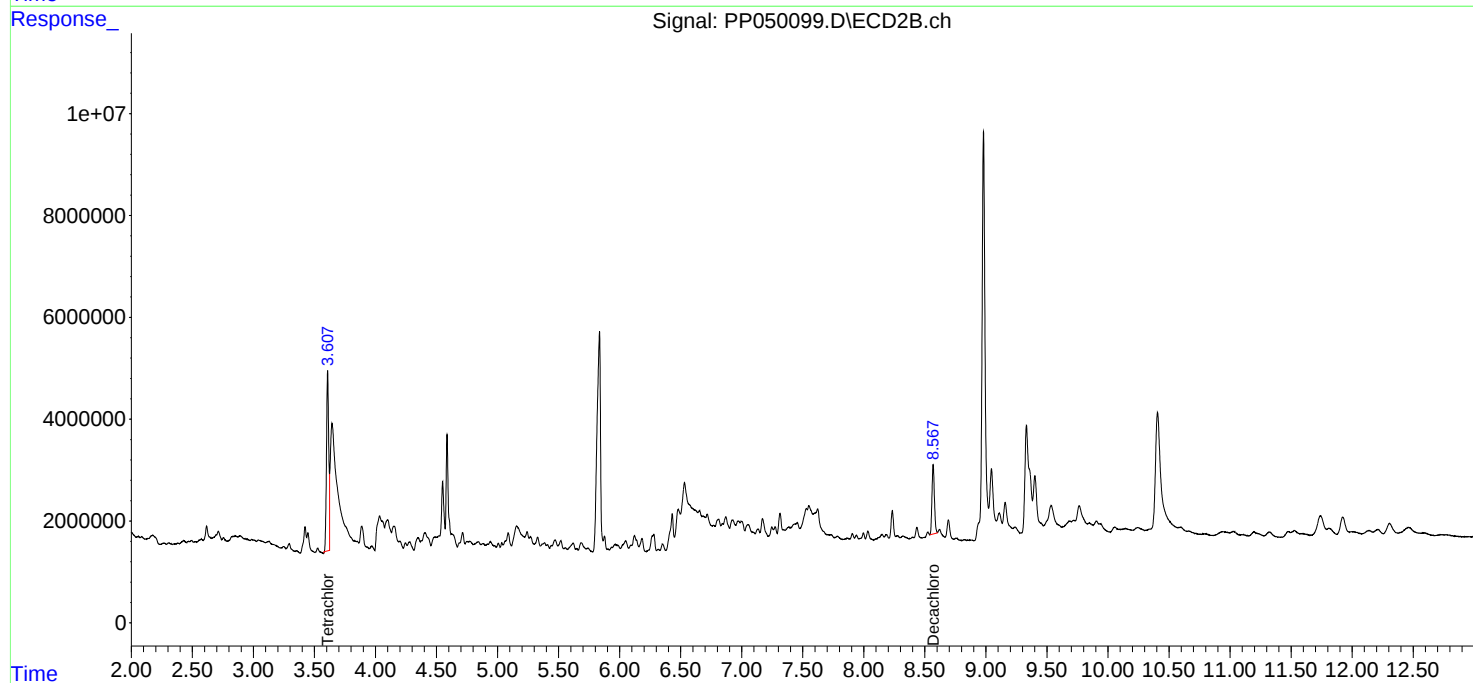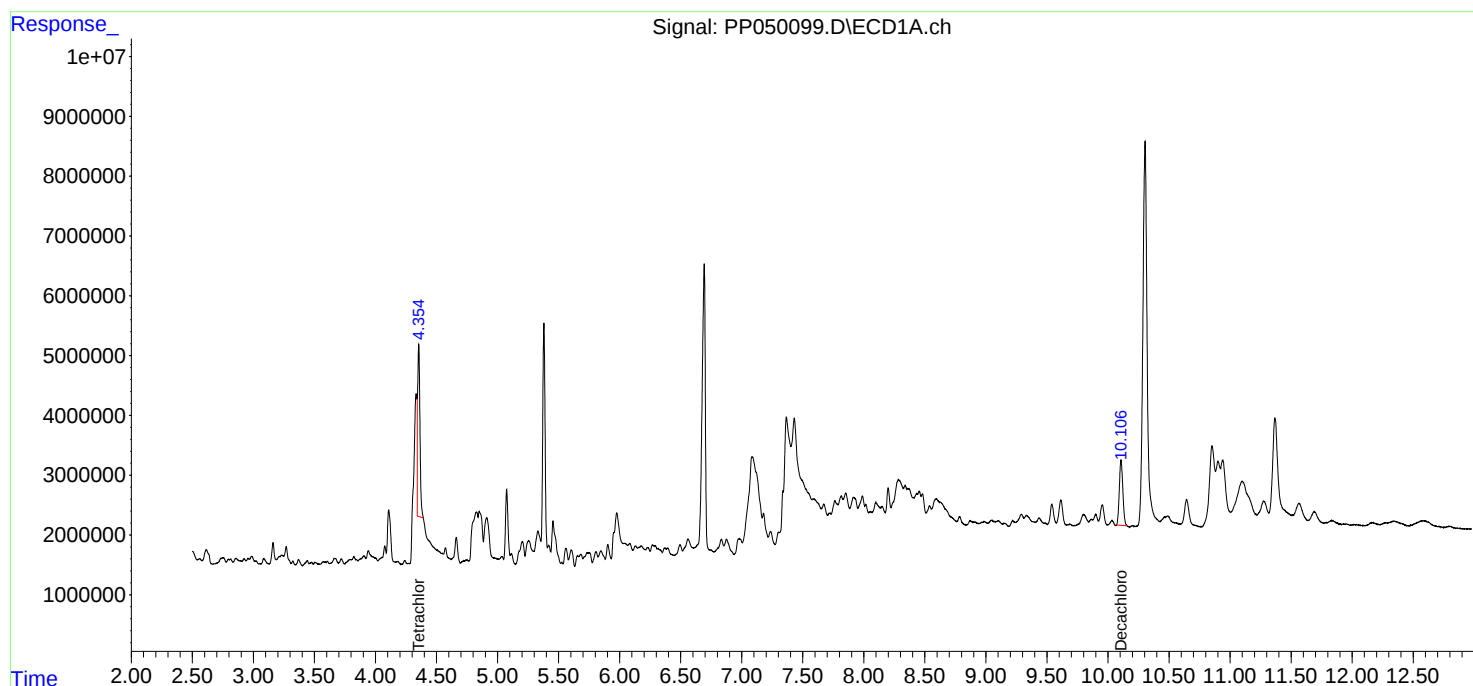

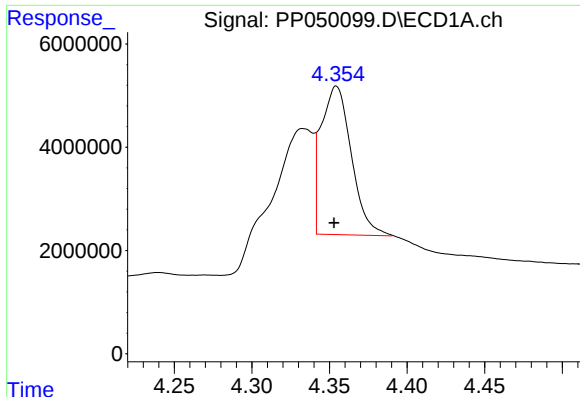


#1 Tetrachloro-m-xylene

R.T.: 4.354 min
Delta R.T.: 0.000 min
Response: 38487414
Conc: 26.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
PLA-155


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/03/2022
Supervised By :Ankita Jodhani 08/03/2022

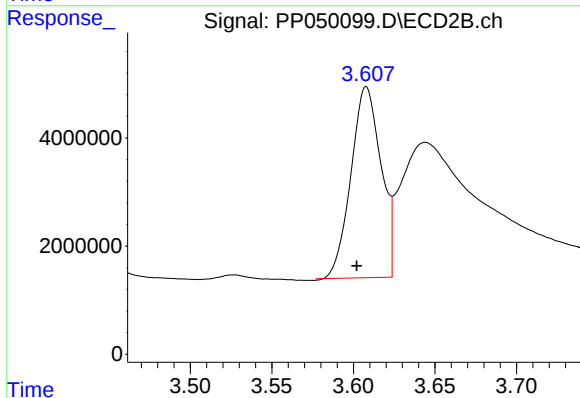


#1 Tetrachloro-m-xylene

R.T.: 3.607 min
Delta R.T.: 0.006 min
Response: 45419482
Conc: 18.58 ng/ml m

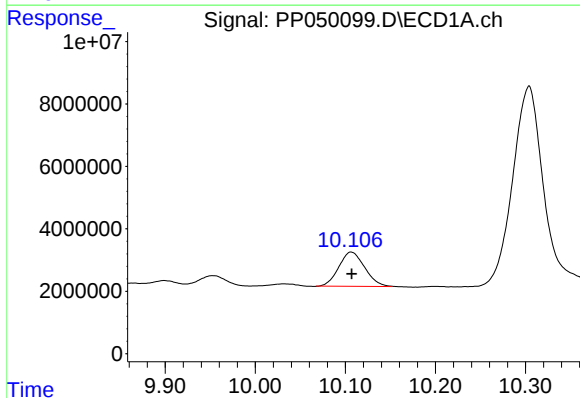

#2 Decachlorobiphenyl

R.T.: 10.106 min
Delta R.T.: -0.001 min
Response: 21884543
Conc: 15.47 ng/ml m

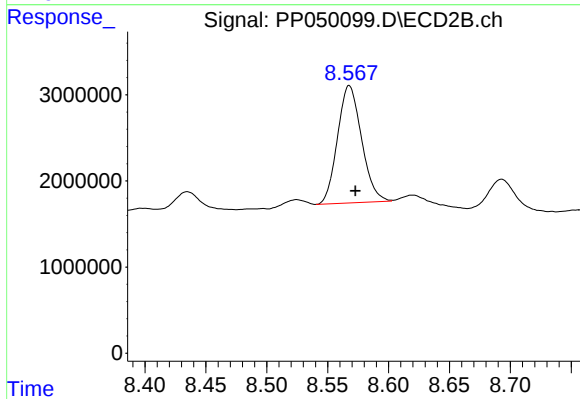

#2 Decachlorobiphenyl

R.T.: 8.567 min
Delta R.T.: -0.006 min
Response: 18697370
Conc: 16.05 ng/ml m