

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080321\
 Data File : PP037962.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Aug 2021 21:12
 Operator : AJ\MA
 Sample : M3259-25
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TOTE-COMP

Manual Integrations
 APPROVED

mohammad
 8/4/2021 11:55:18 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 03:09:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 03 05:09:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.895	3.881	866928	447080	19.456m	17.809m
2) SA Decachlor...	10.888	9.153	269672	299512	10.294	12.790

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080321\
Data File : PP037962.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Aug 2021 21:12
Operator : AJ\MA
Sample : M3259-25
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TOTE-COMP


Manual Integrations
APPROVED

mohammad
8/4/2021 11:55:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 03:09:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080221.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 03 05:09:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

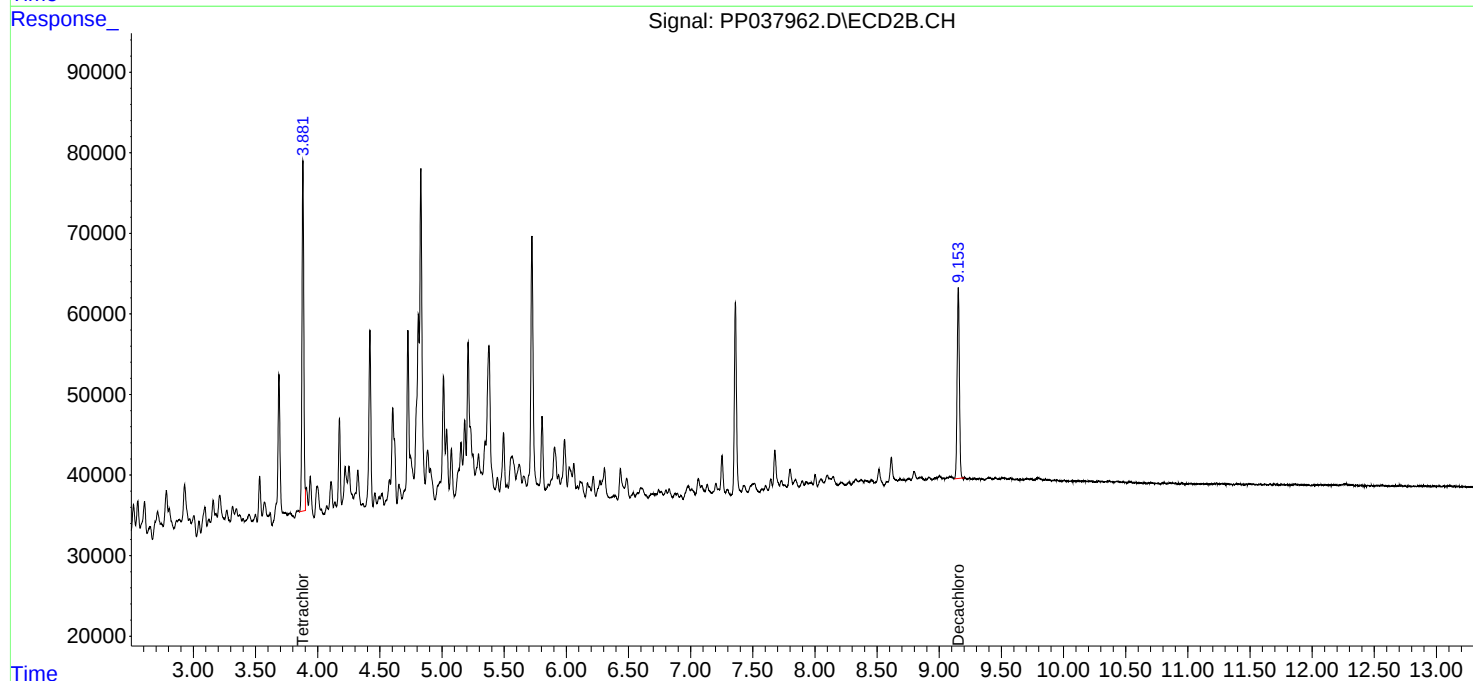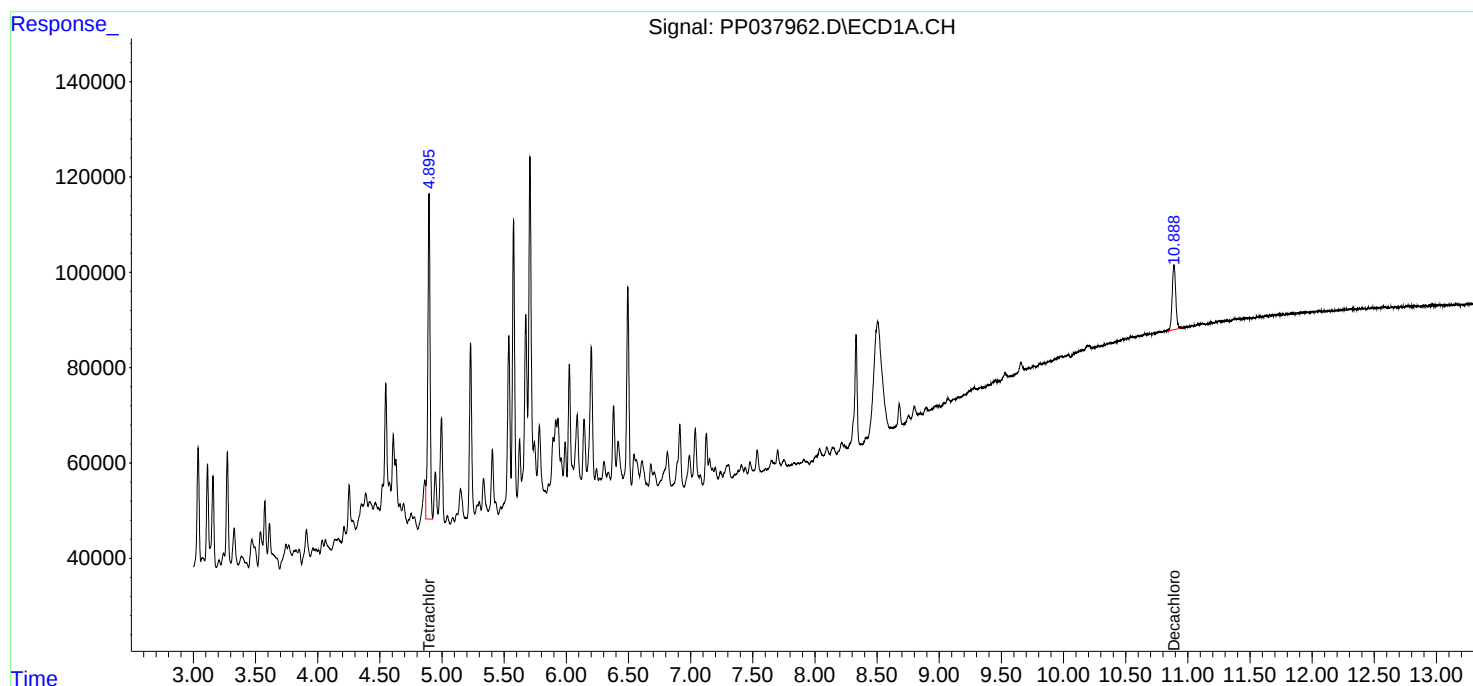

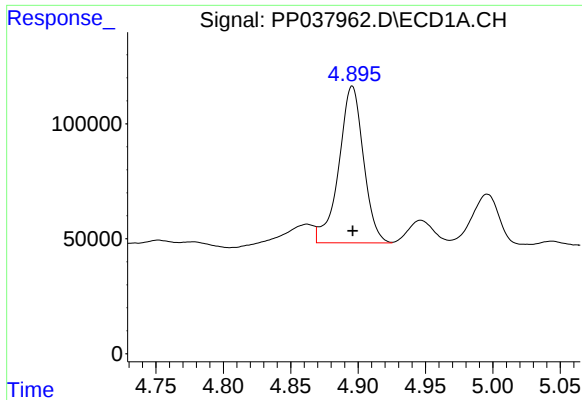


#1 Tetrachloro-m-xylene

R.T.: 4.895 min
Delta R.T.: 0.000 min
Response: 866928
Conc: 19.46 ng/ml m

Instrument :
ECD_P
ClientSampleId :
TOTE-COMP


Manual Integrations
APPROVED

mohammad
8/4/2021 11:55:18 AM

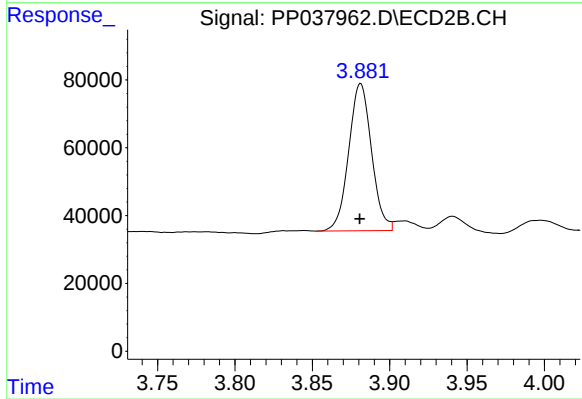


#1 Tetrachloro-m-xylene

R.T.: 3.881 min
Delta R.T.: 0.000 min
Response: 447080
Conc: 17.81 ng/ml m

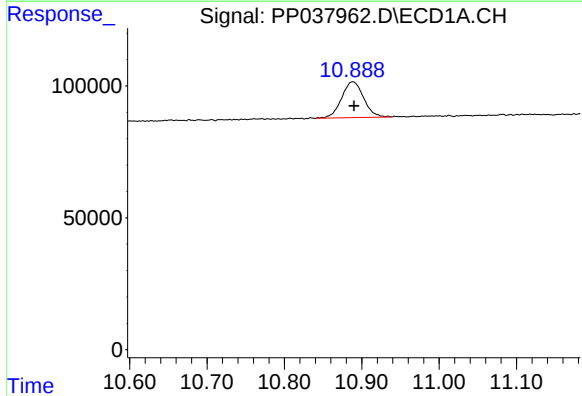

#2 Decachlorobiphenyl

R.T.: 10.888 min
Delta R.T.: -0.002 min
Response: 269672
Conc: 10.29 ng/ml

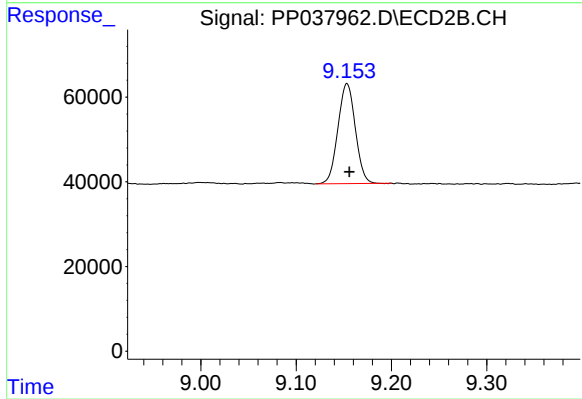

#2 Decachlorobiphenyl

R.T.: 9.153 min
Delta R.T.: -0.003 min
Response: 299512
Conc: 12.79 ng/ml