

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080321\
 Data File : PP037979.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Aug 2021 2:49
 Operator : AJ\MA
 Sample : M3260-03
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 33389

Manual Integrations
 APPROVED

mohammad
 8/4/2021 11:55:45 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 03:21:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 03 05:09:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.894	3.880	767201	456826	17.218m	18.197
2) SA Decachlor...	10.889	9.153	439300	418022	16.768	17.851

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080321\
Data File : PP037979.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Aug 2021 2:49
Operator : AJ\MA
Sample : M3260-03
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
33389


Manual Integrations
APPROVED

mohammad
8/4/2021 11:55:45 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 03:21:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080221.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 03 05:09:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

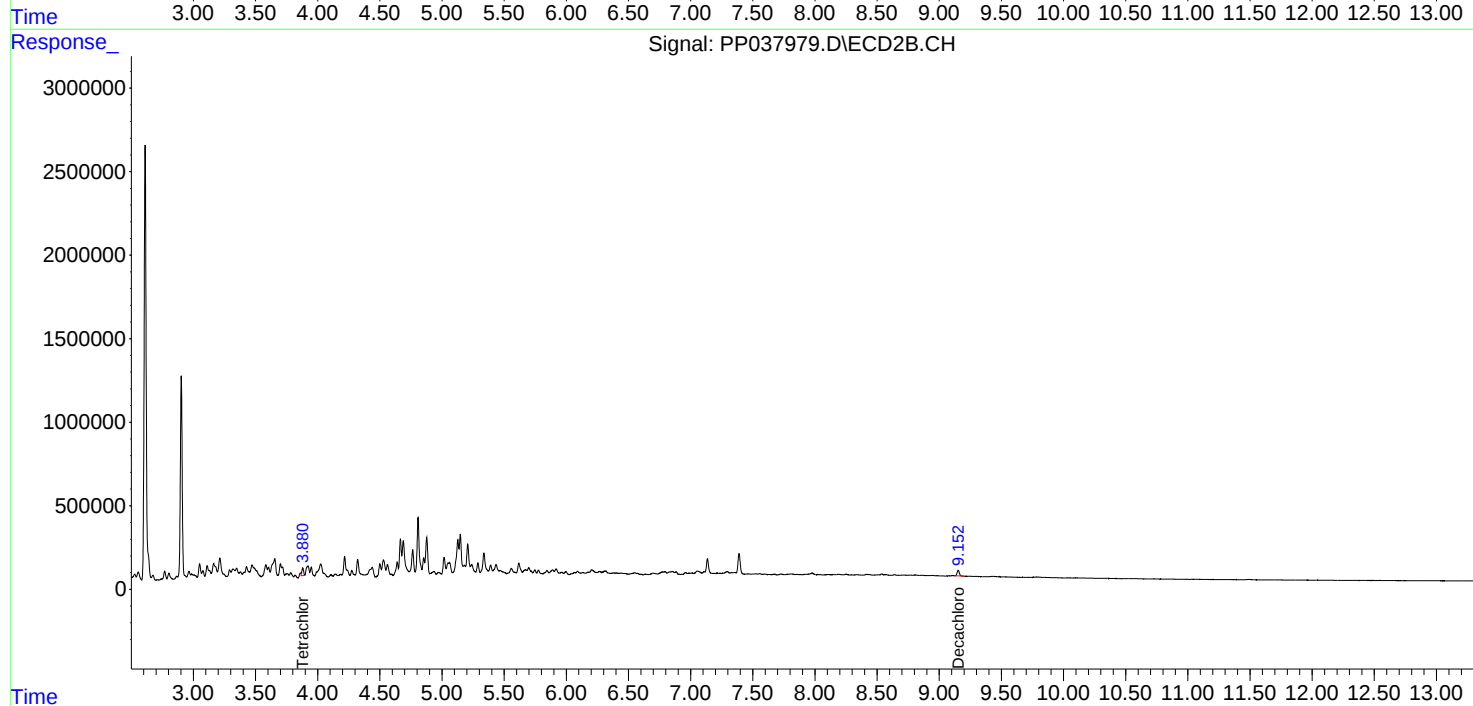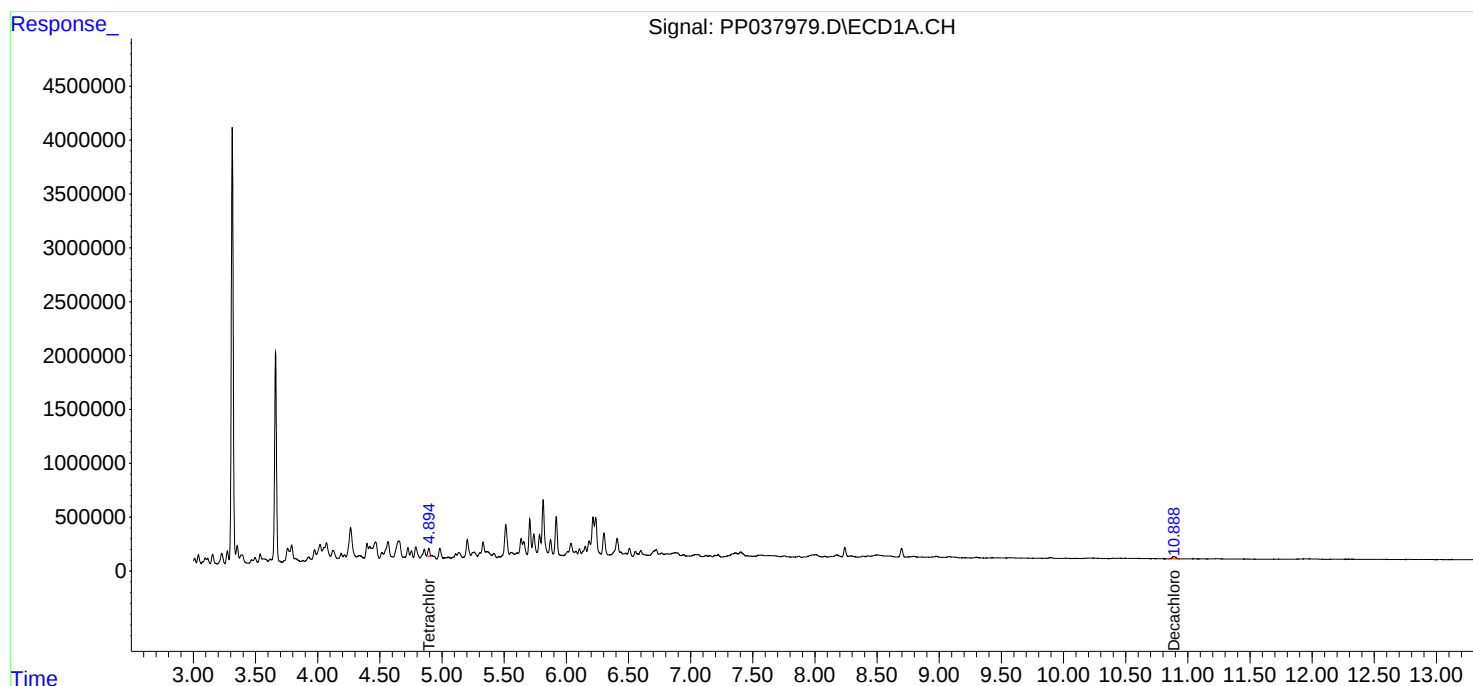

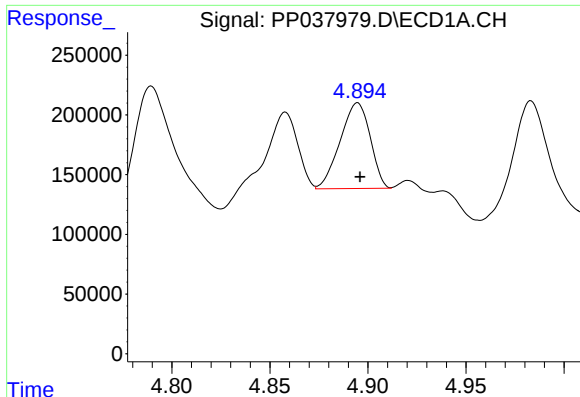


#1 Tetrachloro-m-xylene

R.T.: 4.894 min
Delta R.T.: -0.002 min
Response: 767201
Conc: 17.22 ng/ml m

Instrument :
ECD_P
ClientSampleId :
33389


Manual Integrations
APPROVED

mohammad
8/4/2021 11:55:45 AM

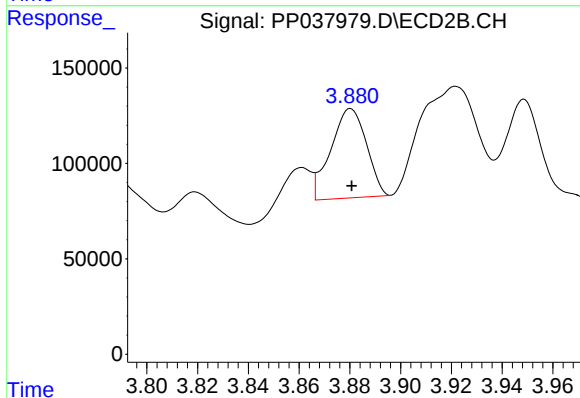


#1 Tetrachloro-m-xylene

R.T.: 3.880 min
Delta R.T.: 0.000 min
Response: 456826
Conc: 18.20 ng/ml

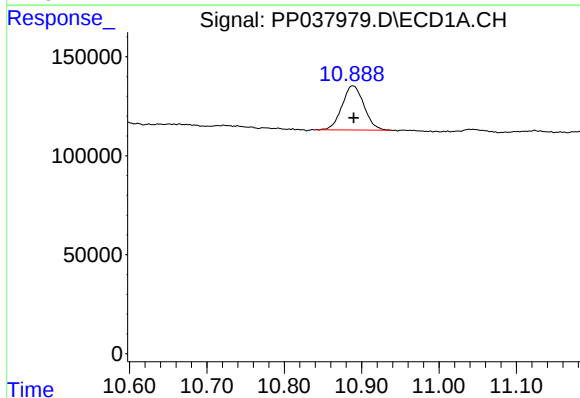

#2 Decachlorobiphenyl

R.T.: 10.889 min
Delta R.T.: -0.001 min
Response: 439300
Conc: 16.77 ng/ml

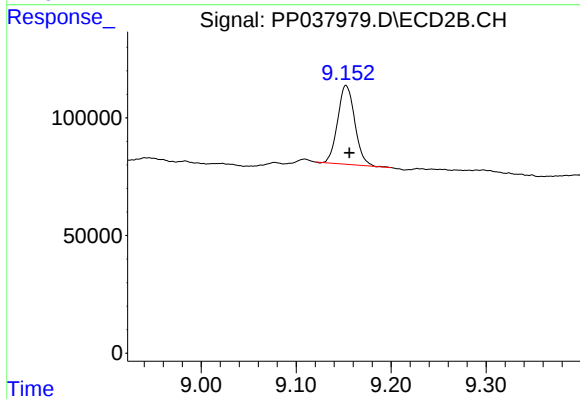

#2 Decachlorobiphenyl

R.T.: 9.153 min
Delta R.T.: -0.004 min
Response: 418022
Conc: 17.85 ng/ml