

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080423\
 Data File : PP059134.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Aug 2023 15:42
 Operator : YP\AJ
 Sample : 03896-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SLUDGE-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/07/2023
 Supervised By :Ankita Jodhani 08/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 06:17:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP073123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 01 05:06:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.420	3.656	7295802	11005391	4.521m	4.551
2) SA Decachlor...	10.216	8.694	2217551	3563761	2.366	2.648

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080423\
Data File : PP059134.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2023 15:42
Operator : YP\AJ
Sample : 03896-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SLUDGE-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/07/2023
Supervised By :Ankita Jodhani 08/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 06:17:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP073123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 01 05:06:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

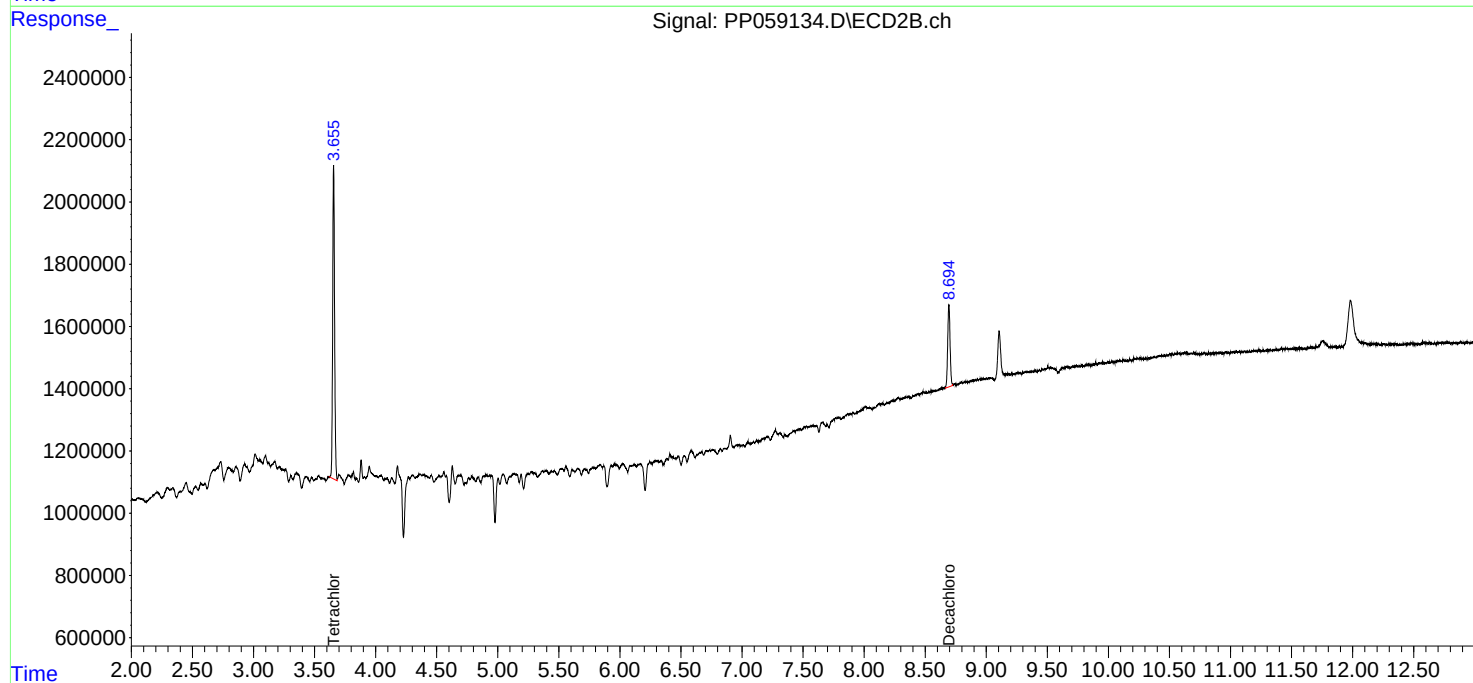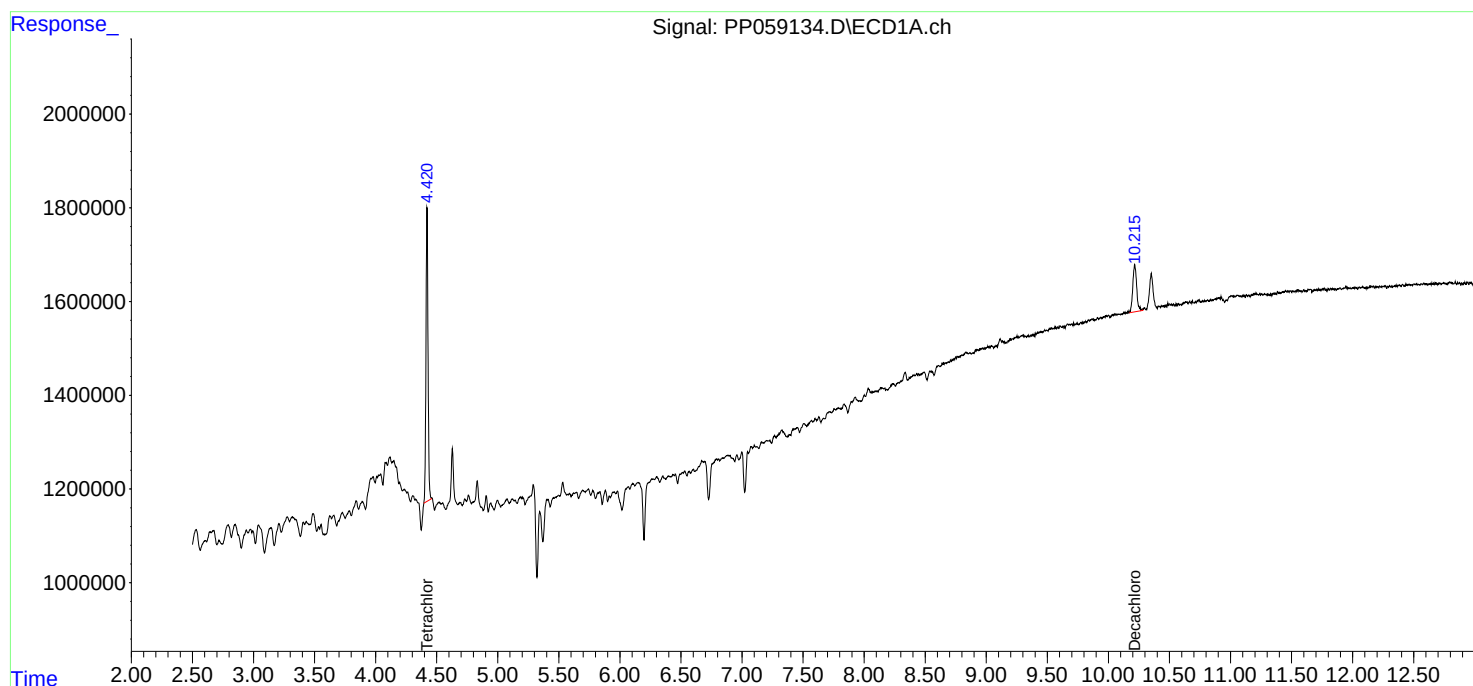

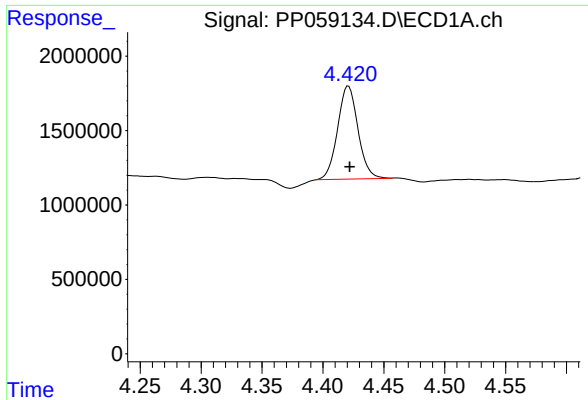


#1 Tetrachloro-m-xylene

R.T.: 4.420 min
Delta R.T.: -0.002 min
Response: 7295802
Conc: 4.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
SLUDGE-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/07/2023
Supervised By :Ankita Jodhani 08/07/2023

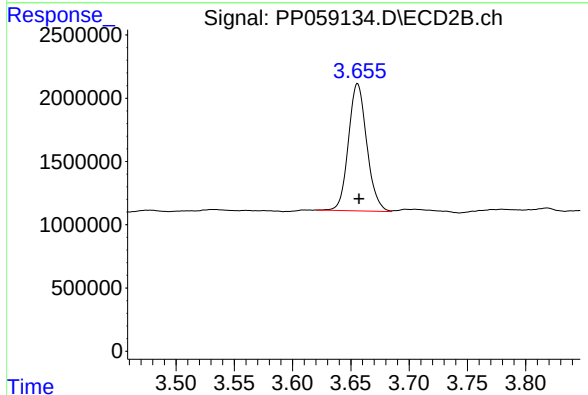


#1 Tetrachloro-m-xylene

R.T.: 3.656 min
Delta R.T.: -0.001 min
Response: 11005391
Conc: 4.55 ng/ml

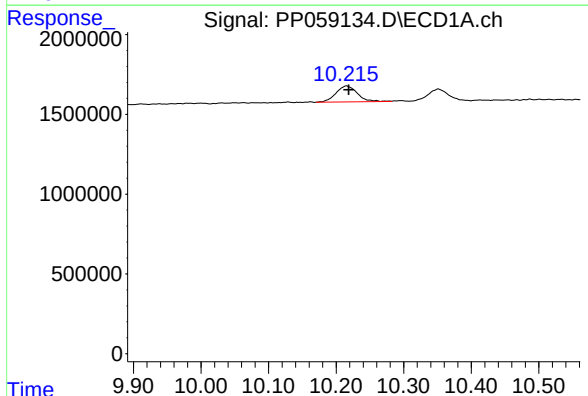

#2 Decachlorobiphenyl

R.T.: 10.216 min
Delta R.T.: -0.003 min
Response: 2217551
Conc: 2.37 ng/ml

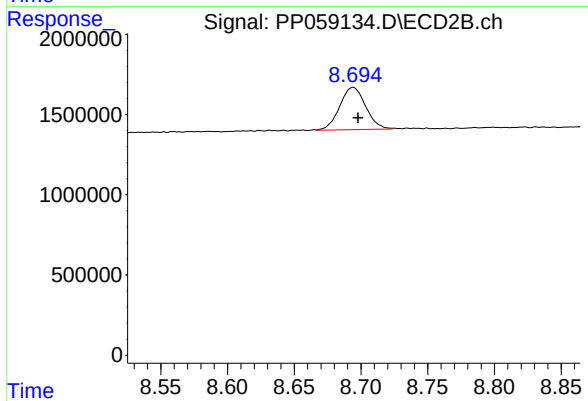

#2 Decachlorobiphenyl

R.T.: 8.694 min
Delta R.T.: -0.004 min
Response: 3563761
Conc: 2.65 ng/ml