

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080423\
 Data File : PP059155.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Aug 2023 22:05
 Operator : YP\AJ
 Sample : 03899-01 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 520

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/07/2023
 Supervised By :Ankita Jodhani 08/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 06:28:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP073123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 01 05:06:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.420	3.658	2024708	2569554	1.255m	1.063
2) SA Decachlor...	10.218	8.695	2584480	4246490	2.757	3.155

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080423\
Data File : PP059155.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2023 22:05
Operator : YP\AJ
Sample : 03899-01 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
520


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/07/2023
Supervised By :Ankita Jodhani 08/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 06:28:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP073123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 01 05:06:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

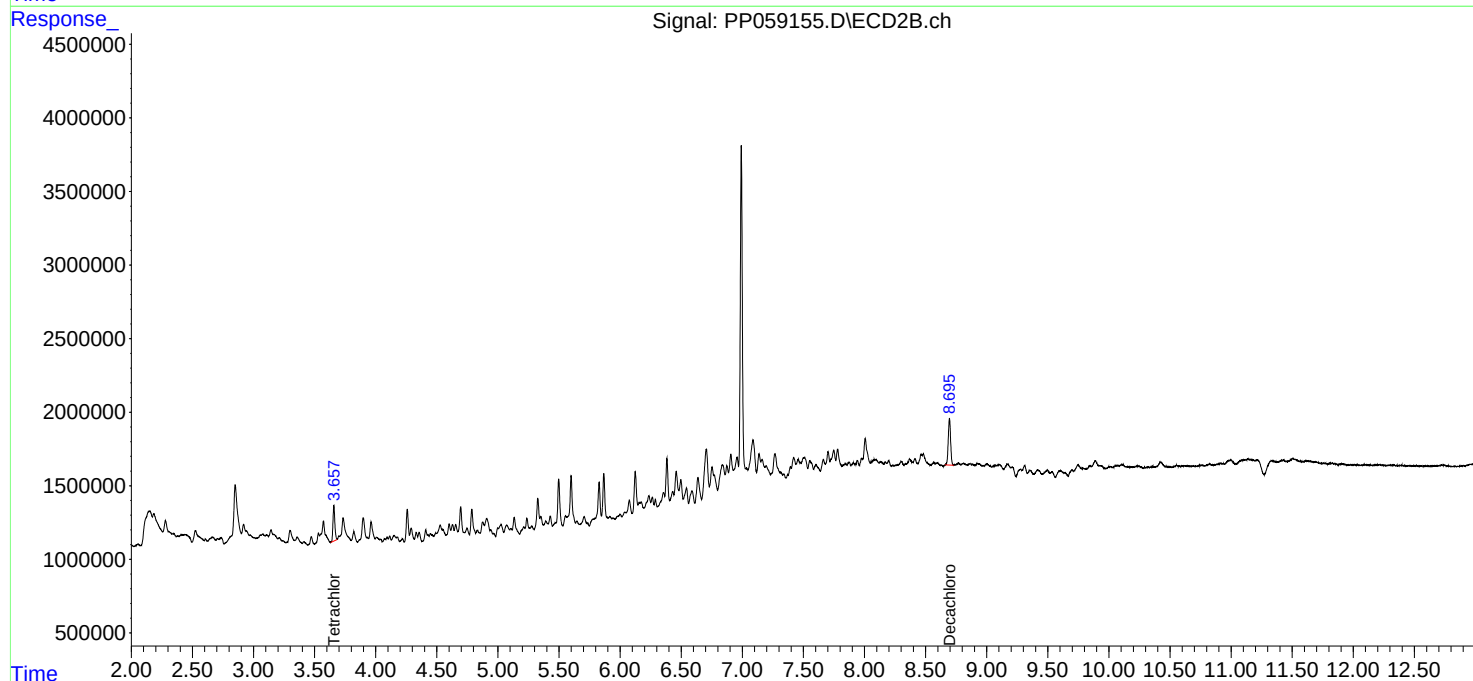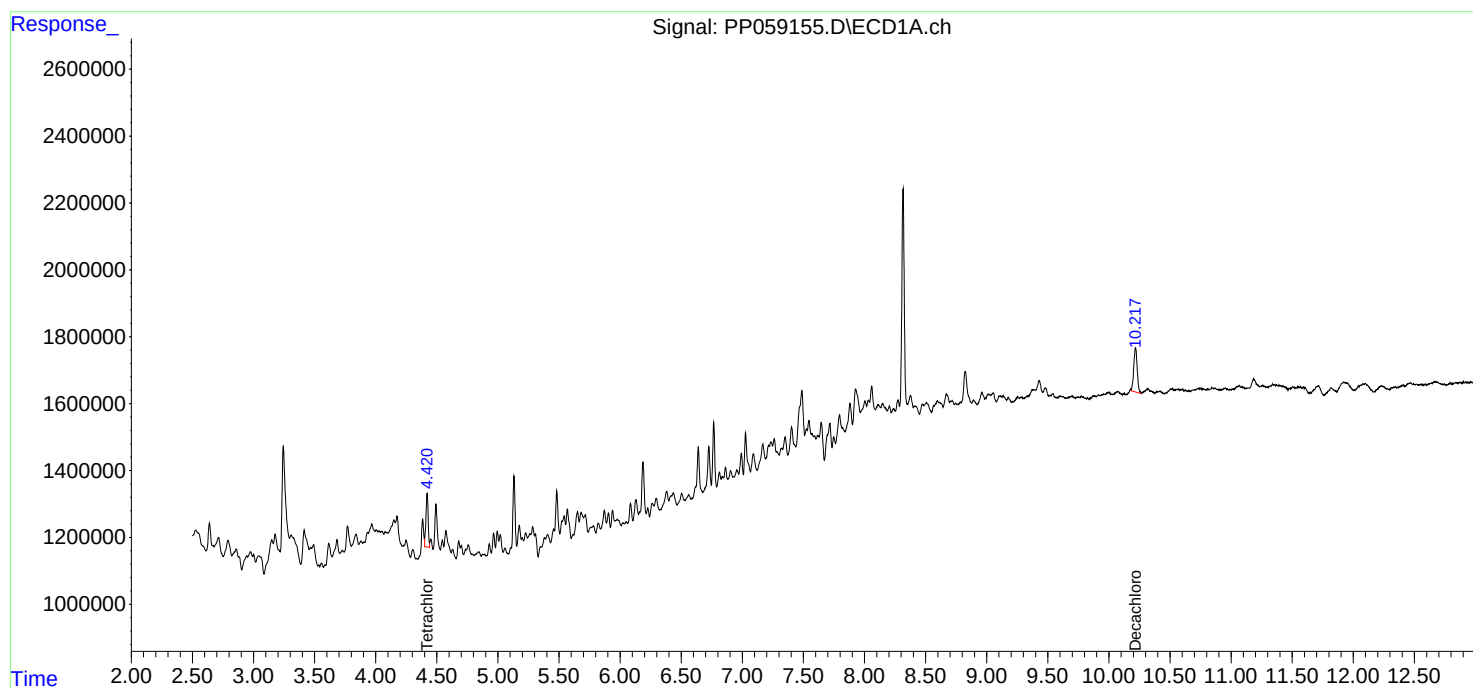

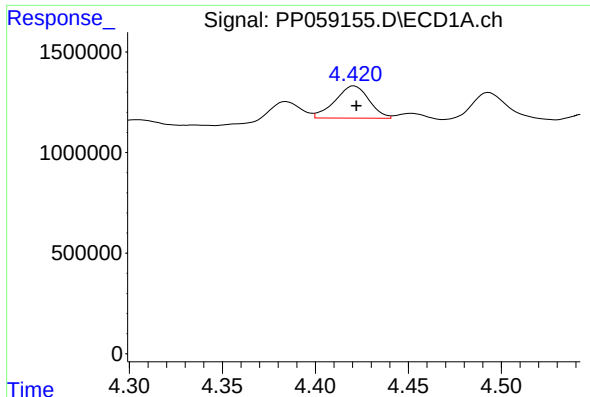


#1 Tetrachloro-m-xylene

R.T.: 4.420 min
Delta R.T.: -0.002 min
Response: 2024708
Conc: 1.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
520


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/07/2023
Supervised By :Ankita Jodhani 08/07/2023

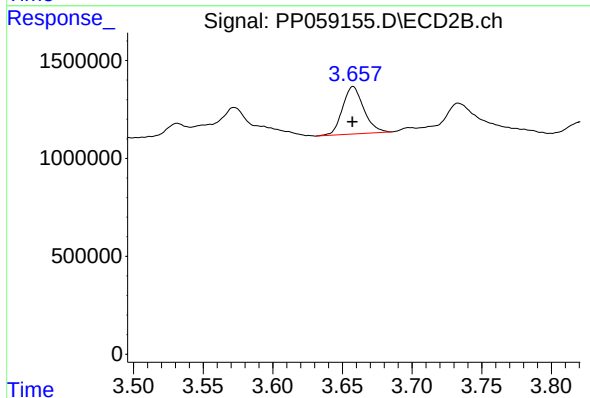


#1 Tetrachloro-m-xylene

R.T.: 3.658 min
Delta R.T.: 0.000 min
Response: 2569554
Conc: 1.06 ng/ml

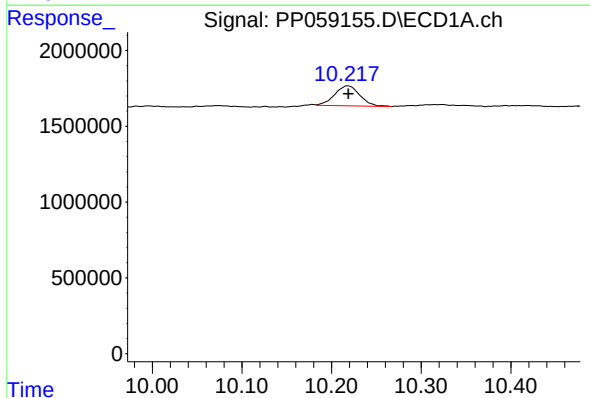

#2 Decachlorobiphenyl

R.T.: 10.218 min
Delta R.T.: 0.000 min
Response: 2584480
Conc: 2.76 ng/ml

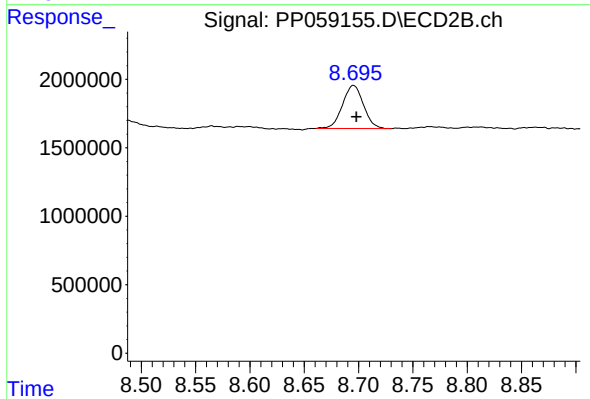

#2 Decachlorobiphenyl

R.T.: 8.695 min
Delta R.T.: -0.003 min
Response: 4246490
Conc: 3.15 ng/ml