

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080525\
 Data File : PP074234.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2025 15:23
 Operator : YP\AJ
 Sample : Q2759-04 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LIQUID-DRUMS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/06/2025
 Supervised By :mohammad ahmed 08/07/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 04:23:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.656	3.795	967780	906818	0.865	0.236m#
2) SA Decachlor...	10.434	8.804	658873	9091885	0.678m	1.512m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080525\
Data File : PP074234.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2025 15:23
Operator : YP\AJ
Sample : Q2759-04 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LIQUID-DRUMS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/06/2025
Supervised By :mohammad ahmed 08/07/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 04:23:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 04 11:01:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

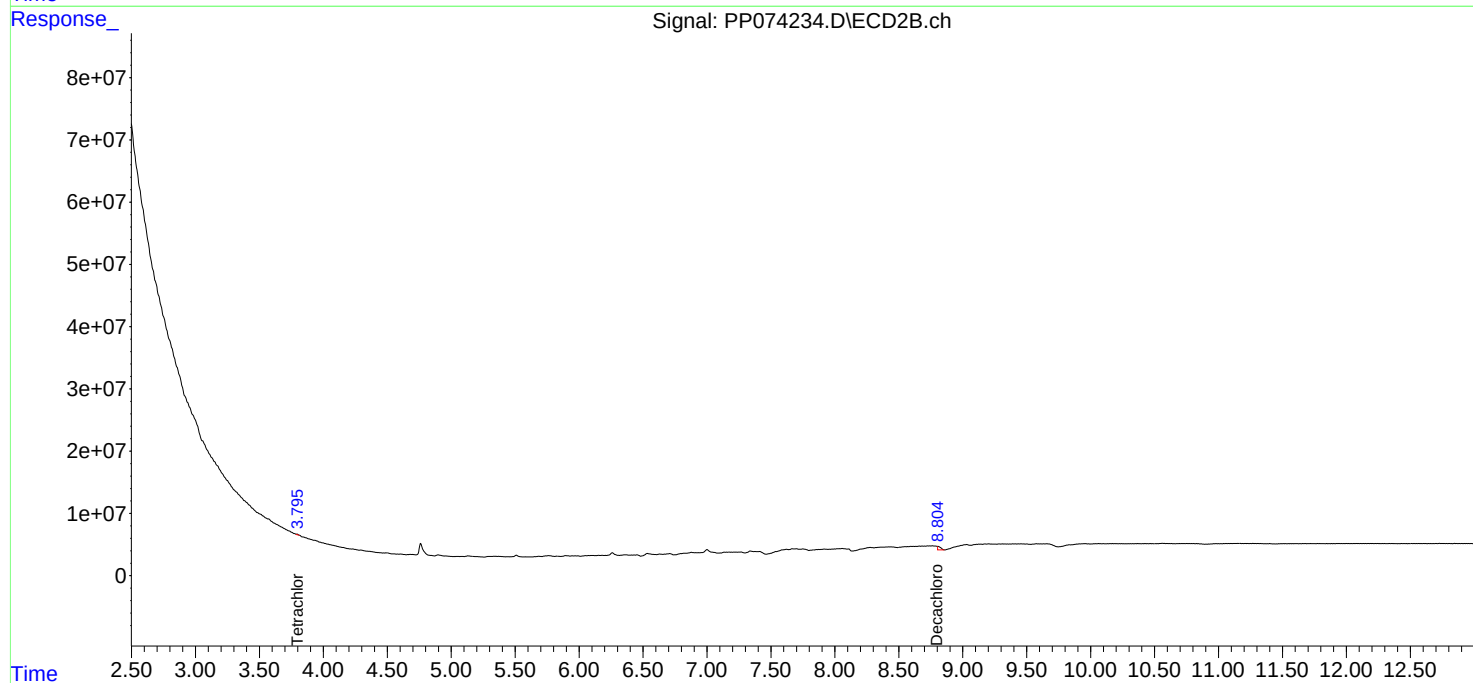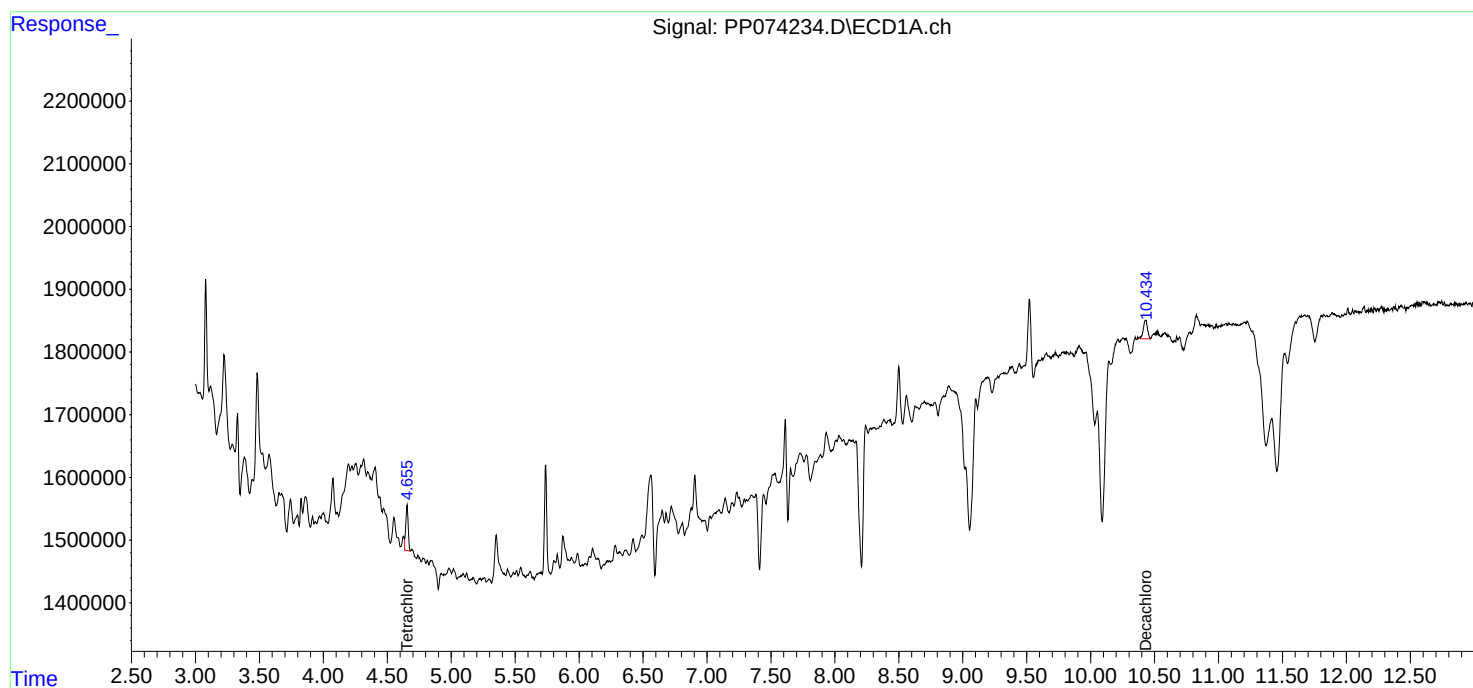

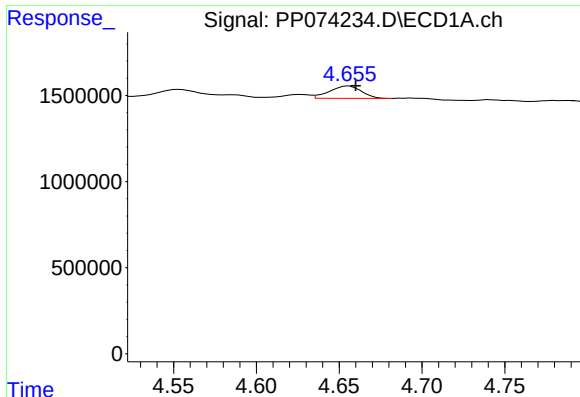


#1 Tetrachloro-m-xylene

R.T.: 4.656 min
Delta R.T.: -0.004 min
Response: 967780
Conc: 0.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
LIQUID-DRUMS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/06/2025
Supervised By :mohammad ahmed 08/07/2025

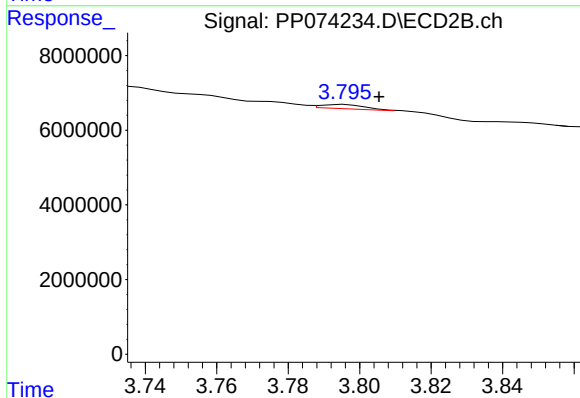


#1 Tetrachloro-m-xylene

R.T.: 3.795 min
Delta R.T.: -0.010 min
Response: 906818
Conc: 0.24 ng/ml m

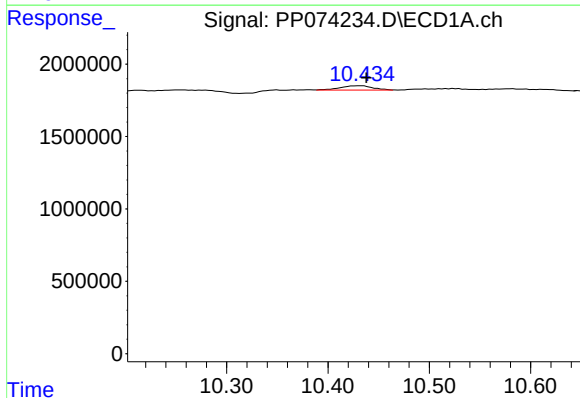

#2 Decachlorobiphenyl

R.T.: 10.434 min
Delta R.T.: -0.004 min
Response: 658873
Conc: 0.68 ng/ml m

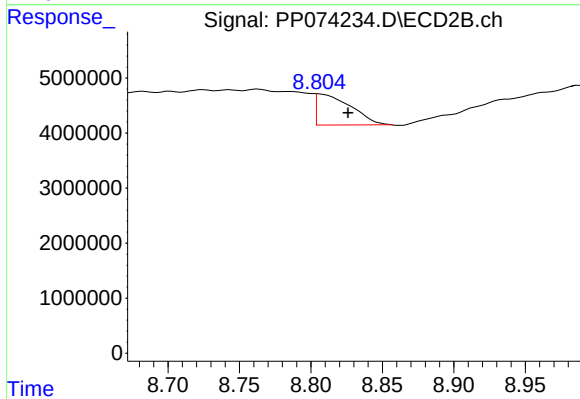

#2 Decachlorobiphenyl

R.T.: 8.804 min
Delta R.T.: -0.022 min
Response: 9091885
Conc: 1.51 ng/ml m