

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080621\
 Data File : PP038071.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Aug 2021 12:02
 Operator : AJ\MA
 Sample : M3296-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-BPM-03-026-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 12:55:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.895	3.881	1191882	722605	26.819	28.056
2)	SA Decachlor...	10.886	9.149	523079	524846	22.994	20.285
Target Compounds							
8)	L2 AR-1221-1	5.145	0.000	228149	0	420.909	N.D. #
9)	L2 AR-1221-2	0.000	4.226	0	12670	N.D.	53.833 #
20)	L4 AR-1242-5	7.204	0.000	16116	0	19.544	N.D. #
25)	L5 AR-1248-5	7.204	0.000	16116	0	12.190	N.D. #
28)	L6 AR-1254-3	7.751f	0.000	45151	0	22.758	N.D. #
33)	L7 AR-1260-3	0.000	7.068	0	12874	N.D.	8.457 #
45)	L9 AR-1268-5	0.000	8.915	0	3215	N.D.	0.339 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080621\
Data File : PP038071.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2021 12:02
Operator : AJ\MA
Sample : M3296-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-026-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 12:55:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

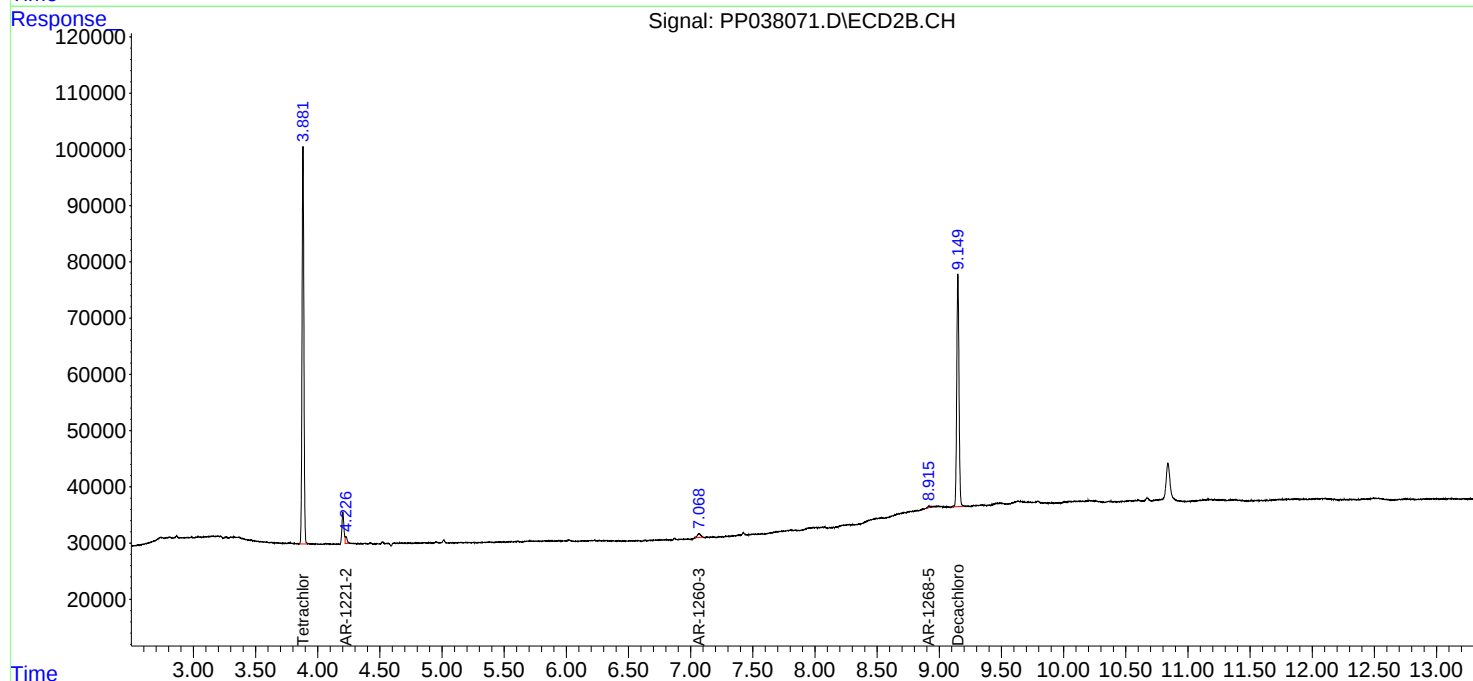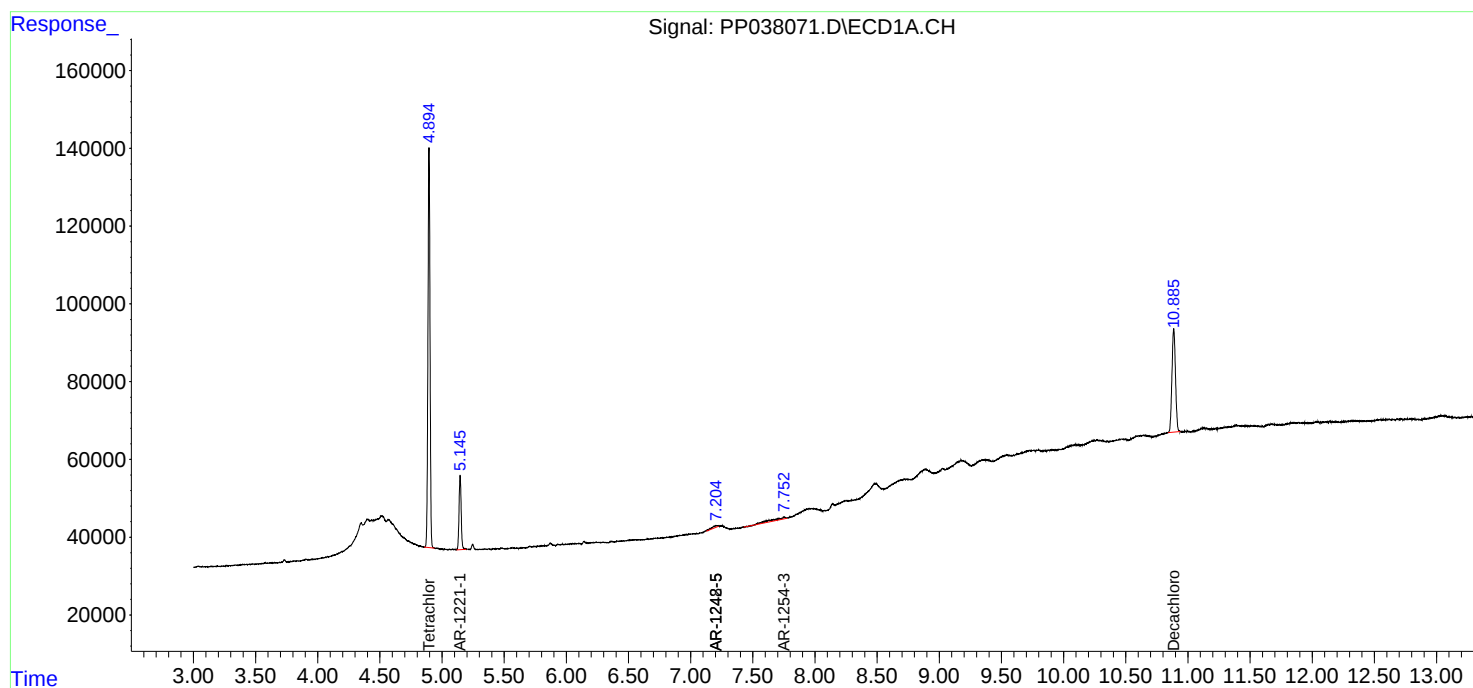


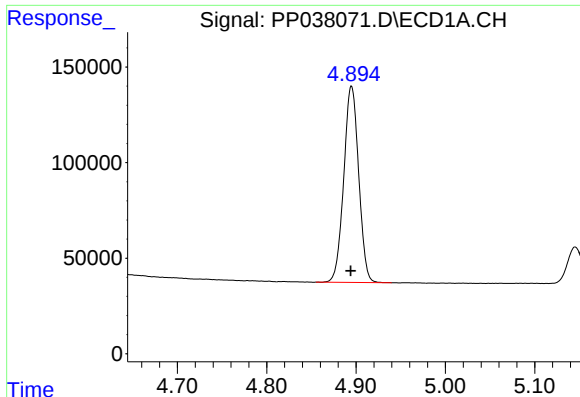

#1 Tetrachloro-m-xylene


R.T.: 4.895 min
Delta R.T.: 0.000 min
Response: 1191882
Conc: 26.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-026-ABCD

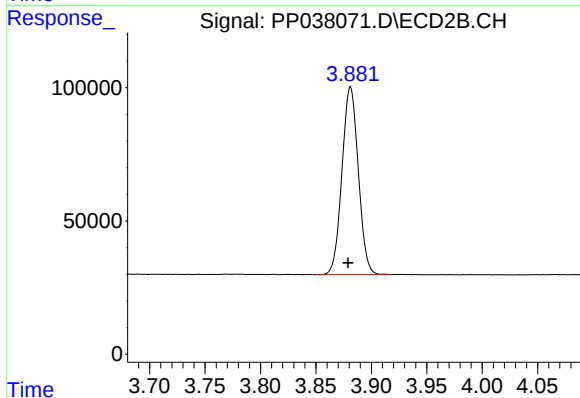


#1 Tetrachloro-m-xylene

R.T.: 3.881 min
Delta R.T.: 0.002 min
Response: 722605
Conc: 28.06 ng/ml

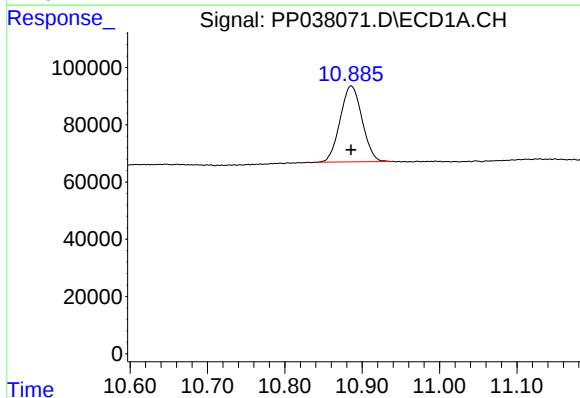


#2 Decachlorobiphenyl

R.T.: 10.886 min
Delta R.T.: 0.000 min
Response: 523079
Conc: 22.99 ng/ml

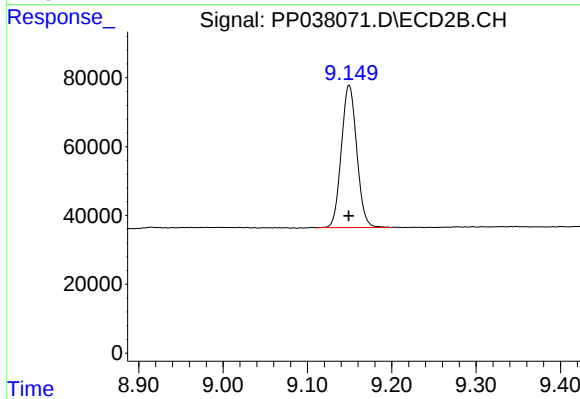

#2 Decachlorobiphenyl


R.T.: 9.149 min
Delta R.T.: 0.000 min
Response: 524846
Conc: 20.29 ng/ml

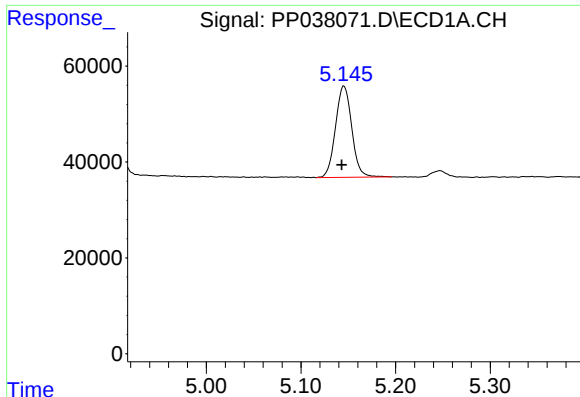

#8 AR-1221-1


R.T.: 5.145 min
Delta R.T.: 0.002 min
Response: 228149
Conc: 420.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-026-ABCD

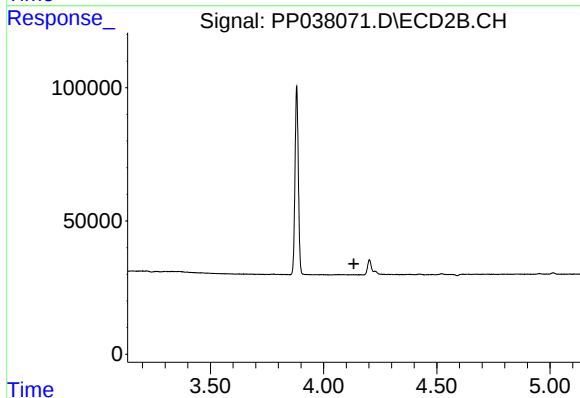


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.134 min
Response: 0
Conc: N.D.

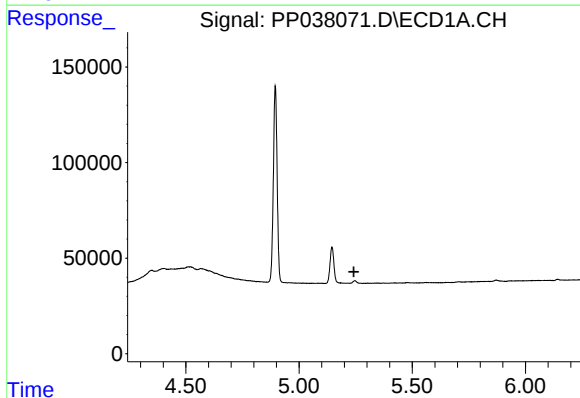


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.242 min
Response: 0
Conc: N.D.

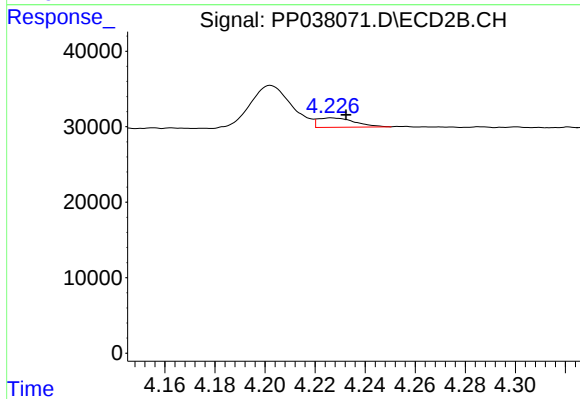

#9 AR-1221-2


R.T.: 4.226 min
Delta R.T.: -0.006 min
Response: 12670
Conc: 53.83 ng/ml

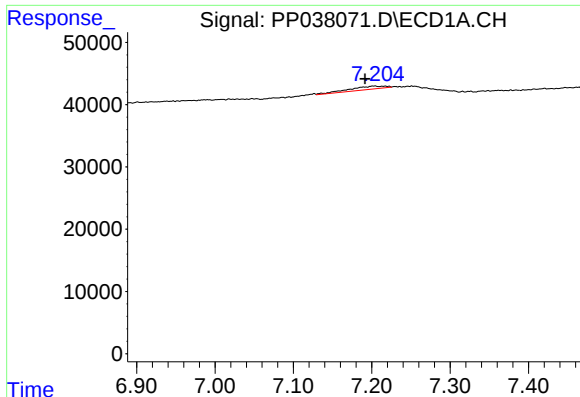

#20 AR-1242-5


R.T.: 7.204 min
Delta R.T.: 0.013 min
Response: 16116
Conc: 19.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-026-ABCD

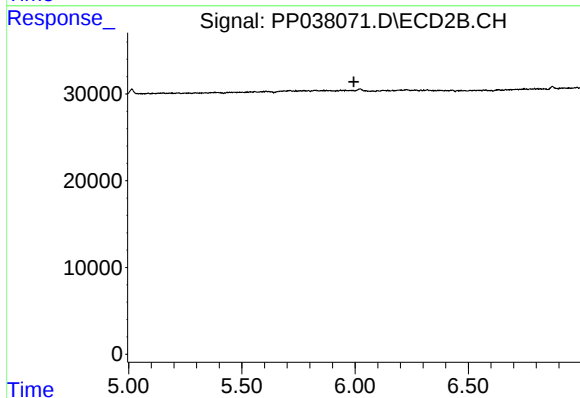


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 5.995 min
Response: 0
Conc: N.D.

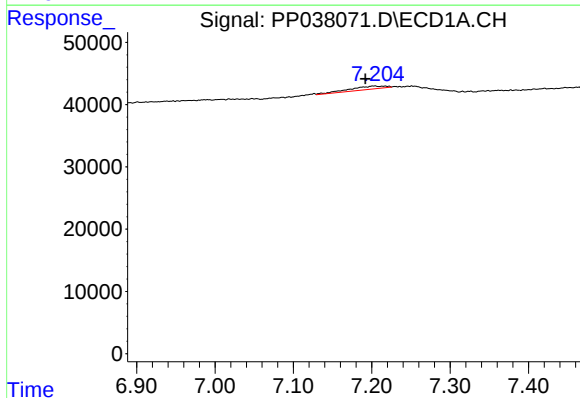


#25 AR-1248-5

R.T.: 7.204 min
Delta R.T.: 0.012 min
Response: 16116
Conc: 12.19 ng/ml

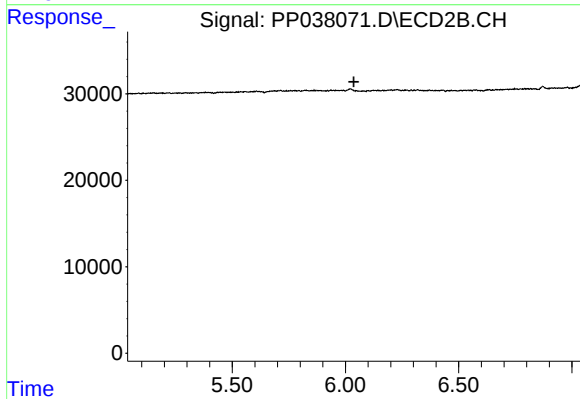

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.037 min
Response: 0
Conc: N.D.

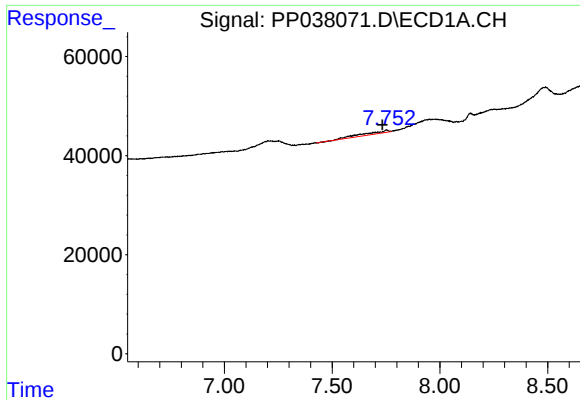

#28 AR-1254-3


R.T.: 7.751 min
Delta R.T.: 0.018 min
Response: 45151
Conc: 22.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-026-ABCD

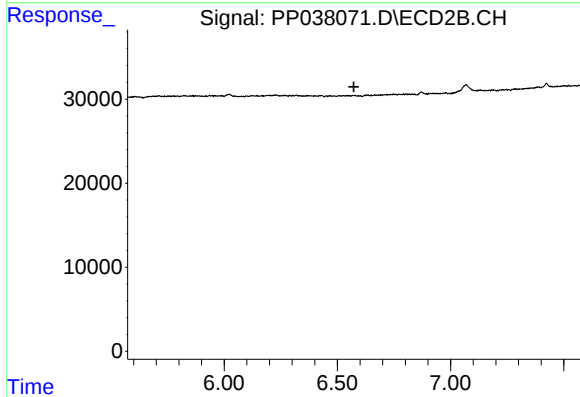


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.573 min
Response: 0
Conc: N.D.

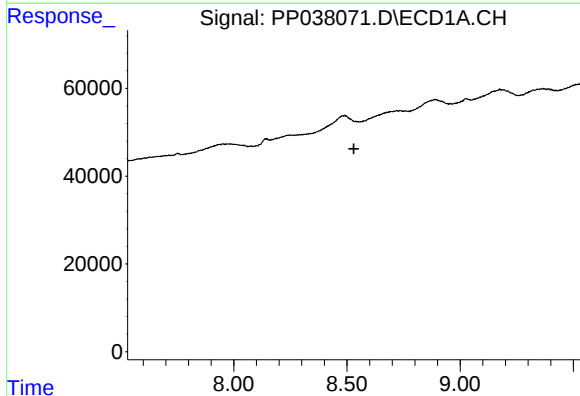


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.530 min
Response: 0
Conc: N.D.

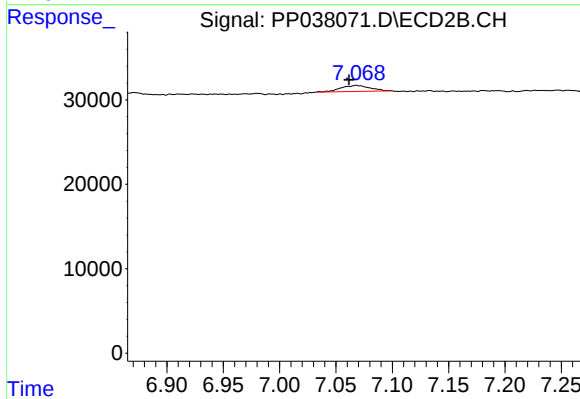

#33 AR-1260-3


R.T.: 7.068 min
Delta R.T.: 0.006 min
Response: 12874
Conc: 8.46 ng/ml

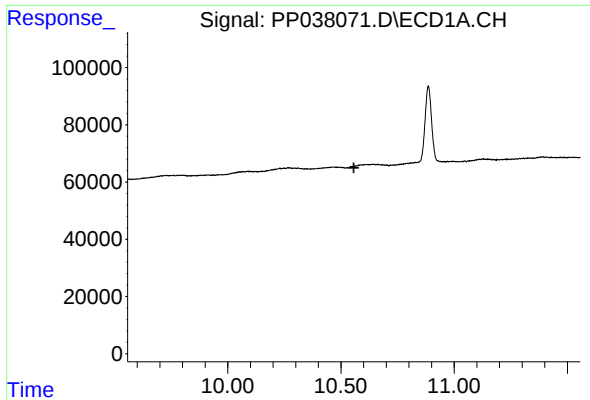

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.557 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-026-ABCD

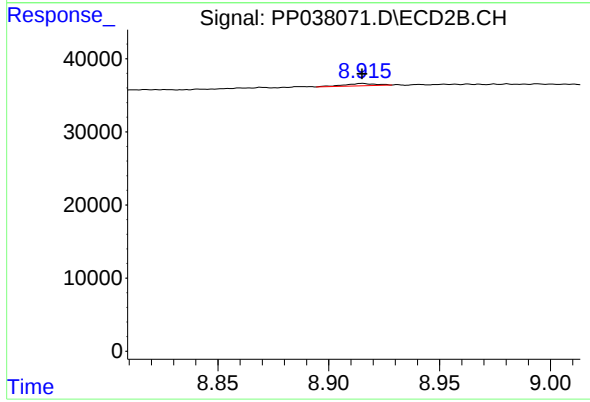

#45 AR-1268-5

R.T.: 8.915 min
Delta R.T.: 0.000 min
Response: 3215
Conc: 0.34 ng/ml