

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080621\
 Data File : PP038105.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Aug 2021 23:30
 Operator : AJ\MA
 Sample : M3291-04
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 02:10:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.894	3.880	854111	550264	19.219	21.365
2)	SA Decachlor...	10.887	9.148	414109	443532	18.204	17.143
Target Compounds							
8)	L2 AR-1221-1	5.145	0.000	63757	0	117.625	N.D. #
9)	L2 AR-1221-2	0.000	4.227	0	8833	N.D.	37.532 #
20)	L4 AR-1242-5	0.000	6.020f	0	6390	N.D.	9.888 #
25)	L5 AR-1248-5	0.000	6.020f	0	6390	N.D.	6.787 #
26)	L6 AR-1254-1	0.000	6.020f	0	6390	N.D.	4.776 #
30)	L6 AR-1254-5	8.478f	0.000	131502	0	90.488	N.D. #
33)	L7 AR-1260-3	0.000	7.063	0	14425	N.D.	9.476 #
45)	L9 AR-1268-5	0.000	8.916	0	6243	N.D.	0.658 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080621\
Data File : PP038105.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2021 23:30
Operator : AJ\MA
Sample : M3291-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
WC-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 02:10:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

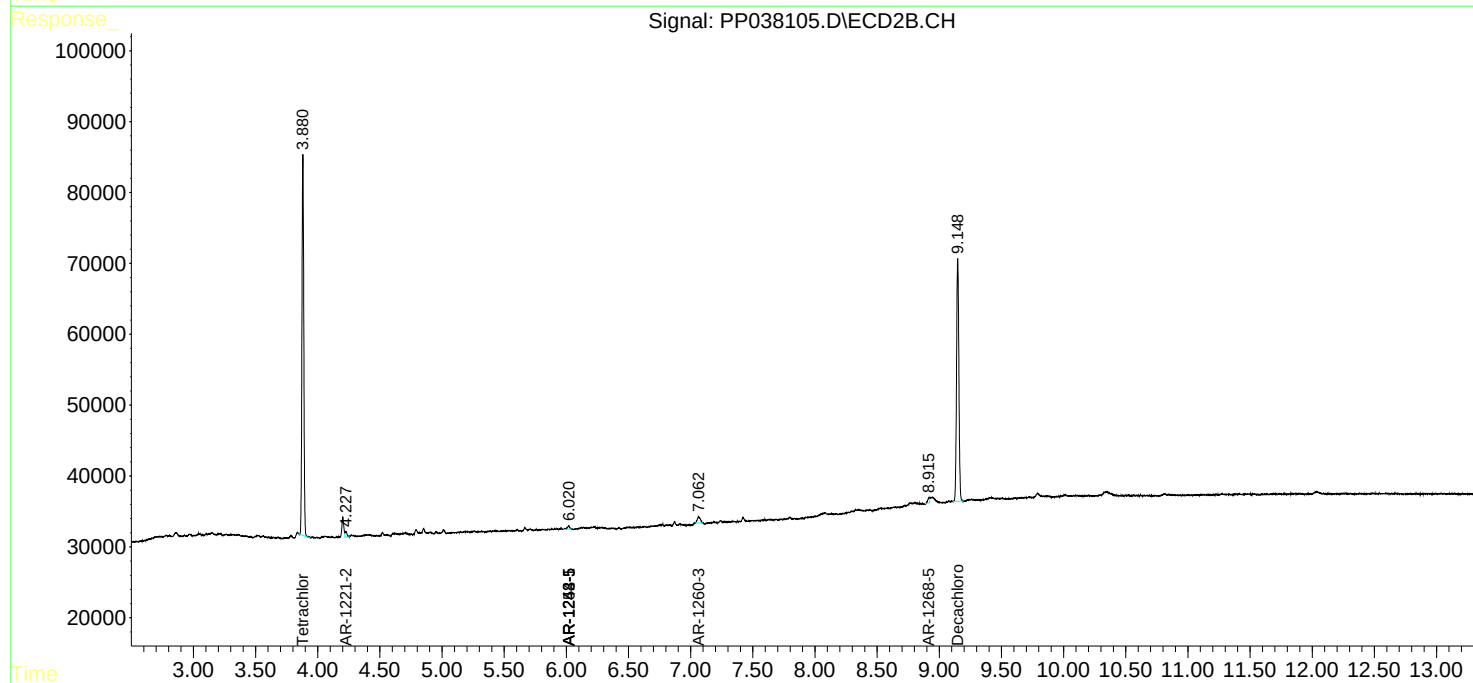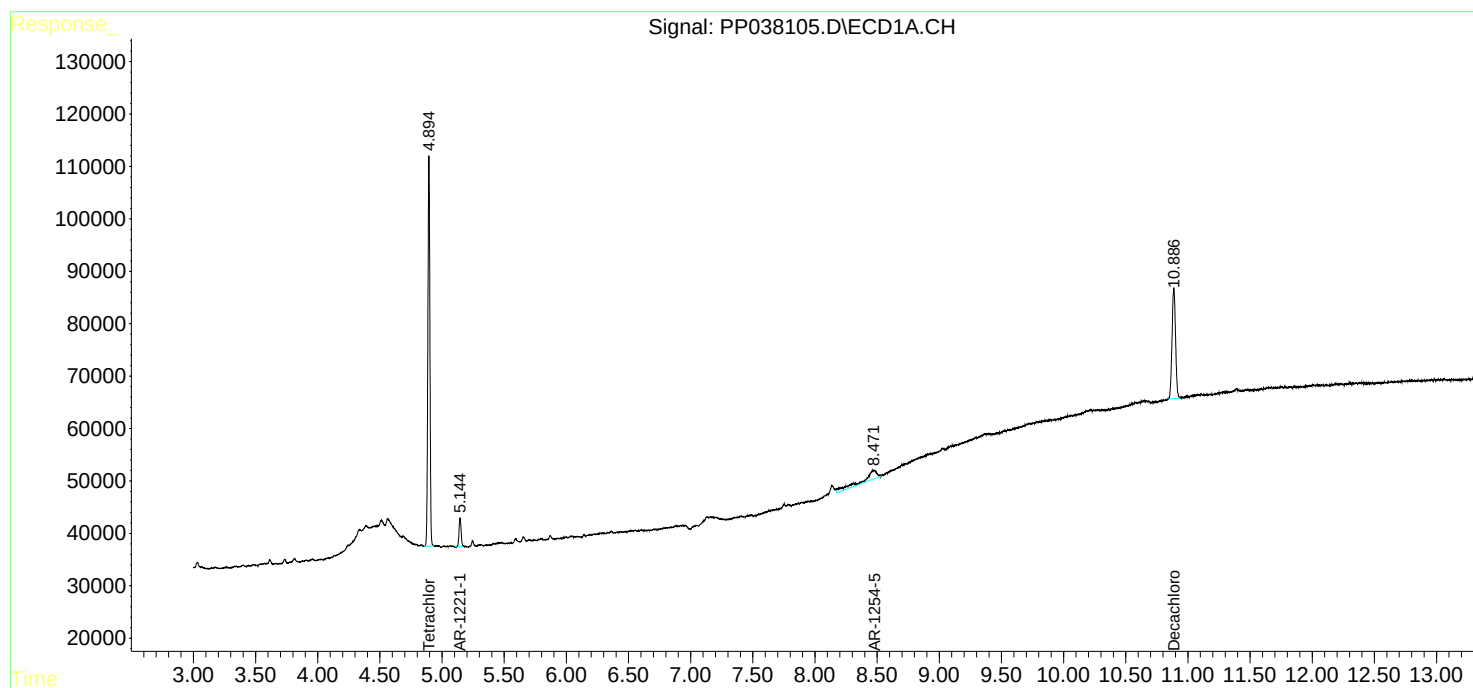


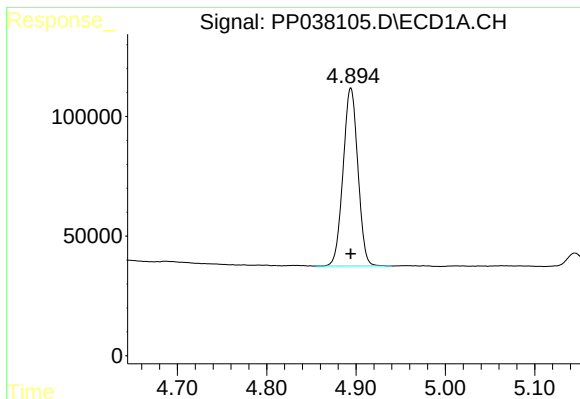

#1 Tetrachloro-m-xylene


R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 854111
Conc: 19.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-2

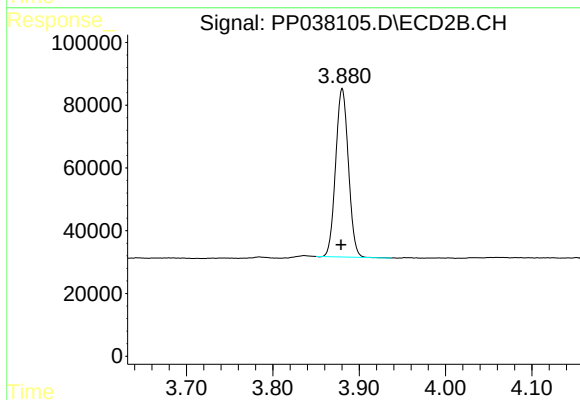


#1 Tetrachloro-m-xylene

R.T.: 3.880 min
Delta R.T.: 0.001 min
Response: 550264
Conc: 21.36 ng/ml

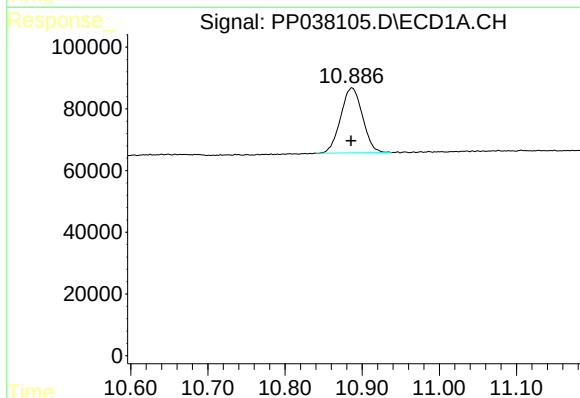


#2 Decachlorobiphenyl

R.T.: 10.887 min
Delta R.T.: 0.001 min
Response: 414109
Conc: 18.20 ng/ml

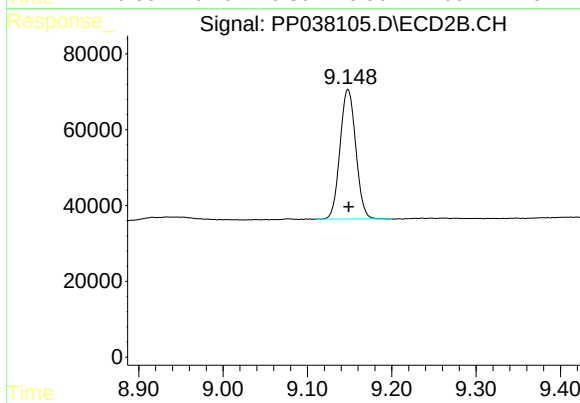

#2 Decachlorobiphenyl


R.T.: 9.148 min
Delta R.T.: 0.000 min
Response: 443532
Conc: 17.14 ng/ml

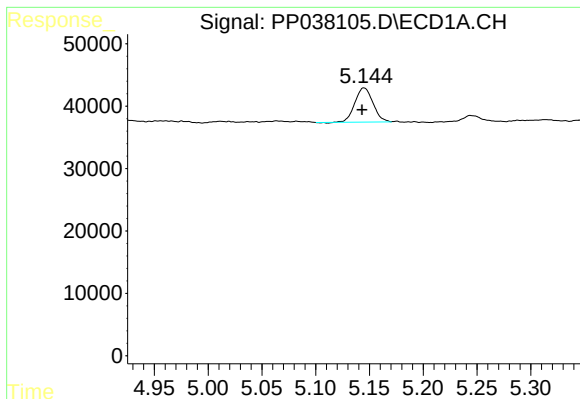

#8 AR-1221-1


R.T.: 5.145 min
Delta R.T.: 0.002 min
Response: 63757
Conc: 117.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-2

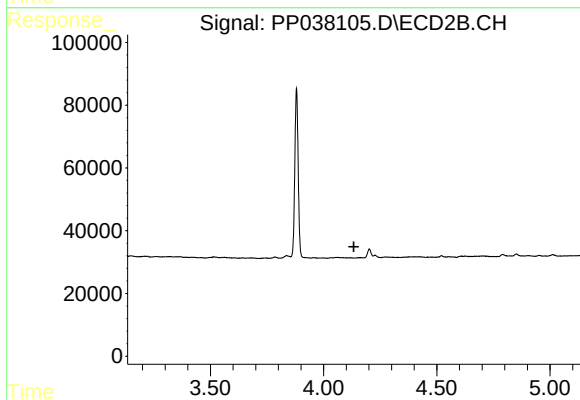


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.134 min
Response: 0
Conc: N.D.

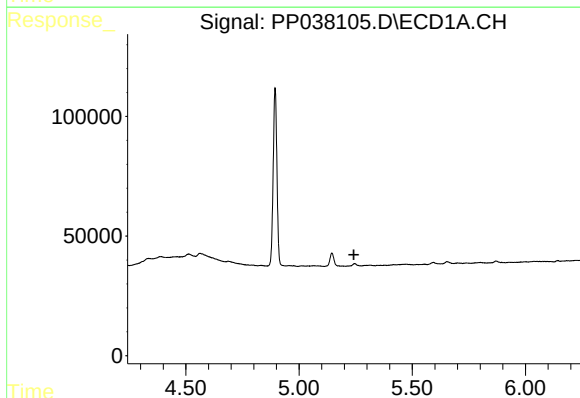


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.242 min
Response: 0
Conc: N.D.

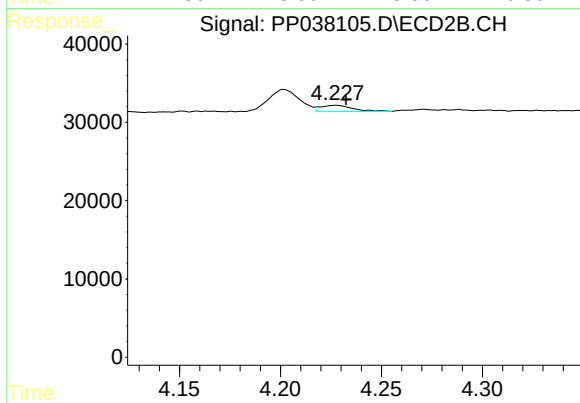

#9 AR-1221-2


R.T.: 4.227 min
Delta R.T.: -0.005 min
Response: 8833
Conc: 37.53 ng/ml

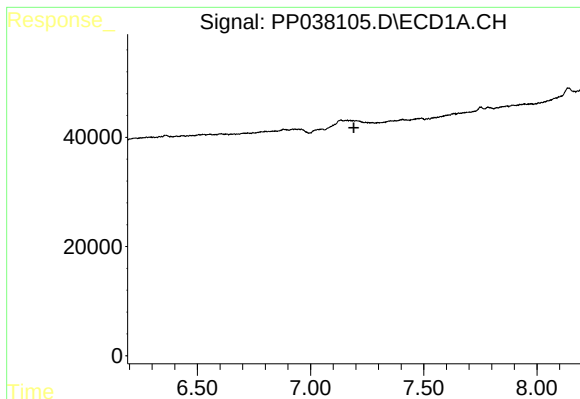

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.192 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
WC-2

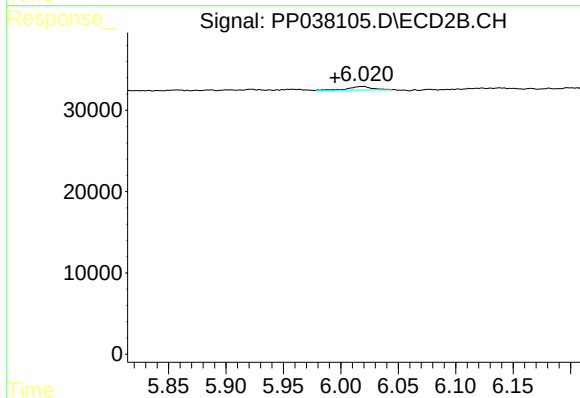


#20 AR-1242-5

R.T.: 6.020 min
Delta R.T.: 0.025 min
Response: 6390
Conc: 9.89 ng/ml

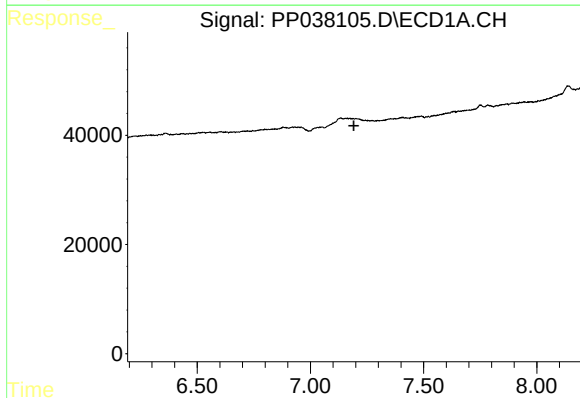


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 7.192 min
Response: 0
Conc: N.D.

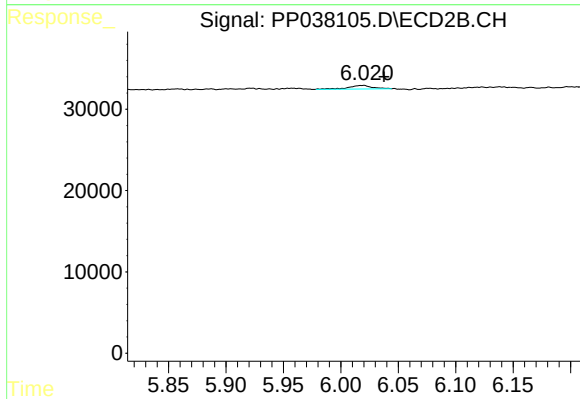

#25 AR-1248-5


R.T.: 6.020 min
Delta R.T.: -0.017 min
Response: 6390
Conc: 6.79 ng/ml

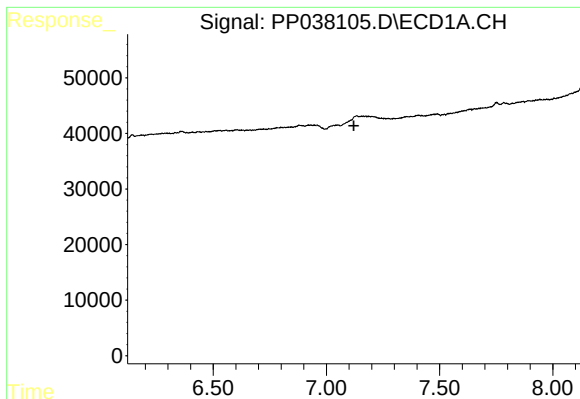

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 7.121 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
WC-2

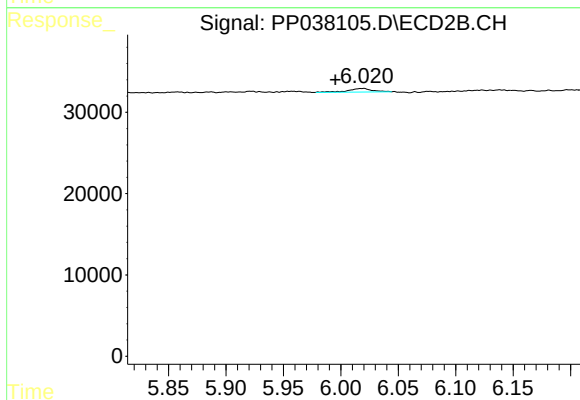


#26 AR-1254-1

R.T.: 6.020 min
Delta R.T.: 0.025 min
Response: 6390
Conc: 4.78 ng/ml

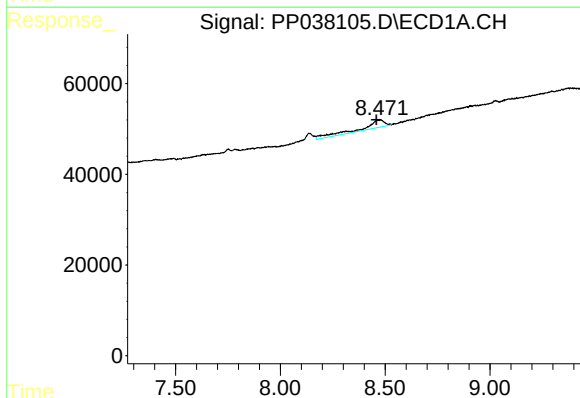


#30 AR-1254-5

R.T.: 8.478 min
Delta R.T.: 0.020 min
Response: 131502
Conc: 90.49 ng/ml

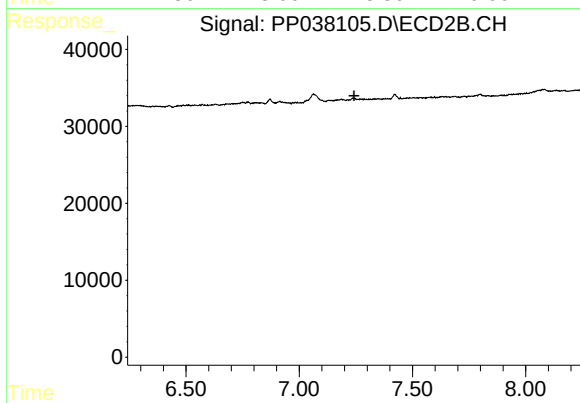

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 7.242 min
Response: 0
Conc: N.D.

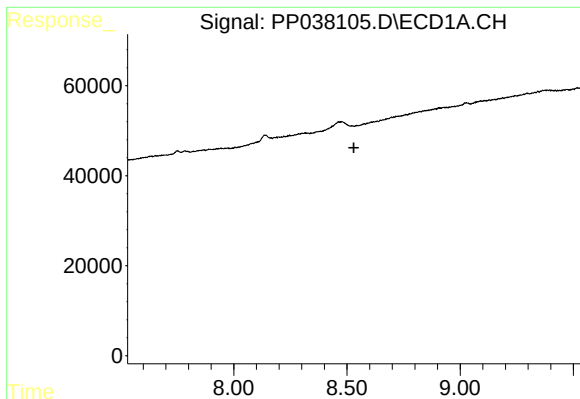

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.530 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
WC-2

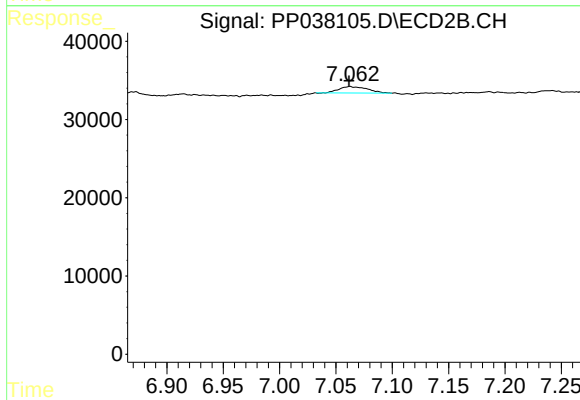


#33 AR-1260-3

R.T.: 7.063 min
Delta R.T.: 0.000 min
Response: 14425
Conc: 9.48 ng/ml

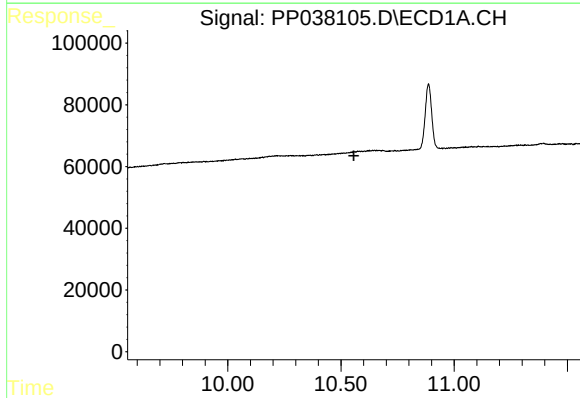

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.557 min
Response: 0
Conc: N.D.

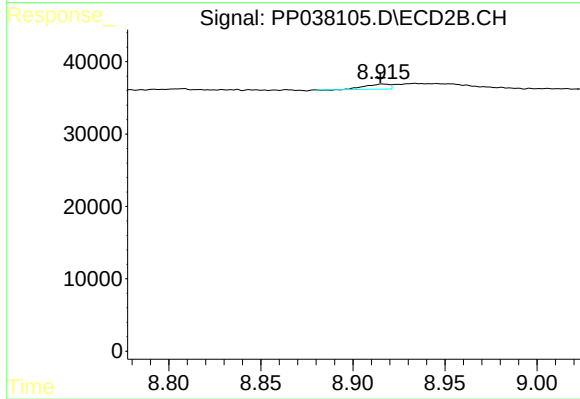

#45 AR-1268-5

R.T.: 8.916 min
Delta R.T.: 0.001 min
Response: 6243
Conc: 0.66 ng/ml