

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080621\
 Data File : PP038065.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Aug 2021 10:21
 Operator : AJ\MA
 Sample : M3290-25
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 P001-B03-BULK011-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 12:53:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.894	3.880	989643	578294	22.269	22.453
2)	SA Decachlor...	10.884	9.148	520515	657141	22.881	25.399

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080621\
Data File : PP038065.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2021 10:21
Operator : AJ\MA
Sample : M3290-25
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
P001-B03-BULK011-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 12:53:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

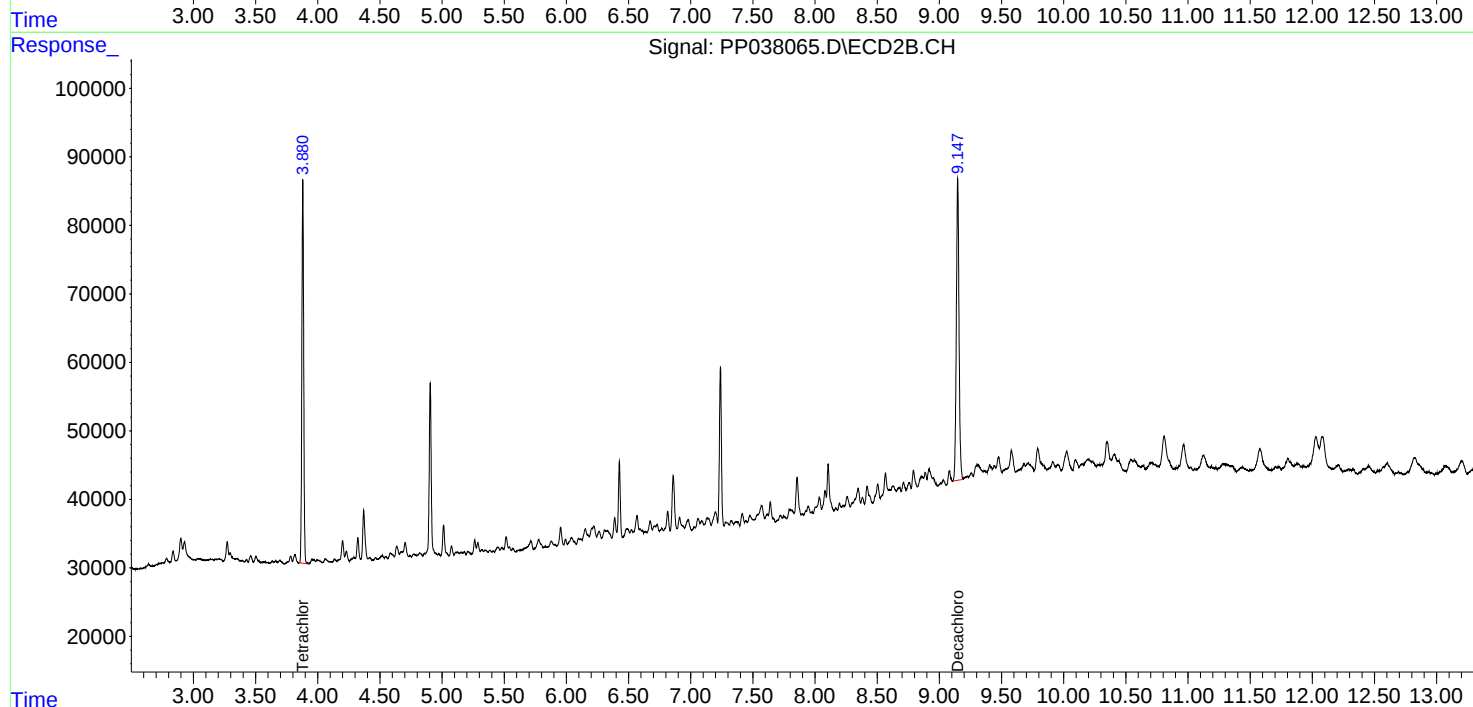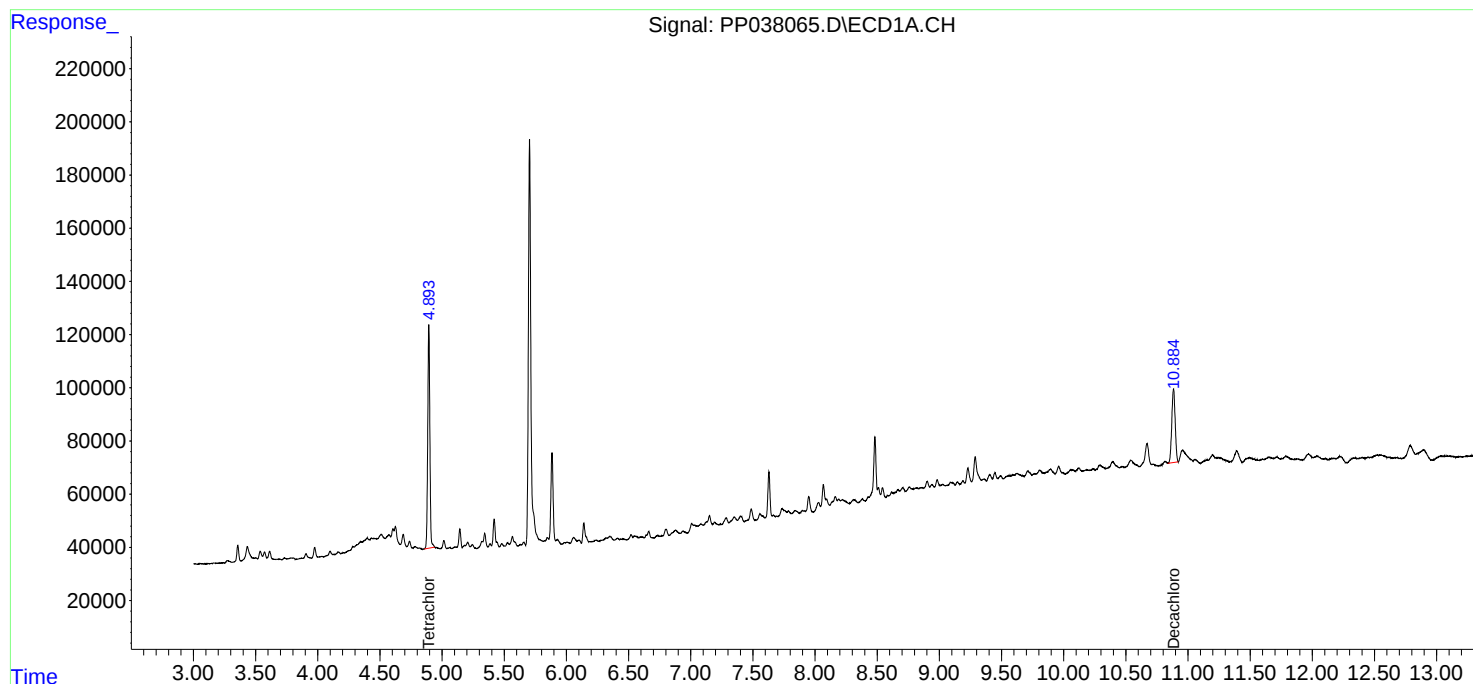


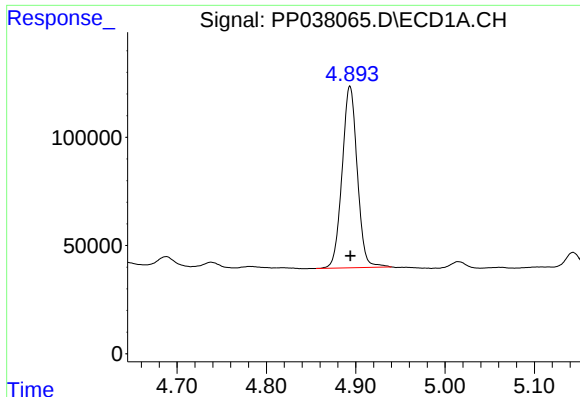

#1 Tetrachloro-m-xylene


R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 989643
Conc: 22.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
P001-B03-BULK011-01

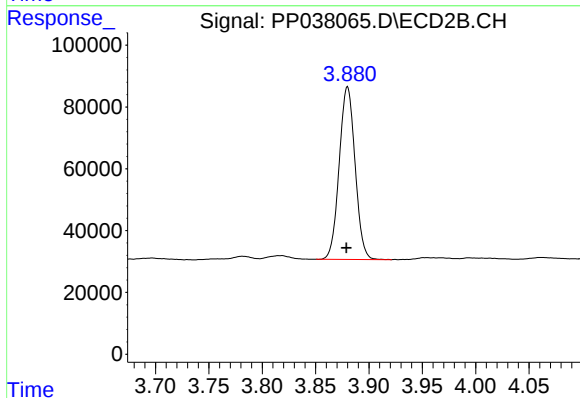


#1 Tetrachloro-m-xylene

R.T.: 3.880 min
Delta R.T.: 0.000 min
Response: 578294
Conc: 22.45 ng/ml

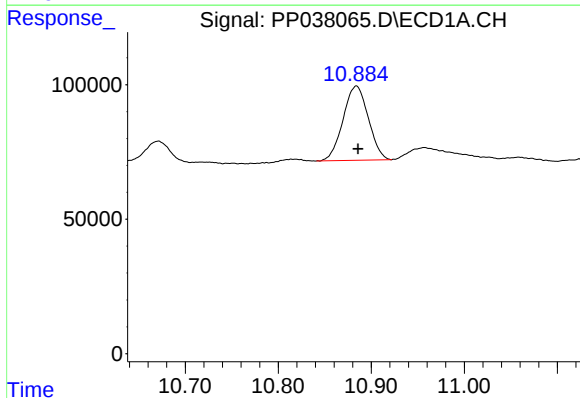

#2 Decachlorobiphenyl

R.T.: 10.884 min
Delta R.T.: -0.002 min
Response: 520515
Conc: 22.88 ng/ml

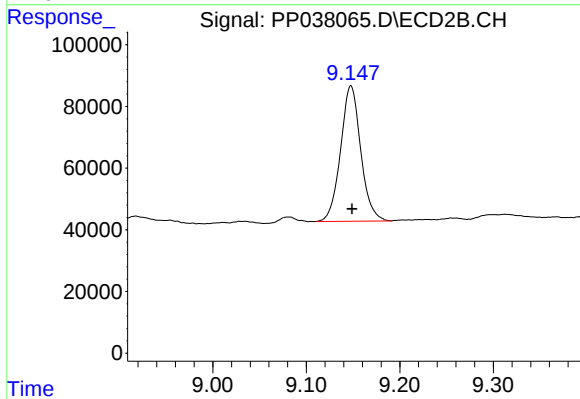

#2 Decachlorobiphenyl

R.T.: 9.148 min
Delta R.T.: -0.001 min
Response: 657141
Conc: 25.40 ng/ml