

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080621\
 Data File : PP038066.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Aug 2021 10:38
 Operator : AJ\MA
 Sample : M3290-26
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 P001-B03-BULK011-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 12:53:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.895	3.882	887014	557194	19.959	21.634
2) SA Decachlor...	10.888	9.150	503433	554438	22.130	21.429

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080621\
Data File : PP038066.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2021 10:38
Operator : AJ\MA
Sample : M3290-26
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
P001-B03-BULK011-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 12:53:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

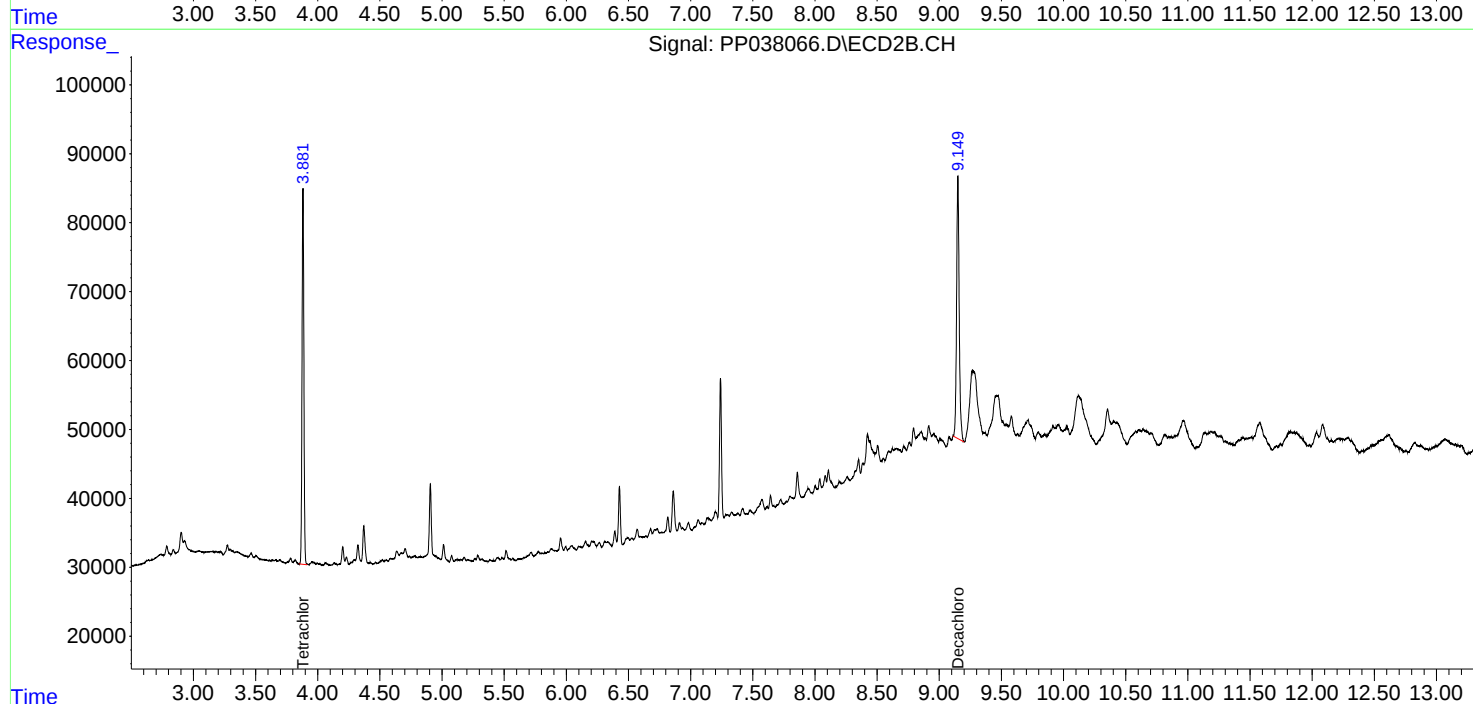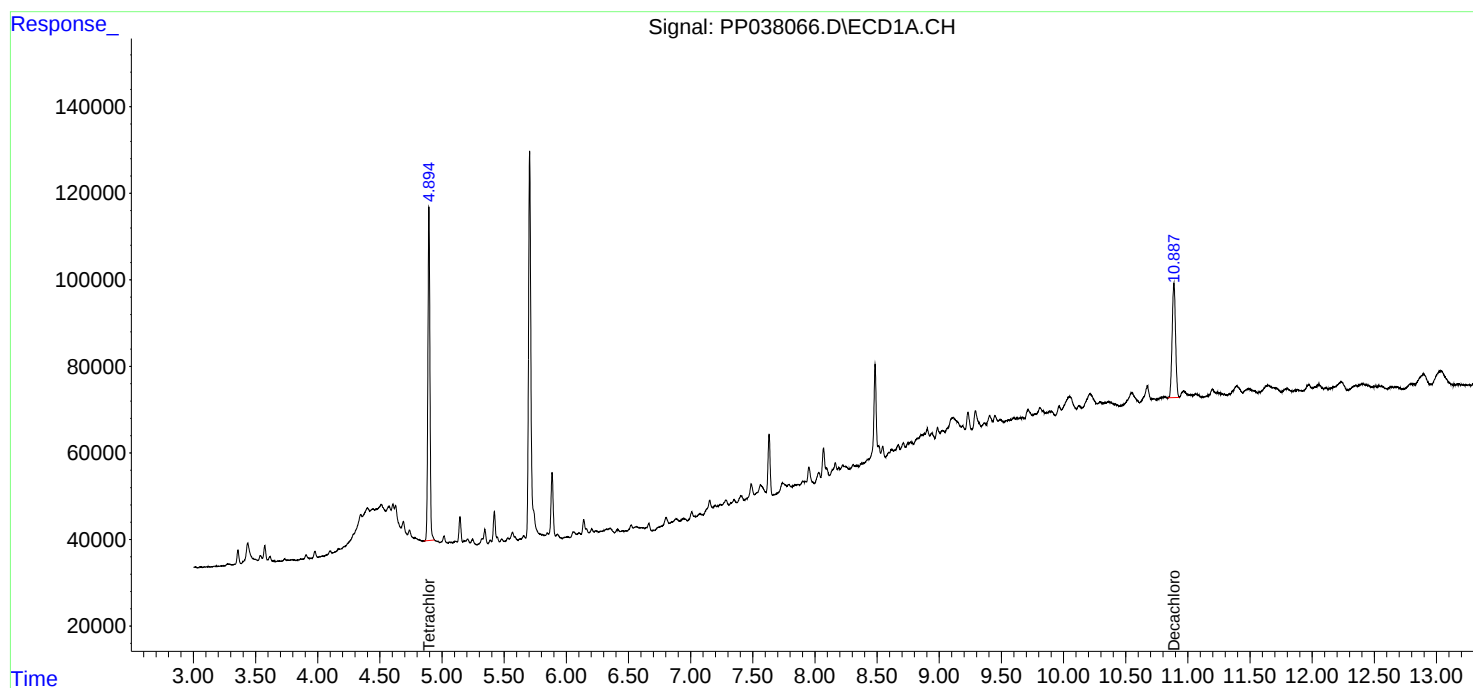


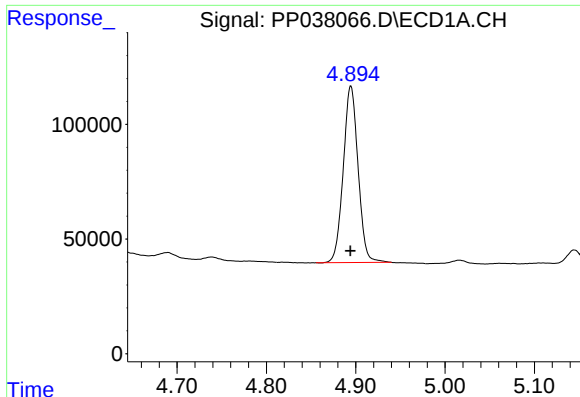

#1 Tetrachloro-m-xylene


R.T.: 4.895 min
Delta R.T.: 0.000 min
Response: 887014
Conc: 19.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
P001-B03-BULK011-02

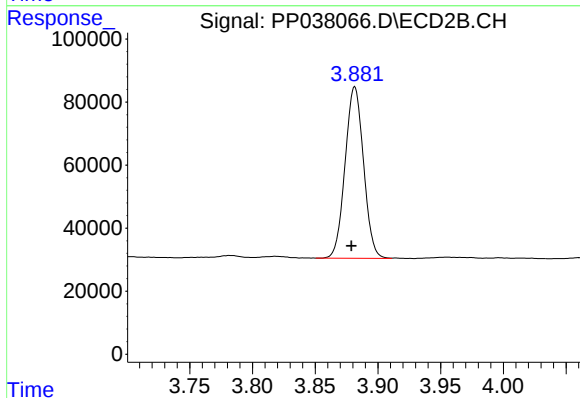


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: 0.003 min
Response: 557194
Conc: 21.63 ng/ml

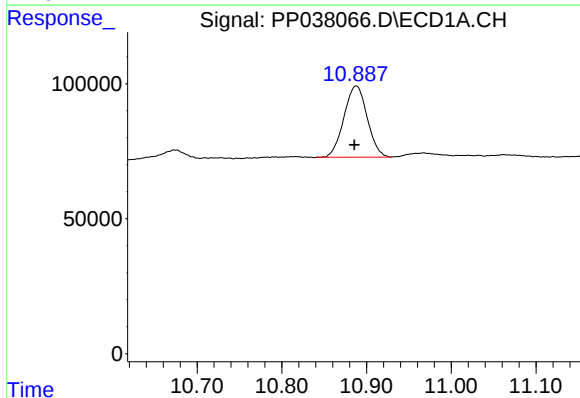

#2 Decachlorobiphenyl

R.T.: 10.888 min
Delta R.T.: 0.002 min
Response: 503433
Conc: 22.13 ng/ml

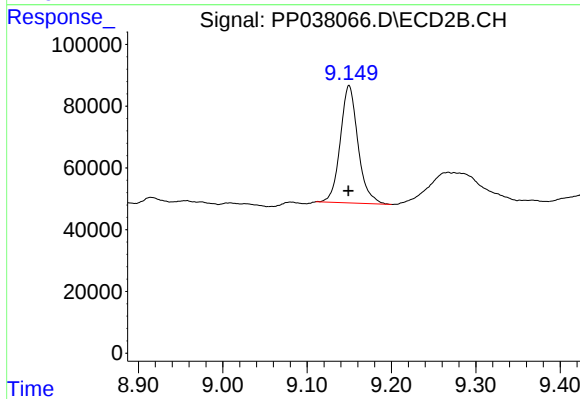

#2 Decachlorobiphenyl

R.T.: 9.150 min
Delta R.T.: 0.000 min
Response: 554438
Conc: 21.43 ng/ml