

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080621\
 Data File : PP038070.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Aug 2021 11:45
 Operator : AJ\MA
 Sample : M3295-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-EF-01-022-ABCD

Manual Integrations
 APPROVED

mohammad
 8/9/2021 4:56:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 12:54:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.895	3.882	994589	644284	22.380m	25.015
2) SA Decachlor...	10.888	9.150	450128	422321	19.787	16.323

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080621\
Data File : PP038070.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2021 11:45
Operator : AJ\MA
Sample : M3295-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
FK-EF-01-022-ABCD


Manual Integrations
APPROVED

mohammad
8/9/2021 4:56:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 12:54:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

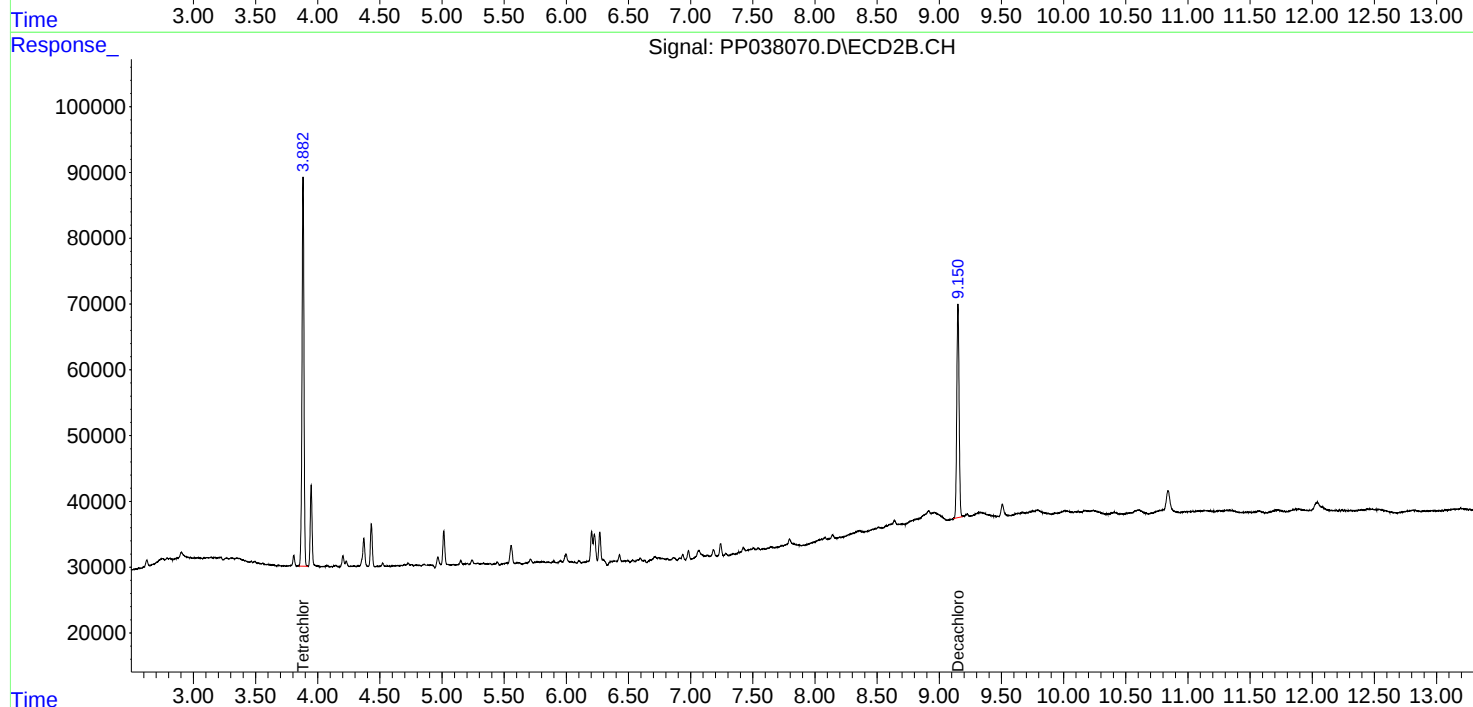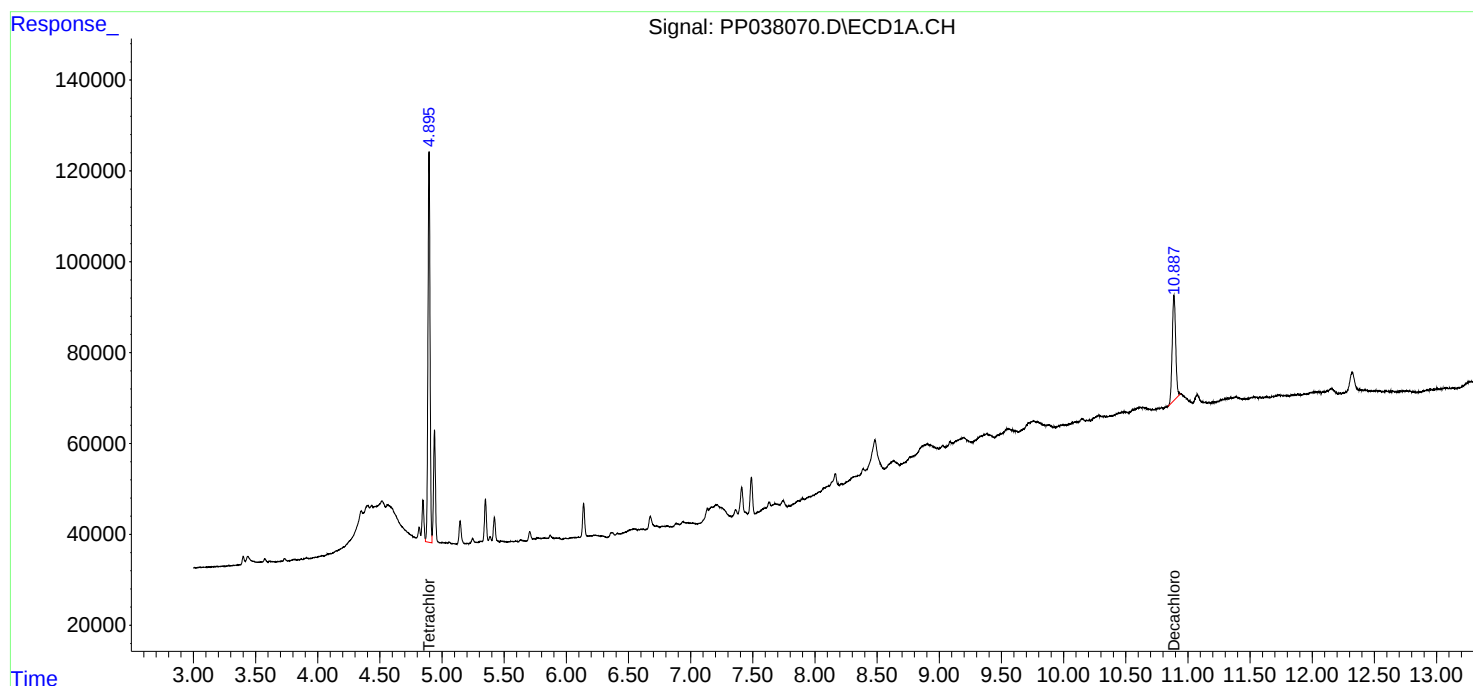

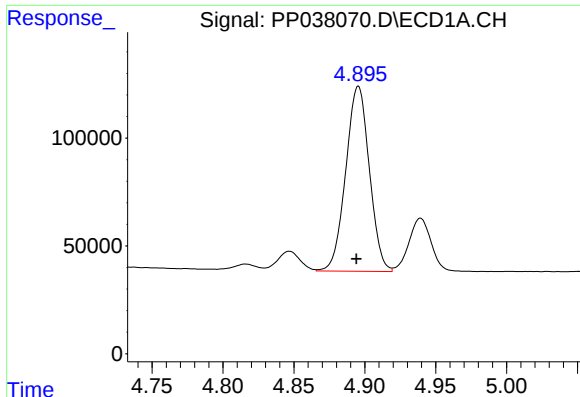


#1 Tetrachloro-m-xylene

R.T.: 4.895 min
Delta R.T.: 0.001 min
Response: 994589
Conc: 22.38 ng/ml m

Instrument :
ECD_P
ClientSampleId :
FK-EF-01-022-ABCD


Manual Integrations
APPROVED

mohammad
8/9/2021 4:56:46 PM

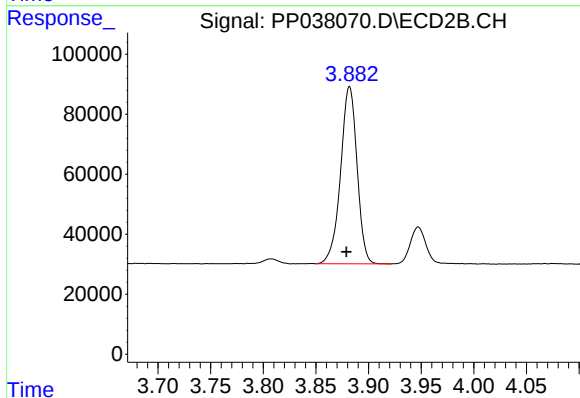


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: 0.003 min
Response: 644284
Conc: 25.02 ng/ml

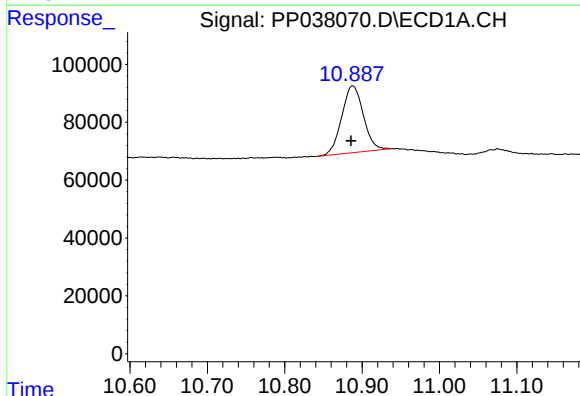

#2 Decachlorobiphenyl

R.T.: 10.888 min
Delta R.T.: 0.002 min
Response: 450128
Conc: 19.79 ng/ml

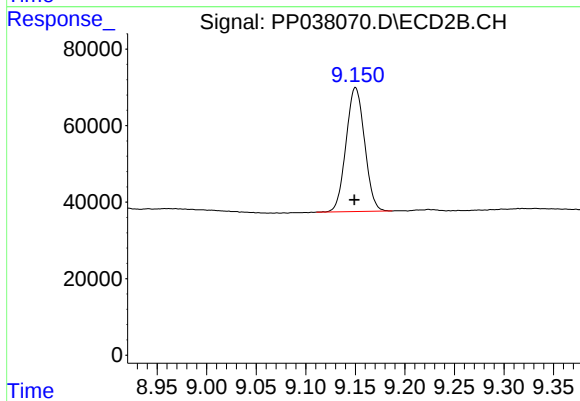

#2 Decachlorobiphenyl

R.T.: 9.150 min
Delta R.T.: 0.001 min
Response: 422321
Conc: 16.32 ng/ml