

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP080621\  
 Data File : PP038071.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 06 Aug 2021 12:02  
 Operator : AJ\MA  
 Sample : M3296-01  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 FK-BPM-03-026-ABCD

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Aug 06 12:55:02 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP080521.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Aug 06 03:08:47 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1  | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|---------|--------|--------|--------|
| -----                       |        |       |         |        |        |        |
| System Monitoring Compounds |        |       |         |        |        |        |
| 1) SA Tetrachlo...          | 4.895  | 3.881 | 1191882 | 722605 | 26.819 | 28.056 |
| 2) SA Decachlor...          | 10.886 | 9.149 | 523079  | 524846 | 22.994 | 20.285 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP080621\  
Data File : PP038071.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 06 Aug 2021 12:02  
Operator : AJ\MA  
Sample : M3296-01  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
FK-BPM-03-026-ABCD

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 06 12:55:02 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP080521.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Aug 06 03:08:47 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

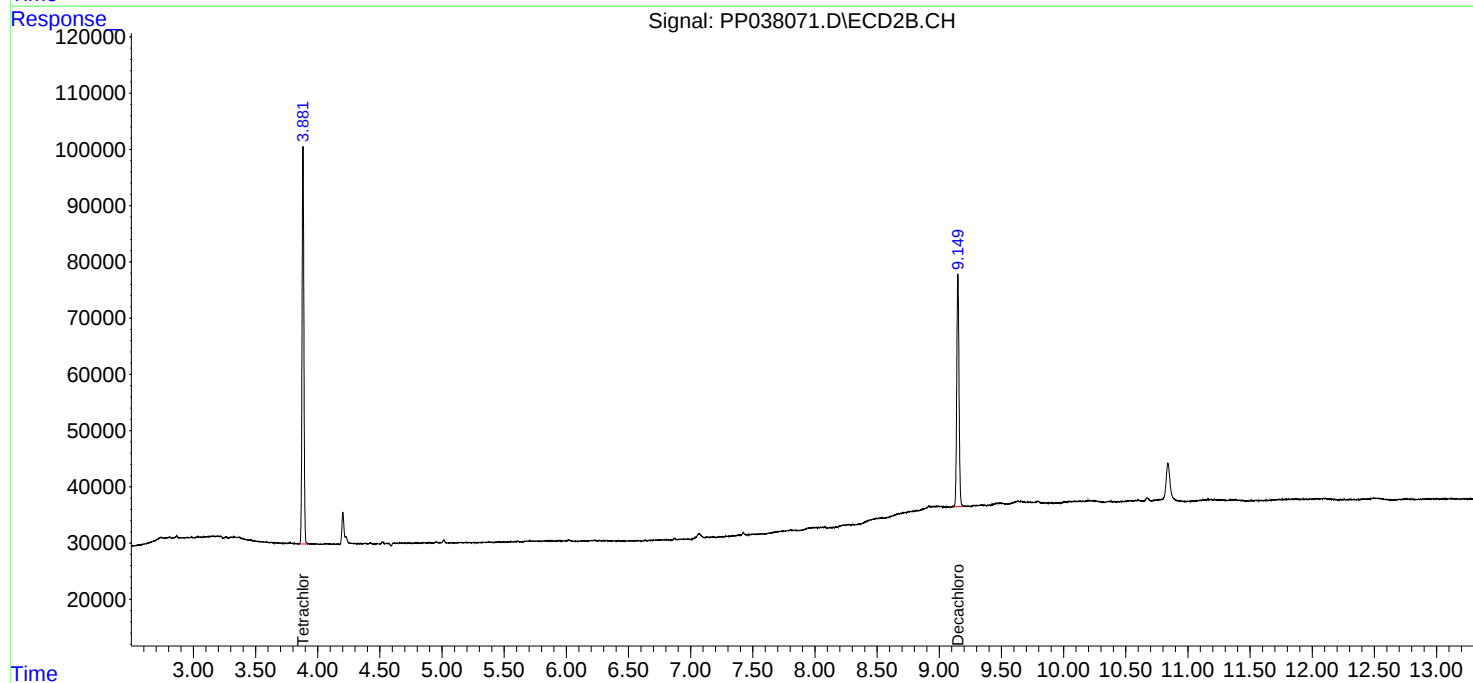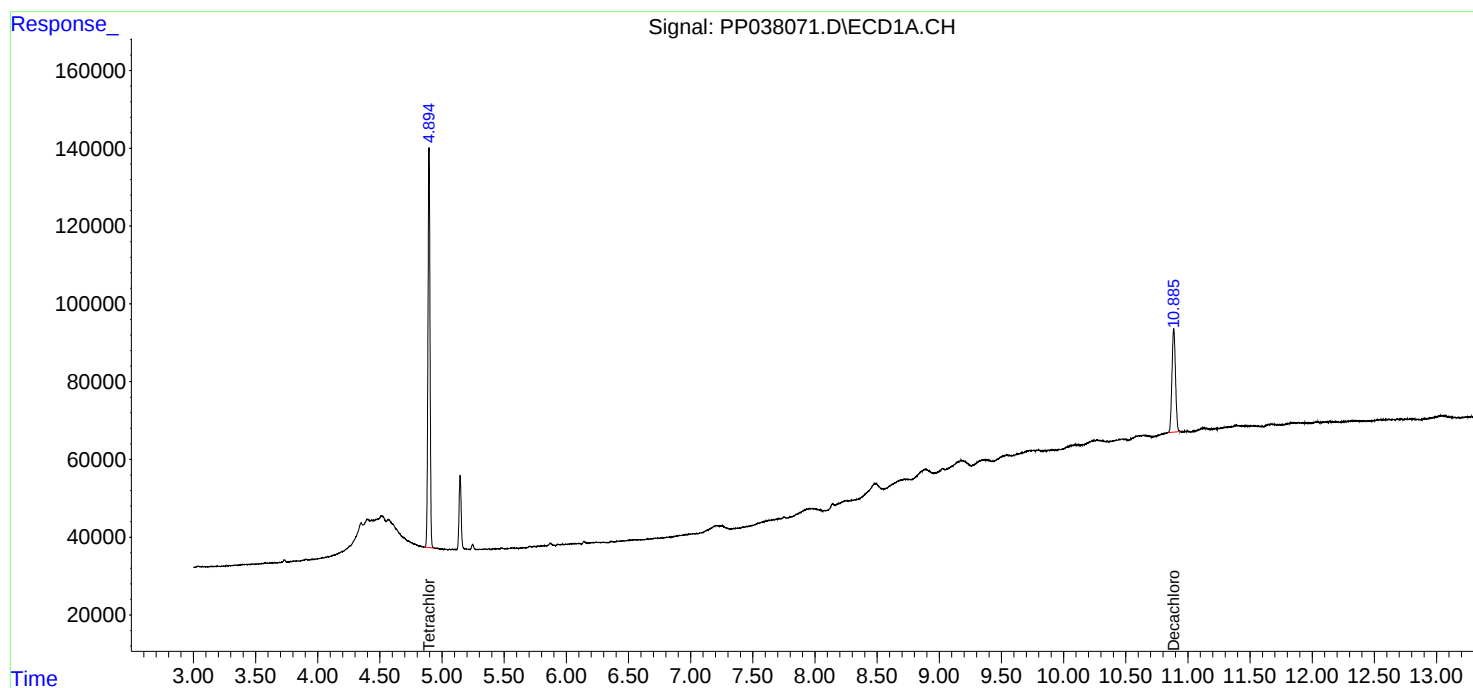


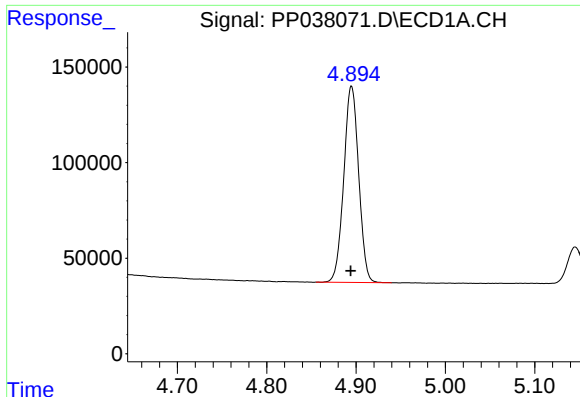

#1 Tetrachloro-m-xylene


R.T.: 4.895 min  
Delta R.T.: 0.000 min  
Response: 1191882  
Conc: 26.82 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
FK-BPM-03-026-ABCD

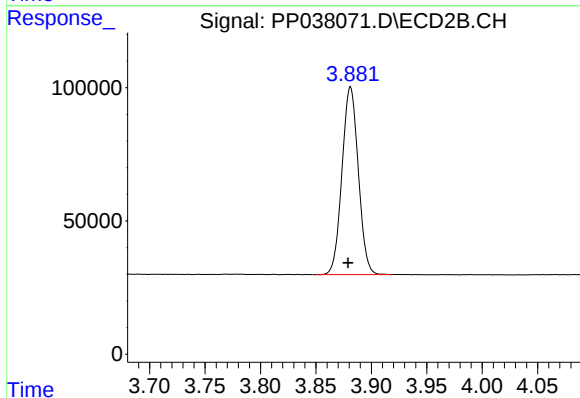


#1 Tetrachloro-m-xylene

R.T.: 3.881 min  
Delta R.T.: 0.002 min  
Response: 722605  
Conc: 28.06 ng/ml

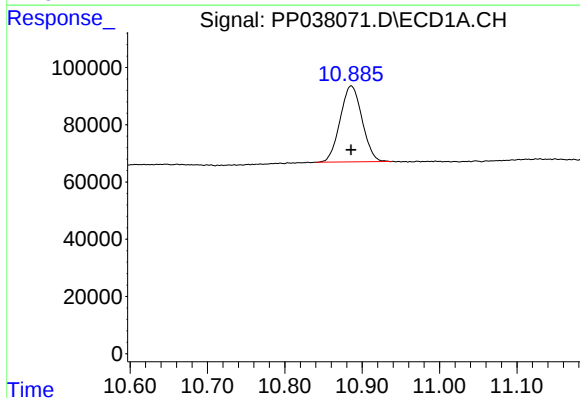

#2 Decachlorobiphenyl

R.T.: 10.886 min  
Delta R.T.: 0.000 min  
Response: 523079  
Conc: 22.99 ng/ml

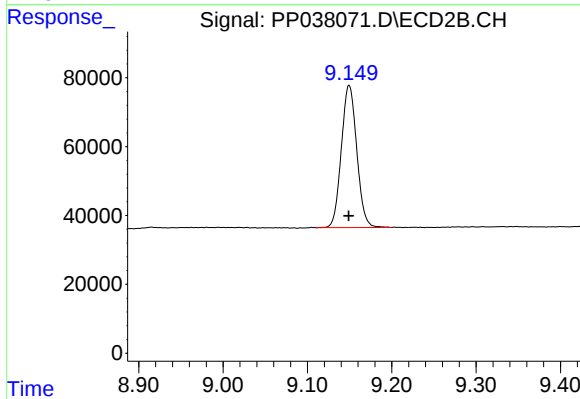

#2 Decachlorobiphenyl

R.T.: 9.149 min  
Delta R.T.: 0.000 min  
Response: 524846  
Conc: 20.29 ng/ml