

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080621\
 Data File : PP038072.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Aug 2021 12:19
 Operator : AJ\MA
 Sample : M3296-01MS
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-BPM-03-026-ABCDMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 12:55:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.894	3.881	955755	554418	21.506	21.526
2) SA Decachlor...	10.884	9.148	390189	393638	17.152	15.214
Target Compounds						
3) L1 AR-1016-1	6.212	5.126	626791	452596	422.055	468.577
4) L1 AR-1016-2	6.236	5.145	882276	632911	414.269	472.429
5) L1 AR-1016-3	6.301	5.335	549530	349663	413.523	475.263
6) L1 AR-1016-4	6.409	5.389	447372	262784	412.050	462.612
7) L1 AR-1016-5	6.723	5.615	402977	339816	401.840	442.855
31) L7 AR-1260-1	7.899	6.709	581803	560792	405.387	430.714
32) L7 AR-1260-2	8.165	6.909	705277	652651	409.652	419.461
33) L7 AR-1260-3	8.530	7.061	411893	616938	344.789	405.291
34) L7 AR-1260-4	8.761	7.544	495073	425861	347.590	348.099
35) L7 AR-1260-5	9.085	7.793	950078	980777	357.836	335.834



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080621\
Data File : PP038072.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2021 12:19
Operator : AJ\MA
Sample : M3296-01MS
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-026-ABCDMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 12:55:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

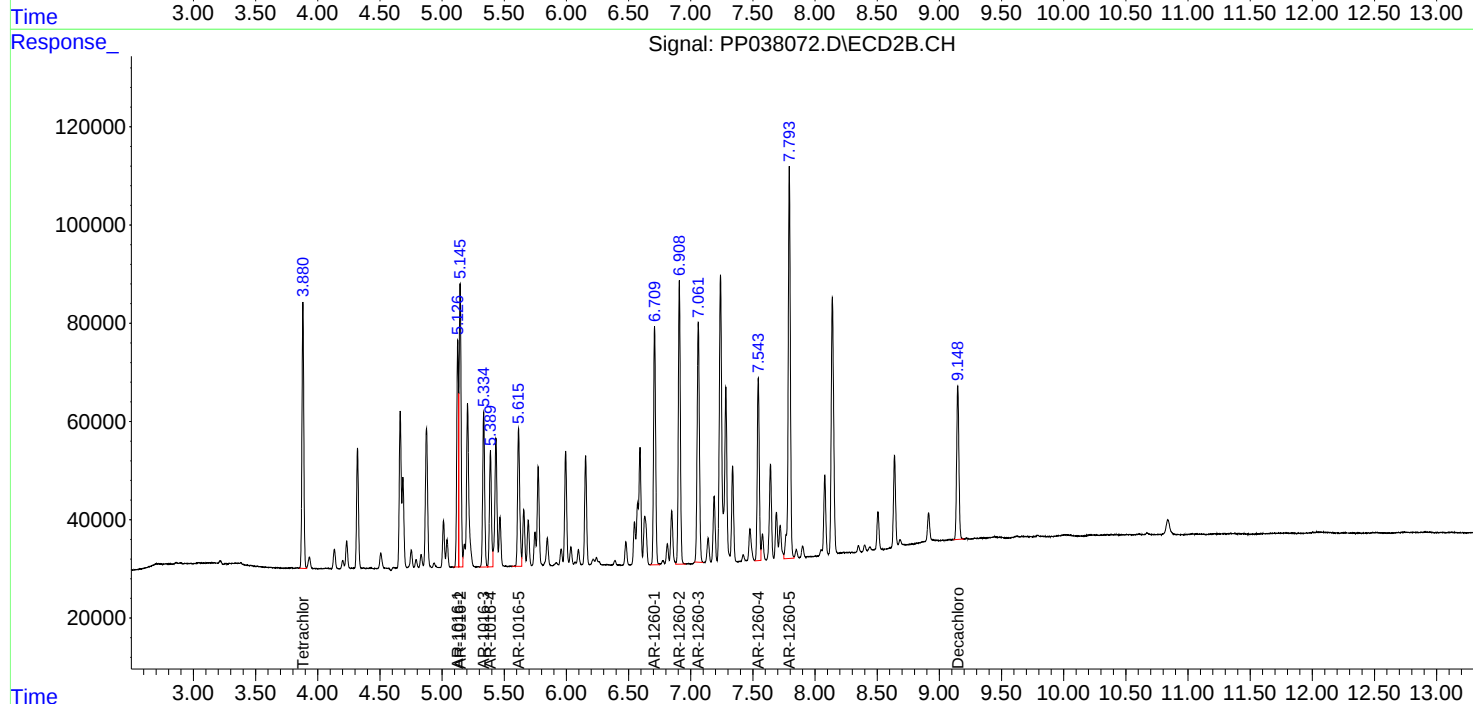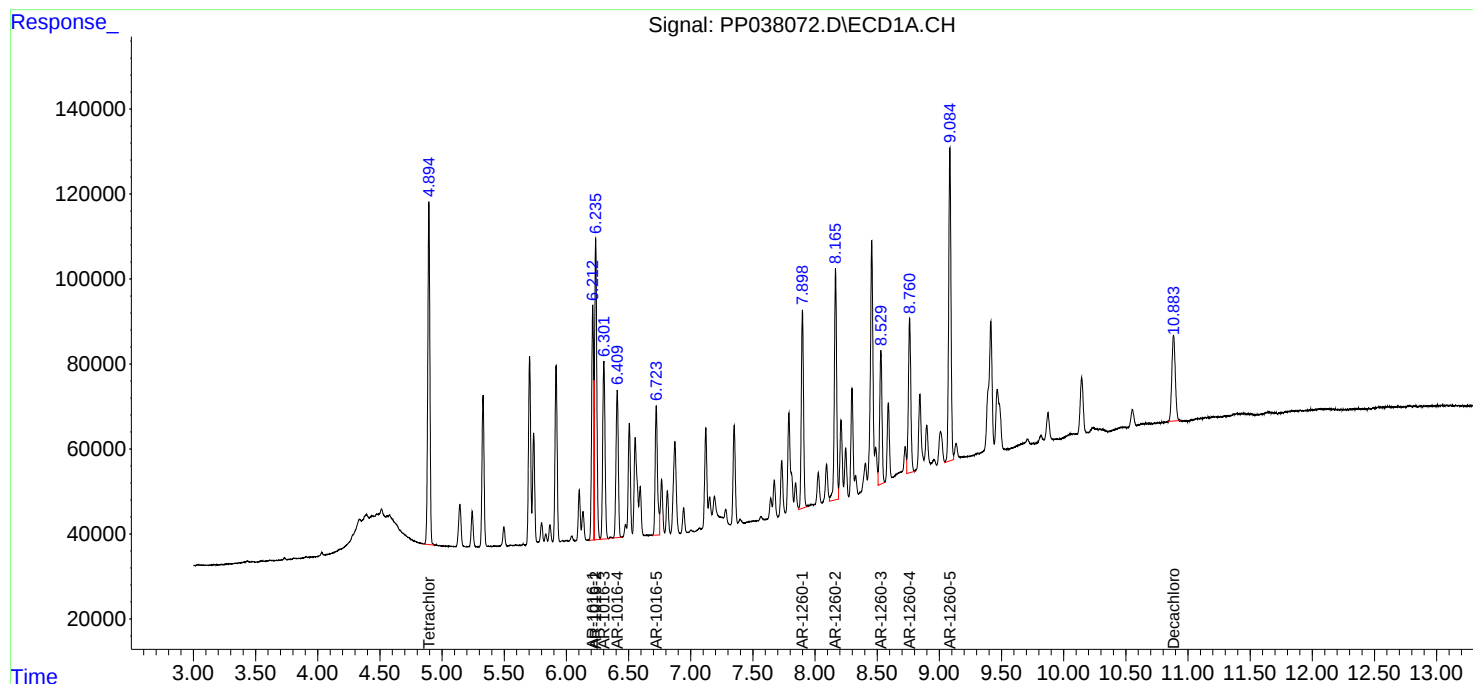


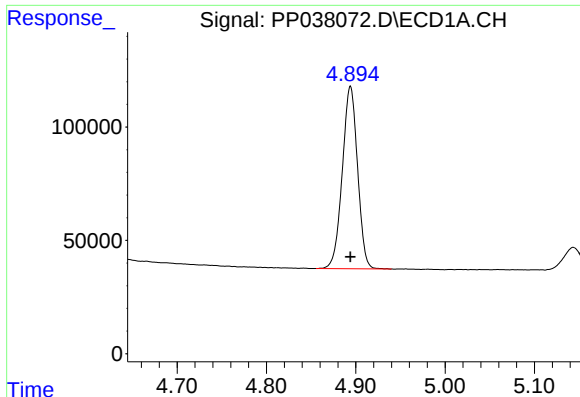

#1 Tetrachloro-m-xylene


R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 955755
Conc: 21.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-026-ABCDMS

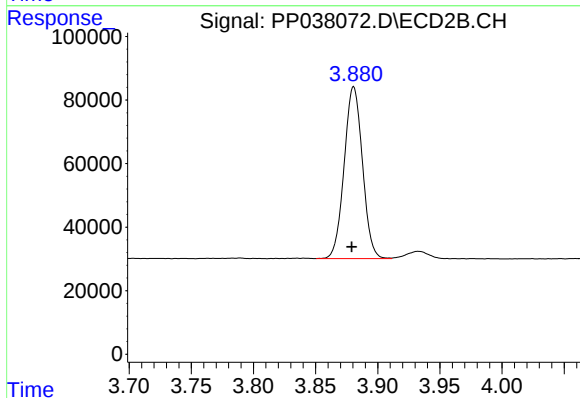


#1 Tetrachloro-m-xylene

R.T.: 3.881 min
Delta R.T.: 0.002 min
Response: 554418
Conc: 21.53 ng/ml

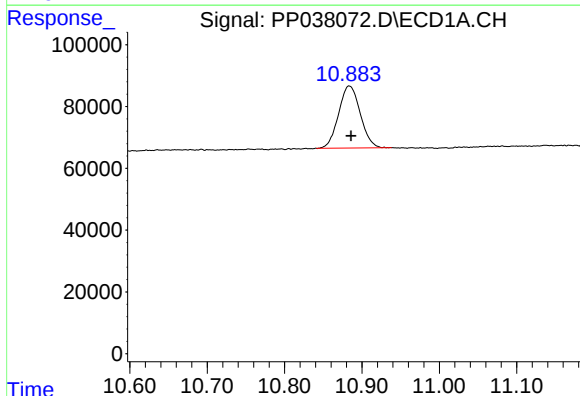


#2 Decachlorobiphenyl

R.T.: 10.884 min
Delta R.T.: -0.002 min
Response: 390189
Conc: 17.15 ng/ml

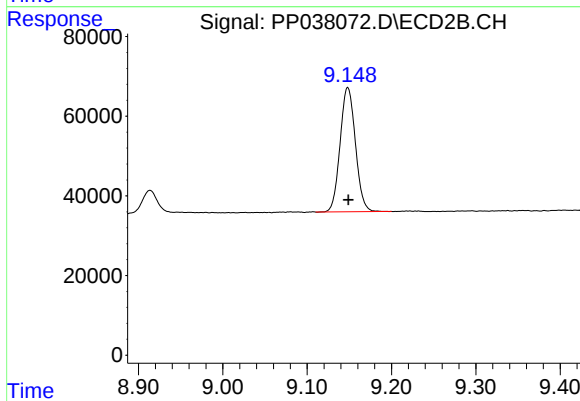

#2 Decachlorobiphenyl


R.T.: 9.148 min
Delta R.T.: 0.000 min
Response: 393638
Conc: 15.21 ng/ml

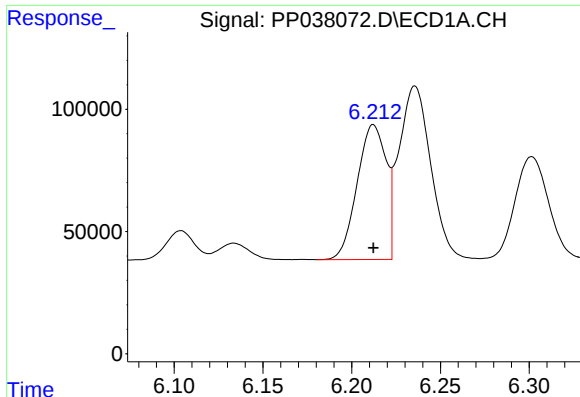

#3 AR-1016-1


R.T.: 6.212 min
Delta R.T.: 0.000 min
Response: 626791
Conc: 422.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-026-ABCDMS

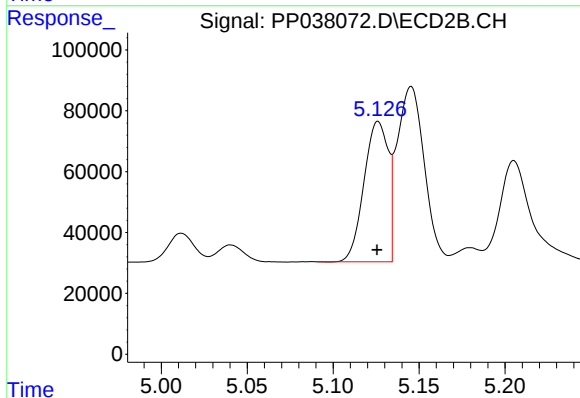


#3 AR-1016-1

R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 452596
Conc: 468.58 ng/ml

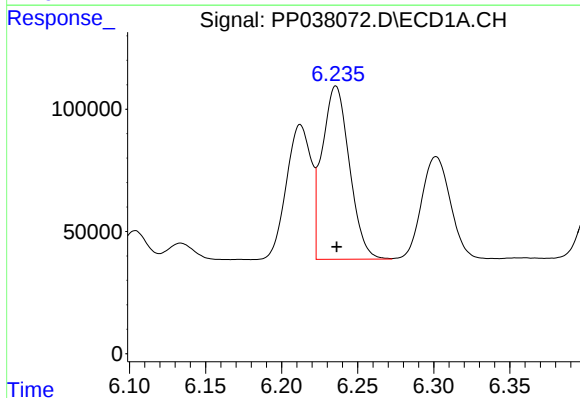


#4 AR-1016-2

R.T.: 6.236 min
Delta R.T.: 0.000 min
Response: 882276
Conc: 414.27 ng/ml

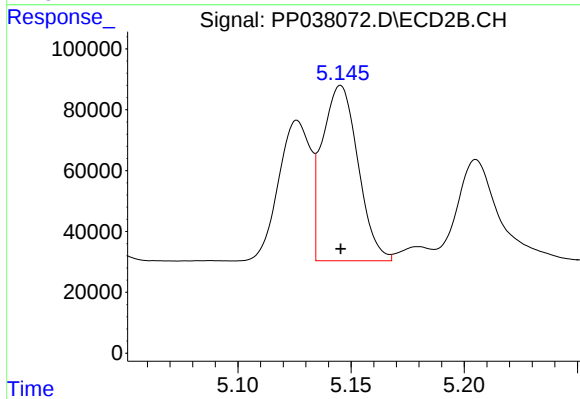

#4 AR-1016-2


R.T.: 5.145 min
Delta R.T.: 0.000 min
Response: 632911
Conc: 472.43 ng/ml

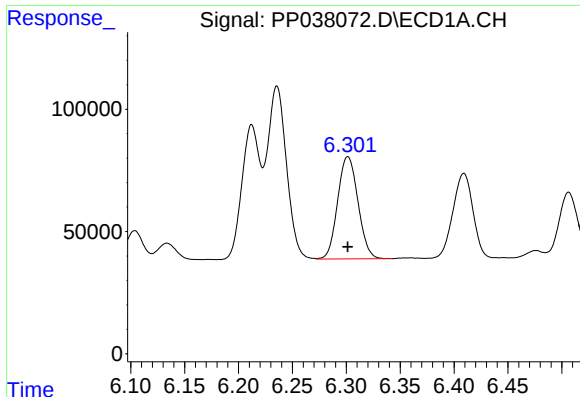

#5 AR-1016-3


R.T.: 6.301 min
Delta R.T.: 0.000 min
Response: 549530
Conc: 413.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-026-ABCDMS

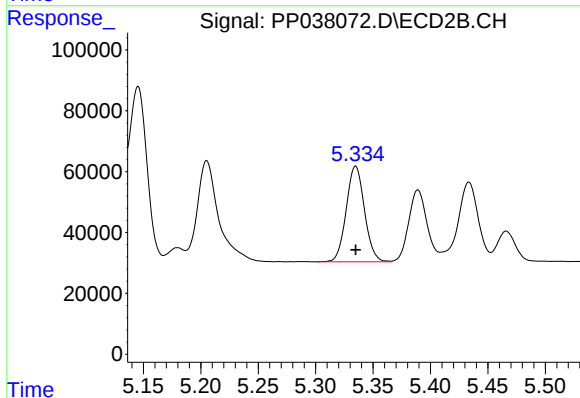


#5 AR-1016-3

R.T.: 5.335 min
Delta R.T.: 0.000 min
Response: 349663
Conc: 475.26 ng/ml

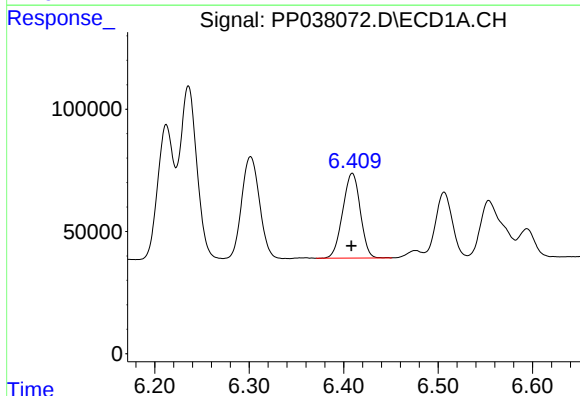


#6 AR-1016-4

R.T.: 6.409 min
Delta R.T.: 0.000 min
Response: 447372
Conc: 412.05 ng/ml

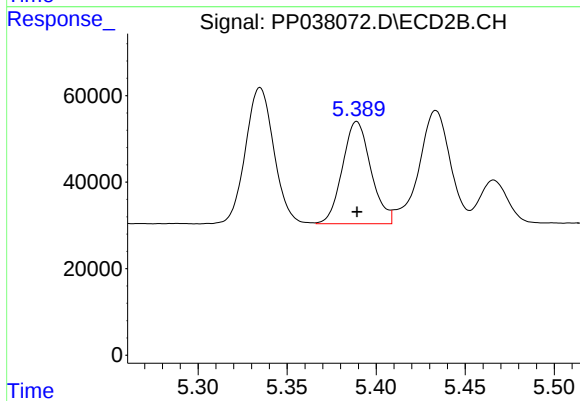

#6 AR-1016-4


R.T.: 5.389 min
Delta R.T.: 0.000 min
Response: 262784
Conc: 462.61 ng/ml

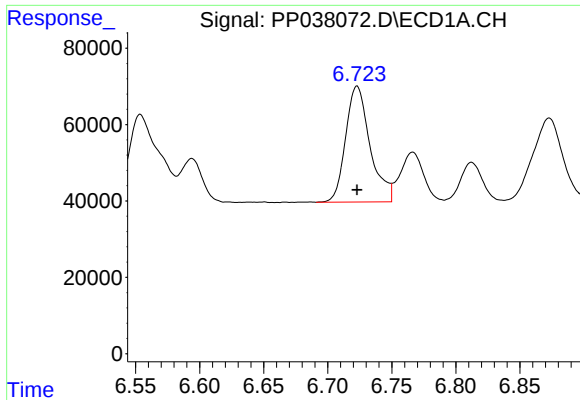

#7 AR-1016-5


R.T.: 6.723 min
Delta R.T.: 0.000 min
Response: 402977
Conc: 401.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-026-ABCDMS

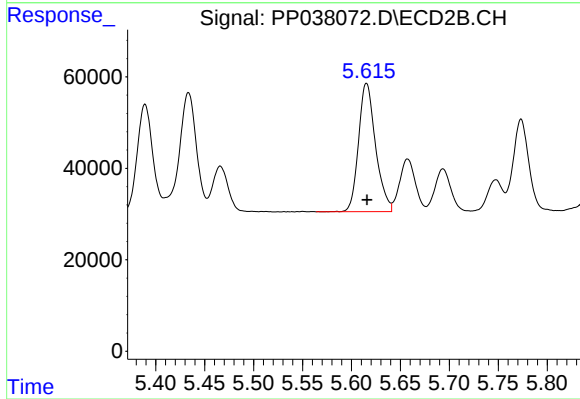


#7 AR-1016-5

R.T.: 5.615 min
Delta R.T.: 0.000 min
Response: 339816
Conc: 442.86 ng/ml

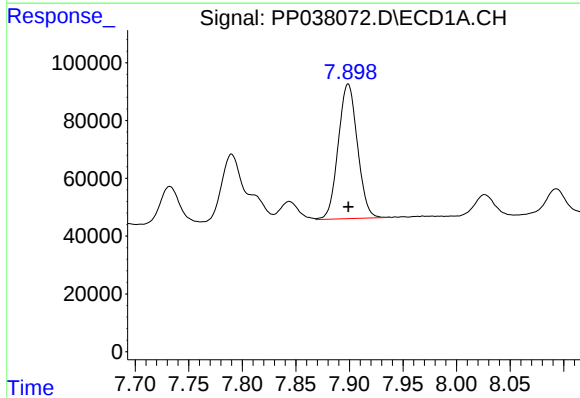


#31 AR-1260-1

R.T.: 7.899 min
Delta R.T.: 0.000 min
Response: 581803
Conc: 405.39 ng/ml

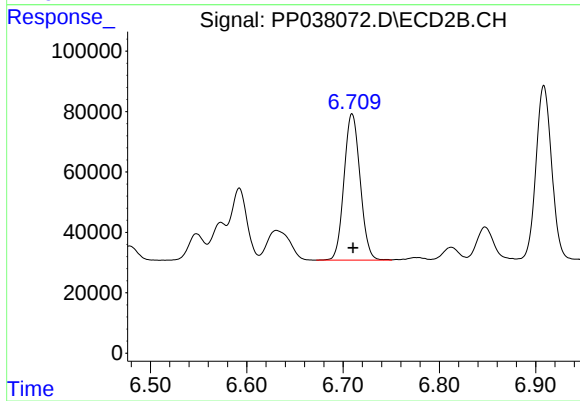

#31 AR-1260-1


R.T.: 6.709 min
Delta R.T.: 0.000 min
Response: 560792
Conc: 430.71 ng/ml

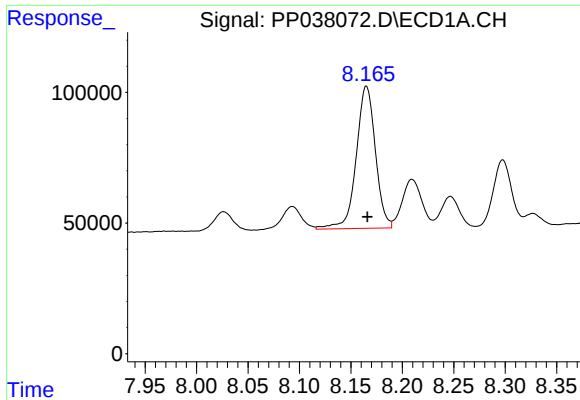

#32 AR-1260-2


R.T.: 8.165 min
Delta R.T.: 0.000 min
Response: 705277
Conc: 409.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-026-ABCDMS

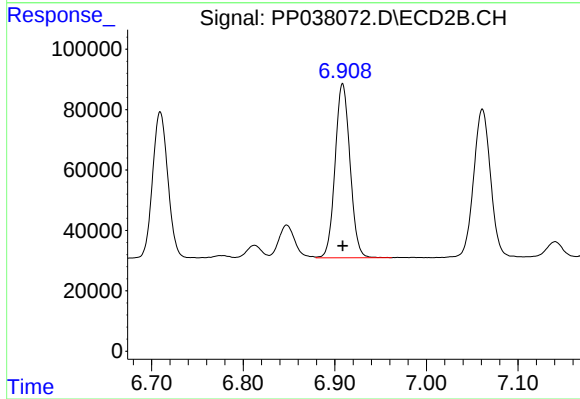


#32 AR-1260-2

R.T.: 6.909 min
Delta R.T.: 0.000 min
Response: 652651
Conc: 419.46 ng/ml

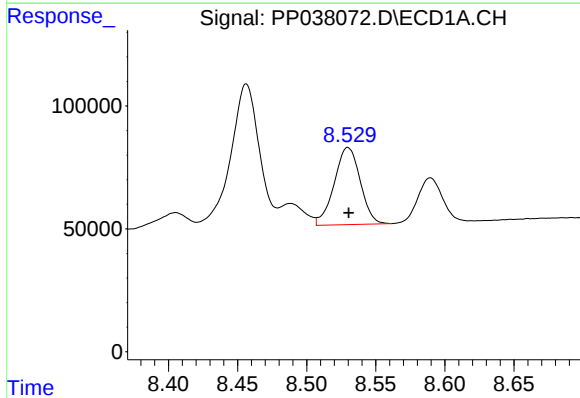


#33 AR-1260-3

R.T.: 8.530 min
Delta R.T.: 0.000 min
Response: 411893
Conc: 344.79 ng/ml

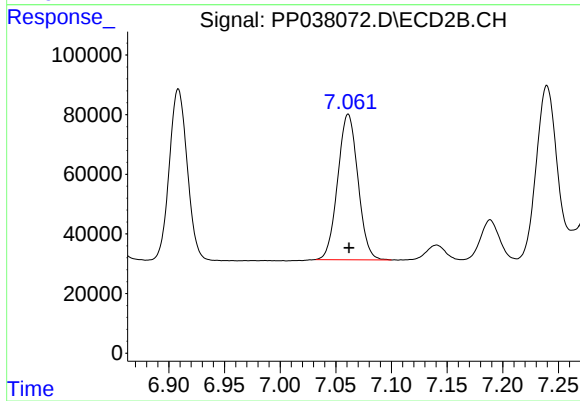

#33 AR-1260-3


R.T.: 7.061 min
Delta R.T.: 0.000 min
Response: 616938
Conc: 405.29 ng/ml

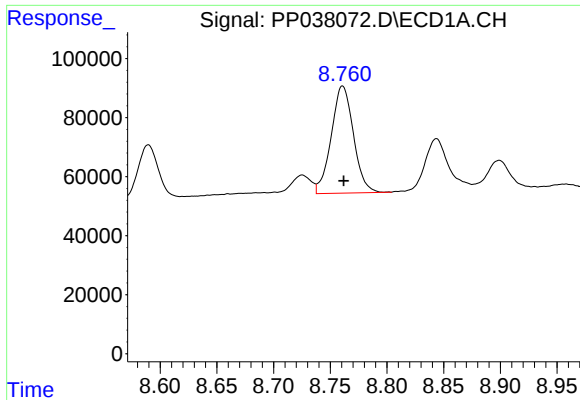

#34 AR-1260-4


R.T.: 8.761 min
Delta R.T.: 0.000 min
Response: 495073
Conc: 347.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-03-026-ABCDMS

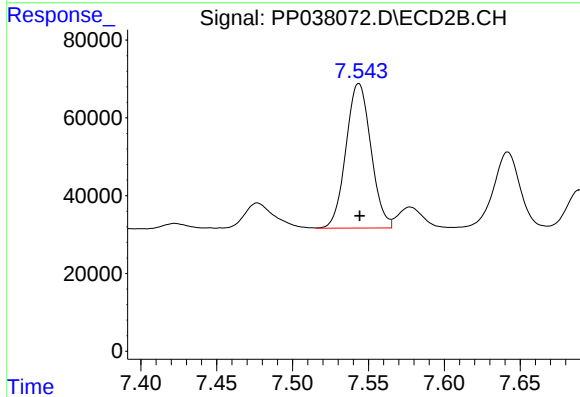


#34 AR-1260-4

R.T.: 7.544 min
Delta R.T.: 0.000 min
Response: 425861
Conc: 348.10 ng/ml

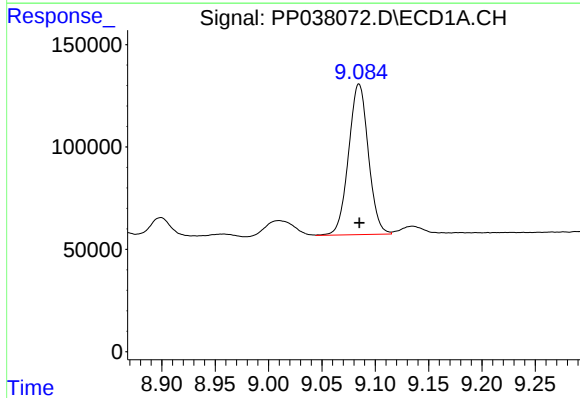

#35 AR-1260-5

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 950078
Conc: 357.84 ng/ml

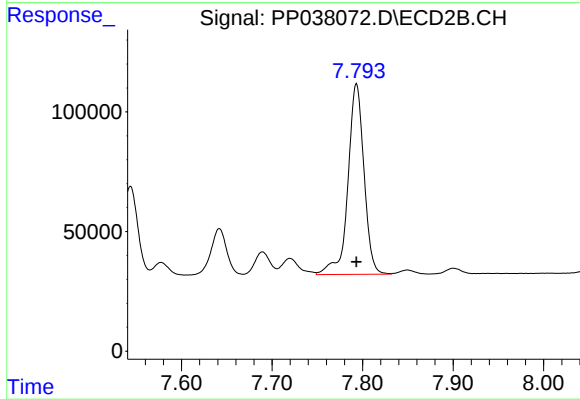

#35 AR-1260-5

R.T.: 7.793 min
Delta R.T.: 0.000 min
Response: 980777
Conc: 335.83 ng/ml