

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080621\
 Data File : PP038089.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Aug 2021 18:42
 Operator : AJ\MA
 Sample : M3299-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20210562-COM-35

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 02:02:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.896	3.883	484074	311434	10.892	12.092
2)	SA Decachlor...	10.888	9.151	222117	226765	9.764	8.765

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080621\
Data File : PP038089.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2021 18:42
Operator : AJ\MA
Sample : M3299-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20210562-COM-35

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 02:02:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

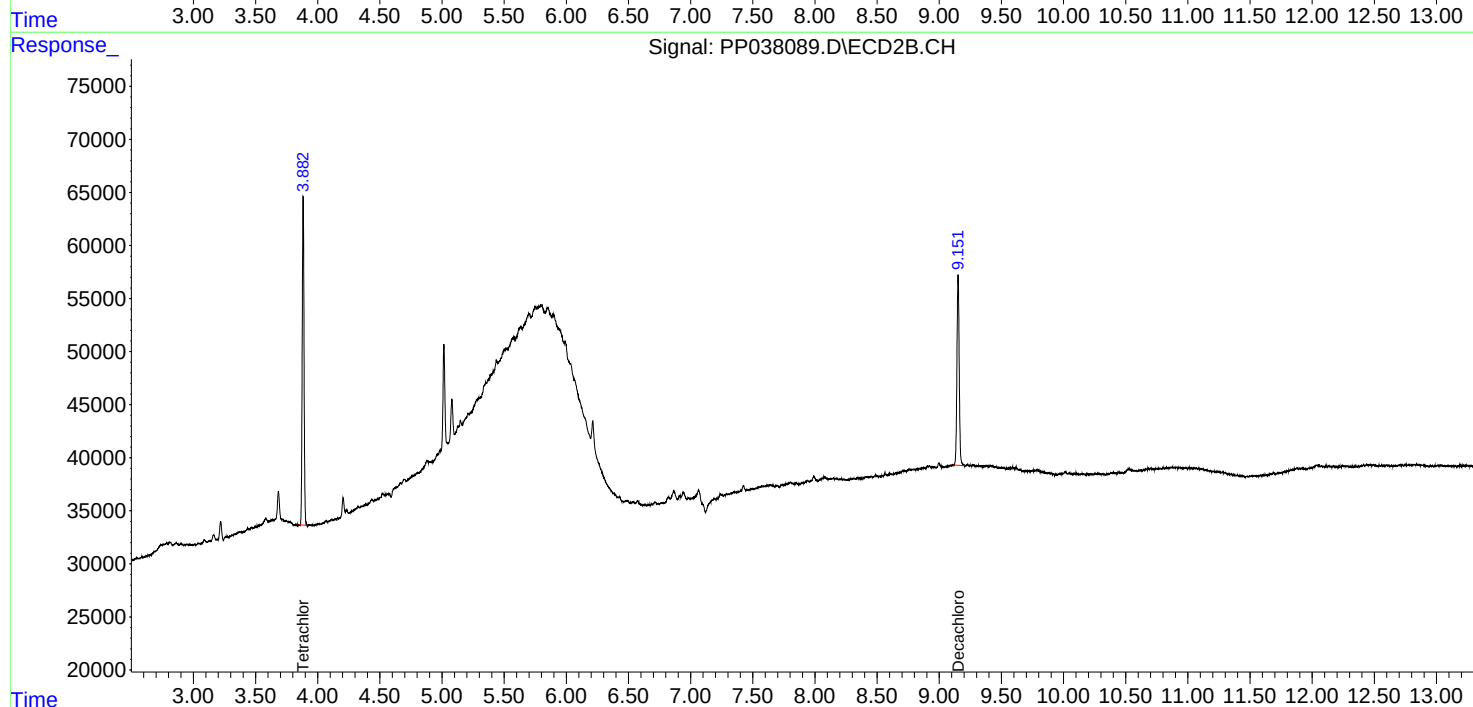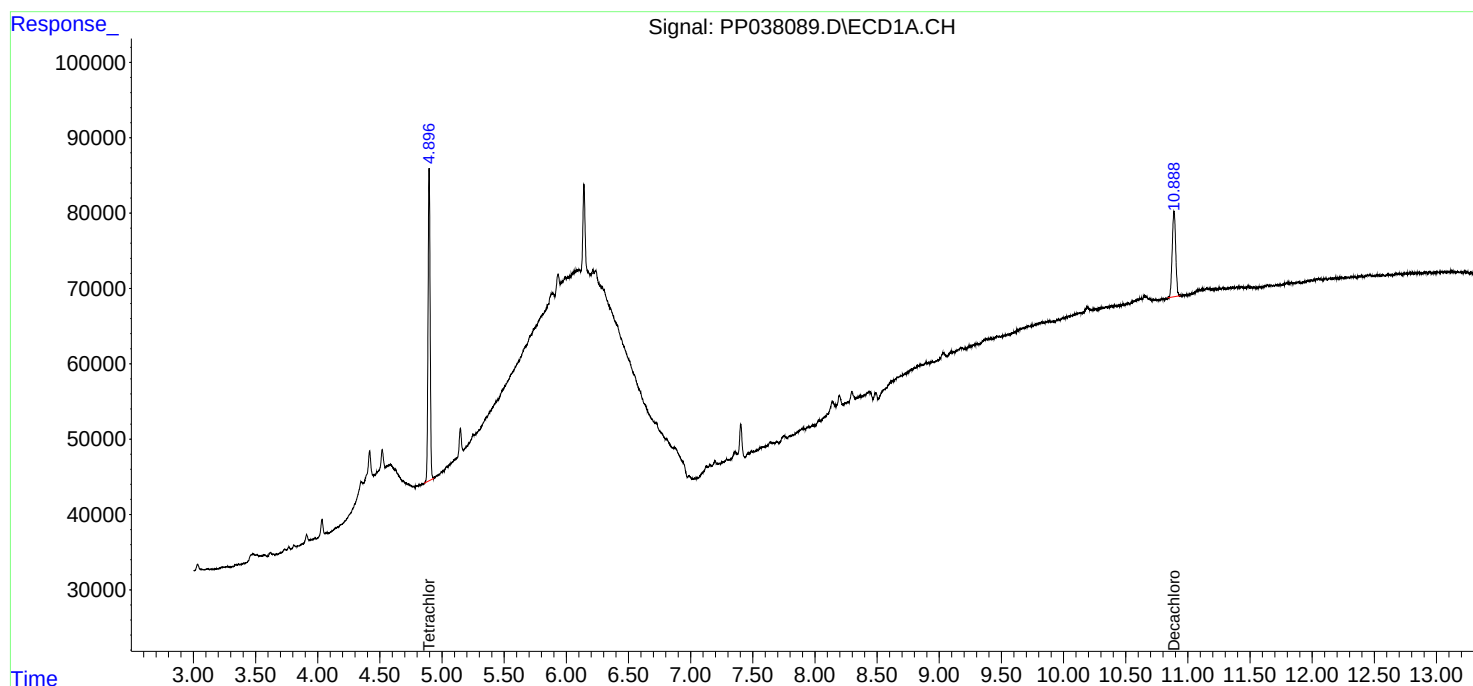


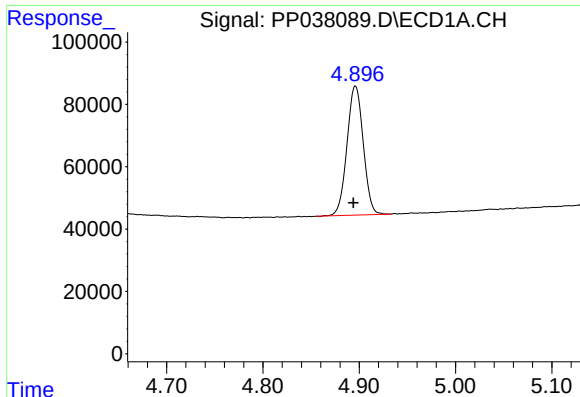

#1 Tetrachloro-m-xylene


R.T.: 4.896 min
Delta R.T.: 0.002 min
Response: 484074
Conc: 10.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
20210562-COM-35

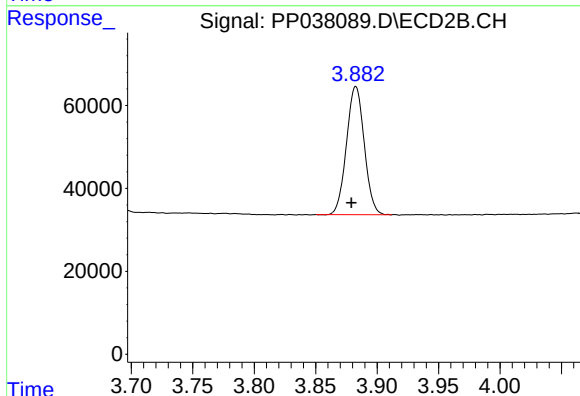


#1 Tetrachloro-m-xylene

R.T.: 3.883 min
Delta R.T.: 0.004 min
Response: 311434
Conc: 12.09 ng/ml

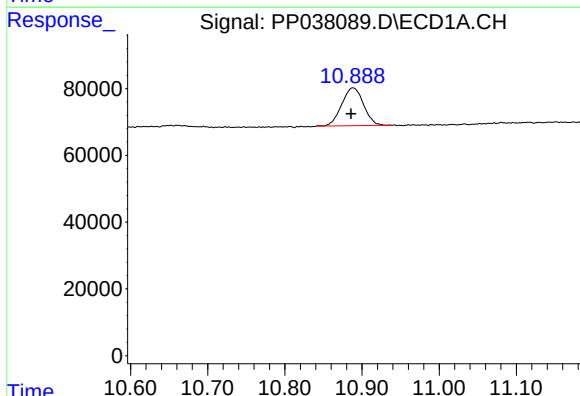

#2 Decachlorobiphenyl

R.T.: 10.888 min
Delta R.T.: 0.002 min
Response: 222117
Conc: 9.76 ng/ml

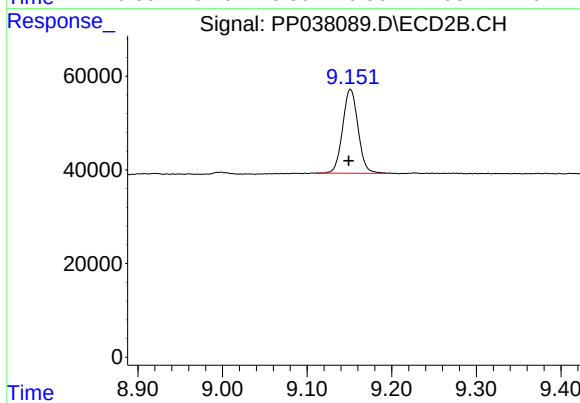

#2 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: 0.002 min
Response: 226765
Conc: 8.76 ng/ml