

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080624\
 Data File : PP066592.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2024 10:18
 Operator : YP\AJ
 Sample : P3390-07
 Misc : AR1660 LOD 25 PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 13:57:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 06 04:00:13 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.778	4.017	32258685	35649390	17.058	16.928
2)	SA Decachlor...	10.791	9.202	39407018	25082618	18.861	18.869
Target Compounds							
3)	L1 AR-1016-1	5.960	5.131	1794724	1355402	24.169	22.013
4)	L1 AR-1016-2	5.984	5.151	2637887	1771102	23.911	20.372
5)	L1 AR-1016-3	6.046	5.333	1677004	968925	25.026	21.276
6)	L1 AR-1016-4	6.146	5.371	1214800	731480	22.001	20.552
7)	L1 AR-1016-5	6.442	5.591	1277120	897096	23.340	19.954
9)	L2 AR-1221-2	5.088	0.000	575483	0	31.545	N.D. #
10)	L2 AR-1221-3	5.152	4.401	840550	859950	15.107	14.964
11)	L3 AR-1232-1	5.152	4.401	840550	859950	18.643	18.344
12)	L3 AR-1232-2	5.689	5.151	1337045	1771102	50.186	43.042
13)	L3 AR-1232-3	5.984	5.333	2637887	968925	52.533	43.566
14)	L3 AR-1232-4	6.146	5.415	1214800	787872	45.211	41.084
15)	L3 AR-1232-5	6.235	5.591	1192522	897096	60.371	44.697 #
16)	L4 AR-1242-1	5.960	5.131	1794724	1355402	30.193	27.352
17)	L4 AR-1242-2	5.984	5.151	2637887	1771102	29.836	25.456
18)	L4 AR-1242-3	6.046	5.333	1677004	968925	31.039	26.308
19)	L4 AR-1242-4	6.146	5.415	1214800	787872	27.302	22.080
20)	L4 AR-1242-5	6.890	5.949	636640	818688	12.499	19.398 #
21)	L5 AR-1248-1	5.960	5.131	1794724	1355402	37.124	33.904
22)	L5 AR-1248-2	6.235	5.371	1192522	731480	16.824	13.812
23)	L5 AR-1248-3	6.442	5.415	1277120	787872	16.526	14.382
24)	L5 AR-1248-4	6.848	5.591	474294	897096	5.335	14.296 #
25)	L5 AR-1248-5	6.890	0.000	636640	0	7.207	N.D. #
26)	L6 AR-1254-1	6.823	5.949	1514322	818688	16.869	9.603 #
27)	L6 AR-1254-2	7.041	6.096	1544123	669236	11.424	8.960
28)	L6 AR-1254-3	7.413	6.523	531477	1395472	3.976	11.962 #
29)	L6 AR-1254-4	7.703	0.000	647742	0	6.300	N.D. #
30)	L6 AR-1254-5	8.119	7.161	4420136	2345216	40.563	21.758 #
31)	L7 AR-1260-1	7.577	6.641	2972094	1934471	27.994	23.785
32)	L7 AR-1260-2	7.832	6.827	4480478	2499240	35.087	25.518 #
33)	L7 AR-1260-3	8.198	6.989	2989140	4115448	33.300	38.982
34)	L7 AR-1260-4	8.442	7.463	2643119	1786495	27.762	24.125
35)	L7 AR-1260-5	8.788	7.703	5096576	4040304	26.835	23.694
36)	L8 AR-1262-1	8.260	7.252	1521277	1017901	24.314	20.099
37)	L8 AR-1262-2	8.788	7.463	5096576	1786495	20.830	16.724
38)	L8 AR-1262-3	9.145f	7.990	2946311	893431	16.408	10.234 #
39)	L8 AR-1262-4	9.222	8.056	967195	2929584	6.575	18.881 #
40)	L8 AR-1262-5	9.950	8.585	1389440	895240	14.766	13.632
41)	L9 AR-1268-1	9.145f	7.990	2946311	893431	9.851	3.854 #
42)	L9 AR-1268-2	9.222	8.056	967195	2929584	3.423	13.955 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080624\
 Data File : PP066592.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2024 10:18
 Operator : YP\AJ
 Sample : P3390-07
 Misc : AR1660 LOD 25 PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 13:57:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 06 04:00:13 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	9.950	8.585	1389440	895240	14.570	13.370
45) L9	AR-1268-5	10.413f	0.000	856176	0	1.114	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080624\
Data File : PP066592.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2024 10:18
Operator : YP\AJ
Sample : P3390-07
Misc : AR1660 LOD 25 PPB
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 13:57:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 06 04:00:13 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

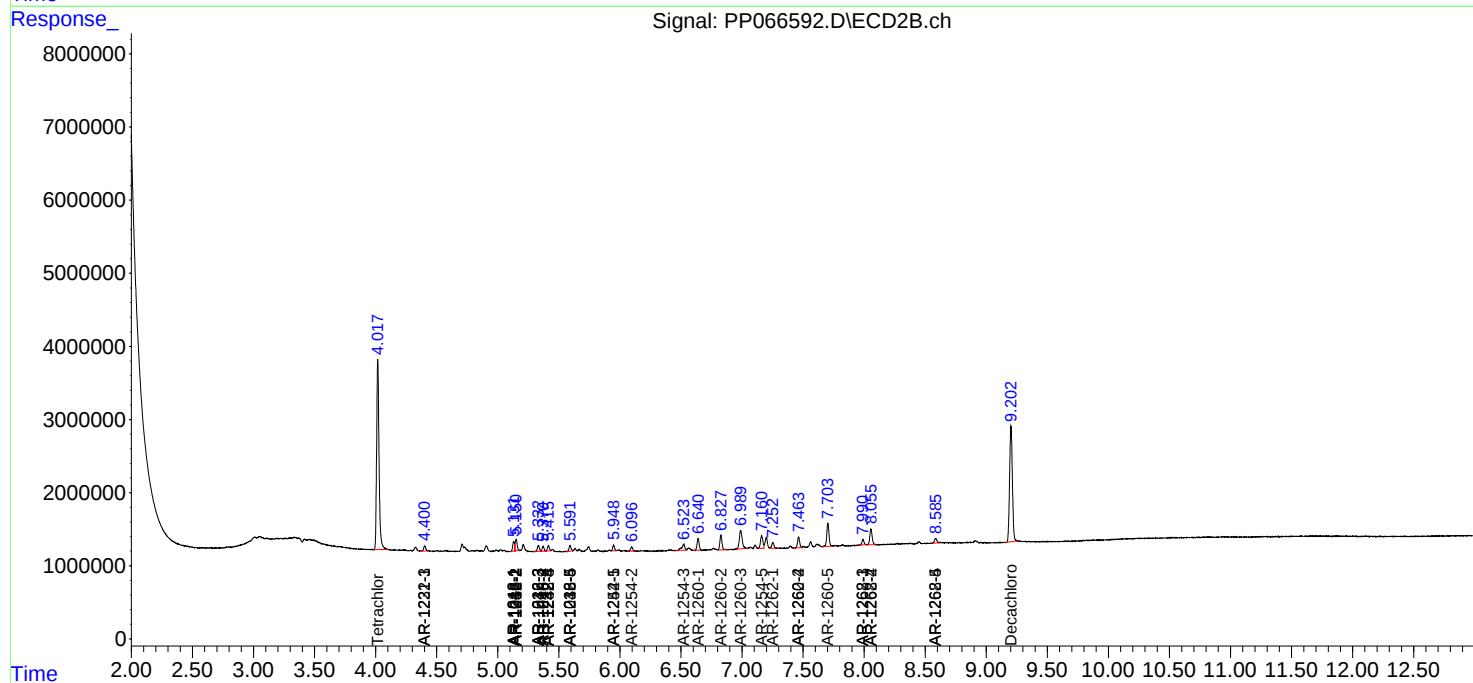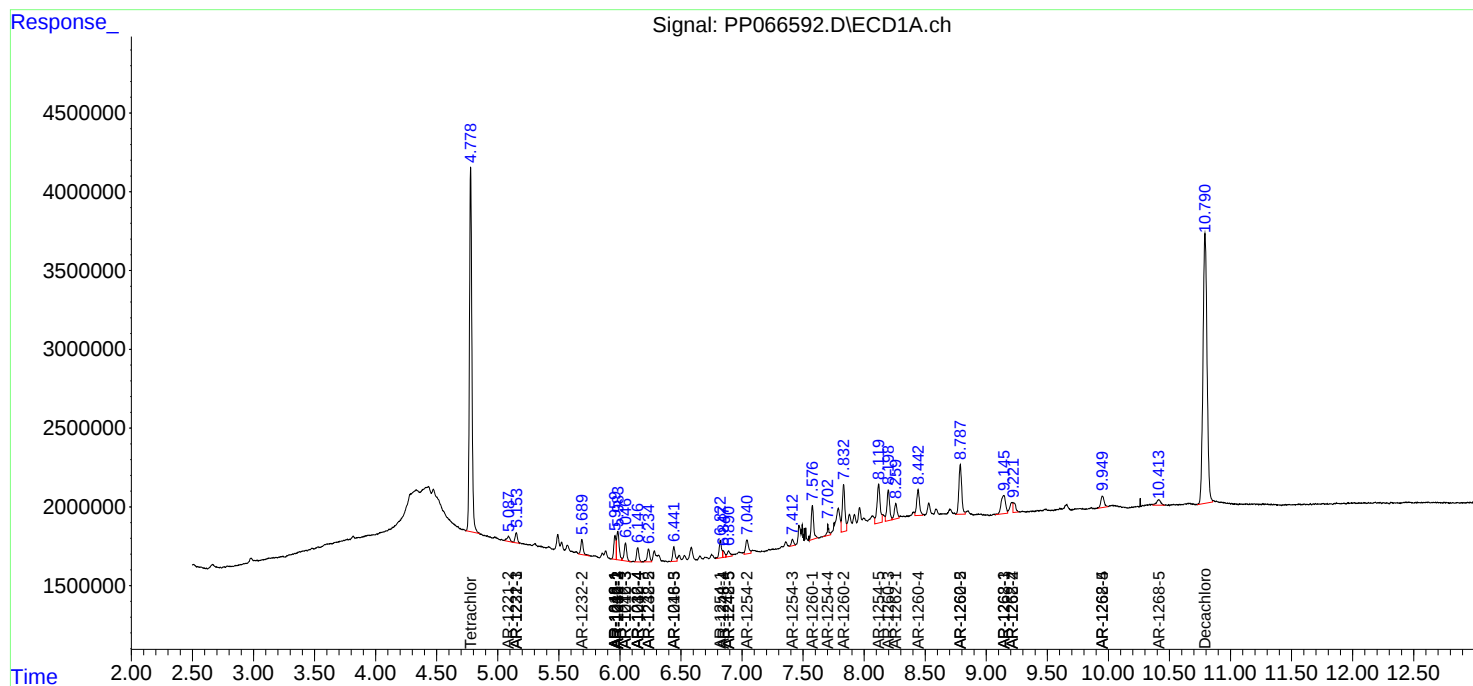


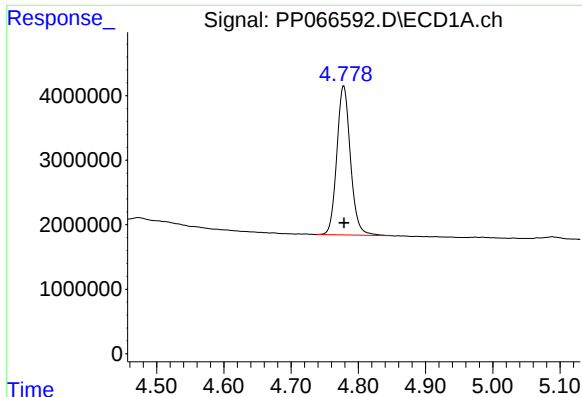

#1 Tetrachloro-m-xylene


R.T.: 4.778 min
Delta R.T.: 0.000 min
Response: 32258685
Conc: 17.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

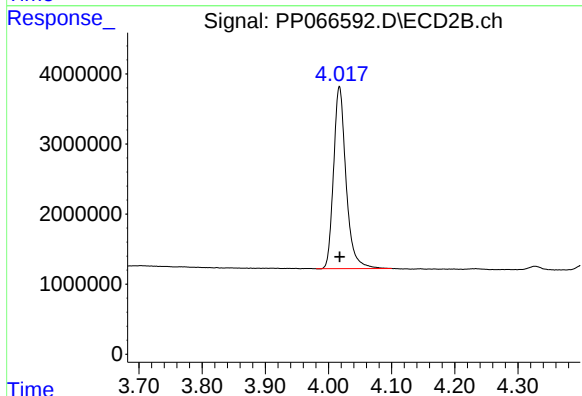


#1 Tetrachloro-m-xylene

R.T.: 4.017 min
Delta R.T.: 0.000 min
Response: 35649390
Conc: 16.93 ng/ml

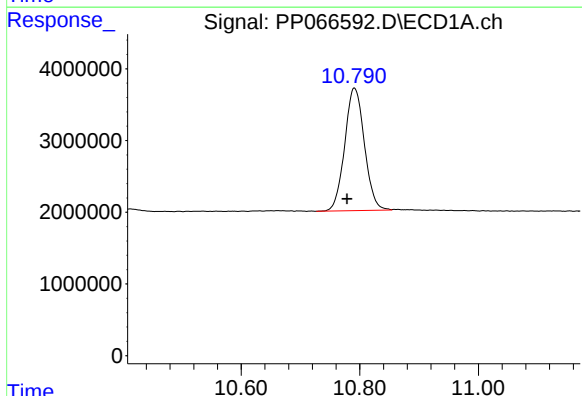


#2 Decachlorobiphenyl

R.T.: 10.791 min
Delta R.T.: 0.013 min
Response: 39407018
Conc: 18.86 ng/ml

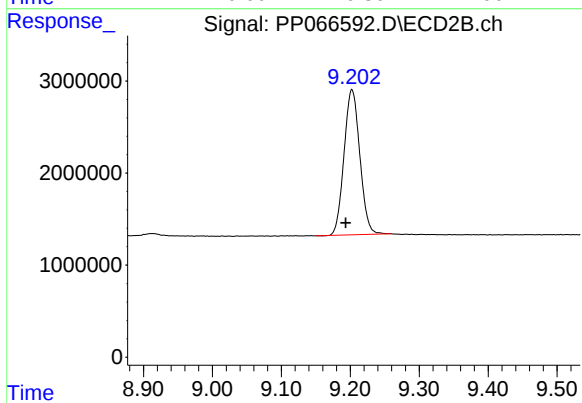

#2 Decachlorobiphenyl


R.T.: 9.202 min
Delta R.T.: 0.009 min
Response: 25082618
Conc: 18.87 ng/ml

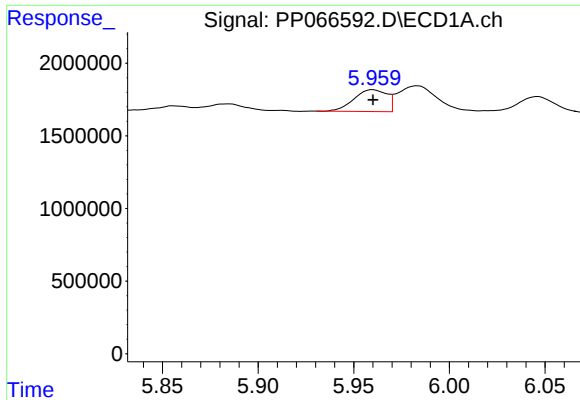

#3 AR-1016-1


R.T.: 5.960 min
Delta R.T.: 0.000 min
Response: 1794724
Conc: 24.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

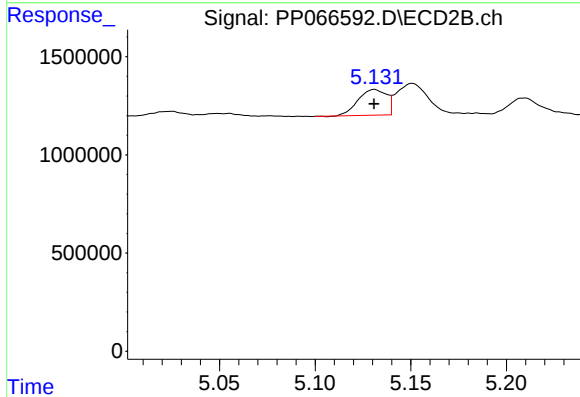


#3 AR-1016-1

R.T.: 5.131 min
Delta R.T.: 0.000 min
Response: 1355402
Conc: 22.01 ng/ml

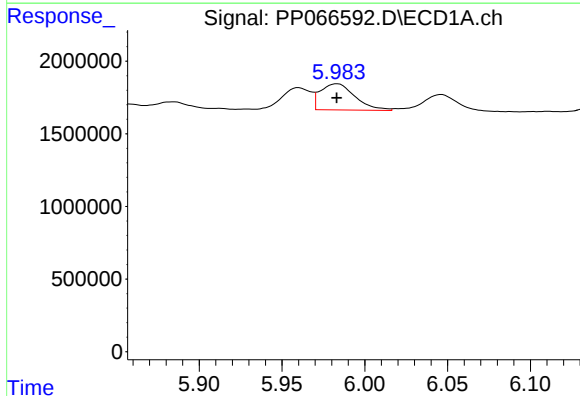


#4 AR-1016-2

R.T.: 5.984 min
Delta R.T.: 0.000 min
Response: 2637887
Conc: 23.91 ng/ml

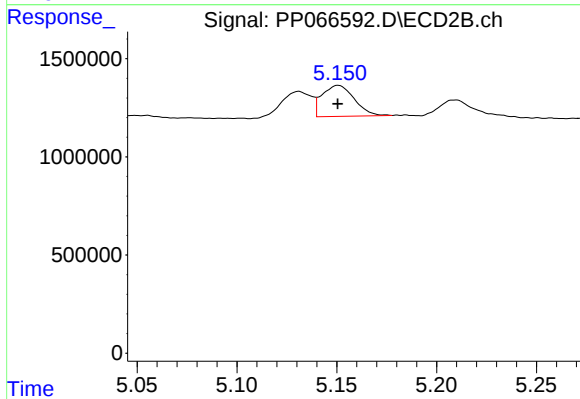

#4 AR-1016-2


R.T.: 5.151 min
Delta R.T.: 0.000 min
Response: 1771102
Conc: 20.37 ng/ml

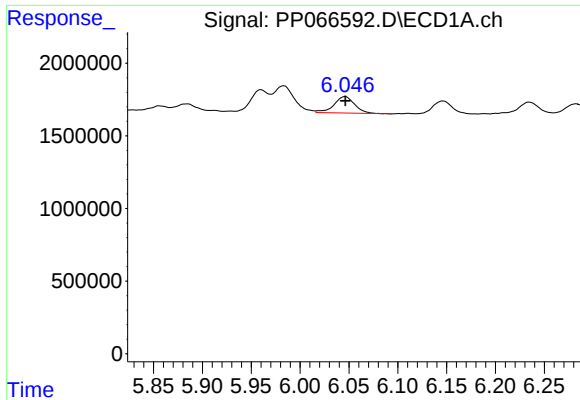

#5 AR-1016-3


R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 1677004
Conc: 25.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

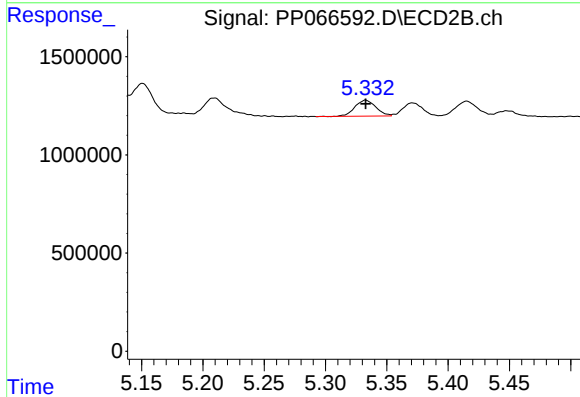


#5 AR-1016-3

R.T.: 5.333 min
Delta R.T.: 0.000 min
Response: 968925
Conc: 21.28 ng/ml

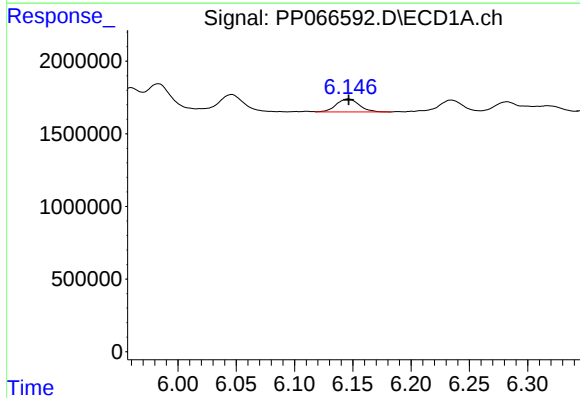


#6 AR-1016-4

R.T.: 6.146 min
Delta R.T.: 0.000 min
Response: 1214800
Conc: 22.00 ng/ml

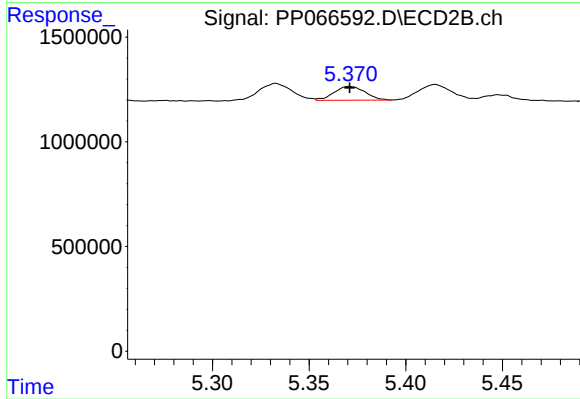

#6 AR-1016-4


R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 731480
Conc: 20.55 ng/ml

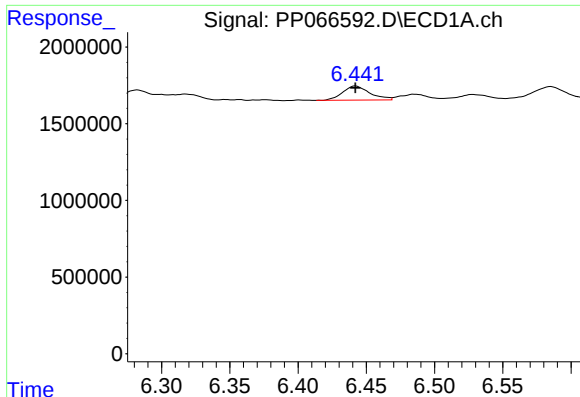

#7 AR-1016-5


R.T.: 6.442 min
Delta R.T.: 0.000 min
Response: 1277120
Conc: 23.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

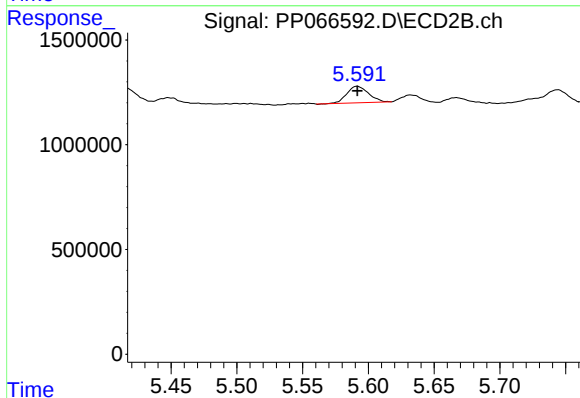


#7 AR-1016-5

R.T.: 5.591 min
Delta R.T.: 0.000 min
Response: 897096
Conc: 19.95 ng/ml

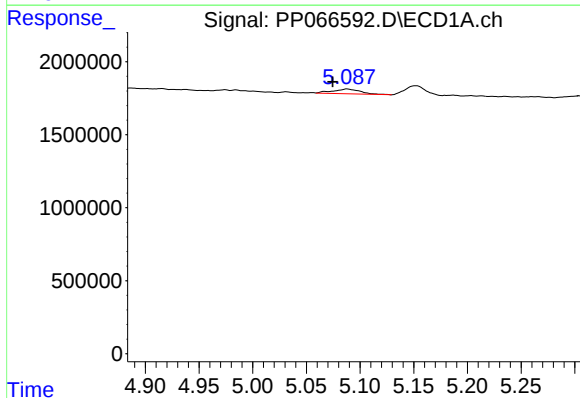


#9 AR-1221-2

R.T.: 5.088 min
Delta R.T.: 0.014 min
Response: 575483
Conc: 31.54 ng/ml

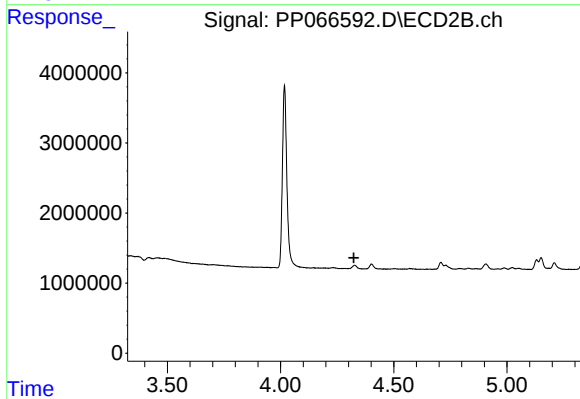

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.324 min
Response: 0
Conc: N.D.

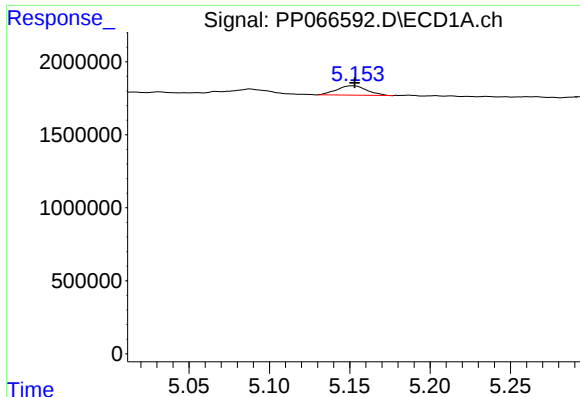

#10 AR-1221-3


R.T.: 5.152 min
Delta R.T.: 0.000 min
Response: 840550
Conc: 15.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

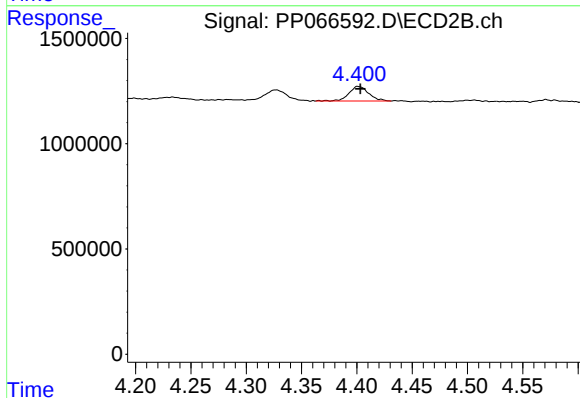


#10 AR-1221-3

R.T.: 4.401 min
Delta R.T.: -0.002 min
Response: 859950
Conc: 14.96 ng/ml

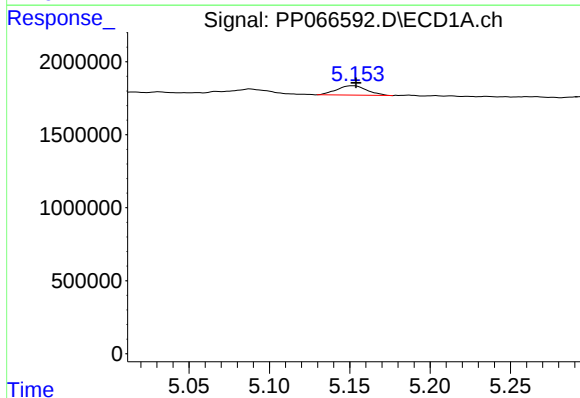


#11 AR-1232-1

R.T.: 5.152 min
Delta R.T.: -0.002 min
Response: 840550
Conc: 18.64 ng/ml

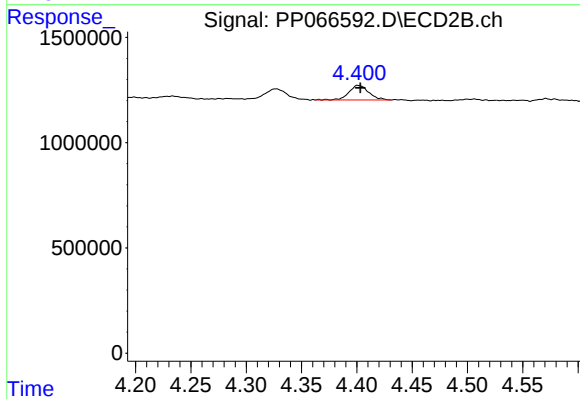

#11 AR-1232-1


R.T.: 4.401 min
Delta R.T.: -0.002 min
Response: 859950
Conc: 18.34 ng/ml

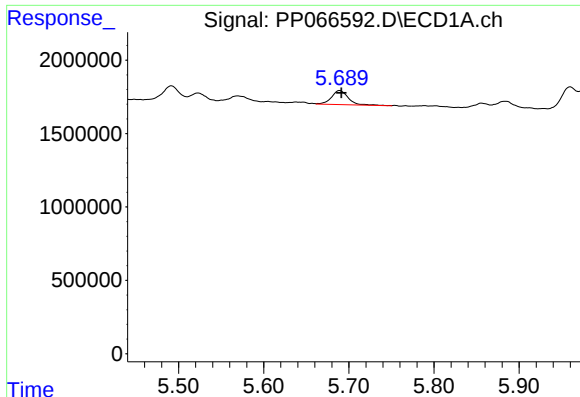

#12 AR-1232-2


R.T.: 5.689 min
Delta R.T.: -0.002 min
Response: 1337045
Conc: 50.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

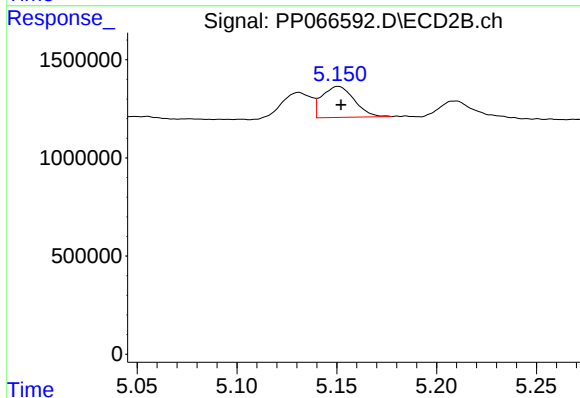


#12 AR-1232-2

R.T.: 5.151 min
Delta R.T.: -0.001 min
Response: 1771102
Conc: 43.04 ng/ml

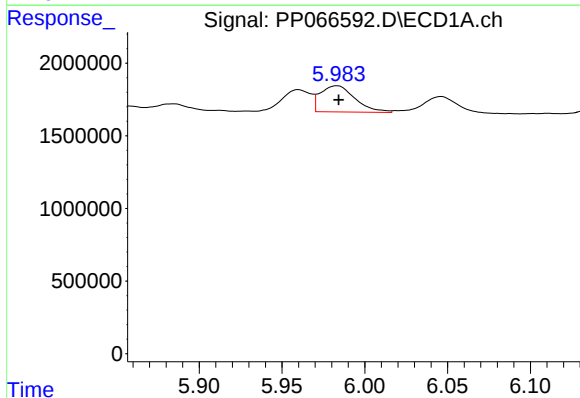


#13 AR-1232-3

R.T.: 5.984 min
Delta R.T.: 0.000 min
Response: 2637887
Conc: 52.53 ng/ml

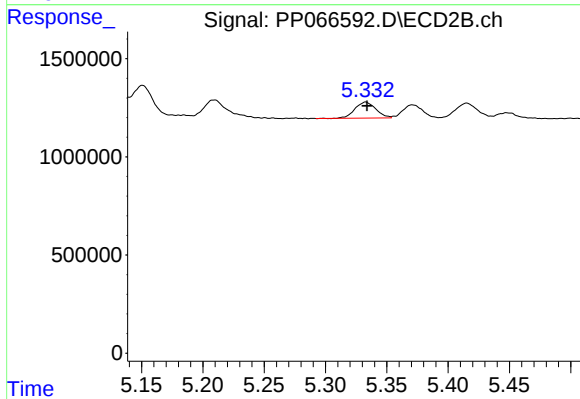

#13 AR-1232-3


R.T.: 5.333 min
Delta R.T.: -0.001 min
Response: 968925
Conc: 43.57 ng/ml

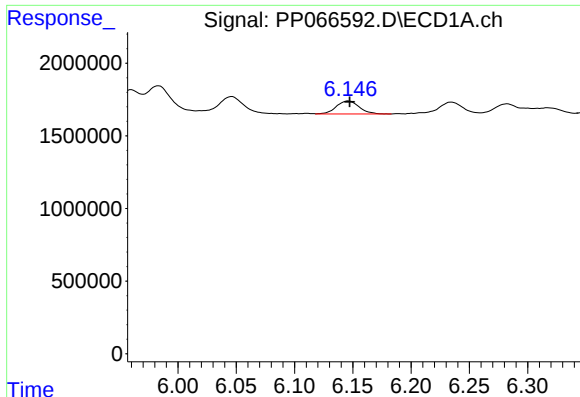

#14 AR-1232-4


R.T.: 6.146 min
Delta R.T.: -0.001 min
Response: 1214800
Conc: 45.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

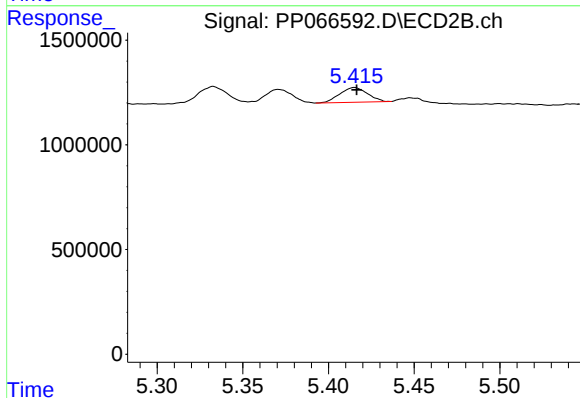


#14 AR-1232-4

R.T.: 5.415 min
Delta R.T.: -0.001 min
Response: 787872
Conc: 41.08 ng/ml

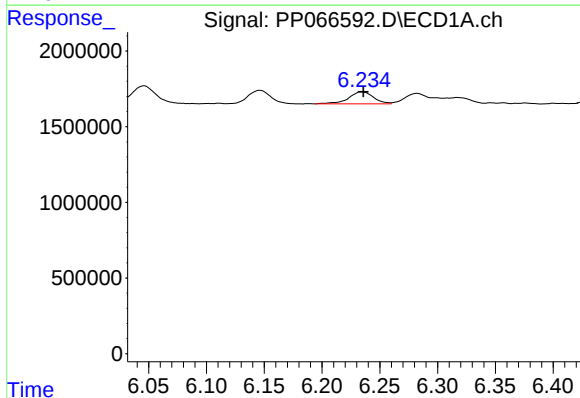


#15 AR-1232-5

R.T.: 6.235 min
Delta R.T.: -0.001 min
Response: 1192522
Conc: 60.37 ng/ml

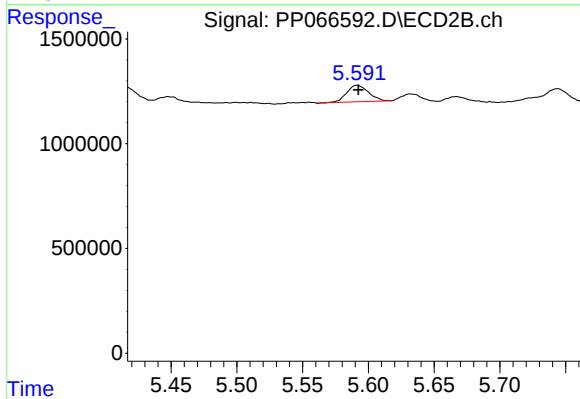

#15 AR-1232-5


R.T.: 5.591 min
Delta R.T.: -0.001 min
Response: 897096
Conc: 44.70 ng/ml

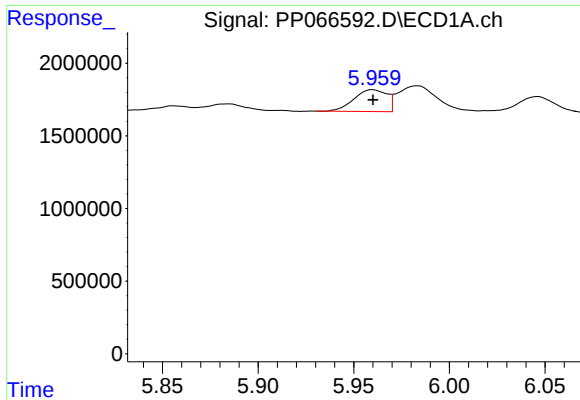

#16 AR-1242-1


R.T.: 5.960 min
Delta R.T.: 0.000 min
Response: 1794724
Conc: 30.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

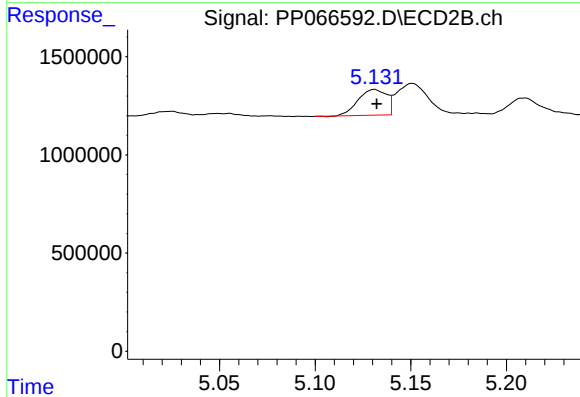


#16 AR-1242-1

R.T.: 5.131 min
Delta R.T.: -0.001 min
Response: 1355402
Conc: 27.35 ng/ml

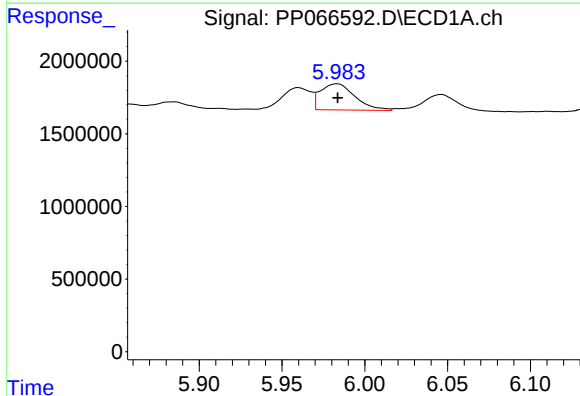


#17 AR-1242-2

R.T.: 5.984 min
Delta R.T.: 0.000 min
Response: 2637887
Conc: 29.84 ng/ml

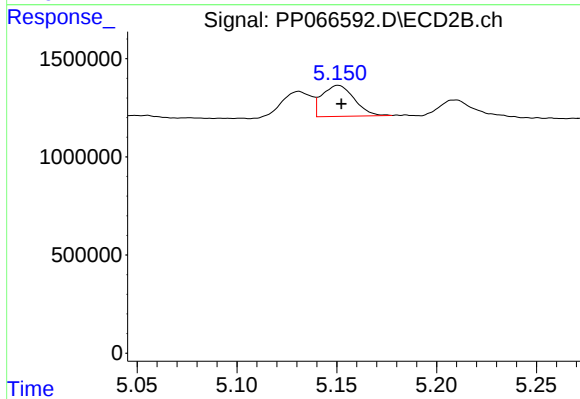

#17 AR-1242-2


R.T.: 5.151 min
Delta R.T.: -0.002 min
Response: 1771102
Conc: 25.46 ng/ml

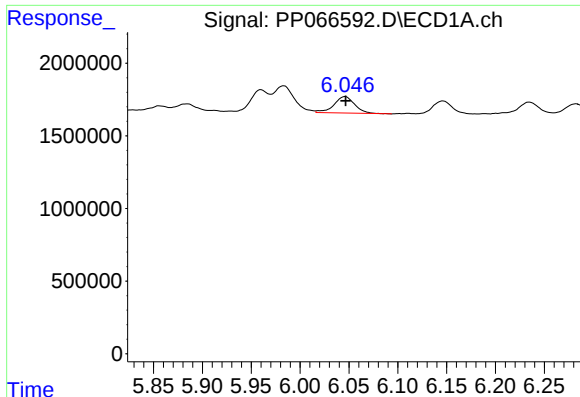

#18 AR-1242-3


R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 1677004
Conc: 31.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

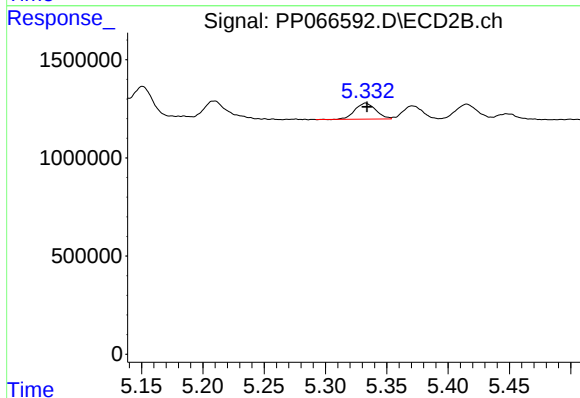


#18 AR-1242-3

R.T.: 5.333 min
Delta R.T.: -0.001 min
Response: 968925
Conc: 26.31 ng/ml

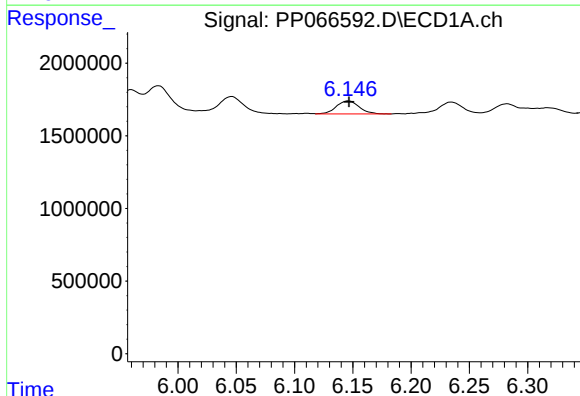


#19 AR-1242-4

R.T.: 6.146 min
Delta R.T.: 0.000 min
Response: 1214800
Conc: 27.30 ng/ml

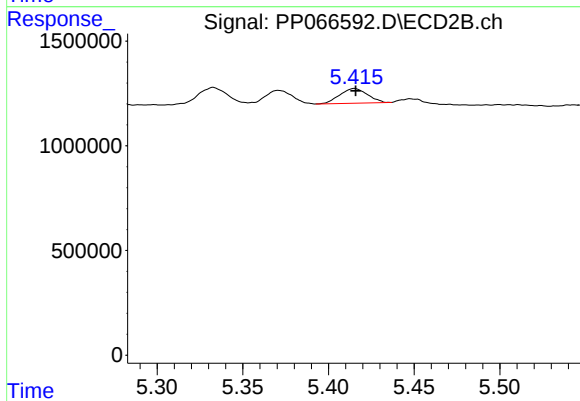

#19 AR-1242-4


R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 787872
Conc: 22.08 ng/ml

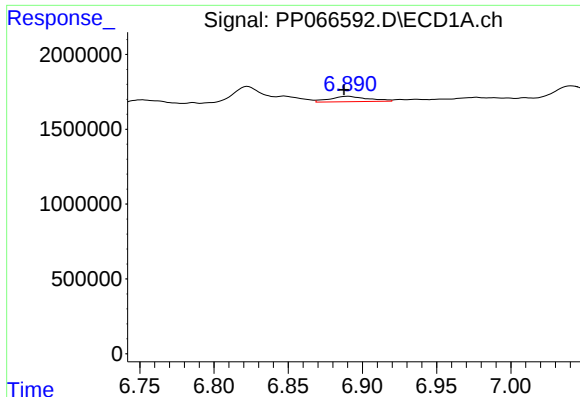

#20 AR-1242-5


R.T.: 6.890 min
Delta R.T.: 0.003 min
Response: 636640
Conc: 12.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

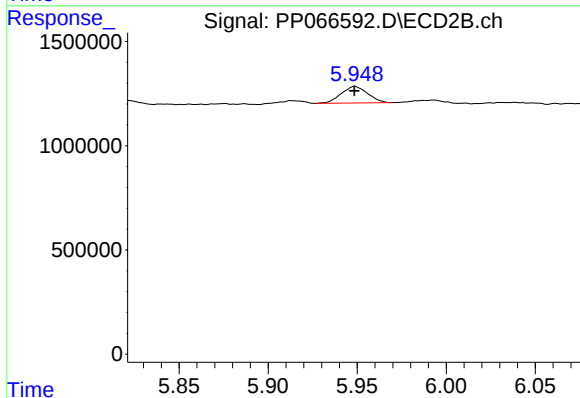


#20 AR-1242-5

R.T.: 5.949 min
Delta R.T.: 0.000 min
Response: 818688
Conc: 19.40 ng/ml

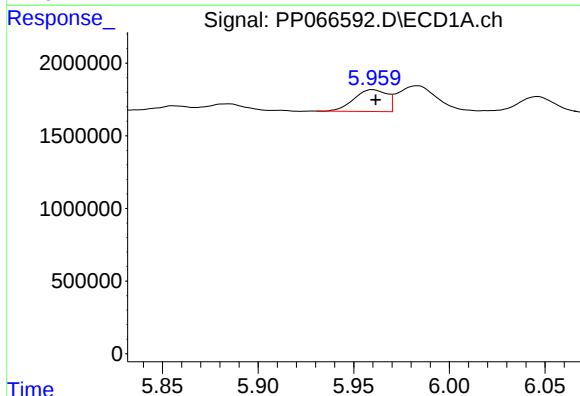


#21 AR-1248-1

R.T.: 5.960 min
Delta R.T.: -0.001 min
Response: 1794724
Conc: 37.12 ng/ml

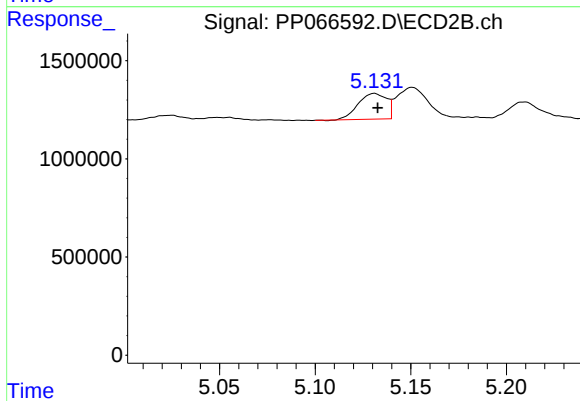

#21 AR-1248-1


R.T.: 5.131 min
Delta R.T.: -0.002 min
Response: 1355402
Conc: 33.90 ng/ml

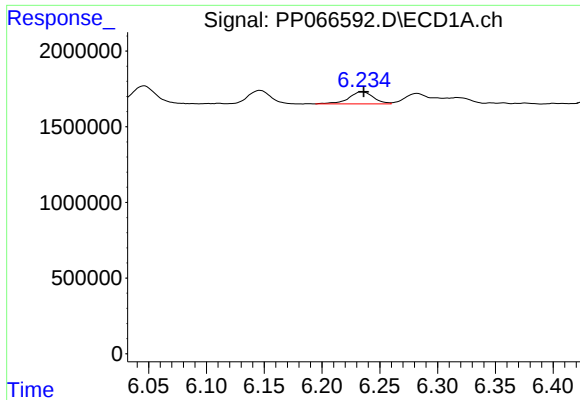

#22 AR-1248-2


R.T.: 6.235 min
Delta R.T.: -0.001 min
Response: 1192522
Conc: 16.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

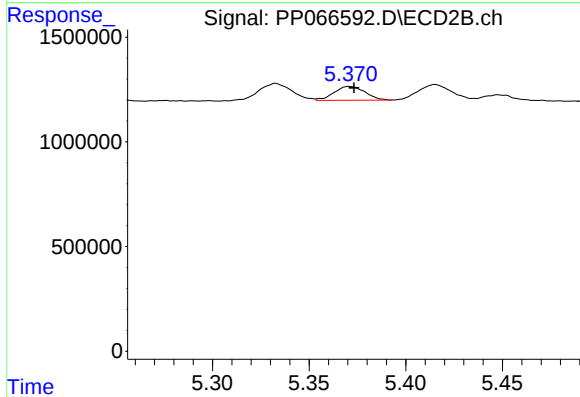


#22 AR-1248-2

R.T.: 5.371 min
Delta R.T.: -0.002 min
Response: 731480
Conc: 13.81 ng/ml

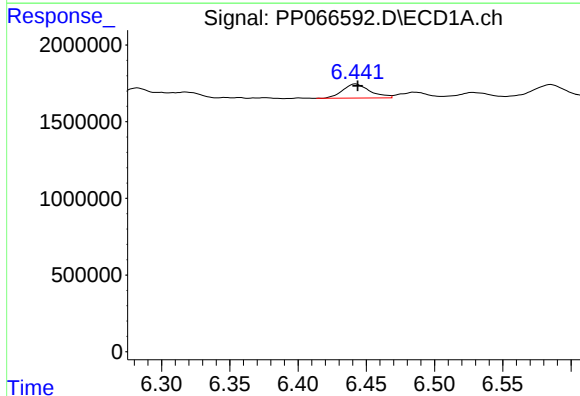


#23 AR-1248-3

R.T.: 6.442 min
Delta R.T.: -0.002 min
Response: 1277120
Conc: 16.53 ng/ml

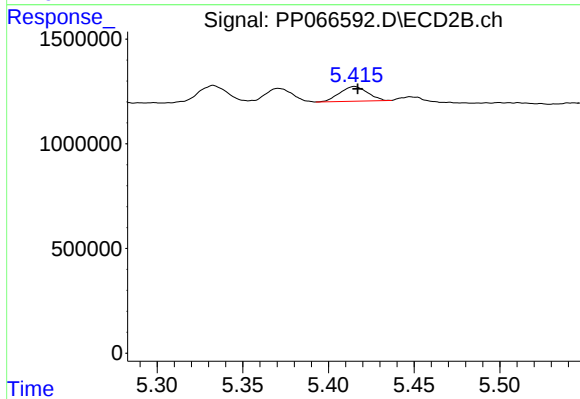

#23 AR-1248-3


R.T.: 5.415 min
Delta R.T.: -0.002 min
Response: 787872
Conc: 14.38 ng/ml

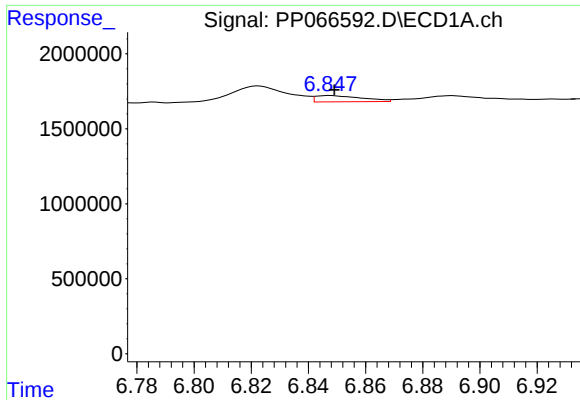

#24 AR-1248-4


R.T.: 6.848 min
Delta R.T.: -0.001 min
Response: 474294
Conc: 5.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

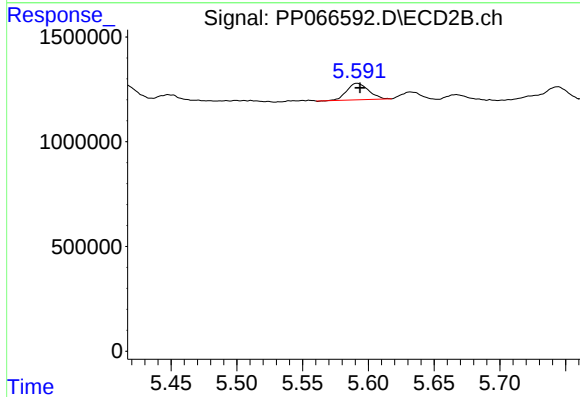


#24 AR-1248-4

R.T.: 5.591 min
Delta R.T.: -0.002 min
Response: 897096
Conc: 14.30 ng/ml

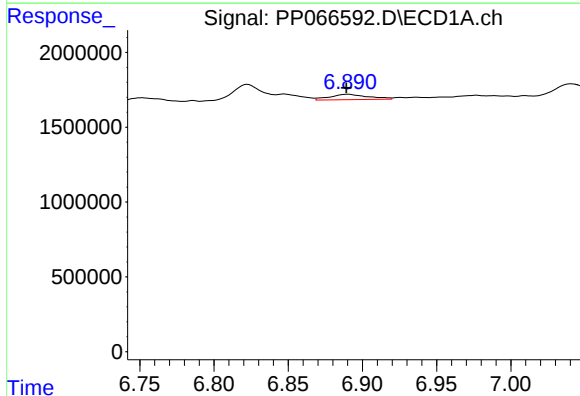


#25 AR-1248-5

R.T.: 6.890 min
Delta R.T.: 0.001 min
Response: 636640
Conc: 7.21 ng/ml

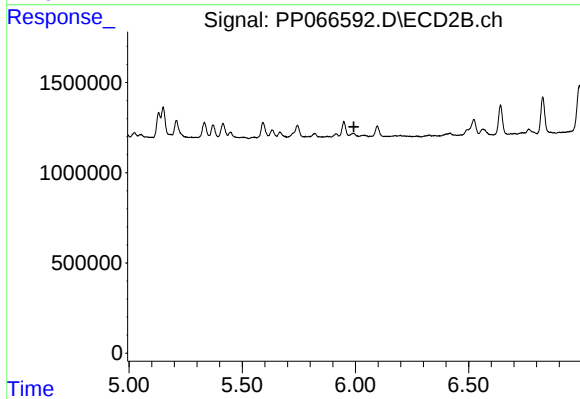

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 5.993 min
Response: 0
Conc: N.D.

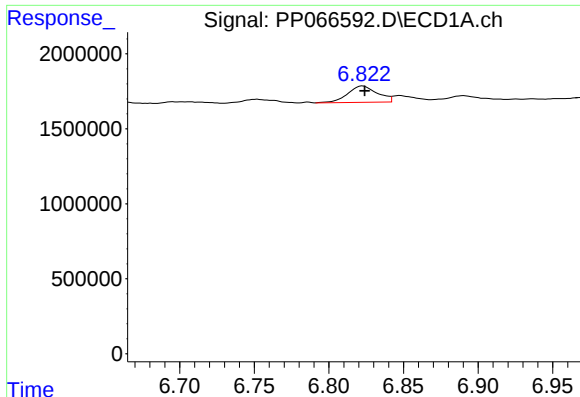

#26 AR-1254-1


R.T.: 6.823 min
Delta R.T.: -0.001 min
Response: 1514322
Conc: 16.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

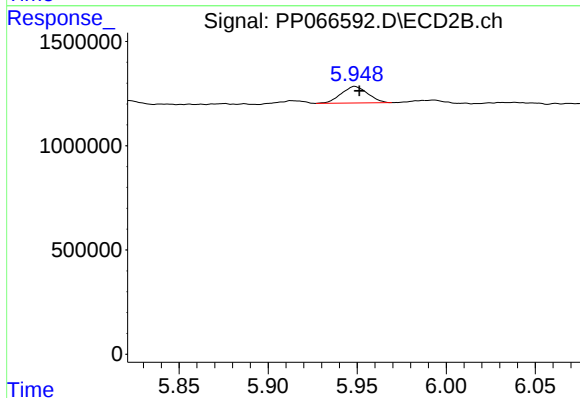


#26 AR-1254-1

R.T.: 5.949 min
Delta R.T.: -0.003 min
Response: 818688
Conc: 9.60 ng/ml

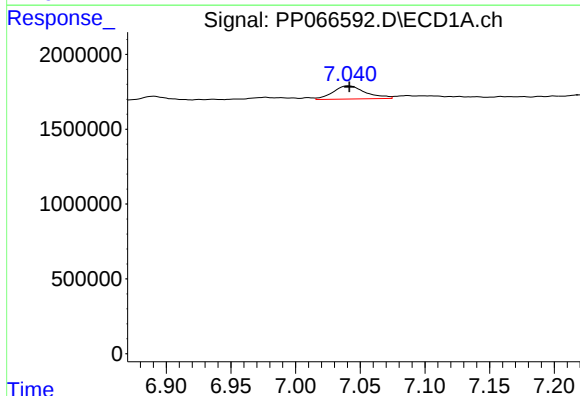


#27 AR-1254-2

R.T.: 7.041 min
Delta R.T.: 0.000 min
Response: 1544123
Conc: 11.42 ng/ml

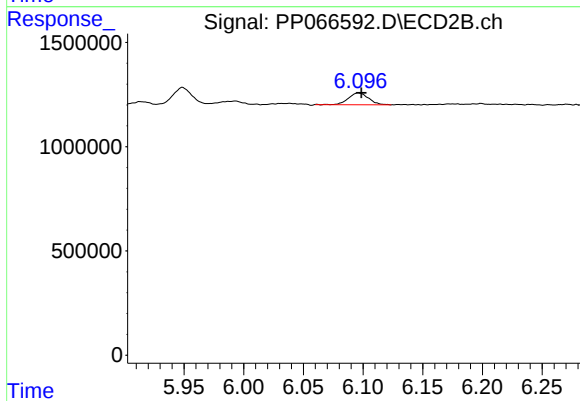

#27 AR-1254-2


R.T.: 6.096 min
Delta R.T.: -0.003 min
Response: 669236
Conc: 8.96 ng/ml

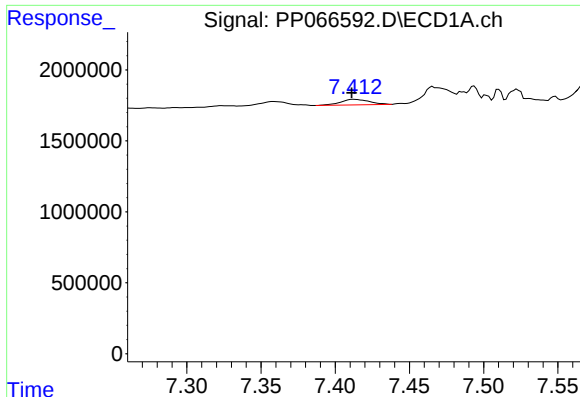

#28 AR-1254-3


R.T.: 7.413 min
Delta R.T.: 0.002 min
Response: 531477
Conc: 3.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

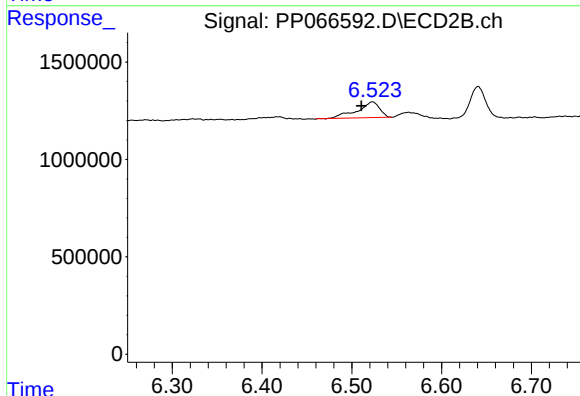


#28 AR-1254-3

R.T.: 6.523 min
Delta R.T.: 0.012 min
Response: 1395472
Conc: 11.96 ng/ml

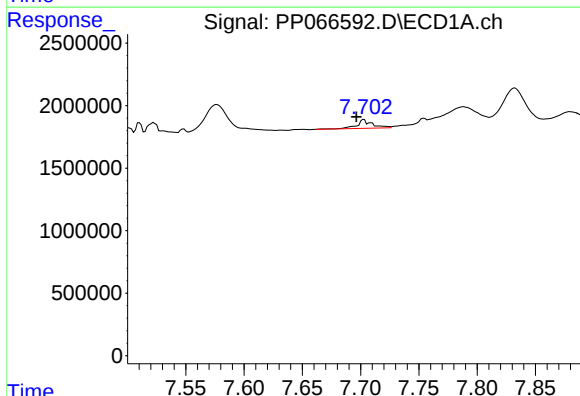


#29 AR-1254-4

R.T.: 7.703 min
Delta R.T.: 0.006 min
Response: 647742
Conc: 6.30 ng/ml

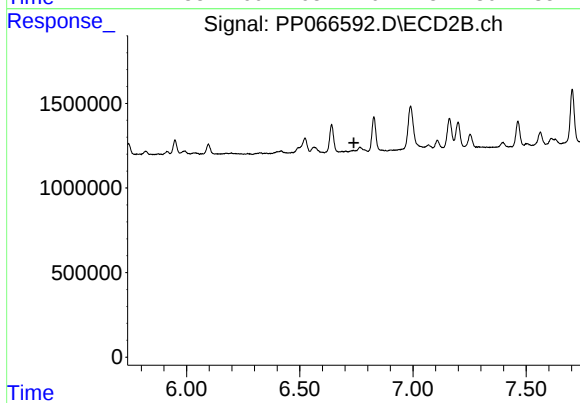

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.739 min
Response: 0
Conc: N.D.

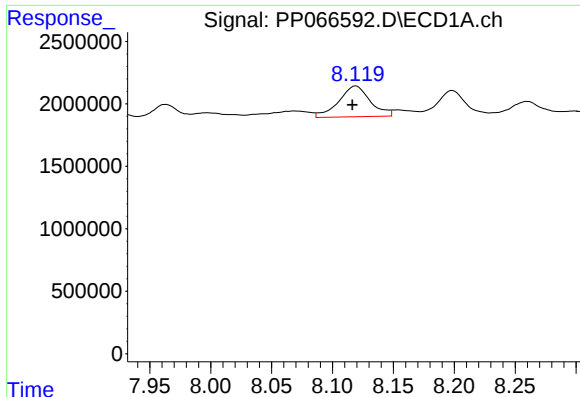

#30 AR-1254-5


R.T.: 8.119 min
Delta R.T.: 0.003 min
Response: 4420136
Conc: 40.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

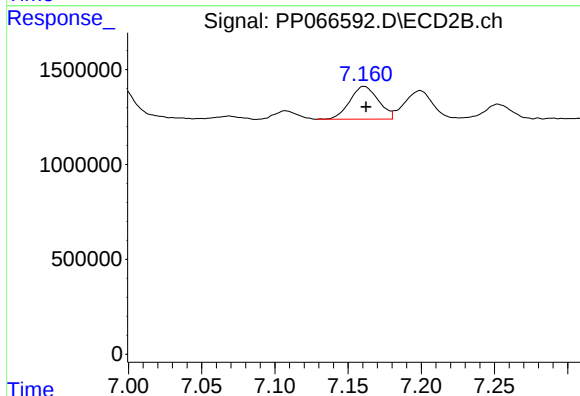


#30 AR-1254-5

R.T.: 7.161 min
Delta R.T.: -0.001 min
Response: 2345216
Conc: 21.76 ng/ml

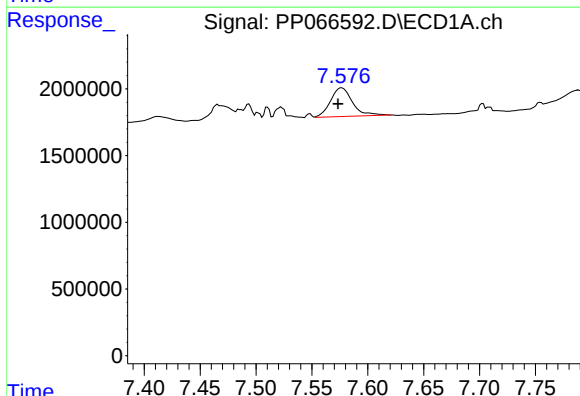


#31 AR-1260-1

R.T.: 7.577 min
Delta R.T.: 0.003 min
Response: 2972094
Conc: 27.99 ng/ml

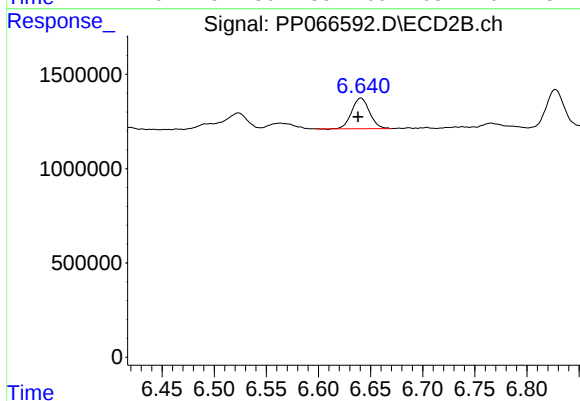

#31 AR-1260-1


R.T.: 6.641 min
Delta R.T.: 0.003 min
Response: 1934471
Conc: 23.79 ng/ml

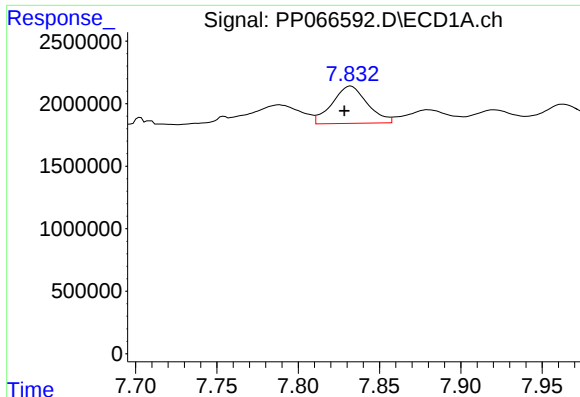

#32 AR-1260-2


R.T.: 7.832 min
Delta R.T.: 0.004 min
Response: 4480478
Conc: 35.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

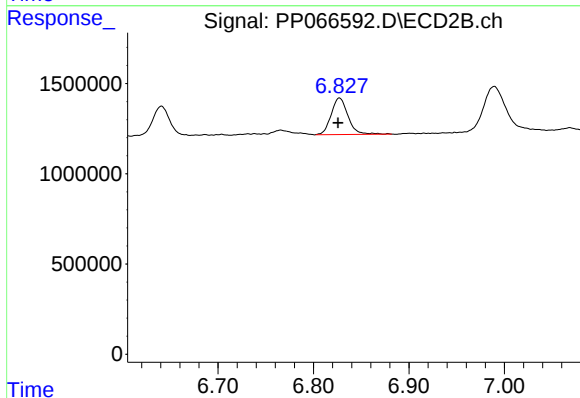


#32 AR-1260-2

R.T.: 6.827 min
Delta R.T.: 0.001 min
Response: 2499240
Conc: 25.52 ng/ml

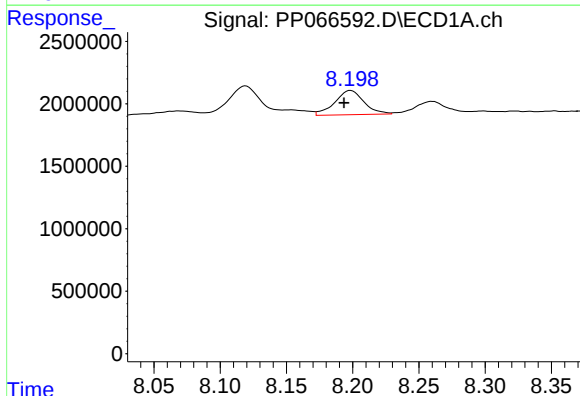


#33 AR-1260-3

R.T.: 8.198 min
Delta R.T.: 0.005 min
Response: 2989140
Conc: 33.30 ng/ml

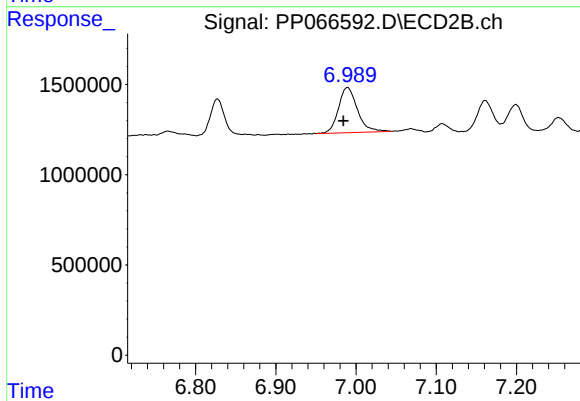

#33 AR-1260-3


R.T.: 6.989 min
Delta R.T.: 0.005 min
Response: 4115448
Conc: 38.98 ng/ml

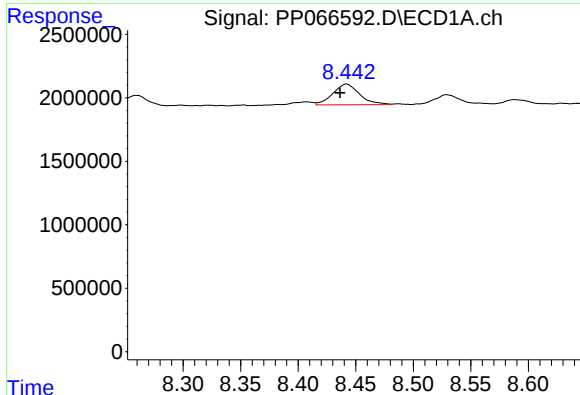

#34 AR-1260-4


R.T.: 8.442 min
Delta R.T.: 0.006 min
Response: 2643119
Conc: 27.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

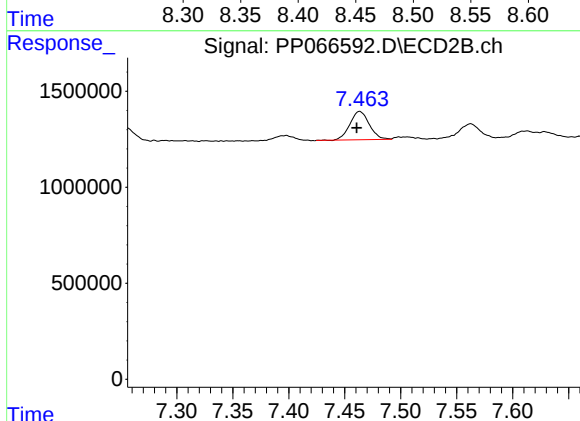


#34 AR-1260-4

R.T.: 7.463 min
Delta R.T.: 0.003 min
Response: 1786495
Conc: 24.13 ng/ml

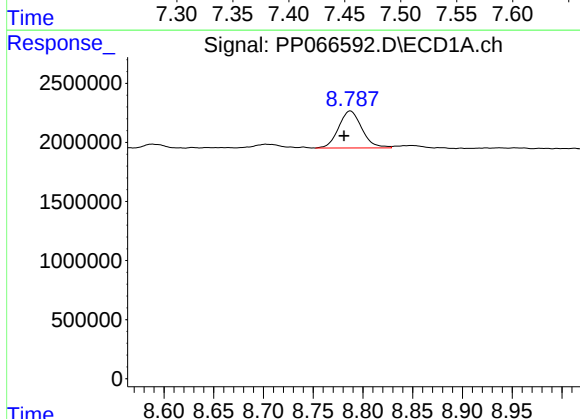


#35 AR-1260-5

R.T.: 8.788 min
Delta R.T.: 0.007 min
Response: 5096576
Conc: 26.83 ng/ml

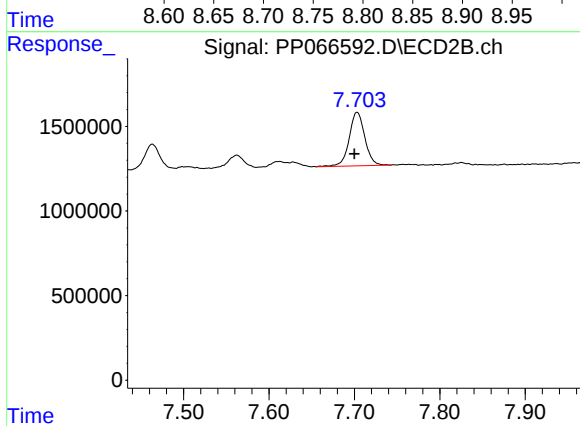

#35 AR-1260-5


R.T.: 7.703 min
Delta R.T.: 0.003 min
Response: 4040304
Conc: 23.69 ng/ml

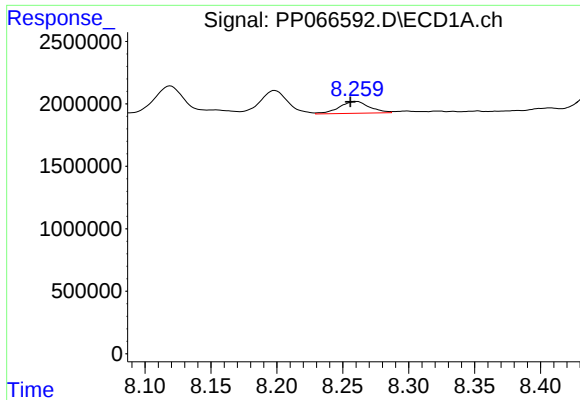

#36 AR-1262-1


R.T.: 8.260 min
Delta R.T.: 0.004 min
Response: 1521277
Conc: 24.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

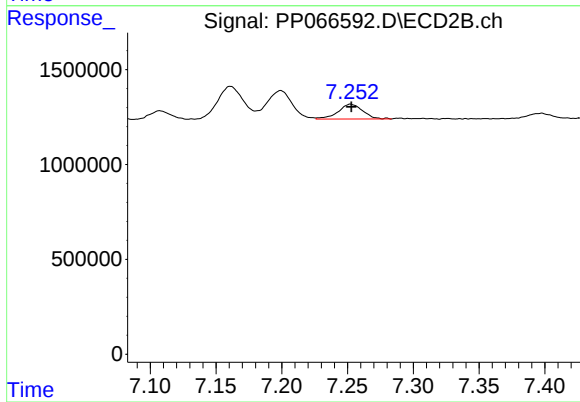


#36 AR-1262-1

R.T.: 7.252 min
Delta R.T.: 0.000 min
Response: 1017901
Conc: 20.10 ng/ml

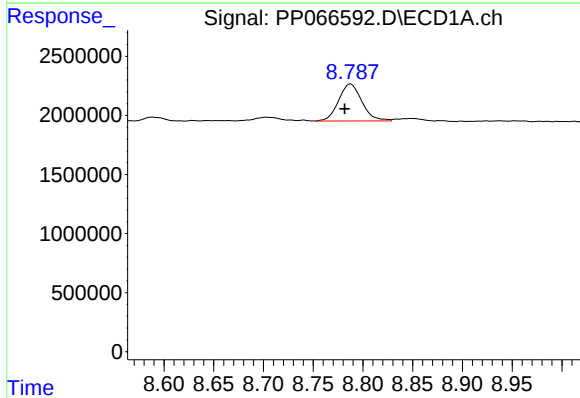


#37 AR-1262-2

R.T.: 8.788 min
Delta R.T.: 0.006 min
Response: 5096576
Conc: 20.83 ng/ml

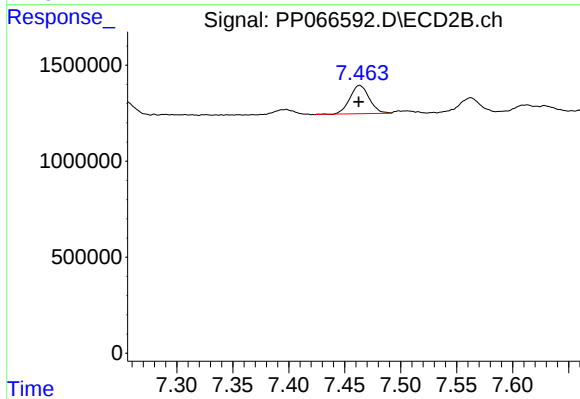

#37 AR-1262-2


R.T.: 7.463 min
Delta R.T.: 0.000 min
Response: 1786495
Conc: 16.72 ng/ml

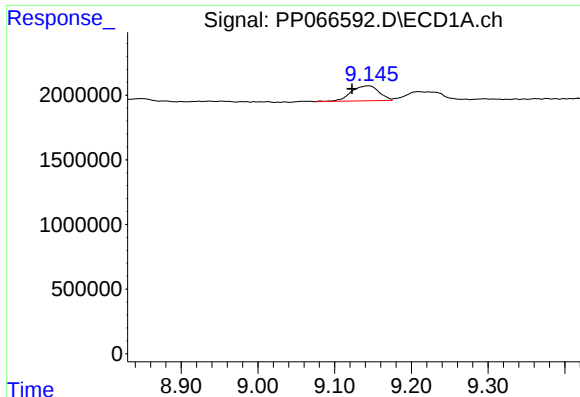

#38 AR-1262-3


R.T.: 9.145 min
Delta R.T.: 0.022 min
Response: 2946311
Conc: 16.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

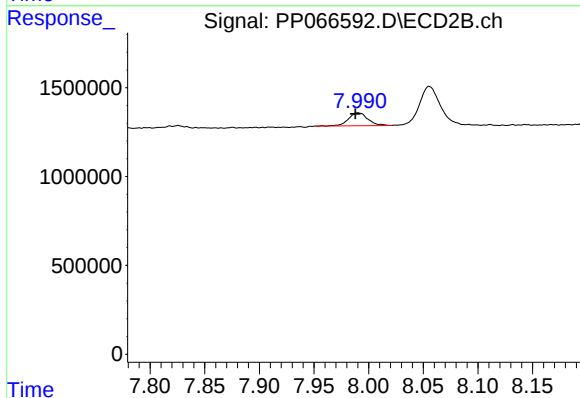


#38 AR-1262-3

R.T.: 7.990 min
Delta R.T.: 0.002 min
Response: 893431
Conc: 10.23 ng/ml

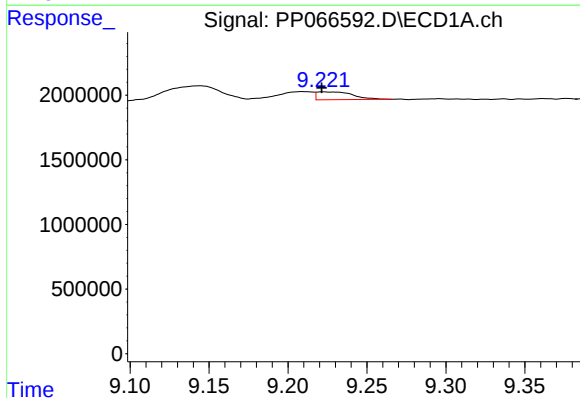


#39 AR-1262-4

R.T.: 9.222 min
Delta R.T.: 0.000 min
Response: 967195
Conc: 6.58 ng/ml

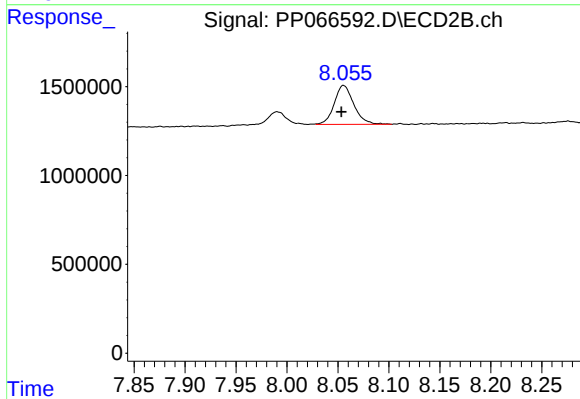

#39 AR-1262-4


R.T.: 8.056 min
Delta R.T.: 0.002 min
Response: 2929584
Conc: 18.88 ng/ml

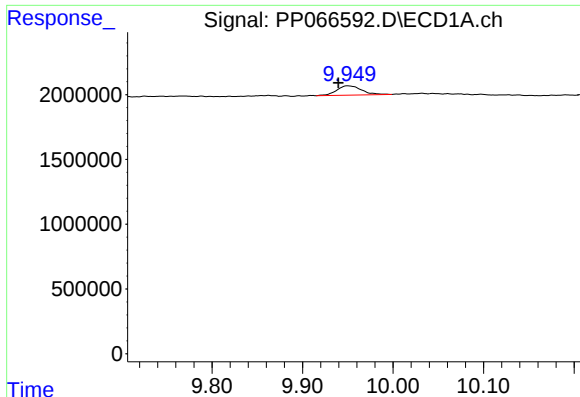

#40 AR-1262-5


R.T.: 9.950 min
Delta R.T.: 0.011 min
Response: 1389440
Conc: 14.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

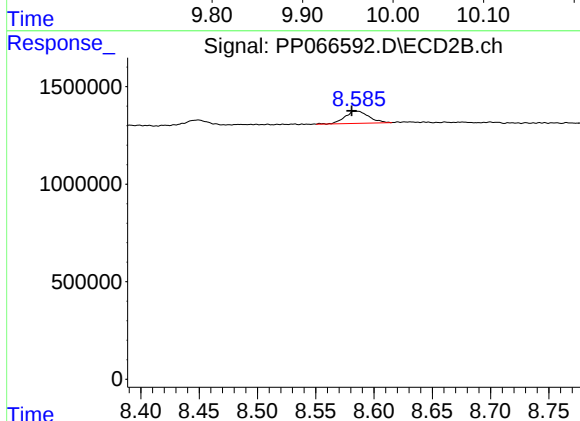


#40 AR-1262-5

R.T.: 8.585 min
Delta R.T.: 0.004 min
Response: 895240
Conc: 13.63 ng/ml

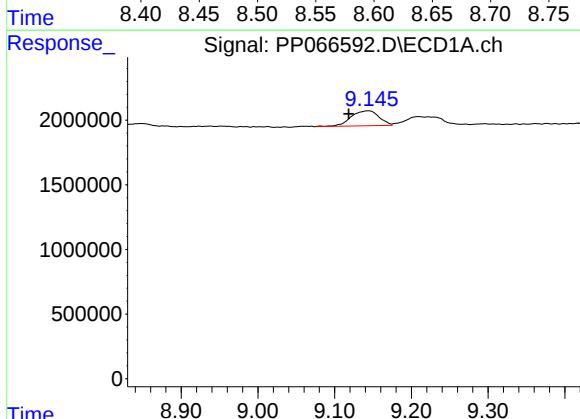


#41 AR-1268-1

R.T.: 9.145 min
Delta R.T.: 0.027 min
Response: 2946311
Conc: 9.85 ng/ml

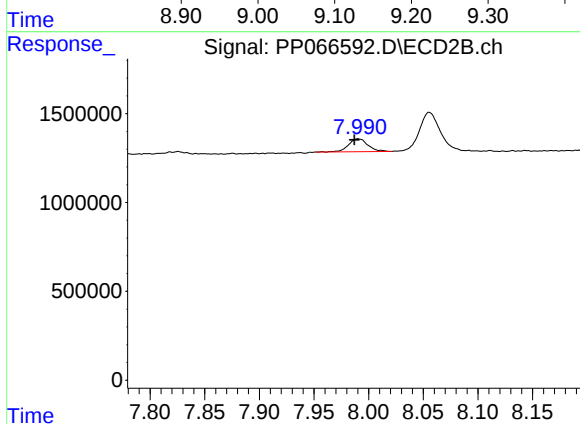

#41 AR-1268-1


R.T.: 7.990 min
Delta R.T.: 0.004 min
Response: 893431
Conc: 3.85 ng/ml

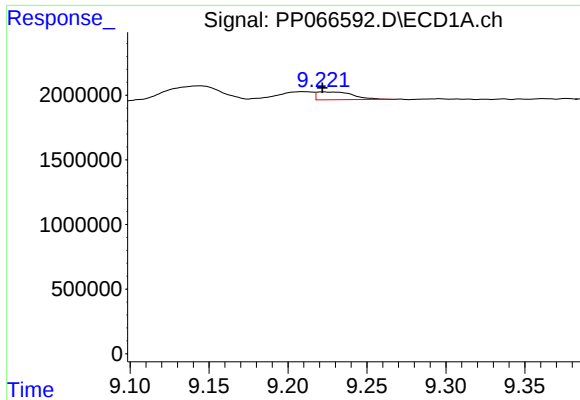

#42 AR-1268-2


R.T.: 9.222 min
Delta R.T.: 0.000 min
Response: 967195
Conc: 3.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

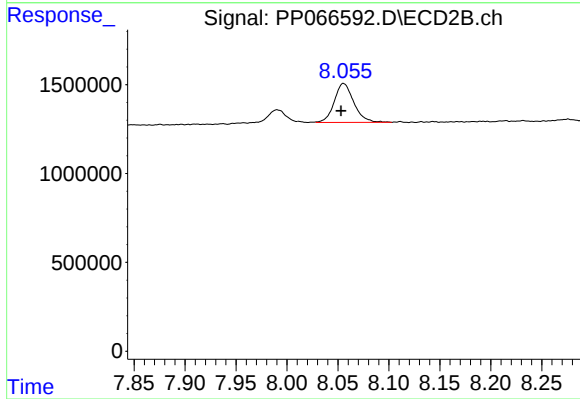


#42 AR-1268-2

R.T.: 8.056 min
Delta R.T.: 0.002 min
Response: 2929584
Conc: 13.95 ng/ml

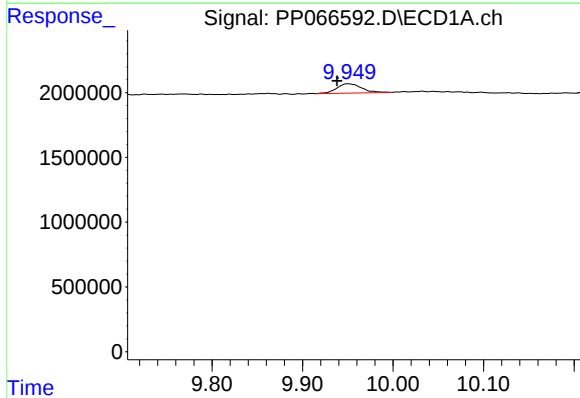


#44 AR-1268-4

R.T.: 9.950 min
Delta R.T.: 0.012 min
Response: 1389440
Conc: 14.57 ng/ml

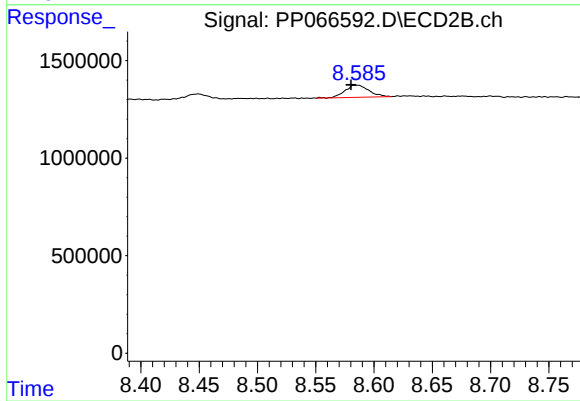

#44 AR-1268-4


R.T.: 8.585 min
Delta R.T.: 0.005 min
Response: 895240
Conc: 13.37 ng/ml

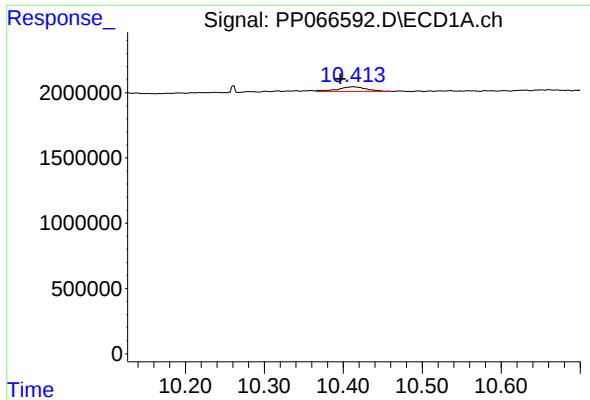

#45 AR-1268-5

R.T.: 10.413 min
Delta R.T.: 0.017 min
Response: 856176
Conc: 1.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

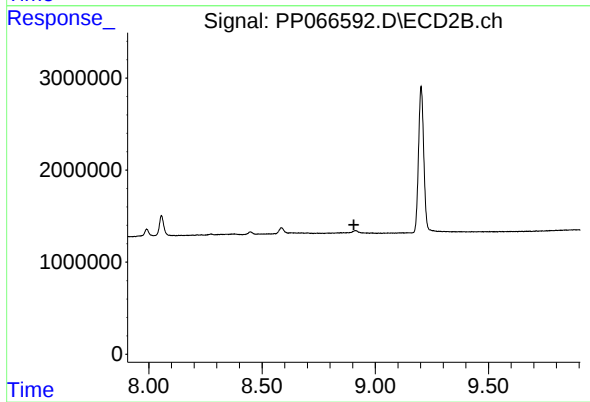

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.906 min
Response: 0
Conc: N.D.