

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080624\
 Data File : PP066598.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2024 12:31
 Operator : YP\AJ
 Sample : P3390-07
 Misc : AR1268 LOD 25 PPB
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 14:00:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 06 04:00:13 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.779	4.018	27794486	30877551	14.697	14.662
2) SA Decachlor...	10.775	9.193	39187543	23965687	18.756	18.028
Target Compounds						
41) L9 AR-1268-1	9.118	7.986	5732291	4750845	19.166	20.492
42) L9 AR-1268-2	9.222	8.051	5329515	4560603	18.862	21.724
43) L9 AR-1268-3	9.474	8.269	5797907	3958576	22.748	21.729
44) L9 AR-1268-4	9.938	8.579	1835247	1397920	19.245	20.878
45) L9 AR-1268-5	10.398	8.904	15801189	10436655	20.559	20.976



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080624\
Data File : PP066598.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2024 12:31
Operator : YP\AJ
Sample : P3390-07
Misc : AR1268 LOD 25 PPB
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 14:00:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 06 04:00:13 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

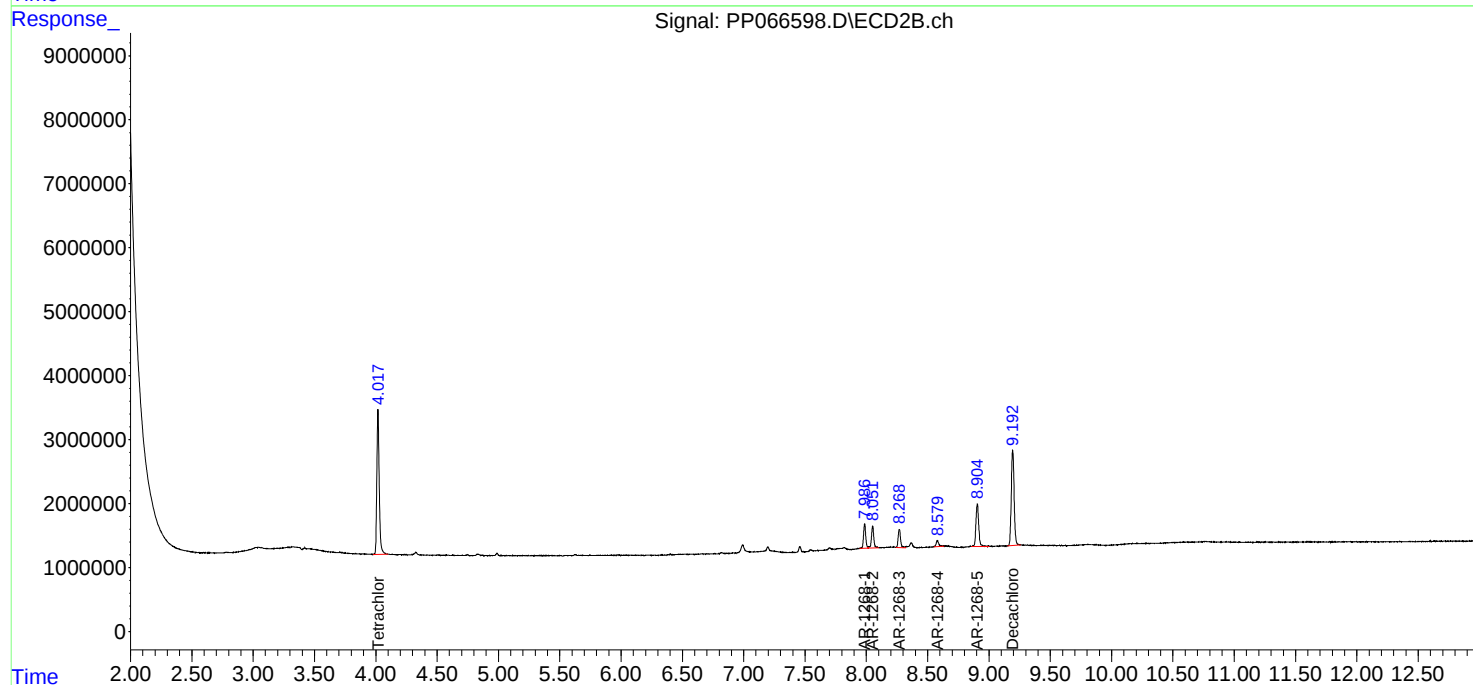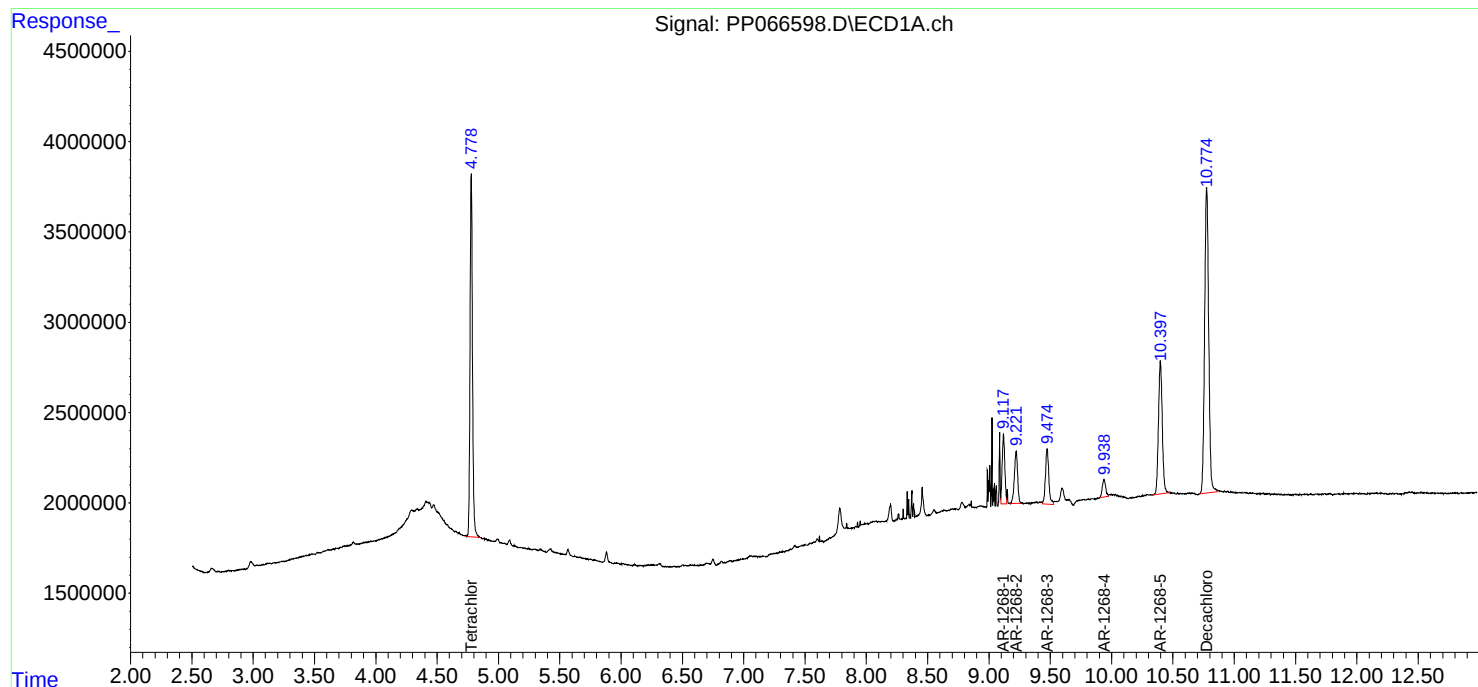


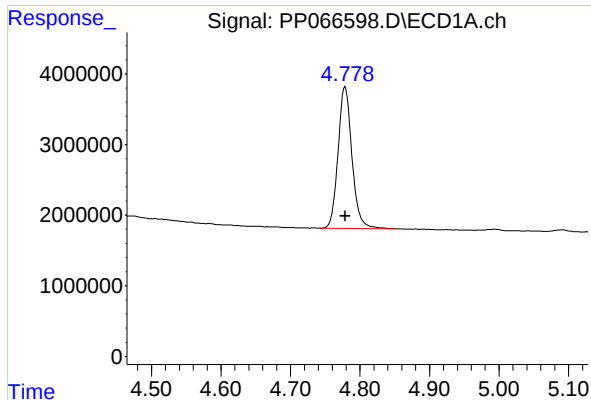

#1 Tetrachloro-m-xylene


R.T.: 4.779 min
Delta R.T.: 0.000 min
Response: 27794486
Conc: 14.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

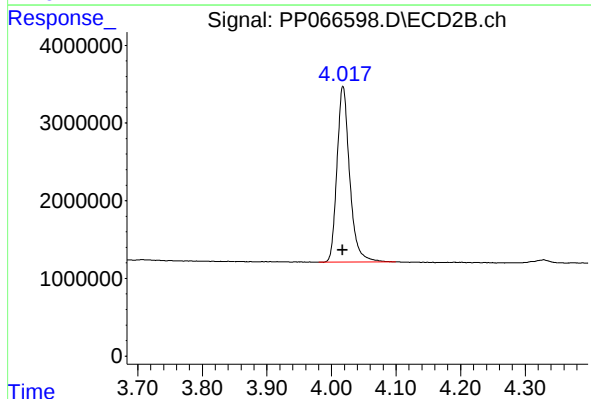


#1 Tetrachloro-m-xylene

R.T.: 4.018 min
Delta R.T.: 0.000 min
Response: 30877551
Conc: 14.66 ng/ml

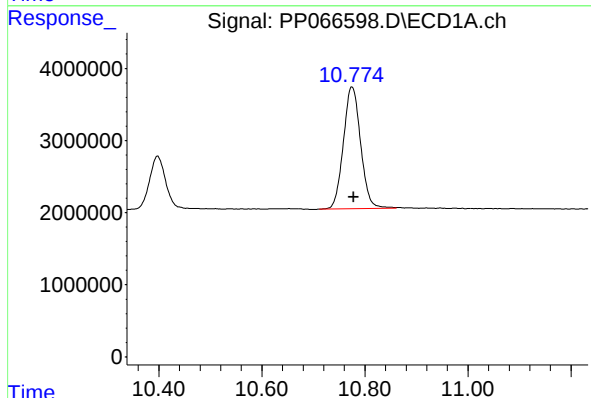


#2 Decachlorobiphenyl

R.T.: 10.775 min
Delta R.T.: -0.004 min
Response: 39187543
Conc: 18.76 ng/ml

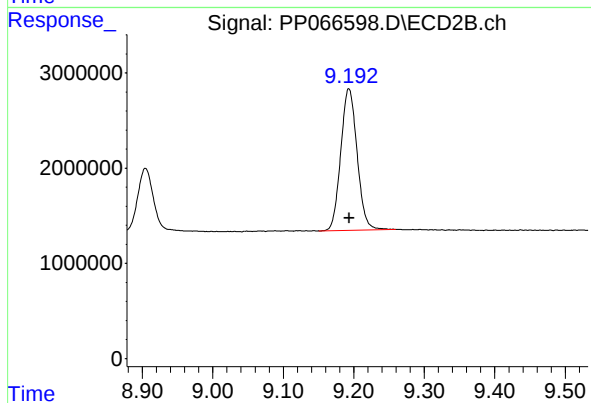

#2 Decachlorobiphenyl


R.T.: 9.193 min
Delta R.T.: 0.000 min
Response: 23965687
Conc: 18.03 ng/ml

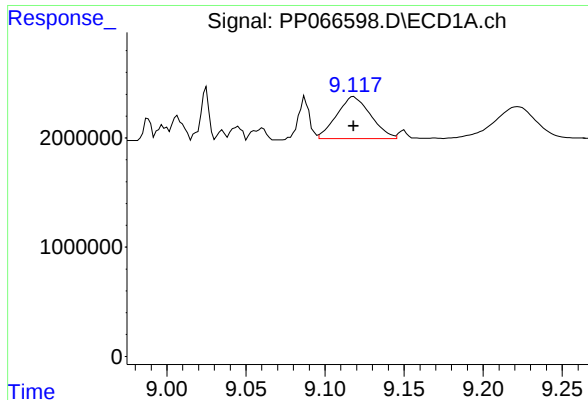

#41 AR-1268-1


R.T.: 9.118 min
Delta R.T.: 0.000 min
Response: 5732291
Conc: 19.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

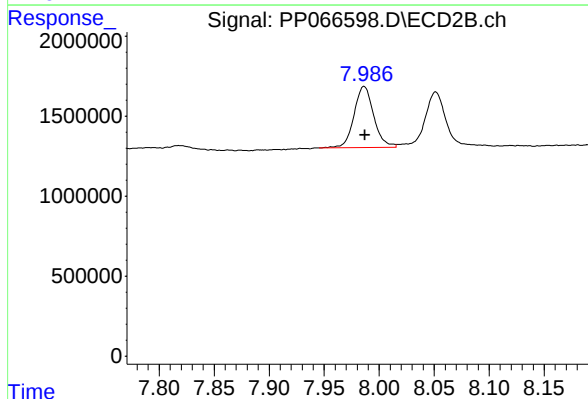


#41 AR-1268-1

R.T.: 7.986 min
Delta R.T.: 0.000 min
Response: 4750845
Conc: 20.49 ng/ml

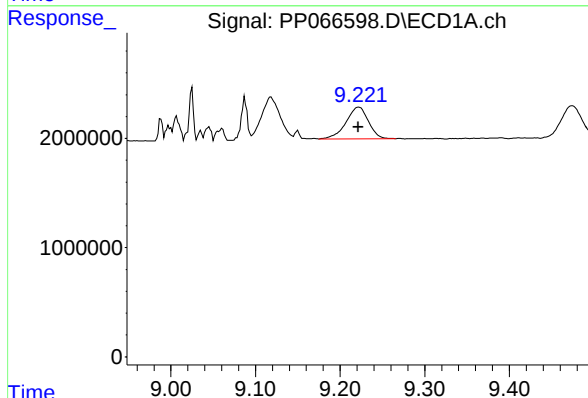


#42 AR-1268-2

R.T.: 9.222 min
Delta R.T.: 0.000 min
Response: 5329515
Conc: 18.86 ng/ml

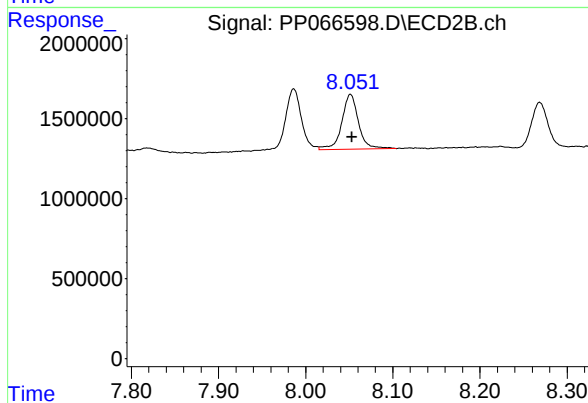

#42 AR-1268-2


R.T.: 8.051 min
Delta R.T.: -0.002 min
Response: 4560603
Conc: 21.72 ng/ml

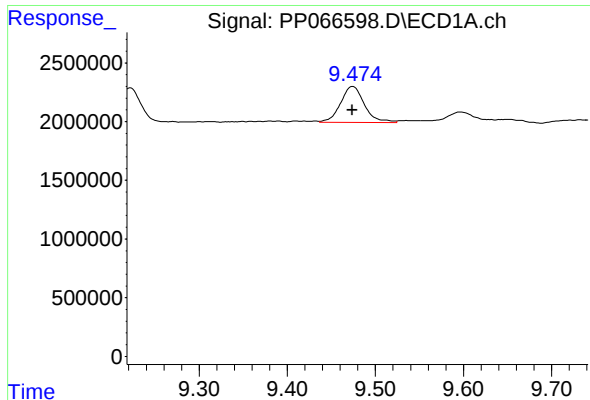

#43 AR-1268-3


R.T.: 9.474 min
Delta R.T.: 0.000 min
Response: 5797907
Conc: 22.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

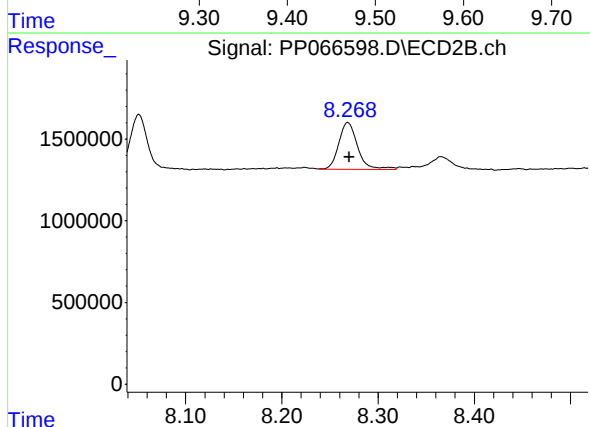


#43 AR-1268-3

R.T.: 8.269 min
Delta R.T.: -0.002 min
Response: 3958576
Conc: 21.73 ng/ml

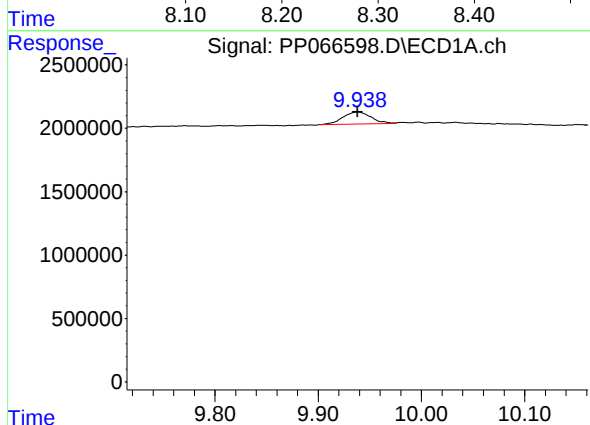


#44 AR-1268-4

R.T.: 9.938 min
Delta R.T.: 0.000 min
Response: 1835247
Conc: 19.25 ng/ml

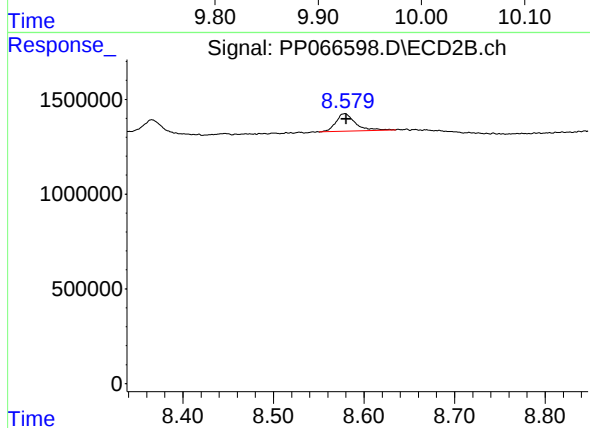

#44 AR-1268-4


R.T.: 8.579 min
Delta R.T.: -0.002 min
Response: 1397920
Conc: 20.88 ng/ml

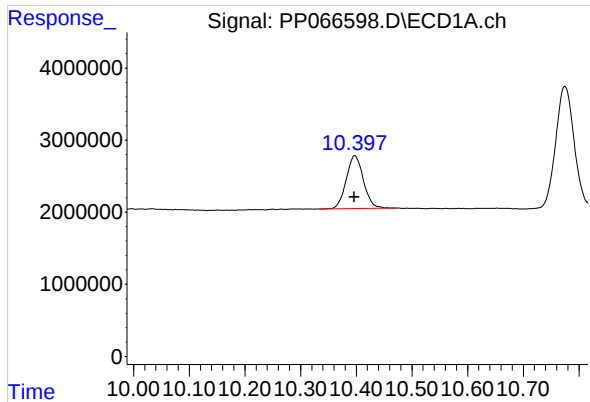

#45 AR-1268-5

R.T.: 10.398 min
Delta R.T.: 0.001 min
Response: 15801189
Conc: 20.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

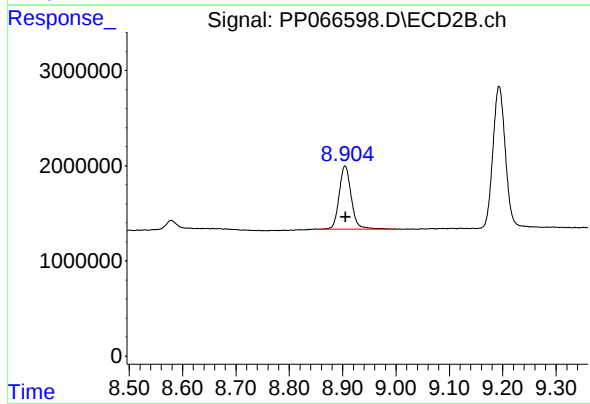

#45 AR-1268-5

R.T.: 8.904 min
Delta R.T.: -0.001 min
Response: 10436655
Conc: 20.98 ng/ml