

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080624\
 Data File : PP066602.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2024 13:54
 Operator : YP\AJ
 Sample : P3390-07
 Misc : AR1262 LOD 25 PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 01:44:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 06 04:00:13 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.781	4.020	31462340	34542035	16.637	16.402
2) SA Decachlor...	10.778	9.194	40334816	25439499	19.305	19.137
Target Compounds						
36) L8 AR-1262-1	8.255	7.252	1901431	1009706	30.390	19.937 #
37) L8 AR-1262-2	8.781	7.461	5731907	2253152	23.427	21.093
38) L8 AR-1262-3	9.124	7.987	3777001	1724328	21.033	19.752
39) L8 AR-1262-4	9.220	8.052	2887219	3097228	19.628	19.962
40) L8 AR-1262-5	9.940	8.580	1807728	1220480	19.212	18.585



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080624\
Data File : PP066602.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2024 13:54
Operator : YP\AJ
Sample : P3390-07
Misc : AR1262 LOD 25 PPB
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 01:44:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 06 04:00:13 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

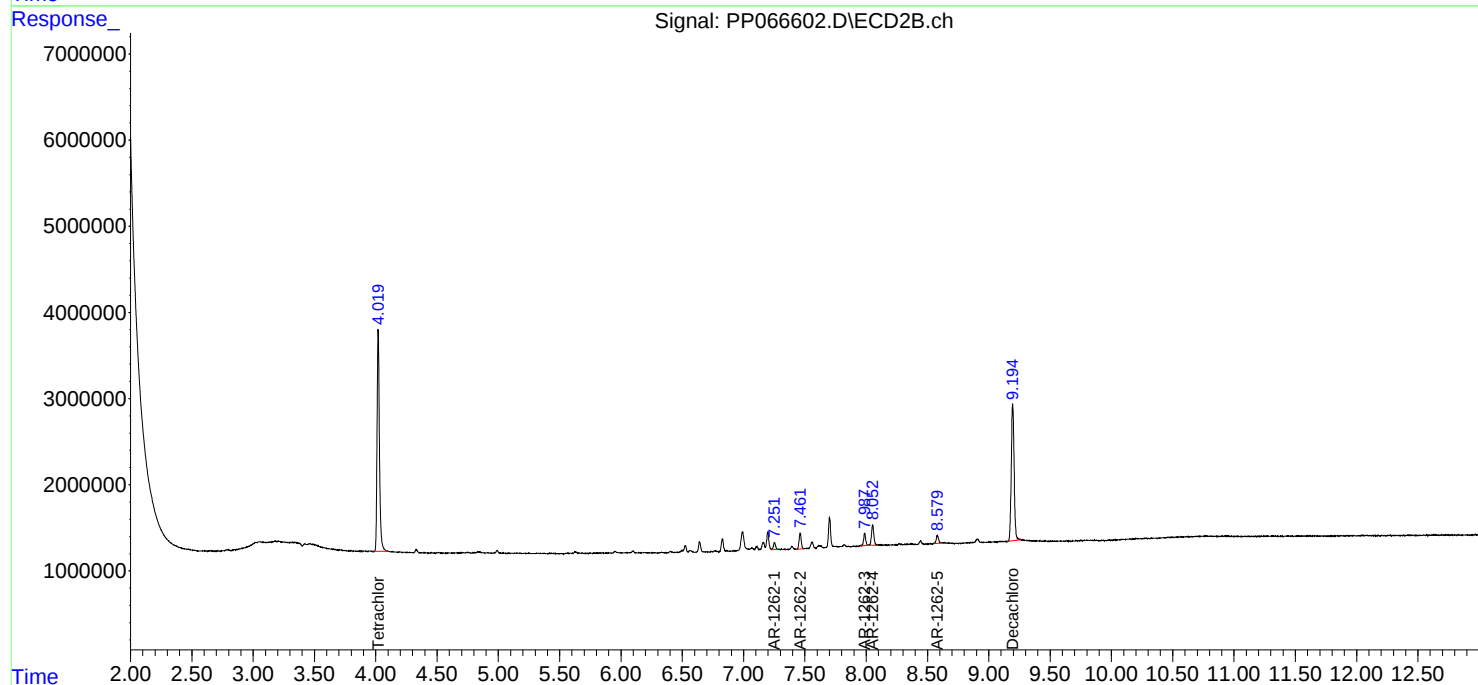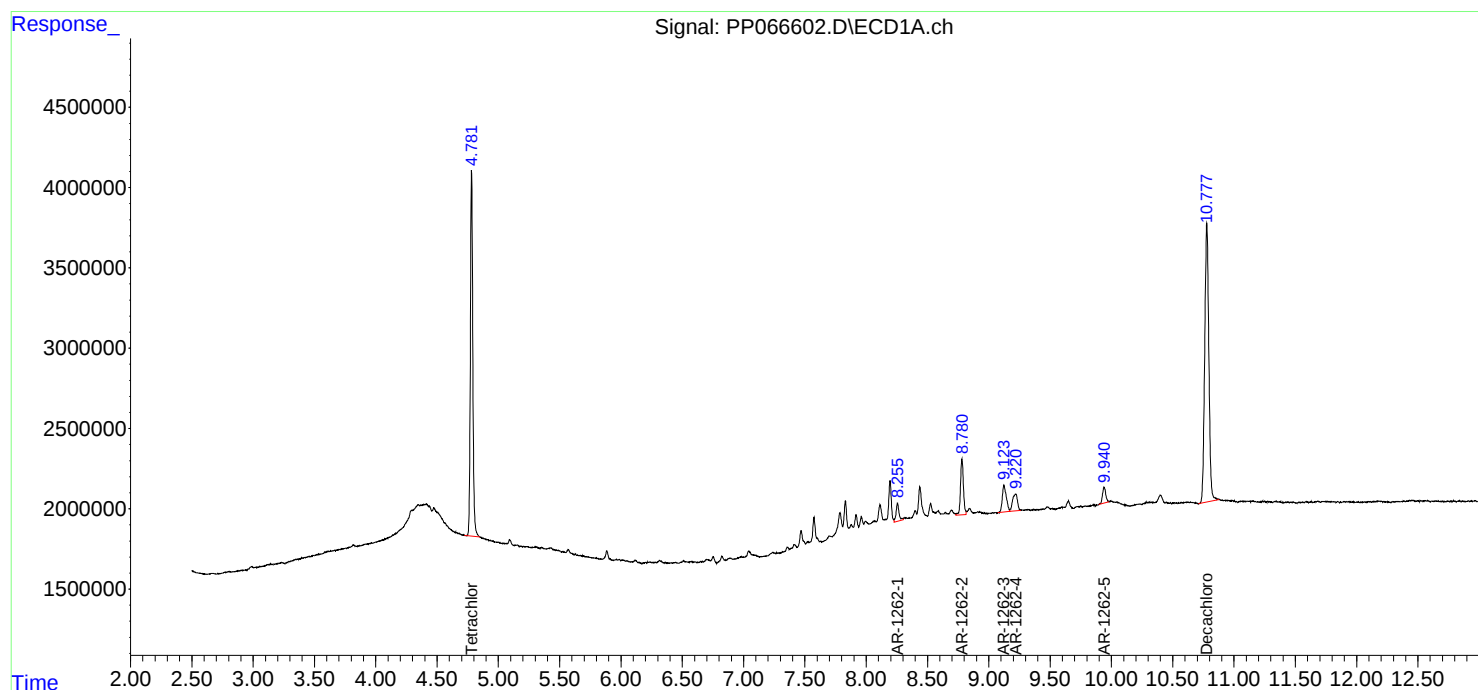


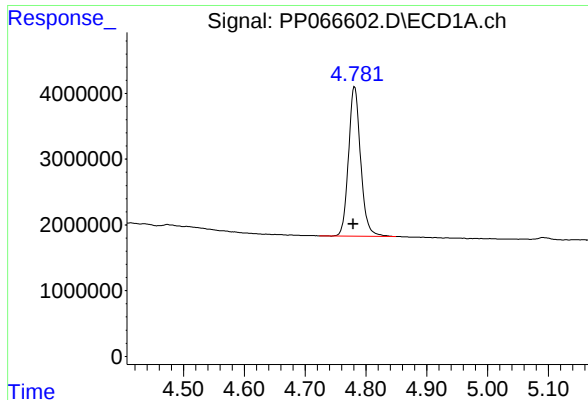

#1 Tetrachloro-m-xylene


R.T.: 4.781 min
Delta R.T.: 0.002 min
Response: 31462340
Conc: 16.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

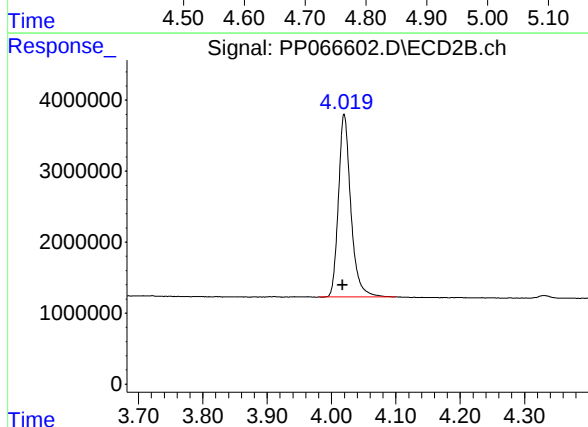


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.002 min
Response: 34542035
Conc: 16.40 ng/ml

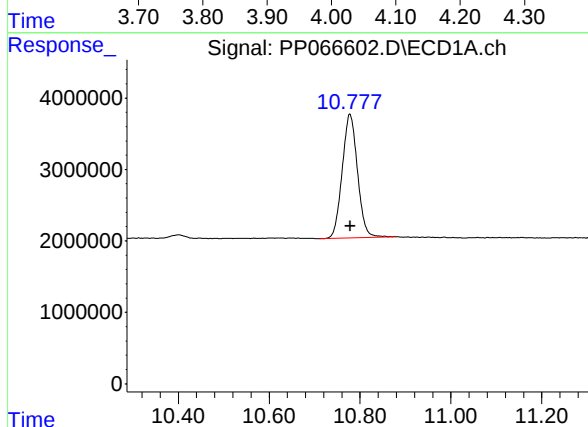


#2 Decachlorobiphenyl

R.T.: 10.778 min
Delta R.T.: -0.001 min
Response: 40334816
Conc: 19.30 ng/ml

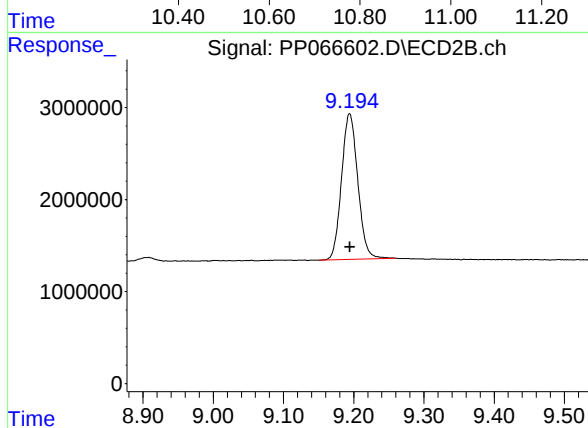

#2 Decachlorobiphenyl


R.T.: 9.194 min
Delta R.T.: 0.000 min
Response: 25439499
Conc: 19.14 ng/ml

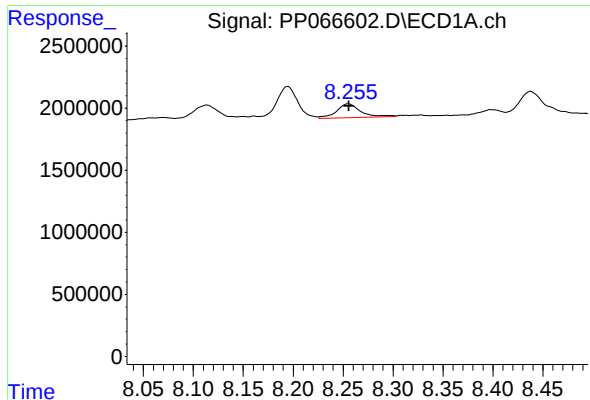

#36 AR-1262-1


R.T.: 8.255 min
Delta R.T.: 0.000 min
Response: 1901431
Conc: 30.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

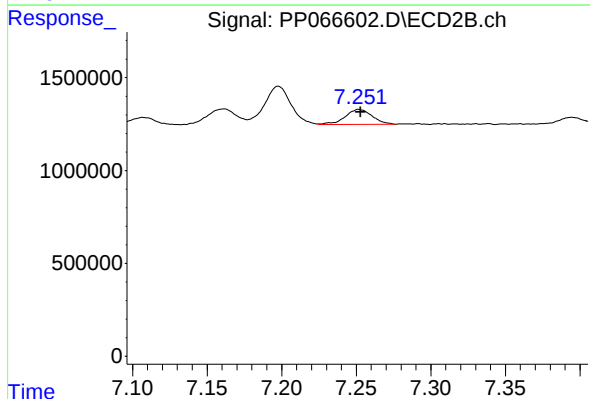


#36 AR-1262-1

R.T.: 7.252 min
Delta R.T.: -0.001 min
Response: 1009706
Conc: 19.94 ng/ml

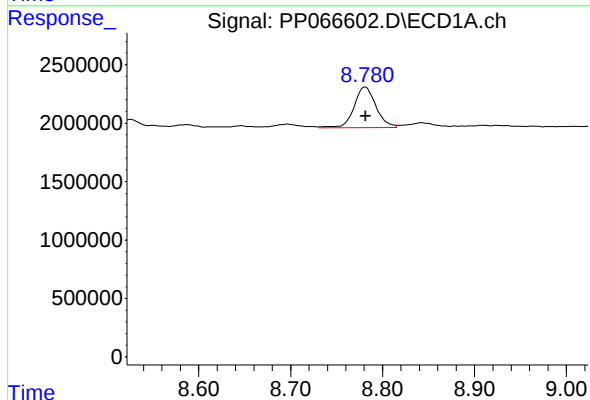


#37 AR-1262-2

R.T.: 8.781 min
Delta R.T.: 0.000 min
Response: 5731907
Conc: 23.43 ng/ml

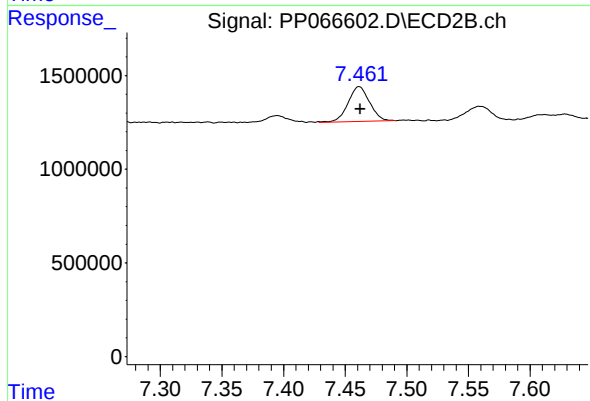

#37 AR-1262-2


R.T.: 7.461 min
Delta R.T.: -0.001 min
Response: 2253152
Conc: 21.09 ng/ml

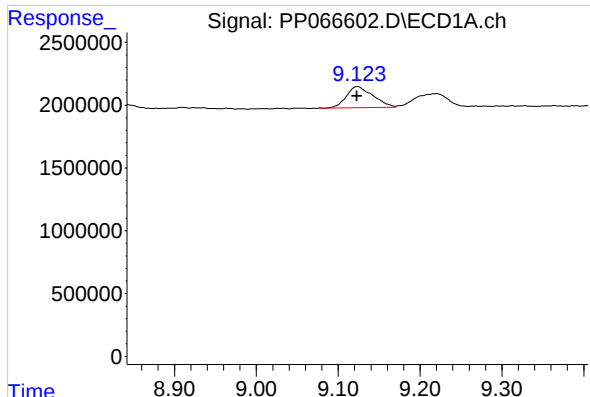

#38 AR-1262-3


R.T.: 9.124 min
Delta R.T.: 0.000 min
Response: 3777001
Conc: 21.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

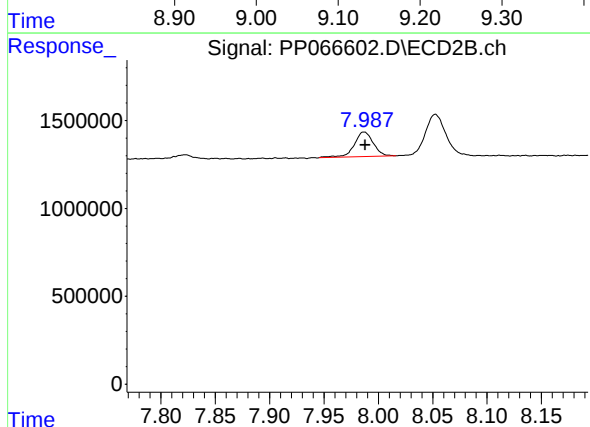


#38 AR-1262-3

R.T.: 7.987 min
Delta R.T.: -0.001 min
Response: 1724328
Conc: 19.75 ng/ml

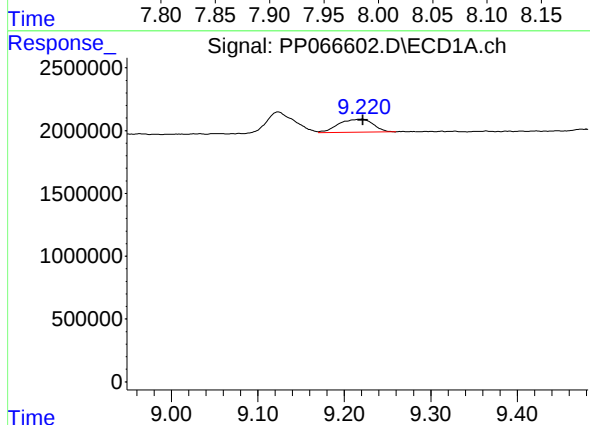


#39 AR-1262-4

R.T.: 9.220 min
Delta R.T.: -0.002 min
Response: 2887219
Conc: 19.63 ng/ml

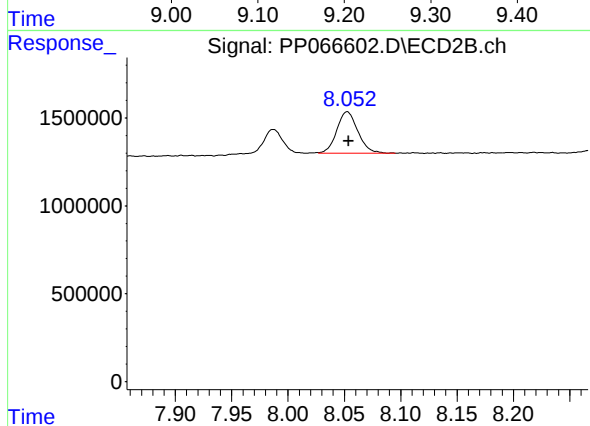

#39 AR-1262-4


R.T.: 8.052 min
Delta R.T.: -0.001 min
Response: 3097228
Conc: 19.96 ng/ml

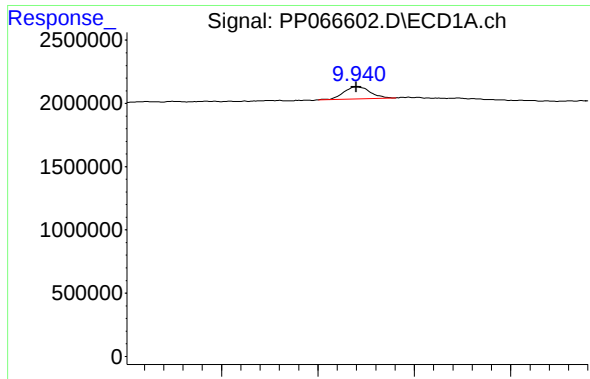

#40 AR-1262-5

R.T.: 9.940 min
Delta R.T.: 0.000 min
Response: 1807728
Conc: 19.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2024

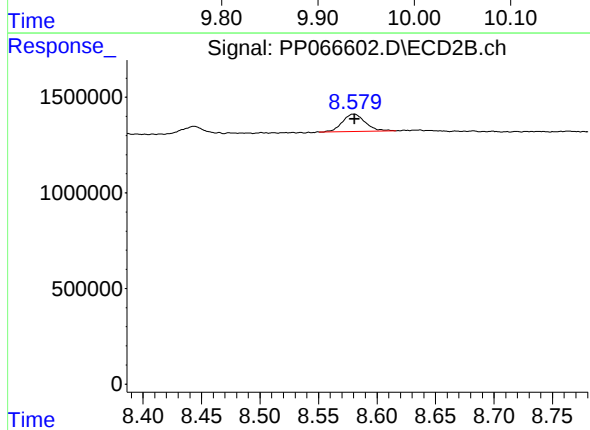

#40 AR-1262-5

R.T.: 8.580 min
Delta R.T.: 0.000 min
Response: 1220480
Conc: 18.58 ng/ml