

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080718\
 Data File : PP026994.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Aug 2018 22:49
 Operator : EI\MA
 Sample : J4327-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-BPM-02-007-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 01:08:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP073018.M
 Quant Title : 8080.M
 QLast Update : Tue Jul 31 01:31:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.043	12.156	73493100	103.5E6	307.731	255.562
Target Compounds							
3) T	4-Nitroph...	11.597	11.300	10171585	8191875	22.176	33.817 #
5) T	DICAMBA	0.000	12.495	0	15902321	N.D.	9.772 #
6) T	MCPP	12.725	0.000	5755692	0	14.835	N.D. #
10) T	Pentachlo...	14.293	0.000	8900857	0	1.169	N.D. #
13) T	2,4-DB	16.352	0.000	59032038	0	269.964	N.D. #
14) T	DINOSEB	17.863	16.940	70516053	36430160	34.867	20.185 #
15) T	Picloram	17.564	0.000	49374305	0	11.955	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080718\
Data File : PP026994.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Aug 2018 22:49
Operator : EI\MA
Sample : J4327-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FK-BPM-02-007-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 01:08:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP073018.M
Quant Title : 8080.M
QLast Update : Tue Jul 31 01:31:14 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

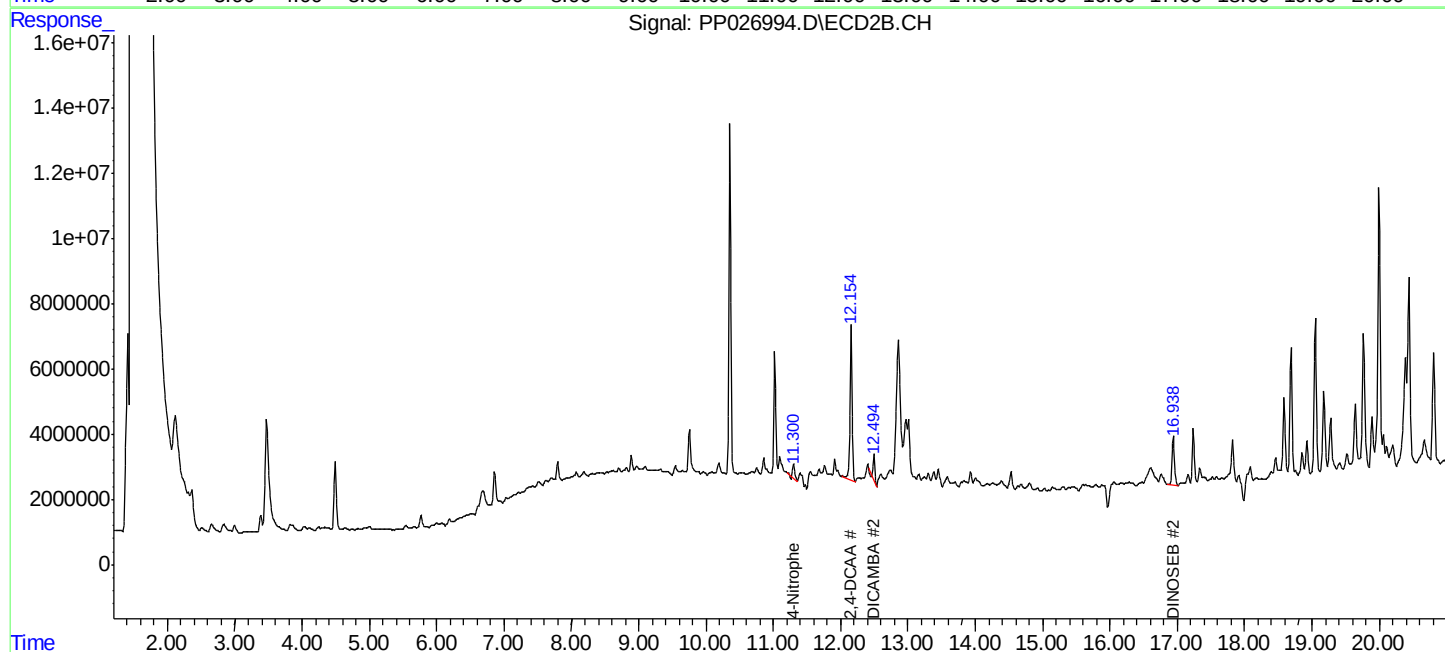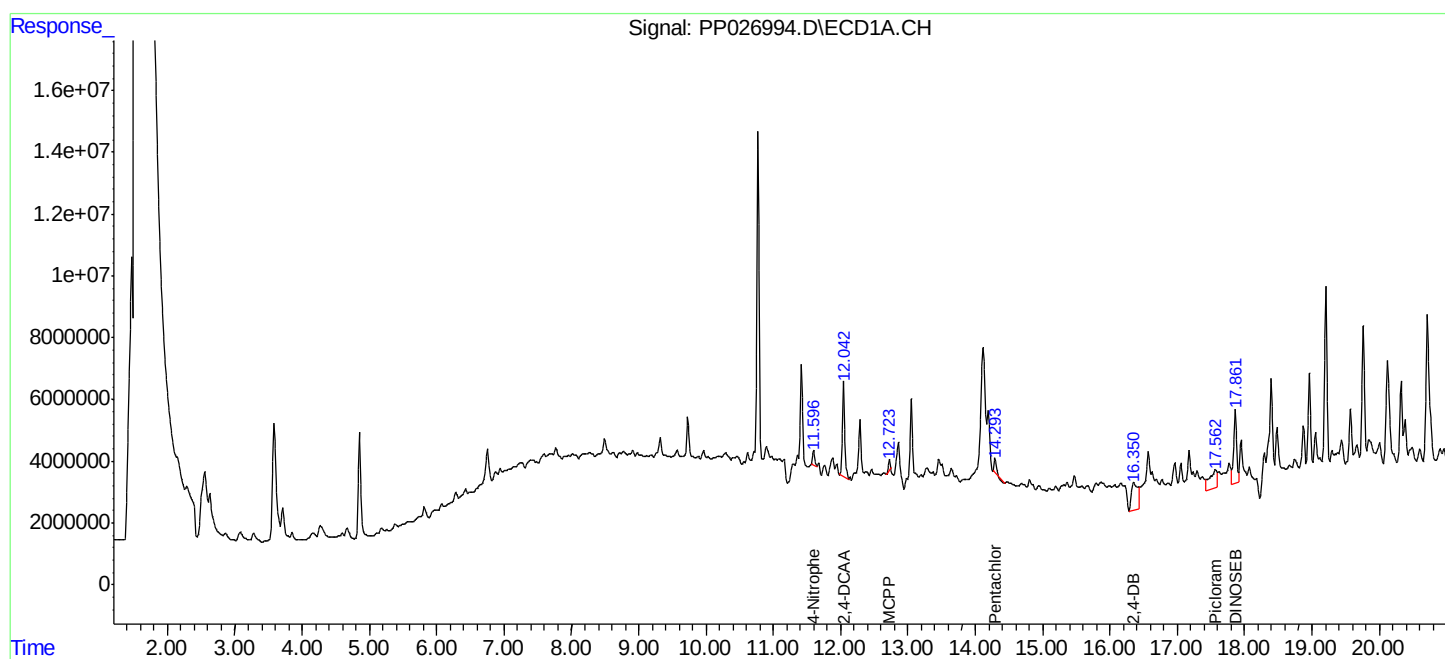


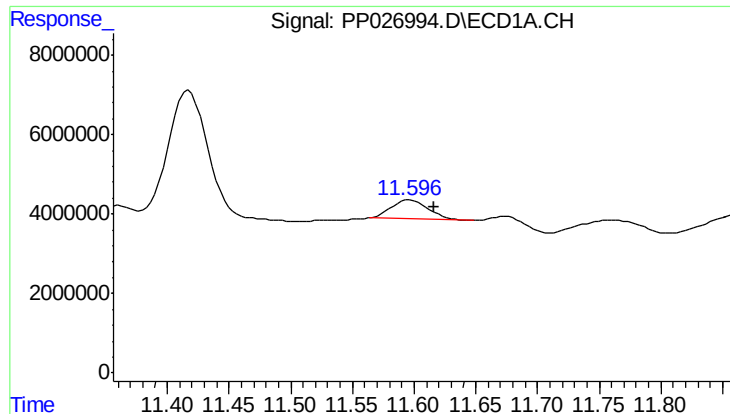

#3 4-Nitrophenol


R.T.: 11.597 min
Delta R.T.: -0.019 min
Response: 10171585
Conc: 22.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-02-007-ABCD

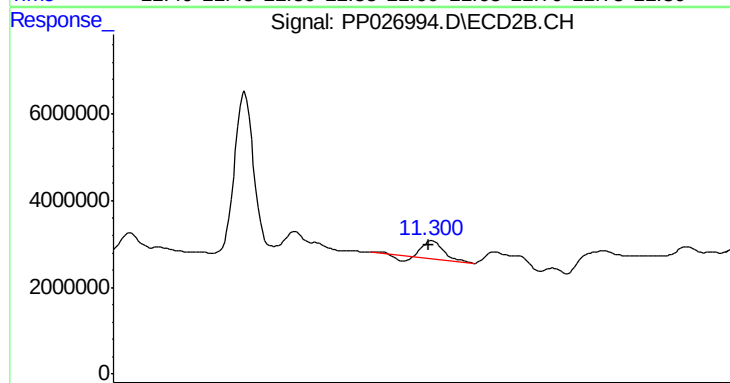


#3 4-Nitrophenol

R.T.: 11.300 min
Delta R.T.: 0.005 min
Response: 8191875
Conc: 33.82 ng/ml

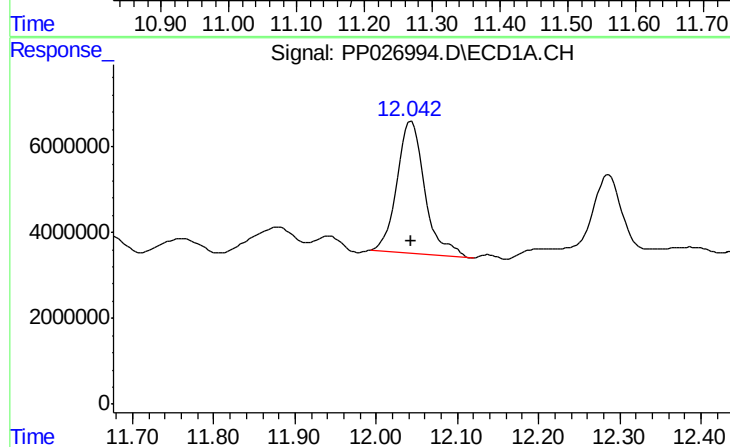


#4 2,4-DCAA

R.T.: 12.043 min
Delta R.T.: 0.000 min
Response: 73493100
Conc: 307.73 ng/ml

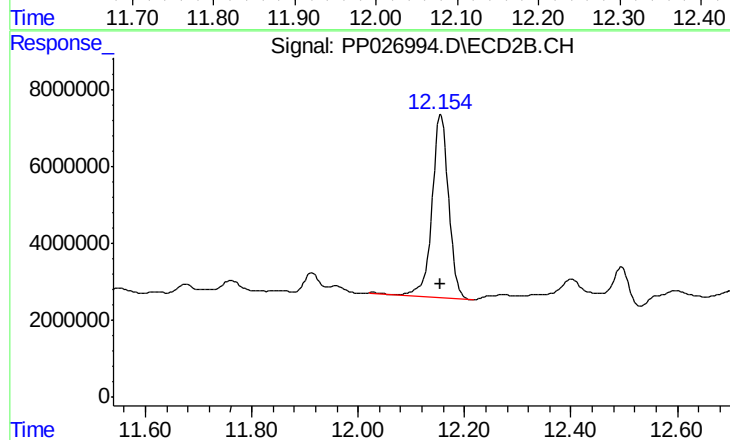

#4 2,4-DCAA


R.T.: 12.156 min
Delta R.T.: 0.000 min
Response: 103485063
Conc: 255.56 ng/ml

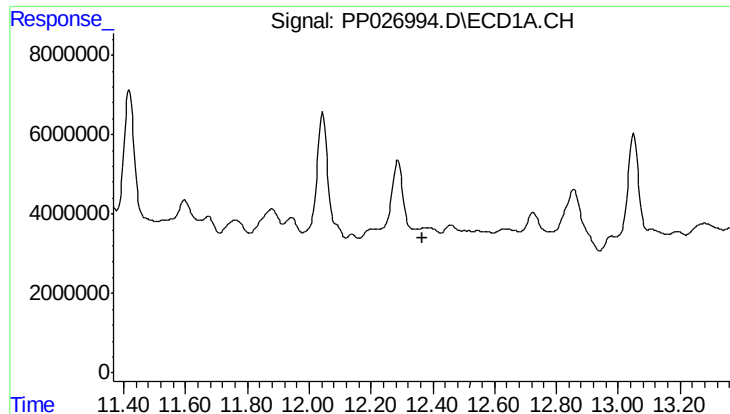

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 12.365 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-BPM-02-007-ABCD

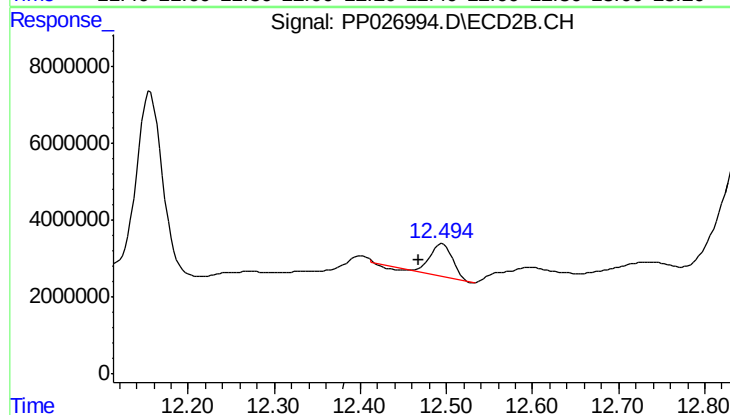


#5 DICAMBA

R.T.: 12.495 min
Delta R.T.: 0.028 min
Response: 15902321
Conc: 9.77 ng/ml

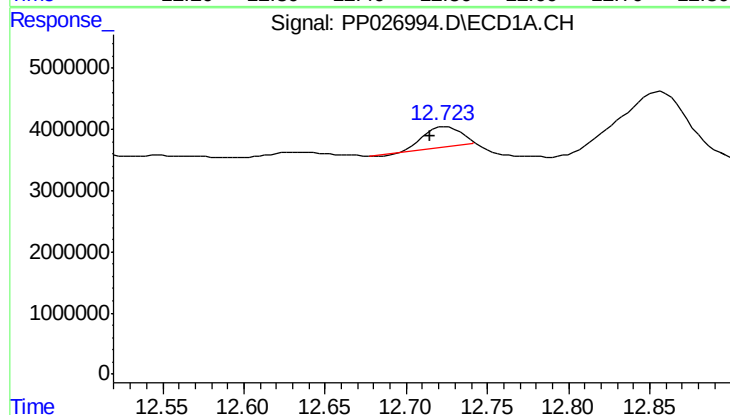


#6 MCP

R.T.: 12.725 min
Delta R.T.: 0.010 min
Response: 5755692
Conc: 14.84 ug/ml

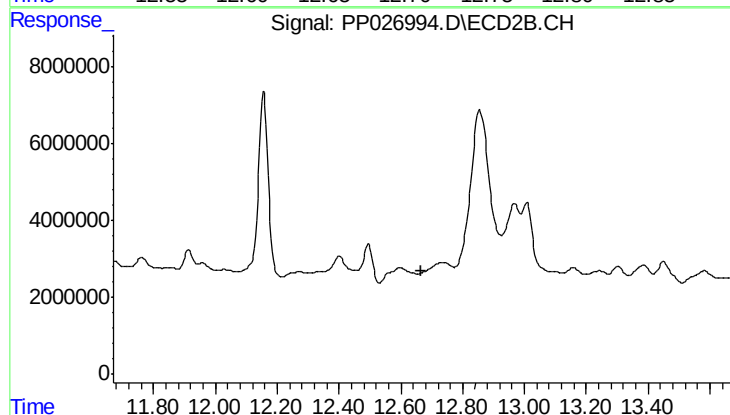

#6 MCP


R.T.: 0.000 min
Exp R.T.: 12.667 min
Response: 0
Conc: N.D.

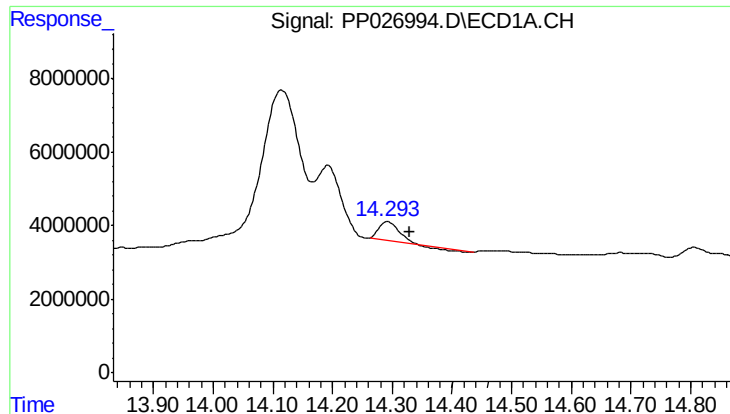

#10 Pentachlorophenol


R.T.: 14.293 min
Delta R.T.: -0.035 min
Response: 8900857
Conc: 1.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-02-007-ABCD

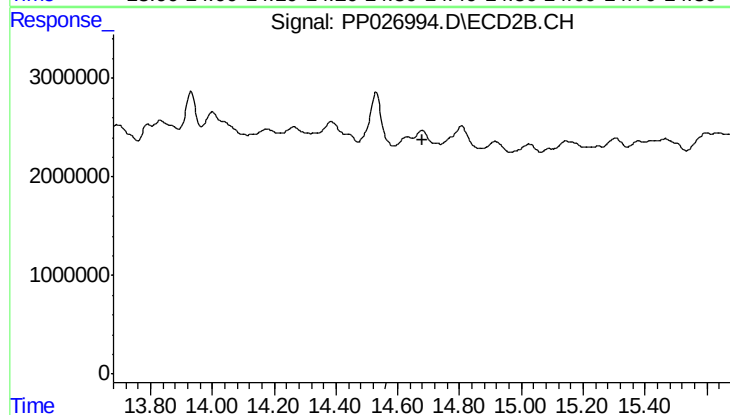


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 14.679 min
Response: 0
Conc: N.D.

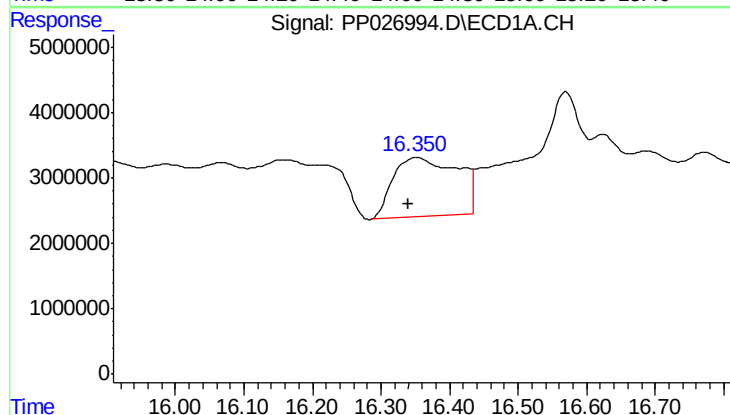


#13 2,4-DB

R.T.: 16.352 min
Delta R.T.: 0.013 min
Response: 59032038
Conc: 269.96 ng/ml

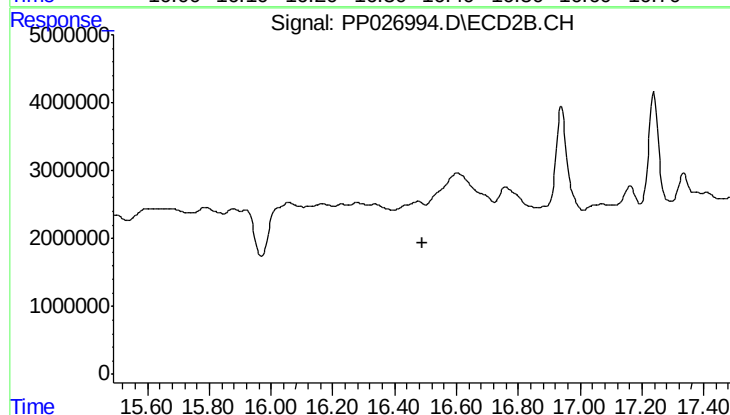

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.489 min
Response: 0
Conc: N.D.

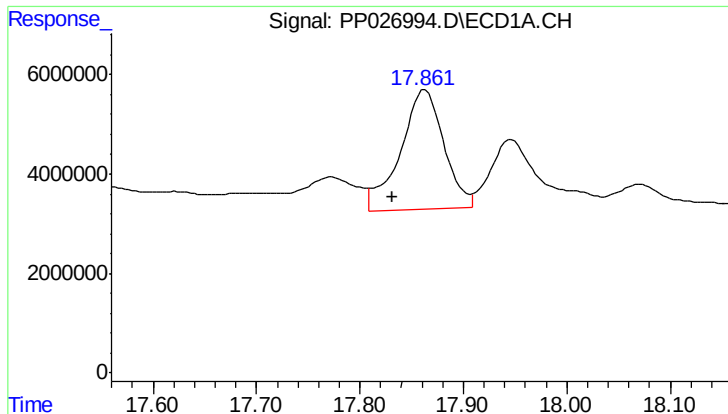

#14 DINOSEB


R.T.: 17.863 min
Delta R.T.: 0.032 min
Response: 70516053
Conc: 34.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-02-007-ABCD

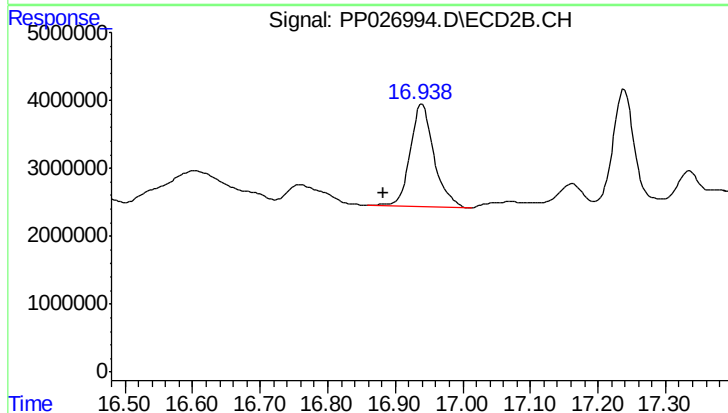


#14 DINOSEB

R.T.: 16.940 min
Delta R.T.: 0.057 min
Response: 36430160
Conc: 20.19 ng/ml

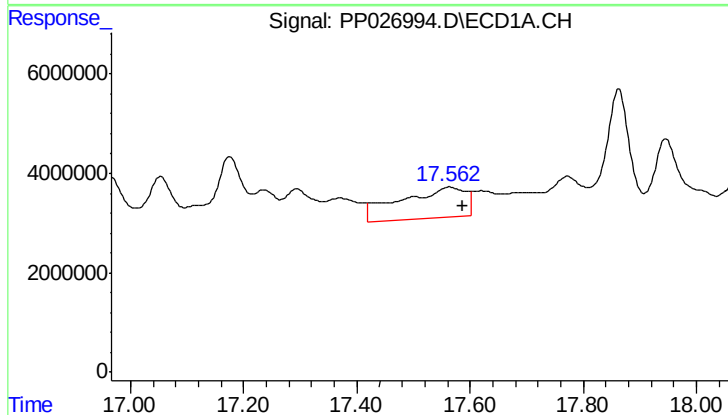

#15 Picloram

R.T.: 17.564 min
Delta R.T.: -0.023 min
Response: 49374305
Conc: 11.96 ng/ml

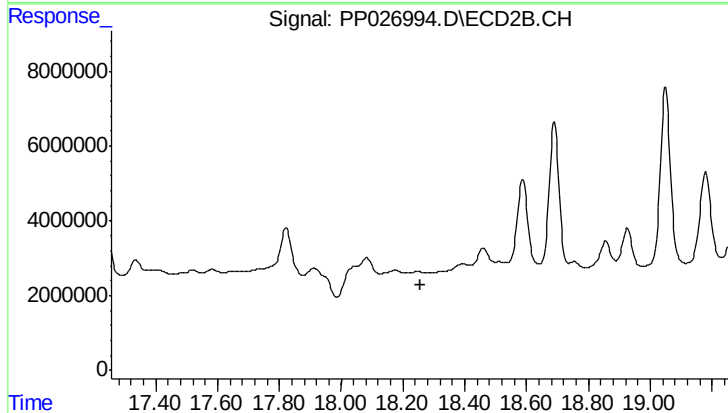

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 18.255 min
Response: 0
Conc: N.D.