

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080725\
 Data File : PP074268.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2025 10:38
 Operator : YP\AJ
 Sample : Q2775-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 60273

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/08/2025
 Supervised By :mohammad ahmed 08/11/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 05:29:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.658	3.776f	13450705	411.9E6	12.028	107.425m#
2) SA Decachlor...	10.434	8.820	11823502	69185899	12.175	11.505

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080725\
Data File : PP074268.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2025 10:38
Operator : YP\AJ
Sample : Q2775-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
60273


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2025
Supervised By :mohammad ahmed 08/11/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 05:29:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 04 11:01:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

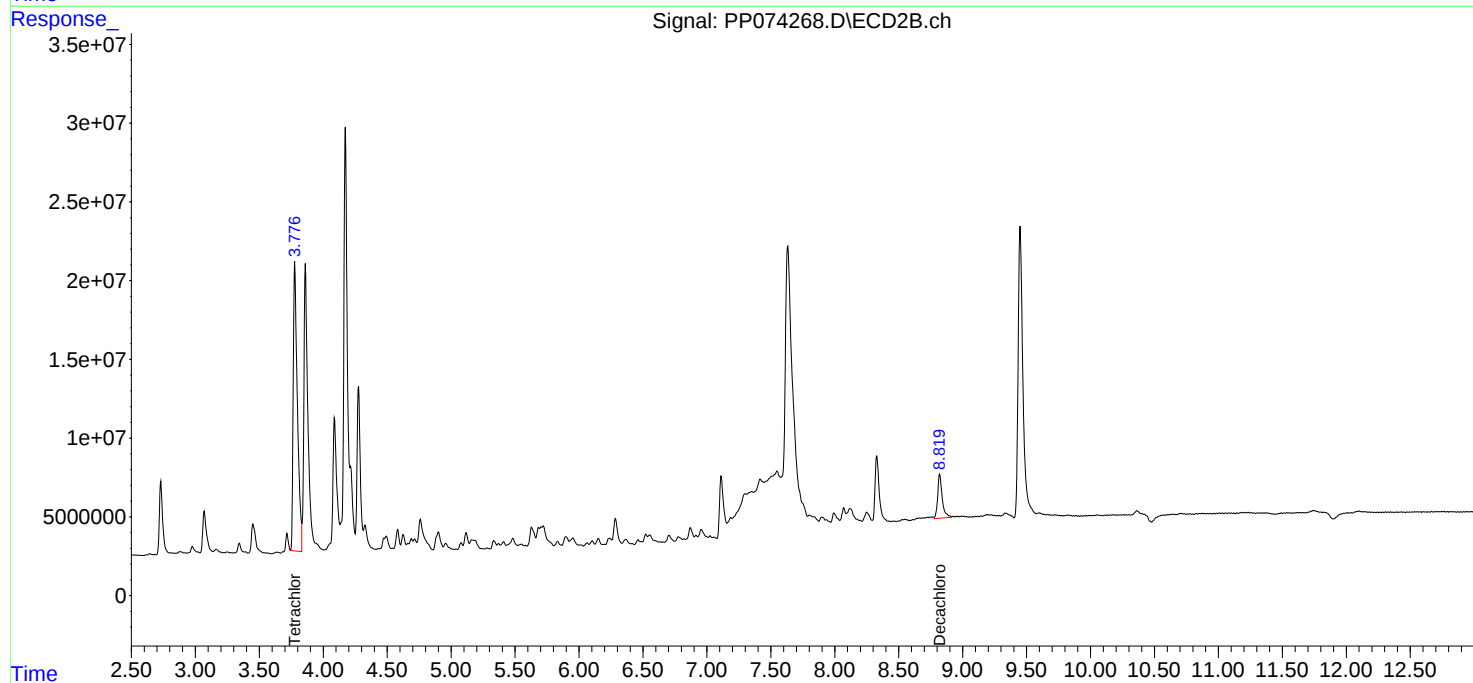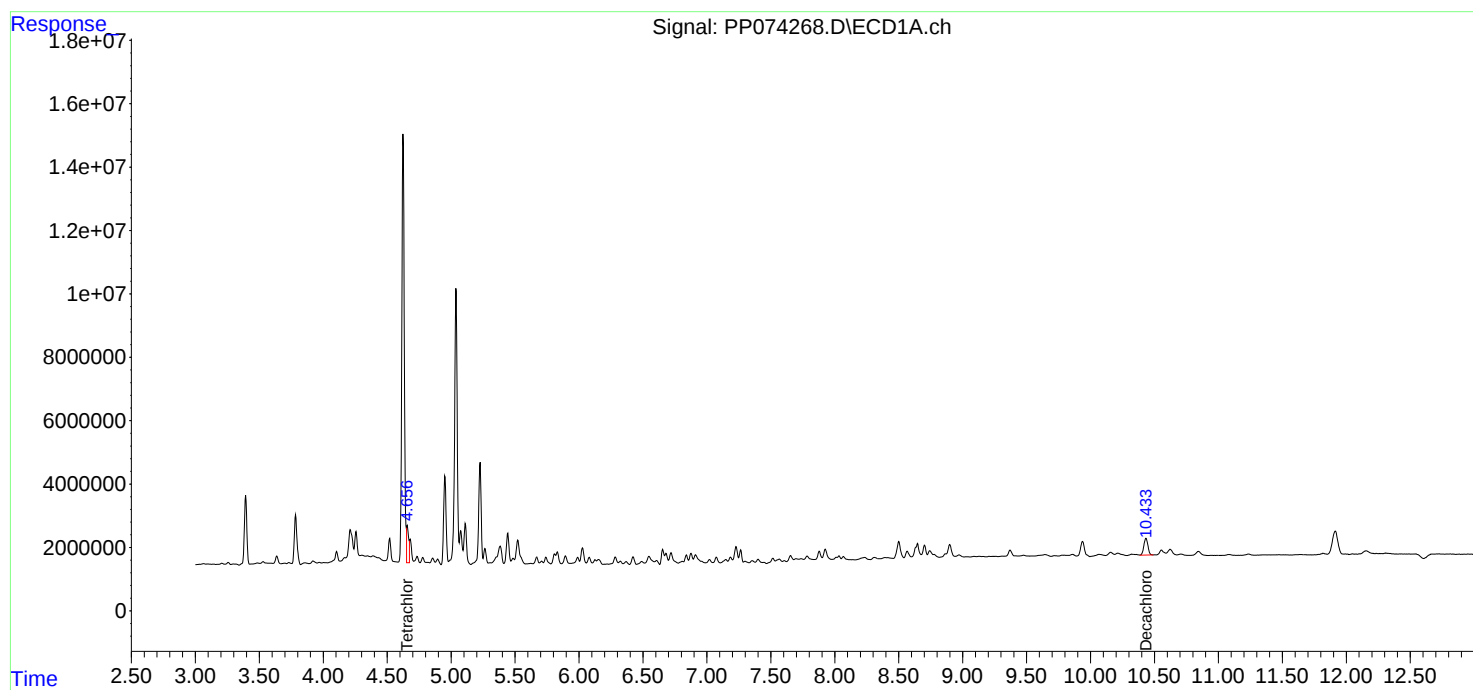

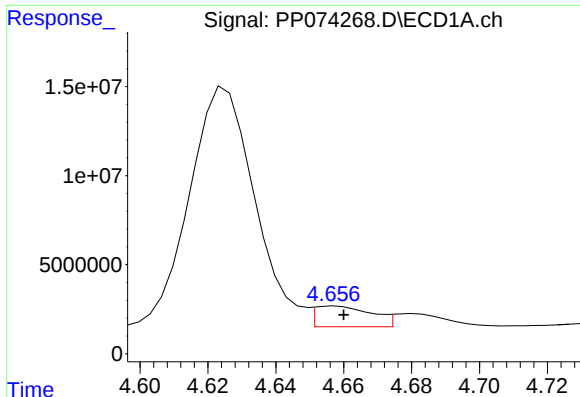


#1 Tetrachloro-m-xylene

R.T.: 4.658 min
Delta R.T.: -0.002 min
Response: 13450705
Conc: 12.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
60273


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2025
Supervised By :mohammad ahmed 08/11/2025

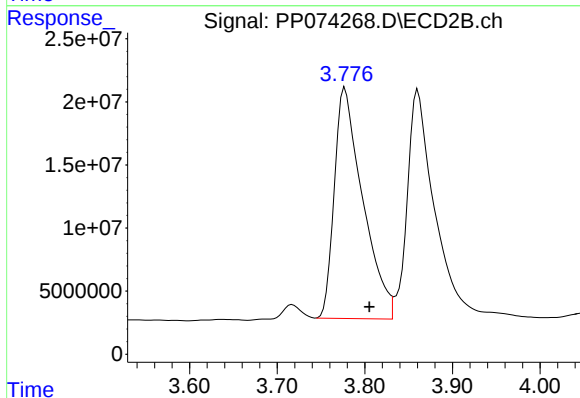


#1 Tetrachloro-m-xylene

R.T.: 3.776 min
Delta R.T.: -0.029 min
Response: 411913540
Conc: 107.43 ng/ml m

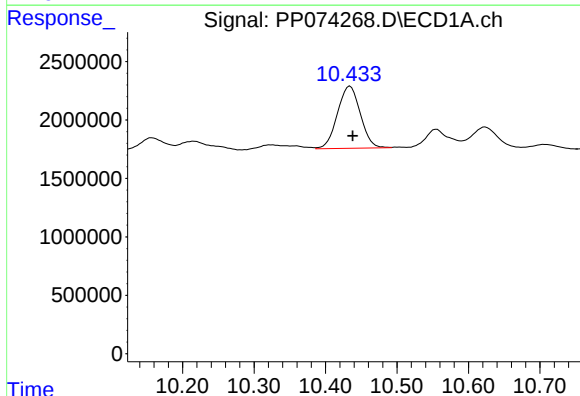

#2 Decachlorobiphenyl

R.T.: 10.434 min
Delta R.T.: -0.004 min
Response: 11823502
Conc: 12.17 ng/ml

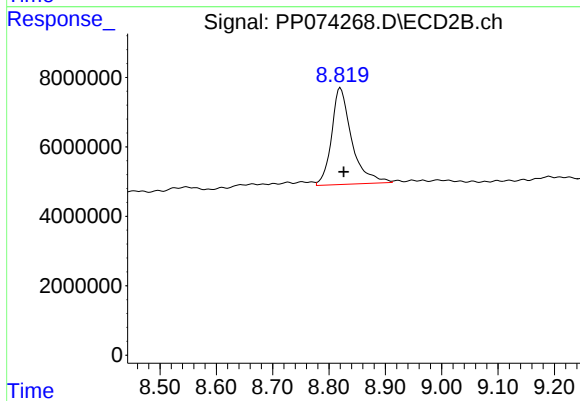

#2 Decachlorobiphenyl

R.T.: 8.820 min
Delta R.T.: -0.006 min
Response: 69185899
Conc: 11.50 ng/ml