

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080822\
 Data File : PP050305.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2022 12:27
 Operator : YP\AJ
 Sample : PB146746BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 03:02:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Aug 07 23:52:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.347	3.593	37619634	72015740	23.371	22.992
2)	SA Decachlor...	10.095	8.558	40969316	34216588	23.266	22.232
Target Compounds							
9)	L2 AR-1221-2	0.000	3.890	0	929196	N.D.	32.540 #
20)	L4 AR-1242-5	0.000	5.485f	0	270448	N.D.	3.891 #
25)	L5 AR-1248-5	0.000	5.485	0	270448	N.D.	2.724 #
26)	L6 AR-1254-1	0.000	5.485f	0	270448	N.D.	2.047 #
32)	L7 AR-1260-2	0.000	6.313	0	754415	N.D.	5.616 #
38)	L8 AR-1262-3	0.000	7.480	0	78599	N.D.	1.083 #
41)	L9 AR-1268-1	0.000	7.480	0	78599	N.D.	0.358 #
45)	L9 AR-1268-5	9.785f	8.313	5357061	118687	8.032	0.216 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080822\
Data File : PP050305.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2022 12:27
Operator : YP\AJ
Sample : PB146746BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 03:02:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Aug 07 23:52:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

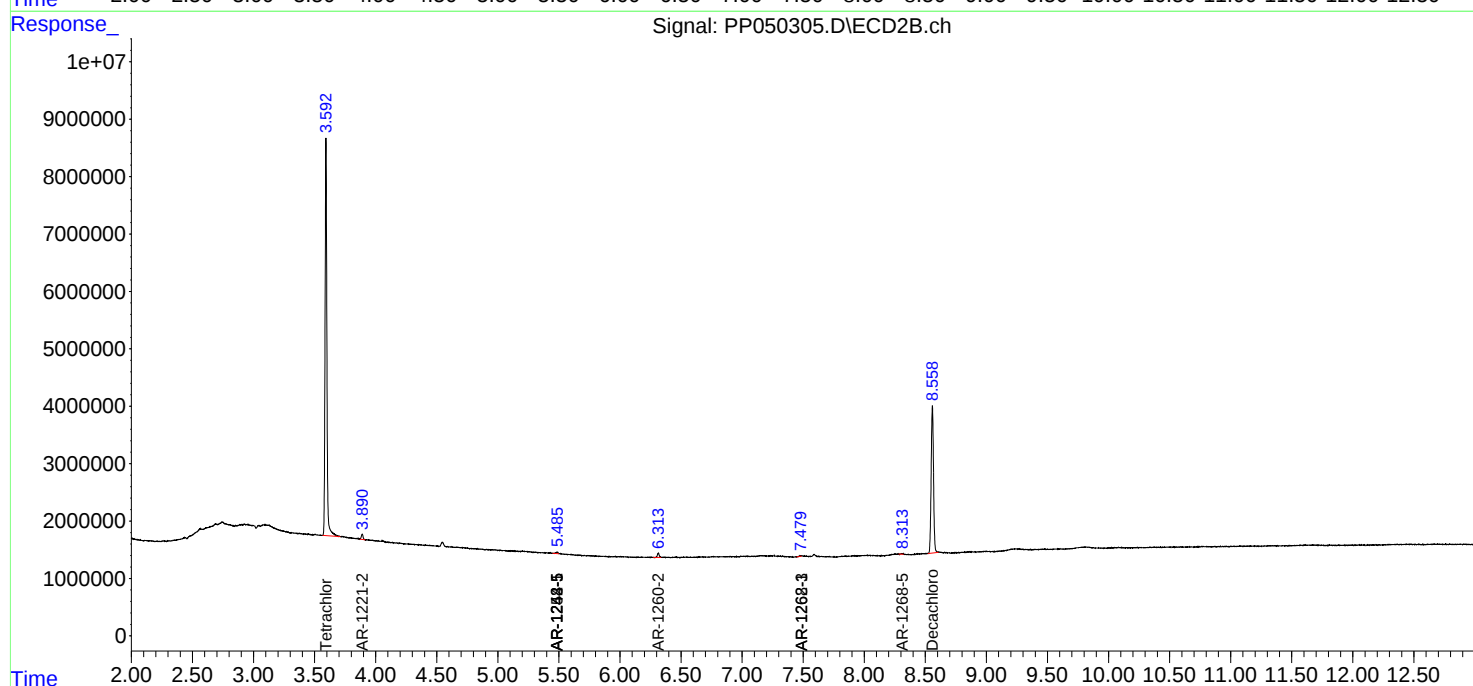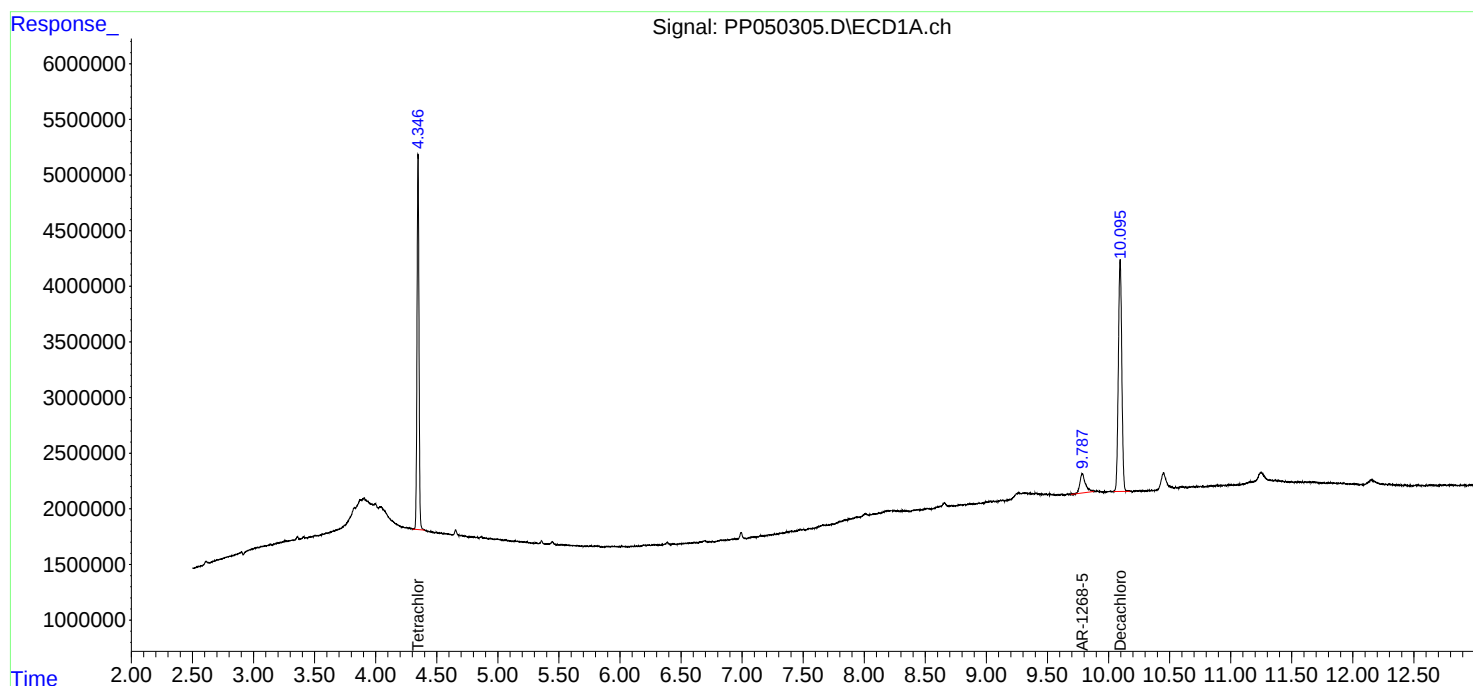


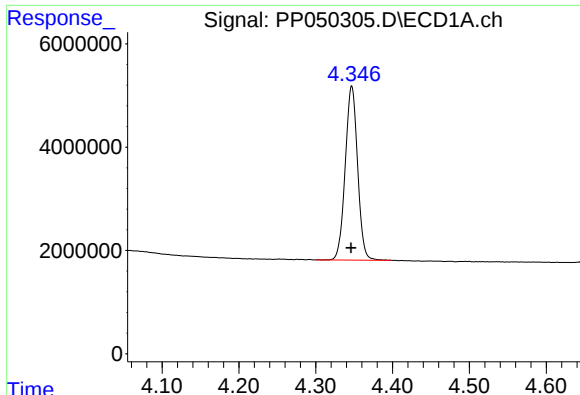

#1 Tetrachloro-m-xylene


R.T.: 4.347 min
Delta R.T.: 0.000 min
Response: 37619634
Conc: 23.37 ng/ml

Instrument :
ECD_P
ClientSampleId :

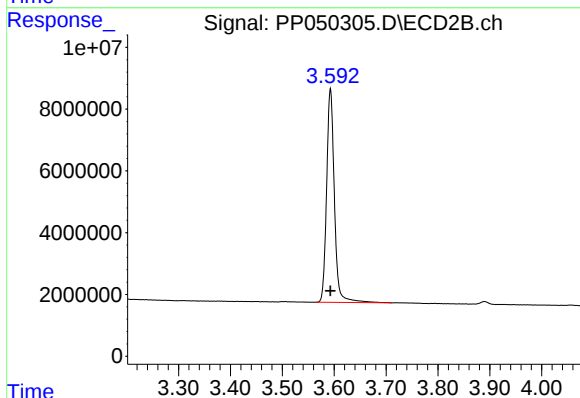


#1 Tetrachloro-m-xylene

R.T.: 3.593 min
Delta R.T.: 0.000 min
Response: 72015740
Conc: 22.99 ng/ml

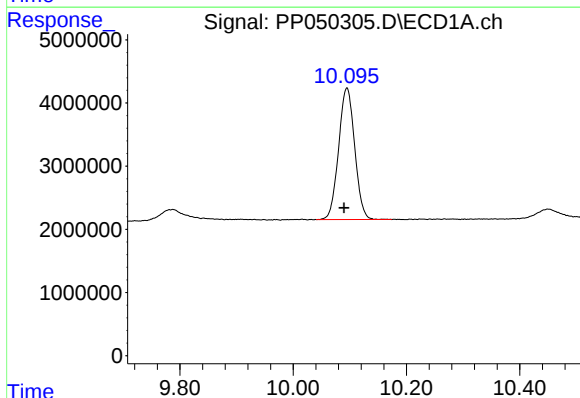


#2 Decachlorobiphenyl

R.T.: 10.095 min
Delta R.T.: 0.005 min
Response: 40969316
Conc: 23.27 ng/ml

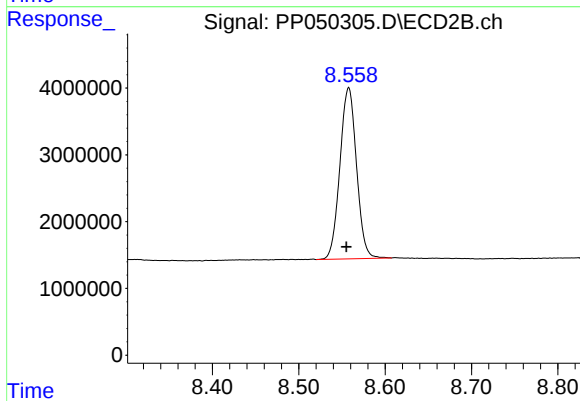

#2 Decachlorobiphenyl


R.T.: 8.558 min
Delta R.T.: 0.003 min
Response: 34216588
Conc: 22.23 ng/ml

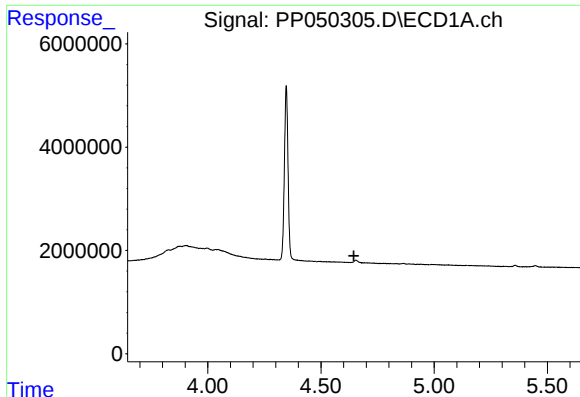

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.646 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

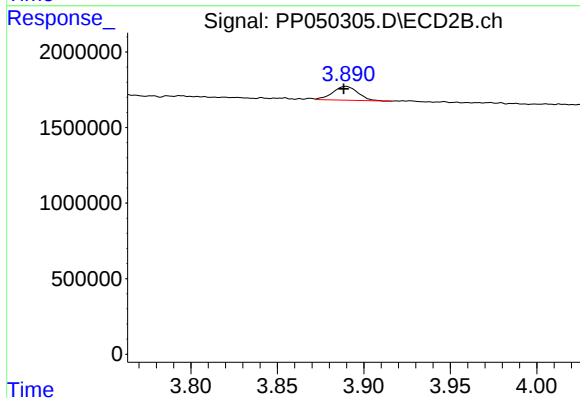


#9 AR-1221-2

R.T.: 3.890 min
Delta R.T.: 0.002 min
Response: 929196
Conc: 32.54 ng/ml

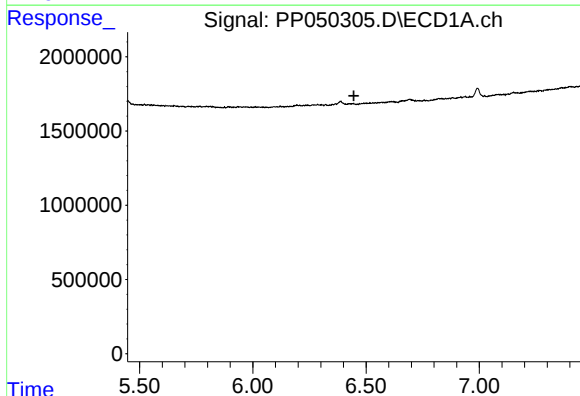


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.446 min
Response: 0
Conc: N.D.

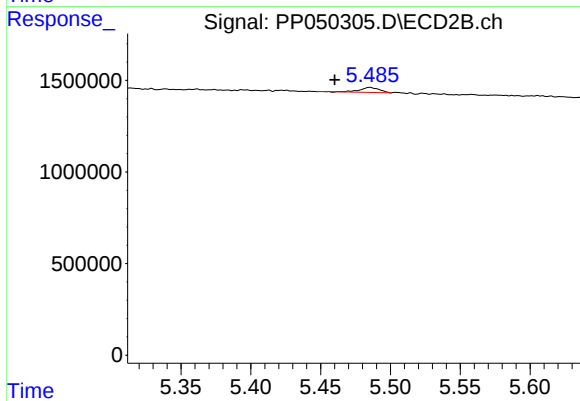

#20 AR-1242-5


R.T.: 5.485 min
Delta R.T.: 0.025 min
Response: 270448
Conc: 3.89 ng/ml

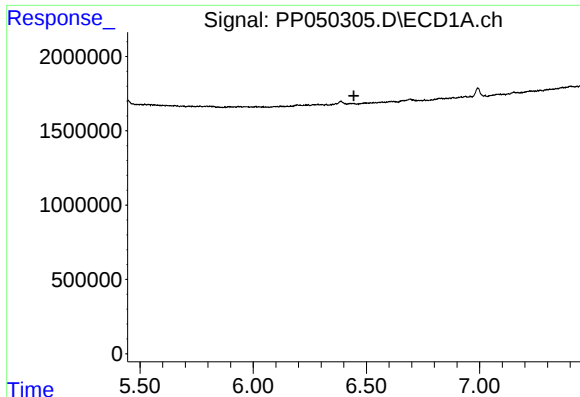

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.445 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

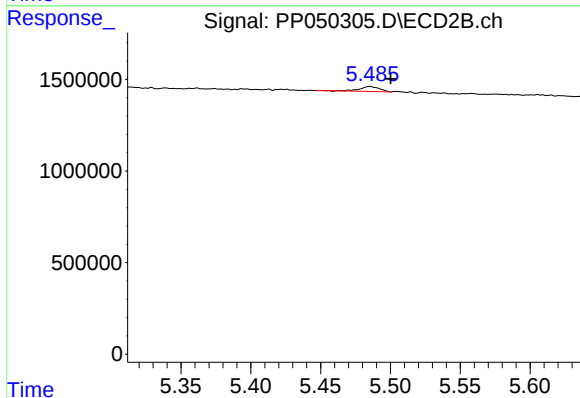


#25 AR-1248-5

R.T.: 5.485 min
Delta R.T.: -0.015 min
Response: 270448
Conc: 2.72 ng/ml

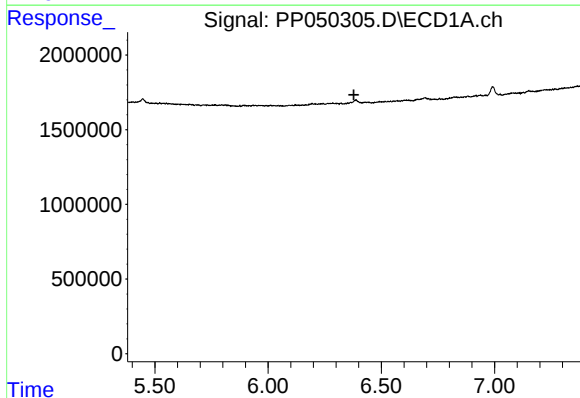


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.379 min
Response: 0
Conc: N.D.

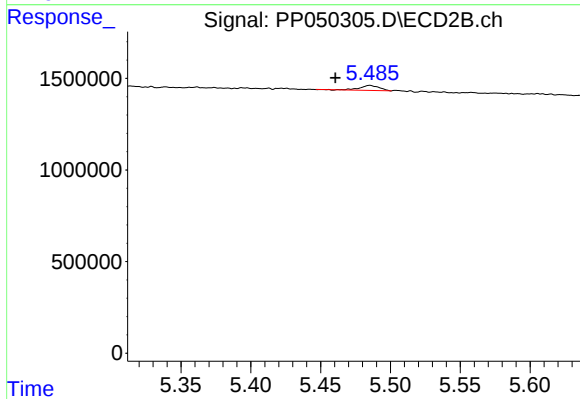

#26 AR-1254-1


R.T.: 5.485 min
Delta R.T.: 0.025 min
Response: 270448
Conc: 2.05 ng/ml

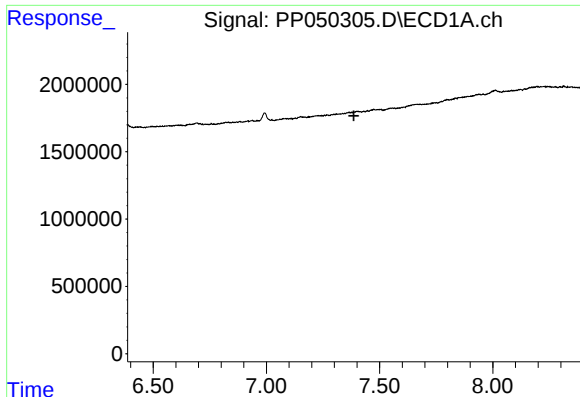

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.386 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

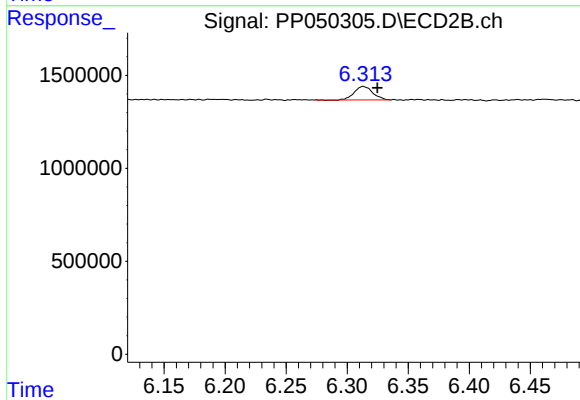


#32 AR-1260-2

R.T.: 6.313 min
Delta R.T.: -0.012 min
Response: 754415
Conc: 5.62 ng/ml

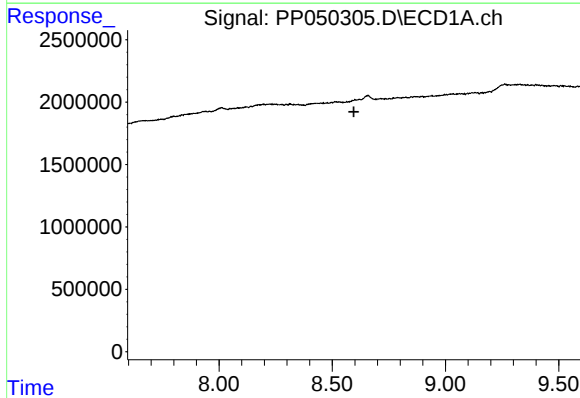


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.596 min
Response: 0
Conc: N.D.

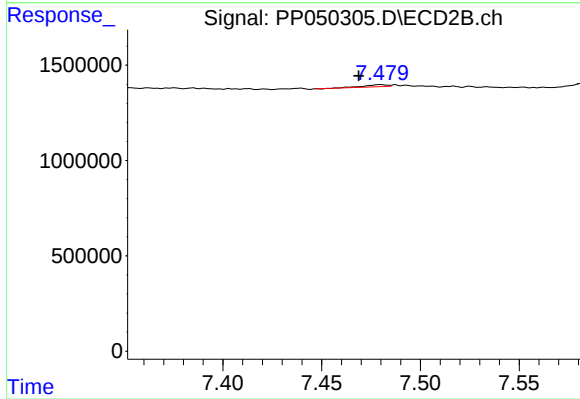

#38 AR-1262-3


R.T.: 7.480 min
Delta R.T.: 0.011 min
Response: 78599
Conc: 1.08 ng/ml

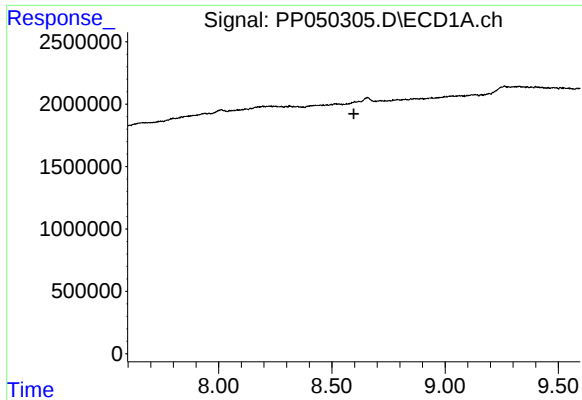

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.597 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

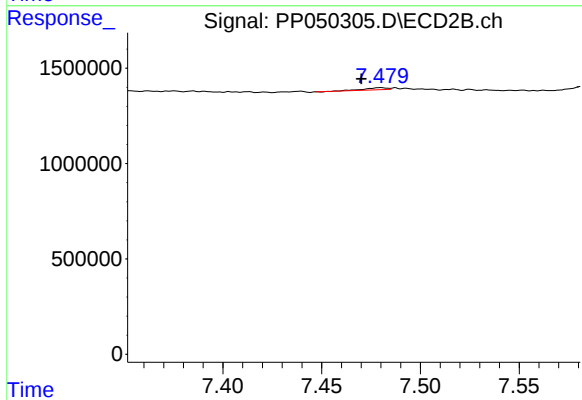


#41 AR-1268-1

R.T.: 7.480 min
Delta R.T.: 0.010 min
Response: 78599
Conc: 0.36 ng/ml

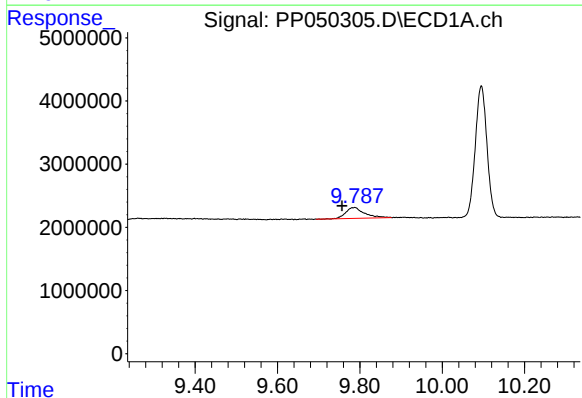

#45 AR-1268-5

R.T.: 9.785 min
Delta R.T.: 0.028 min
Response: 5357061
Conc: 8.03 ng/ml

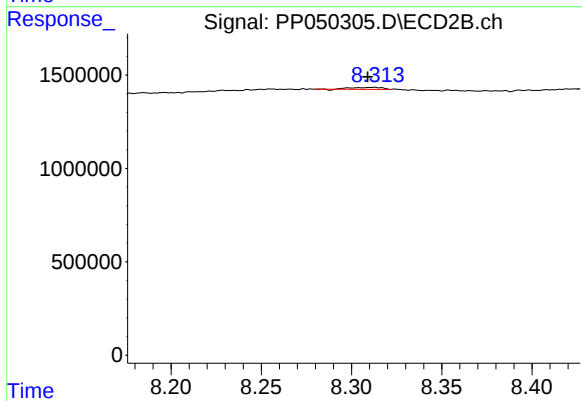

#45 AR-1268-5

R.T.: 8.313 min
Delta R.T.: 0.004 min
Response: 118687
Conc: 0.22 ng/ml