

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
 Data File : PP059217.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2023 22:54
 Operator : YP\AJ
 Sample : 03572-07
 Misc : AR1221 LOD 25 PPB
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 02:40:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.416	3.648	25216609	42552856	20.551	21.002
2)	SA Decachlor...	10.211	8.687	19789126	35246844	25.928	25.054
Target Compounds							
3)	L1 AR-1016-1	5.592	4.743	83125	411910	2.116	6.422 #
4)	L1 AR-1016-2	5.616	4.758	206876	756871	3.649	8.332 #
5)	L1 AR-1016-3	5.672	4.938	196923	123124	5.489	2.563 #
6)	L1 AR-1016-4	5.777	4.989	111038	1032034	3.833	24.994 #
7)	L1 AR-1016-5	6.069	5.193	186090	334691	6.149	6.432
8)	L2 AR-1221-1	4.626	3.865	579340	1153167	36.774	42.480
9)	L2 AR-1221-2	4.724	3.950	1288307	1532199	109.096	76.957 #
10)	L2 AR-1221-3	4.789	4.027	1533402	2378608	43.546	39.954
11)	L3 AR-1232-1	4.789	4.027	1533402	2378608	52.163	50.130
12)	L3 AR-1232-2	5.325	4.758	115938	756871	7.438	17.843 #
13)	L3 AR-1232-3	5.616	4.938	206876	123124	7.835	5.549 #
14)	L3 AR-1232-4	5.777	5.022	111038	488405	8.390	23.131 #
15)	L3 AR-1232-5	5.877	5.193	125812	334691	11.022	14.601 #
16)	L4 AR-1242-1	5.592	4.743	83125	411910	2.428	7.360 #
17)	L4 AR-1242-2	5.616	4.758	206876	756871	4.216	9.492 #
18)	L4 AR-1242-3	5.672	4.938	196923	123124	6.268	2.889 #
19)	L4 AR-1242-4	5.777	5.022	111038	488405	4.330	11.185 #
20)	L4 AR-1242-5	6.515	5.550	170762	628355	6.610	12.650 #
21)	L5 AR-1248-1	5.592	4.743	83125	411910	3.275	10.013 #
22)	L5 AR-1248-2	5.877	4.989	125812	1032034	3.251	17.138 #
23)	L5 AR-1248-3	6.069	5.022	186090	488405	4.405	7.927 #
24)	L5 AR-1248-4	6.477	5.193	218224	334691	5.241	4.649
25)	L5 AR-1248-5	6.515	5.590	170762	392086	4.186	5.942 #
26)	L6 AR-1254-1	6.452	5.550	254320	628355	5.444	6.202
27)	L6 AR-1254-2	6.675	5.696	327723	77837	4.763	0.882 #
28)	L6 AR-1254-3	7.037	6.102	480884	91185	6.967	0.660 #
29)	L6 AR-1254-4	7.334	6.331	42967	98155	0.954	1.221 #
30)	L6 AR-1254-5	7.750	6.753	228822	12998	4.870	0.109 #
31)	L7 AR-1260-1	7.198	6.236	24647	40662	0.451	0.411
32)	L7 AR-1260-2	7.483f	6.424	115320	70739	1.937	0.611 #
33)	L7 AR-1260-3	7.830	6.580	154276	172991	3.920	1.555 #
35)	L7 AR-1260-5	8.385	7.296	24448	147720	0.306	0.801 #
36)	L8 AR-1262-1	7.830	6.841	154276	5510	2.422	0.096 #
37)	L8 AR-1262-2	8.385	7.069f	24448	410294	0.266	3.477 #
38)	L8 AR-1262-3	8.694	7.583	23968	16026	0.372	0.188 #
39)	L8 AR-1262-4	8.775	7.640	26063	57144	0.785	0.378 #
40)	L8 AR-1262-5	9.436	8.141	40650	87483	1.362	1.372
41)	L9 AR-1268-1	8.694	7.583	23968	16026	0.211	0.066 #
42)	L9 AR-1268-2	8.775	7.640	26063	57144	0.265	0.261

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
 Data File : PP059217.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2023 22:54
 Operator : YP\AJ
 Sample : 03572-07
 Misc : AR1221 LOD 25 PPB
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 02:40:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	9.019	7.848	100001	104078	1.079	0.532 #
44) L9	AR-1268-4	9.436	8.141	40650	87483	1.274	1.257
45) L9	AR-1268-5	9.866	8.432	117836	104245	0.434	0.201 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
Data File : PP059217.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2023 22:54
Operator : YP\AJ
Sample : 03572-07
Misc : AR1221 LOD 25 PPB
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 02:40:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

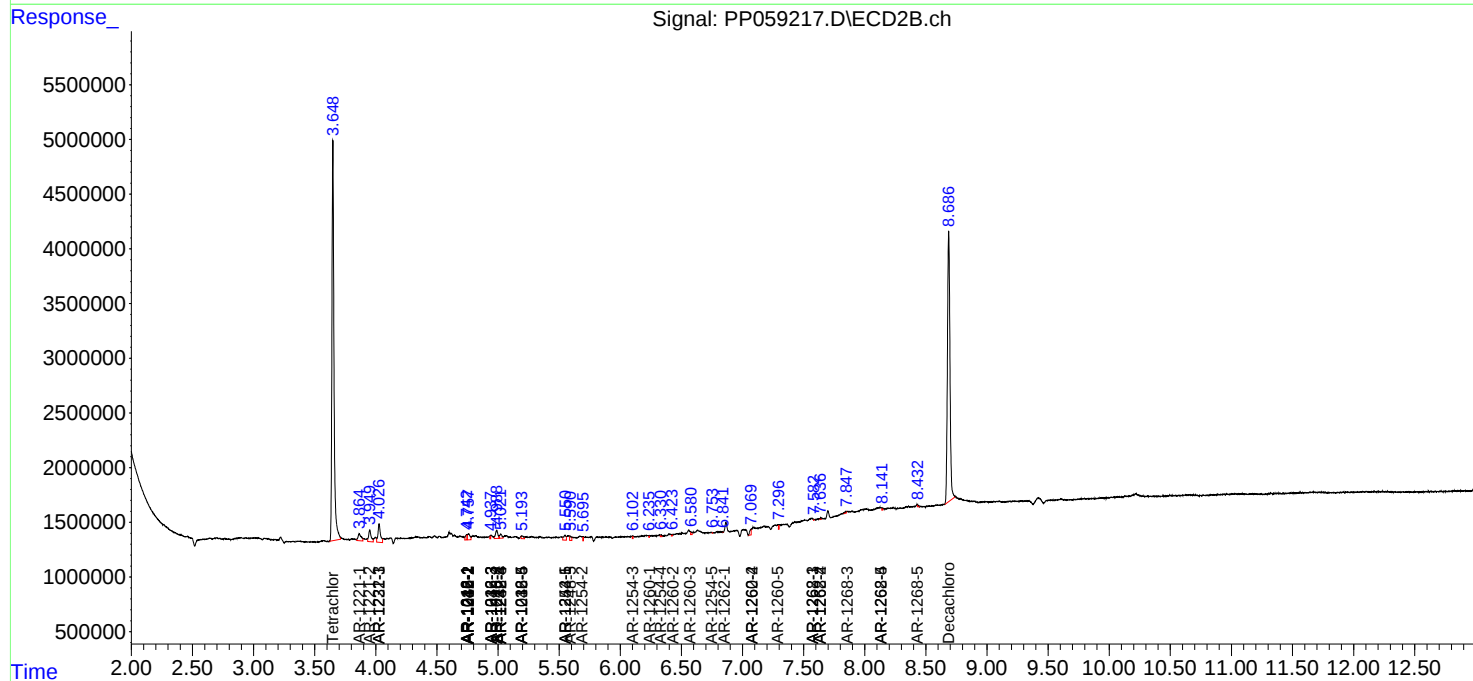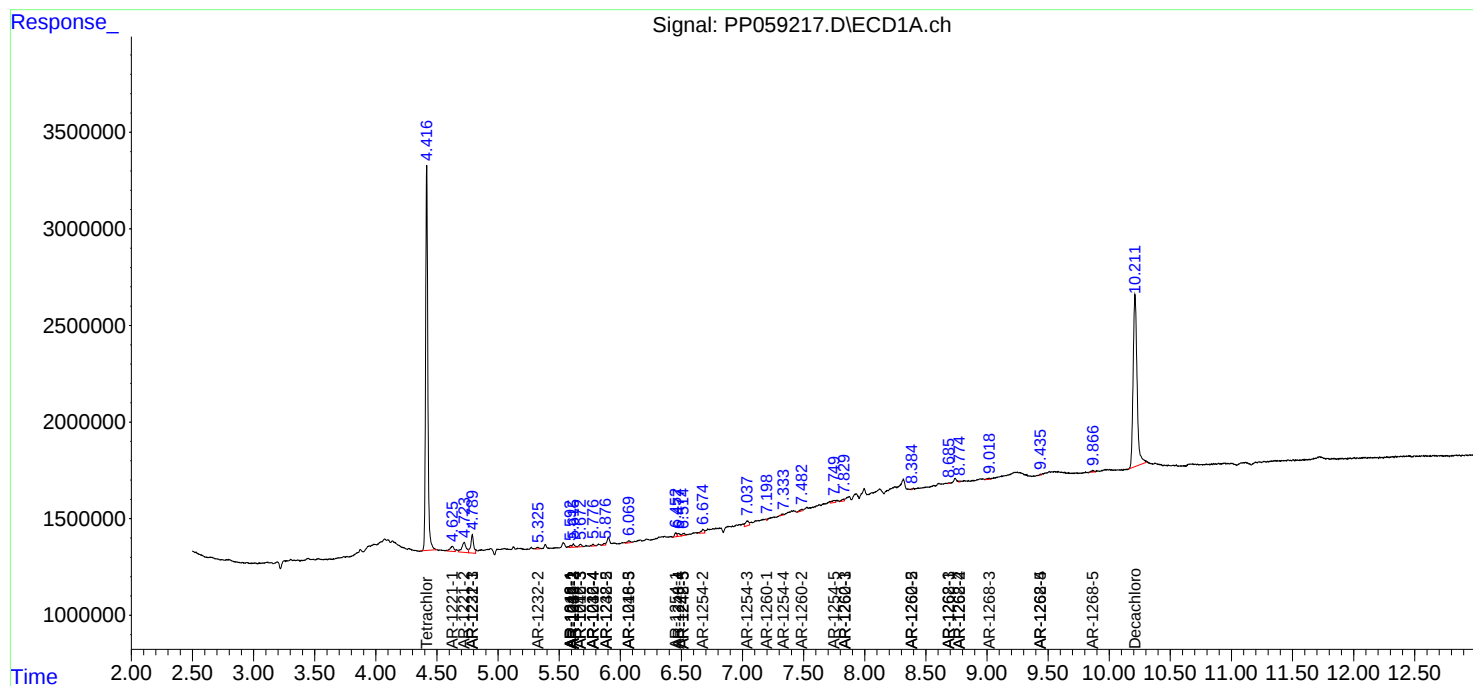


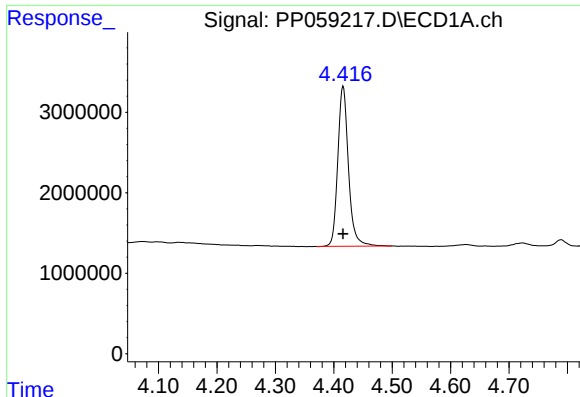

#1 Tetrachloro-m-xylene


R.T.: 4.416 min
Delta R.T.: 0.000 min
Response: 25216609
Conc: 20.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

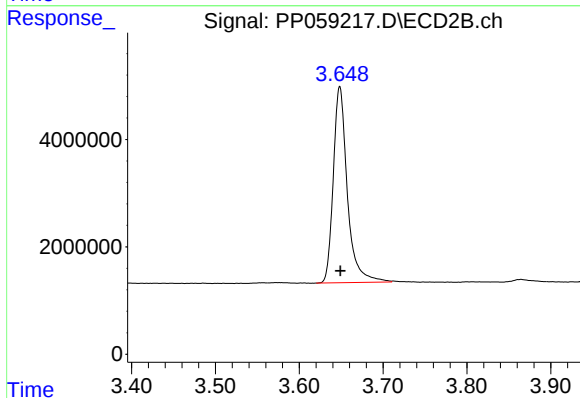


#1 Tetrachloro-m-xylene

R.T.: 3.648 min
Delta R.T.: 0.000 min
Response: 42552856
Conc: 21.00 ng/ml

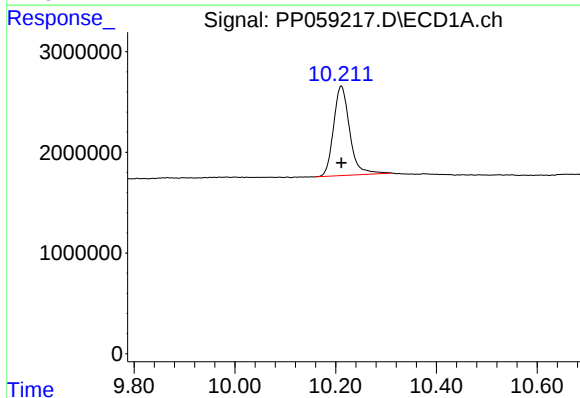


#2 Decachlorobiphenyl

R.T.: 10.211 min
Delta R.T.: 0.000 min
Response: 19789126
Conc: 25.93 ng/ml

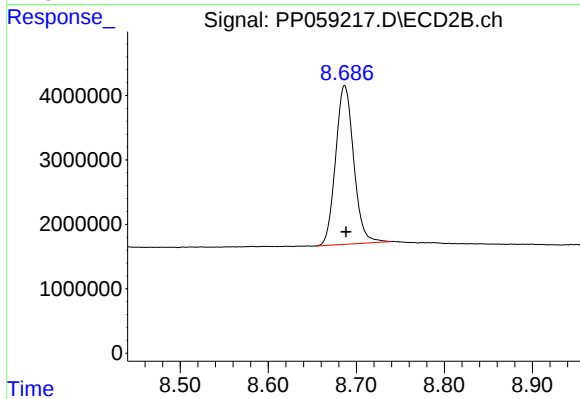

#2 Decachlorobiphenyl


R.T.: 8.687 min
Delta R.T.: -0.002 min
Response: 35246844
Conc: 25.05 ng/ml

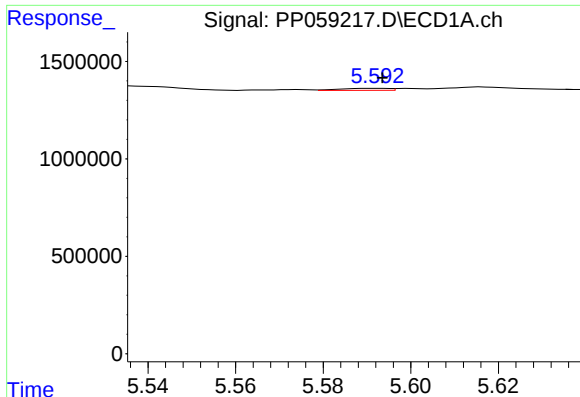

#3 AR-1016-1


R.T.: 5.592 min
Delta R.T.: -0.002 min
Response: 83125
Conc: 2.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

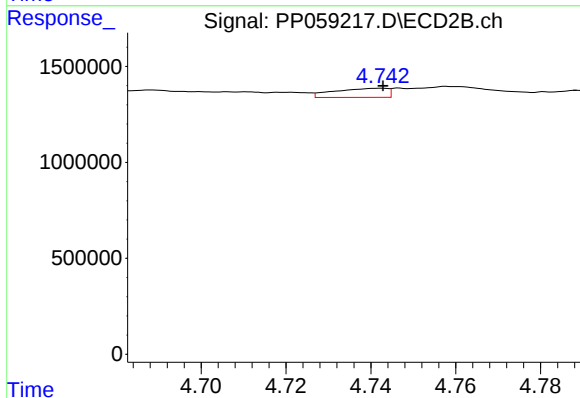


#3 AR-1016-1

R.T.: 4.743 min
Delta R.T.: 0.000 min
Response: 411910
Conc: 6.42 ng/ml

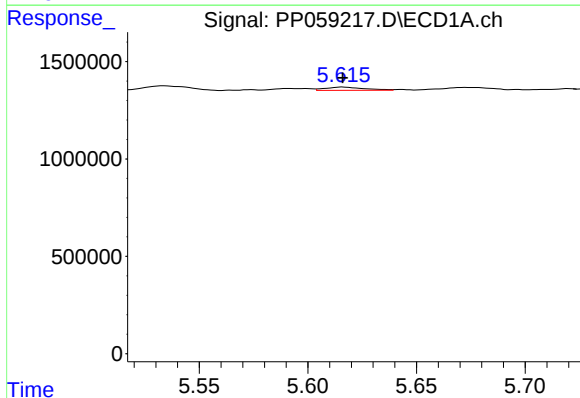


#4 AR-1016-2

R.T.: 5.616 min
Delta R.T.: 0.000 min
Response: 206876
Conc: 3.65 ng/ml

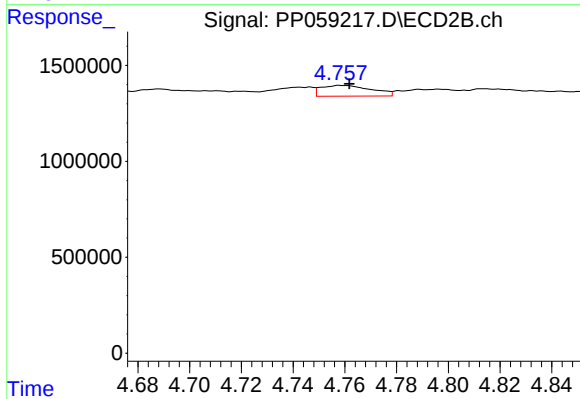

#4 AR-1016-2


R.T.: 4.758 min
Delta R.T.: -0.004 min
Response: 756871
Conc: 8.33 ng/ml

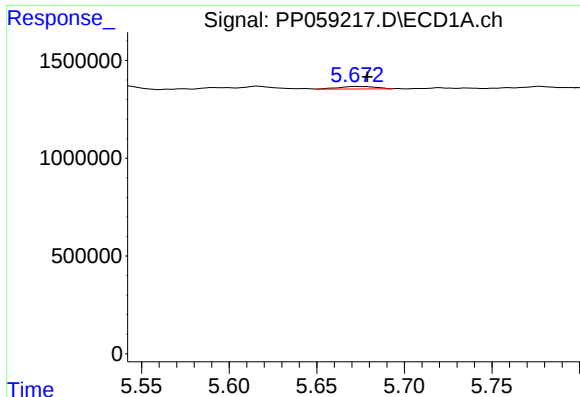

#5 AR-1016-3


R.T.: 5.672 min
Delta R.T.: -0.006 min
Response: 196923
Conc: 5.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

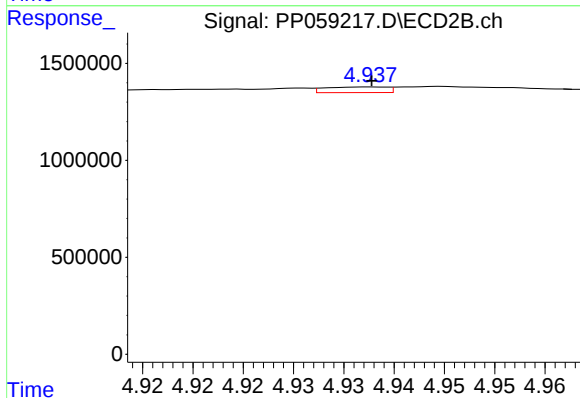


#5 AR-1016-3

R.T.: 4.938 min
Delta R.T.: 0.000 min
Response: 123124
Conc: 2.56 ng/ml

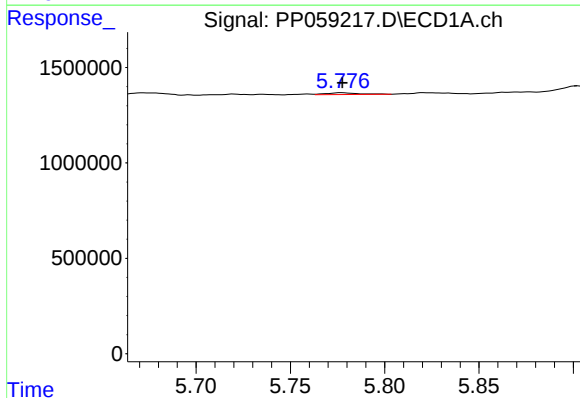


#6 AR-1016-4

R.T.: 5.777 min
Delta R.T.: 0.000 min
Response: 111038
Conc: 3.83 ng/ml

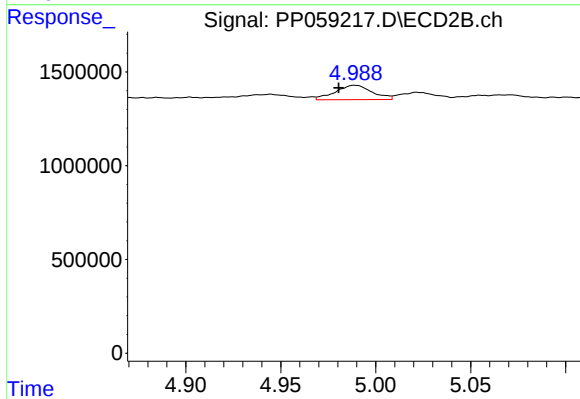

#6 AR-1016-4


R.T.: 4.989 min
Delta R.T.: 0.008 min
Response: 1032034
Conc: 24.99 ng/ml

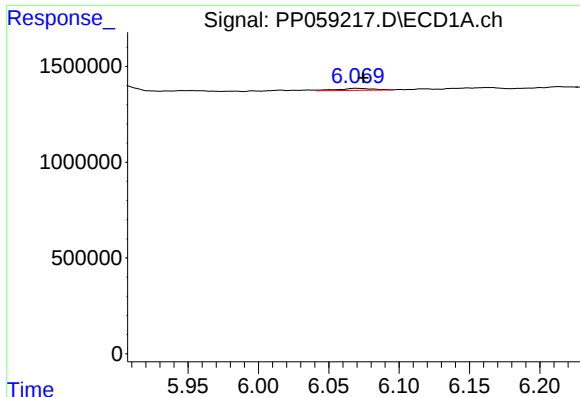

#7 AR-1016-5


R.T.: 6.069 min
Delta R.T.: -0.005 min
Response: 186090
Conc: 6.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

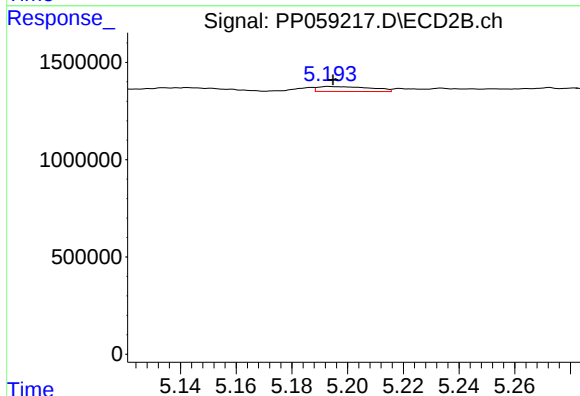


#7 AR-1016-5

R.T.: 5.193 min
Delta R.T.: -0.002 min
Response: 334691
Conc: 6.43 ng/ml

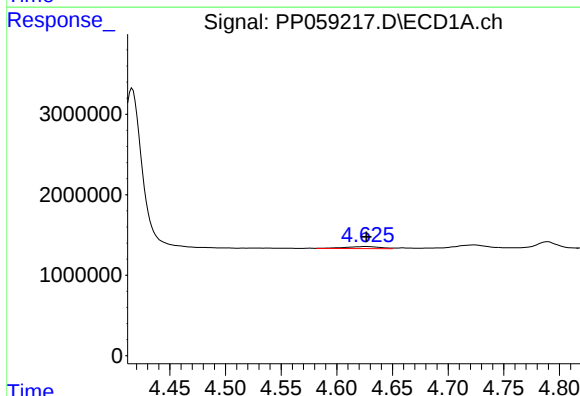


#8 AR-1221-1

R.T.: 4.626 min
Delta R.T.: 0.000 min
Response: 579340
Conc: 36.77 ng/ml

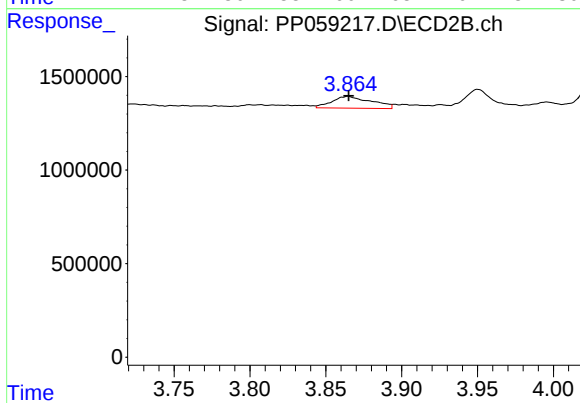

#8 AR-1221-1


R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 1153167
Conc: 42.48 ng/ml

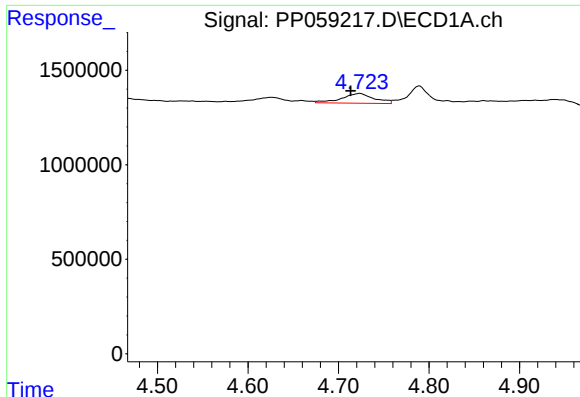

#9 AR-1221-2


R.T.: 4.724 min
Delta R.T.: 0.010 min
Response: 1288307
Conc: 109.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

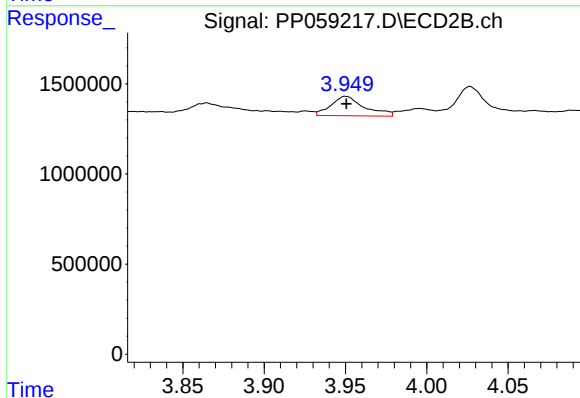


#9 AR-1221-2

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 1532199
Conc: 76.96 ng/ml

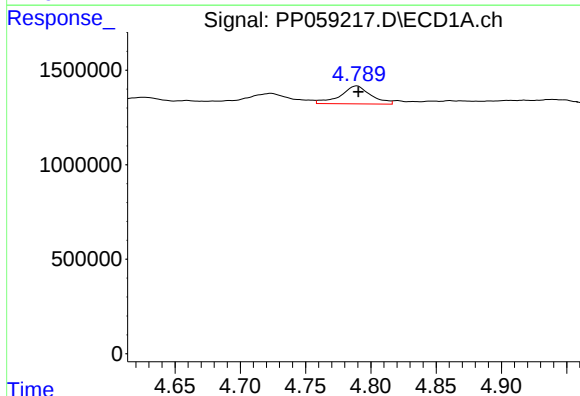


#10 AR-1221-3

R.T.: 4.789 min
Delta R.T.: -0.001 min
Response: 1533402
Conc: 43.55 ng/ml

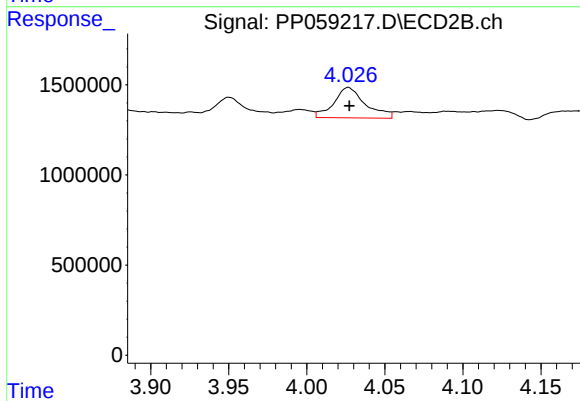

#10 AR-1221-3


R.T.: 4.027 min
Delta R.T.: 0.000 min
Response: 2378608
Conc: 39.95 ng/ml

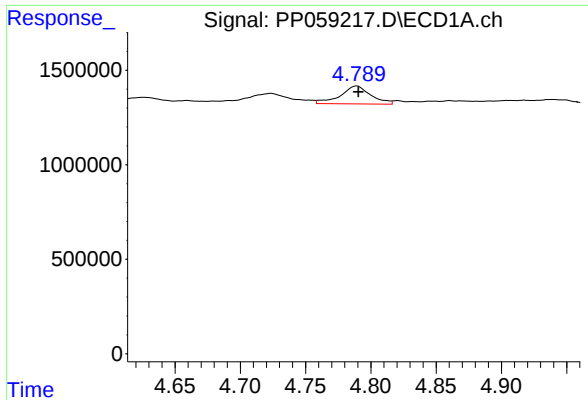

#11 AR-1232-1


R.T.: 4.789 min
Delta R.T.: 0.000 min
Response: 1533402
Conc: 52.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

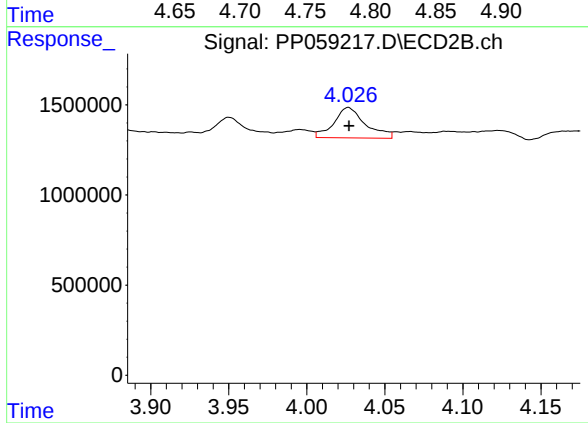


#11 AR-1232-1

R.T.: 4.027 min
Delta R.T.: 0.000 min
Response: 2378608
Conc: 50.13 ng/ml

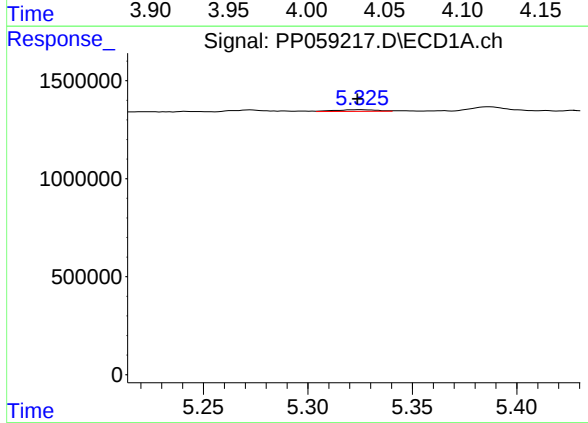


#12 AR-1232-2

R.T.: 5.325 min
Delta R.T.: 0.001 min
Response: 115938
Conc: 7.44 ng/ml

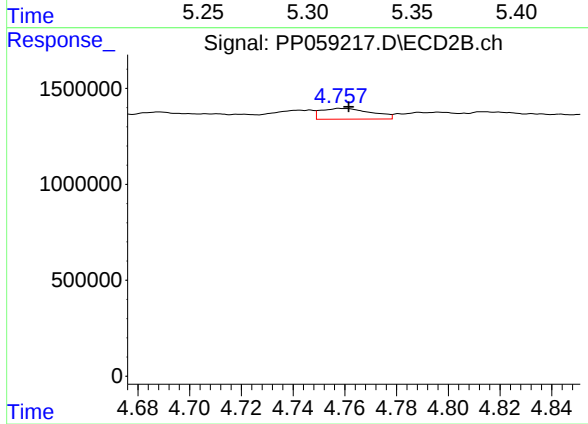

#12 AR-1232-2


R.T.: 4.758 min
Delta R.T.: -0.004 min
Response: 756871
Conc: 17.84 ng/ml

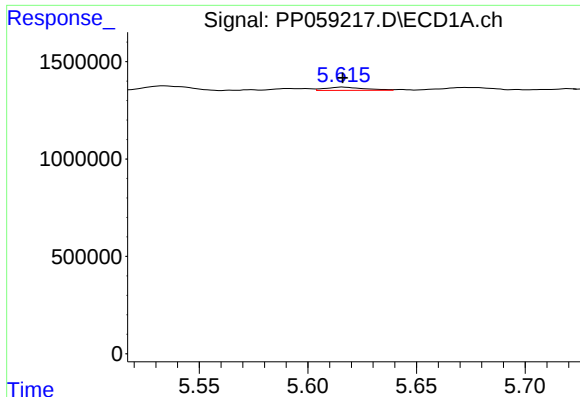

#13 AR-1232-3


R.T.: 5.616 min
Delta R.T.: 0.000 min
Response: 206876
Conc: 7.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

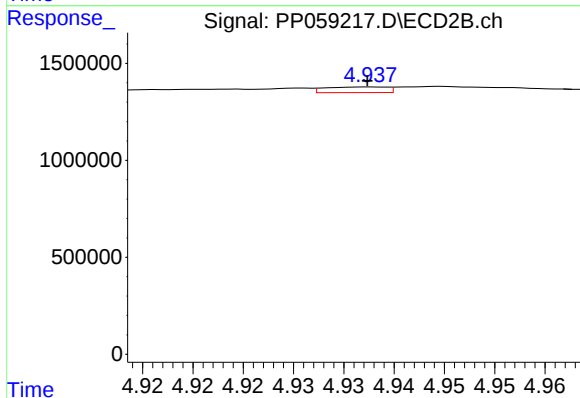


#13 AR-1232-3

R.T.: 4.938 min
Delta R.T.: 0.000 min
Response: 123124
Conc: 5.55 ng/ml

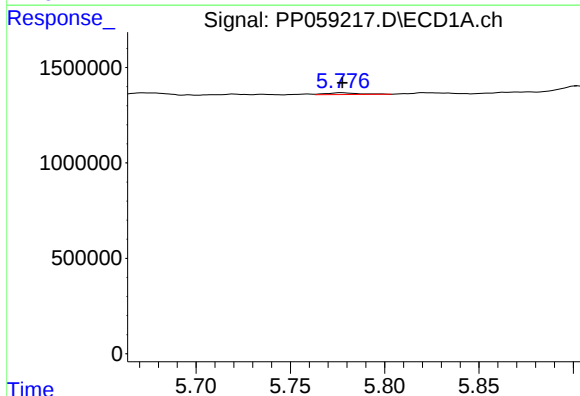


#14 AR-1232-4

R.T.: 5.777 min
Delta R.T.: 0.000 min
Response: 111038
Conc: 8.39 ng/ml

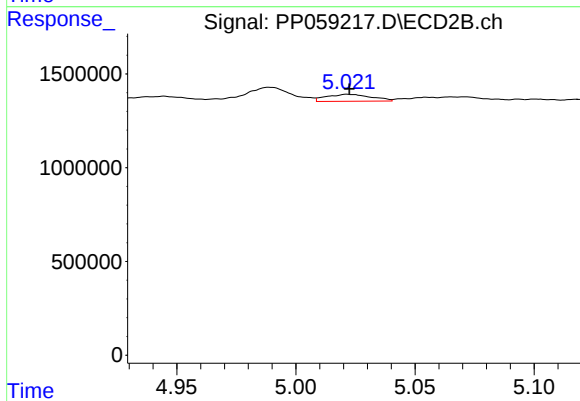

#14 AR-1232-4


R.T.: 5.022 min
Delta R.T.: 0.000 min
Response: 488405
Conc: 23.13 ng/ml

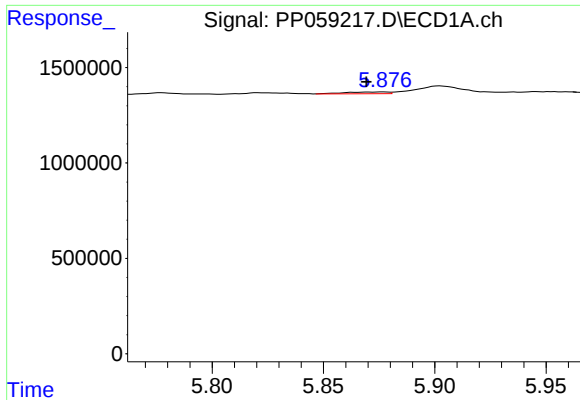

#15 AR-1232-5


R.T.: 5.877 min
Delta R.T.: 0.008 min
Response: 125812
Conc: 11.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

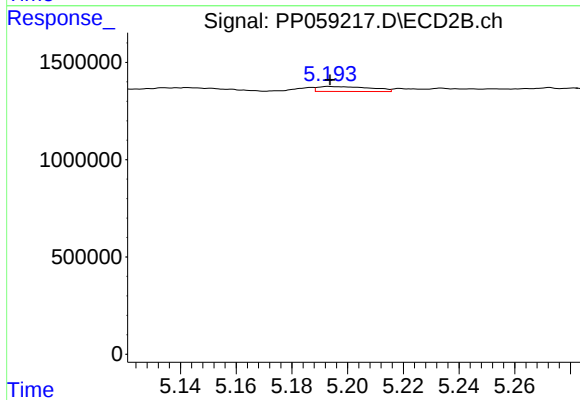


#15 AR-1232-5

R.T.: 5.193 min
Delta R.T.: 0.000 min
Response: 334691
Conc: 14.60 ng/ml

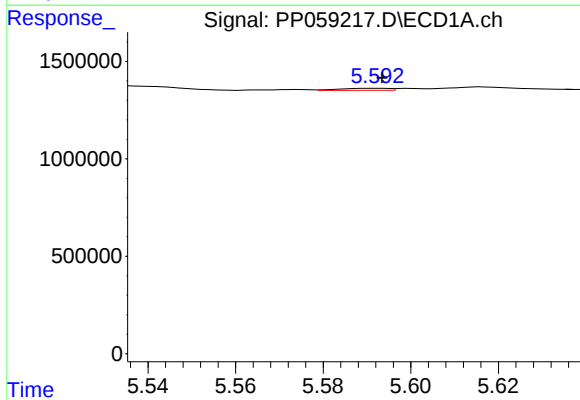


#16 AR-1242-1

R.T.: 5.592 min
Delta R.T.: -0.002 min
Response: 83125
Conc: 2.43 ng/ml

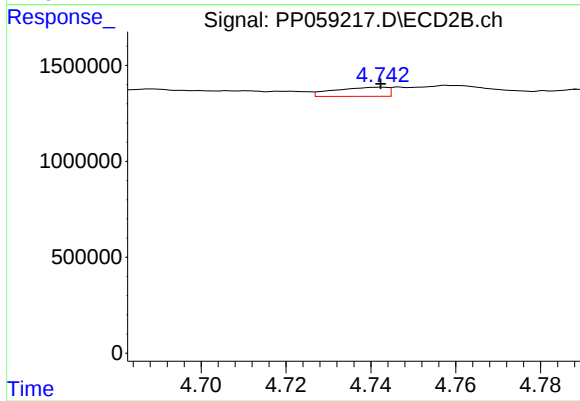

#16 AR-1242-1


R.T.: 4.743 min
Delta R.T.: 0.000 min
Response: 411910
Conc: 7.36 ng/ml

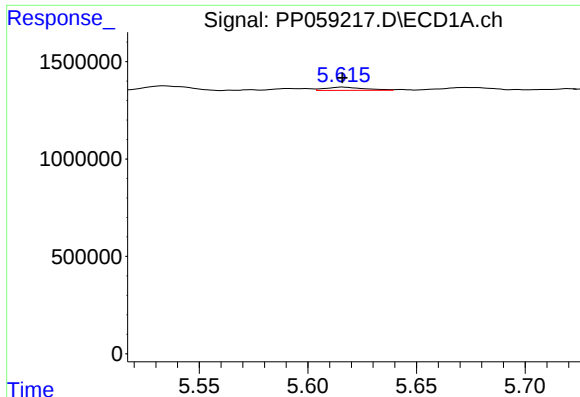

#17 AR-1242-2


R.T.: 5.616 min
Delta R.T.: 0.000 min
Response: 206876
Conc: 4.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

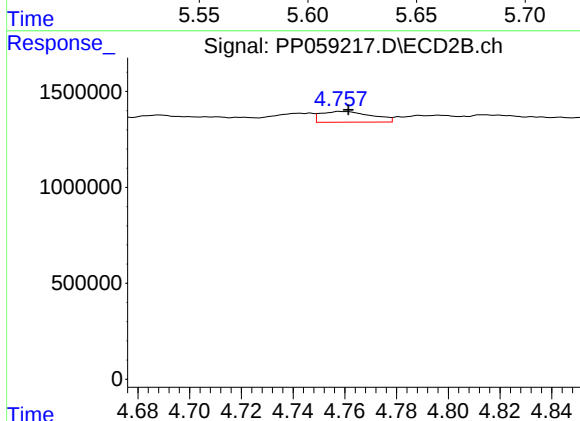


#17 AR-1242-2

R.T.: 4.758 min
Delta R.T.: -0.003 min
Response: 756871
Conc: 9.49 ng/ml

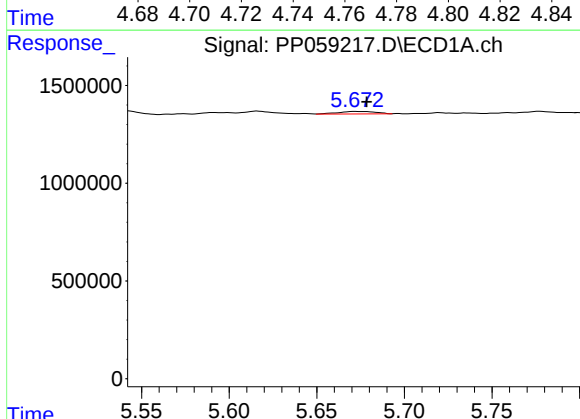


#18 AR-1242-3

R.T.: 5.672 min
Delta R.T.: -0.006 min
Response: 196923
Conc: 6.27 ng/ml

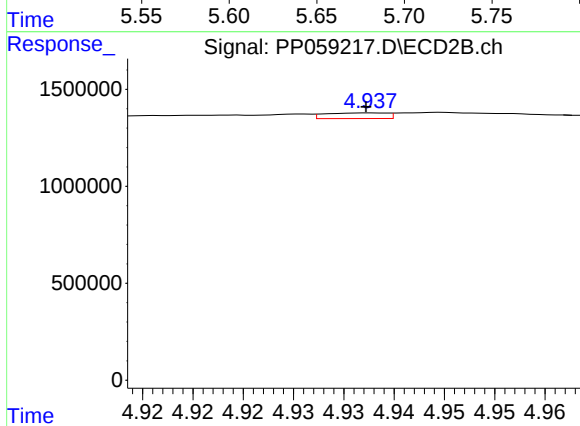

#18 AR-1242-3


R.T.: 4.938 min
Delta R.T.: 0.000 min
Response: 123124
Conc: 2.89 ng/ml

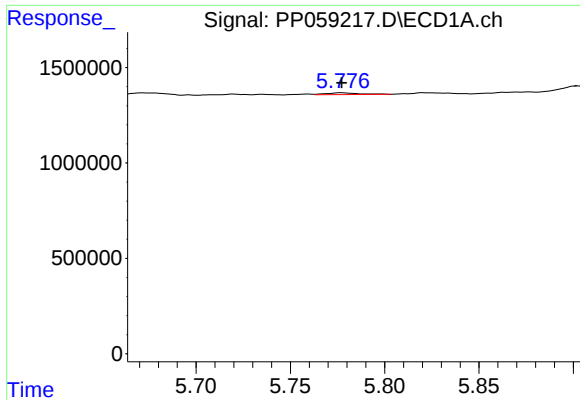

#19 AR-1242-4


R.T.: 5.777 min
Delta R.T.: 0.000 min
Response: 111038
Conc: 4.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

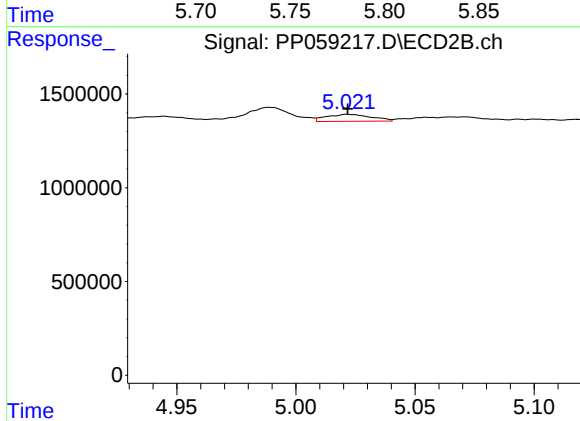


#19 AR-1242-4

R.T.: 5.022 min
Delta R.T.: 0.000 min
Response: 488405
Conc: 11.19 ng/ml

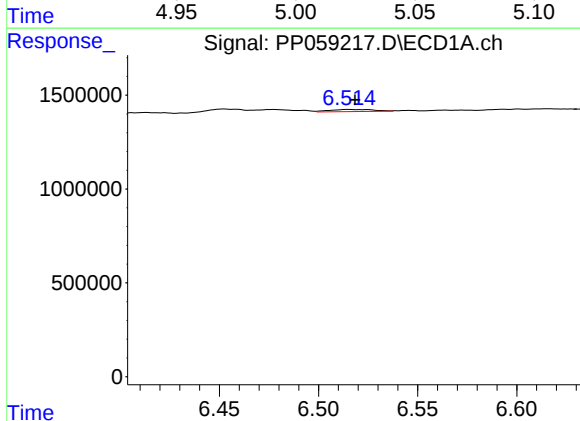


#20 AR-1242-5

R.T.: 6.515 min
Delta R.T.: -0.003 min
Response: 170762
Conc: 6.61 ng/ml

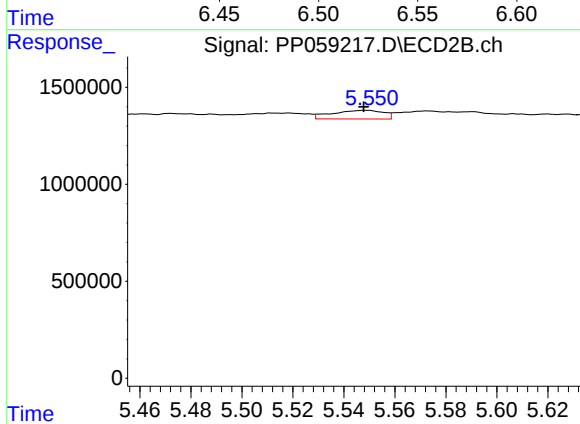

#20 AR-1242-5


R.T.: 5.550 min
Delta R.T.: 0.002 min
Response: 628355
Conc: 12.65 ng/ml

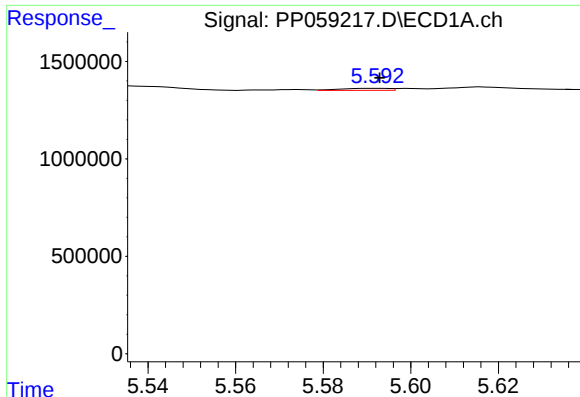

#21 AR-1248-1


R.T.: 5.592 min
Delta R.T.: -0.001 min
Response: 83125
Conc: 3.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

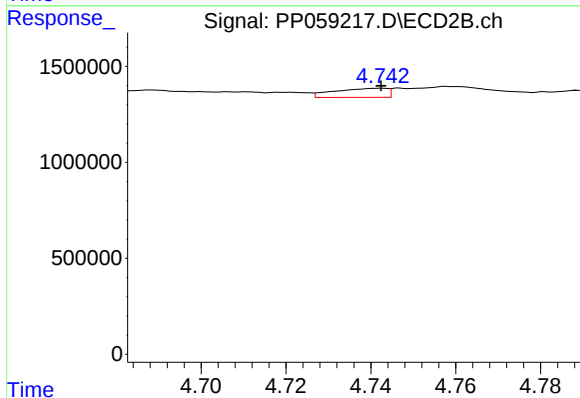


#21 AR-1248-1

R.T.: 4.743 min
Delta R.T.: 0.000 min
Response: 411910
Conc: 10.01 ng/ml

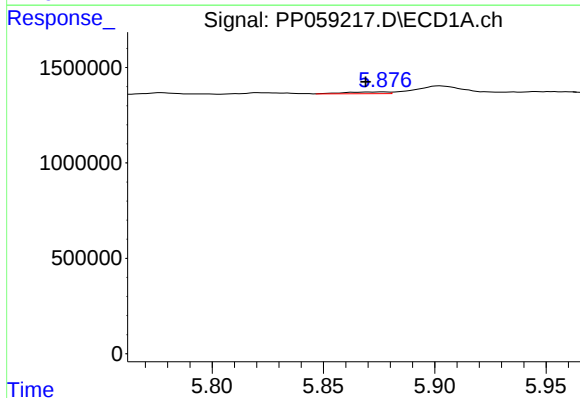


#22 AR-1248-2

R.T.: 5.877 min
Delta R.T.: 0.008 min
Response: 125812
Conc: 3.25 ng/ml

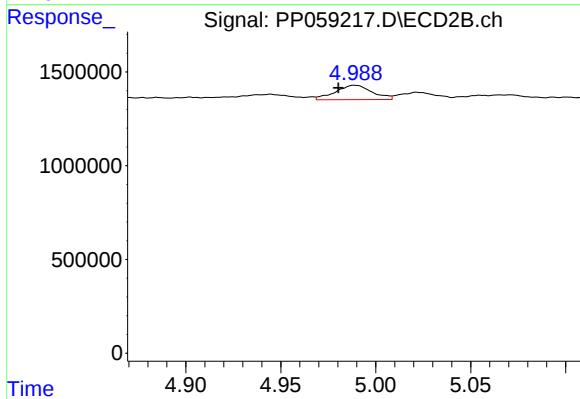

#22 AR-1248-2


R.T.: 4.989 min
Delta R.T.: 0.008 min
Response: 1032034
Conc: 17.14 ng/ml

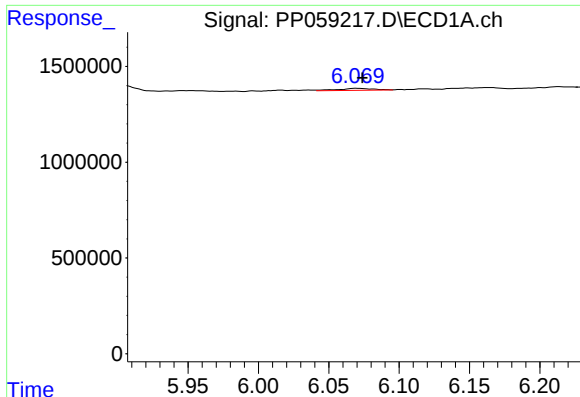

#23 AR-1248-3


R.T.: 6.069 min
Delta R.T.: -0.005 min
Response: 186090
Conc: 4.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

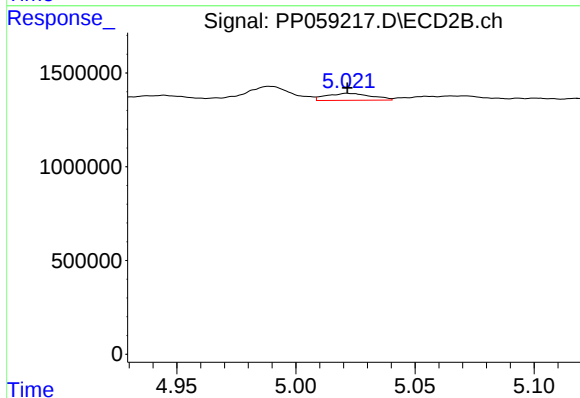


#23 AR-1248-3

R.T.: 5.022 min
Delta R.T.: 0.000 min
Response: 488405
Conc: 7.93 ng/ml

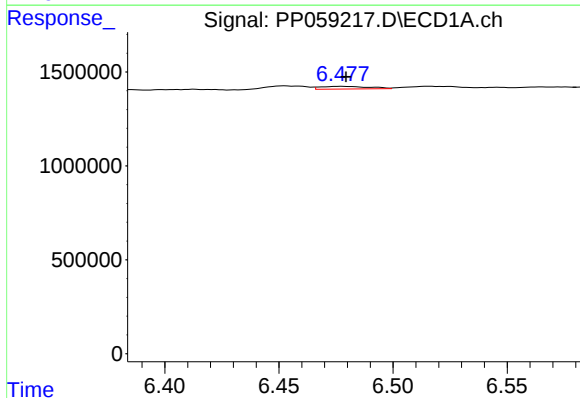


#24 AR-1248-4

R.T.: 6.477 min
Delta R.T.: -0.002 min
Response: 218224
Conc: 5.24 ng/ml

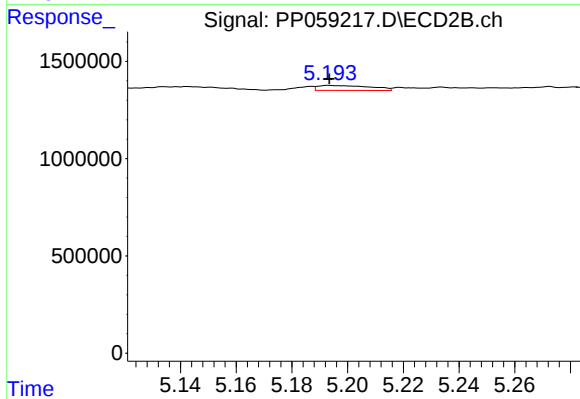

#24 AR-1248-4


R.T.: 5.193 min
Delta R.T.: 0.000 min
Response: 334691
Conc: 4.65 ng/ml

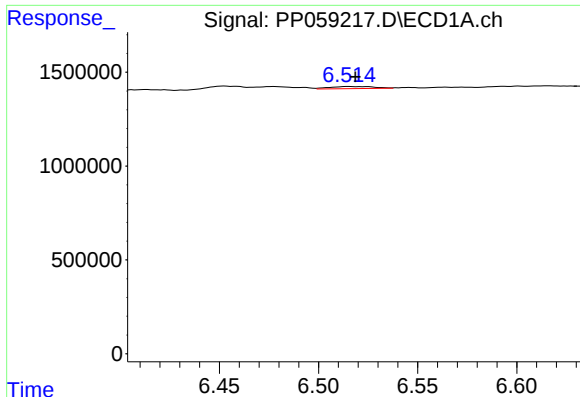

#25 AR-1248-5


R.T.: 6.515 min
Delta R.T.: -0.003 min
Response: 170762
Conc: 4.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

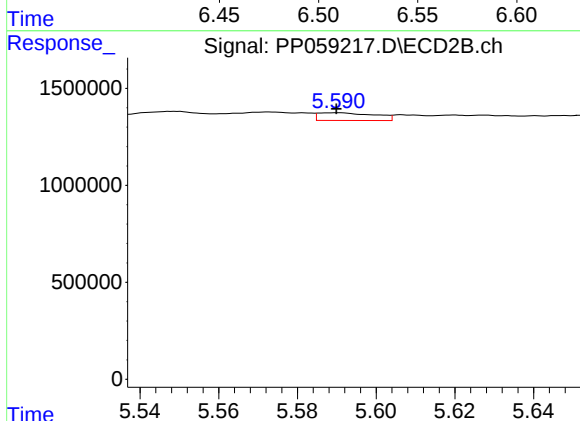


#25 AR-1248-5

R.T.: 5.590 min
Delta R.T.: 0.000 min
Response: 392086
Conc: 5.94 ng/ml

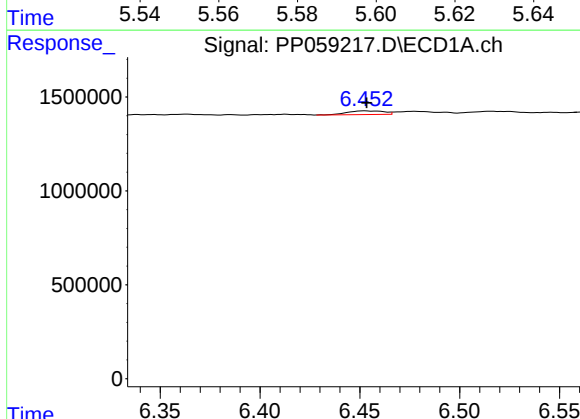


#26 AR-1254-1

R.T.: 6.452 min
Delta R.T.: 0.000 min
Response: 254320
Conc: 5.44 ng/ml

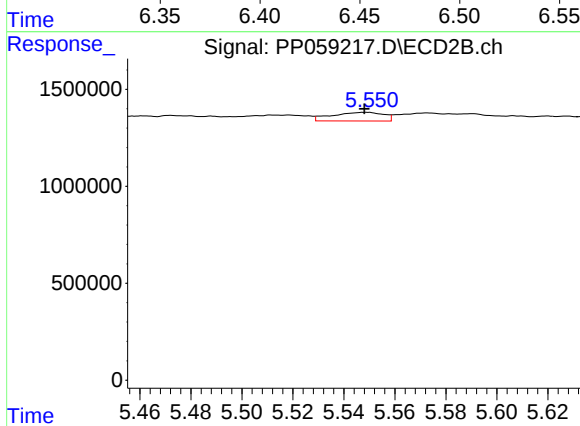

#26 AR-1254-1


R.T.: 5.550 min
Delta R.T.: 0.002 min
Response: 628355
Conc: 6.20 ng/ml

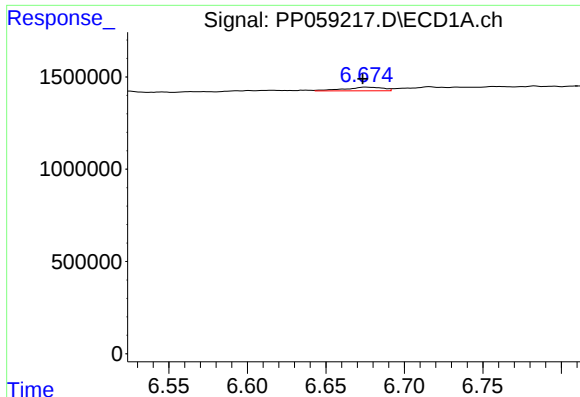

#27 AR-1254-2


R.T.: 6.675 min
Delta R.T.: 0.002 min
Response: 327723
Conc: 4.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

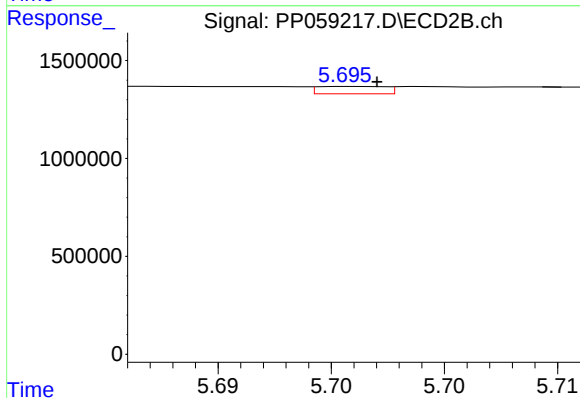


#27 AR-1254-2

R.T.: 5.696 min
Delta R.T.: 0.000 min
Response: 77837
Conc: 0.88 ng/ml

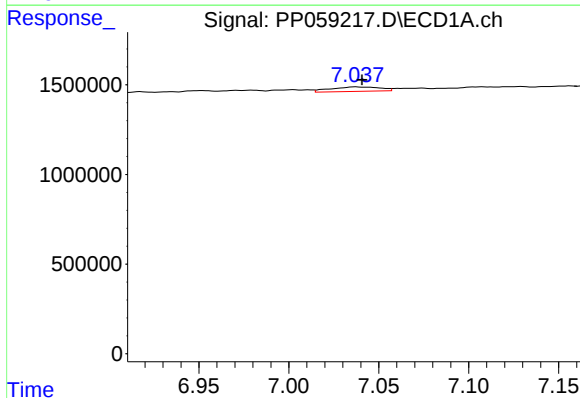


#28 AR-1254-3

R.T.: 7.037 min
Delta R.T.: -0.004 min
Response: 480884
Conc: 6.97 ng/ml

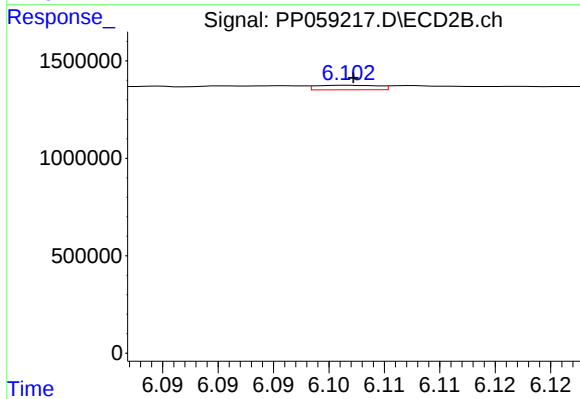

#28 AR-1254-3


R.T.: 6.102 min
Delta R.T.: 0.000 min
Response: 91185
Conc: 0.66 ng/ml

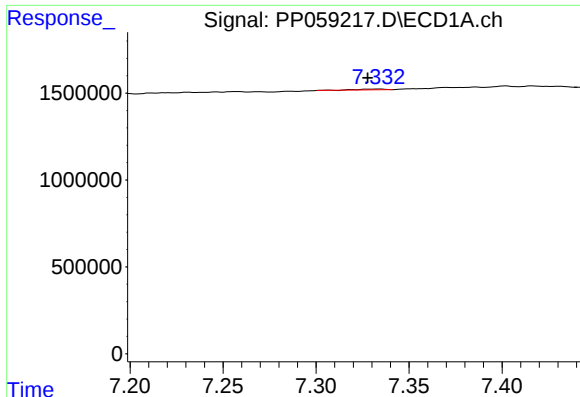

#29 AR-1254-4


R.T.: 7.334 min
Delta R.T.: 0.006 min
Response: 42967
Conc: 0.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

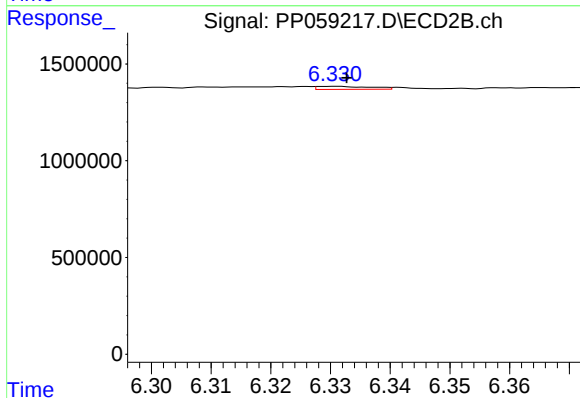


#29 AR-1254-4

R.T.: 6.331 min
Delta R.T.: -0.002 min
Response: 98155
Conc: 1.22 ng/ml

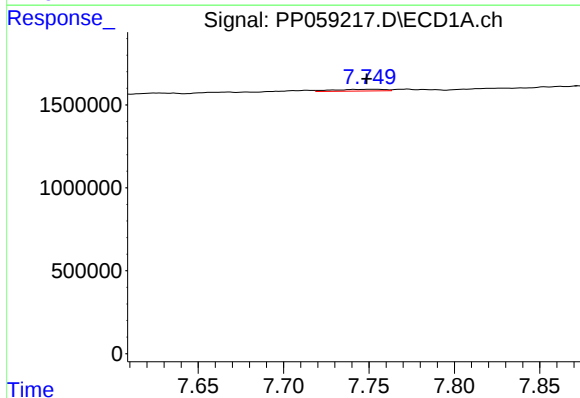


#30 AR-1254-5

R.T.: 7.750 min
Delta R.T.: 0.001 min
Response: 228822
Conc: 4.87 ng/ml

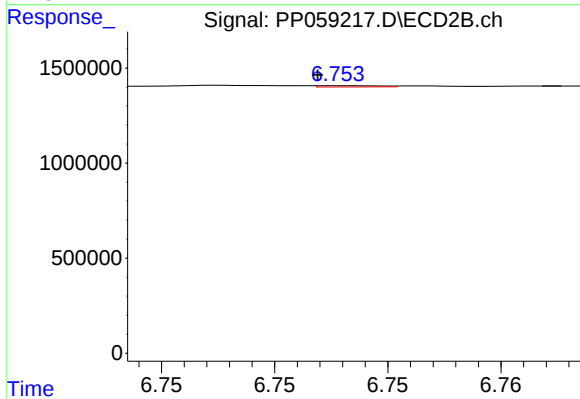

#30 AR-1254-5


R.T.: 6.753 min
Delta R.T.: 0.001 min
Response: 12998
Conc: 0.11 ng/ml

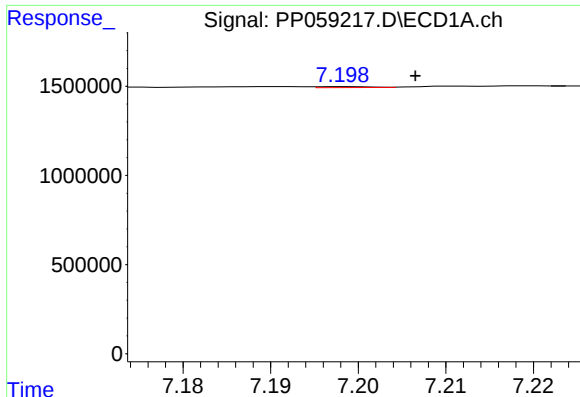

#31 AR-1260-1


R.T.: 7.198 min
Delta R.T.: -0.008 min
Response: 24647
Conc: 0.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

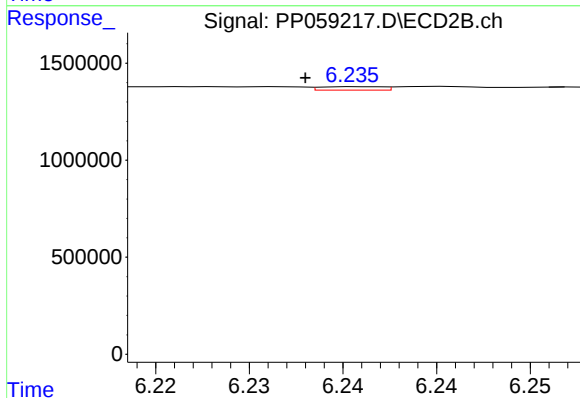


#31 AR-1260-1

R.T.: 6.236 min
Delta R.T.: 0.003 min
Response: 40662
Conc: 0.41 ng/ml

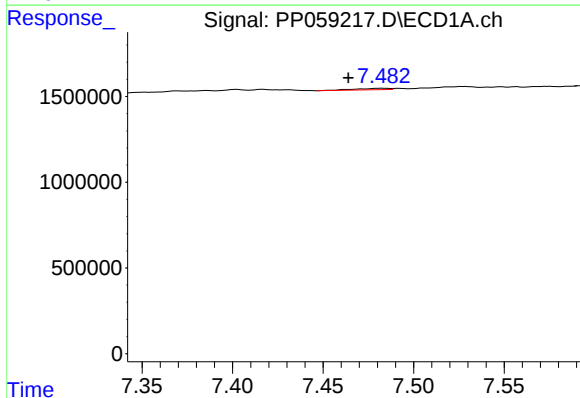


#32 AR-1260-2

R.T.: 7.483 min
Delta R.T.: 0.019 min
Response: 115320
Conc: 1.94 ng/ml

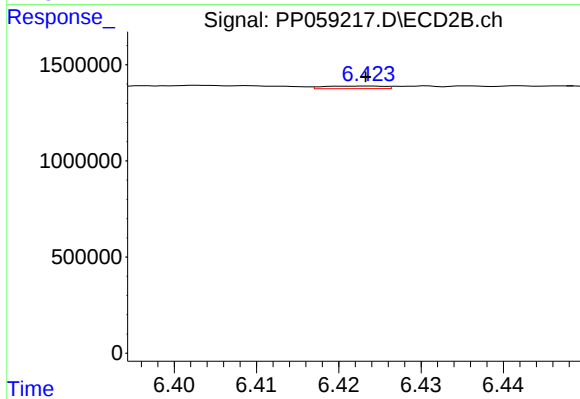

#32 AR-1260-2


R.T.: 6.424 min
Delta R.T.: 0.000 min
Response: 70739
Conc: 0.61 ng/ml

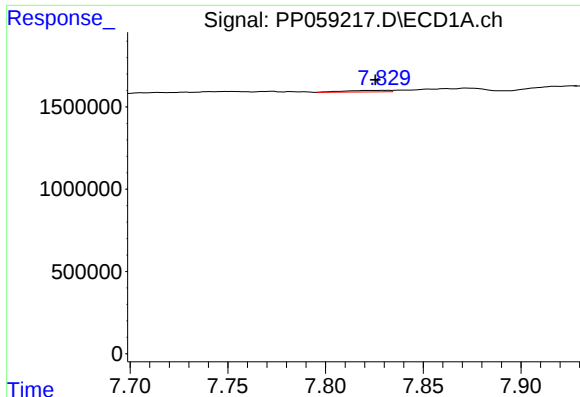

#33 AR-1260-3


R.T.: 7.830 min
Delta R.T.: 0.005 min
Response: 154276
Conc: 3.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

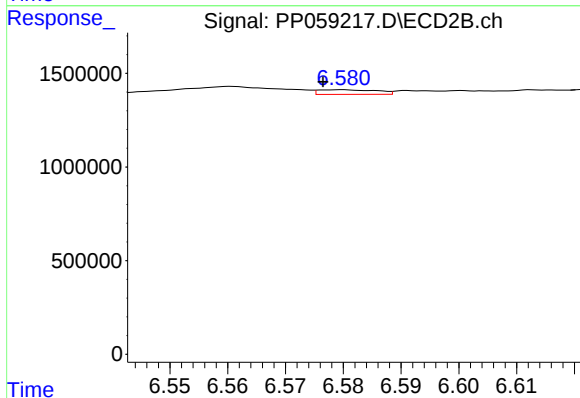


#33 AR-1260-3

R.T.: 6.580 min
Delta R.T.: 0.004 min
Response: 172991
Conc: 1.56 ng/ml

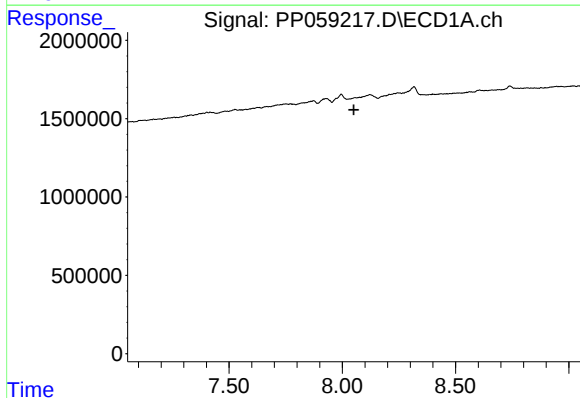


#34 AR-1260-4

R.T.: 8.056 min
Delta R.T.: 0.004 min
Response: -333839
Conc: N.D.

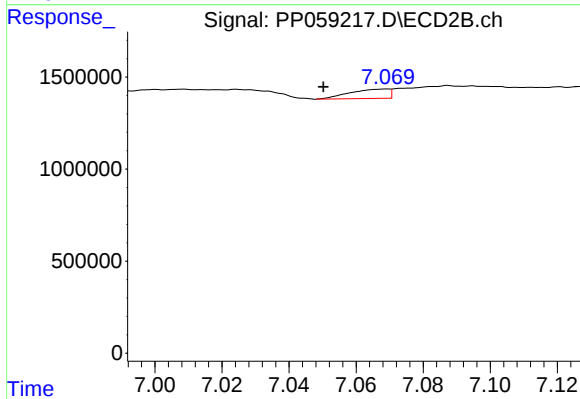

#34 AR-1260-4


R.T.: 7.069 min
Delta R.T.: 0.019 min
Response: 410294
Conc: 4.73 ng/ml

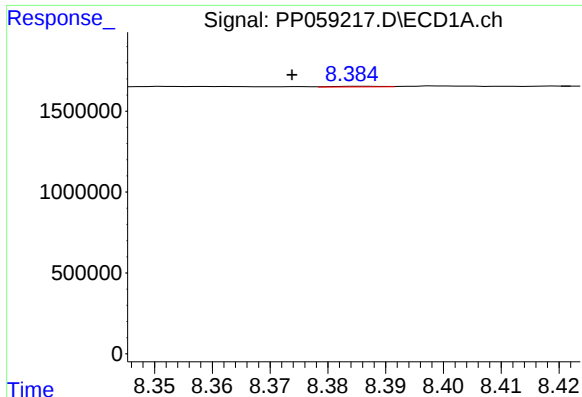

#35 AR-1260-5


R.T.: 8.385 min
Delta R.T.: 0.011 min
Response: 24448
Conc: 0.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

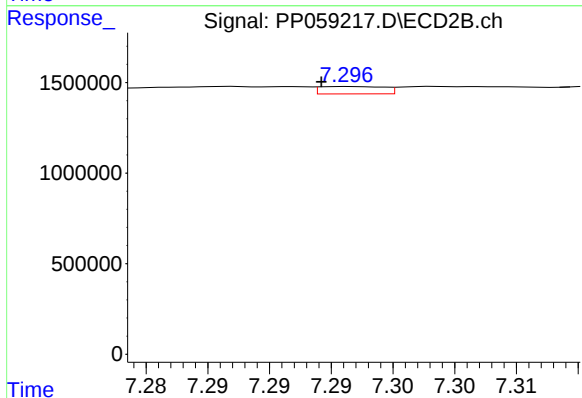


#35 AR-1260-5

R.T.: 7.296 min
Delta R.T.: 0.002 min
Response: 147720
Conc: 0.80 ng/ml

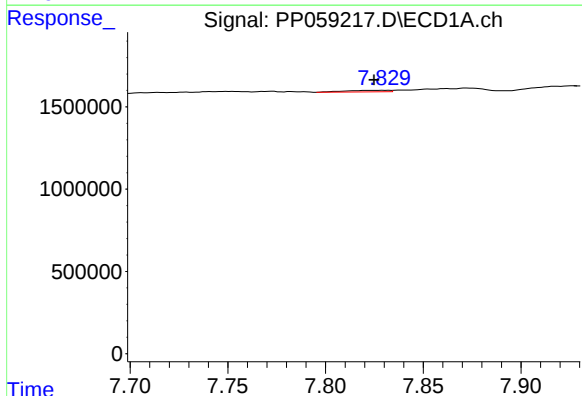


#36 AR-1262-1

R.T.: 7.830 min
Delta R.T.: 0.005 min
Response: 154276
Conc: 2.42 ng/ml

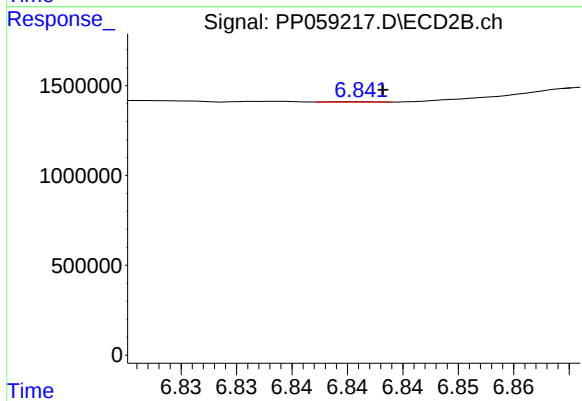

#36 AR-1262-1


R.T.: 6.841 min
Delta R.T.: -0.002 min
Response: 5510
Conc: 0.10 ng/ml

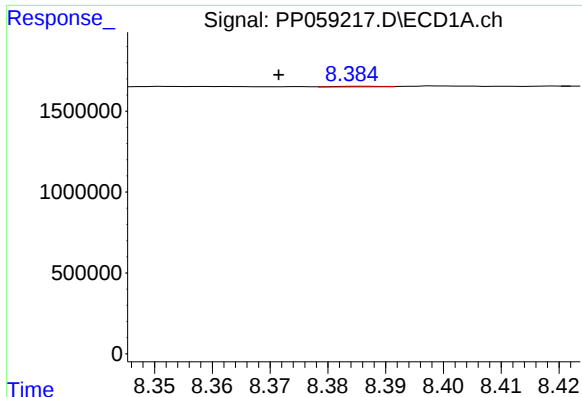

#37 AR-1262-2


R.T.: 8.385 min
Delta R.T.: 0.014 min
Response: 24448
Conc: 0.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

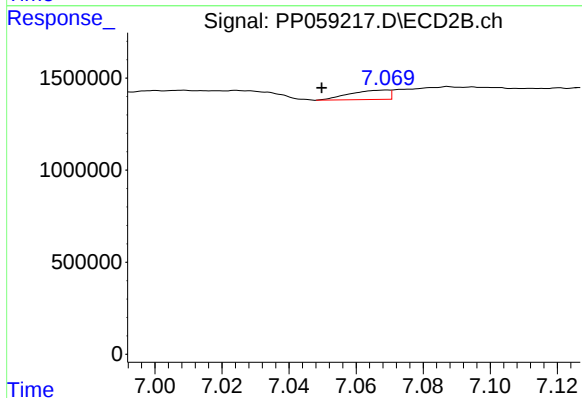


#37 AR-1262-2

R.T.: 7.069 min
Delta R.T.: 0.019 min
Response: 410294
Conc: 3.48 ng/ml

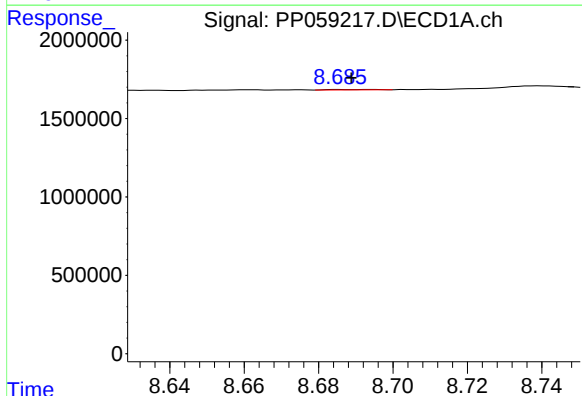


#38 AR-1262-3

R.T.: 8.694 min
Delta R.T.: 0.006 min
Response: 23968
Conc: 0.37 ng/ml

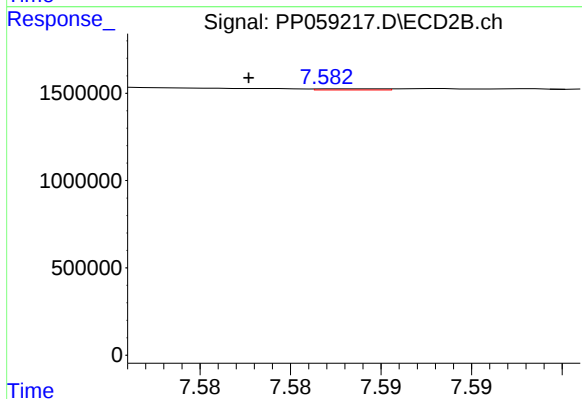

#38 AR-1262-3


R.T.: 7.583 min
Delta R.T.: 0.005 min
Response: 16026
Conc: 0.19 ng/ml

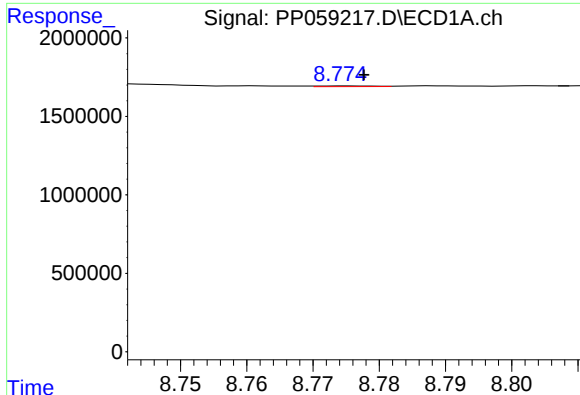

#39 AR-1262-4


R.T.: 8.775 min
Delta R.T.: -0.003 min
Response: 26063
Conc: 0.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

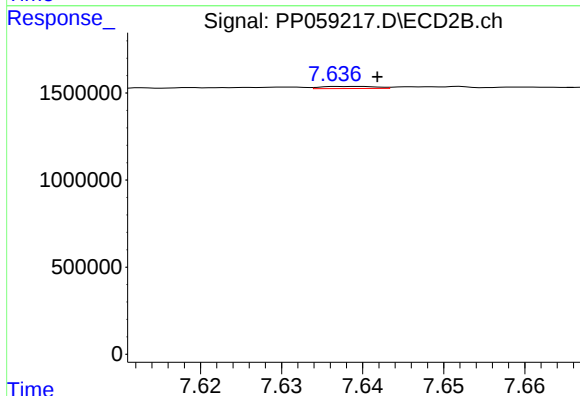


#39 AR-1262-4

R.T.: 7.640 min
Delta R.T.: -0.002 min
Response: 57144
Conc: 0.38 ng/ml

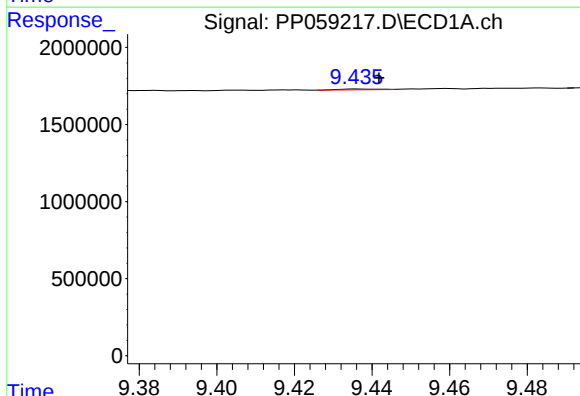


#40 AR-1262-5

R.T.: 9.436 min
Delta R.T.: -0.005 min
Response: 40650
Conc: 1.36 ng/ml

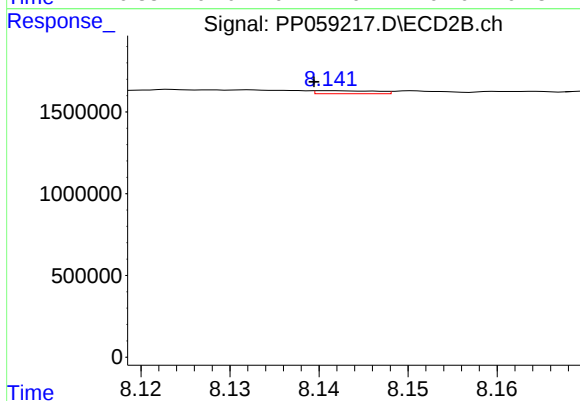

#40 AR-1262-5


R.T.: 8.141 min
Delta R.T.: 0.002 min
Response: 87483
Conc: 1.37 ng/ml

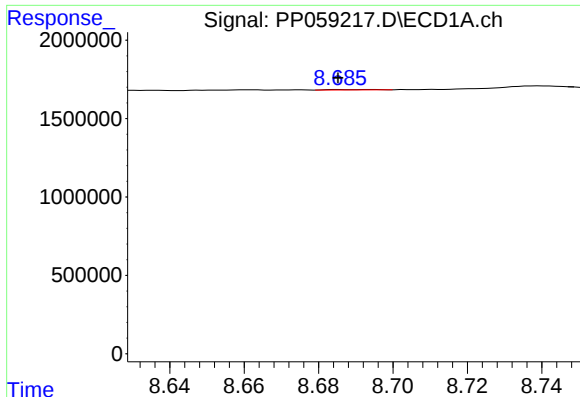

#41 AR-1268-1


R.T.: 8.694 min
Delta R.T.: 0.009 min
Response: 23968
Conc: 0.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

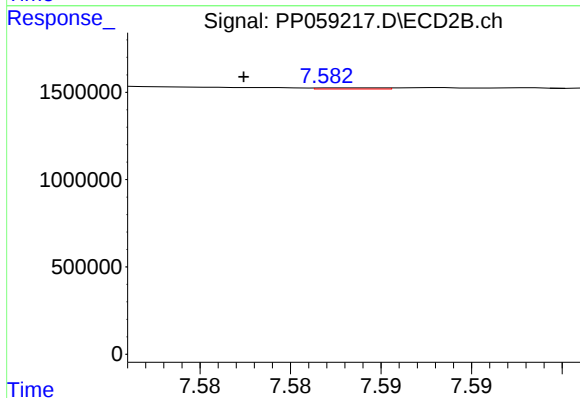


#41 AR-1268-1

R.T.: 7.583 min
Delta R.T.: 0.005 min
Response: 16026
Conc: 0.07 ng/ml

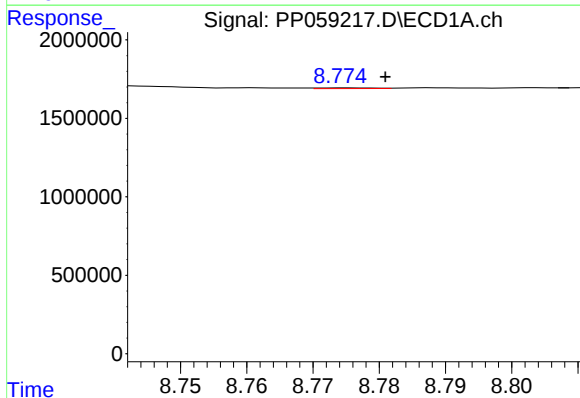


#42 AR-1268-2

R.T.: 8.775 min
Delta R.T.: -0.006 min
Response: 26063
Conc: 0.26 ng/ml

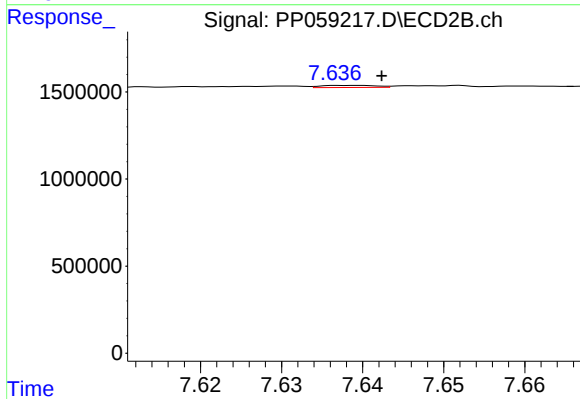

#42 AR-1268-2


R.T.: 7.640 min
Delta R.T.: -0.003 min
Response: 57144
Conc: 0.26 ng/ml

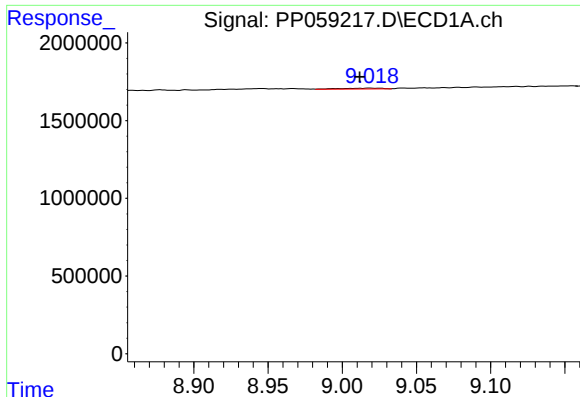

#43 AR-1268-3


R.T.: 9.019 min
Delta R.T.: 0.007 min
Response: 100001
Conc: 1.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

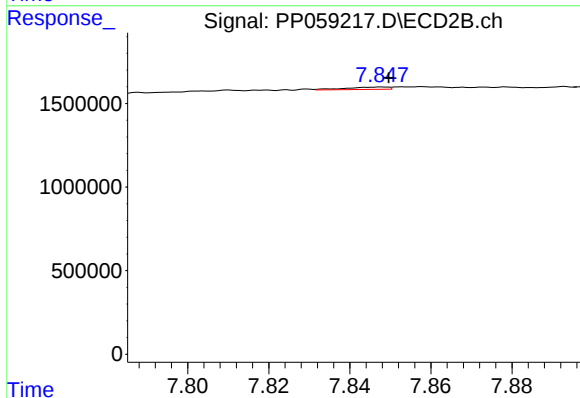


#43 AR-1268-3

R.T.: 7.848 min
Delta R.T.: -0.002 min
Response: 104078
Conc: 0.53 ng/ml

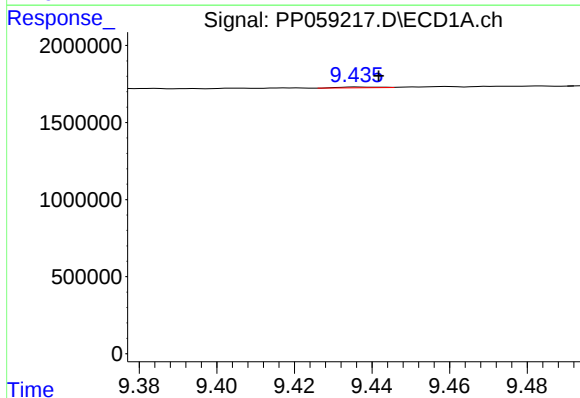


#44 AR-1268-4

R.T.: 9.436 min
Delta R.T.: -0.005 min
Response: 40650
Conc: 1.27 ng/ml

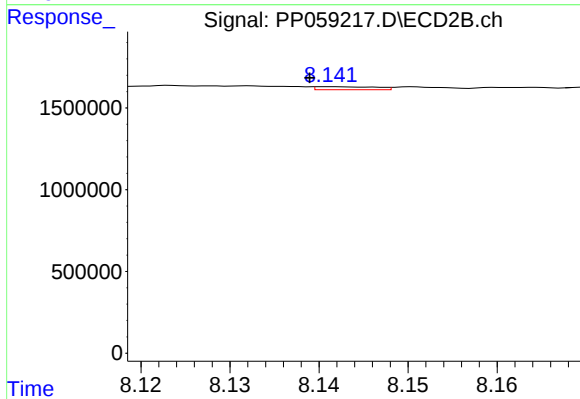

#44 AR-1268-4


R.T.: 8.141 min
Delta R.T.: 0.002 min
Response: 87483
Conc: 1.26 ng/ml

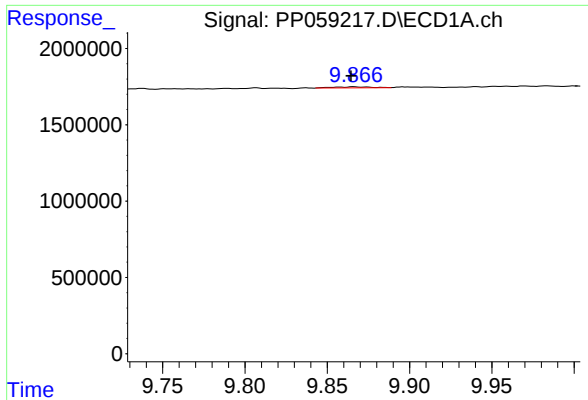

#45 AR-1268-5

R.T.: 9.866 min
Delta R.T.: 0.002 min
Response: 117836
Conc: 0.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

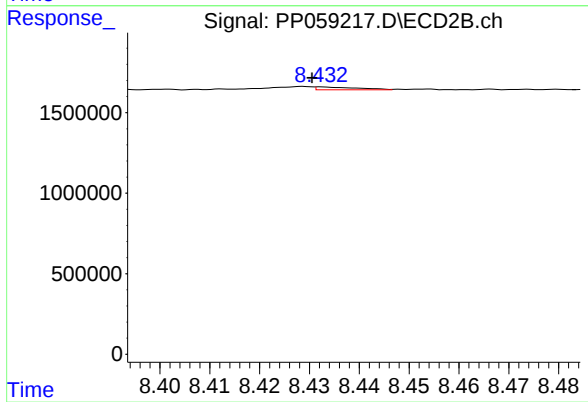

#45 AR-1268-5

R.T.: 8.432 min
Delta R.T.: 0.002 min
Response: 104245
Conc: 0.20 ng/ml