

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
 Data File : PP059218.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2023 23:10
 Operator : YP\AJ
 Sample : 03572-07
 Misc : AR1232 LOD 25 PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 02:41:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.416	3.648	24120202	40706303	19.657	20.091
2)	SA Decachlor...	10.211	8.685	18674481	32463534	24.468	23.076
Target Compounds							
3)	L1 AR-1016-1	5.593	4.742	451319	1119960	11.487	17.462 #
4)	L1 AR-1016-2	5.616	4.761	687430	1358551	12.127	14.956
5)	L1 AR-1016-3	5.678	4.937	445613	849978	12.422	17.690 #
6)	L1 AR-1016-4	5.777	4.979	295362	663649	10.196	16.072 #
7)	L1 AR-1016-5	6.072	5.193	384838	721806	12.716	13.872
8)	L2 AR-1221-1	4.625	3.867	368540	143758	23.393	5.296 #
9)	L2 AR-1221-2	4.725	3.949	987903	1055954	83.657	53.037 #
10)	L2 AR-1221-3	4.790	4.026	1186654	1666964	33.699	28.000
11)	L3 AR-1232-1	4.790	4.026	1186654	1666964	40.367	35.132
12)	L3 AR-1232-2	5.324	4.761	382431	1358551	24.535	32.027 #
13)	L3 AR-1232-3	5.616	4.937	687430	849978	26.033	38.308 #
14)	L3 AR-1232-4	5.777	5.022	295362	824710	22.318	39.059 #
15)	L3 AR-1232-5	5.870	5.193	267707	721806	23.453	31.489 #
16)	L4 AR-1242-1	5.593	4.742	451319	1119960	13.184	20.012 #
17)	L4 AR-1242-2	5.616	4.761	687430	1358551	14.009	17.038
18)	L4 AR-1242-3	5.678	4.937	445613	849978	14.183	19.944 #
19)	L4 AR-1242-4	5.777	5.022	295362	824710	11.518	18.887 #
20)	L4 AR-1242-5	6.517	5.547	366714	925565	14.195	18.633 #
21)	L5 AR-1248-1	5.593	4.742	451319	1119960	17.782	27.225 #
22)	L5 AR-1248-2	5.870	4.979	267707	663649	6.917	11.021 #
23)	L5 AR-1248-3	6.072	5.022	384838	824710	9.109	13.386 #
24)	L5 AR-1248-4	6.479	5.193	428180	721806	10.284	10.026
25)	L5 AR-1248-5	6.517	5.589	366714	855046	8.990	12.958 #
26)	L6 AR-1254-1	6.453	5.547	290688	925565	6.223	9.135 #
27)	L6 AR-1254-2	6.676	5.700	488624	285645	7.101	3.236 #
28)	L6 AR-1254-3	7.040	6.102	331869	186861	4.808	1.352 #
29)	L6 AR-1254-4	7.329	6.330	98314	182582	2.184	2.271
30)	L6 AR-1254-5	7.752	6.756	203584	75981	4.333	0.635 #
31)	L7 AR-1260-1	7.222	6.238	175944	58161	3.216	0.587 #
32)	L7 AR-1260-2	0.000	6.427	0	70006	N.D.	0.605 #
33)	L7 AR-1260-3	7.824	6.578	83987	169448	2.134	1.523 #
34)	L7 AR-1260-4	8.059	7.062	83430	126576	1.878	1.460
35)	L7 AR-1260-5	8.356f	7.292	39734	93552	0.497	0.508
36)	L8 AR-1262-1	7.824	6.841	83987	5792	1.319	0.101 #
37)	L8 AR-1262-2	8.356f	7.062	39734	126576	0.433	1.073 #
38)	L8 AR-1262-3	8.677	7.578	16220	21500	0.252	0.253
39)	L8 AR-1262-4	8.781	7.639	54024	48634	1.627	0.322 #
40)	L8 AR-1262-5	9.440	8.136	24642	82482	0.826	1.293 #
41)	L9 AR-1268-1	8.677	7.578	16220	21500	0.143	0.088 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
 Data File : PP059218.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2023 23:10
 Operator : YP\AJ
 Sample : 03572-07
 Misc : AR1232 LOD 25 PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 02:41:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.781	7.639	54024	48634	0.549	0.222 #
43) L9	AR-1268-3	9.010	7.852	58775	253916	0.634	1.299 #
44) L9	AR-1268-4	9.440	8.136	24642	82482	0.772	1.185 #
45) L9	AR-1268-5	9.864	8.428	74022	127911	0.273	0.247



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
Data File : PP059218.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2023 23:10
Operator : YP\AJ
Sample : 03572-07
Misc : AR1232 LOD 25 PPB
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 02:41:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

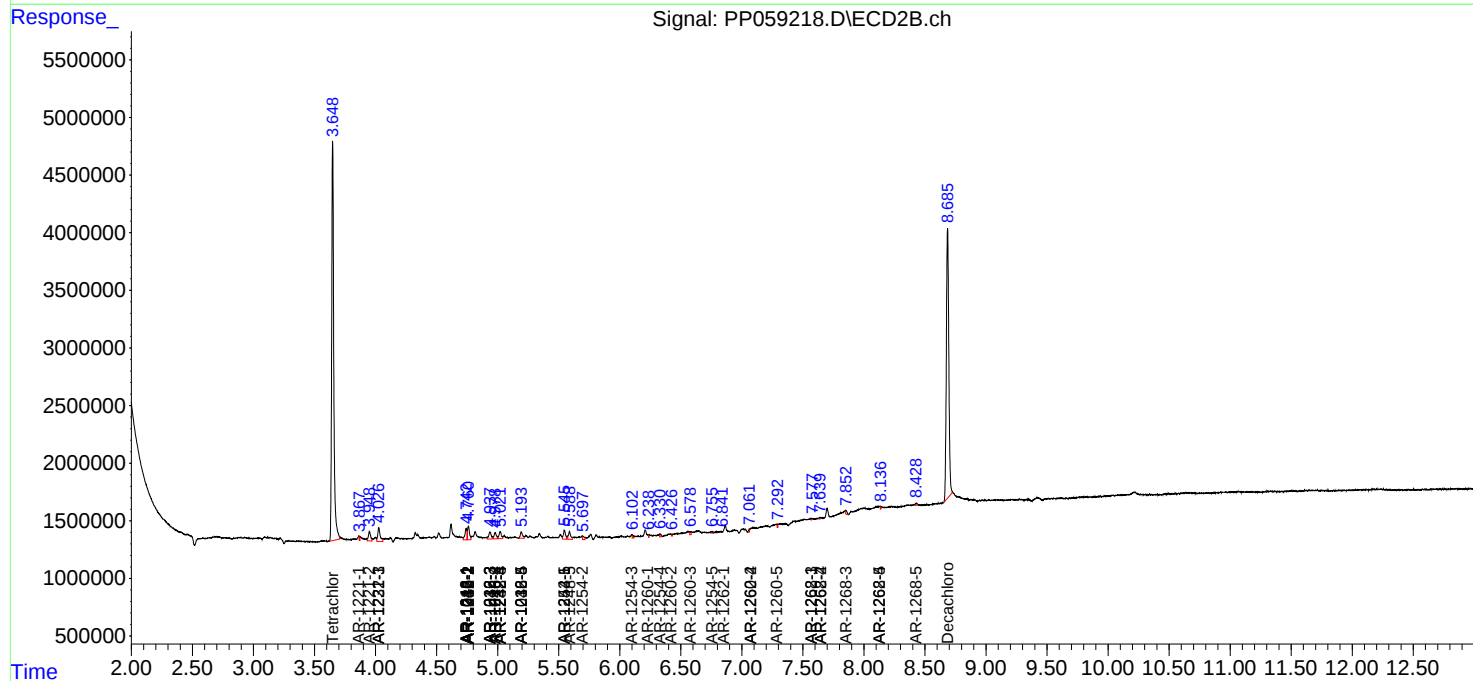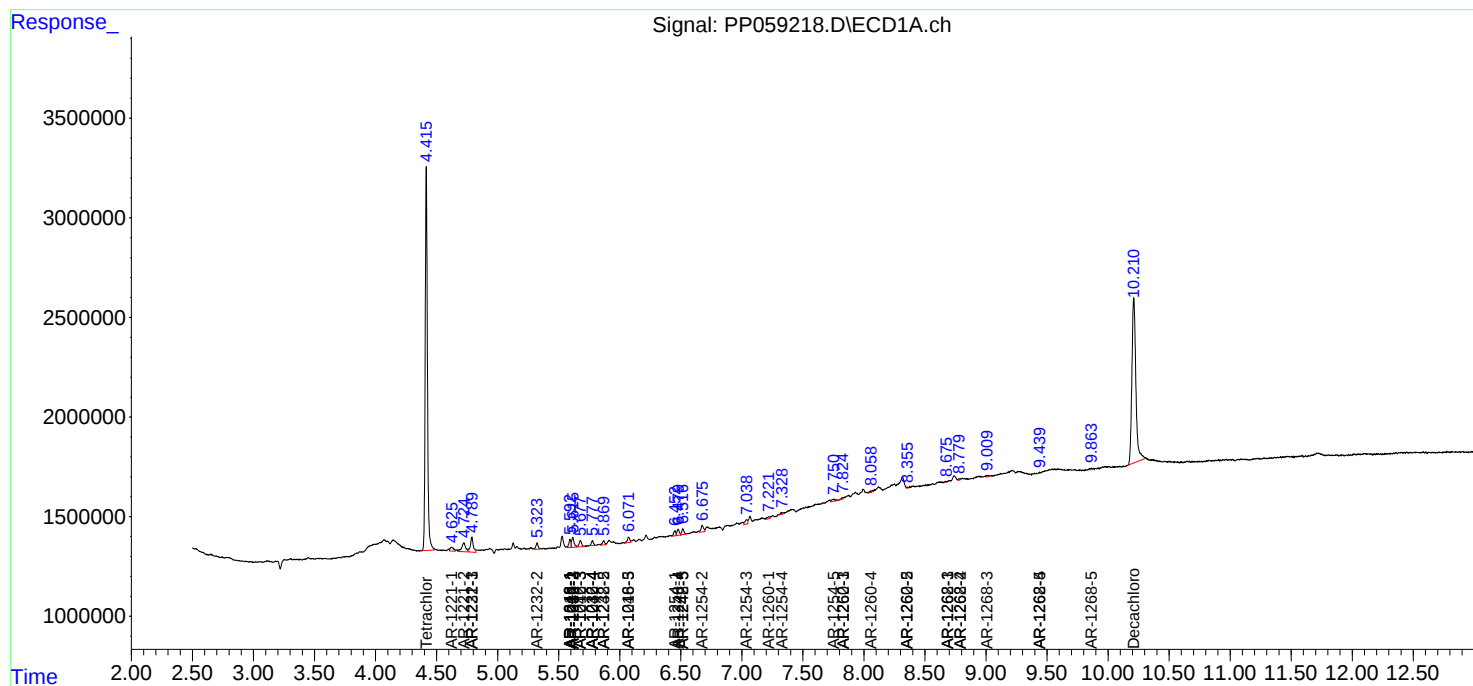


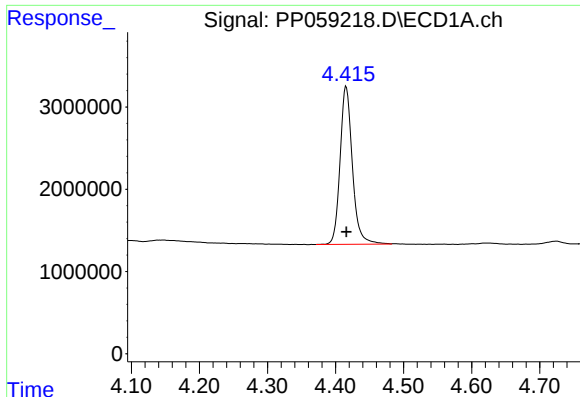

#1 Tetrachloro-m-xylene


R.T.: 4.416 min
Delta R.T.: 0.000 min
Response: 24120202
Conc: 19.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

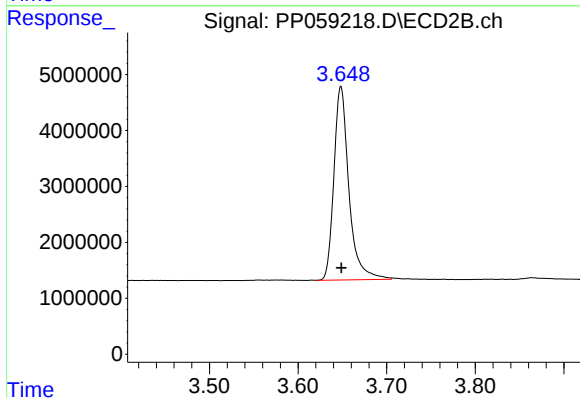


#1 Tetrachloro-m-xylene

R.T.: 3.648 min
Delta R.T.: 0.000 min
Response: 40706303
Conc: 20.09 ng/ml

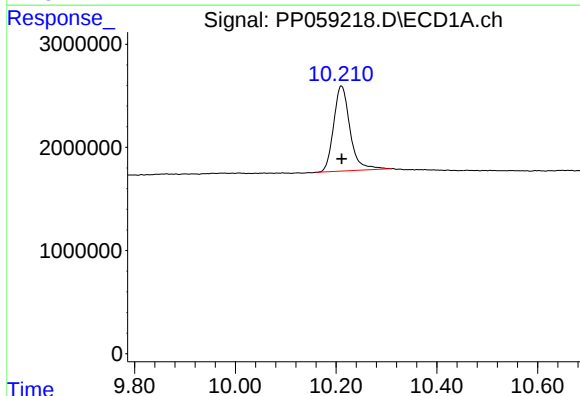


#2 Decachlorobiphenyl

R.T.: 10.211 min
Delta R.T.: 0.000 min
Response: 18674481
Conc: 24.47 ng/ml

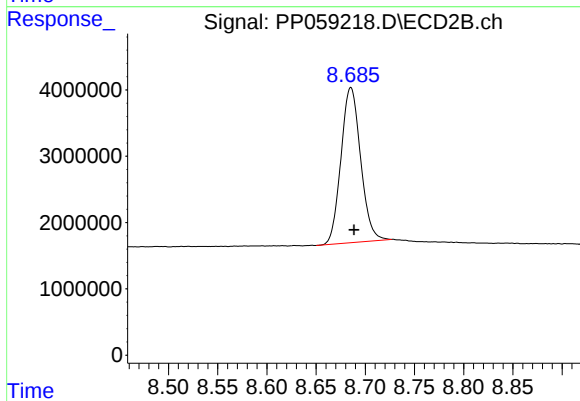

#2 Decachlorobiphenyl


R.T.: 8.685 min
Delta R.T.: -0.003 min
Response: 32463534
Conc: 23.08 ng/ml

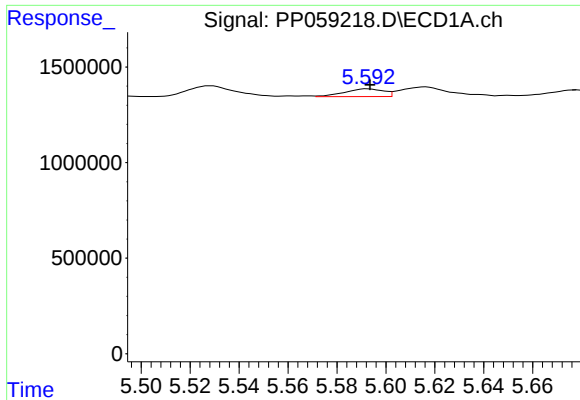

#3 AR-1016-1


R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 451319
Conc: 11.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

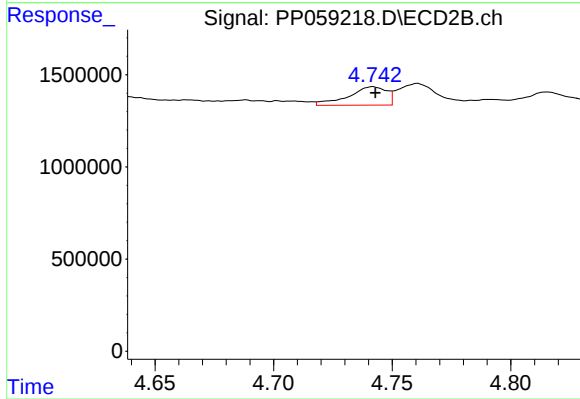


#3 AR-1016-1

R.T.: 4.742 min
Delta R.T.: -0.001 min
Response: 1119960
Conc: 17.46 ng/ml

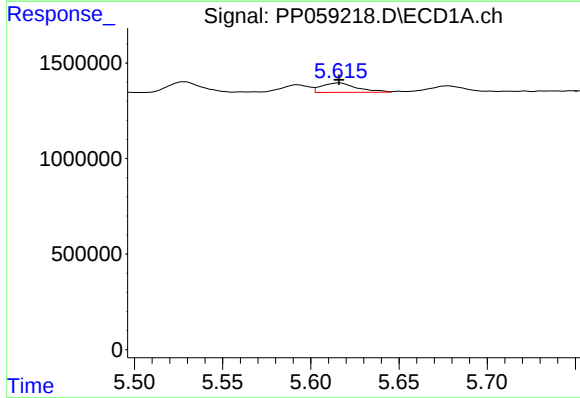


#4 AR-1016-2

R.T.: 5.616 min
Delta R.T.: 0.000 min
Response: 687430
Conc: 12.13 ng/ml

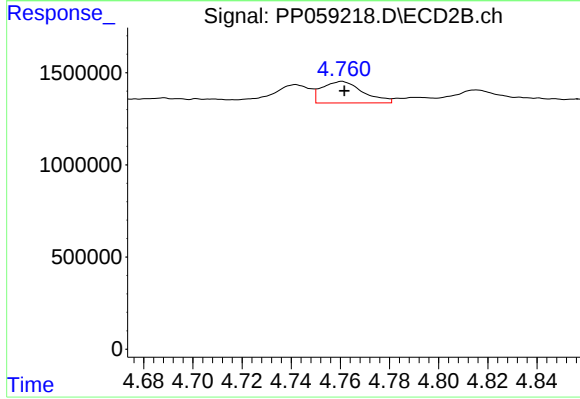

#4 AR-1016-2


R.T.: 4.761 min
Delta R.T.: 0.000 min
Response: 1358551
Conc: 14.96 ng/ml

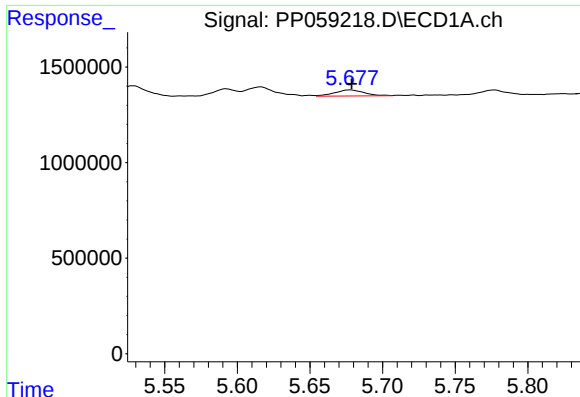

#5 AR-1016-3


R.T.: 5.678 min
Delta R.T.: -0.001 min
Response: 445613
Conc: 12.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

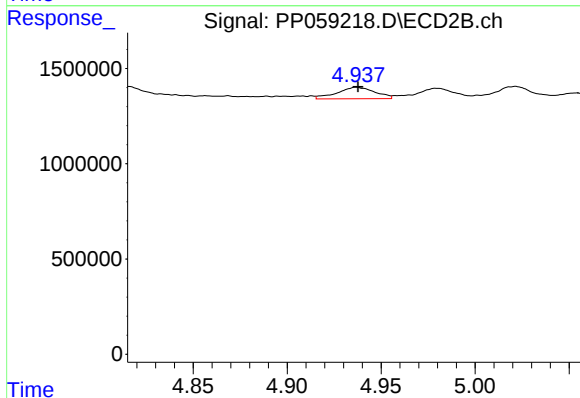


#5 AR-1016-3

R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 849978
Conc: 17.69 ng/ml

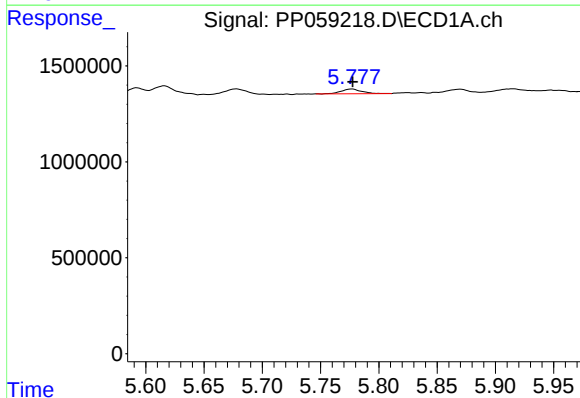


#6 AR-1016-4

R.T.: 5.777 min
Delta R.T.: 0.000 min
Response: 295362
Conc: 10.20 ng/ml

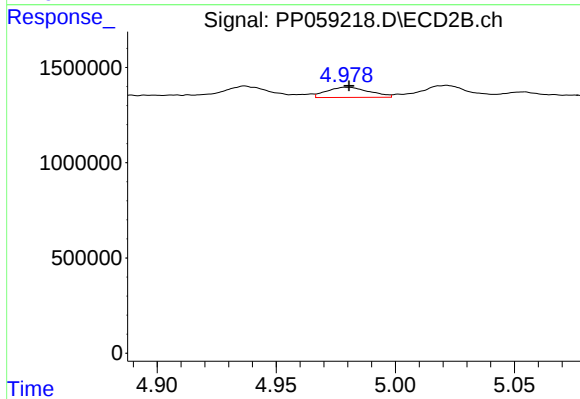

#6 AR-1016-4


R.T.: 4.979 min
Delta R.T.: -0.002 min
Response: 663649
Conc: 16.07 ng/ml

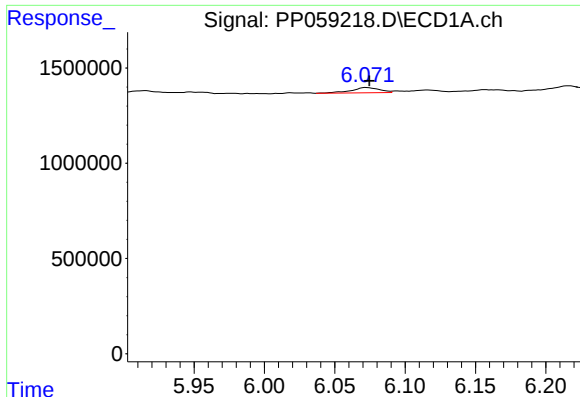

#7 AR-1016-5


R.T.: 6.072 min
Delta R.T.: -0.002 min
Response: 384838
Conc: 12.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

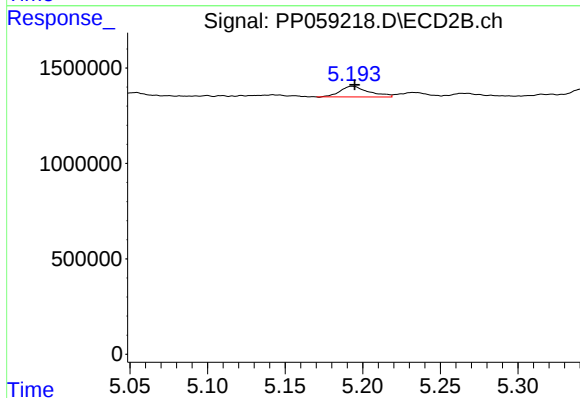


#7 AR-1016-5

R.T.: 5.193 min
Delta R.T.: -0.002 min
Response: 721806
Conc: 13.87 ng/ml

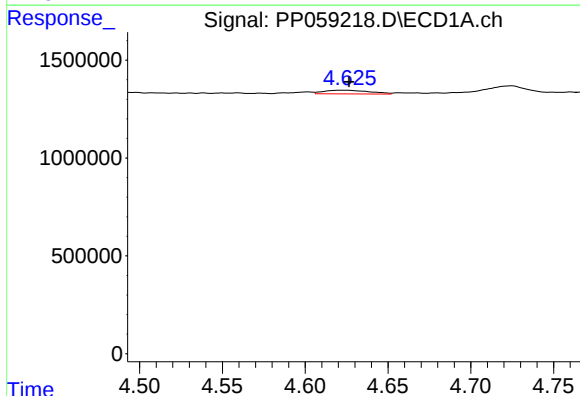


#8 AR-1221-1

R.T.: 4.625 min
Delta R.T.: -0.001 min
Response: 368540
Conc: 23.39 ng/ml

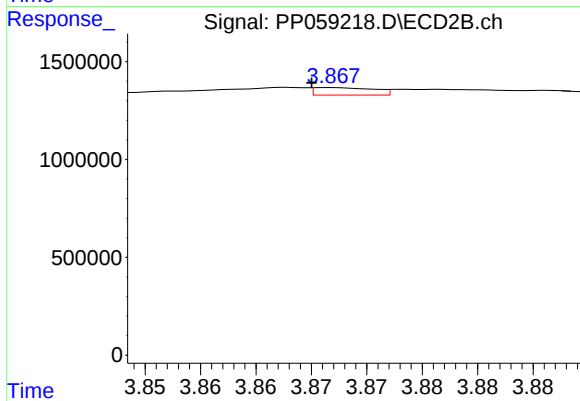

#8 AR-1221-1


R.T.: 3.867 min
Delta R.T.: 0.002 min
Response: 143758
Conc: 5.30 ng/ml

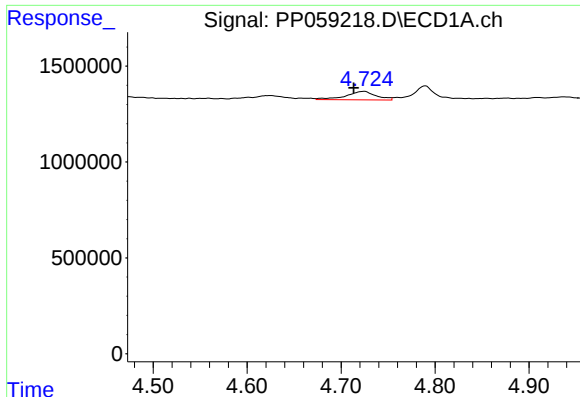

#9 AR-1221-2


R.T.: 4.725 min
Delta R.T.: 0.011 min
Response: 987903
Conc: 83.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

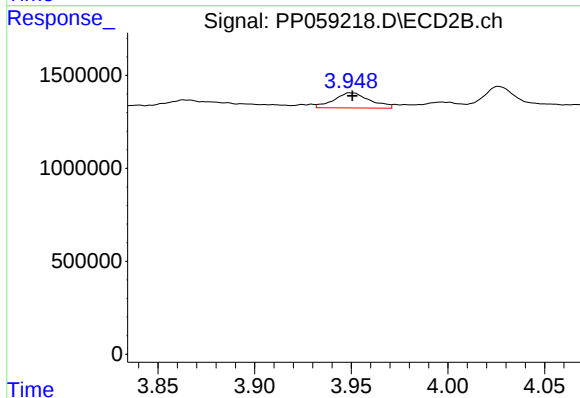


#9 AR-1221-2

R.T.: 3.949 min
Delta R.T.: -0.002 min
Response: 1055954
Conc: 53.04 ng/ml

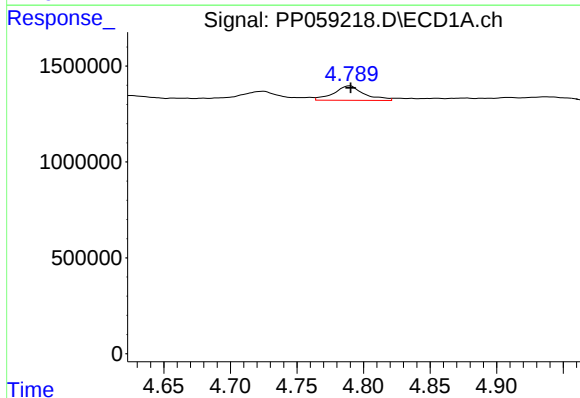


#10 AR-1221-3

R.T.: 4.790 min
Delta R.T.: 0.000 min
Response: 1186654
Conc: 33.70 ng/ml

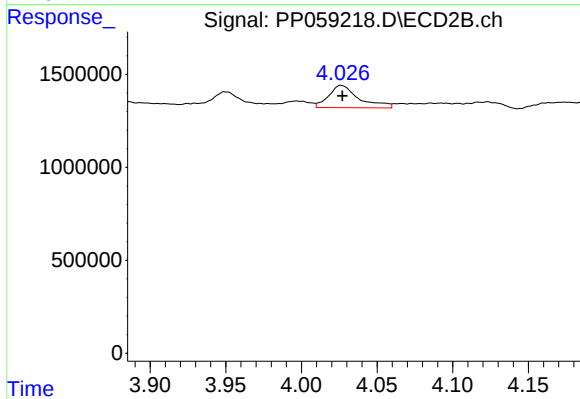

#10 AR-1221-3


R.T.: 4.026 min
Delta R.T.: -0.001 min
Response: 1666964
Conc: 28.00 ng/ml

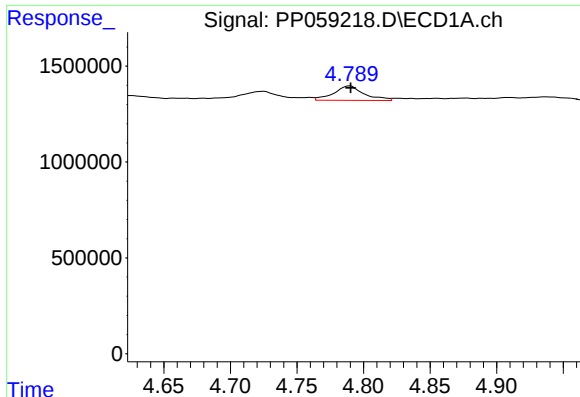

#11 AR-1232-1


R.T.: 4.790 min
Delta R.T.: 0.000 min
Response: 1186654
Conc: 40.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

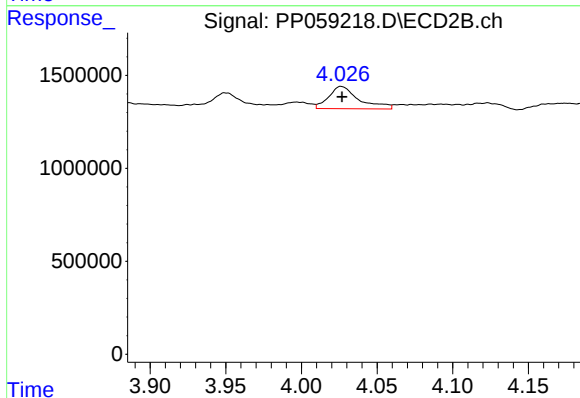


#11 AR-1232-1

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 1666964
Conc: 35.13 ng/ml

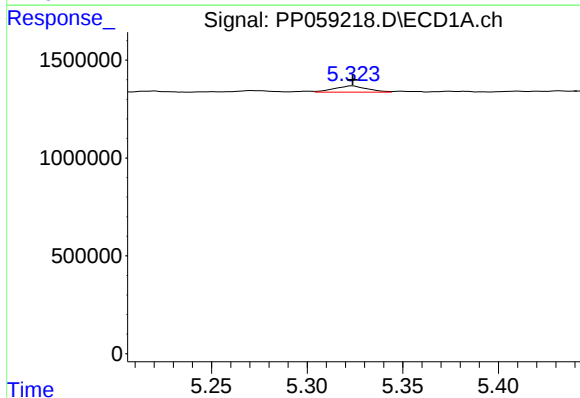


#12 AR-1232-2

R.T.: 5.324 min
Delta R.T.: 0.000 min
Response: 382431
Conc: 24.54 ng/ml

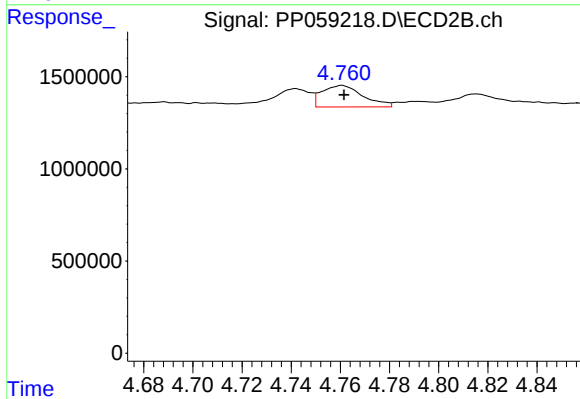

#12 AR-1232-2


R.T.: 4.761 min
Delta R.T.: 0.000 min
Response: 1358551
Conc: 32.03 ng/ml

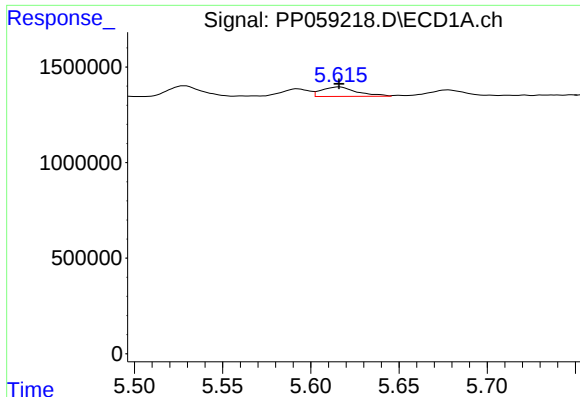

#13 AR-1232-3


R.T.: 5.616 min
Delta R.T.: 0.000 min
Response: 687430
Conc: 26.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

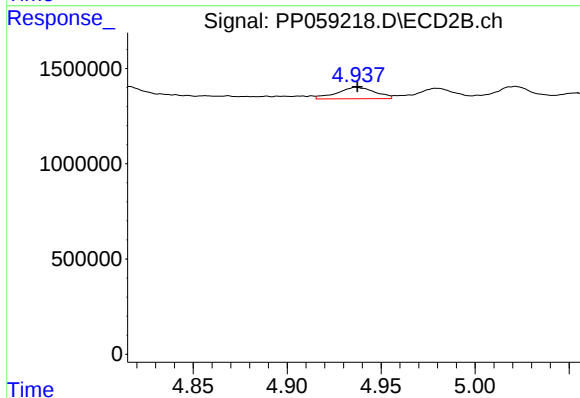


#13 AR-1232-3

R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 849978
Conc: 38.31 ng/ml

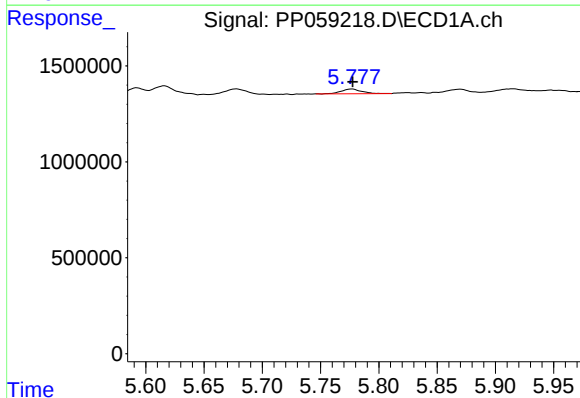


#14 AR-1232-4

R.T.: 5.777 min
Delta R.T.: 0.000 min
Response: 295362
Conc: 22.32 ng/ml

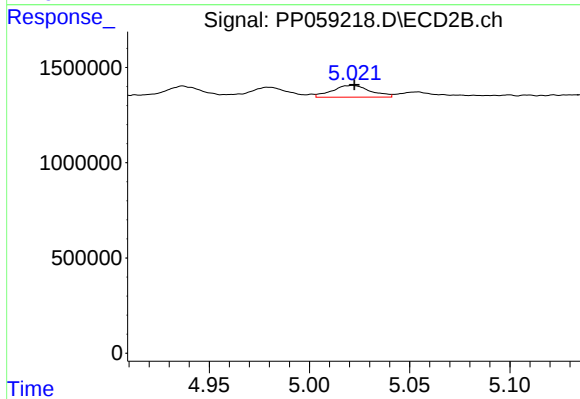

#14 AR-1232-4


R.T.: 5.022 min
Delta R.T.: 0.000 min
Response: 824710
Conc: 39.06 ng/ml

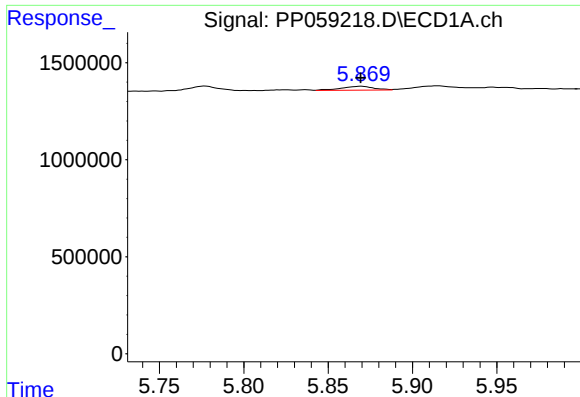

#15 AR-1232-5


R.T.: 5.870 min
Delta R.T.: 0.000 min
Response: 267707
Conc: 23.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

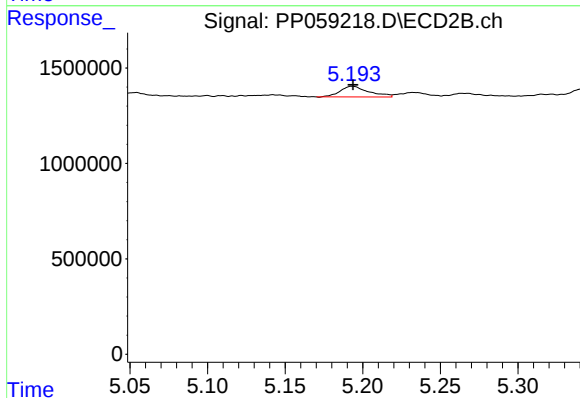


#15 AR-1232-5

R.T.: 5.193 min
Delta R.T.: 0.000 min
Response: 721806
Conc: 31.49 ng/ml

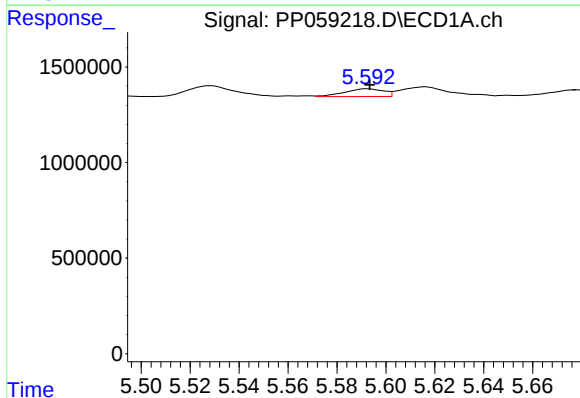


#16 AR-1242-1

R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 451319
Conc: 13.18 ng/ml

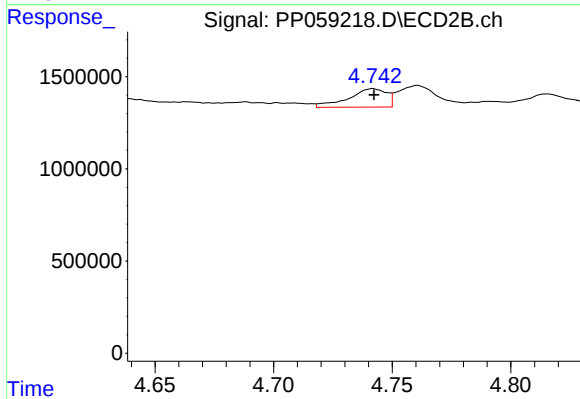

#16 AR-1242-1


R.T.: 4.742 min
Delta R.T.: 0.000 min
Response: 1119960
Conc: 20.01 ng/ml

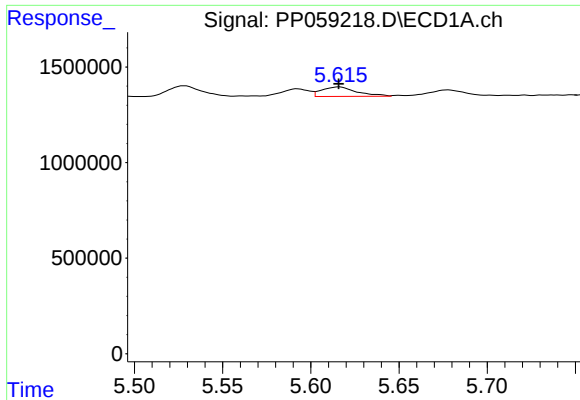

#17 AR-1242-2


R.T.: 5.616 min
Delta R.T.: 0.000 min
Response: 687430
Conc: 14.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

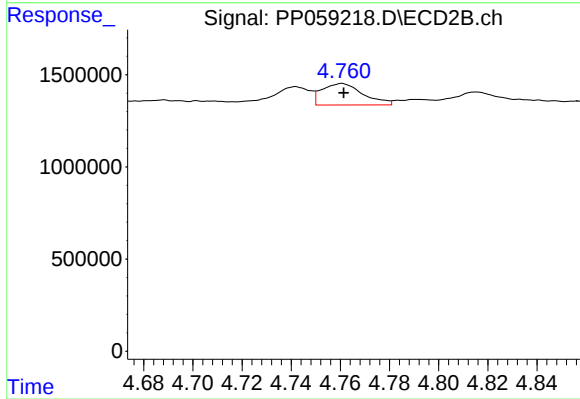


#17 AR-1242-2

R.T.: 4.761 min
Delta R.T.: 0.000 min
Response: 1358551
Conc: 17.04 ng/ml

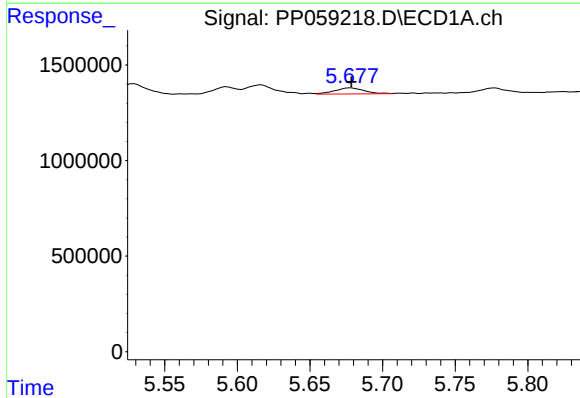


#18 AR-1242-3

R.T.: 5.678 min
Delta R.T.: 0.000 min
Response: 445613
Conc: 14.18 ng/ml

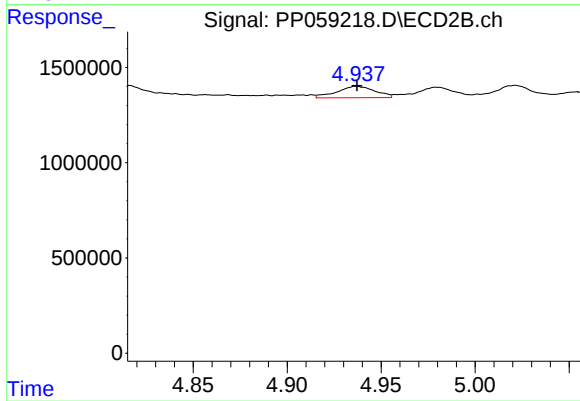

#18 AR-1242-3


R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 849978
Conc: 19.94 ng/ml

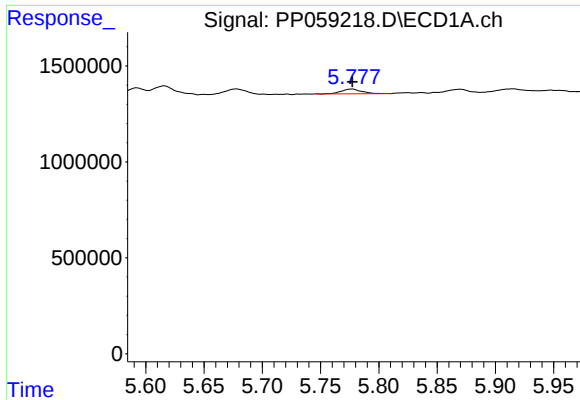

#19 AR-1242-4


R.T.: 5.777 min
Delta R.T.: 0.000 min
Response: 295362
Conc: 11.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

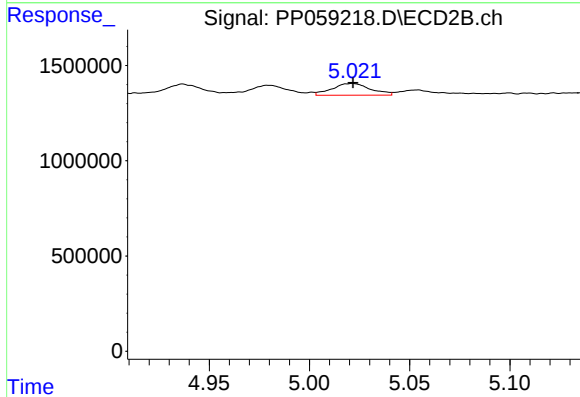


#19 AR-1242-4

R.T.: 5.022 min
Delta R.T.: 0.000 min
Response: 824710
Conc: 18.89 ng/ml

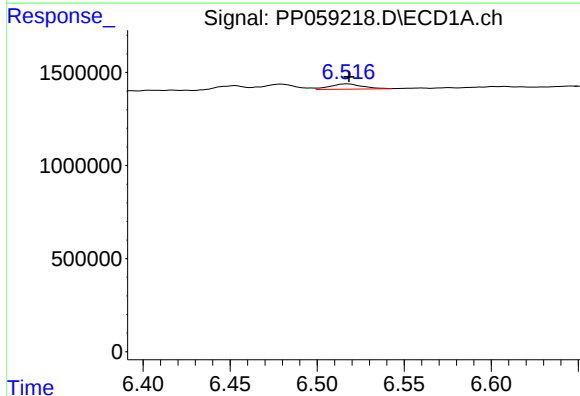


#20 AR-1242-5

R.T.: 6.517 min
Delta R.T.: -0.001 min
Response: 366714
Conc: 14.19 ng/ml

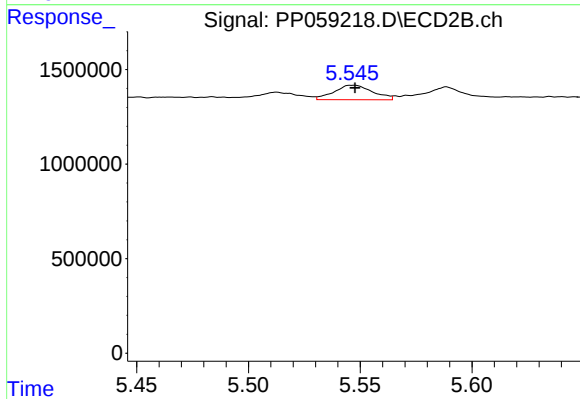

#20 AR-1242-5


R.T.: 5.547 min
Delta R.T.: 0.000 min
Response: 925565
Conc: 18.63 ng/ml

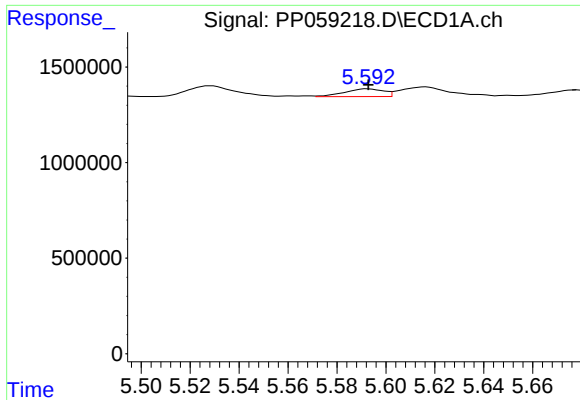

#21 AR-1248-1


R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 451319
Conc: 17.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

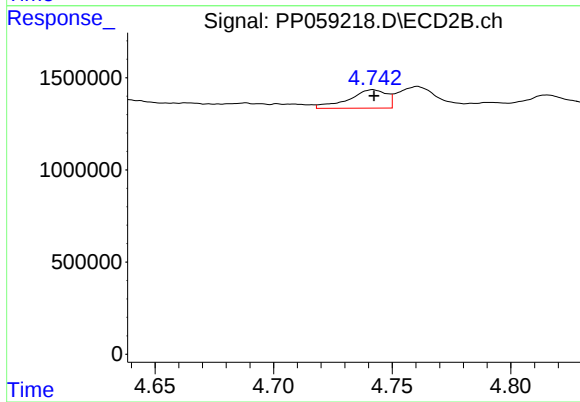


#21 AR-1248-1

R.T.: 4.742 min
Delta R.T.: 0.000 min
Response: 1119960
Conc: 27.22 ng/ml

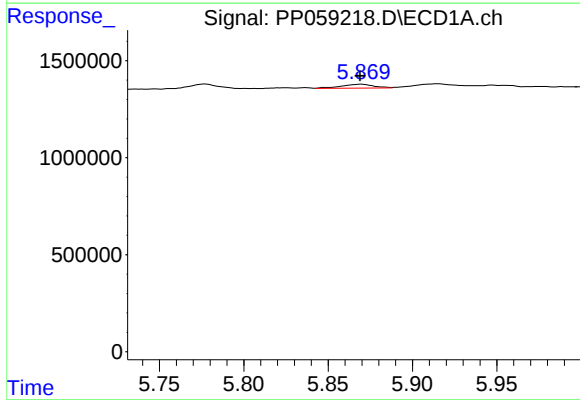


#22 AR-1248-2

R.T.: 5.870 min
Delta R.T.: 0.001 min
Response: 267707
Conc: 6.92 ng/ml

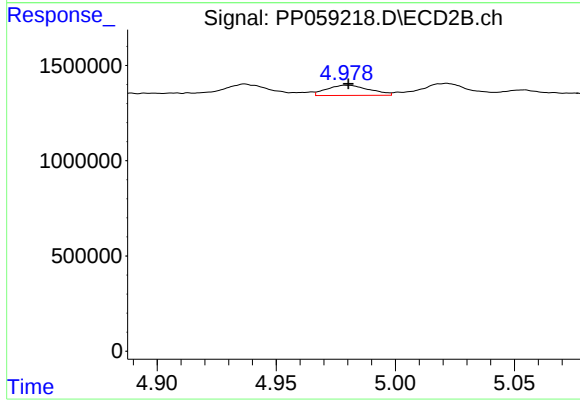

#22 AR-1248-2


R.T.: 4.979 min
Delta R.T.: -0.002 min
Response: 663649
Conc: 11.02 ng/ml

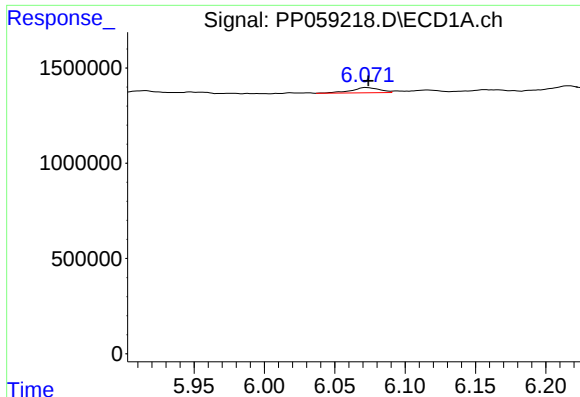

#23 AR-1248-3


R.T.: 6.072 min
Delta R.T.: -0.002 min
Response: 384838
Conc: 9.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

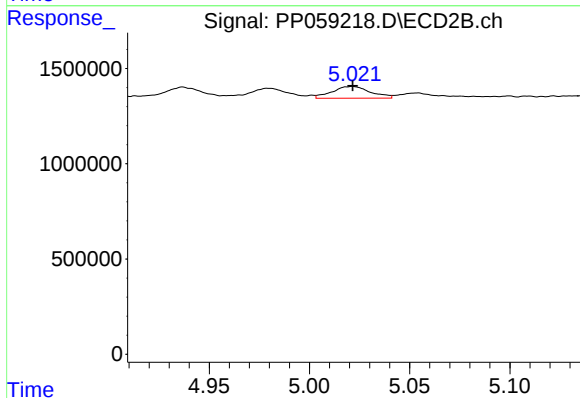


#23 AR-1248-3

R.T.: 5.022 min
Delta R.T.: 0.000 min
Response: 824710
Conc: 13.39 ng/ml

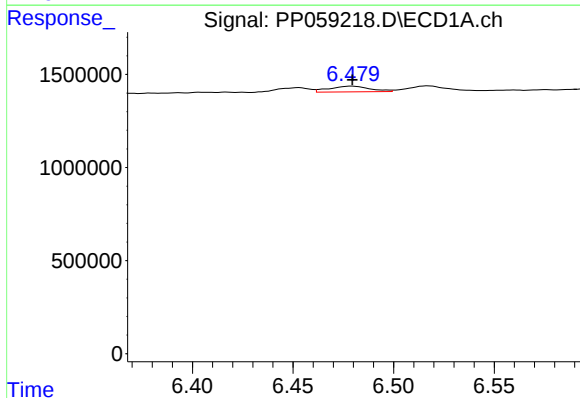


#24 AR-1248-4

R.T.: 6.479 min
Delta R.T.: 0.000 min
Response: 428180
Conc: 10.28 ng/ml

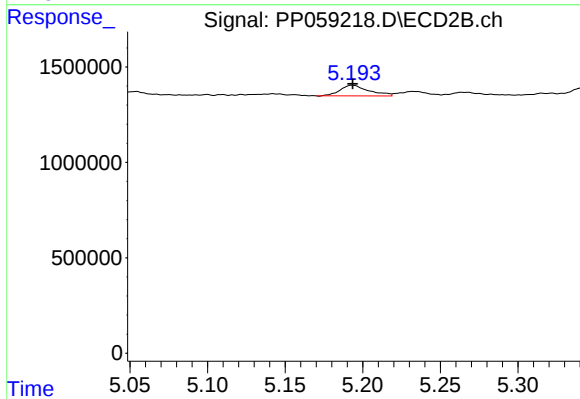

#24 AR-1248-4


R.T.: 5.193 min
Delta R.T.: 0.000 min
Response: 721806
Conc: 10.03 ng/ml

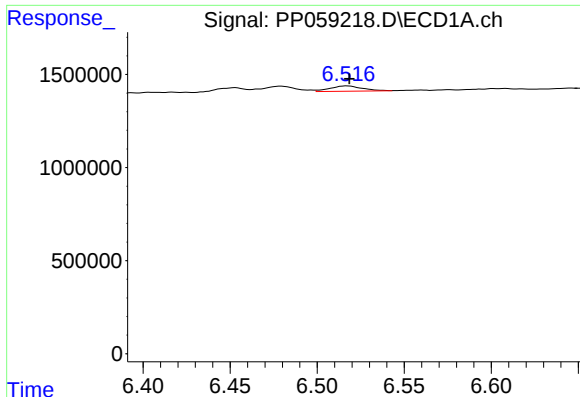

#25 AR-1248-5


R.T.: 6.517 min
Delta R.T.: -0.001 min
Response: 366714
Conc: 8.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

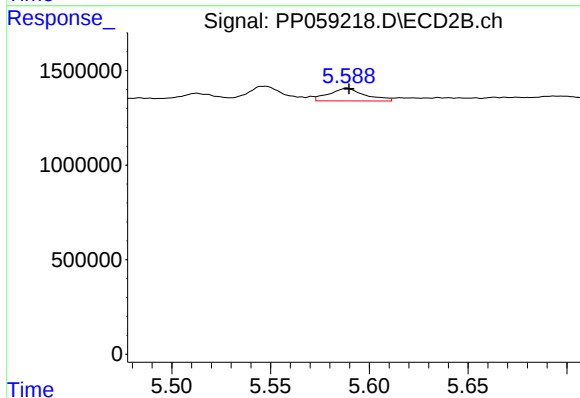


#25 AR-1248-5

R.T.: 5.589 min
Delta R.T.: -0.001 min
Response: 855046
Conc: 12.96 ng/ml

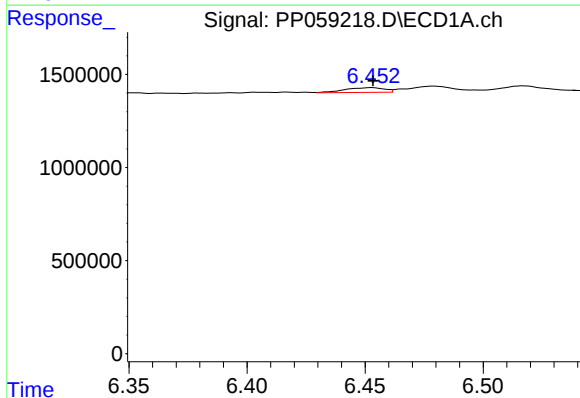


#26 AR-1254-1

R.T.: 6.453 min
Delta R.T.: 0.000 min
Response: 290688
Conc: 6.22 ng/ml

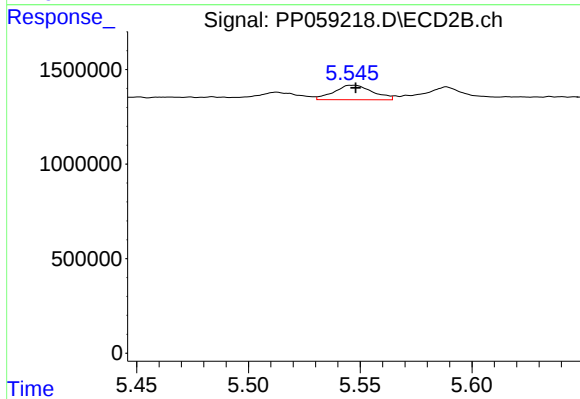

#26 AR-1254-1


R.T.: 5.547 min
Delta R.T.: 0.000 min
Response: 925565
Conc: 9.14 ng/ml

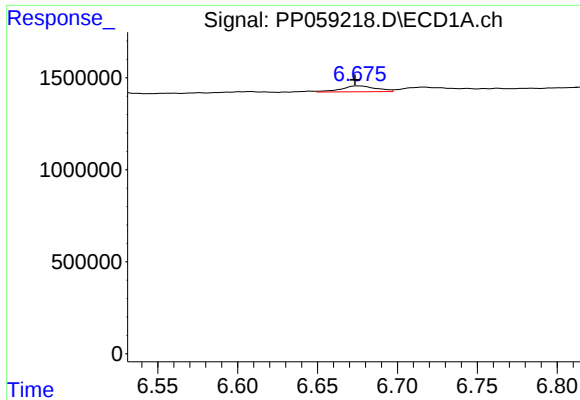

#27 AR-1254-2


R.T.: 6.676 min
Delta R.T.: 0.003 min
Response: 488624
Conc: 7.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

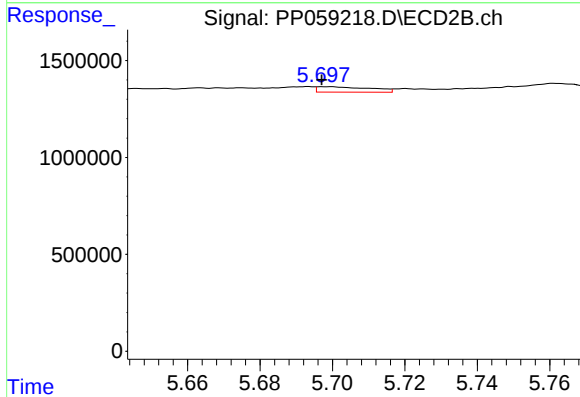


#27 AR-1254-2

R.T.: 5.700 min
Delta R.T.: 0.003 min
Response: 285645
Conc: 3.24 ng/ml

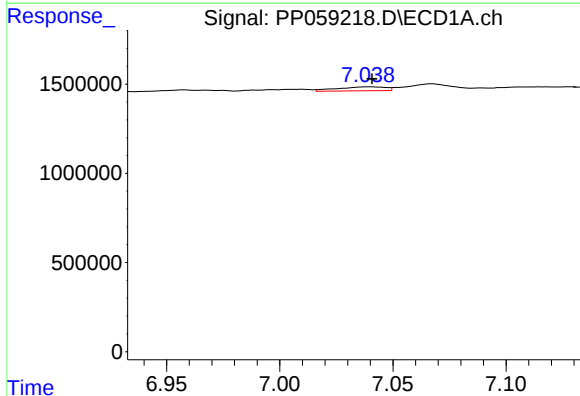


#28 AR-1254-3

R.T.: 7.040 min
Delta R.T.: -0.001 min
Response: 331869
Conc: 4.81 ng/ml

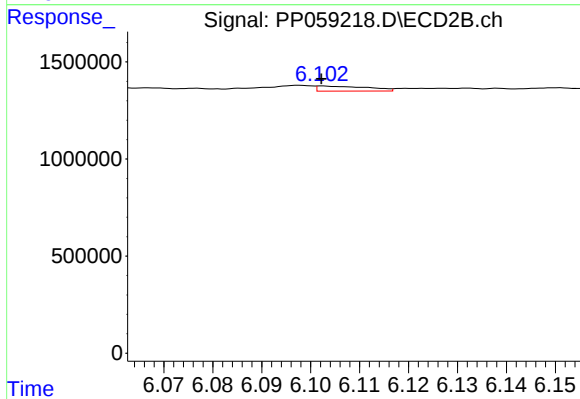

#28 AR-1254-3


R.T.: 6.102 min
Delta R.T.: 0.000 min
Response: 186861
Conc: 1.35 ng/ml

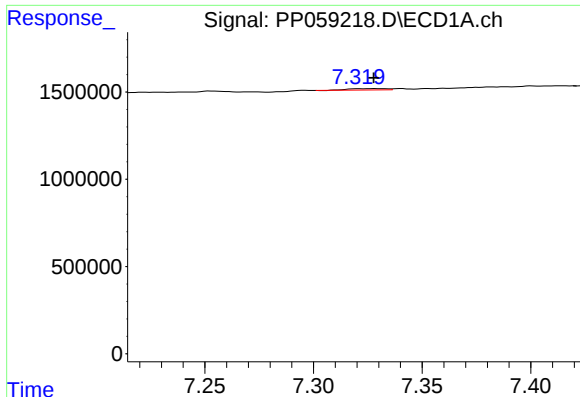

#29 AR-1254-4


R.T.: 7.329 min
Delta R.T.: 0.000 min
Response: 98314
Conc: 2.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

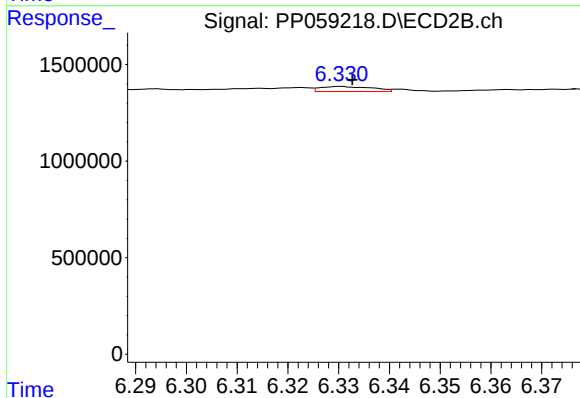


#29 AR-1254-4

R.T.: 6.330 min
Delta R.T.: -0.002 min
Response: 182582
Conc: 2.27 ng/ml

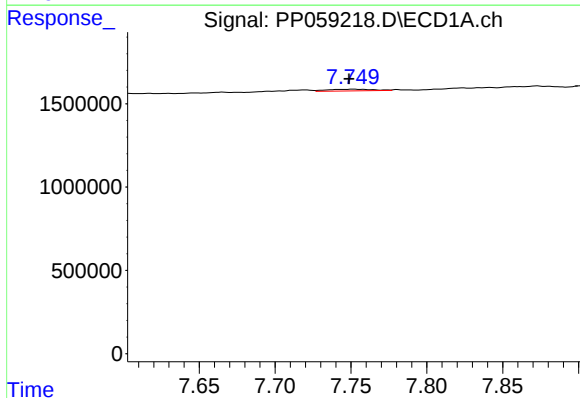


#30 AR-1254-5

R.T.: 7.752 min
Delta R.T.: 0.003 min
Response: 203584
Conc: 4.33 ng/ml

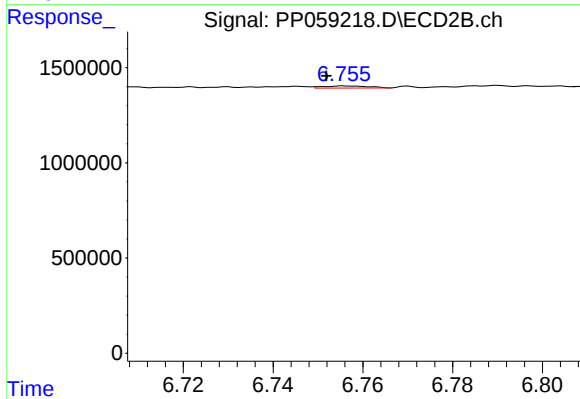

#30 AR-1254-5


R.T.: 6.756 min
Delta R.T.: 0.004 min
Response: 75981
Conc: 0.64 ng/ml

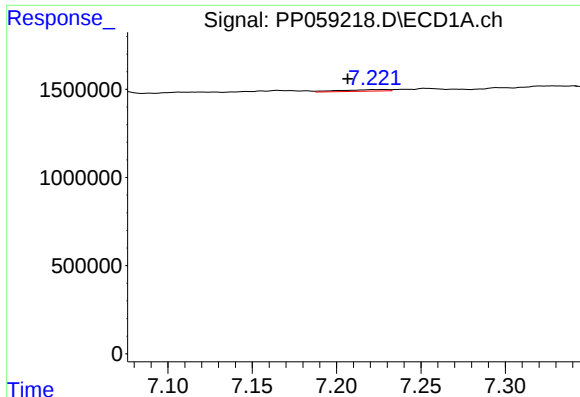

#31 AR-1260-1


R.T.: 7.222 min
Delta R.T.: 0.015 min
Response: 175944
Conc: 3.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

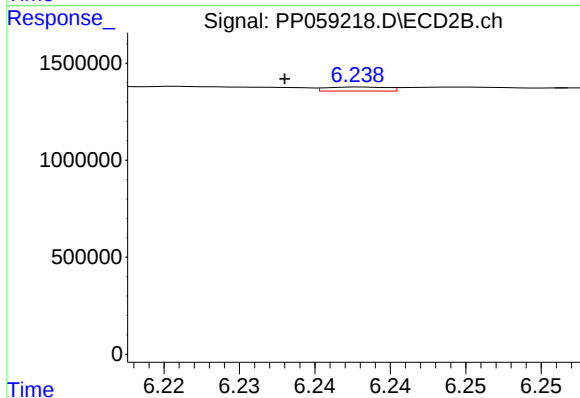


#31 AR-1260-1

R.T.: 6.238 min
Delta R.T.: 0.005 min
Response: 58161
Conc: 0.59 ng/ml

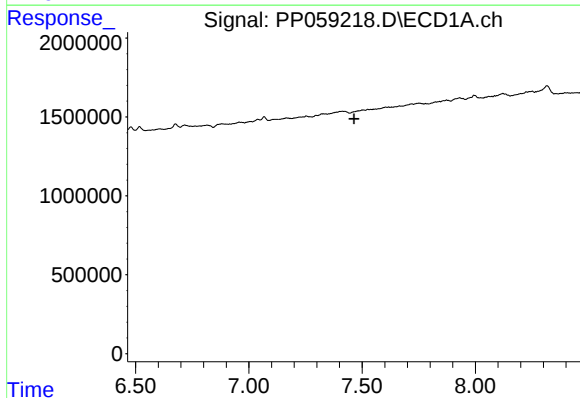


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.464 min
Response: 0
Conc: N.D.

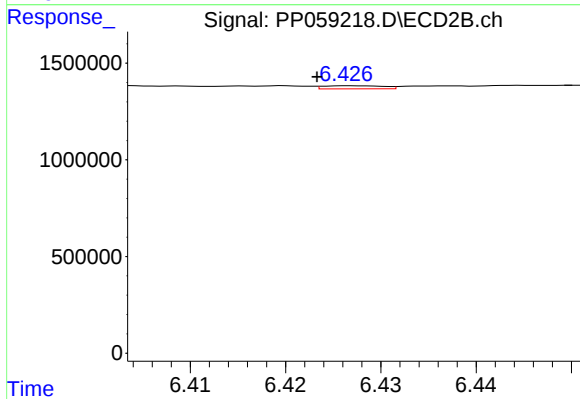

#32 AR-1260-2


R.T.: 6.427 min
Delta R.T.: 0.003 min
Response: 70006
Conc: 0.61 ng/ml

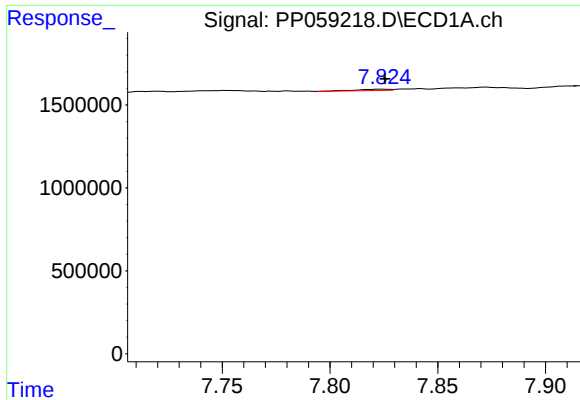

#33 AR-1260-3


R.T.: 7.824 min
Delta R.T.: -0.002 min
Response: 83987
Conc: 2.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

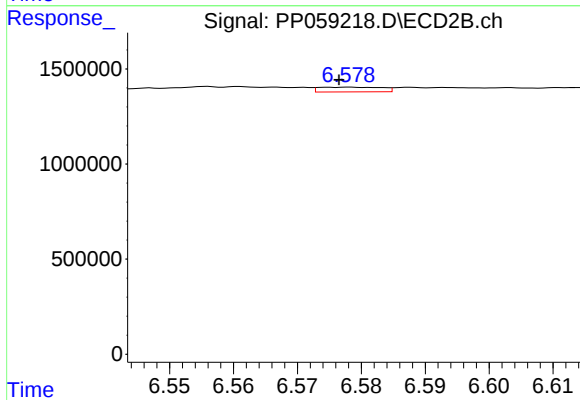


#33 AR-1260-3

R.T.: 6.578 min
Delta R.T.: 0.002 min
Response: 169448
Conc: 1.52 ng/ml

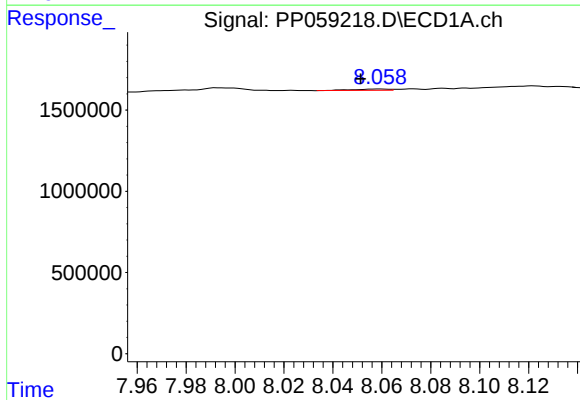


#34 AR-1260-4

R.T.: 8.059 min
Delta R.T.: 0.008 min
Response: 83430
Conc: 1.88 ng/ml

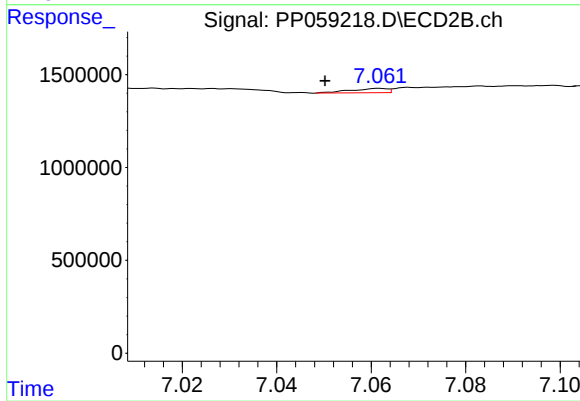

#34 AR-1260-4


R.T.: 7.062 min
Delta R.T.: 0.012 min
Response: 126576
Conc: 1.46 ng/ml

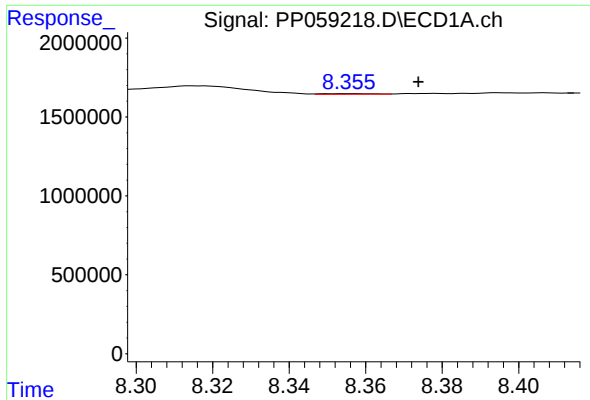

#35 AR-1260-5


R.T.: 8.356 min
Delta R.T.: -0.018 min
Response: 39734
Conc: 0.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

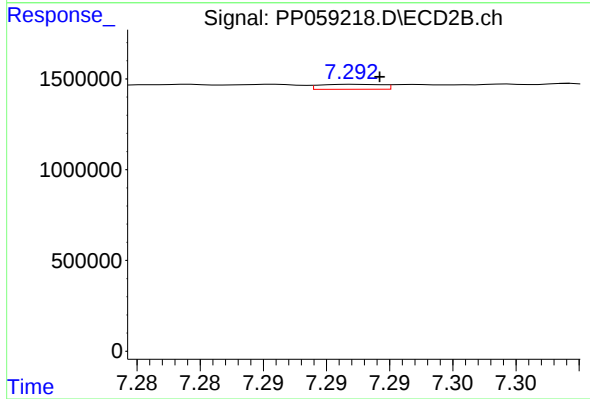


#35 AR-1260-5

R.T.: 7.292 min
Delta R.T.: -0.002 min
Response: 93552
Conc: 0.51 ng/ml

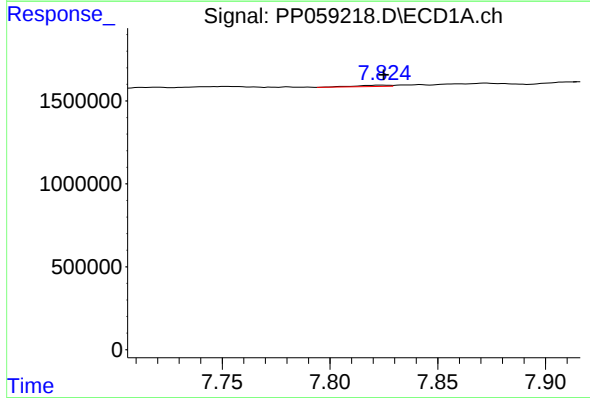


#36 AR-1262-1

R.T.: 7.824 min
Delta R.T.: 0.000 min
Response: 83987
Conc: 1.32 ng/ml

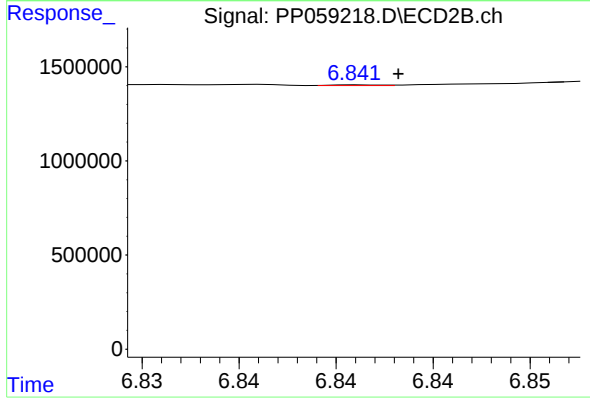

#36 AR-1262-1


R.T.: 6.841 min
Delta R.T.: -0.002 min
Response: 5792
Conc: 0.10 ng/ml

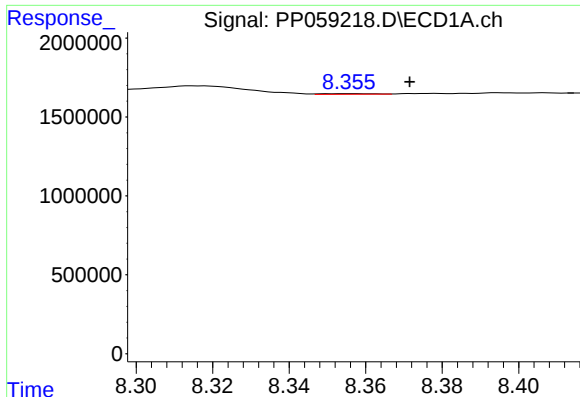

#37 AR-1262-2


R.T.: 8.356 min
Delta R.T.: -0.016 min
Response: 39734
Conc: 0.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

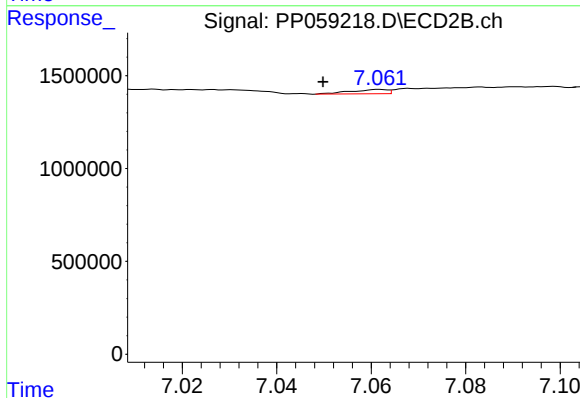


#37 AR-1262-2

R.T.: 7.062 min
Delta R.T.: 0.012 min
Response: 126576
Conc: 1.07 ng/ml

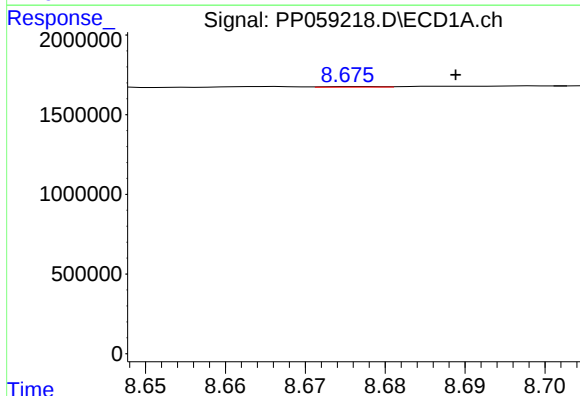


#38 AR-1262-3

R.T.: 8.677 min
Delta R.T.: -0.012 min
Response: 16220
Conc: 0.25 ng/ml

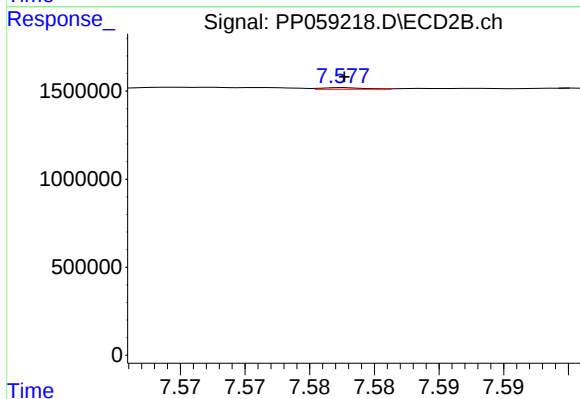

#38 AR-1262-3


R.T.: 7.578 min
Delta R.T.: 0.000 min
Response: 21500
Conc: 0.25 ng/ml

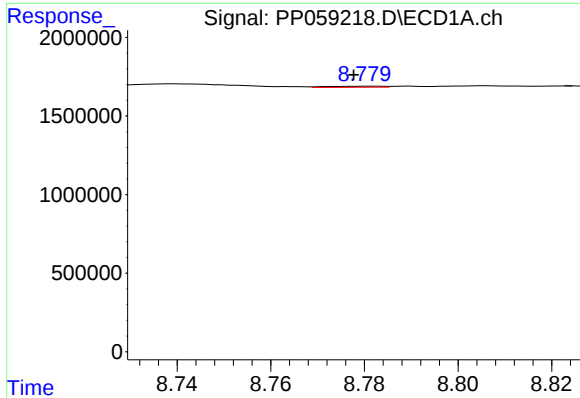

#39 AR-1262-4


R.T.: 8.781 min
Delta R.T.: 0.003 min
Response: 54024
Conc: 1.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

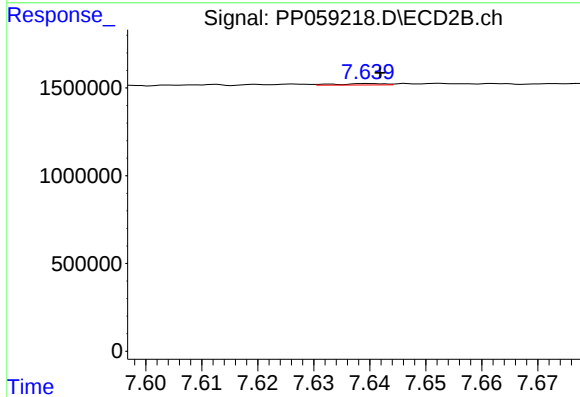


#39 AR-1262-4

R.T.: 7.639 min
Delta R.T.: -0.002 min
Response: 48634
Conc: 0.32 ng/ml

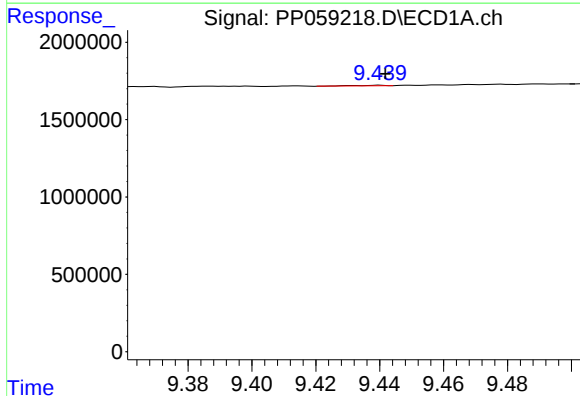


#40 AR-1262-5

R.T.: 9.440 min
Delta R.T.: -0.002 min
Response: 24642
Conc: 0.83 ng/ml

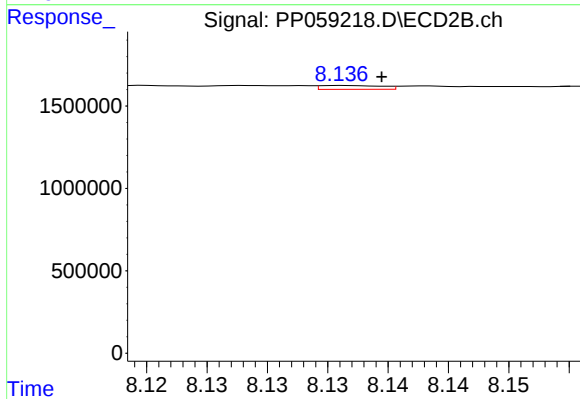

#40 AR-1262-5


R.T.: 8.136 min
Delta R.T.: -0.003 min
Response: 82482
Conc: 1.29 ng/ml

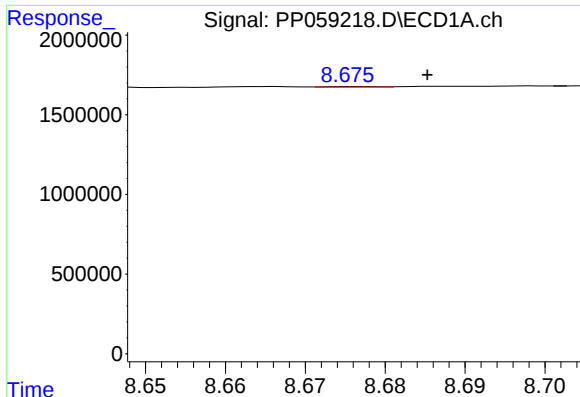

#41 AR-1268-1


R.T.: 8.677 min
Delta R.T.: -0.009 min
Response: 16220
Conc: 0.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

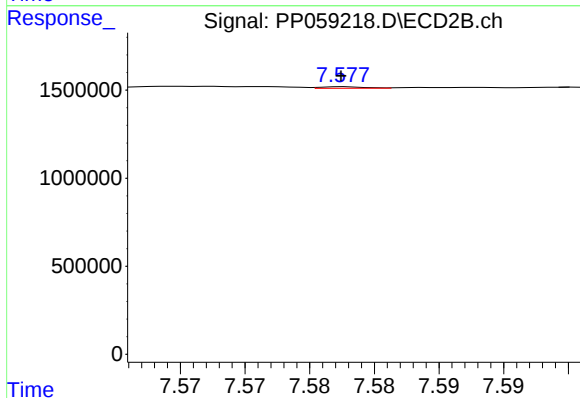


#41 AR-1268-1

R.T.: 7.578 min
Delta R.T.: 0.000 min
Response: 21500
Conc: 0.09 ng/ml

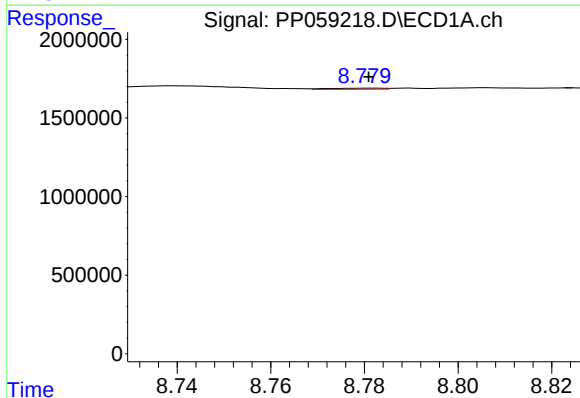


#42 AR-1268-2

R.T.: 8.781 min
Delta R.T.: 0.000 min
Response: 54024
Conc: 0.55 ng/ml

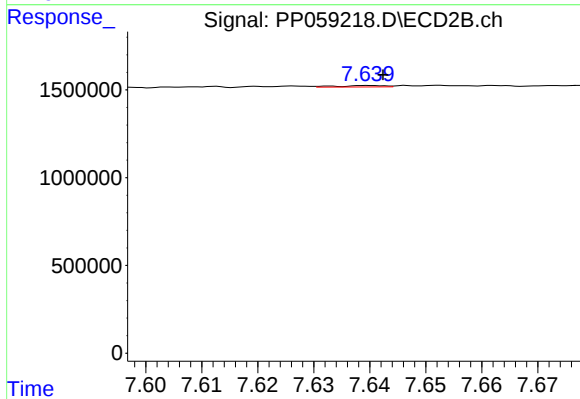

#42 AR-1268-2


R.T.: 7.639 min
Delta R.T.: -0.003 min
Response: 48634
Conc: 0.22 ng/ml

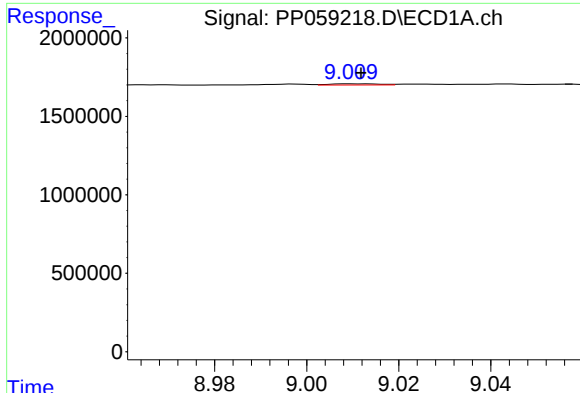

#43 AR-1268-3


R.T.: 9.010 min
Delta R.T.: -0.002 min
Response: 58775
Conc: 0.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

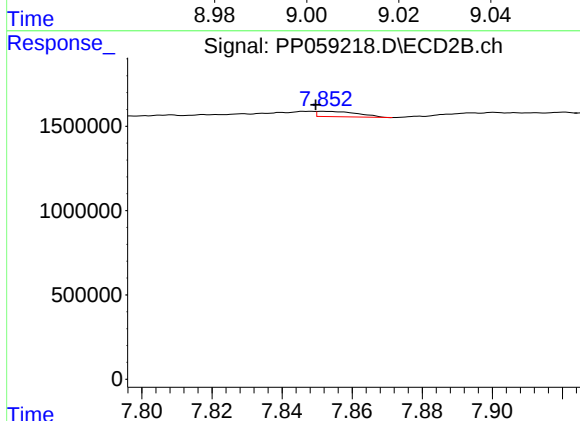


#43 AR-1268-3

R.T.: 7.852 min
Delta R.T.: 0.002 min
Response: 253916
Conc: 1.30 ng/ml

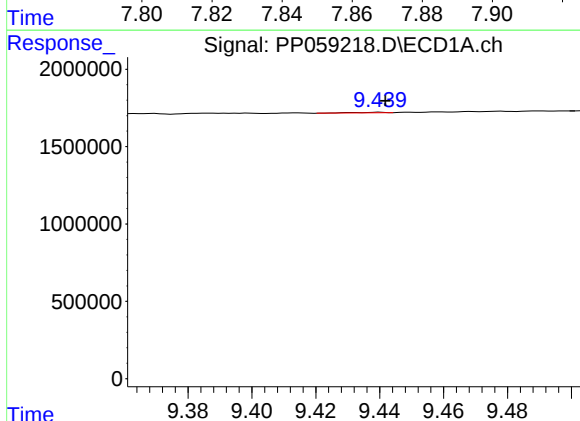


#44 AR-1268-4

R.T.: 9.440 min
Delta R.T.: -0.002 min
Response: 24642
Conc: 0.77 ng/ml

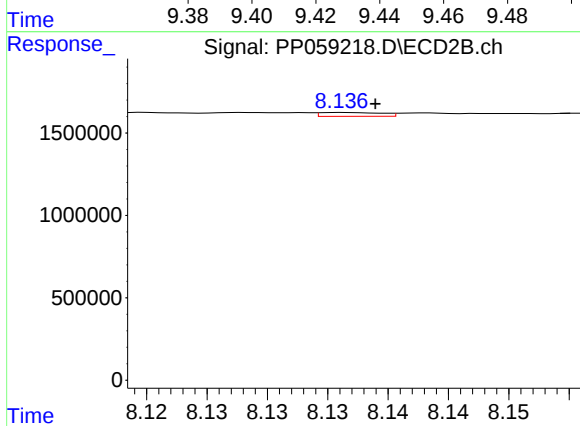

#44 AR-1268-4


R.T.: 8.136 min
Delta R.T.: -0.003 min
Response: 82482
Conc: 1.19 ng/ml

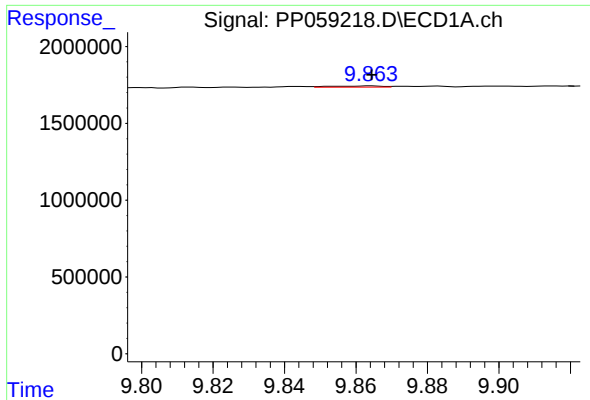

#45 AR-1268-5

R.T.: 9.864 min
Delta R.T.: 0.000 min
Response: 74022
Conc: 0.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

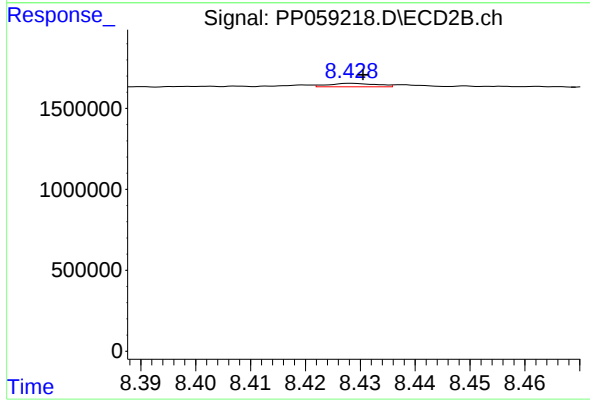

#45 AR-1268-5

R.T.: 8.428 min
Delta R.T.: -0.002 min
Response: 127911
Conc: 0.25 ng/ml