

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
 Data File : PP059222.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2023 00:15
 Operator : YP\AJ
 Sample : 03572-07
 Misc : AR1262 LOD 25 PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 02:44:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.415	3.648	24019553	40897029	19.575	20.185
2)	SA Decachlor...	10.210	8.685	18624780	33596544	24.402	23.881
Target Compounds							
3)	L1 AR-1016-1	5.594	4.744	96102	226316	2.446	3.529 #
4)	L1 AR-1016-2	5.620	4.758	180322	408320	3.181	4.495 #
5)	L1 AR-1016-3	5.674	4.936	118423	100974	3.301	2.102 #
6)	L1 AR-1016-4	5.774	4.982	30611	299166	1.057	7.245 #
7)	L1 AR-1016-5	6.071	5.194	147955	123240	4.889	2.369 #
8)	L2 AR-1221-1	4.629	3.860	83409	90079	5.294	3.318 #
9)	L2 AR-1221-2	4.724	3.949	771336	1067103	65.318	53.597
10)	L2 AR-1221-3	4.790	4.028	525718	143787	14.930	2.415 #
11)	L3 AR-1232-1	4.790	4.028	525718	143787	17.884	3.030 #
12)	L3 AR-1232-2	5.325	4.758	72647	408320	4.661	9.626 #
13)	L3 AR-1232-3	5.620	4.936	180322	100974	6.829	4.551 #
14)	L3 AR-1232-4	5.774	5.022	30611	514187	2.313	24.353 #
15)	L3 AR-1232-5	5.867	5.194	116519	123240	10.208	5.376 #
16)	L4 AR-1242-1	5.594	4.744	96102	226316	2.807	4.044 #
17)	L4 AR-1242-2	5.620	4.758	180322	408320	3.675	5.121 #
18)	L4 AR-1242-3	5.674	4.936	118423	100974	3.769	2.369 #
19)	L4 AR-1242-4	5.774	5.022	30611	514187	1.194	11.775 #
20)	L4 AR-1242-5	6.516	5.548	147605	756824	5.714	15.236 #
21)	L5 AR-1248-1	5.594	4.744	96102	226316	3.786	5.501 #
22)	L5 AR-1248-2	5.867	4.982	116519	299166	3.010	4.968 #
23)	L5 AR-1248-3	6.071	5.022	147955	514187	3.502	8.346 #
24)	L5 AR-1248-4	6.479	5.194	130840	123240	3.143	1.712 #
25)	L5 AR-1248-5	6.516	5.589	147605	359355	3.619	5.446 #
26)	L6 AR-1254-1	6.453	5.548	380978	756824	8.155	7.470
27)	L6 AR-1254-2	6.673	5.697	453757	962213	6.595	10.900 #
28)	L6 AR-1254-3	7.041	6.116	392236	1748355	5.683	12.647 #
29)	L6 AR-1254-4	7.324	6.331	69915	170509	1.553	2.121 #
30)	L6 AR-1254-5	7.744	6.749	1319954	1729115	28.092	14.459 #
31)	L7 AR-1260-1	7.205	6.231	1597913	2540297	29.207	25.650
32)	L7 AR-1260-2	7.463	6.421	1319186	2721010	22.157	23.516
33)	L7 AR-1260-3	7.825	6.577	1872951	3084809	47.591	27.733 #
34)	L7 AR-1260-4	8.050	7.048	1357813	2834498	30.572	32.695
35)	L7 AR-1260-5	8.371	7.292	2347780	6096818	29.358	33.077
36)	L8 AR-1262-1	7.825	6.843	1872951	1474799	29.407	25.633
37)	L8 AR-1262-2	8.371	7.048	2347780	2834498	25.565	24.022
38)	L8 AR-1262-3	8.688	7.577	1680863	2412627	26.119	28.351
39)	L8 AR-1262-4	8.779	7.640	803487	3985299	24.196	26.382
40)	L8 AR-1262-5	9.443	8.138	652150	2100326	21.854	32.933 #
41)	L9 AR-1268-1	8.688	7.577	1680863	2412627	14.801	9.894 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
 Data File : PP059222.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2023 00:15
 Operator : YP\AJ
 Sample : 03572-07
 Misc : AR1262 LOD 25 PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 02:44:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.779	7.640	803487	3985299	8.164	18.196 #
43) L9	AR-1268-3	9.014	7.849	121291	596235	1.308	3.049 #
44) L9	AR-1268-4	9.443	8.138	652150	2100326	20.443	30.181 #
45) L9	AR-1268-5	9.865	8.430	311792	768459	1.149	1.482 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
Data File : PP059222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2023 00:15
Operator : YP\AJ
Sample : 03572-07
Misc : AR1262 LOD 25 PPB
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 02:44:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

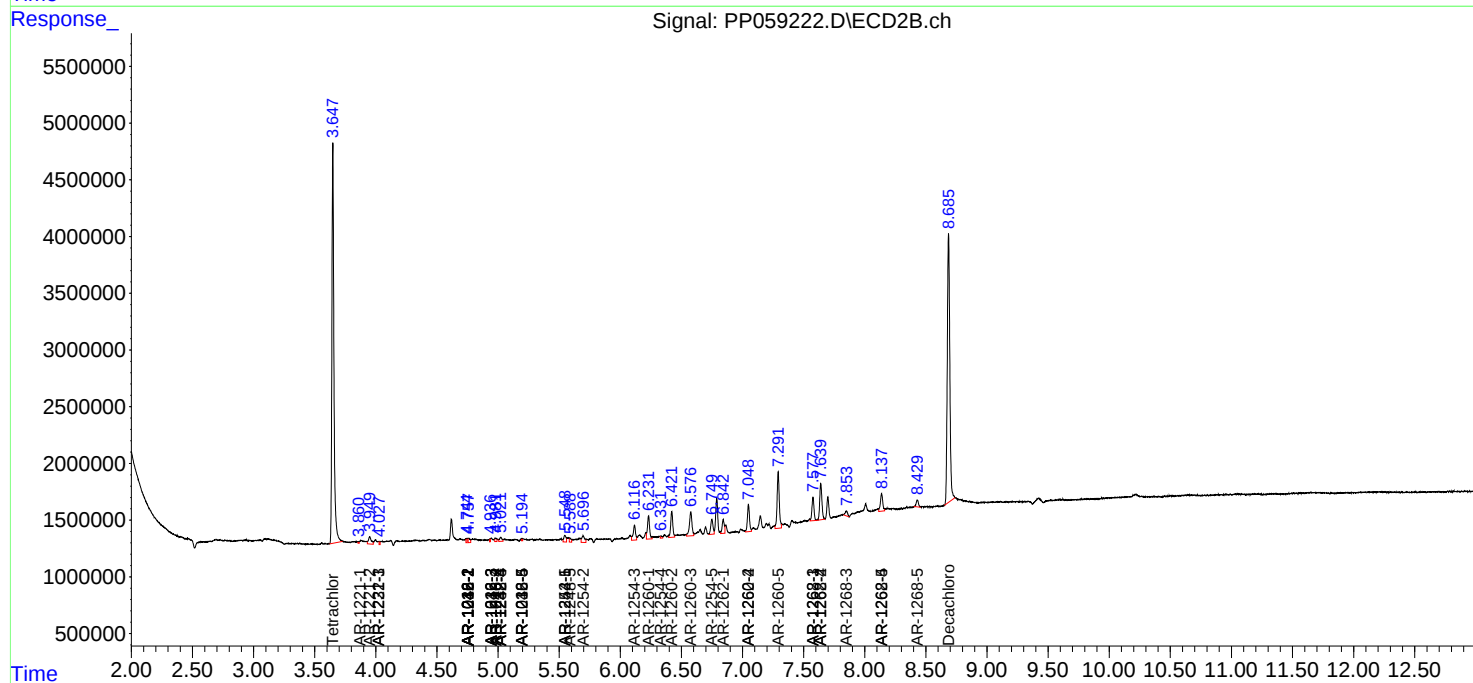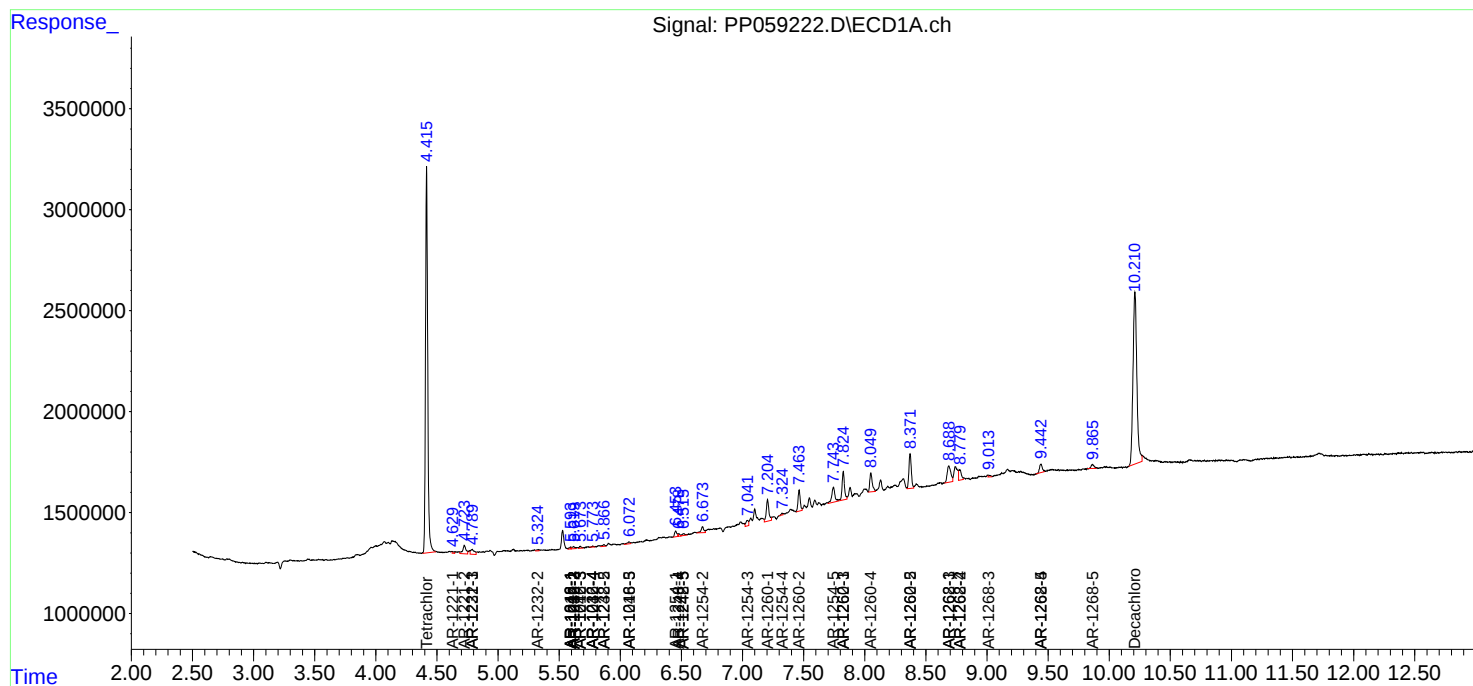


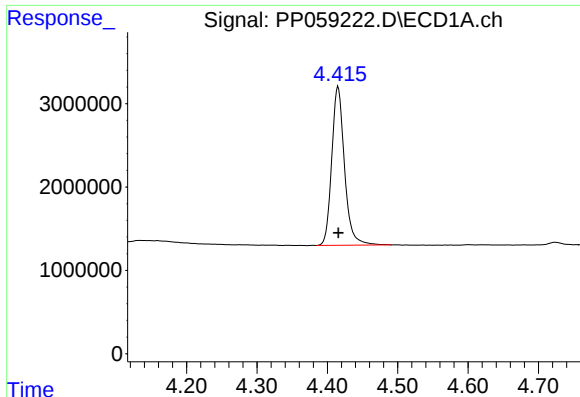

#1 Tetrachloro-m-xylene


R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 24019553
Conc: 19.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

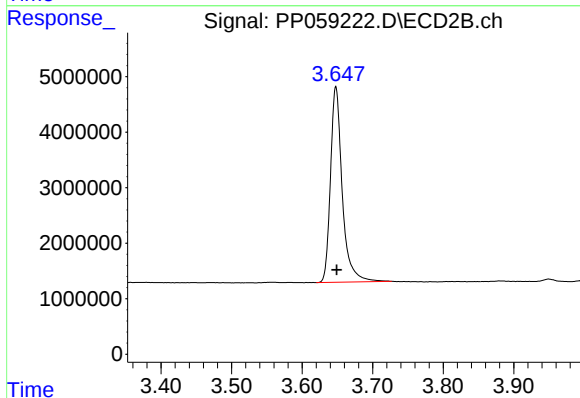


#1 Tetrachloro-m-xylene

R.T.: 3.648 min
Delta R.T.: 0.000 min
Response: 40897029
Conc: 20.18 ng/ml

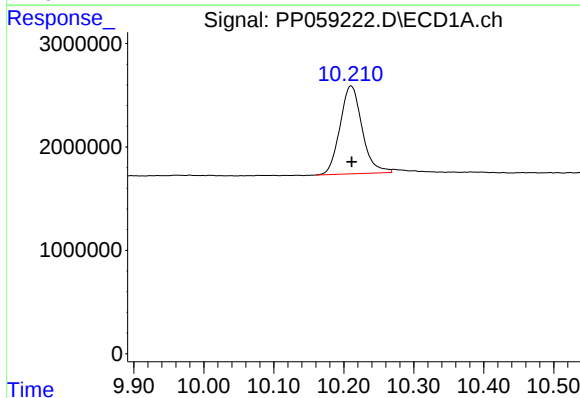


#2 Decachlorobiphenyl

R.T.: 10.210 min
Delta R.T.: 0.000 min
Response: 18624780
Conc: 24.40 ng/ml

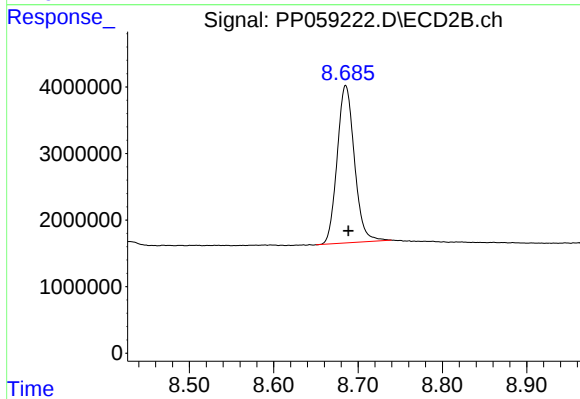

#2 Decachlorobiphenyl


R.T.: 8.685 min
Delta R.T.: -0.003 min
Response: 33596544
Conc: 23.88 ng/ml

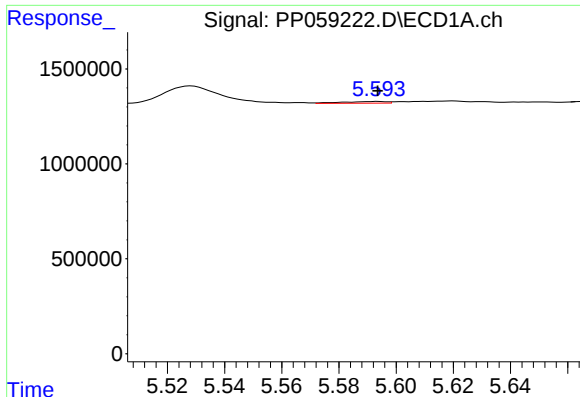

#3 AR-1016-1


R.T.: 5.594 min
Delta R.T.: 0.000 min
Response: 96102
Conc: 2.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

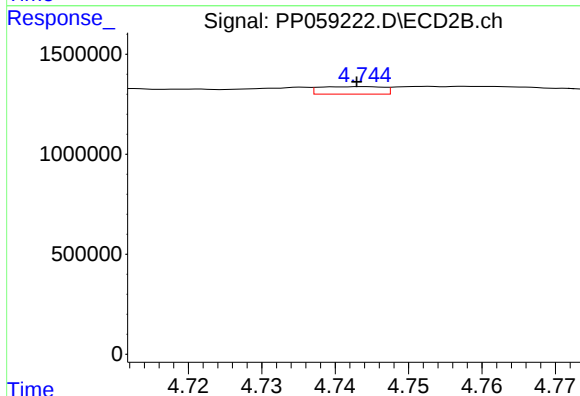


#3 AR-1016-1

R.T.: 4.744 min
Delta R.T.: 0.001 min
Response: 226316
Conc: 3.53 ng/ml

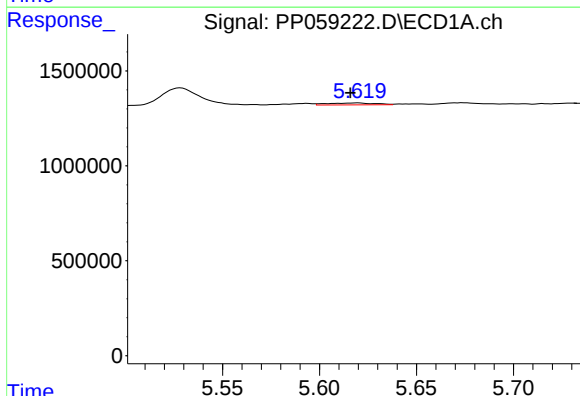


#4 AR-1016-2

R.T.: 5.620 min
Delta R.T.: 0.004 min
Response: 180322
Conc: 3.18 ng/ml

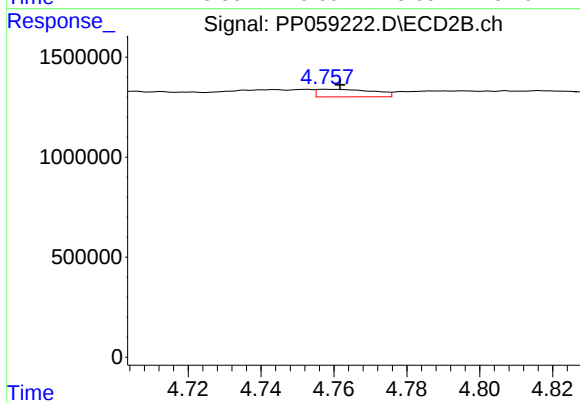

#4 AR-1016-2


R.T.: 4.758 min
Delta R.T.: -0.004 min
Response: 408320
Conc: 4.49 ng/ml

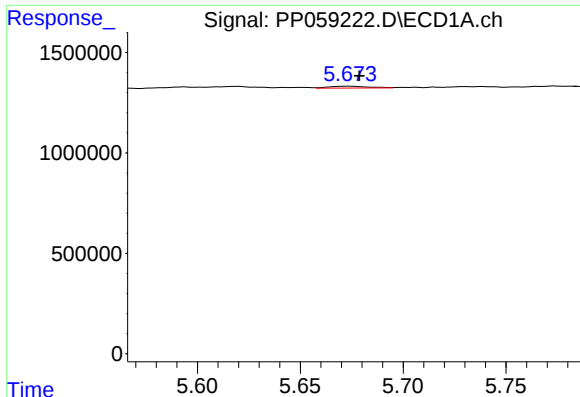

#5 AR-1016-3


R.T.: 5.674 min
Delta R.T.: -0.005 min
Response: 118423
Conc: 3.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

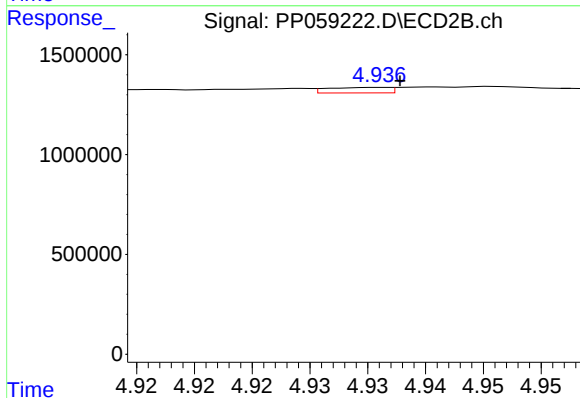


#5 AR-1016-3

R.T.: 4.936 min
Delta R.T.: -0.002 min
Response: 100974
Conc: 2.10 ng/ml

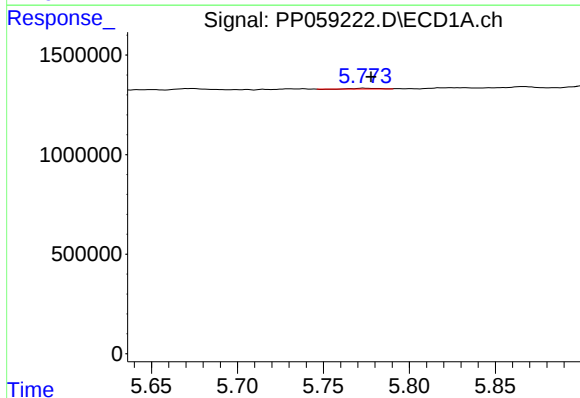


#6 AR-1016-4

R.T.: 5.774 min
Delta R.T.: -0.004 min
Response: 30611
Conc: 1.06 ng/ml

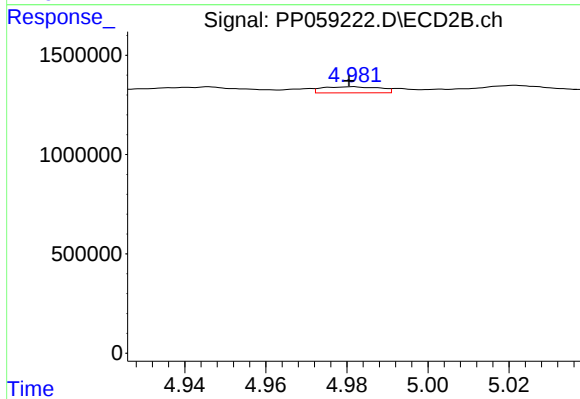

#6 AR-1016-4


R.T.: 4.982 min
Delta R.T.: 0.001 min
Response: 299166
Conc: 7.25 ng/ml

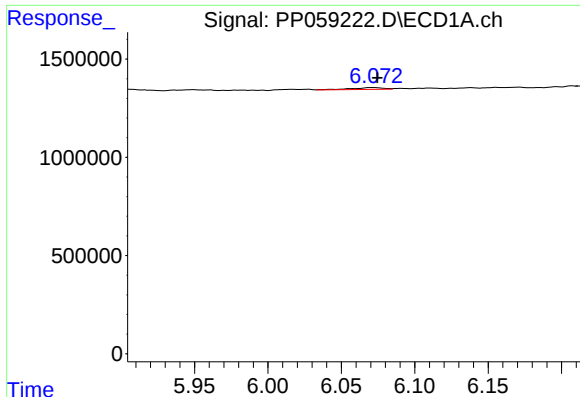

#7 AR-1016-5


R.T.: 6.071 min
Delta R.T.: -0.003 min
Response: 147955
Conc: 4.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

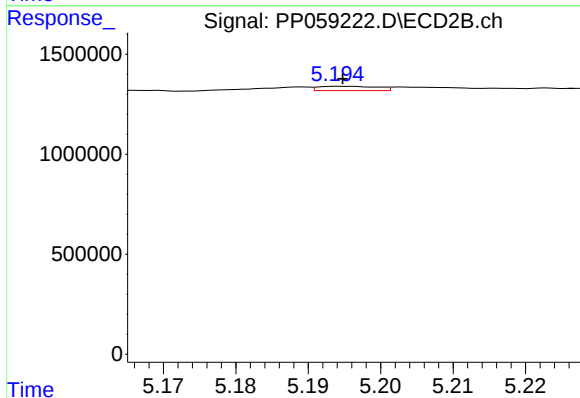


#7 AR-1016-5

R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 123240
Conc: 2.37 ng/ml

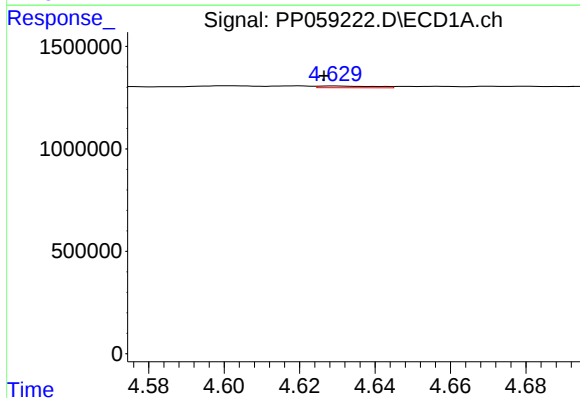


#8 AR-1221-1

R.T.: 4.629 min
Delta R.T.: 0.003 min
Response: 83409
Conc: 5.29 ng/ml

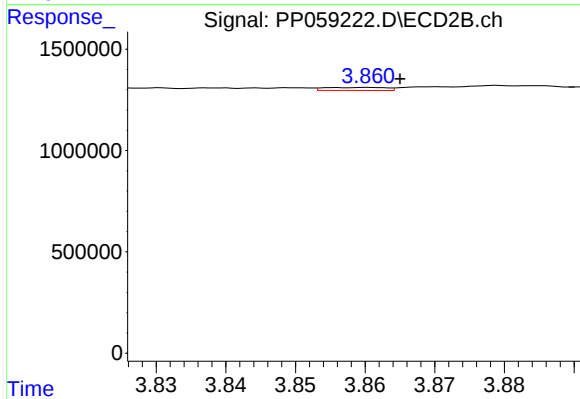

#8 AR-1221-1


R.T.: 3.860 min
Delta R.T.: -0.005 min
Response: 90079
Conc: 3.32 ng/ml

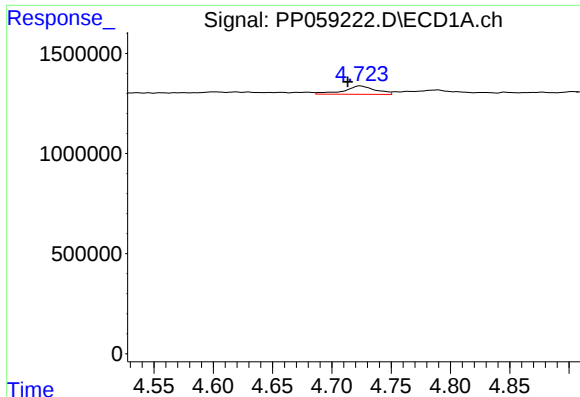

#9 AR-1221-2


R.T.: 4.724 min
Delta R.T.: 0.010 min
Response: 771336
Conc: 65.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

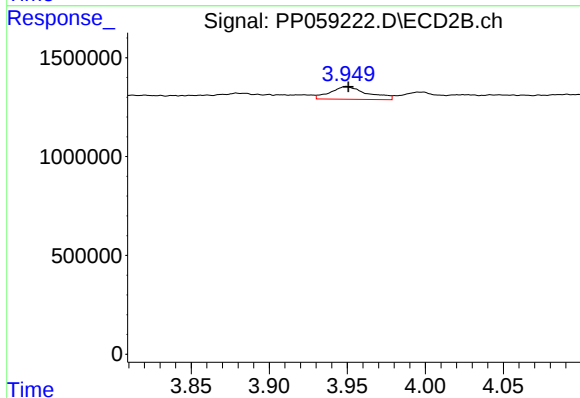


#9 AR-1221-2

R.T.: 3.949 min
Delta R.T.: -0.001 min
Response: 1067103
Conc: 53.60 ng/ml

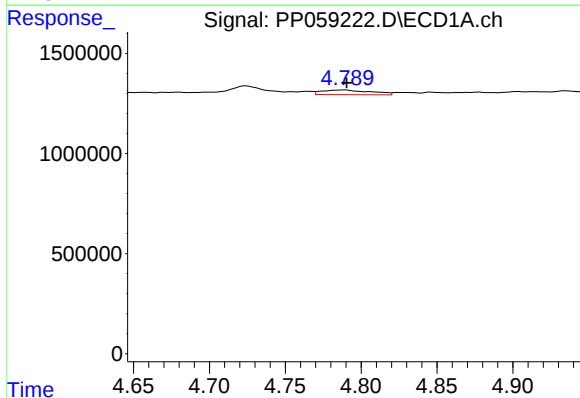


#10 AR-1221-3

R.T.: 4.790 min
Delta R.T.: 0.000 min
Response: 525718
Conc: 14.93 ng/ml

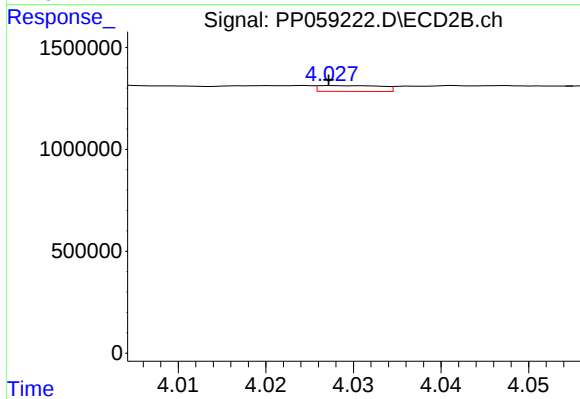

#10 AR-1221-3


R.T.: 4.028 min
Delta R.T.: 0.000 min
Response: 143787
Conc: 2.42 ng/ml

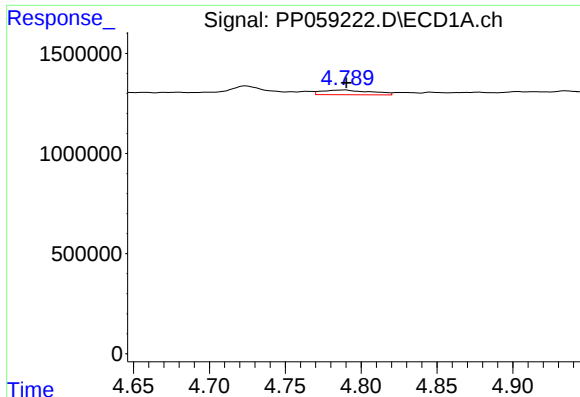

#11 AR-1232-1


R.T.: 4.790 min
Delta R.T.: 0.000 min
Response: 525718
Conc: 17.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

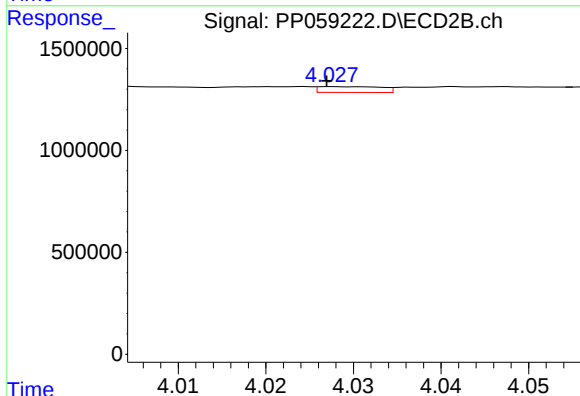


#11 AR-1232-1

R.T.: 4.028 min
Delta R.T.: 0.000 min
Response: 143787
Conc: 3.03 ng/ml

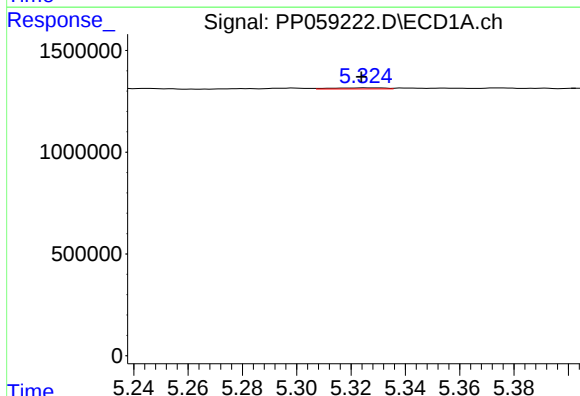


#12 AR-1232-2

R.T.: 5.325 min
Delta R.T.: 0.002 min
Response: 72647
Conc: 4.66 ng/ml

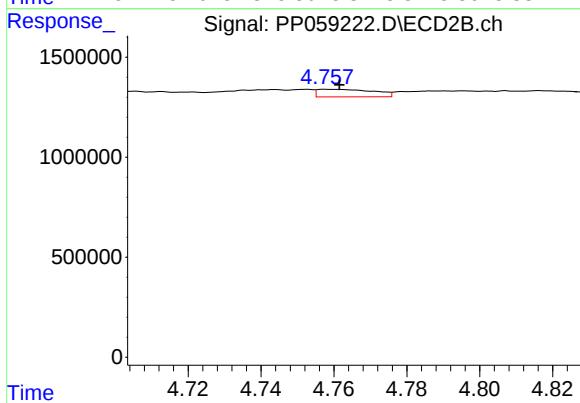

#12 AR-1232-2


R.T.: 4.758 min
Delta R.T.: -0.004 min
Response: 408320
Conc: 9.63 ng/ml

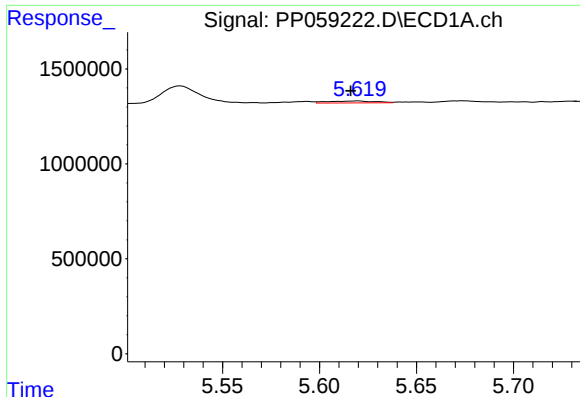

#13 AR-1232-3


R.T.: 5.620 min
Delta R.T.: 0.004 min
Response: 180322
Conc: 6.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

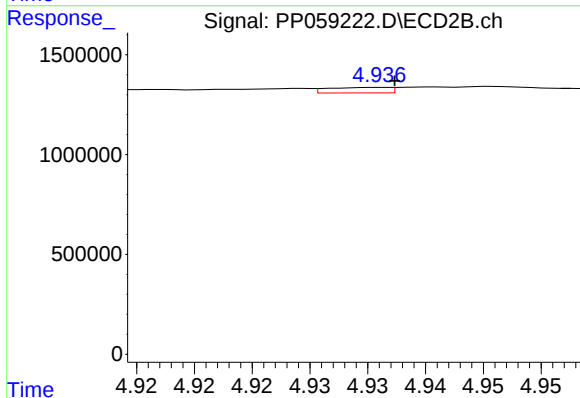


#13 AR-1232-3

R.T.: 4.936 min
Delta R.T.: -0.001 min
Response: 100974
Conc: 4.55 ng/ml

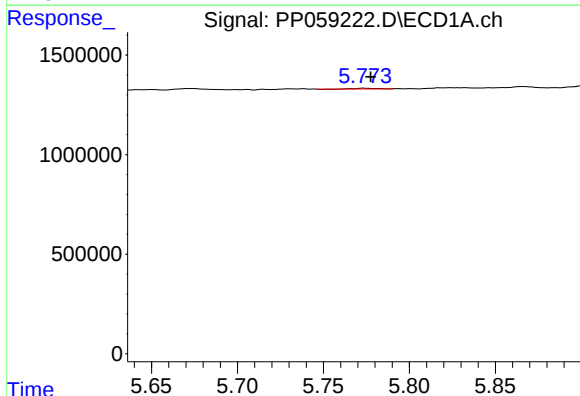


#14 AR-1232-4

R.T.: 5.774 min
Delta R.T.: -0.004 min
Response: 30611
Conc: 2.31 ng/ml

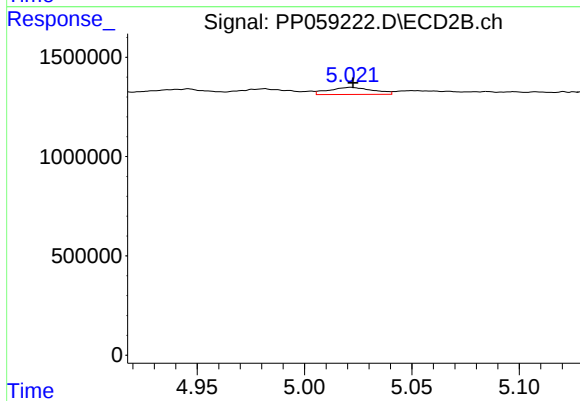

#14 AR-1232-4


R.T.: 5.022 min
Delta R.T.: 0.000 min
Response: 514187
Conc: 24.35 ng/ml

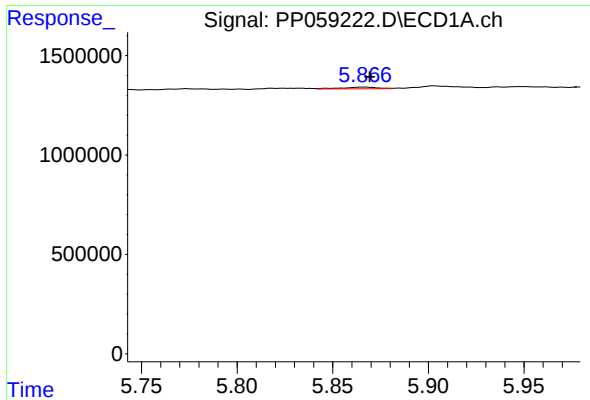

#15 AR-1232-5


R.T.: 5.867 min
Delta R.T.: -0.003 min
Response: 116519
Conc: 10.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

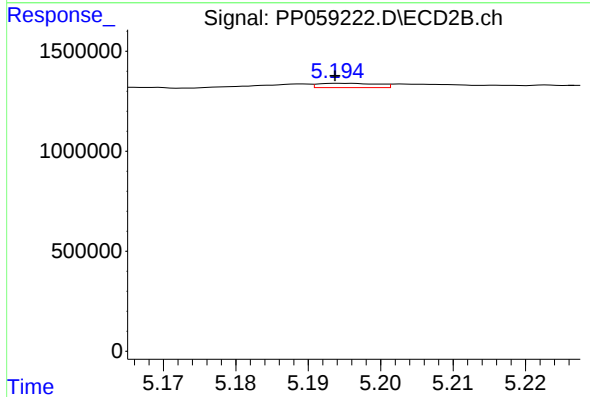


#15 AR-1232-5

R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 123240
Conc: 5.38 ng/ml

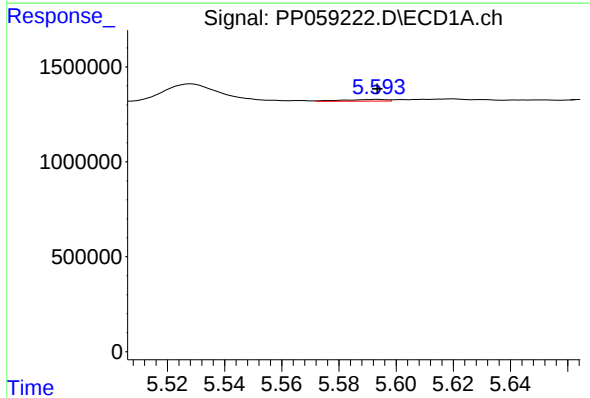


#16 AR-1242-1

R.T.: 5.594 min
Delta R.T.: 0.000 min
Response: 96102
Conc: 2.81 ng/ml

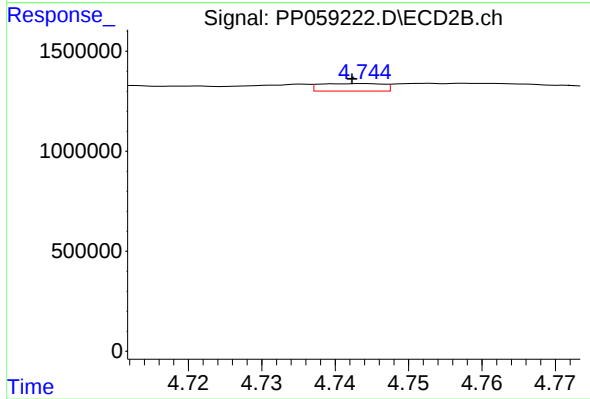

#16 AR-1242-1


R.T.: 4.744 min
Delta R.T.: 0.002 min
Response: 226316
Conc: 4.04 ng/ml

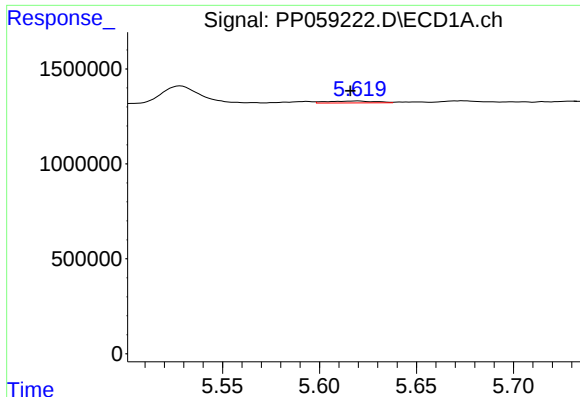

#17 AR-1242-2


R.T.: 5.620 min
Delta R.T.: 0.004 min
Response: 180322
Conc: 3.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

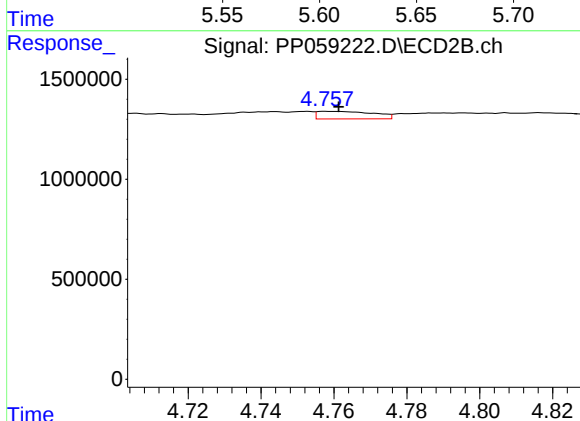


#17 AR-1242-2

R.T.: 4.758 min
Delta R.T.: -0.004 min
Response: 408320
Conc: 5.12 ng/ml

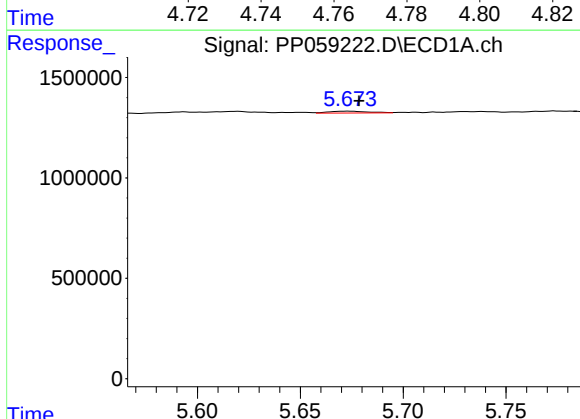


#18 AR-1242-3

R.T.: 5.674 min
Delta R.T.: -0.005 min
Response: 118423
Conc: 3.77 ng/ml

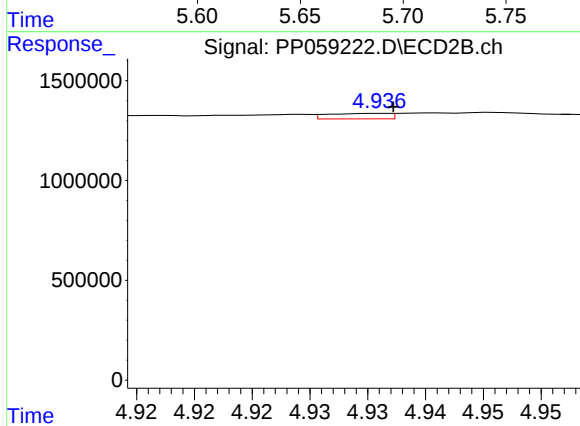

#18 AR-1242-3


R.T.: 4.936 min
Delta R.T.: -0.001 min
Response: 100974
Conc: 2.37 ng/ml

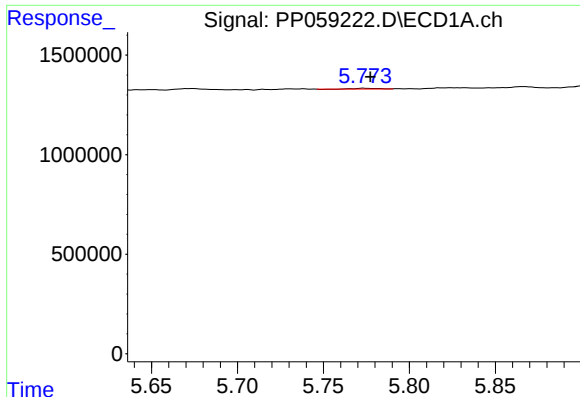

#19 AR-1242-4


R.T.: 5.774 min
Delta R.T.: -0.004 min
Response: 30611
Conc: 1.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

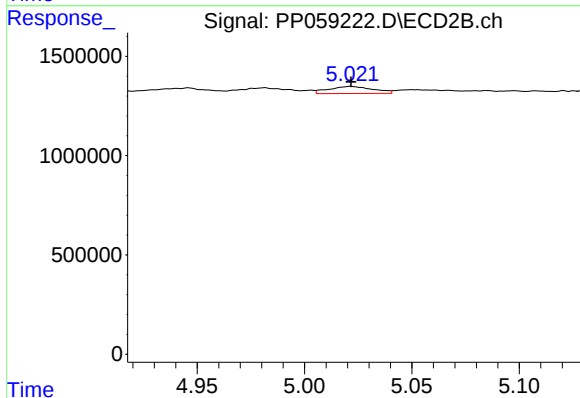


#19 AR-1242-4

R.T.: 5.022 min
Delta R.T.: 0.000 min
Response: 514187
Conc: 11.78 ng/ml

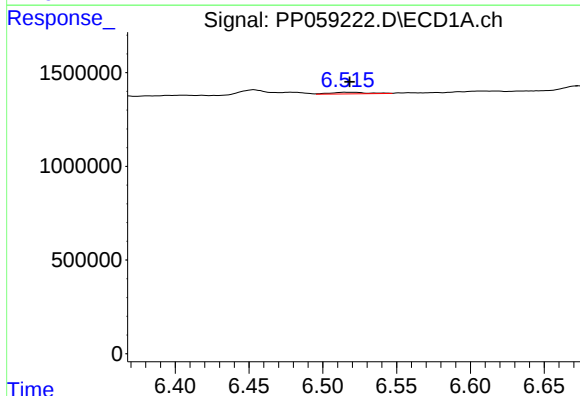


#20 AR-1242-5

R.T.: 6.516 min
Delta R.T.: -0.002 min
Response: 147605
Conc: 5.71 ng/ml

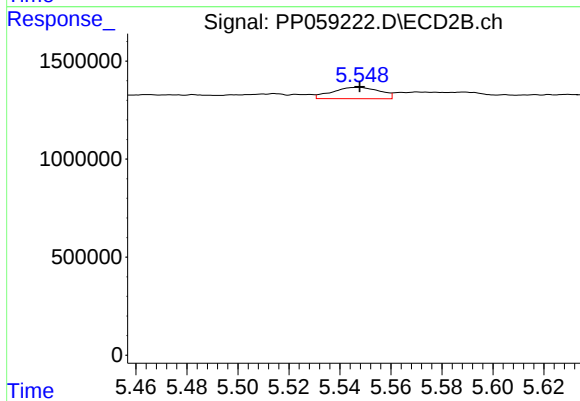

#20 AR-1242-5


R.T.: 5.548 min
Delta R.T.: 0.000 min
Response: 756824
Conc: 15.24 ng/ml

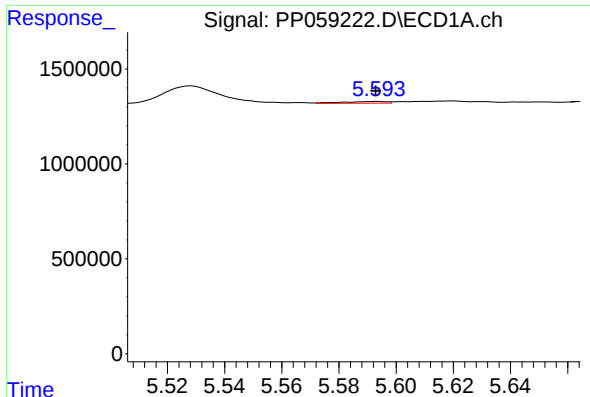

#21 AR-1248-1


R.T.: 5.594 min
Delta R.T.: 0.000 min
Response: 96102
Conc: 3.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

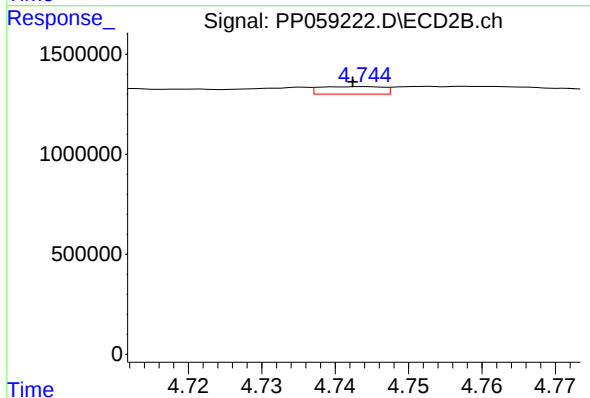


#21 AR-1248-1

R.T.: 4.744 min
Delta R.T.: 0.002 min
Response: 226316
Conc: 5.50 ng/ml

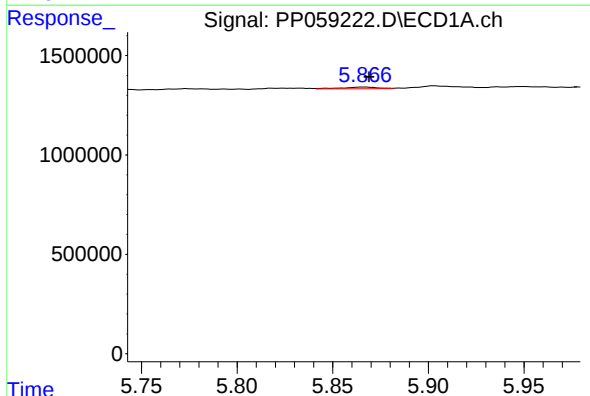


#22 AR-1248-2

R.T.: 5.867 min
Delta R.T.: -0.002 min
Response: 116519
Conc: 3.01 ng/ml

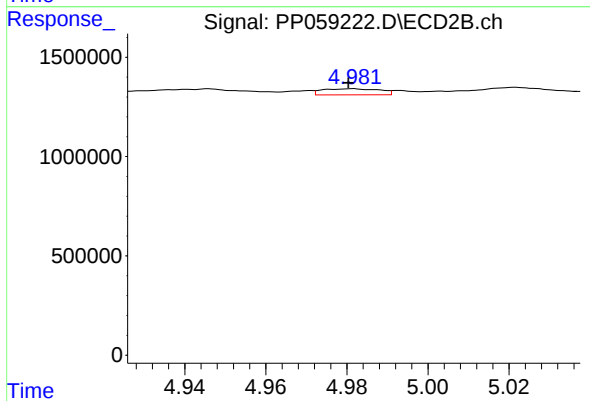

#22 AR-1248-2


R.T.: 4.982 min
Delta R.T.: 0.001 min
Response: 299166
Conc: 4.97 ng/ml

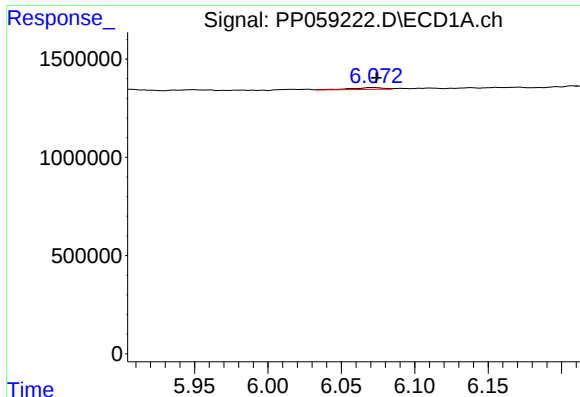

#23 AR-1248-3


R.T.: 6.071 min
Delta R.T.: -0.003 min
Response: 147955
Conc: 3.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

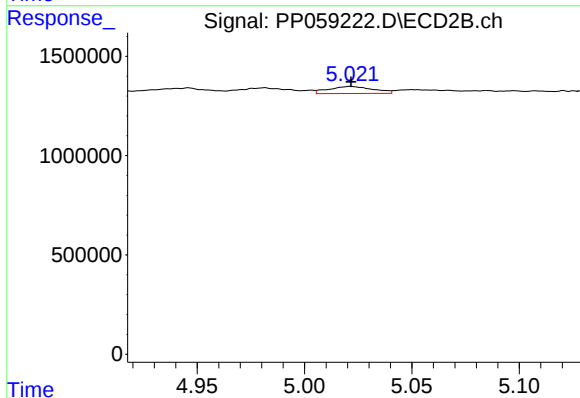


#23 AR-1248-3

R.T.: 5.022 min
Delta R.T.: 0.000 min
Response: 514187
Conc: 8.35 ng/ml

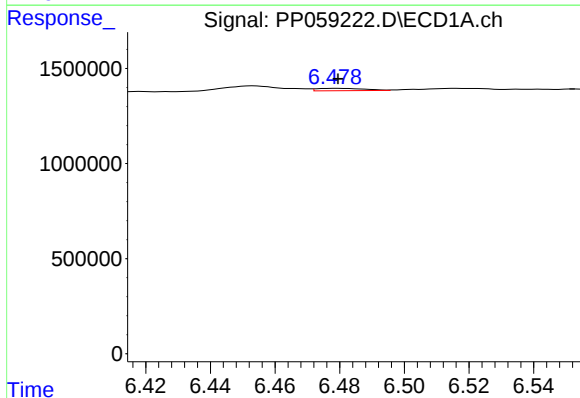


#24 AR-1248-4

R.T.: 6.479 min
Delta R.T.: 0.000 min
Response: 130840
Conc: 3.14 ng/ml

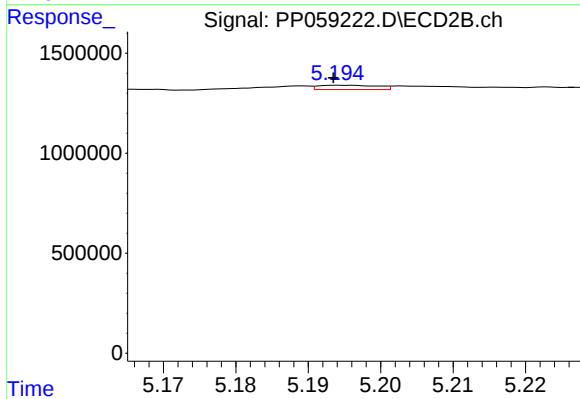

#24 AR-1248-4


R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 123240
Conc: 1.71 ng/ml

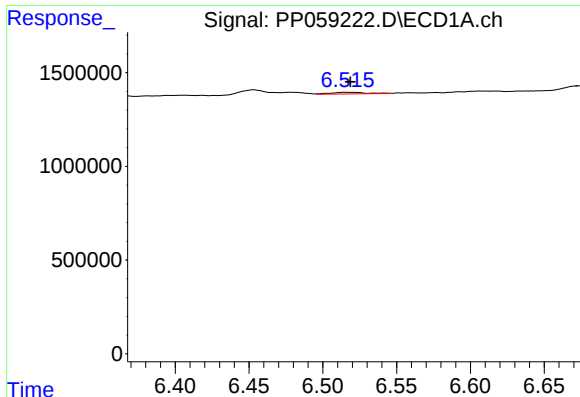

#25 AR-1248-5


R.T.: 6.516 min
Delta R.T.: -0.003 min
Response: 147605
Conc: 3.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

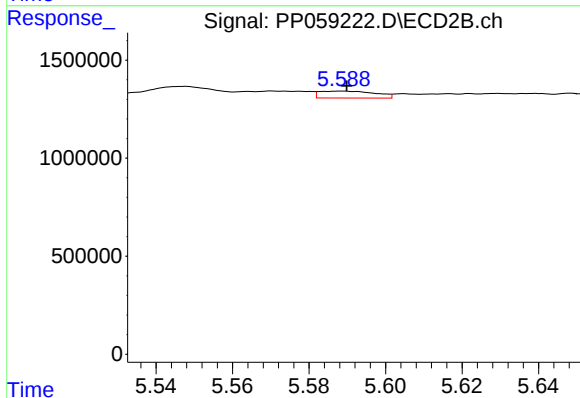


#25 AR-1248-5

R.T.: 5.589 min
Delta R.T.: -0.001 min
Response: 359355
Conc: 5.45 ng/ml

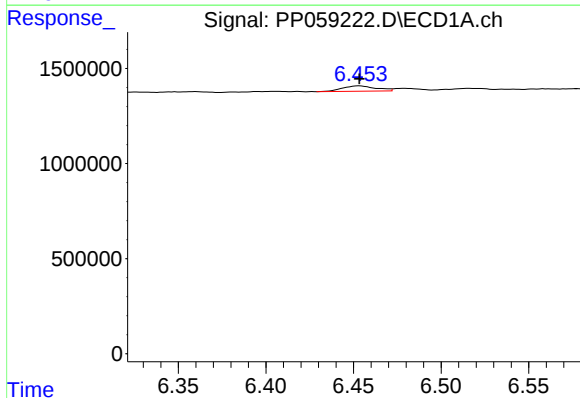


#26 AR-1254-1

R.T.: 6.453 min
Delta R.T.: 0.000 min
Response: 380978
Conc: 8.16 ng/ml

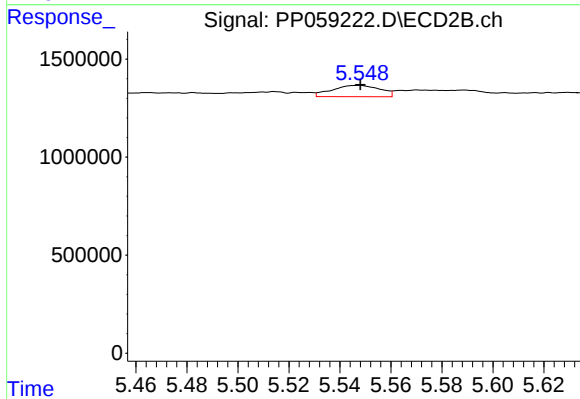

#26 AR-1254-1


R.T.: 5.548 min
Delta R.T.: 0.000 min
Response: 756824
Conc: 7.47 ng/ml

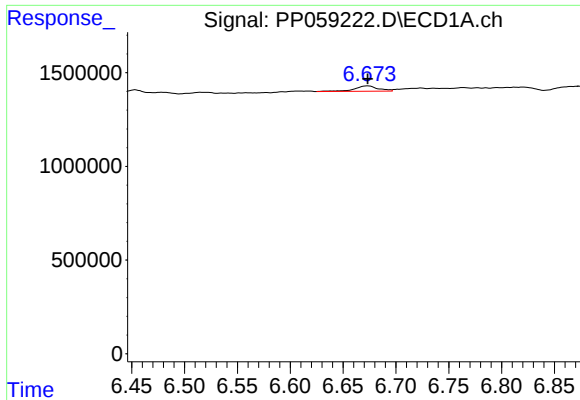

#27 AR-1254-2


R.T.: 6.673 min
Delta R.T.: 0.000 min
Response: 453757
Conc: 6.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

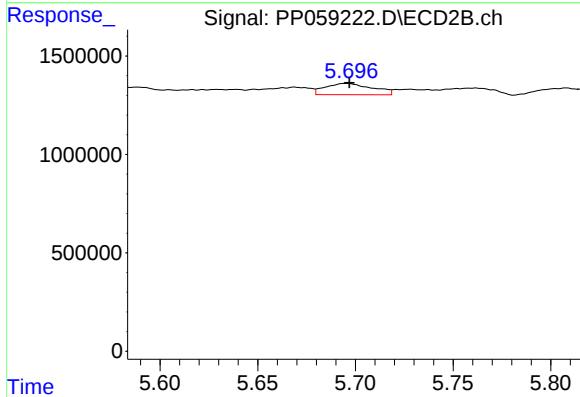


#27 AR-1254-2

R.T.: 5.697 min
Delta R.T.: 0.000 min
Response: 962213
Conc: 10.90 ng/ml

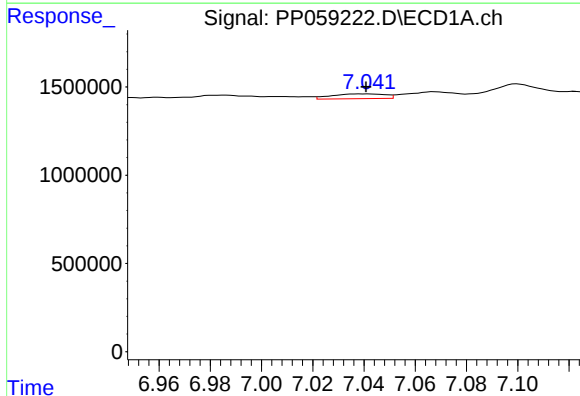


#28 AR-1254-3

R.T.: 7.041 min
Delta R.T.: 0.000 min
Response: 392236
Conc: 5.68 ng/ml

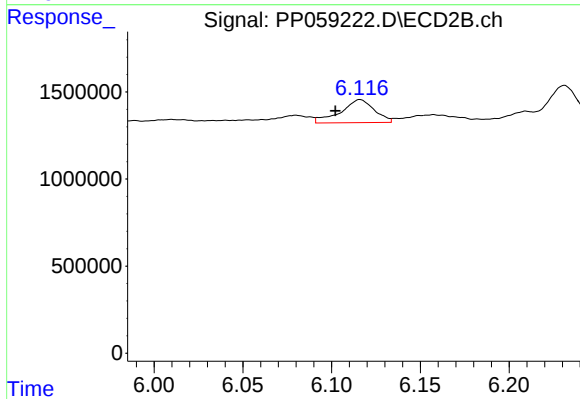

#28 AR-1254-3


R.T.: 6.116 min
Delta R.T.: 0.014 min
Response: 1748355
Conc: 12.65 ng/ml

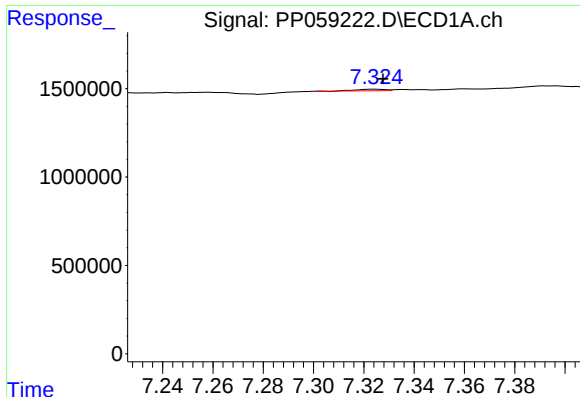

#29 AR-1254-4


R.T.: 7.324 min
Delta R.T.: -0.003 min
Response: 69915
Conc: 1.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

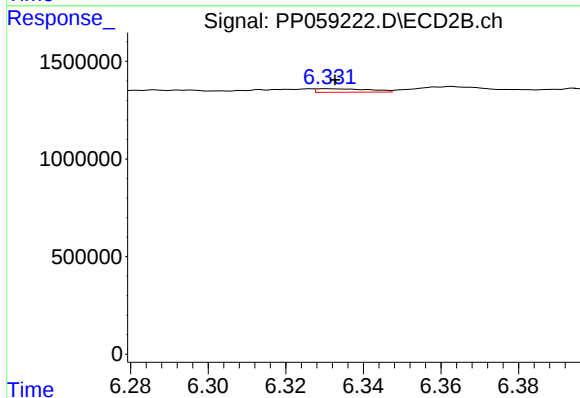


#29 AR-1254-4

R.T.: 6.331 min
Delta R.T.: -0.002 min
Response: 170509
Conc: 2.12 ng/ml

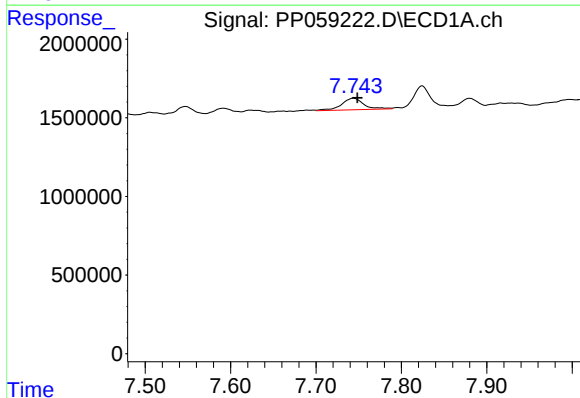


#30 AR-1254-5

R.T.: 7.744 min
Delta R.T.: -0.005 min
Response: 1319954
Conc: 28.09 ng/ml

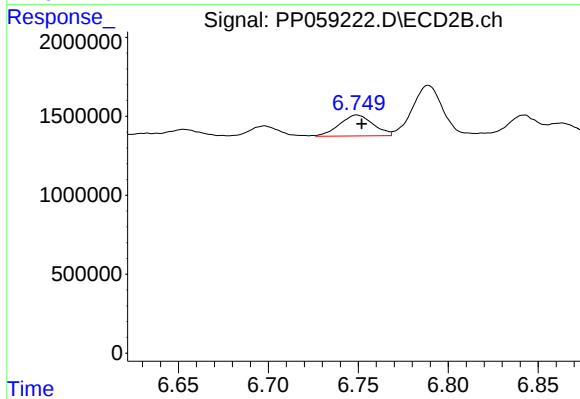

#30 AR-1254-5


R.T.: 6.749 min
Delta R.T.: -0.003 min
Response: 1729115
Conc: 14.46 ng/ml

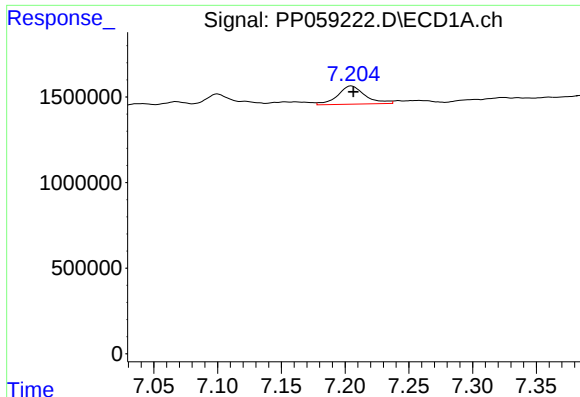

#31 AR-1260-1


R.T.: 7.205 min
Delta R.T.: -0.001 min
Response: 1597913
Conc: 29.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

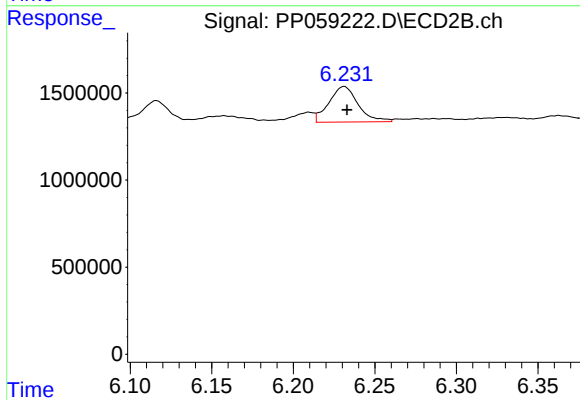


#31 AR-1260-1

R.T.: 6.231 min
Delta R.T.: -0.002 min
Response: 2540297
Conc: 25.65 ng/ml

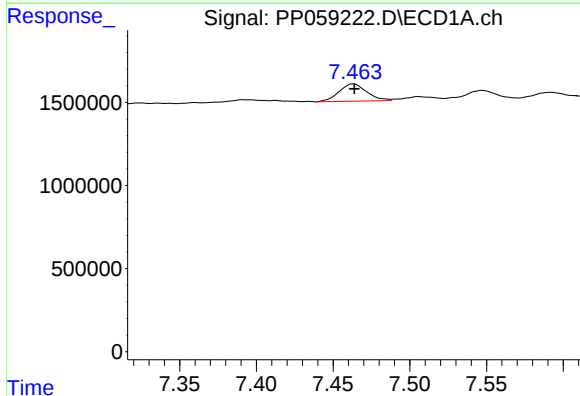


#32 AR-1260-2

R.T.: 7.463 min
Delta R.T.: 0.000 min
Response: 1319186
Conc: 22.16 ng/ml

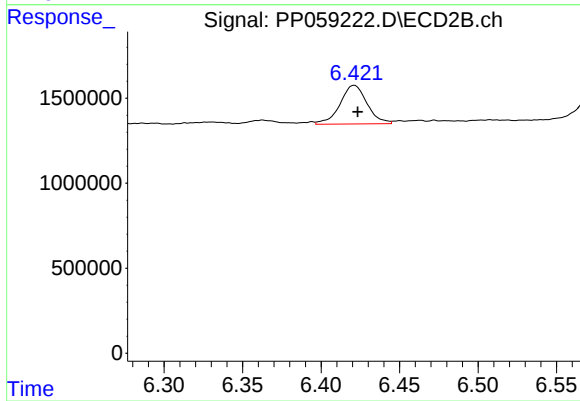

#32 AR-1260-2


R.T.: 6.421 min
Delta R.T.: -0.002 min
Response: 2721010
Conc: 23.52 ng/ml

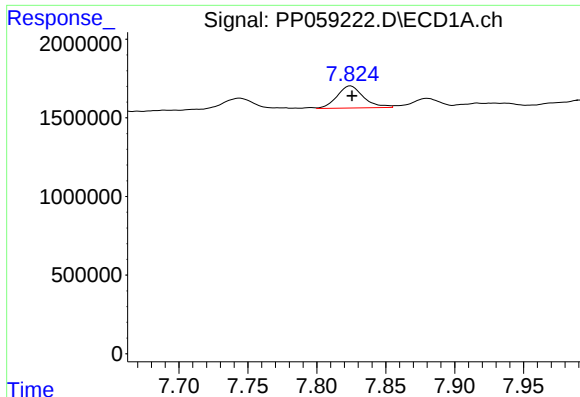

#33 AR-1260-3


R.T.: 7.825 min
Delta R.T.: 0.000 min
Response: 1872951
Conc: 47.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

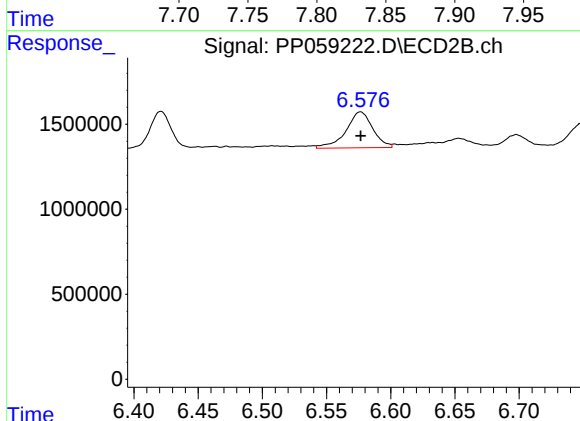


#33 AR-1260-3

R.T.: 6.577 min
Delta R.T.: 0.000 min
Response: 3084809
Conc: 27.73 ng/ml

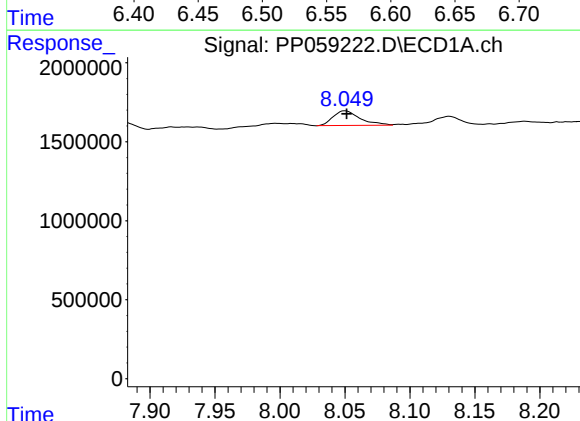


#34 AR-1260-4

R.T.: 8.050 min
Delta R.T.: -0.001 min
Response: 1357813
Conc: 30.57 ng/ml

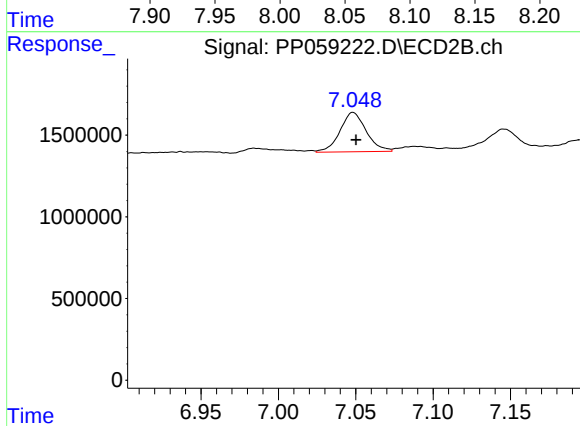

#34 AR-1260-4


R.T.: 7.048 min
Delta R.T.: -0.002 min
Response: 2834498
Conc: 32.70 ng/ml

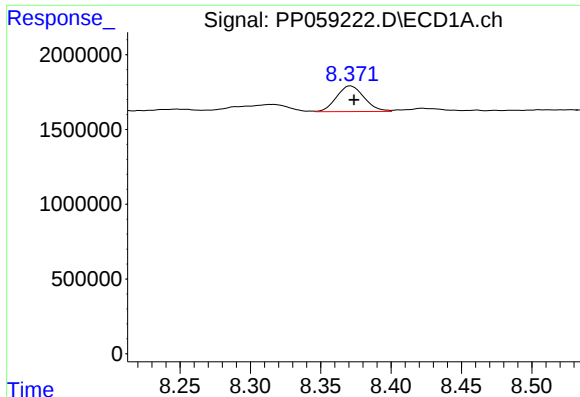

#35 AR-1260-5


R.T.: 8.371 min
Delta R.T.: -0.003 min
Response: 2347780
Conc: 29.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

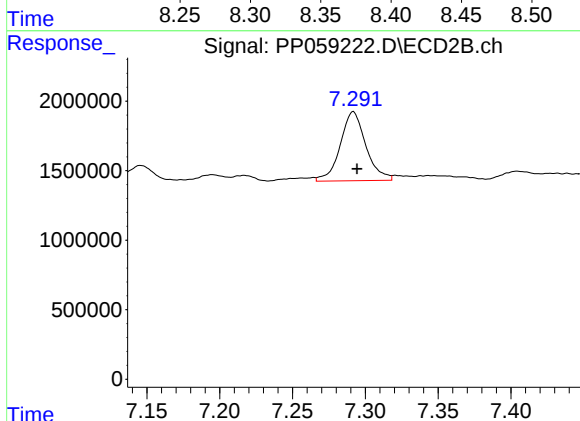


#35 AR-1260-5

R.T.: 7.292 min
Delta R.T.: -0.002 min
Response: 6096818
Conc: 33.08 ng/ml

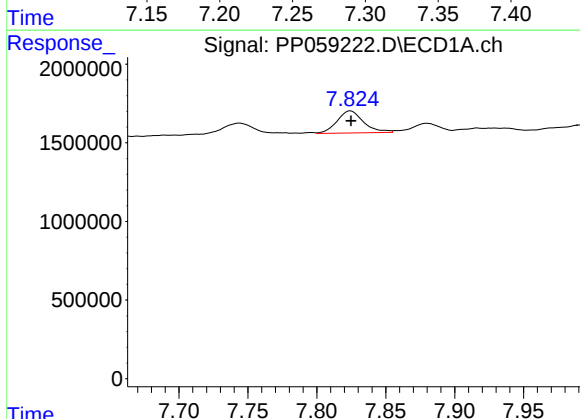


#36 AR-1262-1

R.T.: 7.825 min
Delta R.T.: 0.000 min
Response: 1872951
Conc: 29.41 ng/ml

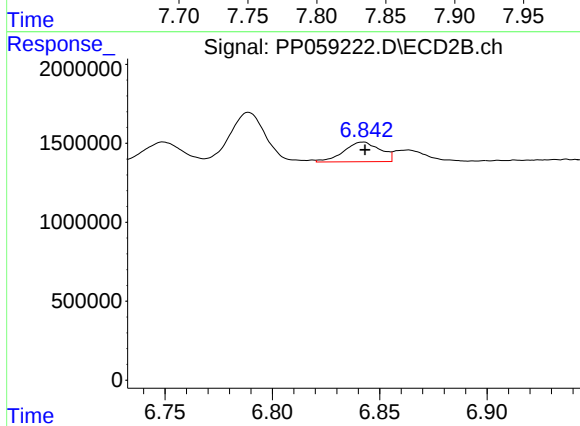

#36 AR-1262-1


R.T.: 6.843 min
Delta R.T.: 0.000 min
Response: 1474799
Conc: 25.63 ng/ml

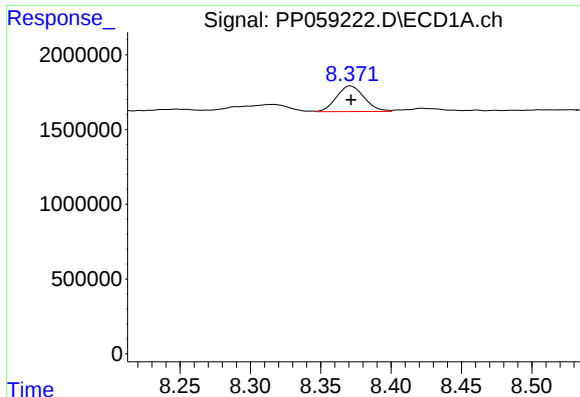

#37 AR-1262-2


R.T.: 8.371 min
Delta R.T.: 0.000 min
Response: 2347780
Conc: 25.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

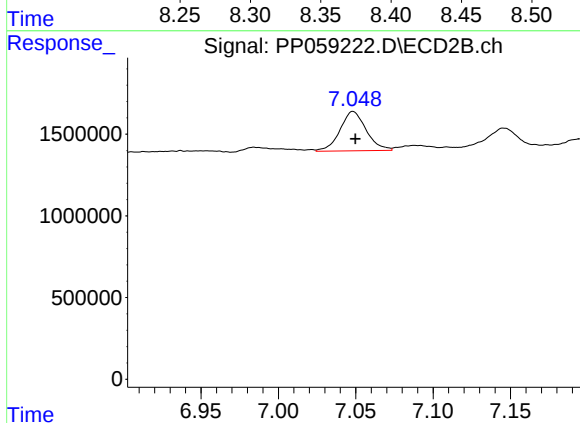


#37 AR-1262-2

R.T.: 7.048 min
Delta R.T.: -0.002 min
Response: 2834498
Conc: 24.02 ng/ml

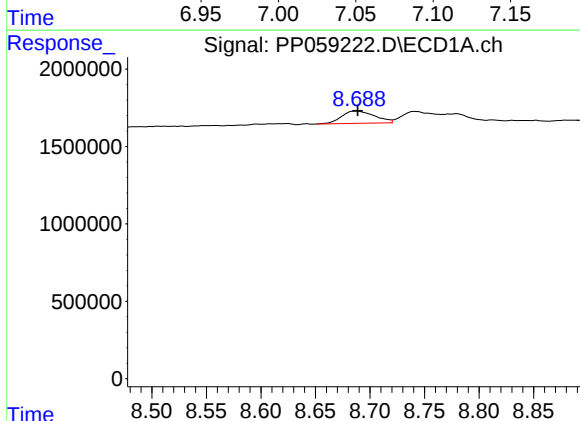


#38 AR-1262-3

R.T.: 8.688 min
Delta R.T.: 0.000 min
Response: 1680863
Conc: 26.12 ng/ml

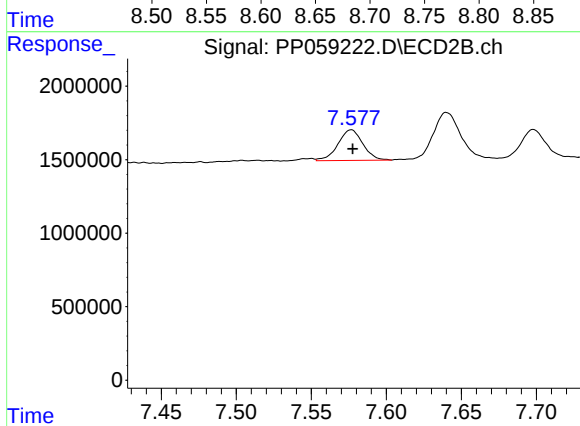

#38 AR-1262-3


R.T.: 7.577 min
Delta R.T.: 0.000 min
Response: 2412627
Conc: 28.35 ng/ml

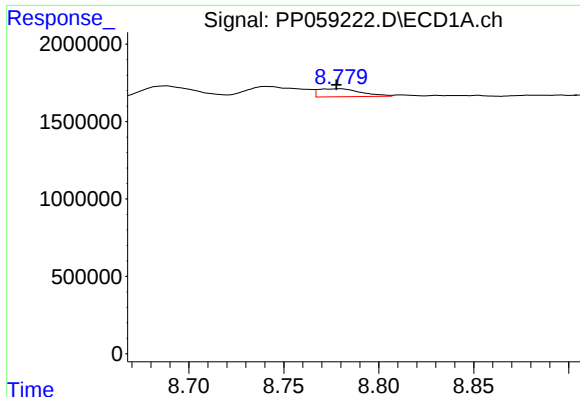

#39 AR-1262-4


R.T.: 8.779 min
Delta R.T.: 0.002 min
Response: 803487
Conc: 24.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

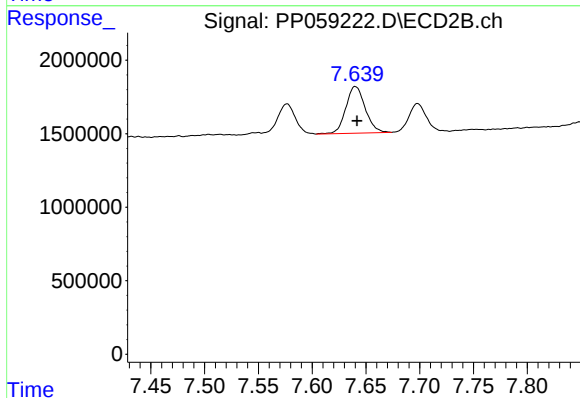


#39 AR-1262-4

R.T.: 7.640 min
Delta R.T.: -0.002 min
Response: 3985299
Conc: 26.38 ng/ml

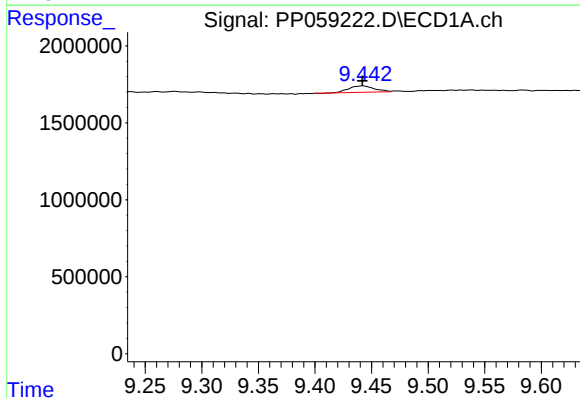


#40 AR-1262-5

R.T.: 9.443 min
Delta R.T.: 0.000 min
Response: 652150
Conc: 21.85 ng/ml

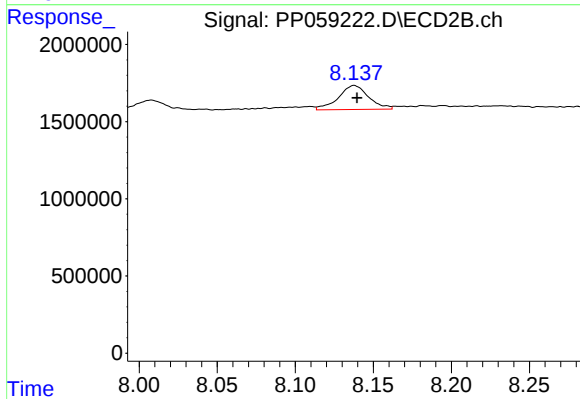

#40 AR-1262-5


R.T.: 8.138 min
Delta R.T.: -0.002 min
Response: 2100326
Conc: 32.93 ng/ml

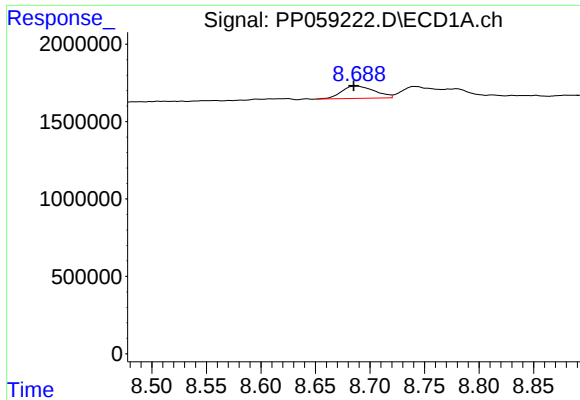

#41 AR-1268-1


R.T.: 8.688 min
Delta R.T.: 0.003 min
Response: 1680863
Conc: 14.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

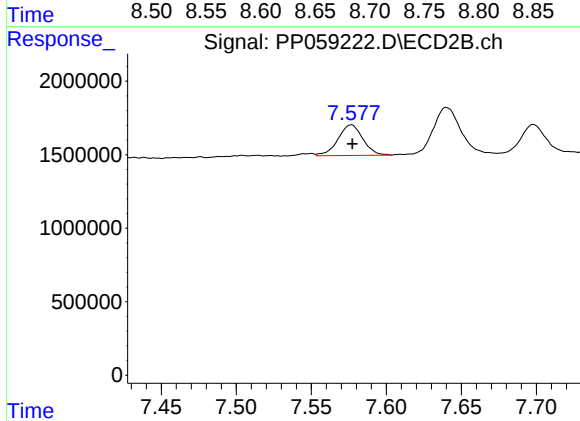


#41 AR-1268-1

R.T.: 7.577 min
Delta R.T.: 0.000 min
Response: 2412627
Conc: 9.89 ng/ml

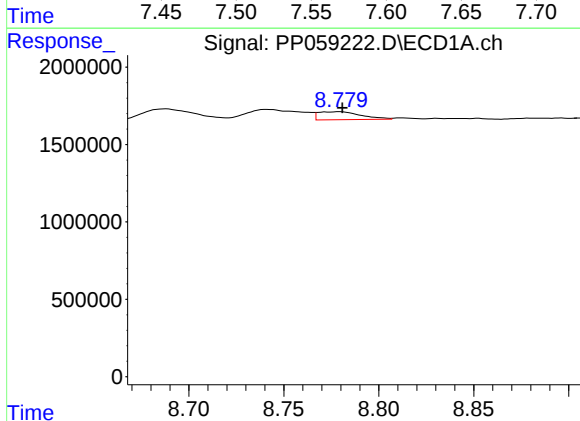


#42 AR-1268-2

R.T.: 8.779 min
Delta R.T.: -0.001 min
Response: 803487
Conc: 8.16 ng/ml

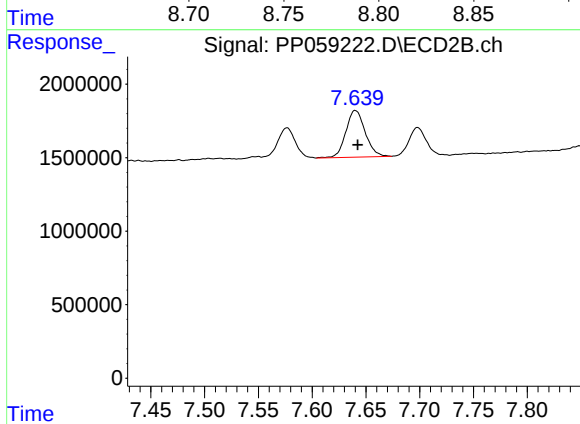

#42 AR-1268-2


R.T.: 7.640 min
Delta R.T.: -0.002 min
Response: 3985299
Conc: 18.20 ng/ml

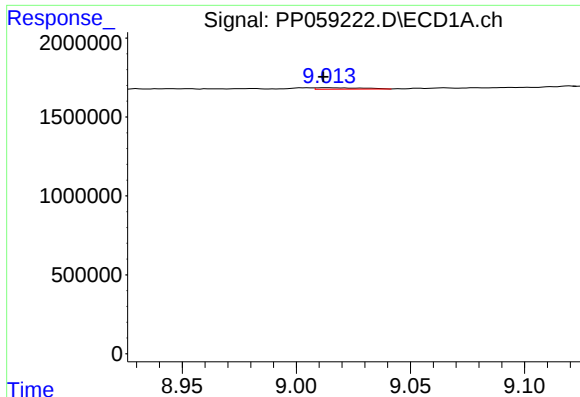

#43 AR-1268-3


R.T.: 9.014 min
Delta R.T.: 0.002 min
Response: 121291
Conc: 1.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

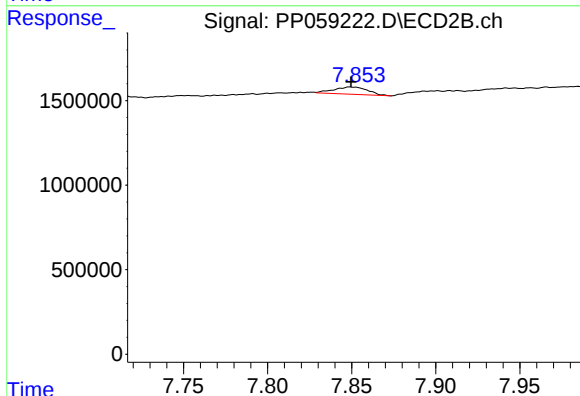


#43 AR-1268-3

R.T.: 7.849 min
Delta R.T.: 0.000 min
Response: 596235
Conc: 3.05 ng/ml

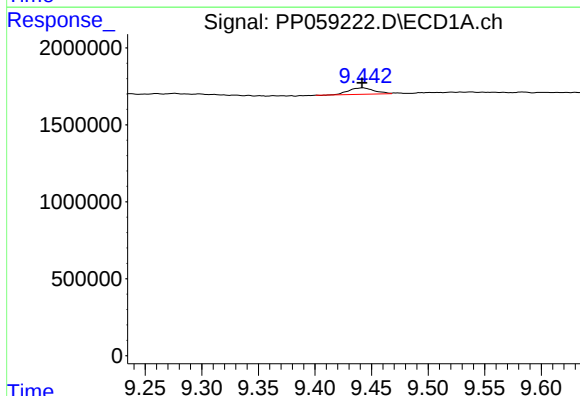


#44 AR-1268-4

R.T.: 9.443 min
Delta R.T.: 0.000 min
Response: 652150
Conc: 20.44 ng/ml

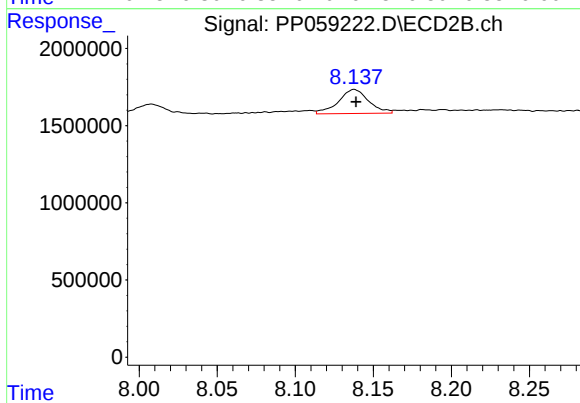

#44 AR-1268-4


R.T.: 8.138 min
Delta R.T.: -0.001 min
Response: 2100326
Conc: 30.18 ng/ml

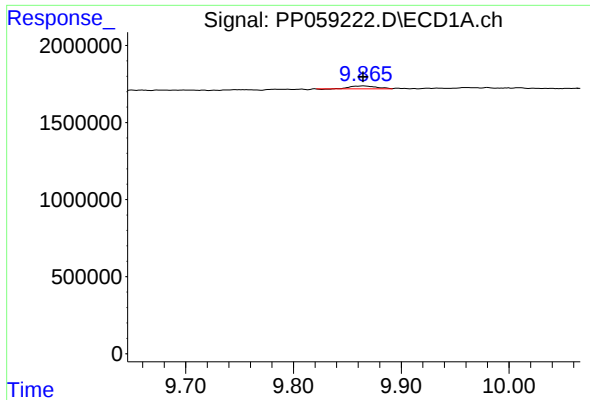

#45 AR-1268-5

R.T.: 9.865 min
Delta R.T.: 0.000 min
Response: 311792
Conc: 1.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

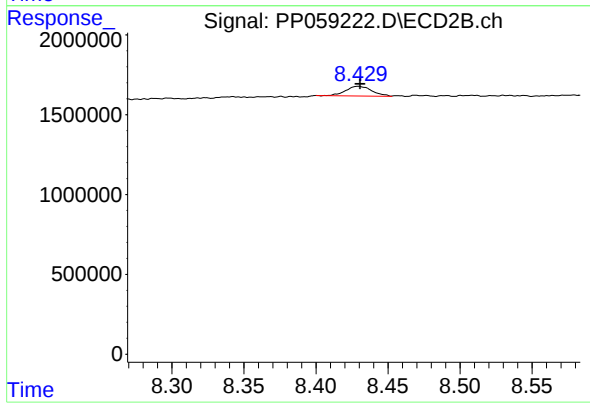

#45 AR-1268-5

R.T.: 8.430 min
Delta R.T.: 0.000 min
Response: 768459
Conc: 1.48 ng/ml