

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
 Data File : PP059247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2023 07:51
 Operator : YP\AJ
 Sample : 03572-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 08:21:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.414	3.647	23769116	40960231	19.371	20.216
2)	SA Decachlor...	10.206	8.683	19040569	33076508	24.947	23.512
Target Compounds							
3)	L1 AR-1016-1	5.592	4.740	1646441	2909582	41.907	45.365
4)	L1 AR-1016-2	5.614	4.759	2327964	4113629	41.067	45.285
5)	L1 AR-1016-3	5.676	4.935	1575247	2143267	43.910	44.607
6)	L1 AR-1016-4	5.775	4.978	1171547	1977068	40.444	47.881
7)	L1 AR-1016-5	6.072	5.191	1310256	2356763	43.295	45.294
8)	L2 AR-1221-1	4.623	3.862	289962	291208	18.405	10.727 #
9)	L2 AR-1221-2	4.723	3.947	738465	818542	62.534	41.113 #
10)	L2 AR-1221-3	4.788	4.025	1162335	1563542	33.009	26.263
11)	L3 AR-1232-1	4.788	4.025	1162335	1563542	39.540	32.952
12)	L3 AR-1232-2	5.321	4.759	1287169	4113629	82.579	96.977
13)	L3 AR-1232-3	5.614	4.935	2327964	2143267	88.162	96.597
14)	L3 AR-1232-4	5.775	5.020	1171547	2229165	88.522	105.576
15)	L3 AR-1232-5	5.867	5.191	1134629	2356763	99.402	102.813
16)	L4 AR-1242-1	5.592	4.740	1646441	2909582	48.098	51.990
17)	L4 AR-1242-2	5.614	4.759	2327964	4113629	47.442	51.590
18)	L4 AR-1242-3	5.676	4.935	1575247	2143267	50.138	50.289
19)	L4 AR-1242-4	5.775	5.020	1171547	2229165	45.685	51.050
20)	L4 AR-1242-5	6.517	5.545	371308	2511911	14.373	50.569 #
21)	L5 AR-1248-1	5.592	4.740	1646441	2909582	64.871	70.728
22)	L5 AR-1248-2	5.867	4.978	1134629	1977068	29.315	32.832
23)	L5 AR-1248-3	6.072	5.020	1310256	2229165	31.015	36.182
24)	L5 AR-1248-4	6.478	5.191	463935	2356763	11.143	32.735 #
25)	L5 AR-1248-5	6.517	5.586	371308	704488	9.103	10.676
26)	L6 AR-1254-1	6.451	5.545	1209555	2511911	25.892	24.793
27)	L6 AR-1254-2	6.671	5.694	1040251	1912616	15.118	21.666 #
28)	L6 AR-1254-3	7.040	6.116	579934	3201412	8.402	23.157 #
29)	L6 AR-1254-4	7.326	6.333	321431	365499	7.140	4.547 #
30)	L6 AR-1254-5	7.745	6.748	2993436	5560895	63.708	46.501 #
31)	L7 AR-1260-1	7.204	6.230	2986498	5912762	54.589	59.702
32)	L7 AR-1260-2	7.462	6.420	2888467	5928296	48.514	51.234
33)	L7 AR-1260-3	7.823	6.573	2039203	5482776	51.816	49.291
34)	L7 AR-1260-4	8.049	7.047	1914414	3987803	43.104	45.998
35)	L7 AR-1260-5	8.370	7.291	3678132	8773112	45.994	47.596
36)	L8 AR-1262-1	7.823	6.841	2039203	2524176	32.017	43.872 #
37)	L8 AR-1262-2	8.370	7.047	3678132	3987803	40.051	33.796
38)	L8 AR-1262-3	8.696	7.575	2408487	1959267	37.426	23.023 #
39)	L8 AR-1262-4	8.775	7.638	699567	6081032	21.067	40.255 #
40)	L8 AR-1262-5	9.439	8.137	757607	2313448	25.388	36.275 #
41)	L9 AR-1268-1	8.696	7.575	2408487	1959267	21.207	8.035 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
 Data File : PP059247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2023 07:51
 Operator : YP\AJ
 Sample : 03572-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 08:21:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.775	7.638	699567	6081032	7.108	27.765 #
43) L9	AR-1268-3	9.009	7.848	92720	756436	1.000	3.869 #
44) L9	AR-1268-4	9.439	8.137	757607	2313448	23.749	33.244 #
45) L9	AR-1268-5	9.864	8.428	310782	673735	1.145	1.300


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
Data File : PP059247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2023 07:51
Operator : YP\AJ
Sample : 03572-07
Misc : AR1660 LOD 40 PPB
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 08:21:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

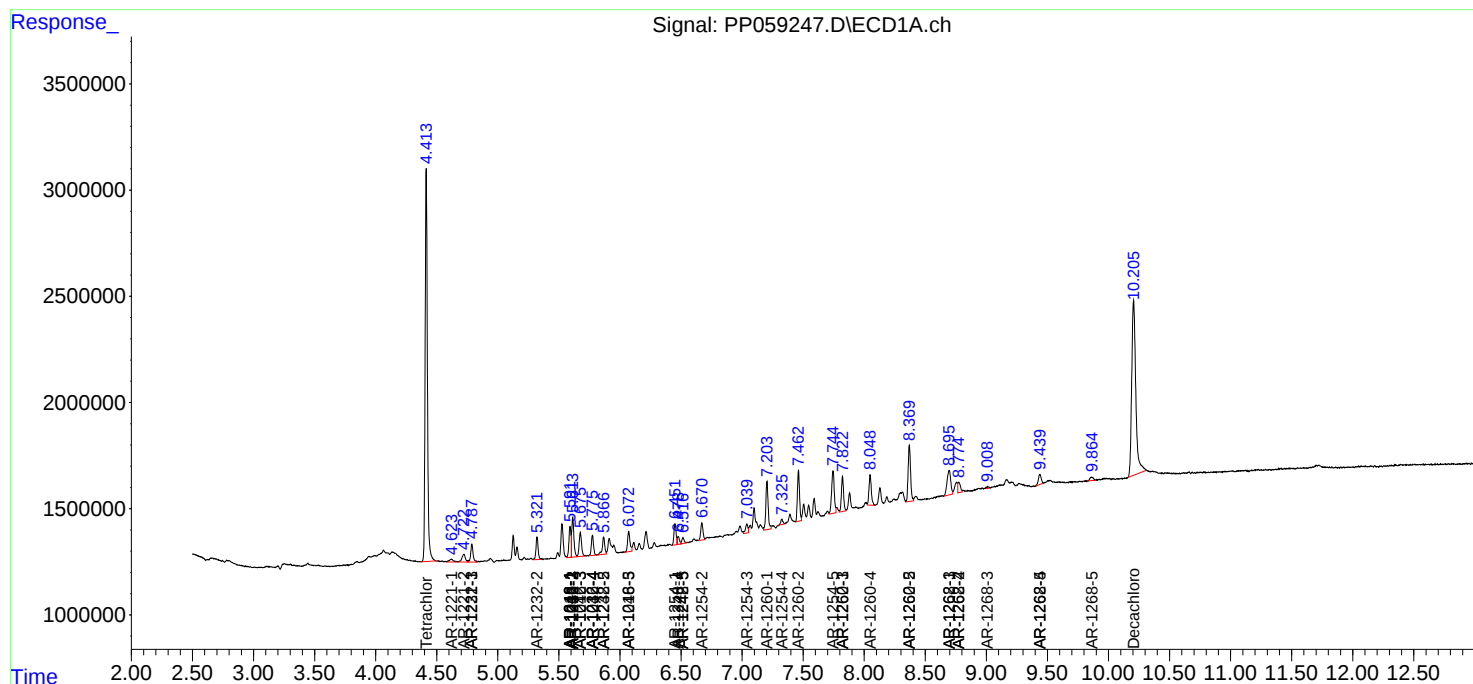


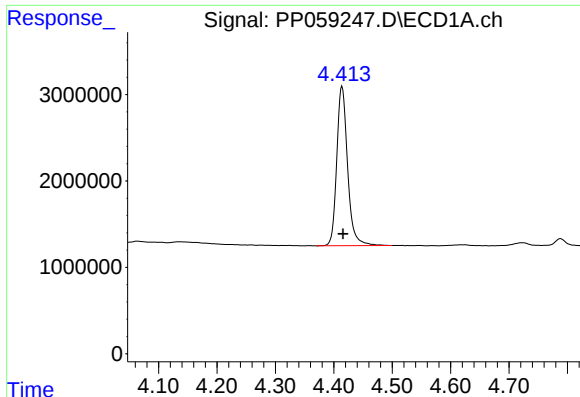

#1 Tetrachloro-m-xylene


R.T.: 4.414 min
Delta R.T.: -0.002 min
Response: 23769116
Conc: 19.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

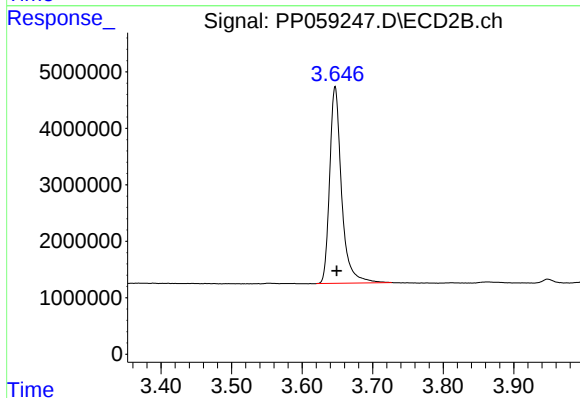


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: -0.002 min
Response: 40960231
Conc: 20.22 ng/ml

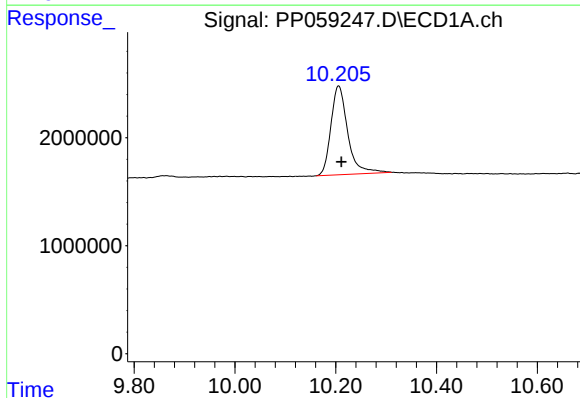


#2 Decachlorobiphenyl

R.T.: 10.206 min
Delta R.T.: -0.006 min
Response: 19040569
Conc: 24.95 ng/ml

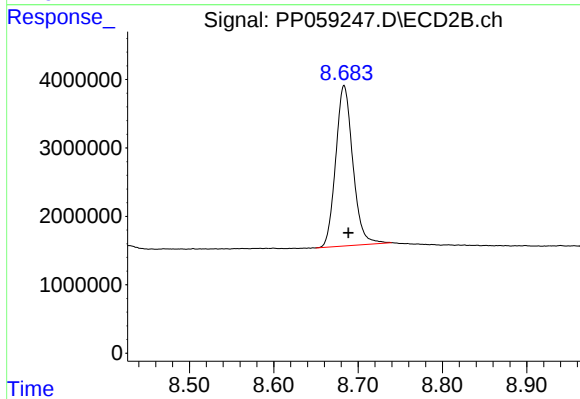

#2 Decachlorobiphenyl


R.T.: 8.683 min
Delta R.T.: -0.005 min
Response: 33076508
Conc: 23.51 ng/ml

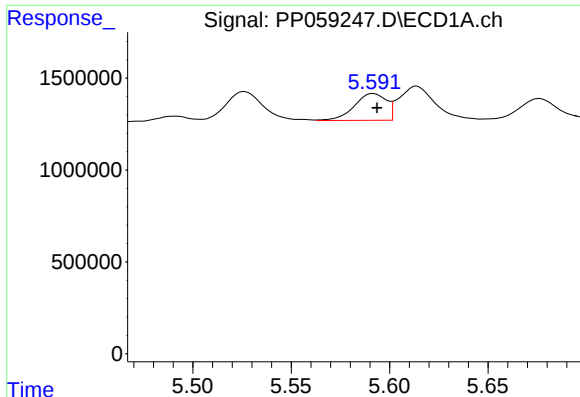

#3 AR-1016-1


R.T.: 5.592 min
Delta R.T.: -0.002 min
Response: 1646441
Conc: 41.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

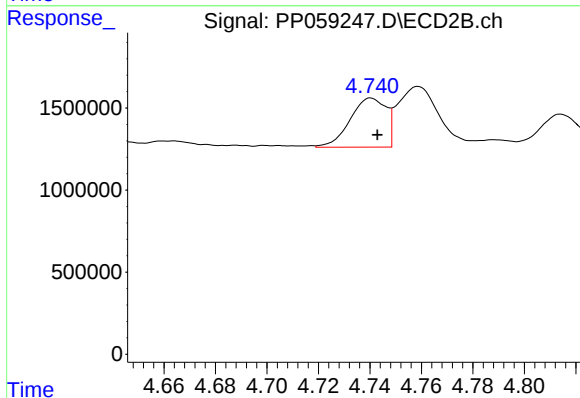


#3 AR-1016-1

R.T.: 4.740 min
Delta R.T.: -0.003 min
Response: 2909582
Conc: 45.36 ng/ml

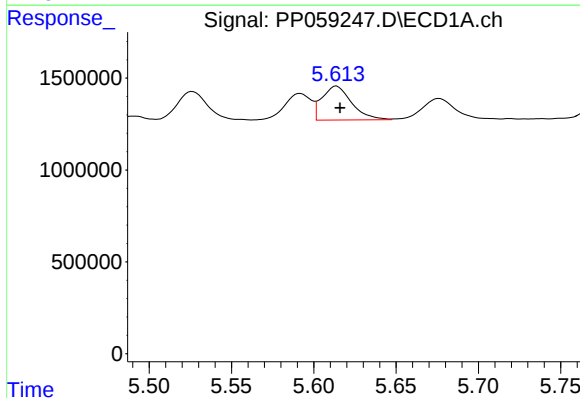


#4 AR-1016-2

R.T.: 5.614 min
Delta R.T.: -0.002 min
Response: 2327964
Conc: 41.07 ng/ml

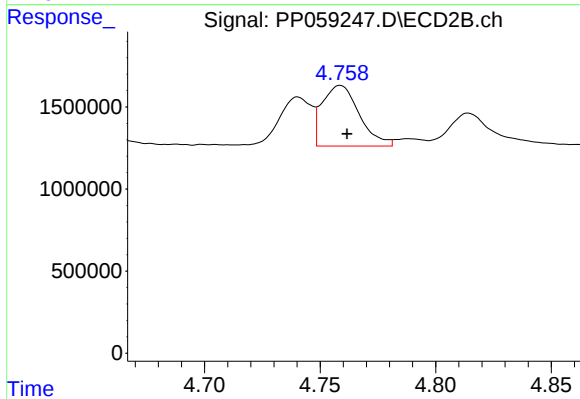

#4 AR-1016-2


R.T.: 4.759 min
Delta R.T.: -0.003 min
Response: 4113629
Conc: 45.28 ng/ml

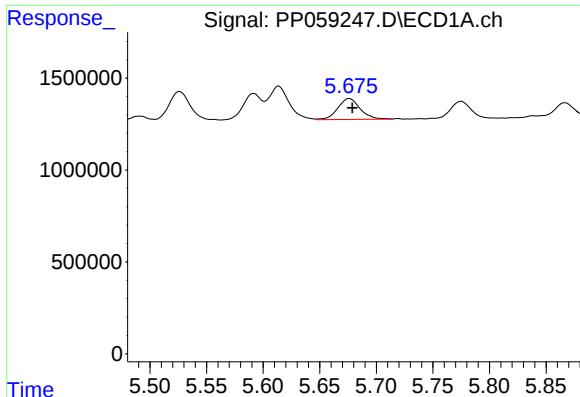

#5 AR-1016-3


R.T.: 5.676 min
Delta R.T.: -0.003 min
Response: 1575247
Conc: 43.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

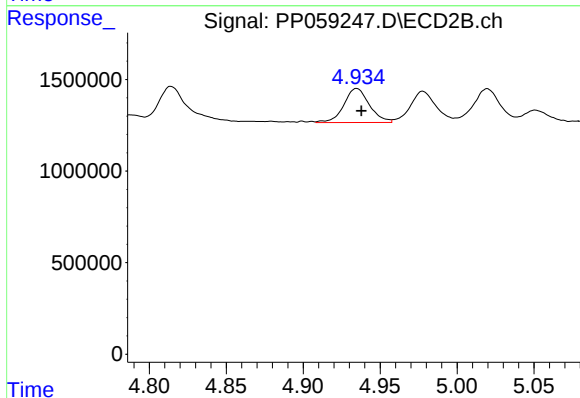


#5 AR-1016-3

R.T.: 4.935 min
Delta R.T.: -0.003 min
Response: 2143267
Conc: 44.61 ng/ml

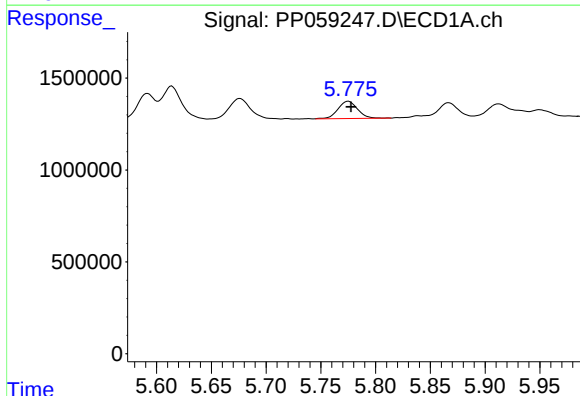


#6 AR-1016-4

R.T.: 5.775 min
Delta R.T.: -0.002 min
Response: 1171547
Conc: 40.44 ng/ml

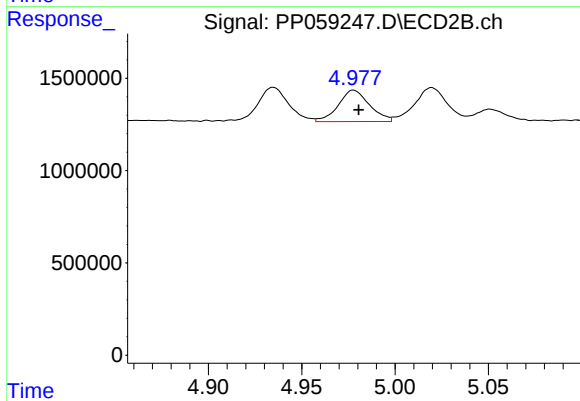

#6 AR-1016-4


R.T.: 4.978 min
Delta R.T.: -0.003 min
Response: 1977068
Conc: 47.88 ng/ml

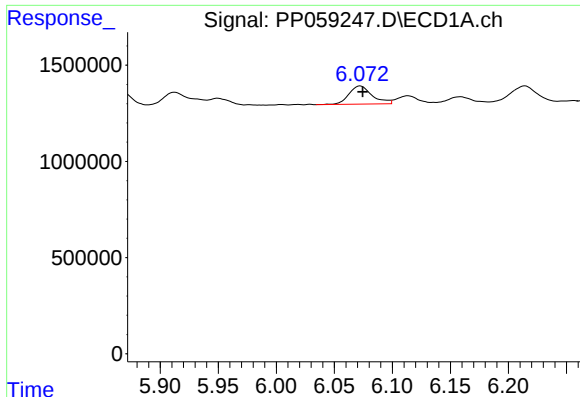

#7 AR-1016-5


R.T.: 6.072 min
Delta R.T.: -0.002 min
Response: 1310256
Conc: 43.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

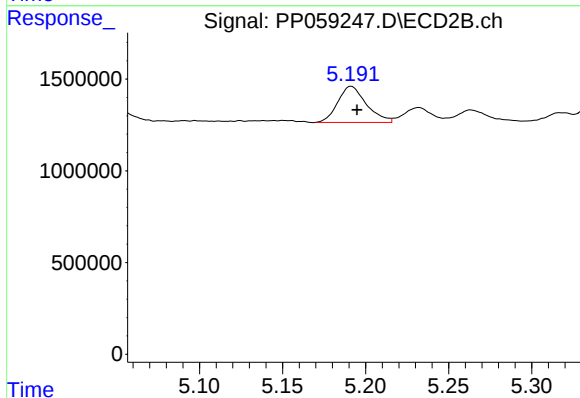


#7 AR-1016-5

R.T.: 5.191 min
Delta R.T.: -0.004 min
Response: 2356763
Conc: 45.29 ng/ml

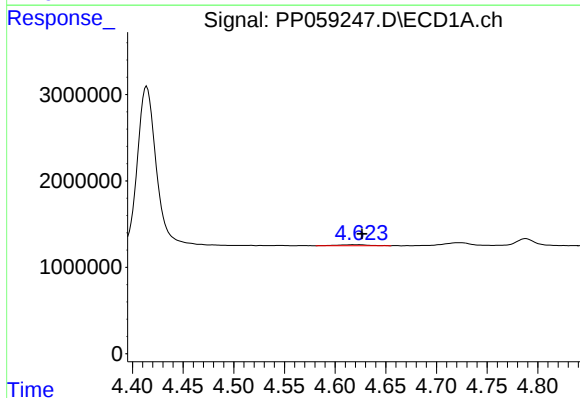


#8 AR-1221-1

R.T.: 4.623 min
Delta R.T.: -0.003 min
Response: 289962
Conc: 18.41 ng/ml

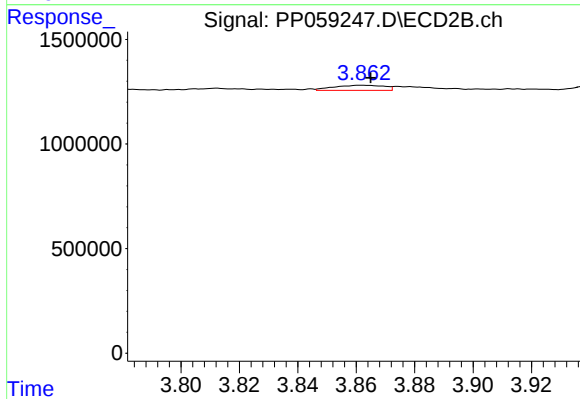

#8 AR-1221-1


R.T.: 3.862 min
Delta R.T.: -0.003 min
Response: 291208
Conc: 10.73 ng/ml

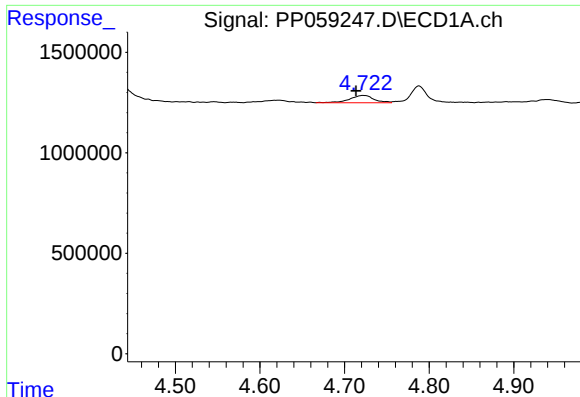

#9 AR-1221-2


R.T.: 4.723 min
Delta R.T.: 0.009 min
Response: 738465
Conc: 62.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

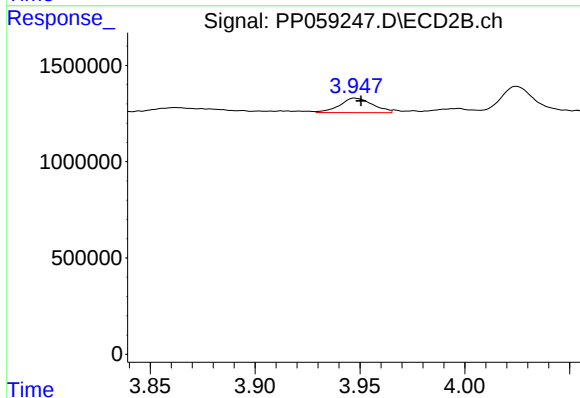


#9 AR-1221-2

R.T.: 3.947 min
Delta R.T.: -0.003 min
Response: 818542
Conc: 41.11 ng/ml

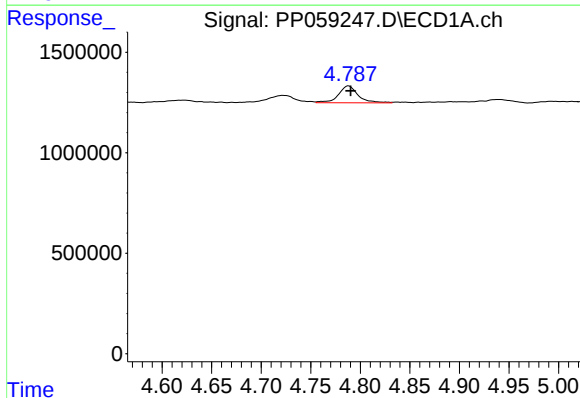


#10 AR-1221-3

R.T.: 4.788 min
Delta R.T.: -0.002 min
Response: 1162335
Conc: 33.01 ng/ml

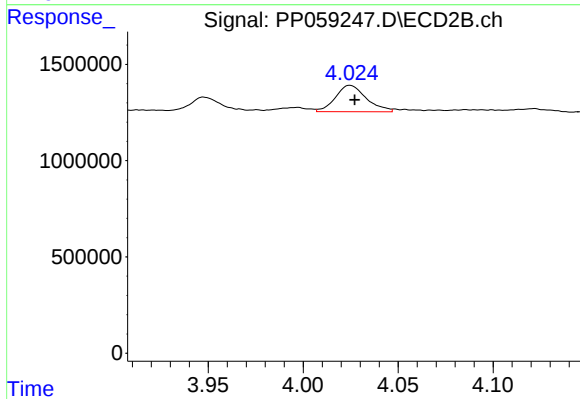

#10 AR-1221-3


R.T.: 4.025 min
Delta R.T.: -0.003 min
Response: 1563542
Conc: 26.26 ng/ml

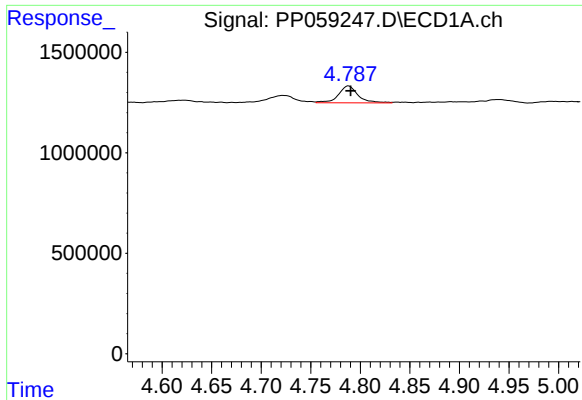

#11 AR-1232-1


R.T.: 4.788 min
Delta R.T.: -0.002 min
Response: 1162335
Conc: 39.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

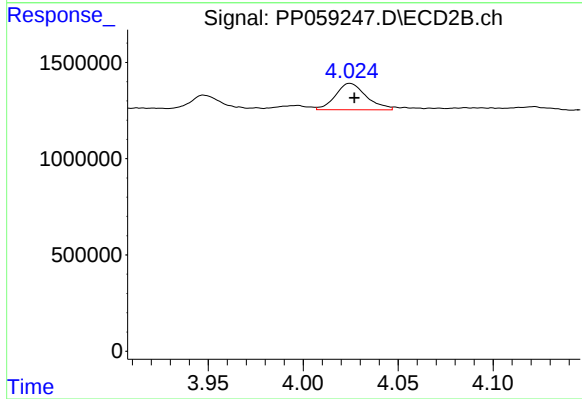


#11 AR-1232-1

R.T.: 4.025 min
Delta R.T.: -0.002 min
Response: 1563542
Conc: 32.95 ng/ml

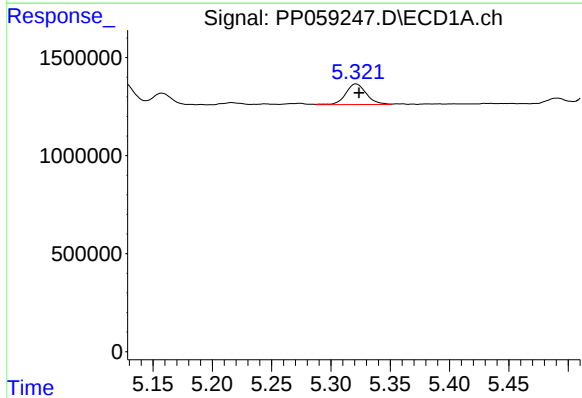


#12 AR-1232-2

R.T.: 5.321 min
Delta R.T.: -0.002 min
Response: 1287169
Conc: 82.58 ng/ml

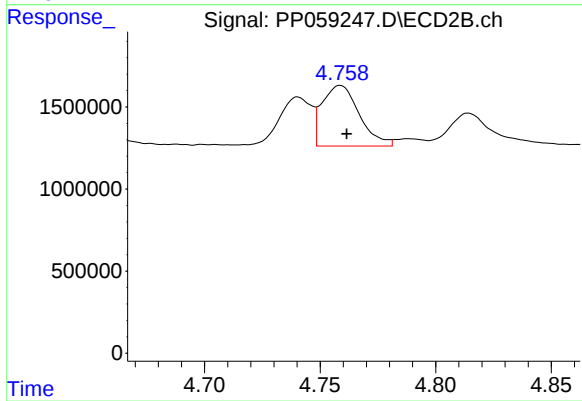

#12 AR-1232-2


R.T.: 4.759 min
Delta R.T.: -0.003 min
Response: 4113629
Conc: 96.98 ng/ml

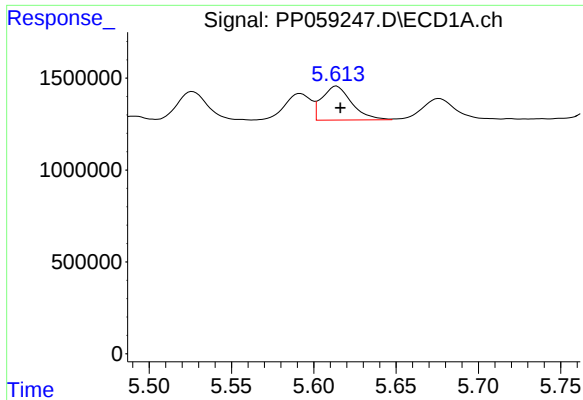

#13 AR-1232-3


R.T.: 5.614 min
Delta R.T.: -0.002 min
Response: 2327964
Conc: 88.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

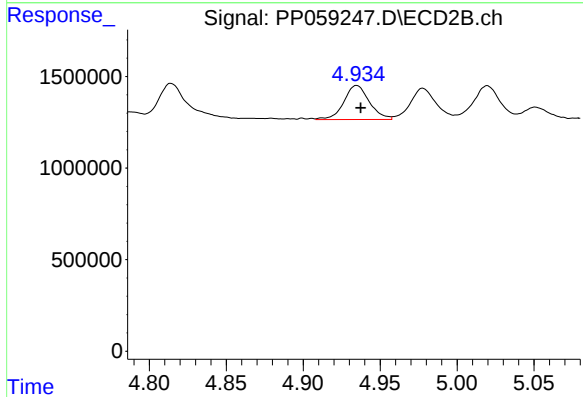


#13 AR-1232-3

R.T.: 4.935 min
Delta R.T.: -0.003 min
Response: 2143267
Conc: 96.60 ng/ml

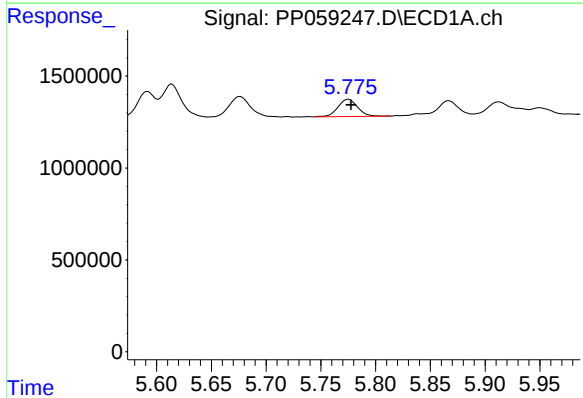


#14 AR-1232-4

R.T.: 5.775 min
Delta R.T.: -0.002 min
Response: 1171547
Conc: 88.52 ng/ml

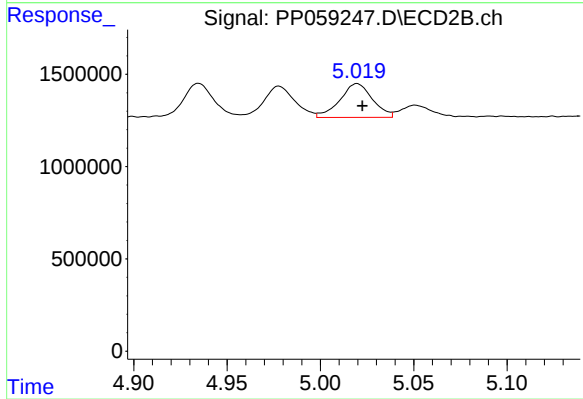

#14 AR-1232-4


R.T.: 5.020 min
Delta R.T.: -0.003 min
Response: 2229165
Conc: 105.58 ng/ml

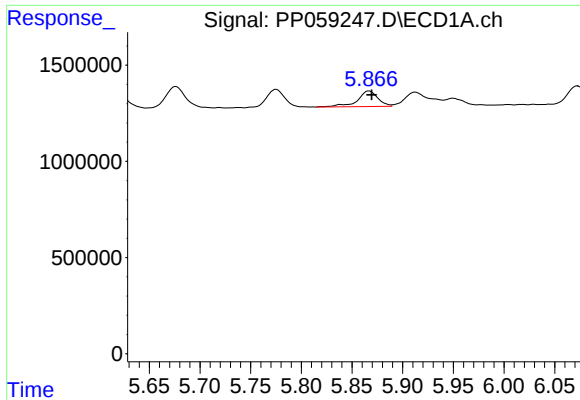

#15 AR-1232-5


R.T.: 5.867 min
Delta R.T.: -0.003 min
Response: 1134629
Conc: 99.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

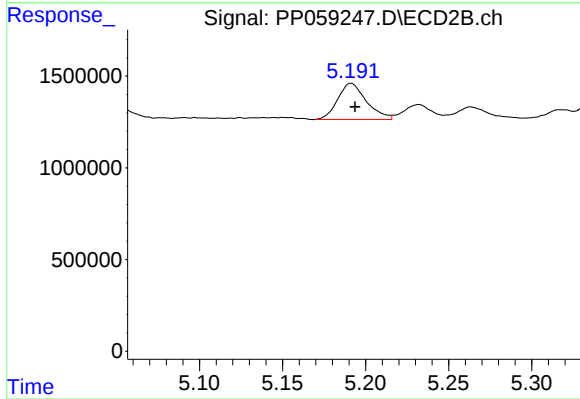


#15 AR-1232-5

R.T.: 5.191 min
Delta R.T.: -0.002 min
Response: 2356763
Conc: 102.81 ng/ml

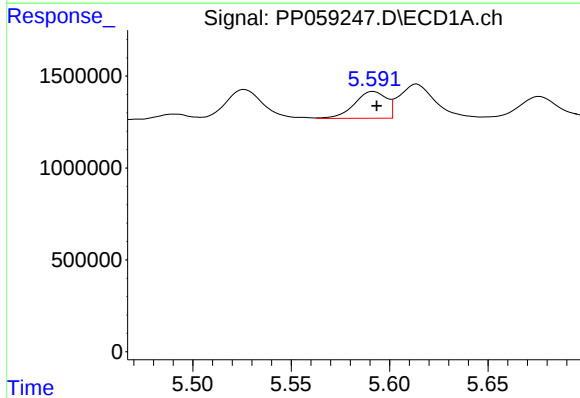


#16 AR-1242-1

R.T.: 5.592 min
Delta R.T.: -0.002 min
Response: 1646441
Conc: 48.10 ng/ml

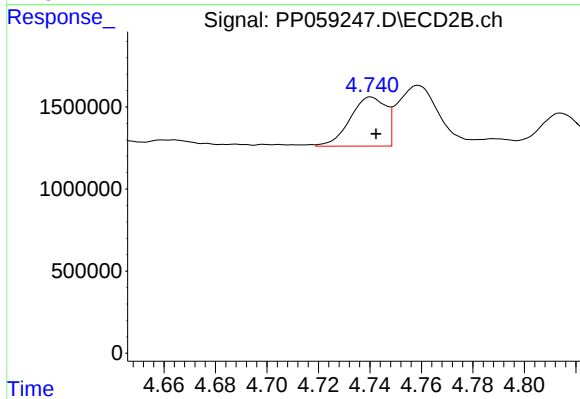

#16 AR-1242-1


R.T.: 4.740 min
Delta R.T.: -0.002 min
Response: 2909582
Conc: 51.99 ng/ml

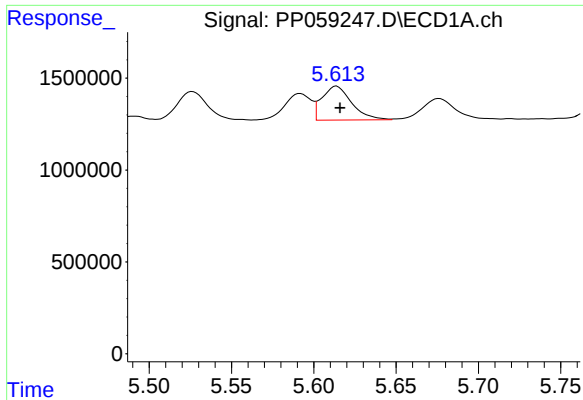

#17 AR-1242-2


R.T.: 5.614 min
Delta R.T.: -0.002 min
Response: 2327964
Conc: 47.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

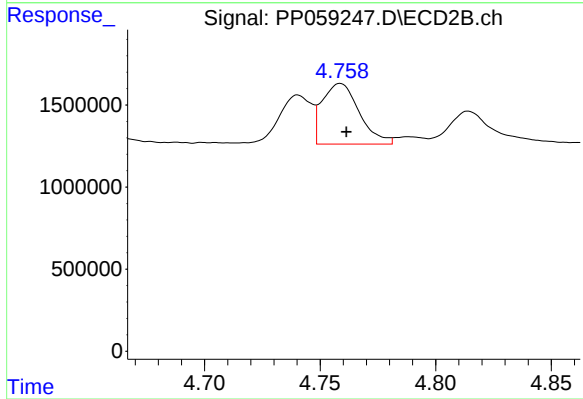


#17 AR-1242-2

R.T.: 4.759 min
Delta R.T.: -0.003 min
Response: 4113629
Conc: 51.59 ng/ml

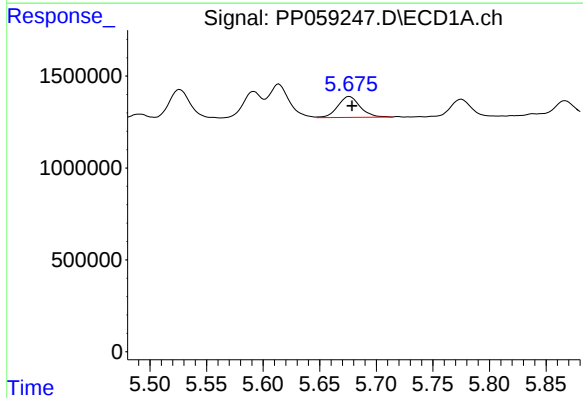


#18 AR-1242-3

R.T.: 5.676 min
Delta R.T.: -0.002 min
Response: 1575247
Conc: 50.14 ng/ml

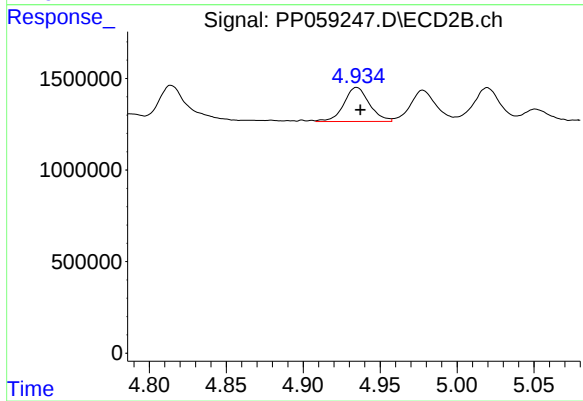

#18 AR-1242-3


R.T.: 4.935 min
Delta R.T.: -0.003 min
Response: 2143267
Conc: 50.29 ng/ml

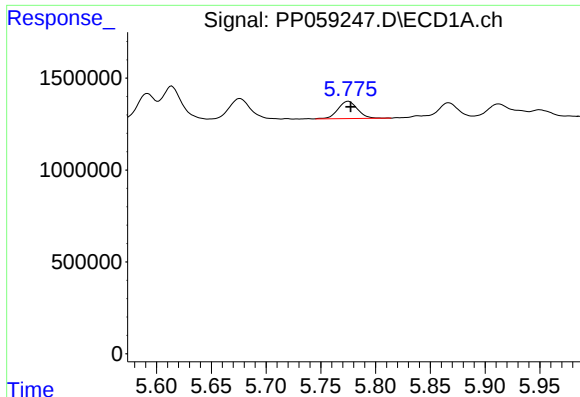

#19 AR-1242-4


R.T.: 5.775 min
Delta R.T.: -0.002 min
Response: 1171547
Conc: 45.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

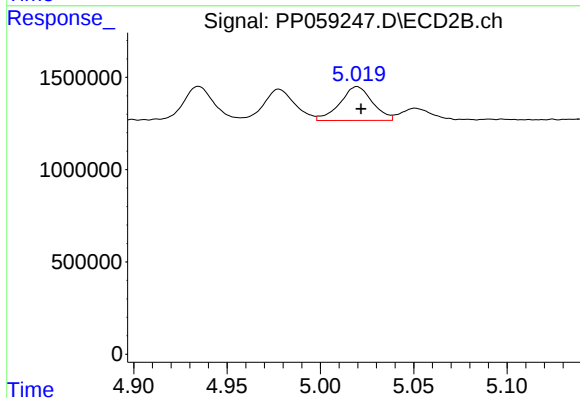


#19 AR-1242-4

R.T.: 5.020 min
Delta R.T.: -0.002 min
Response: 2229165
Conc: 51.05 ng/ml

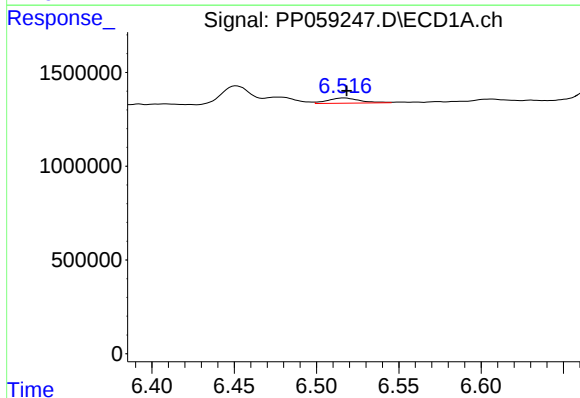


#20 AR-1242-5

R.T.: 6.517 min
Delta R.T.: -0.002 min
Response: 371308
Conc: 14.37 ng/ml

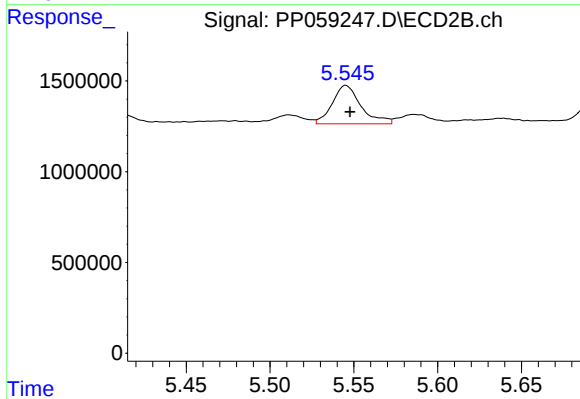

#20 AR-1242-5


R.T.: 5.545 min
Delta R.T.: -0.003 min
Response: 2511911
Conc: 50.57 ng/ml

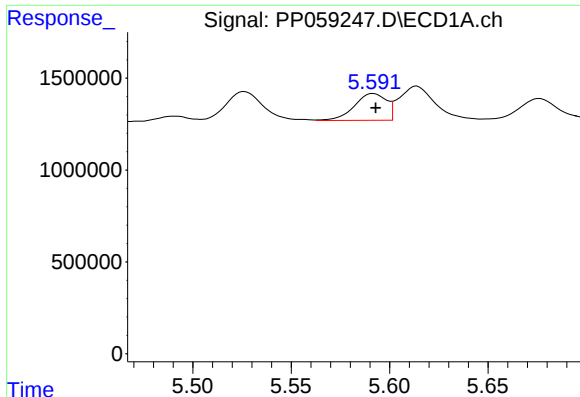

#21 AR-1248-1


R.T.: 5.592 min
Delta R.T.: -0.001 min
Response: 1646441
Conc: 64.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

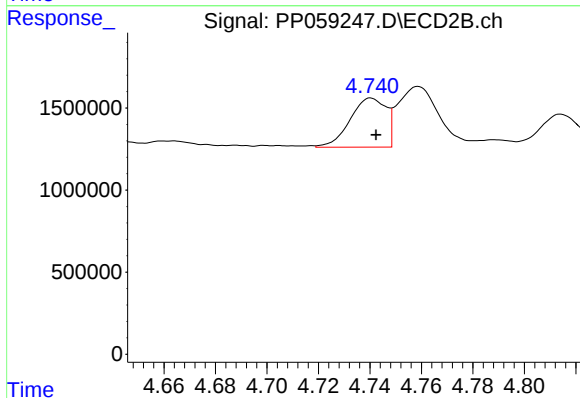


#21 AR-1248-1

R.T.: 4.740 min
Delta R.T.: -0.002 min
Response: 2909582
Conc: 70.73 ng/ml

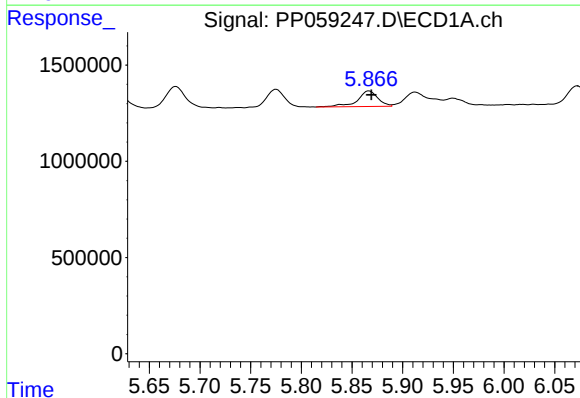


#22 AR-1248-2

R.T.: 5.867 min
Delta R.T.: -0.002 min
Response: 1134629
Conc: 29.31 ng/ml

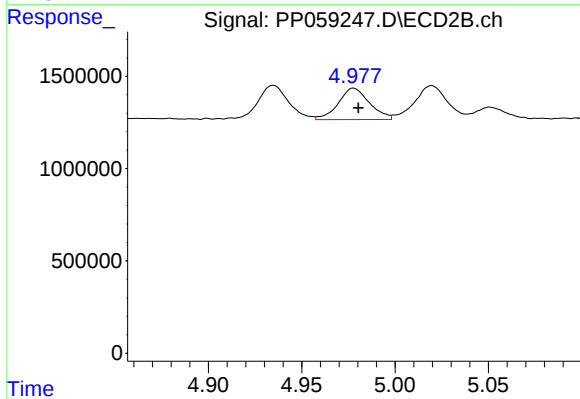

#22 AR-1248-2


R.T.: 4.978 min
Delta R.T.: -0.003 min
Response: 1977068
Conc: 32.83 ng/ml

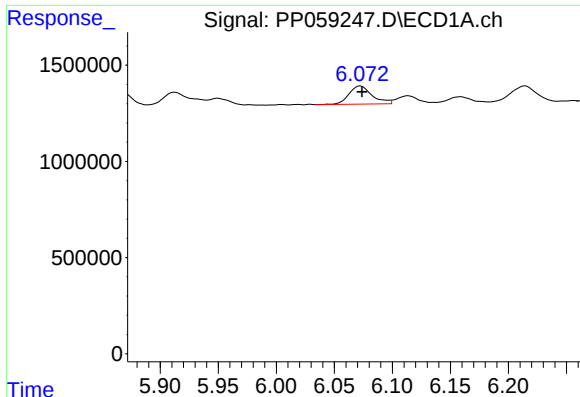

#23 AR-1248-3


R.T.: 6.072 min
Delta R.T.: -0.002 min
Response: 1310256
Conc: 31.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

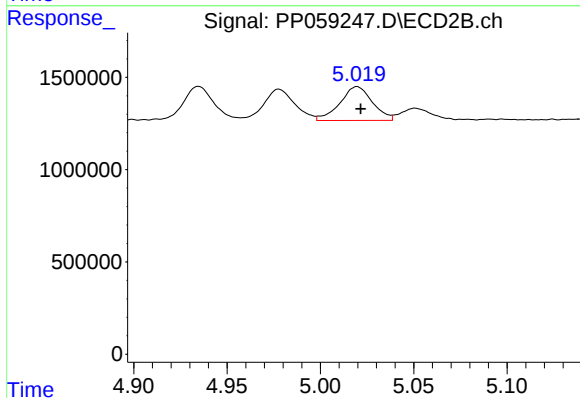


#23 AR-1248-3

R.T.: 5.020 min
Delta R.T.: -0.002 min
Response: 2229165
Conc: 36.18 ng/ml

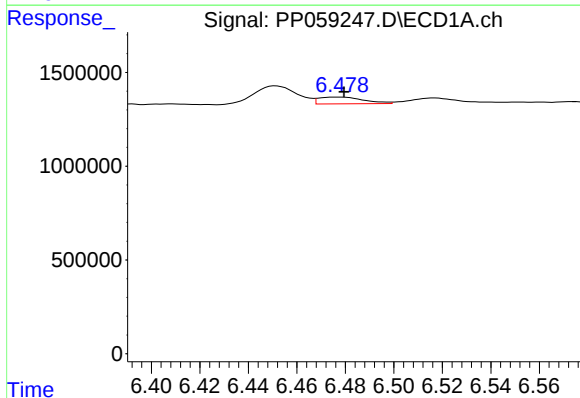


#24 AR-1248-4

R.T.: 6.478 min
Delta R.T.: -0.001 min
Response: 463935
Conc: 11.14 ng/ml

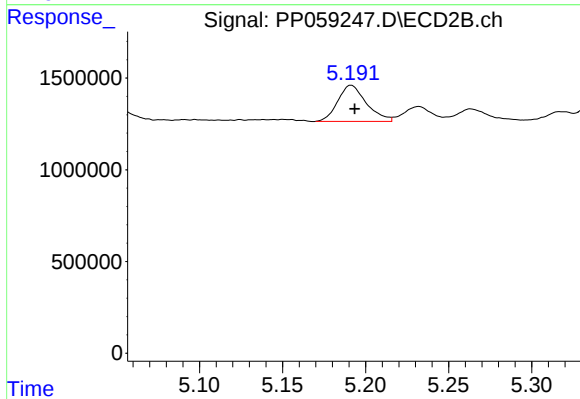

#24 AR-1248-4


R.T.: 5.191 min
Delta R.T.: -0.002 min
Response: 2356763
Conc: 32.73 ng/ml

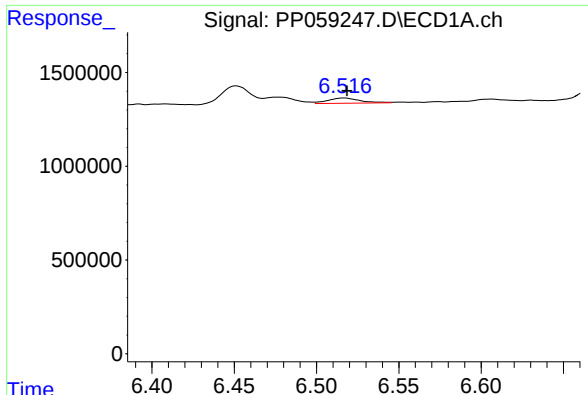

#25 AR-1248-5


R.T.: 6.517 min
Delta R.T.: -0.002 min
Response: 371308
Conc: 9.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

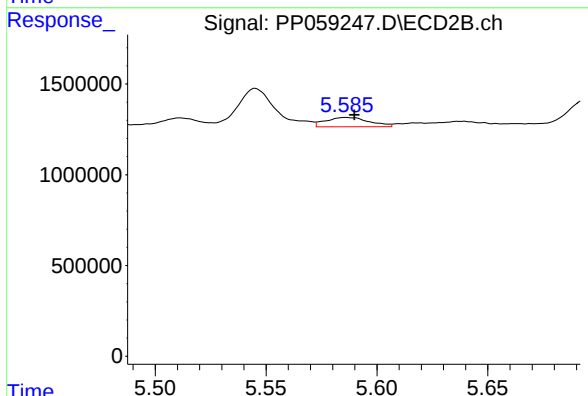


#25 AR-1248-5

R.T.: 5.586 min
Delta R.T.: -0.004 min
Response: 704488
Conc: 10.68 ng/ml

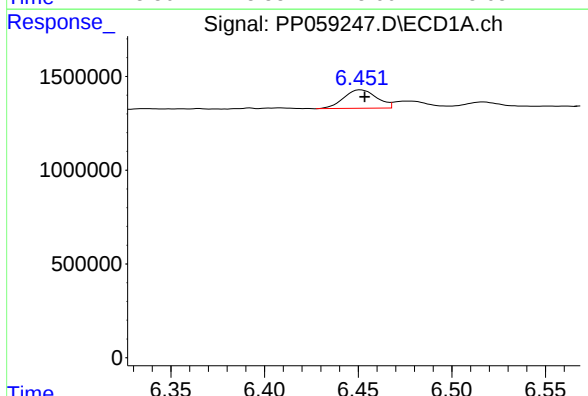


#26 AR-1254-1

R.T.: 6.451 min
Delta R.T.: -0.002 min
Response: 1209555
Conc: 25.89 ng/ml

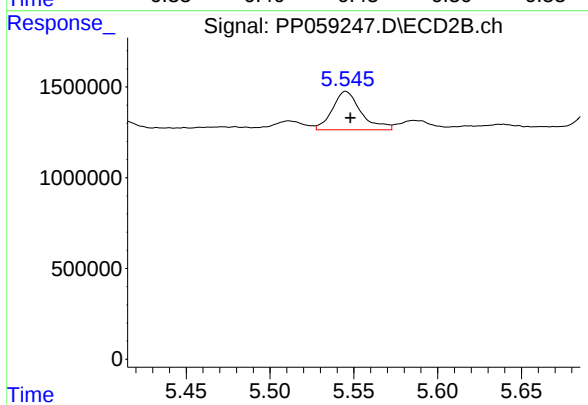

#26 AR-1254-1


R.T.: 5.545 min
Delta R.T.: -0.003 min
Response: 2511911
Conc: 24.79 ng/ml

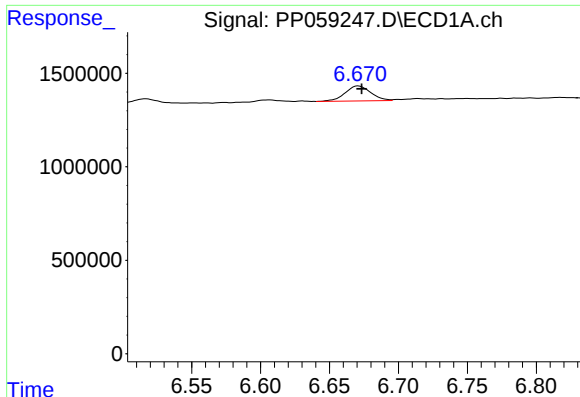

#27 AR-1254-2


R.T.: 6.671 min
Delta R.T.: -0.002 min
Response: 1040251
Conc: 15.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

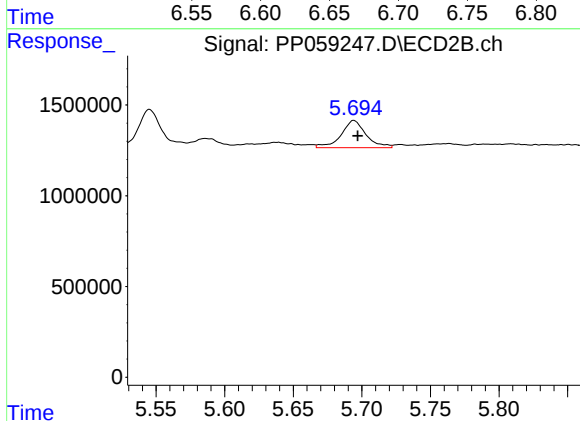


#27 AR-1254-2

R.T.: 5.694 min
Delta R.T.: -0.003 min
Response: 1912616
Conc: 21.67 ng/ml

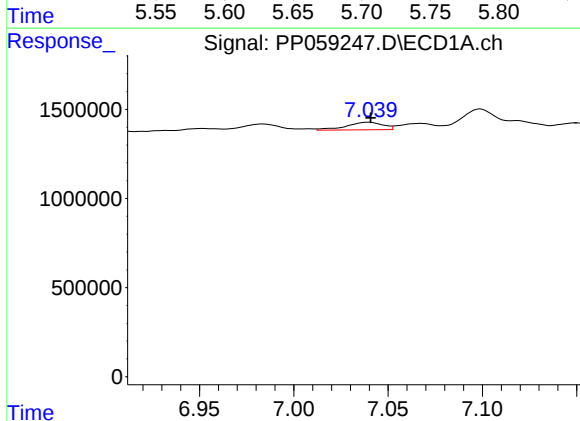


#28 AR-1254-3

R.T.: 7.040 min
Delta R.T.: -0.001 min
Response: 579934
Conc: 8.40 ng/ml

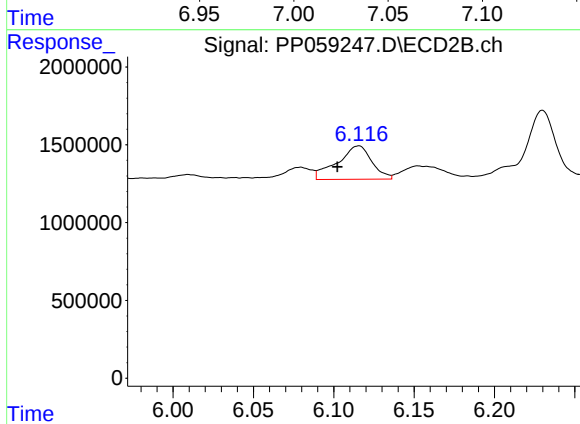

#28 AR-1254-3


R.T.: 6.116 min
Delta R.T.: 0.014 min
Response: 3201412
Conc: 23.16 ng/ml

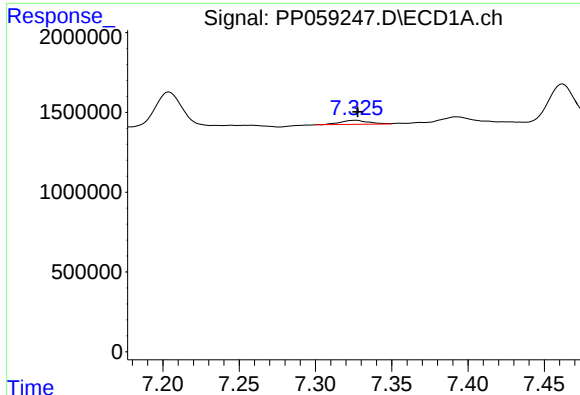

#29 AR-1254-4


R.T.: 7.326 min
Delta R.T.: -0.002 min
Response: 321431
Conc: 7.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

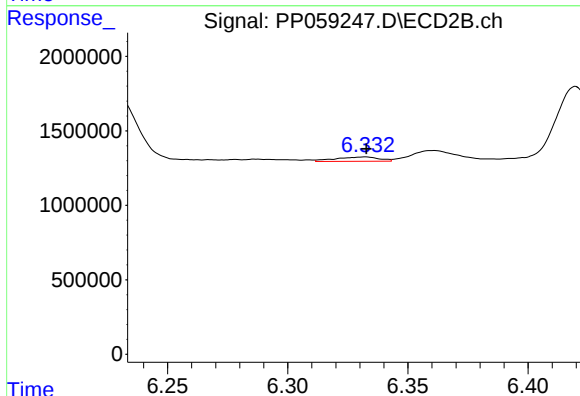


#29 AR-1254-4

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 365499
Conc: 4.55 ng/ml

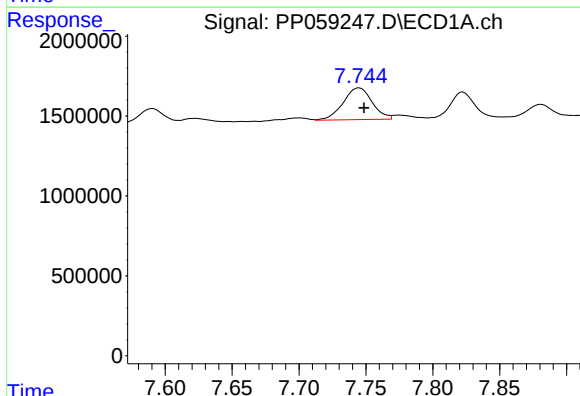


#30 AR-1254-5

R.T.: 7.745 min
Delta R.T.: -0.004 min
Response: 2993436
Conc: 63.71 ng/ml

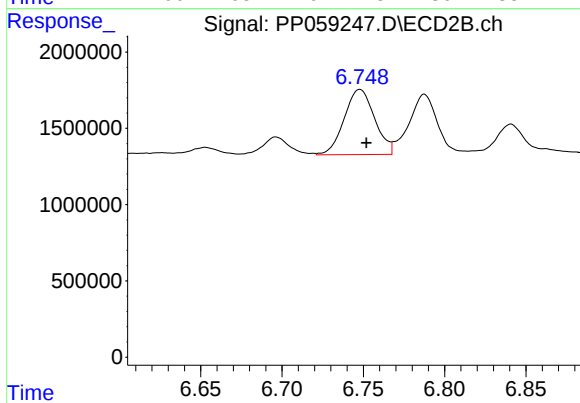

#30 AR-1254-5


R.T.: 6.748 min
Delta R.T.: -0.004 min
Response: 5560895
Conc: 46.50 ng/ml

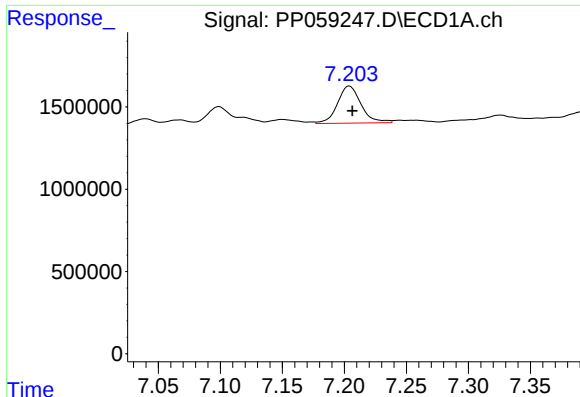

#31 AR-1260-1


R.T.: 7.204 min
Delta R.T.: -0.002 min
Response: 2986498
Conc: 54.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

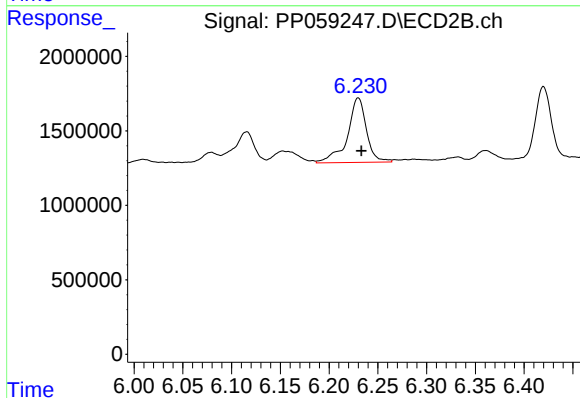


#31 AR-1260-1

R.T.: 6.230 min
Delta R.T.: -0.003 min
Response: 5912762
Conc: 59.70 ng/ml

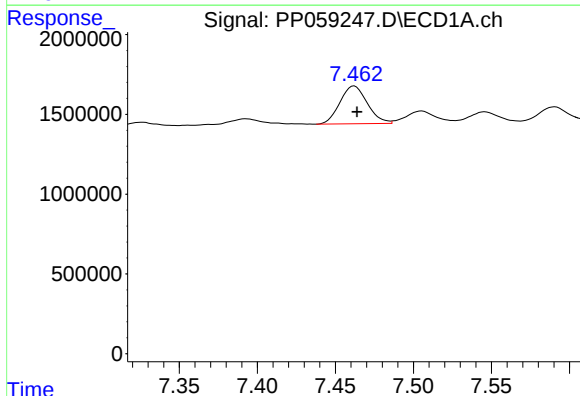


#32 AR-1260-2

R.T.: 7.462 min
Delta R.T.: -0.002 min
Response: 2888467
Conc: 48.51 ng/ml

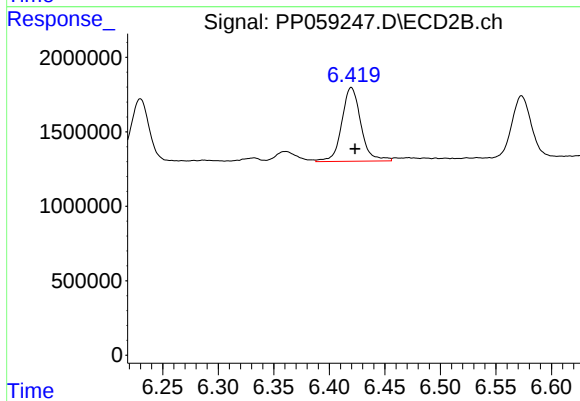

#32 AR-1260-2


R.T.: 6.420 min
Delta R.T.: -0.003 min
Response: 5928296
Conc: 51.23 ng/ml

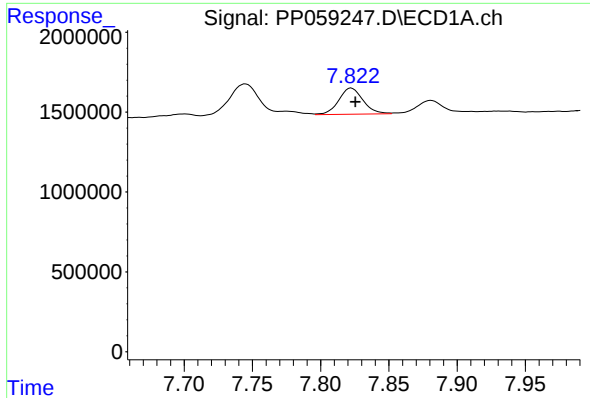

#33 AR-1260-3


R.T.: 7.823 min
Delta R.T.: -0.003 min
Response: 2039203
Conc: 51.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

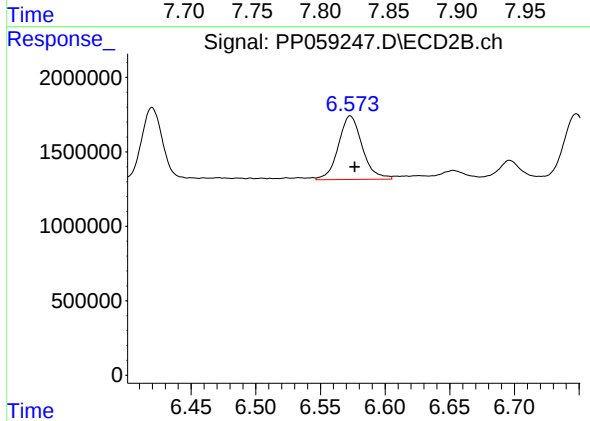


#33 AR-1260-3

R.T.: 6.573 min
Delta R.T.: -0.003 min
Response: 5482776
Conc: 49.29 ng/ml

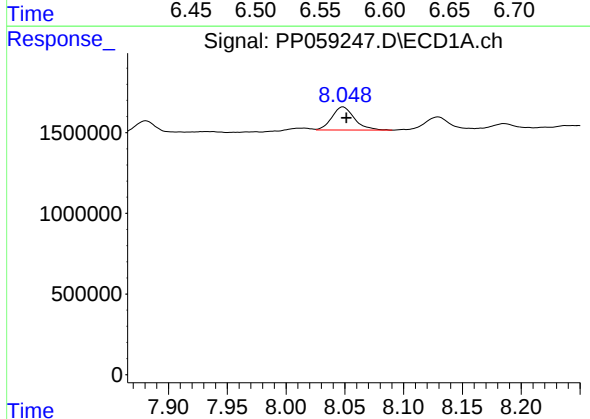


#34 AR-1260-4

R.T.: 8.049 min
Delta R.T.: -0.003 min
Response: 1914414
Conc: 43.10 ng/ml

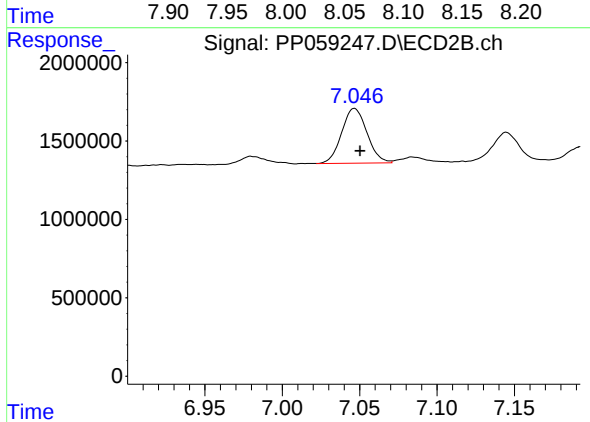

#34 AR-1260-4


R.T.: 7.047 min
Delta R.T.: -0.004 min
Response: 3987803
Conc: 46.00 ng/ml

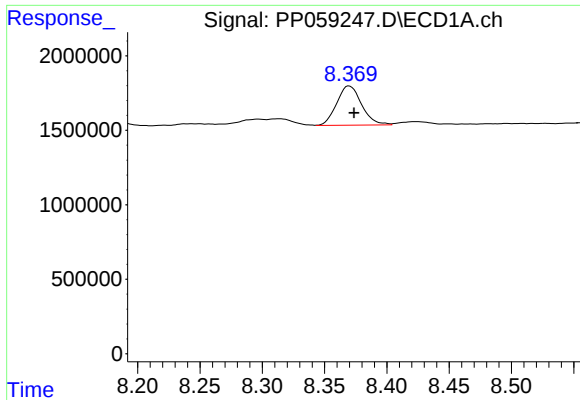

#35 AR-1260-5


R.T.: 8.370 min
Delta R.T.: -0.004 min
Response: 3678132
Conc: 45.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

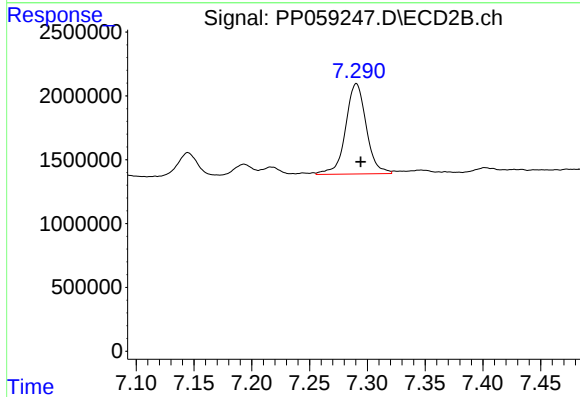


#35 AR-1260-5

R.T.: 7.291 min
Delta R.T.: -0.004 min
Response: 8773112
Conc: 47.60 ng/ml

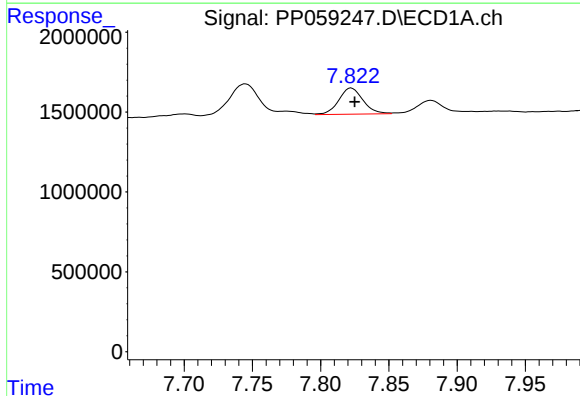


#36 AR-1262-1

R.T.: 7.823 min
Delta R.T.: -0.002 min
Response: 2039203
Conc: 32.02 ng/ml

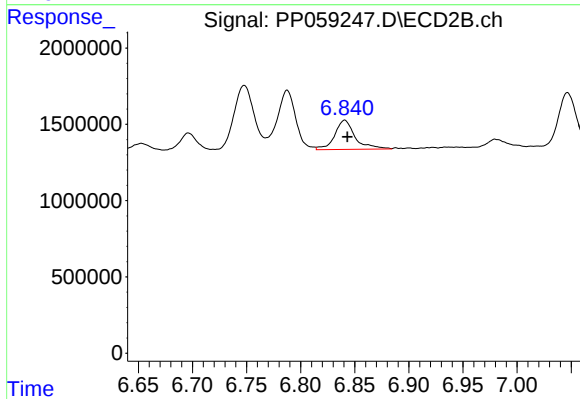

#36 AR-1262-1


R.T.: 6.841 min
Delta R.T.: -0.002 min
Response: 2524176
Conc: 43.87 ng/ml

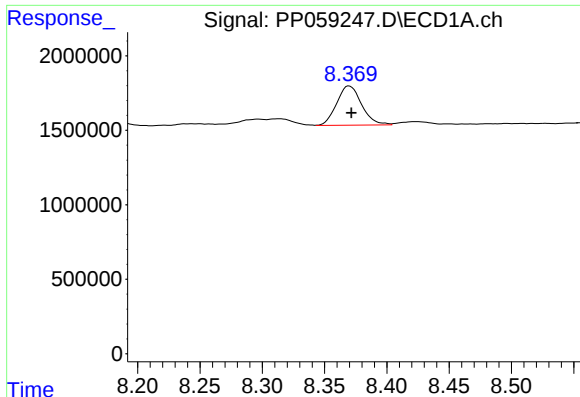

#37 AR-1262-2


R.T.: 8.370 min
Delta R.T.: -0.002 min
Response: 3678132
Conc: 40.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

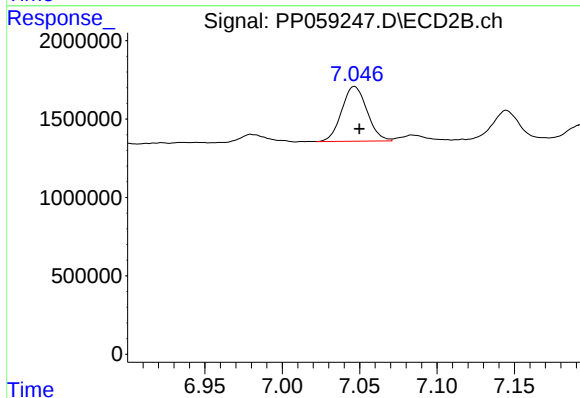


#37 AR-1262-2

R.T.: 7.047 min
Delta R.T.: -0.003 min
Response: 3987803
Conc: 33.80 ng/ml

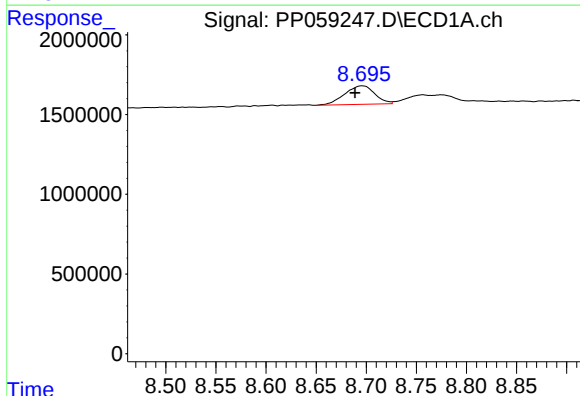


#38 AR-1262-3

R.T.: 8.696 min
Delta R.T.: 0.007 min
Response: 2408487
Conc: 37.43 ng/ml

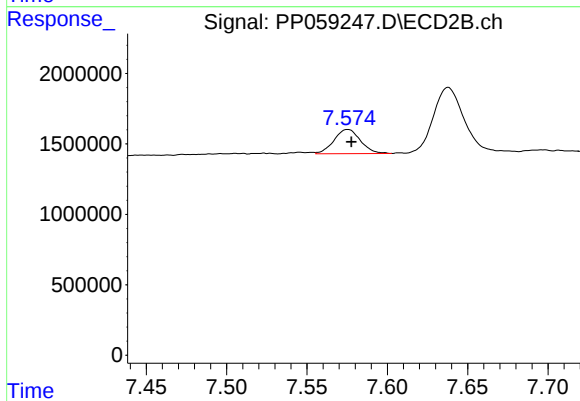

#38 AR-1262-3


R.T.: 7.575 min
Delta R.T.: -0.002 min
Response: 1959267
Conc: 23.02 ng/ml

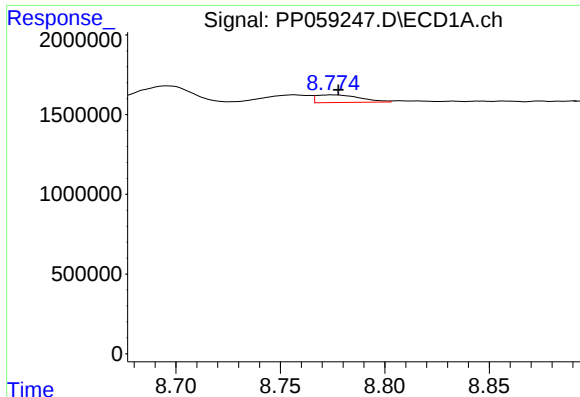

#39 AR-1262-4


R.T.: 8.775 min
Delta R.T.: -0.003 min
Response: 699567
Conc: 21.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

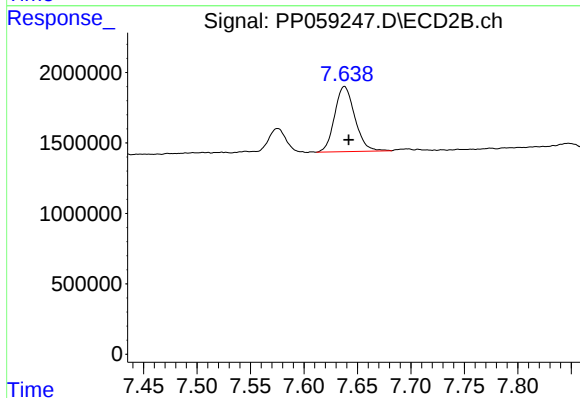


#39 AR-1262-4

R.T.: 7.638 min
Delta R.T.: -0.004 min
Response: 6081032
Conc: 40.26 ng/ml

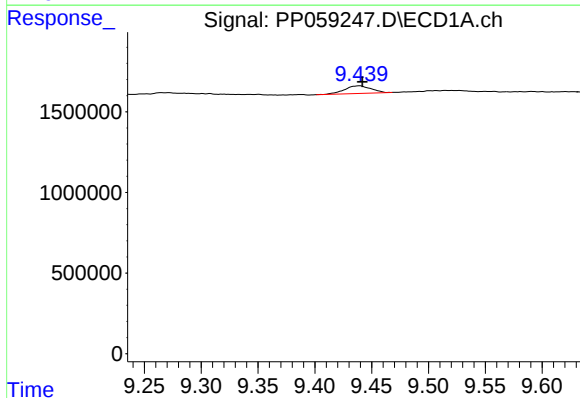


#40 AR-1262-5

R.T.: 9.439 min
Delta R.T.: -0.002 min
Response: 757607
Conc: 25.39 ng/ml

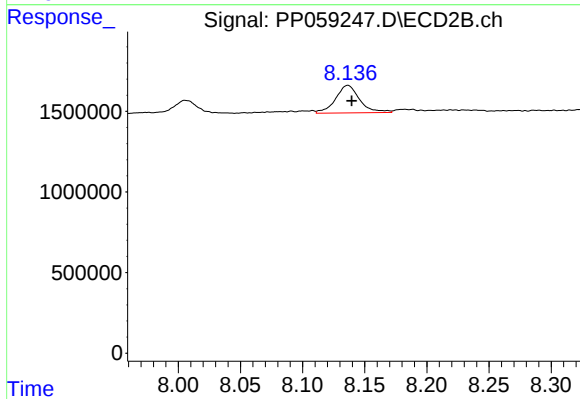

#40 AR-1262-5


R.T.: 8.137 min
Delta R.T.: -0.003 min
Response: 2313448
Conc: 36.27 ng/ml

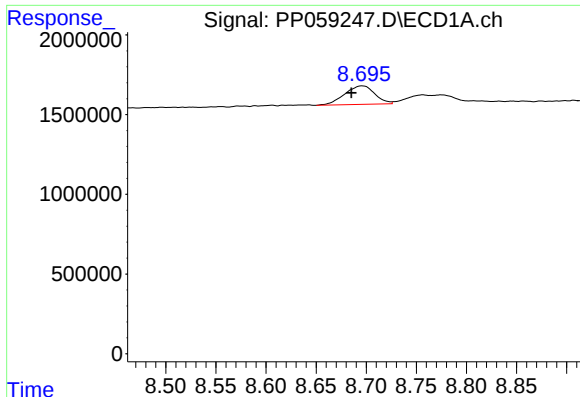

#41 AR-1268-1


R.T.: 8.696 min
Delta R.T.: 0.011 min
Response: 2408487
Conc: 21.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

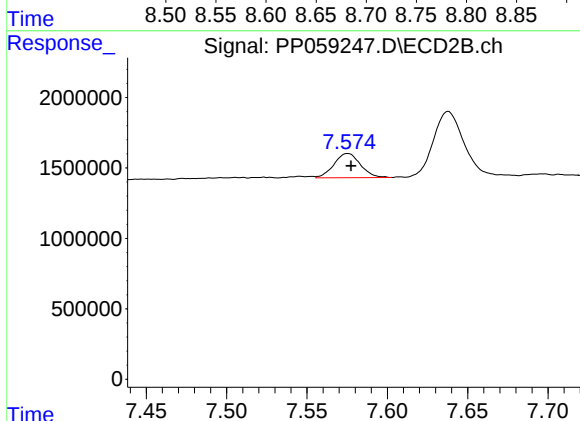


#41 AR-1268-1

R.T.: 7.575 min
Delta R.T.: -0.002 min
Response: 1959267
Conc: 8.03 ng/ml

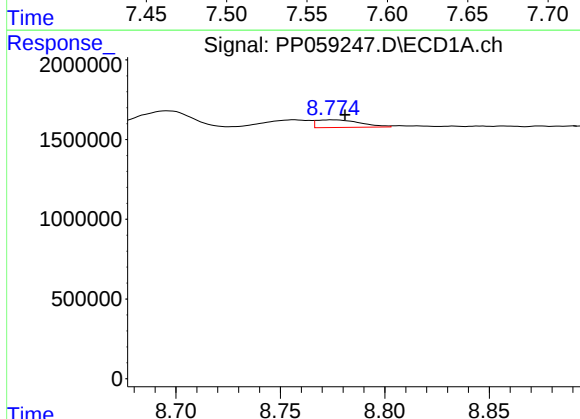


#42 AR-1268-2

R.T.: 8.775 min
Delta R.T.: -0.006 min
Response: 699567
Conc: 7.11 ng/ml

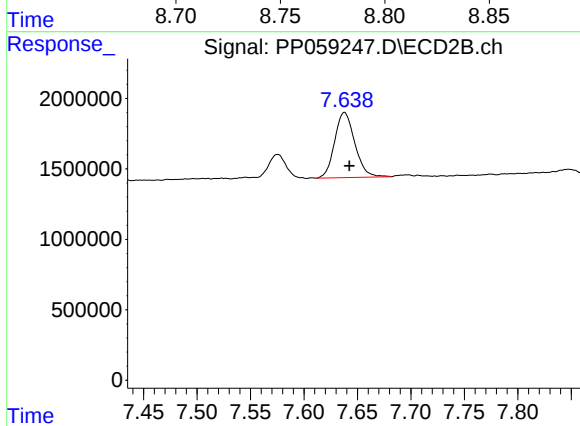

#42 AR-1268-2


R.T.: 7.638 min
Delta R.T.: -0.004 min
Response: 6081032
Conc: 27.76 ng/ml

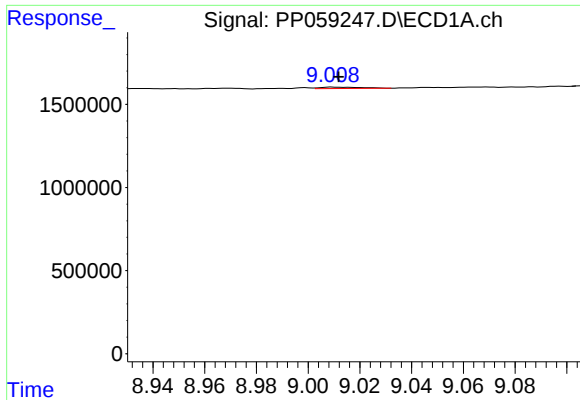

#43 AR-1268-3


R.T.: 9.009 min
Delta R.T.: -0.002 min
Response: 92720
Conc: 1.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

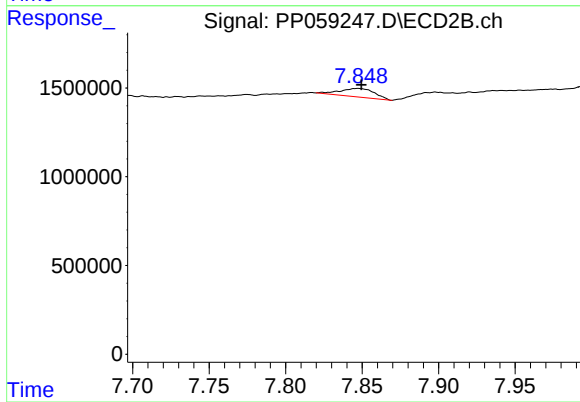


#43 AR-1268-3

R.T.: 7.848 min
Delta R.T.: -0.002 min
Response: 756436
Conc: 3.87 ng/ml

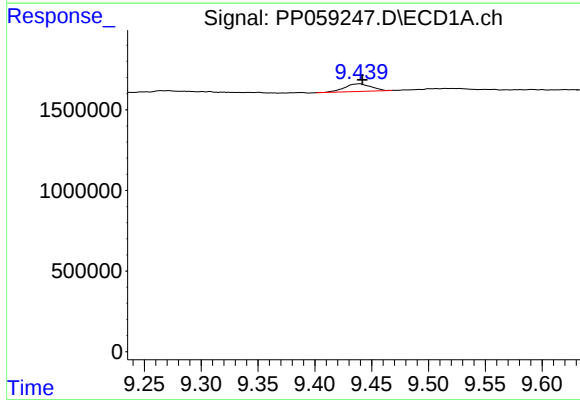


#44 AR-1268-4

R.T.: 9.439 min
Delta R.T.: -0.002 min
Response: 757607
Conc: 23.75 ng/ml

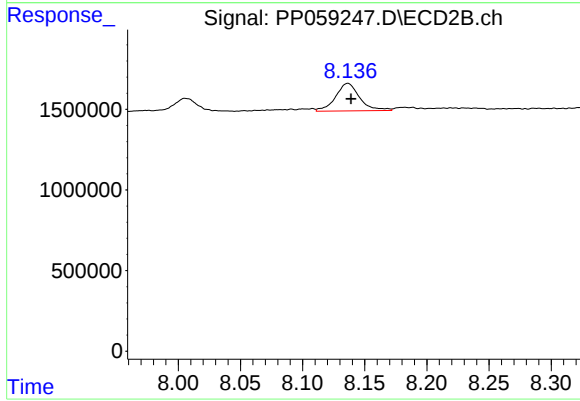

#44 AR-1268-4


R.T.: 8.137 min
Delta R.T.: -0.002 min
Response: 2313448
Conc: 33.24 ng/ml

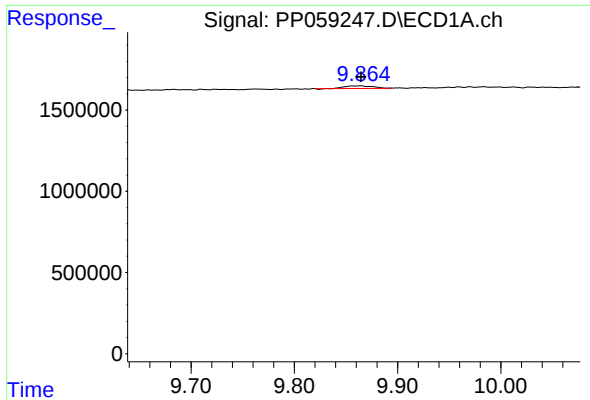

#45 AR-1268-5

R.T.: 9.864 min
Delta R.T.: 0.000 min
Response: 310782
Conc: 1.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

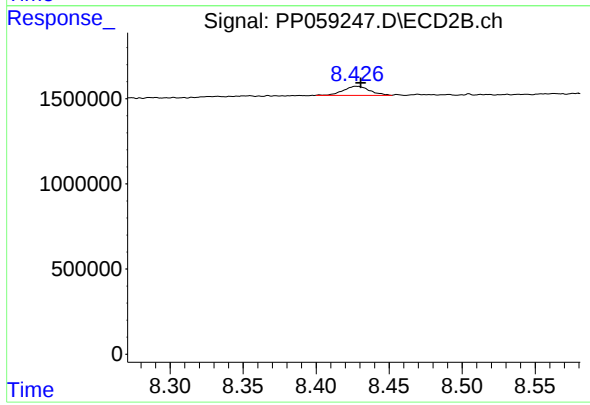

#45 AR-1268-5

R.T.: 8.428 min
Delta R.T.: -0.003 min
Response: 673735
Conc: 1.30 ng/ml