

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
 Data File : PP059250.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2023 08:40
 Operator : YP\AJ
 Sample : 03572-07
 Misc : AR1242 LOD 40 PPB
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 08:57:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.414	3.647	23775241	40286893	19.376	19.884
2)	SA Decachlor...	10.206	8.682	18795728	33446373	24.626	23.775
Target Compounds							
3)	L1 AR-1016-1	5.592	4.740	1361192	2373243	34.646	37.002
4)	L1 AR-1016-2	5.614	4.758	1848886	3464912	32.615	38.143
5)	L1 AR-1016-3	5.676	4.934	1293049	1838532	36.044	38.265
6)	L1 AR-1016-4	5.775	4.977	908249	1672474	31.355	40.504 #
7)	L1 AR-1016-5	6.072	5.191	1029242	1853614	34.009	35.624
8)	L2 AR-1221-1	4.619	3.865	260263	117709	16.520	4.336 #
9)	L2 AR-1221-2	4.723	3.949	690002	827543	58.431	41.565 #
10)	L2 AR-1221-3	4.788	4.025	1064136	1357694	30.220	22.805
11)	L3 AR-1232-1	4.788	4.025	1064136	1357694	36.199	28.614
12)	L3 AR-1232-2	5.321	4.758	1020089	3464912	65.445	81.684
13)	L3 AR-1232-3	5.614	4.934	1848886	1838532	70.019	82.862
14)	L3 AR-1232-4	5.775	5.019	908249	1920849	68.627	90.974 #
15)	L3 AR-1232-5	5.866	5.191	881030	1853614	77.185	80.864
16)	L4 AR-1242-1	5.592	4.740	1361192	2373243	39.765	42.406
17)	L4 AR-1242-2	5.614	4.758	1848886	3464912	37.678	43.454
18)	L4 AR-1242-3	5.676	4.934	1293049	1838532	41.156	43.139
19)	L4 AR-1242-4	5.775	5.019	908249	1920849	35.417	43.990
20)	L4 AR-1242-5	6.516	5.545	987892	2176373	38.240	43.814
21)	L5 AR-1248-1	5.592	4.740	1361192	2373243	53.632	57.690
22)	L5 AR-1248-2	5.866	4.977	881030	1672474	22.762	27.774
23)	L5 AR-1248-3	6.072	5.019	1029242	1920849	24.363	31.178 #
24)	L5 AR-1248-4	6.476	5.191	983573	1853614	23.624	25.746
25)	L5 AR-1248-5	6.516	5.587	987892	1717682	24.218	26.031
26)	L6 AR-1254-1	6.450	5.545	795045	2176373	17.019	21.481 #
27)	L6 AR-1254-2	6.674	5.693	1009634	732559	14.673	8.298 #
28)	L6 AR-1254-3	7.038	6.099	518036	949771	7.506	6.870
29)	L6 AR-1254-4	7.326	6.329	263107	640421	5.845	7.967 #
30)	L6 AR-1254-5	7.751	6.748	165230	197463	3.516	1.651 #
31)	L7 AR-1260-1	7.216	6.240	133872	532345	2.447	5.375 #
32)	L7 AR-1260-2	7.467	6.427	118671	170522	1.993	1.474 #
33)	L7 AR-1260-3	7.835	6.577	109634	75415	2.786	0.678 #
34)	L7 AR-1260-4	8.052	7.023f	22111	145051	0.498	1.673 #
35)	L7 AR-1260-5	8.364	7.297	45987	65560	0.575	0.356 #
36)	L8 AR-1262-1	7.835	6.839	109634	13657	1.721	0.237 #
37)	L8 AR-1262-2	8.364	7.023f	45987	145051	0.501	1.229 #
38)	L8 AR-1262-3	8.692	7.575	35479	22905	0.551	0.269 #
39)	L8 AR-1262-4	8.786	7.645	87555	100580	2.637	0.666 #
40)	L8 AR-1262-5	9.431	8.141	-4475	91983	N.D.	1.442 #
41)	L9 AR-1268-1	8.683	7.575	46450	22905	0.409	0.094 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
Data File : PP059250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2023 08:40
Operator : YP\AJ
Sample : 03572-07
Misc : AR1242 LOD 40 PPB
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 08:57:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.786	7.645	87555	100580	0.890	0.459 #
43)	L9 AR-1268-3	9.003	7.848	64799	800416	0.699	4.094 #
44)	L9 AR-1268-4	9.431	8.141	-4475	91983	N.D.	1.322 #
45)	L9 AR-1268-5	9.864	8.430	80519	126892	0.297	0.245



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
Data File : PP059250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2023 08:40
Operator : YP\AJ
Sample : 03572-07
Misc : AR1242 LOD 40 PPB
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 08:57:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

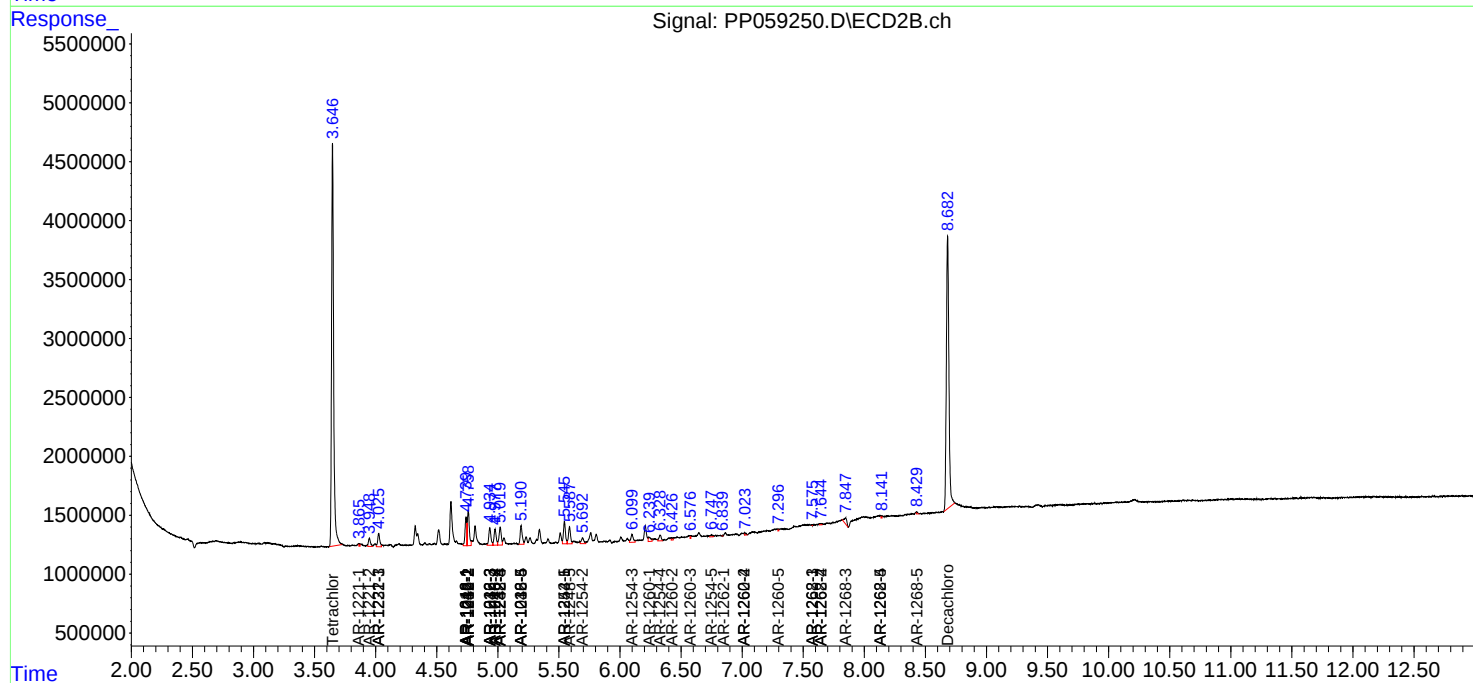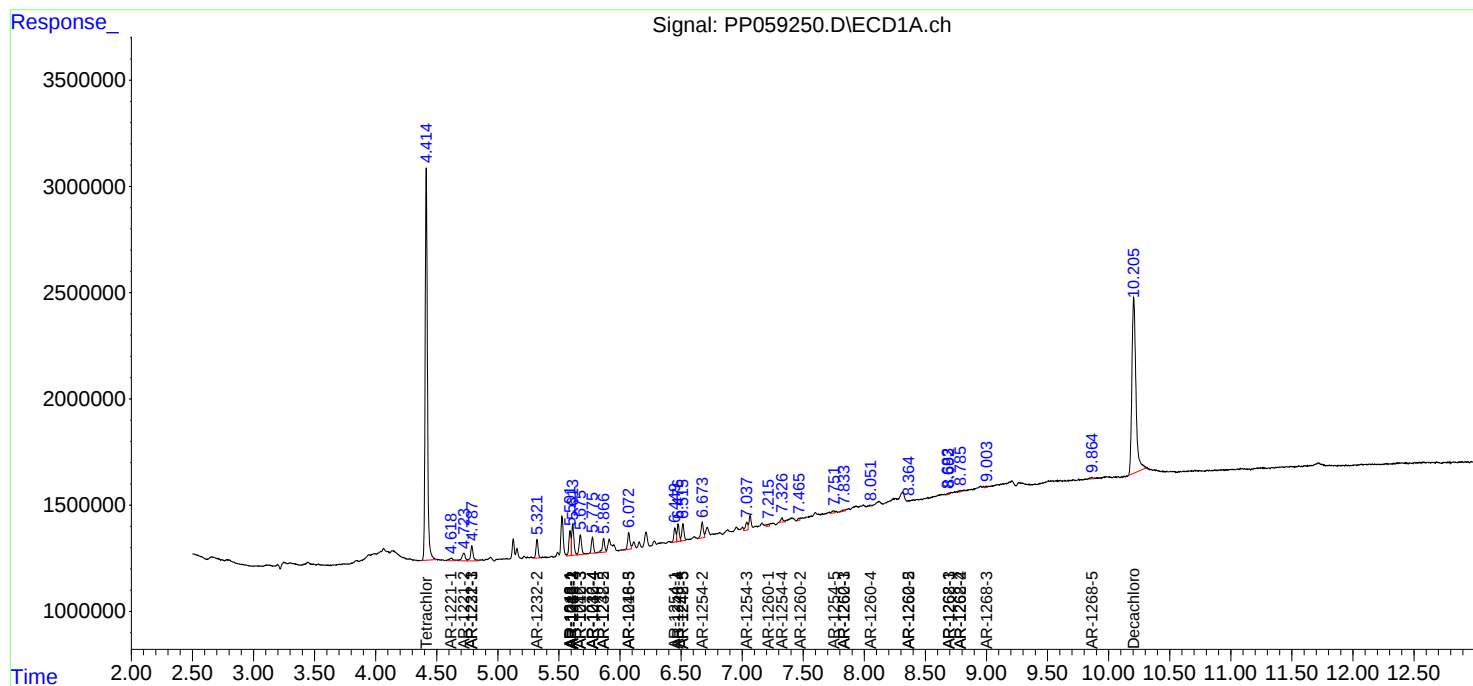


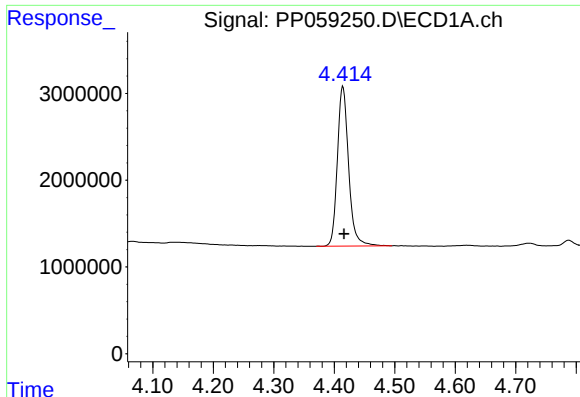

#1 Tetrachloro-m-xylene


R.T.: 4.414 min
Delta R.T.: -0.002 min
Response: 23775241
Conc: 19.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

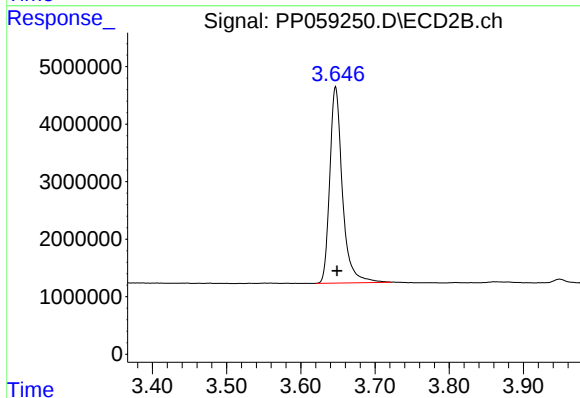


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: -0.002 min
Response: 40286893
Conc: 19.88 ng/ml

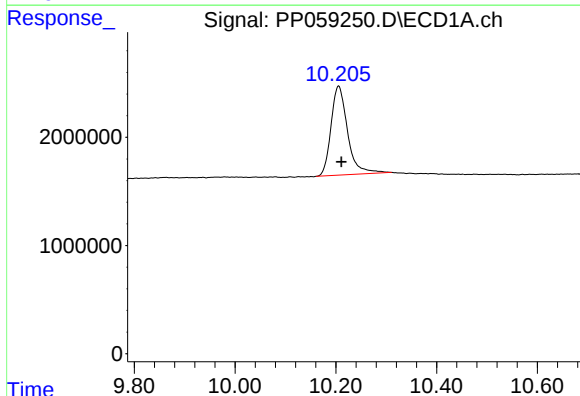


#2 Decachlorobiphenyl

R.T.: 10.206 min
Delta R.T.: -0.006 min
Response: 18795728
Conc: 24.63 ng/ml

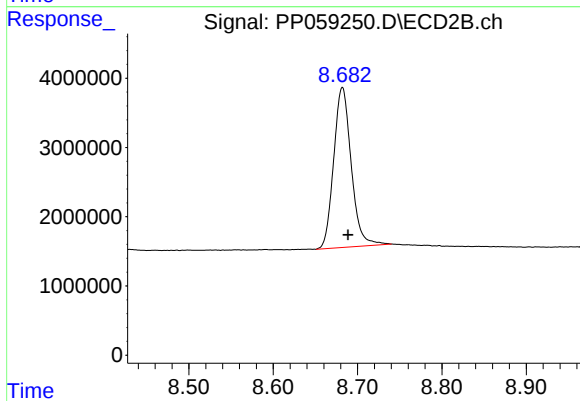

#2 Decachlorobiphenyl


R.T.: 8.682 min
Delta R.T.: -0.006 min
Response: 33446373
Conc: 23.77 ng/ml

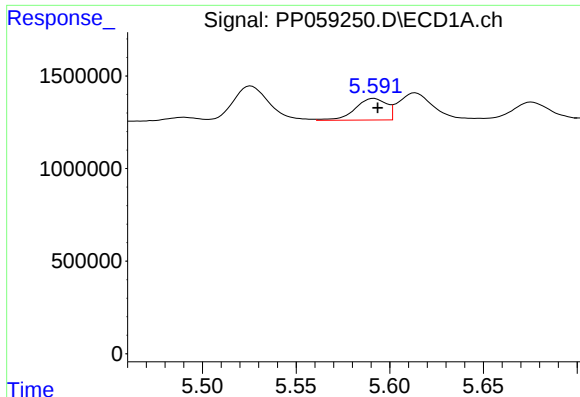

#3 AR-1016-1


R.T.: 5.592 min
Delta R.T.: -0.002 min
Response: 1361192
Conc: 34.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

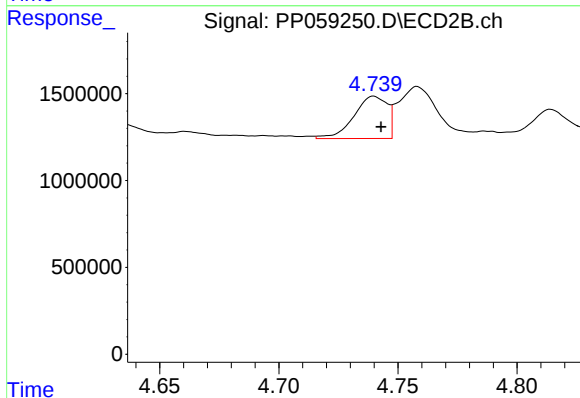


#3 AR-1016-1

R.T.: 4.740 min
Delta R.T.: -0.003 min
Response: 2373243
Conc: 37.00 ng/ml

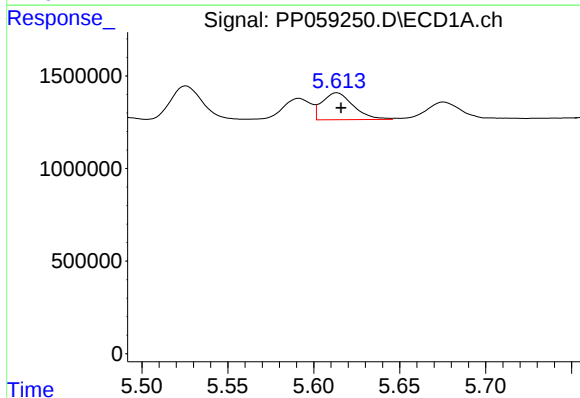


#4 AR-1016-2

R.T.: 5.614 min
Delta R.T.: -0.002 min
Response: 1848886
Conc: 32.62 ng/ml

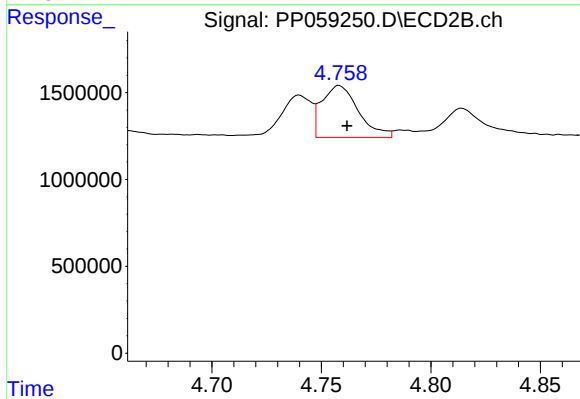

#4 AR-1016-2


R.T.: 4.758 min
Delta R.T.: -0.004 min
Response: 3464912
Conc: 38.14 ng/ml

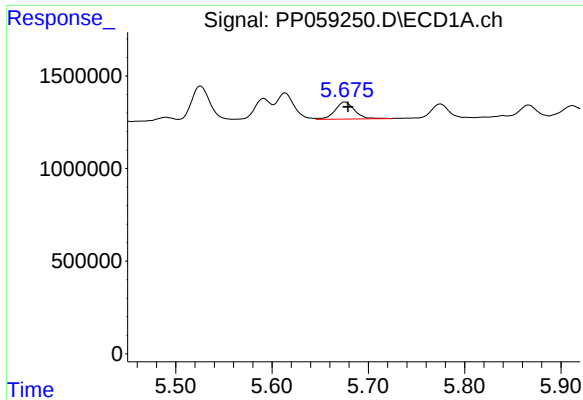

#5 AR-1016-3


R.T.: 5.676 min
Delta R.T.: -0.003 min
Response: 1293049
Conc: 36.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

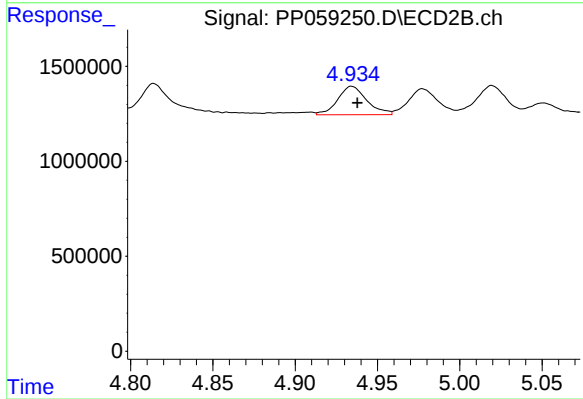


#5 AR-1016-3

R.T.: 4.934 min
Delta R.T.: -0.004 min
Response: 1838532
Conc: 38.26 ng/ml

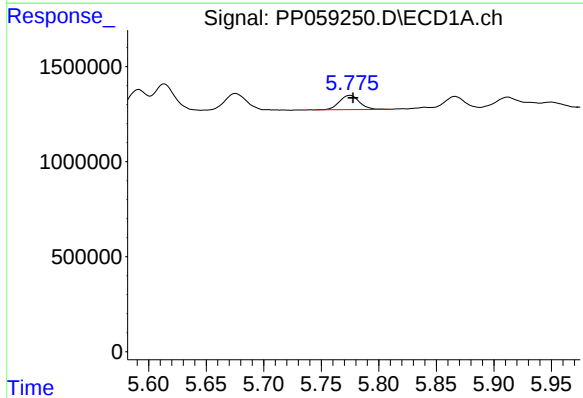


#6 AR-1016-4

R.T.: 5.775 min
Delta R.T.: -0.003 min
Response: 908249
Conc: 31.35 ng/ml

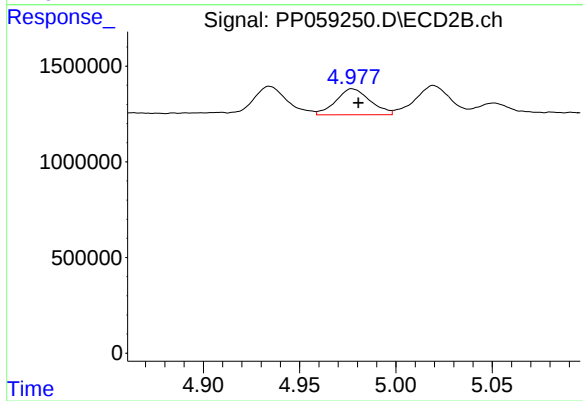

#6 AR-1016-4


R.T.: 4.977 min
Delta R.T.: -0.003 min
Response: 1672474
Conc: 40.50 ng/ml

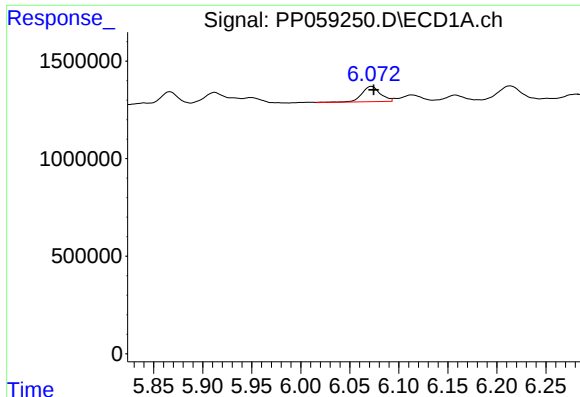

#7 AR-1016-5


R.T.: 6.072 min
Delta R.T.: -0.002 min
Response: 1029242
Conc: 34.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

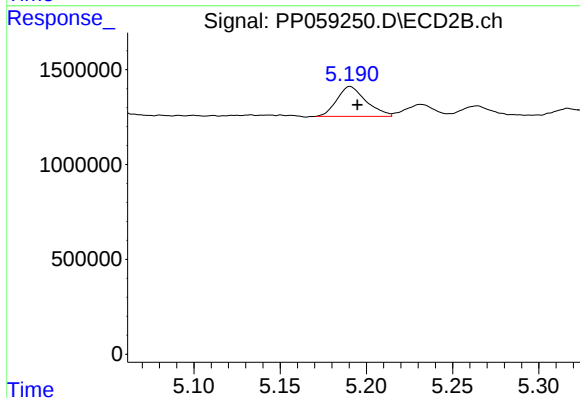


#7 AR-1016-5

R.T.: 5.191 min
Delta R.T.: -0.004 min
Response: 1853614
Conc: 35.62 ng/ml

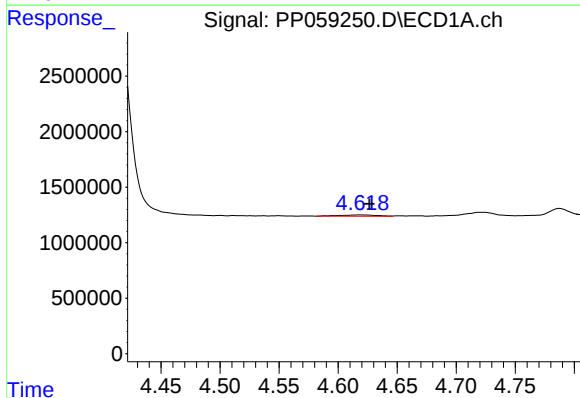


#8 AR-1221-1

R.T.: 4.619 min
Delta R.T.: -0.007 min
Response: 260263
Conc: 16.52 ng/ml

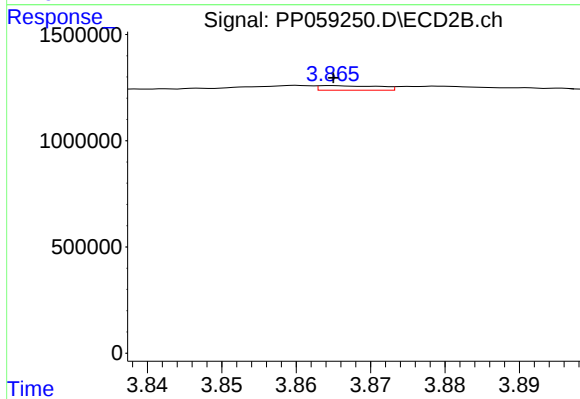

#8 AR-1221-1


R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 117709
Conc: 4.34 ng/ml

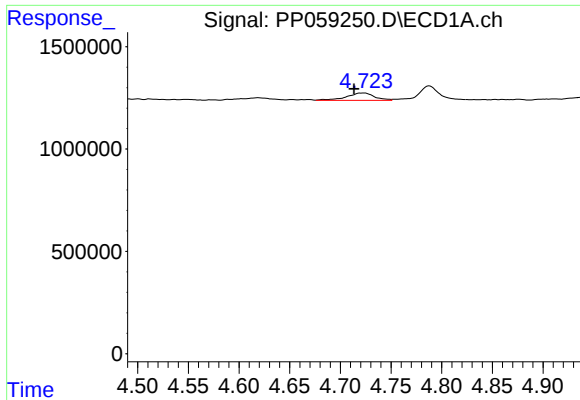

#9 AR-1221-2


R.T.: 4.723 min
Delta R.T.: 0.010 min
Response: 690002
Conc: 58.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

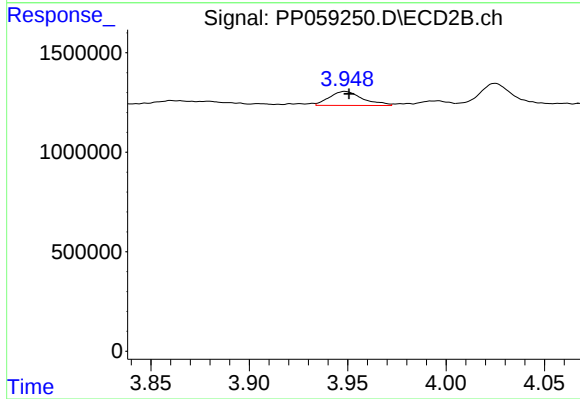


#9 AR-1221-2

R.T.: 3.949 min
Delta R.T.: -0.002 min
Response: 827543
Conc: 41.56 ng/ml

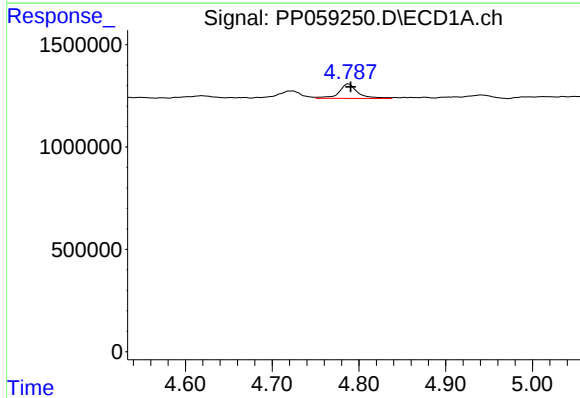


#10 AR-1221-3

R.T.: 4.788 min
Delta R.T.: -0.003 min
Response: 1064136
Conc: 30.22 ng/ml

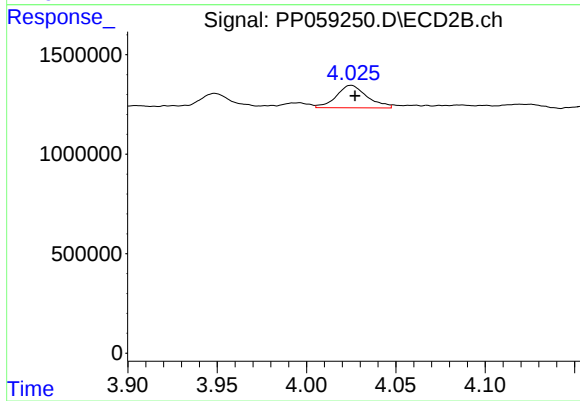

#10 AR-1221-3


R.T.: 4.025 min
Delta R.T.: -0.002 min
Response: 1357694
Conc: 22.81 ng/ml

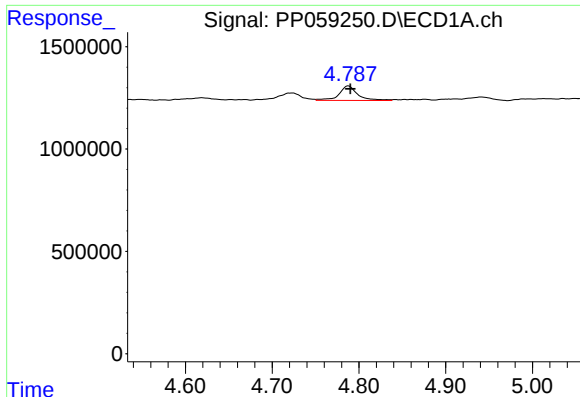

#11 AR-1232-1


R.T.: 4.788 min
Delta R.T.: -0.003 min
Response: 1064136
Conc: 36.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

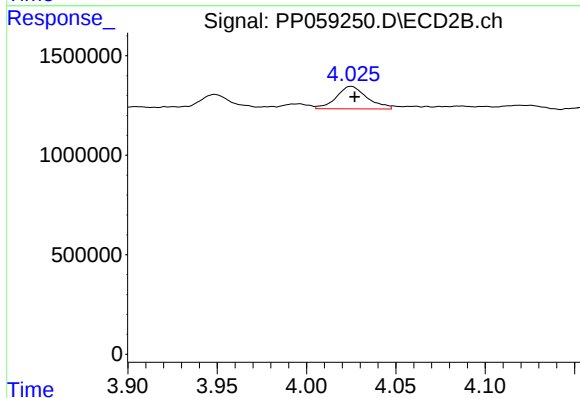


#11 AR-1232-1

R.T.: 4.025 min
Delta R.T.: -0.002 min
Response: 1357694
Conc: 28.61 ng/ml

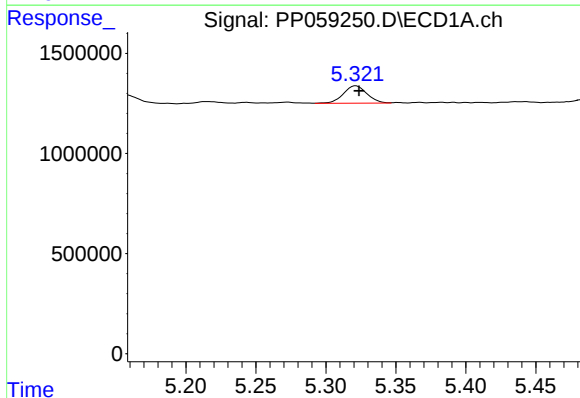


#12 AR-1232-2

R.T.: 5.321 min
Delta R.T.: -0.002 min
Response: 1020089
Conc: 65.44 ng/ml

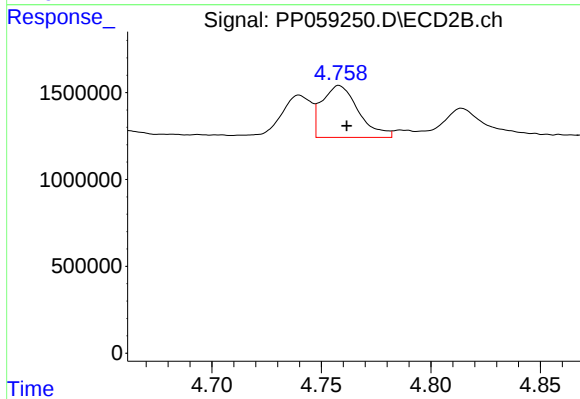

#12 AR-1232-2


R.T.: 4.758 min
Delta R.T.: -0.003 min
Response: 3464912
Conc: 81.68 ng/ml

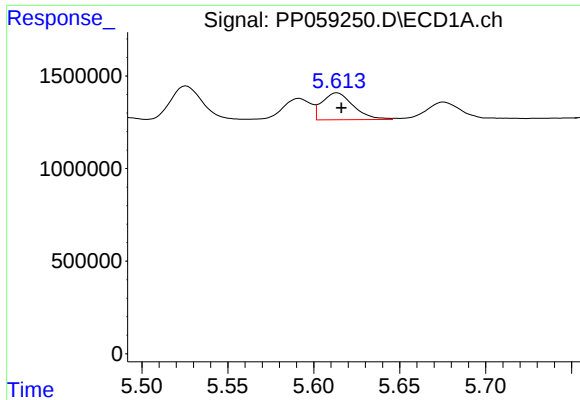

#13 AR-1232-3


R.T.: 5.614 min
Delta R.T.: -0.002 min
Response: 1848886
Conc: 70.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

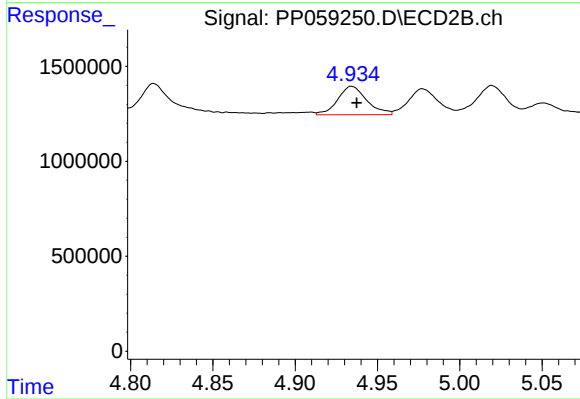


#13 AR-1232-3

R.T.: 4.934 min
Delta R.T.: -0.003 min
Response: 1838532
Conc: 82.86 ng/ml

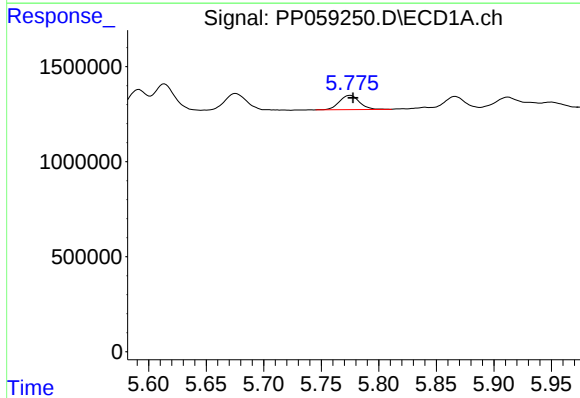


#14 AR-1232-4

R.T.: 5.775 min
Delta R.T.: -0.003 min
Response: 908249
Conc: 68.63 ng/ml

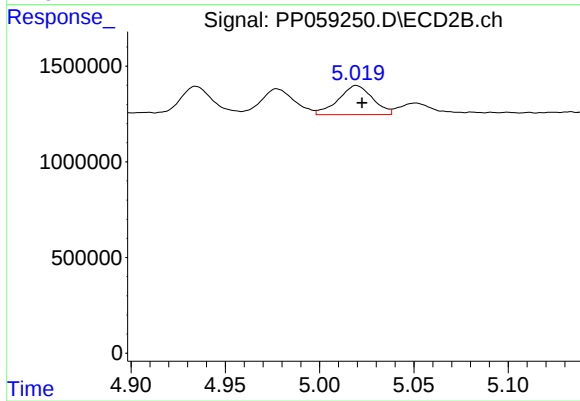

#14 AR-1232-4


R.T.: 5.019 min
Delta R.T.: -0.003 min
Response: 1920849
Conc: 90.97 ng/ml

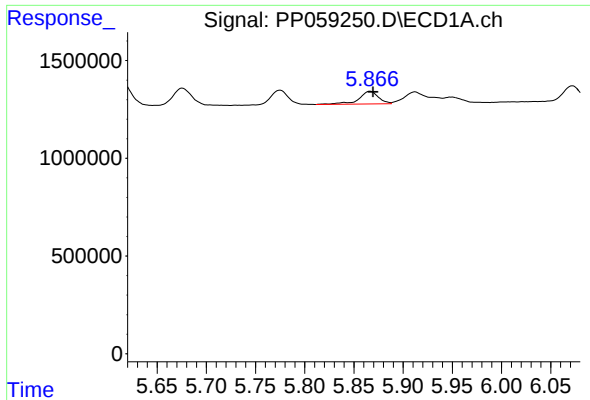

#15 AR-1232-5


R.T.: 5.866 min
Delta R.T.: -0.003 min
Response: 881030
Conc: 77.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

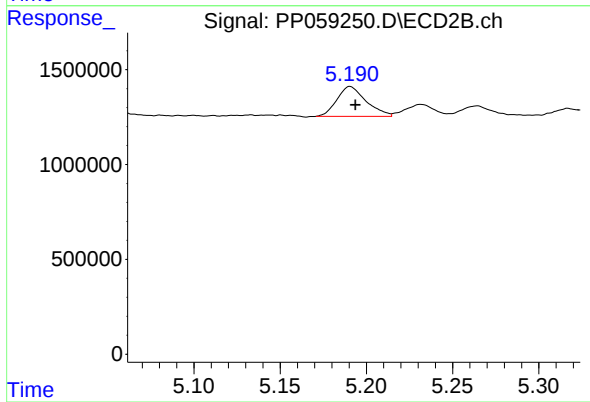


#15 AR-1232-5

R.T.: 5.191 min
Delta R.T.: -0.003 min
Response: 1853614
Conc: 80.86 ng/ml

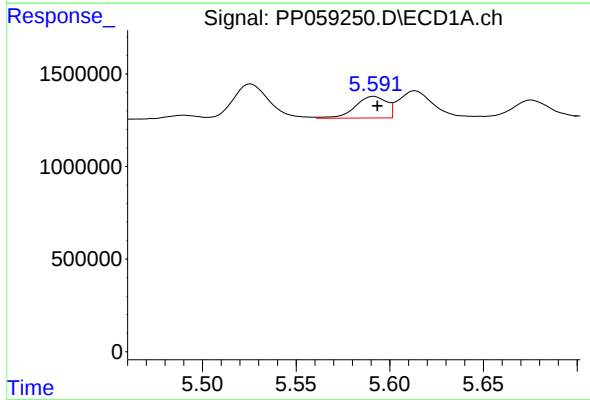


#16 AR-1242-1

R.T.: 5.592 min
Delta R.T.: -0.002 min
Response: 1361192
Conc: 39.76 ng/ml

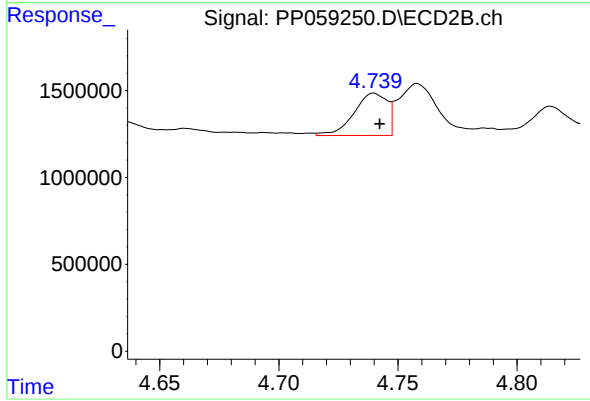

#16 AR-1242-1


R.T.: 4.740 min
Delta R.T.: -0.002 min
Response: 2373243
Conc: 42.41 ng/ml

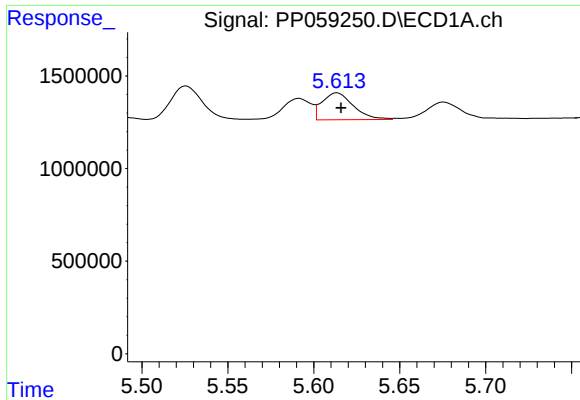

#17 AR-1242-2


R.T.: 5.614 min
Delta R.T.: -0.002 min
Response: 1848886
Conc: 37.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

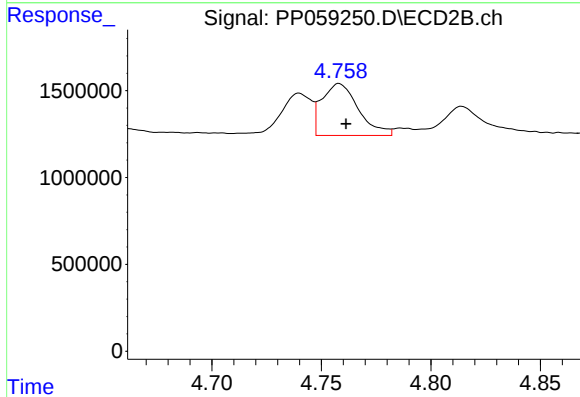


#17 AR-1242-2

R.T.: 4.758 min
Delta R.T.: -0.003 min
Response: 3464912
Conc: 43.45 ng/ml

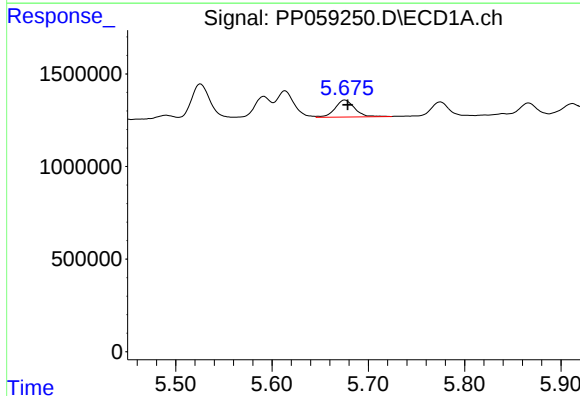


#18 AR-1242-3

R.T.: 5.676 min
Delta R.T.: -0.003 min
Response: 1293049
Conc: 41.16 ng/ml

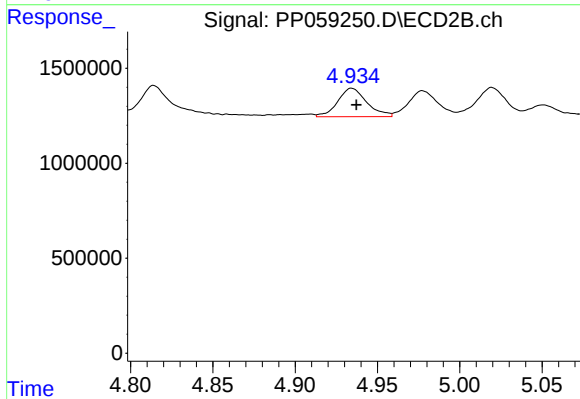

#18 AR-1242-3


R.T.: 4.934 min
Delta R.T.: -0.003 min
Response: 1838532
Conc: 43.14 ng/ml

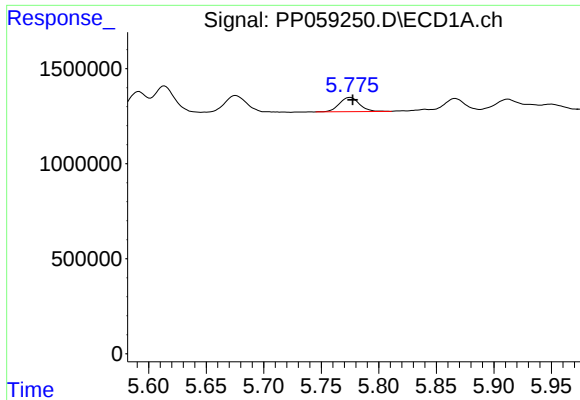

#19 AR-1242-4


R.T.: 5.775 min
Delta R.T.: -0.002 min
Response: 908249
Conc: 35.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

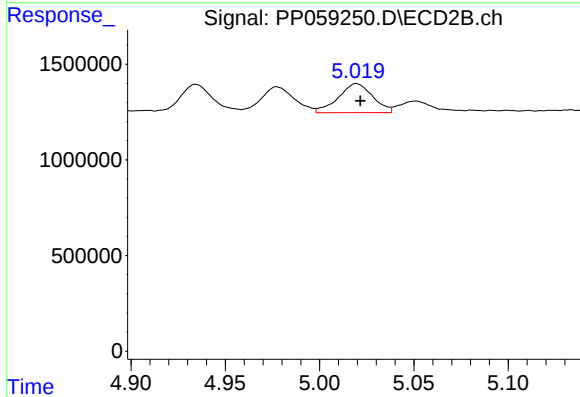


#19 AR-1242-4

R.T.: 5.019 min
Delta R.T.: -0.002 min
Response: 1920849
Conc: 43.99 ng/ml

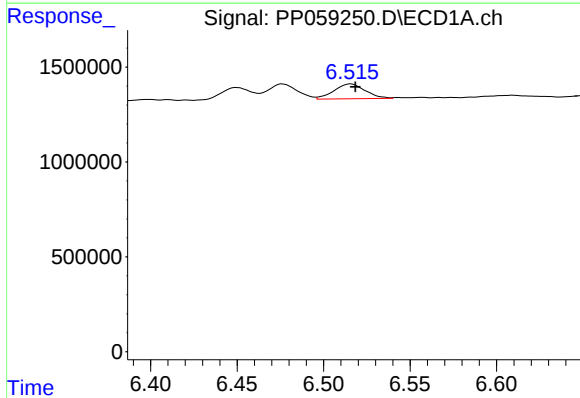


#20 AR-1242-5

R.T.: 6.516 min
Delta R.T.: -0.003 min
Response: 987892
Conc: 38.24 ng/ml

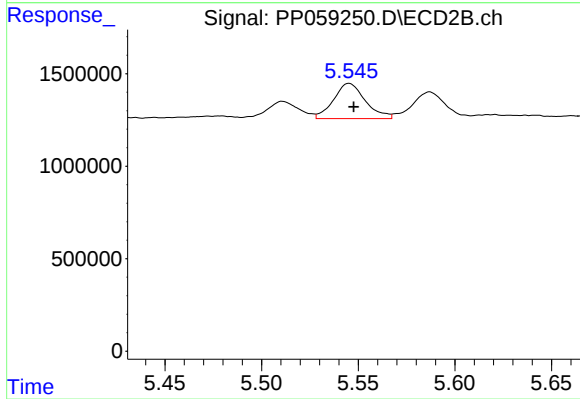

#20 AR-1242-5


R.T.: 5.545 min
Delta R.T.: -0.002 min
Response: 2176373
Conc: 43.81 ng/ml

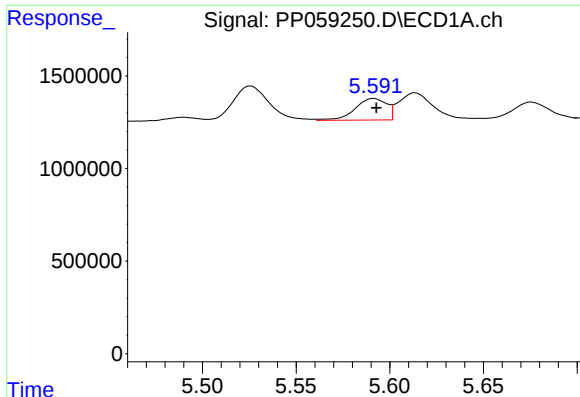

#21 AR-1248-1


R.T.: 5.592 min
Delta R.T.: -0.001 min
Response: 1361192
Conc: 53.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

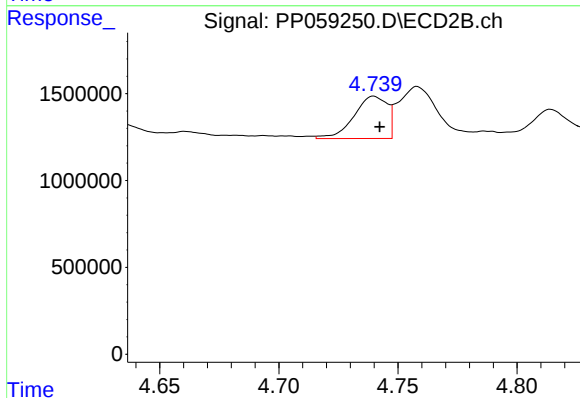


#21 AR-1248-1

R.T.: 4.740 min
Delta R.T.: -0.003 min
Response: 2373243
Conc: 57.69 ng/ml

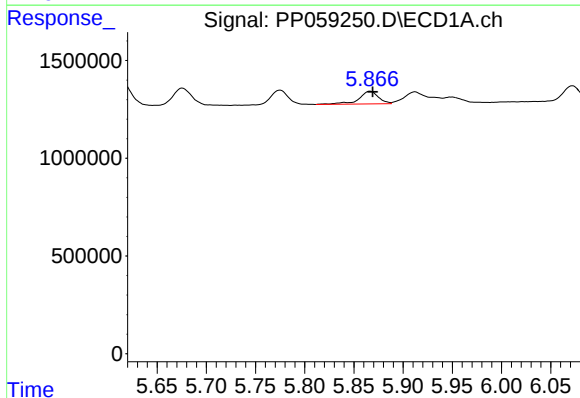


#22 AR-1248-2

R.T.: 5.866 min
Delta R.T.: -0.003 min
Response: 881030
Conc: 22.76 ng/ml

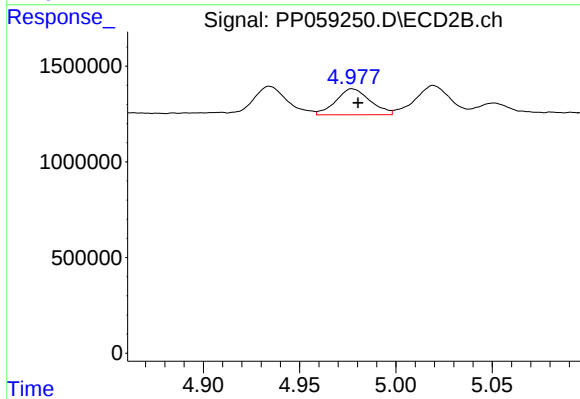

#22 AR-1248-2


R.T.: 4.977 min
Delta R.T.: -0.003 min
Response: 1672474
Conc: 27.77 ng/ml

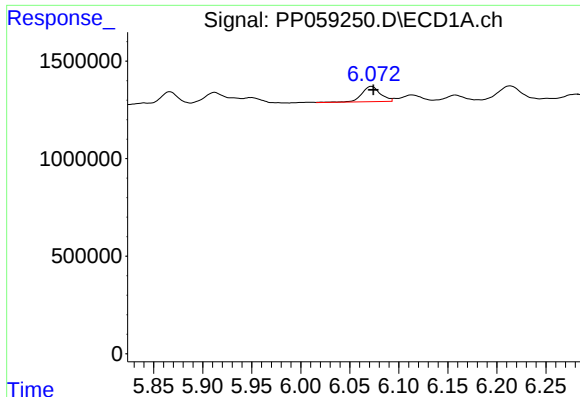

#23 AR-1248-3


R.T.: 6.072 min
Delta R.T.: -0.002 min
Response: 1029242
Conc: 24.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

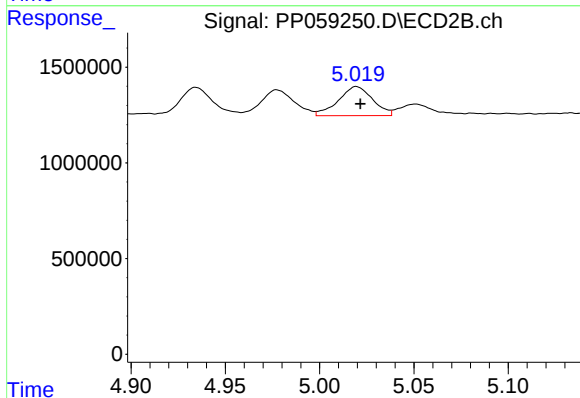


#23 AR-1248-3

R.T.: 5.019 min
Delta R.T.: -0.002 min
Response: 1920849
Conc: 31.18 ng/ml

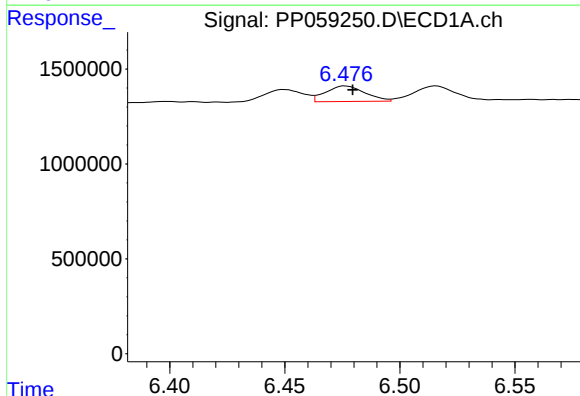


#24 AR-1248-4

R.T.: 6.476 min
Delta R.T.: -0.003 min
Response: 983573
Conc: 23.62 ng/ml

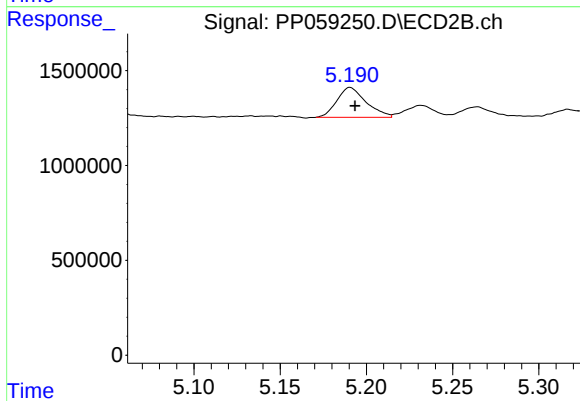

#24 AR-1248-4


R.T.: 5.191 min
Delta R.T.: -0.003 min
Response: 1853614
Conc: 25.75 ng/ml

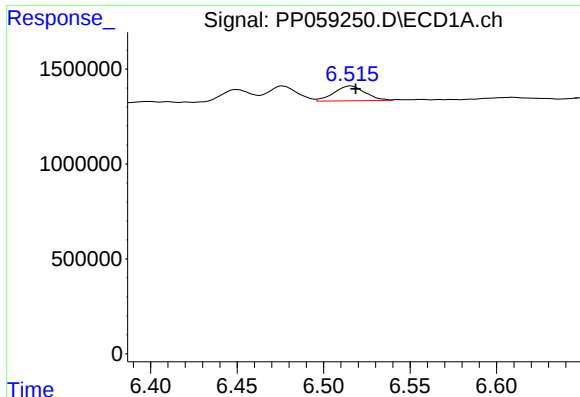

#25 AR-1248-5


R.T.: 6.516 min
Delta R.T.: -0.003 min
Response: 987892
Conc: 24.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

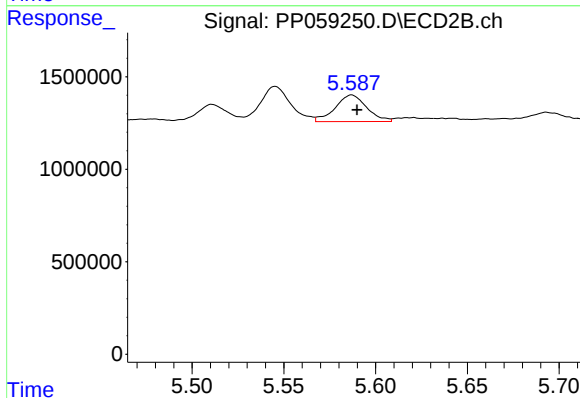


#25 AR-1248-5

R.T.: 5.587 min
Delta R.T.: -0.003 min
Response: 1717682
Conc: 26.03 ng/ml

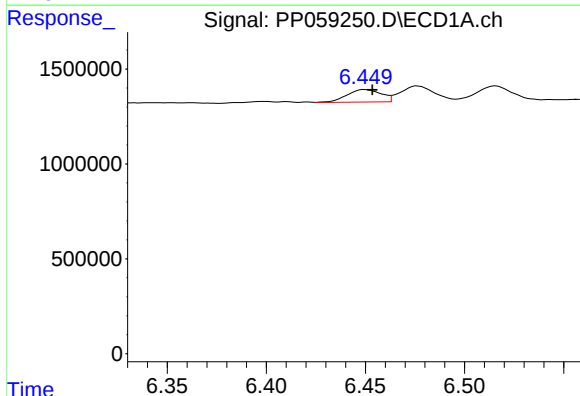


#26 AR-1254-1

R.T.: 6.450 min
Delta R.T.: -0.004 min
Response: 795045
Conc: 17.02 ng/ml

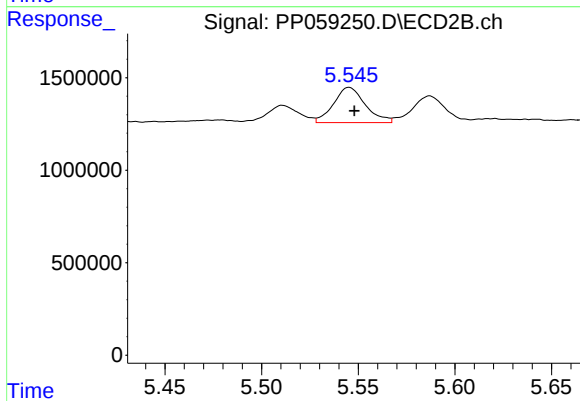

#26 AR-1254-1


R.T.: 5.545 min
Delta R.T.: -0.003 min
Response: 2176373
Conc: 21.48 ng/ml

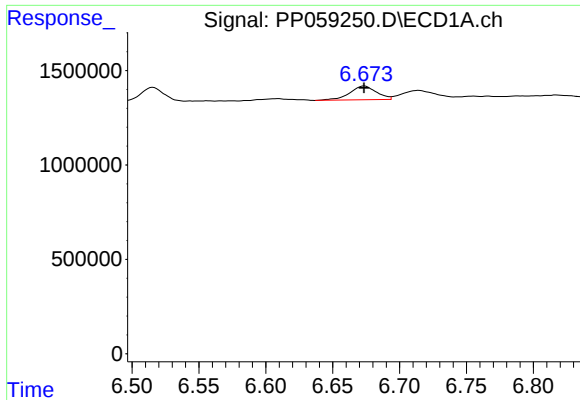

#27 AR-1254-2


R.T.: 6.674 min
Delta R.T.: 0.000 min
Response: 1009634
Conc: 14.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

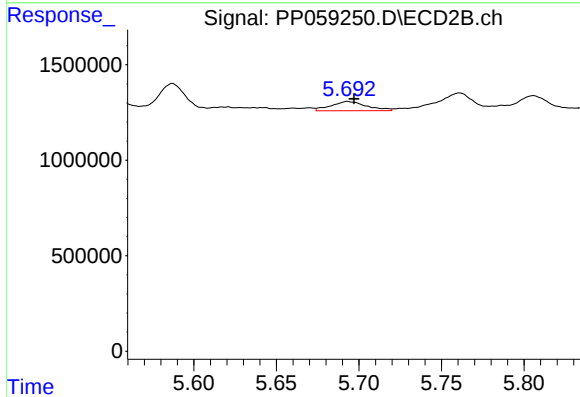


#27 AR-1254-2

R.T.: 5.693 min
Delta R.T.: -0.004 min
Response: 732559
Conc: 8.30 ng/ml

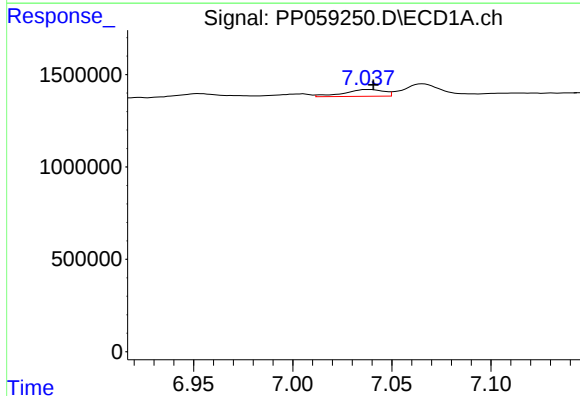


#28 AR-1254-3

R.T.: 7.038 min
Delta R.T.: -0.003 min
Response: 518036
Conc: 7.51 ng/ml

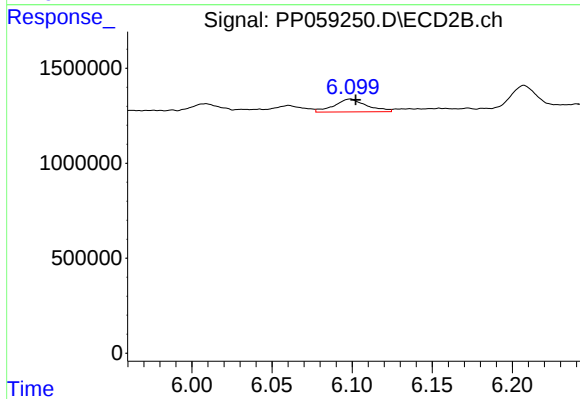

#28 AR-1254-3


R.T.: 6.099 min
Delta R.T.: -0.003 min
Response: 949771
Conc: 6.87 ng/ml

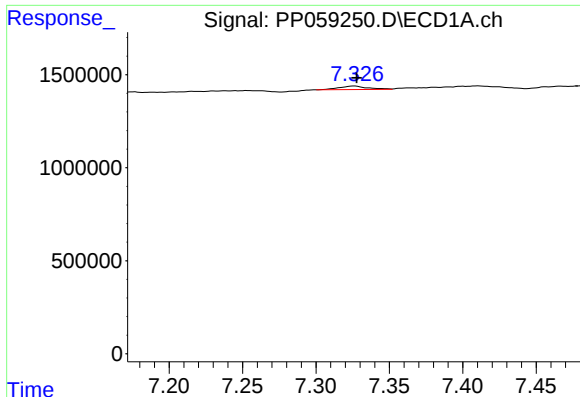

#29 AR-1254-4


R.T.: 7.326 min
Delta R.T.: -0.001 min
Response: 263107
Conc: 5.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

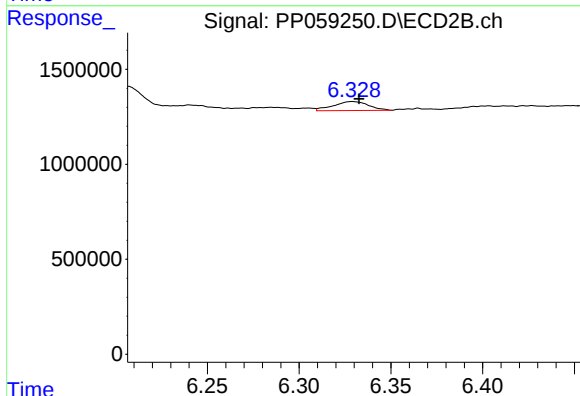


#29 AR-1254-4

R.T.: 6.329 min
Delta R.T.: -0.004 min
Response: 640421
Conc: 7.97 ng/ml

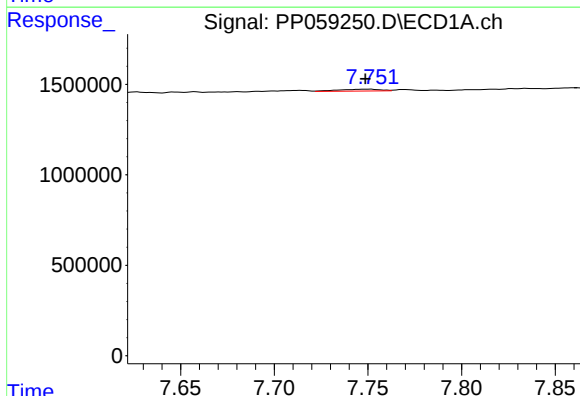


#30 AR-1254-5

R.T.: 7.751 min
Delta R.T.: 0.002 min
Response: 165230
Conc: 3.52 ng/ml

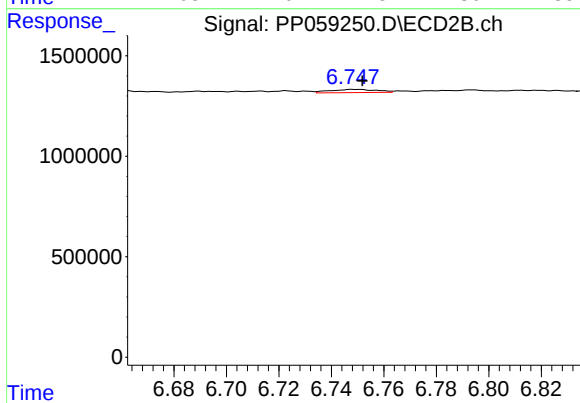

#30 AR-1254-5


R.T.: 6.748 min
Delta R.T.: -0.004 min
Response: 197463
Conc: 1.65 ng/ml

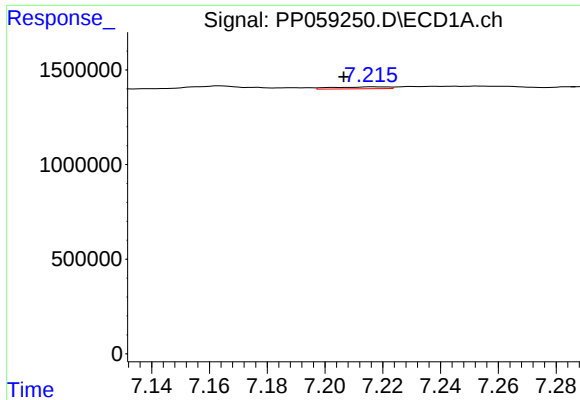

#31 AR-1260-1


R.T.: 7.216 min
Delta R.T.: 0.010 min
Response: 133872
Conc: 2.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

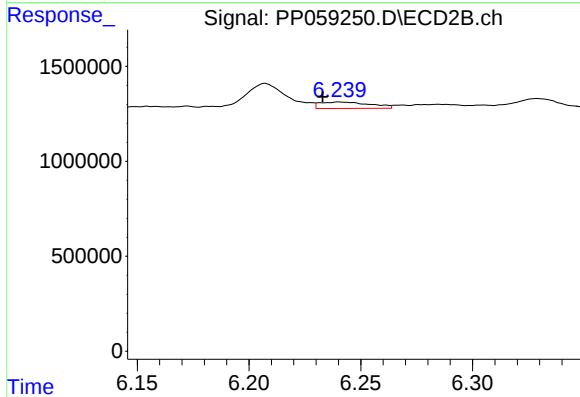


#31 AR-1260-1

R.T.: 6.240 min
Delta R.T.: 0.007 min
Response: 532345
Conc: 5.38 ng/ml

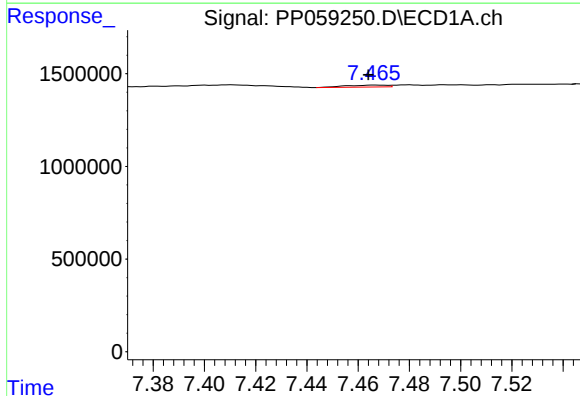


#32 AR-1260-2

R.T.: 7.467 min
Delta R.T.: 0.003 min
Response: 118671
Conc: 1.99 ng/ml

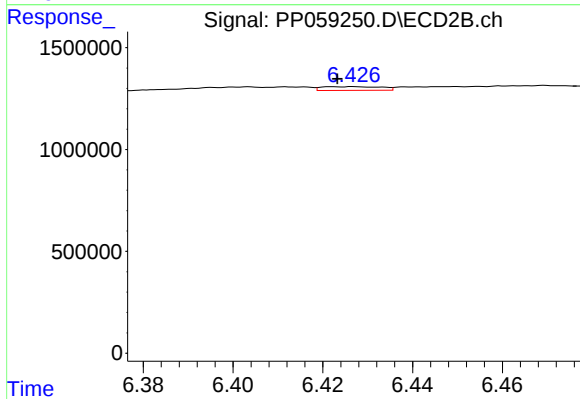

#32 AR-1260-2


R.T.: 6.427 min
Delta R.T.: 0.004 min
Response: 170522
Conc: 1.47 ng/ml

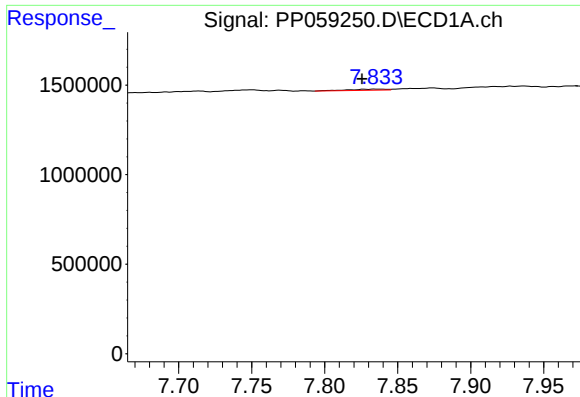

#33 AR-1260-3


R.T.: 7.835 min
Delta R.T.: 0.009 min
Response: 109634
Conc: 2.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

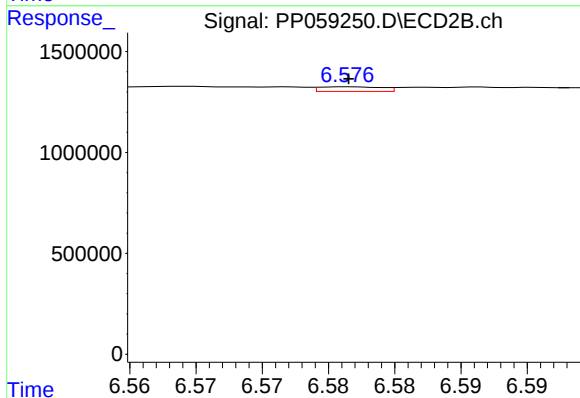


#33 AR-1260-3

R.T.: 6.577 min
Delta R.T.: 0.000 min
Response: 75415
Conc: 0.68 ng/ml

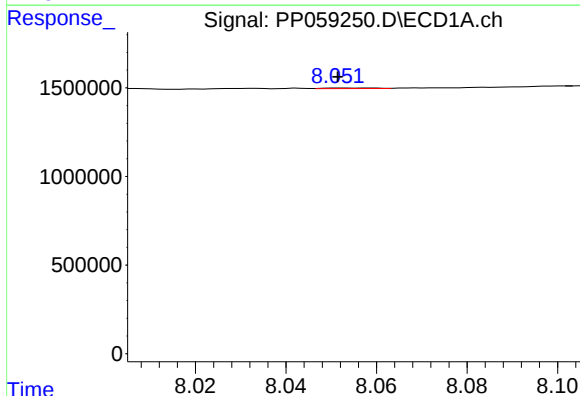


#34 AR-1260-4

R.T.: 8.052 min
Delta R.T.: 0.000 min
Response: 22111
Conc: 0.50 ng/ml

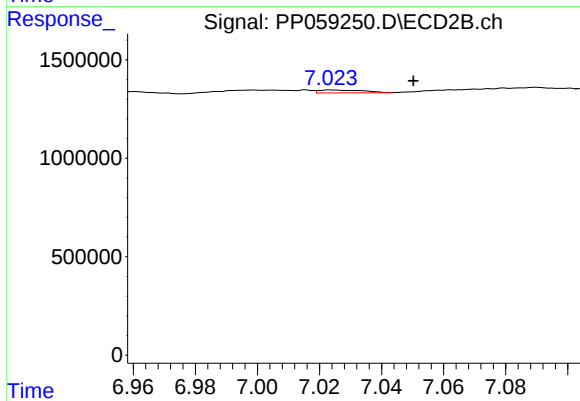

#34 AR-1260-4


R.T.: 7.023 min
Delta R.T.: -0.027 min
Response: 145051
Conc: 1.67 ng/ml

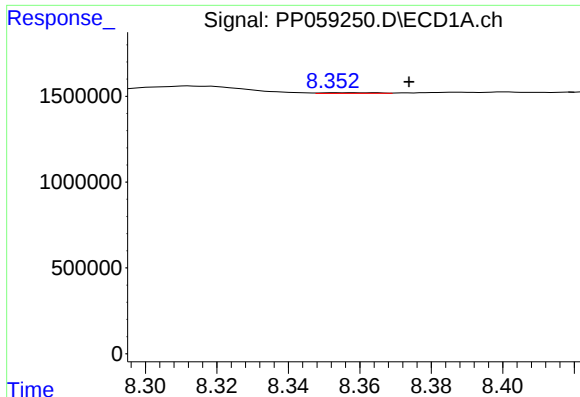

#35 AR-1260-5


R.T.: 8.364 min
Delta R.T.: -0.010 min
Response: 45987
Conc: 0.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

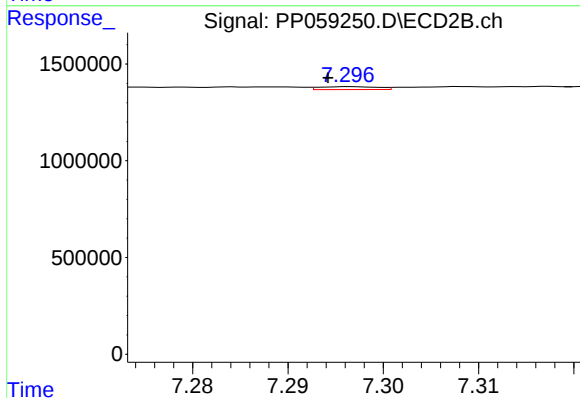


#35 AR-1260-5

R.T.: 7.297 min
Delta R.T.: 0.002 min
Response: 65560
Conc: 0.36 ng/ml

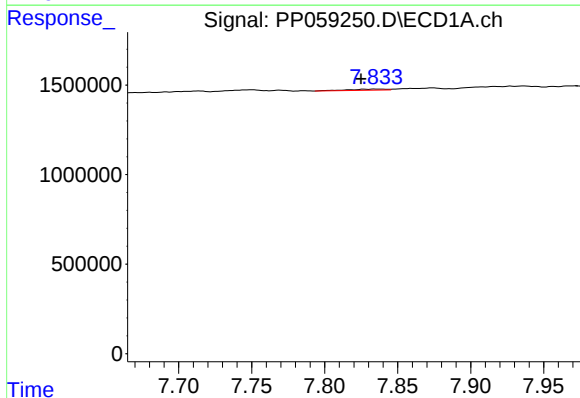


#36 AR-1262-1

R.T.: 7.835 min
Delta R.T.: 0.010 min
Response: 109634
Conc: 1.72 ng/ml

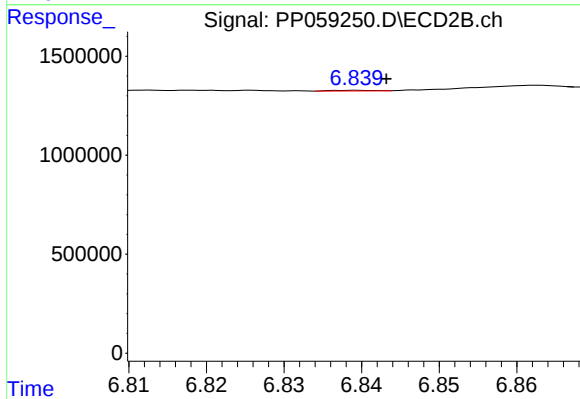

#36 AR-1262-1


R.T.: 6.839 min
Delta R.T.: -0.004 min
Response: 13657
Conc: 0.24 ng/ml

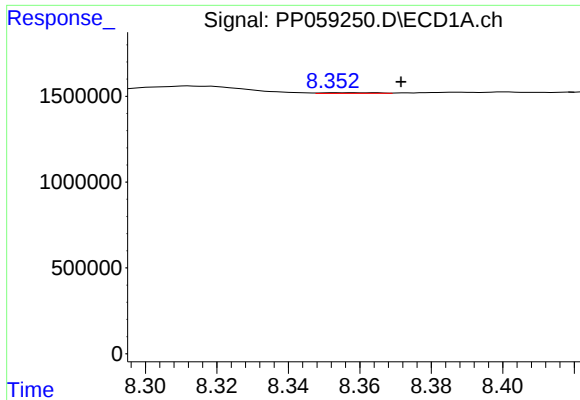

#37 AR-1262-2


R.T.: 8.364 min
Delta R.T.: -0.007 min
Response: 45987
Conc: 0.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

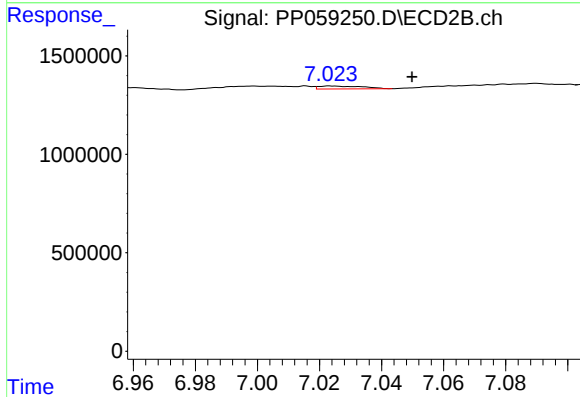


#37 AR-1262-2

R.T.: 7.023 min
Delta R.T.: -0.026 min
Response: 145051
Conc: 1.23 ng/ml

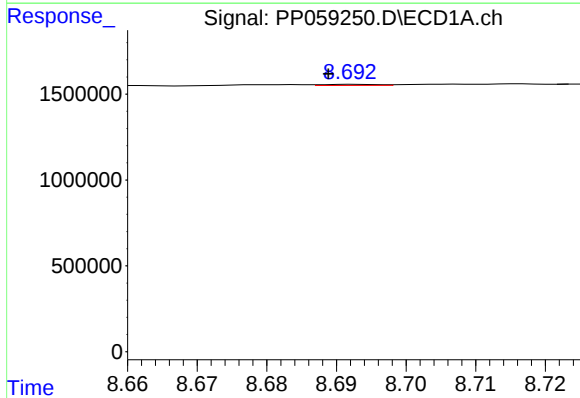


#38 AR-1262-3

R.T.: 8.692 min
Delta R.T.: 0.003 min
Response: 35479
Conc: 0.55 ng/ml

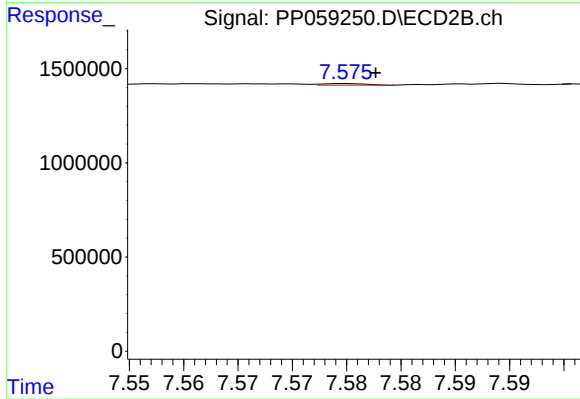

#38 AR-1262-3


R.T.: 7.575 min
Delta R.T.: -0.003 min
Response: 22905
Conc: 0.27 ng/ml

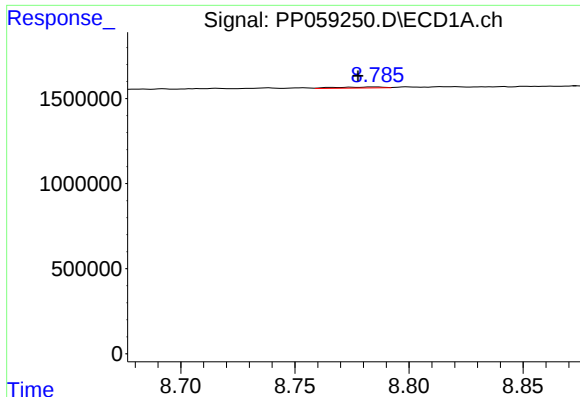

#39 AR-1262-4


R.T.: 8.786 min
Delta R.T.: 0.008 min
Response: 87555
Conc: 2.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

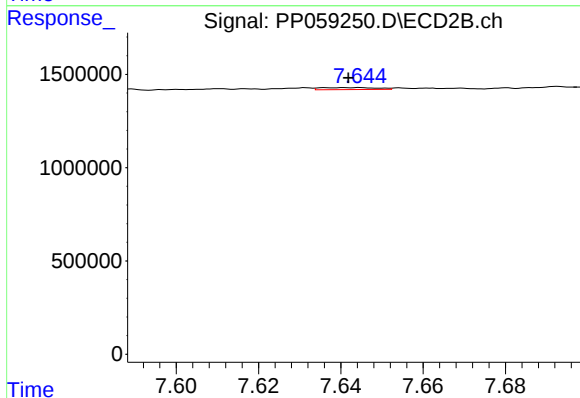


#39 AR-1262-4

R.T.: 7.645 min
Delta R.T.: 0.003 min
Response: 100580
Conc: 0.67 ng/ml

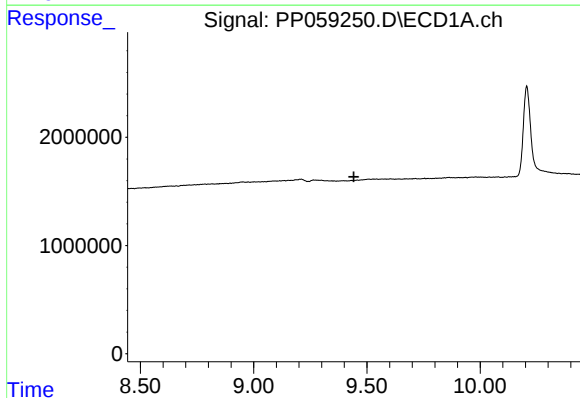


#40 AR-1262-5

R.T.: 9.431 min
Delta R.T.: -0.011 min
Response: -4475
Conc: N.D.

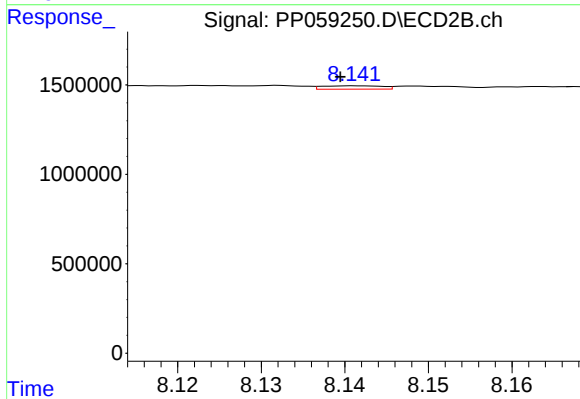

#40 AR-1262-5


R.T.: 8.141 min
Delta R.T.: 0.002 min
Response: 91983
Conc: 1.44 ng/ml

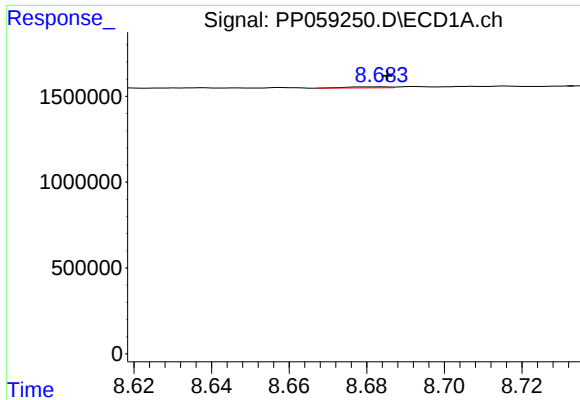

#41 AR-1268-1


R.T.: 8.683 min
Delta R.T.: -0.002 min
Response: 46450
Conc: 0.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

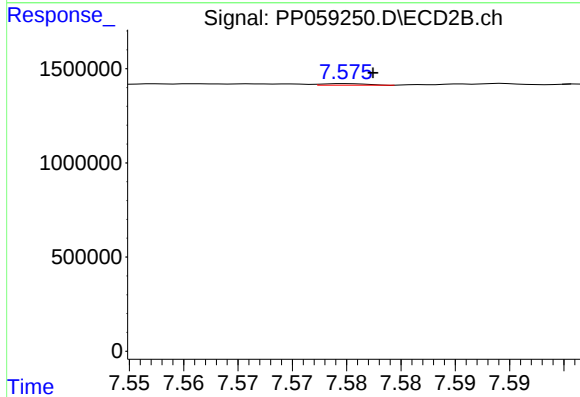


#41 AR-1268-1

R.T.: 7.575 min
Delta R.T.: -0.002 min
Response: 22905
Conc: 0.09 ng/ml

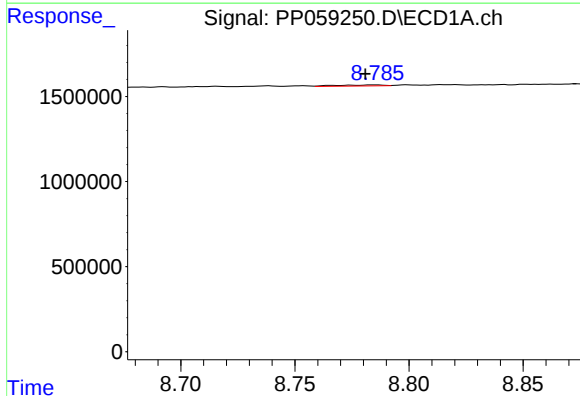


#42 AR-1268-2

R.T.: 8.786 min
Delta R.T.: 0.005 min
Response: 87555
Conc: 0.89 ng/ml

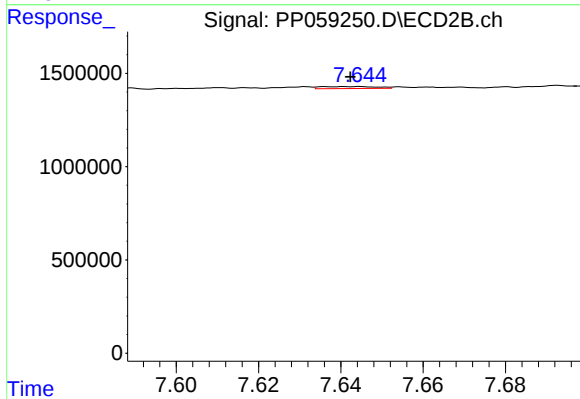

#42 AR-1268-2


R.T.: 7.645 min
Delta R.T.: 0.002 min
Response: 100580
Conc: 0.46 ng/ml

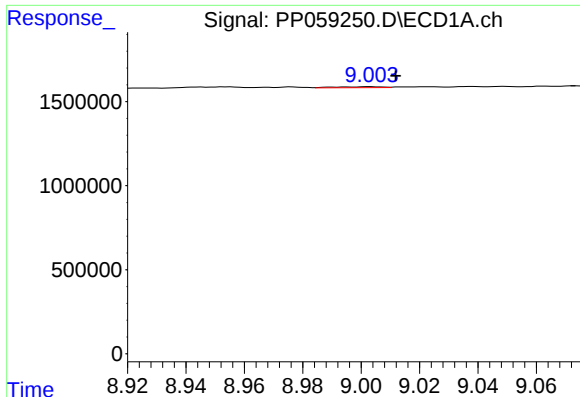

#43 AR-1268-3


R.T.: 9.003 min
Delta R.T.: -0.009 min
Response: 64799
Conc: 0.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

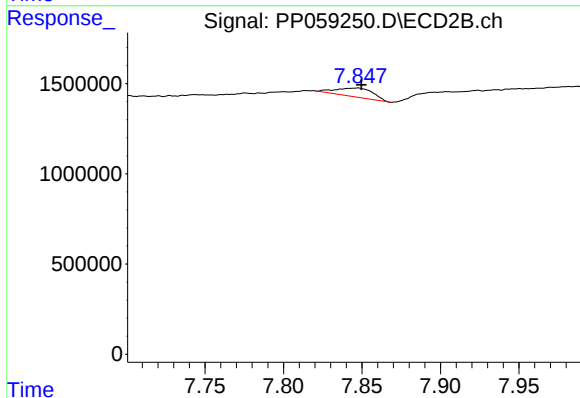


#43 AR-1268-3

R.T.: 7.848 min
Delta R.T.: -0.002 min
Response: 800416
Conc: 4.09 ng/ml

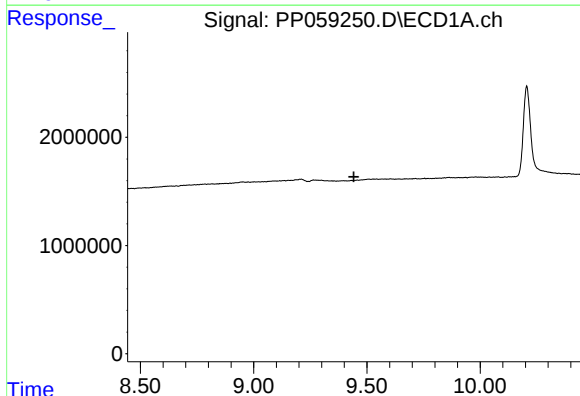


#44 AR-1268-4

R.T.: 9.431 min
Delta R.T.: -0.011 min
Response: -4475
Conc: N.D.

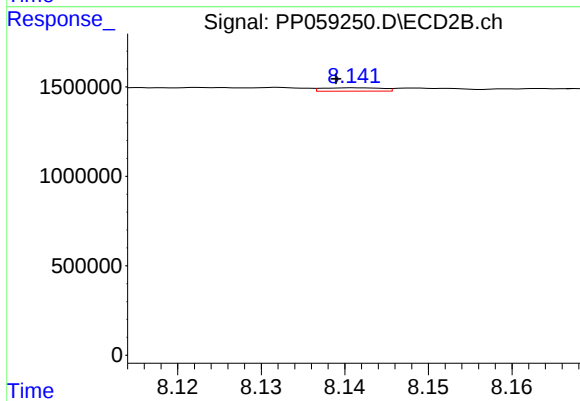

#44 AR-1268-4


R.T.: 8.141 min
Delta R.T.: 0.003 min
Response: 91983
Conc: 1.32 ng/ml

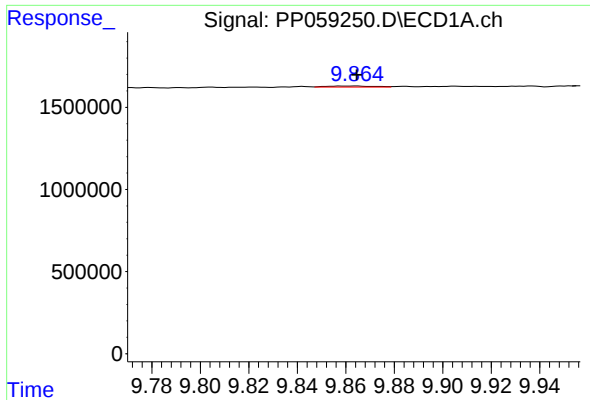

#45 AR-1268-5

R.T.: 9.864 min
Delta R.T.: 0.000 min
Response: 80519
Conc: 0.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

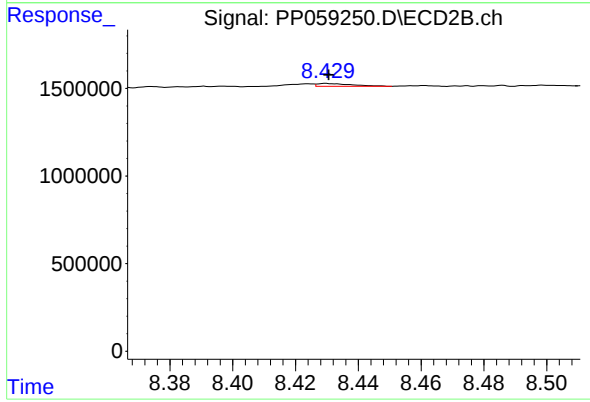

#45 AR-1268-5

R.T.: 8.430 min
Delta R.T.: 0.000 min
Response: 126892
Conc: 0.24 ng/ml