

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
 Data File : PP059252.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2023 09:13
 Operator : YP\AJ
 Sample : 03572-07
 Misc : AR1254 LOD 40 PPB
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 09:25:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.415	3.647	22712876	38731165	18.510	19.116
2)	SA Decachlor...	10.208	8.683	18181638	32208080	23.822	22.894
Target Compounds							
3)	L1 AR-1016-1	5.593	4.743	104777	275255	2.667	4.292 #
4)	L1 AR-1016-2	5.619	4.754	134772	293124	2.377	3.227 #
5)	L1 AR-1016-3	5.671	4.934	131560	78294	3.667	1.630 #
6)	L1 AR-1016-4	5.778	4.978	9351	2061028	0.323	49.914 #
7)	L1 AR-1016-5	6.071	5.190	672429	1087856	22.219	20.907
8)	L2 AR-1221-1	4.630	3.863	58087	23328	3.687	0.859 #
9)	L2 AR-1221-2	4.725	3.949	529026	717333	44.799	36.029
10)	L2 AR-1221-3	4.787	4.029	201167	83911	5.713	1.409 #
11)	L3 AR-1232-1	4.787	4.029	201167	83911	6.843	1.768 #
12)	L3 AR-1232-2	5.329	4.754	69451	293124	4.456	6.910 #
13)	L3 AR-1232-3	5.619	4.934	134772	78294	5.104	3.529 #
14)	L3 AR-1232-4	5.778	5.019	9351	798211	0.707	37.804 #
15)	L3 AR-1232-5	5.867	5.190	1011823	1087856	88.643	47.458 #
16)	L4 AR-1242-1	5.593	4.743	104777	275255	3.061	4.918 #
17)	L4 AR-1242-2	5.619	4.754	134772	293124	2.747	3.676 #
18)	L4 AR-1242-3	5.671	4.934	131560	78294	4.187	1.837 #
19)	L4 AR-1242-4	5.778	5.019	9351	798211	0.365	18.280 #
20)	L4 AR-1242-5	6.519	5.546	586165	4385827	22.689	88.294 #
21)	L5 AR-1248-1	5.593	4.743	104777	275255	4.128	6.691 #
22)	L5 AR-1248-2	5.867	4.978	1011823	2061028	26.142	34.226 #
23)	L5 AR-1248-3	6.071	5.019	672429	798211	15.917	12.956
24)	L5 AR-1248-4	6.477	5.190	874782	1087856	21.011	15.110 #
25)	L5 AR-1248-5	6.519	5.586	586165	531569	14.370	8.056 #
26)	L6 AR-1254-1	6.452	5.546	1970388	4385827	42.179	43.289
27)	L6 AR-1254-2	6.672	5.694	2990970	3717642	43.468	42.113
28)	L6 AR-1254-3	7.039	6.099	3141409	5535366	45.514	40.040
29)	L6 AR-1254-4	7.326	6.329	1917697	3142060	42.601	39.090
30)	L6 AR-1254-5	7.746	6.749	2070968	4873070	44.075	40.749
31)	L7 AR-1260-1	7.205	6.230	1274993	2810706	23.305	28.380
32)	L7 AR-1260-2	7.462	6.420	1167895	2414818	19.616	20.870
33)	L7 AR-1260-3	7.825	6.572	76814	2741452	1.952	24.646 #
34)	L7 AR-1260-4	8.035	7.041	543544	65946	12.238	0.761 #
35)	L7 AR-1260-5	8.370	7.288	257781	806273	3.223	4.374 #
36)	L8 AR-1262-1	7.825	6.841	76814	82156	1.206	1.428
37)	L8 AR-1262-2	8.370	7.041	257781	65946	2.807	0.559 #
38)	L8 AR-1262-3	8.699	7.571	194848	51200	3.028	0.602 #
39)	L8 AR-1262-4	8.783	7.637	31610	543382	0.952	3.597 #
40)	L8 AR-1262-5	9.442	8.138	43945	101549	1.473	1.592
41)	L9 AR-1268-1	8.699	7.571	194848	51200	1.716	0.210 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
 Data File : PP059252.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2023 09:13
 Operator : YP\AJ
 Sample : 03572-07
 Misc : AR1254 LOD 40 PPB
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 09:25:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.783	7.637	31610	543382	0.321	2.481 #
43) L9	AR-1268-3	9.008	7.852	105094	294258	1.134	1.505 #
44) L9	AR-1268-4	9.442	8.138	43945	101549	1.378	1.459
45) L9	AR-1268-5	9.872	8.426	20497	181248	0.076	0.350 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
Data File : PP059252.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2023 09:13
Operator : YP\AJ
Sample : 03572-07
Misc : AR1254 LOD 40 PPB
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 09:25:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

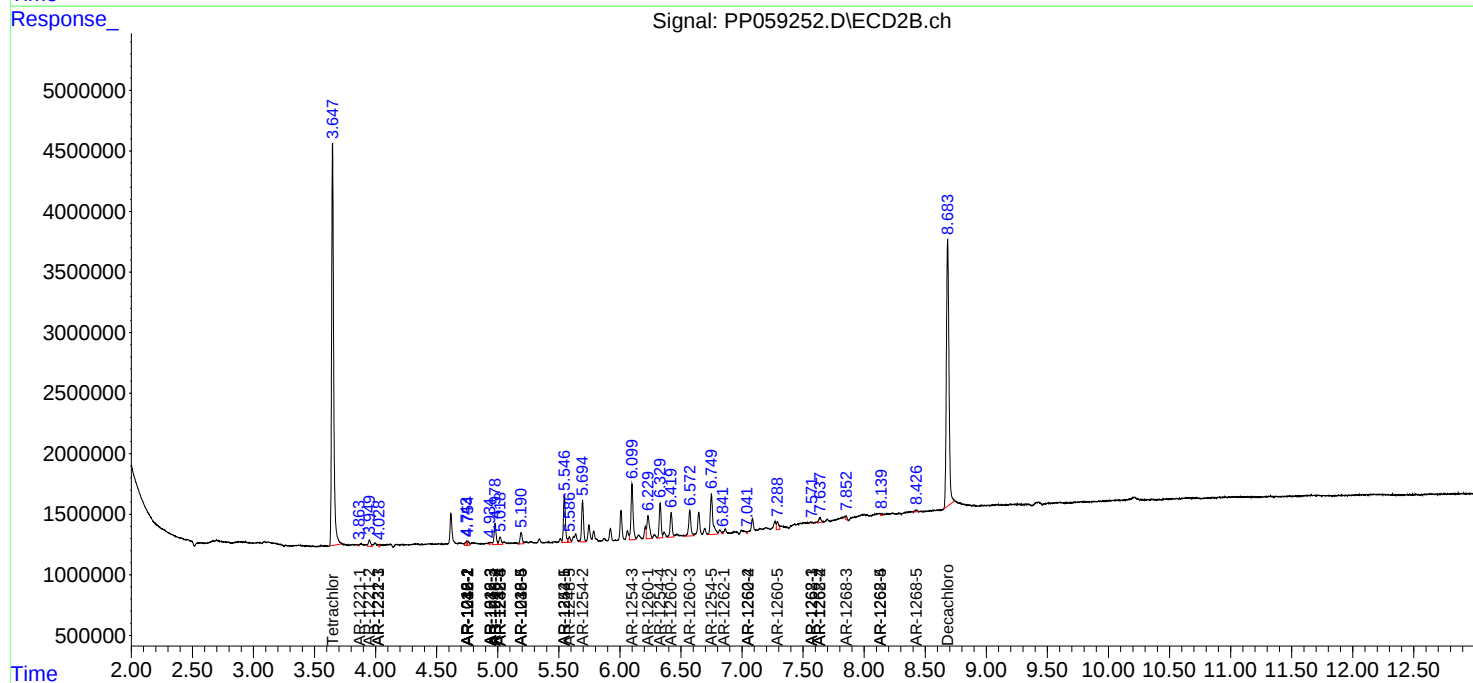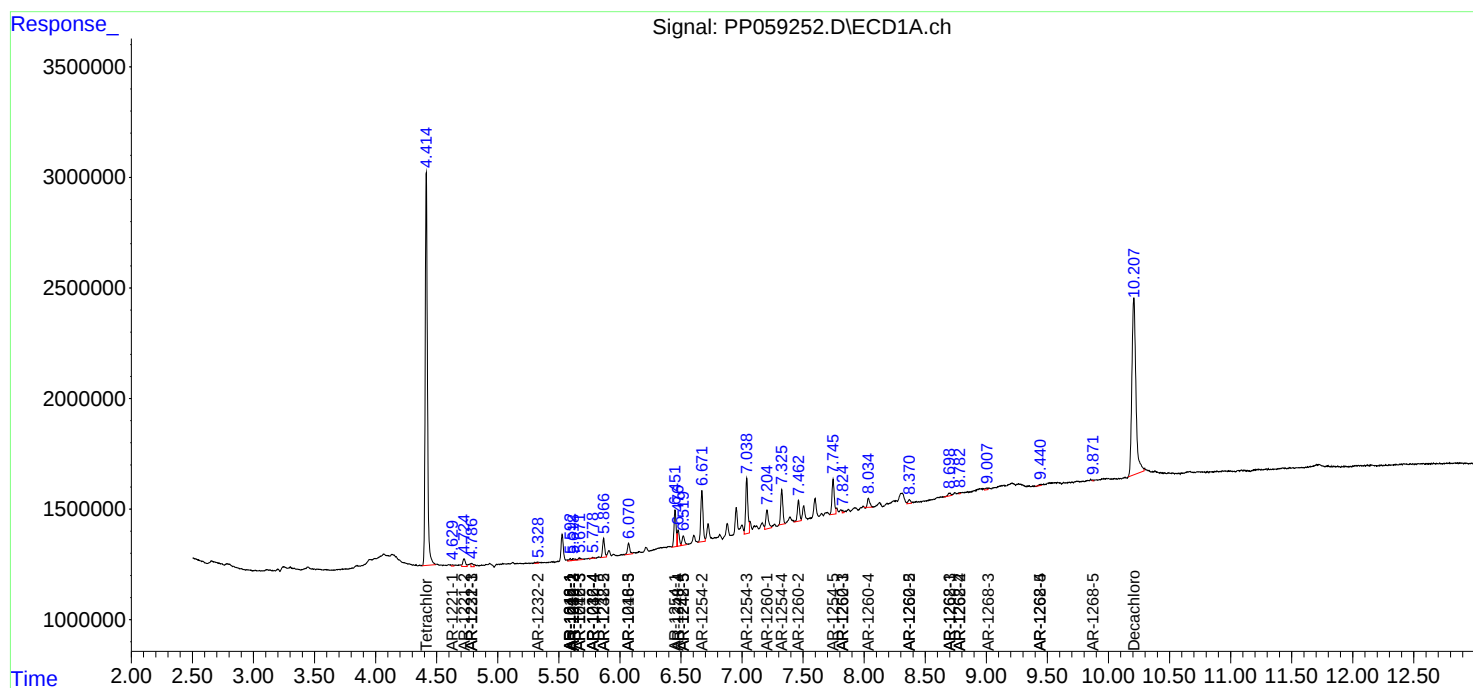


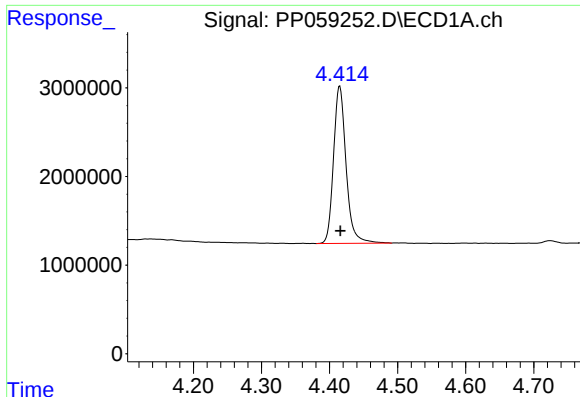

#1 Tetrachloro-m-xylene


R.T.: 4.415 min
Delta R.T.: -0.001 min
Response: 22712876
Conc: 18.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

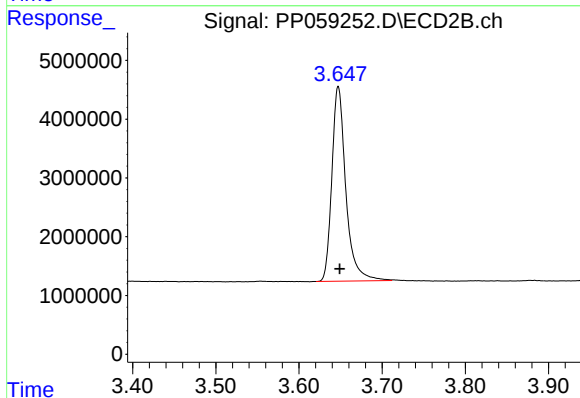


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: -0.002 min
Response: 38731165
Conc: 19.12 ng/ml

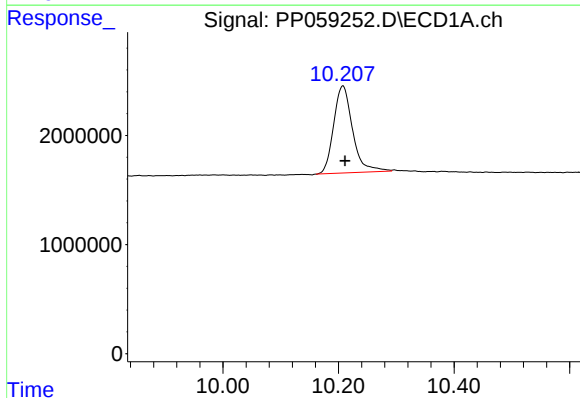


#2 Decachlorobiphenyl

R.T.: 10.208 min
Delta R.T.: -0.004 min
Response: 18181638
Conc: 23.82 ng/ml

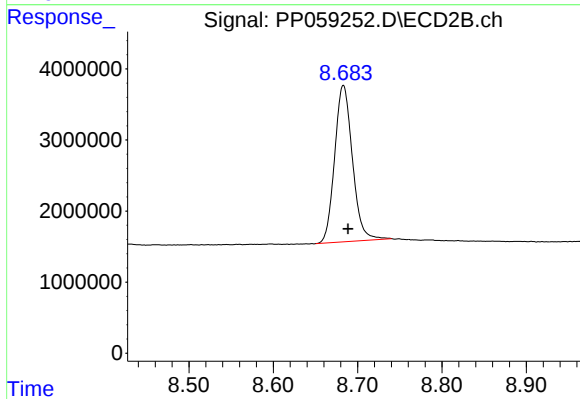

#2 Decachlorobiphenyl


R.T.: 8.683 min
Delta R.T.: -0.005 min
Response: 32208080
Conc: 22.89 ng/ml

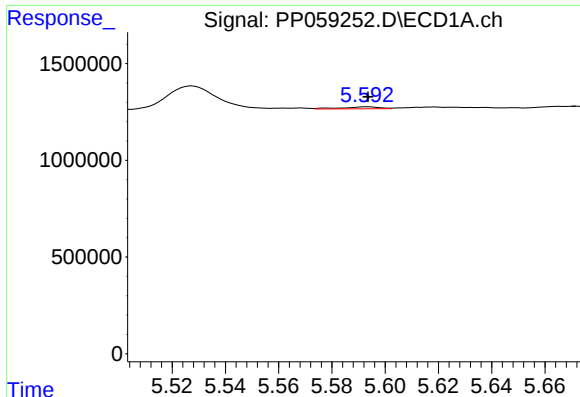

#3 AR-1016-1


R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 104777
Conc: 2.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

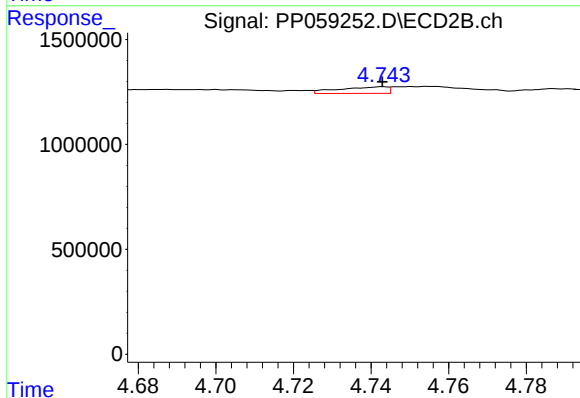


#3 AR-1016-1

R.T.: 4.743 min
Delta R.T.: 0.000 min
Response: 275255
Conc: 4.29 ng/ml

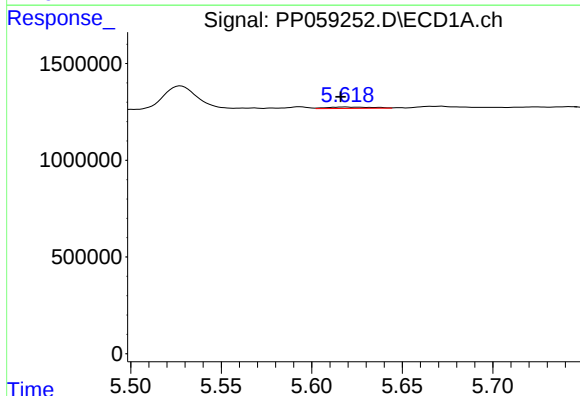


#4 AR-1016-2

R.T.: 5.619 min
Delta R.T.: 0.003 min
Response: 134772
Conc: 2.38 ng/ml

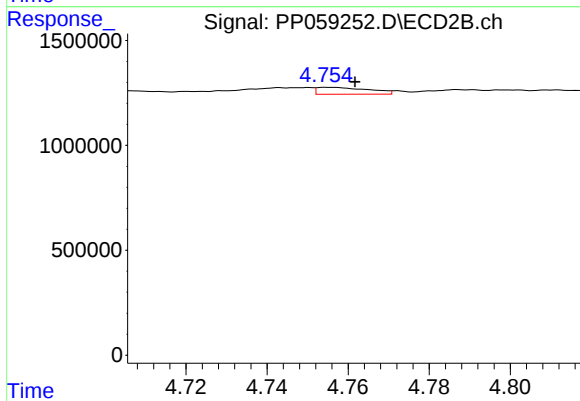

#4 AR-1016-2


R.T.: 4.754 min
Delta R.T.: -0.007 min
Response: 293124
Conc: 3.23 ng/ml

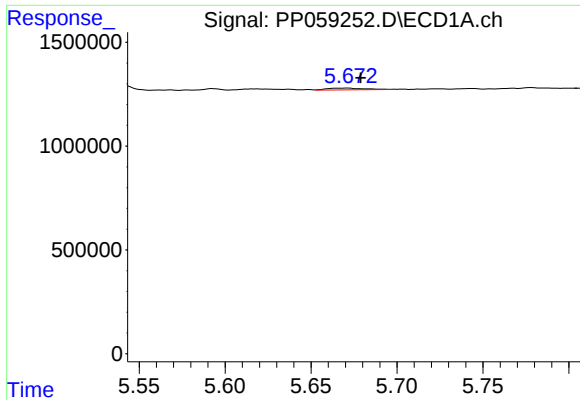

#5 AR-1016-3


R.T.: 5.671 min
Delta R.T.: -0.007 min
Response: 131560
Conc: 3.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

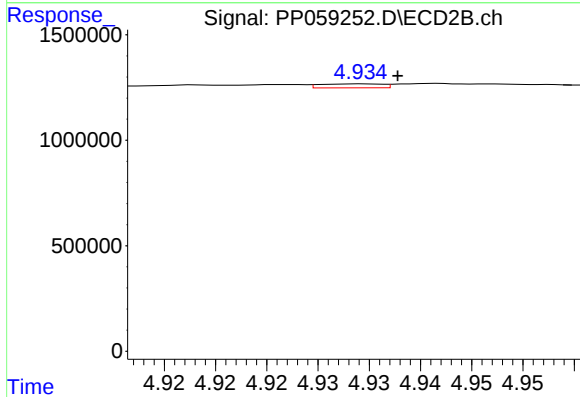


#5 AR-1016-3

R.T.: 4.934 min
Delta R.T.: -0.004 min
Response: 78294
Conc: 1.63 ng/ml

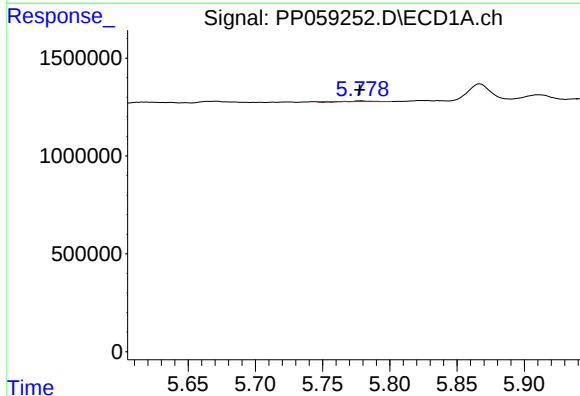


#6 AR-1016-4

R.T.: 5.778 min
Delta R.T.: 0.000 min
Response: 9351
Conc: 0.32 ng/ml

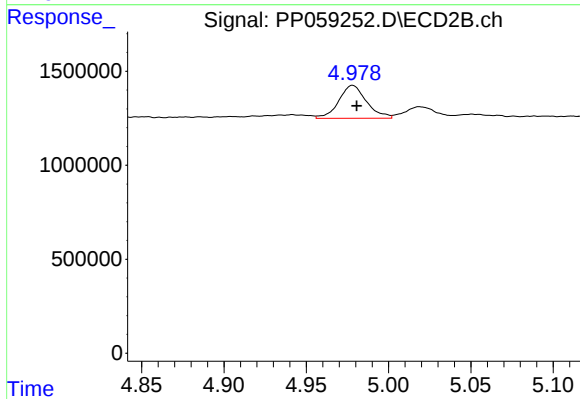

#6 AR-1016-4


R.T.: 4.978 min
Delta R.T.: -0.002 min
Response: 2061028
Conc: 49.91 ng/ml

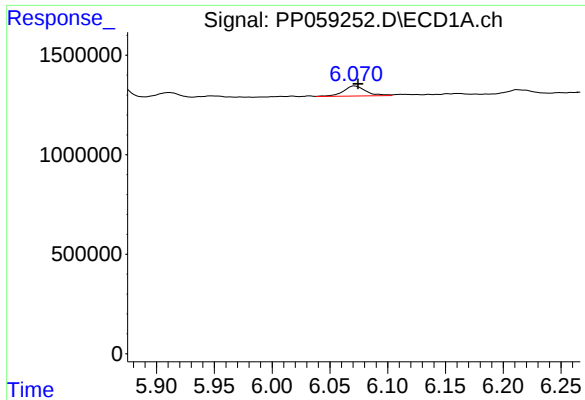

#7 AR-1016-5


R.T.: 6.071 min
Delta R.T.: -0.003 min
Response: 672429
Conc: 22.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

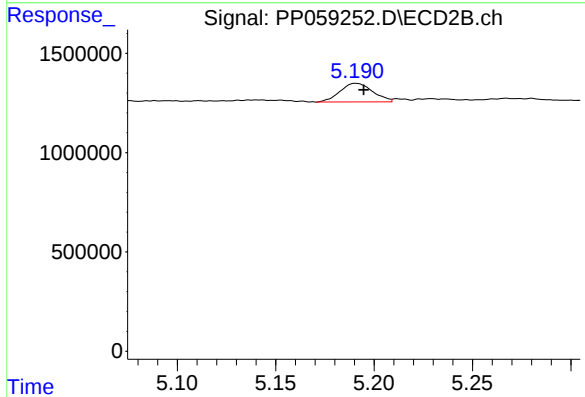


#7 AR-1016-5

R.T.: 5.190 min
Delta R.T.: -0.004 min
Response: 1087856
Conc: 20.91 ng/ml

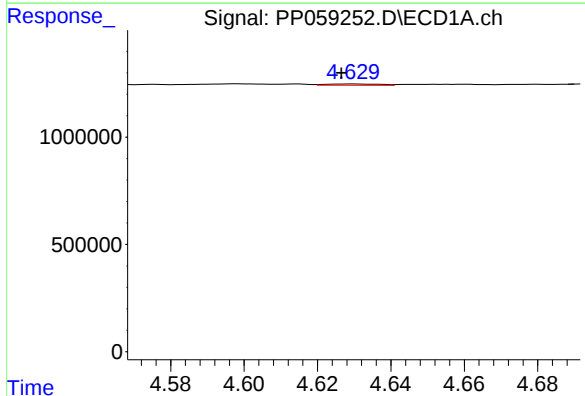


#8 AR-1221-1

R.T.: 4.630 min
Delta R.T.: 0.003 min
Response: 58087
Conc: 3.69 ng/ml

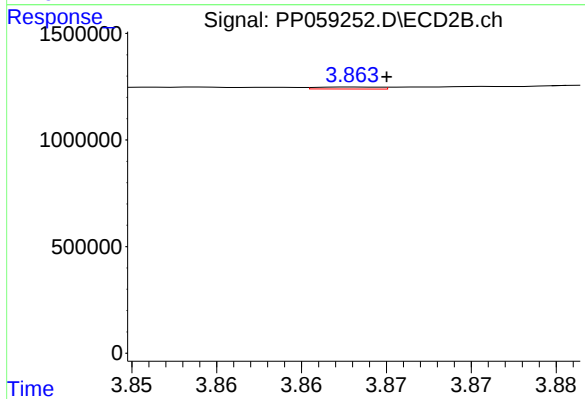

#8 AR-1221-1


R.T.: 3.863 min
Delta R.T.: -0.002 min
Response: 23328
Conc: 0.86 ng/ml

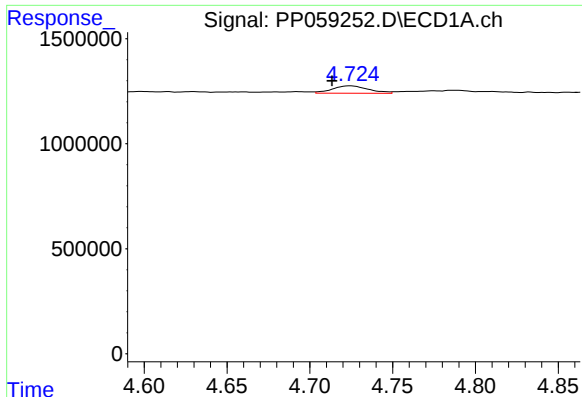

#9 AR-1221-2


R.T.: 4.725 min
Delta R.T.: 0.011 min
Response: 529026
Conc: 44.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

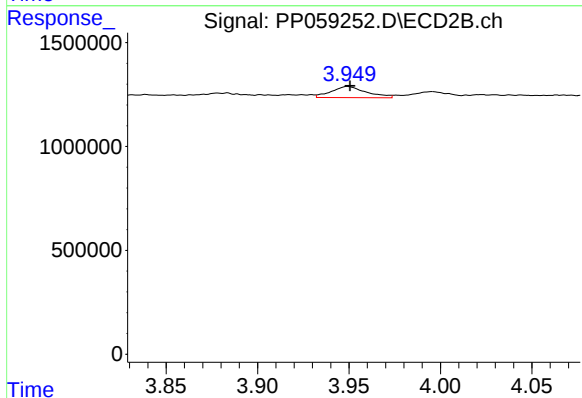


#9 AR-1221-2

R.T.: 3.949 min
Delta R.T.: -0.002 min
Response: 717333
Conc: 36.03 ng/ml

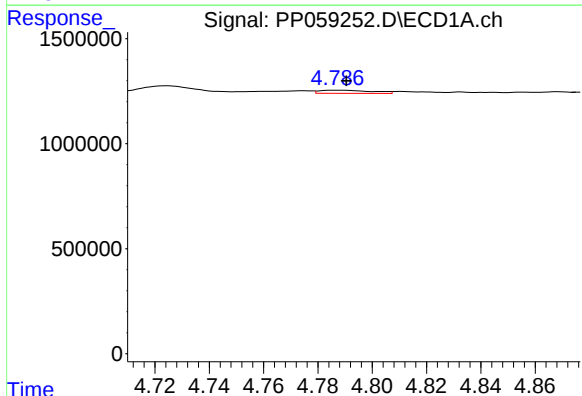


#10 AR-1221-3

R.T.: 4.787 min
Delta R.T.: -0.004 min
Response: 201167
Conc: 5.71 ng/ml

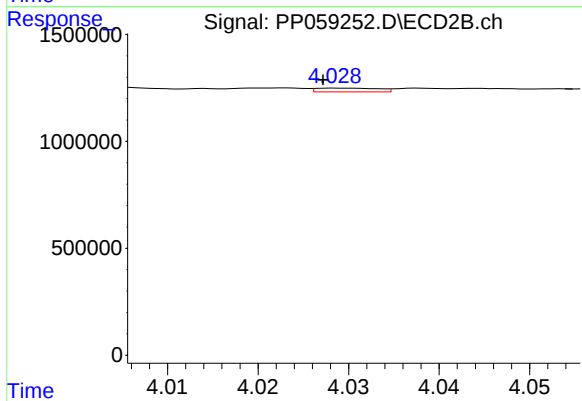

#10 AR-1221-3


R.T.: 4.029 min
Delta R.T.: 0.002 min
Response: 83911
Conc: 1.41 ng/ml

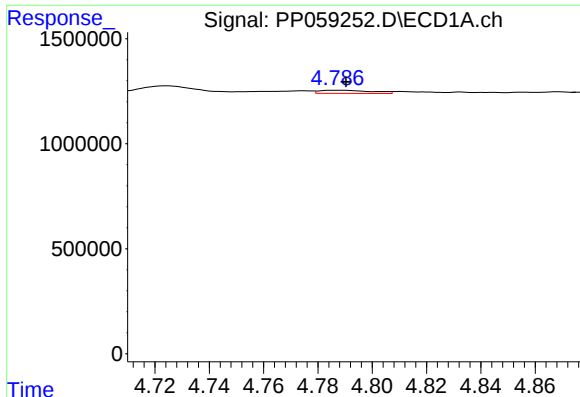

#11 AR-1232-1


R.T.: 4.787 min
Delta R.T.: -0.003 min
Response: 201167
Conc: 6.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

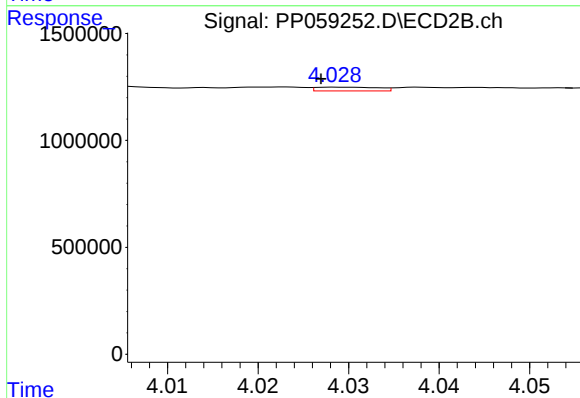


#11 AR-1232-1

R.T.: 4.029 min
Delta R.T.: 0.002 min
Response: 83911
Conc: 1.77 ng/ml

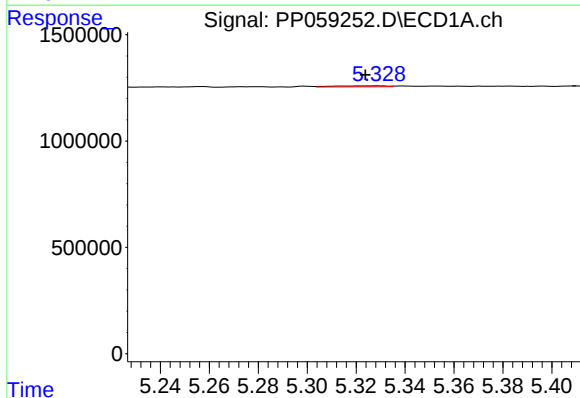


#12 AR-1232-2

R.T.: 5.329 min
Delta R.T.: 0.005 min
Response: 69451
Conc: 4.46 ng/ml

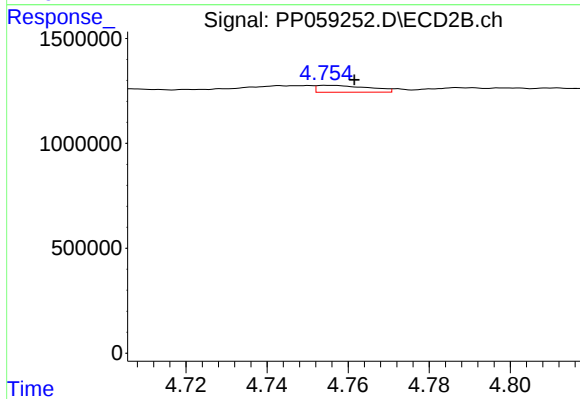

#12 AR-1232-2


R.T.: 4.754 min
Delta R.T.: -0.007 min
Response: 293124
Conc: 6.91 ng/ml

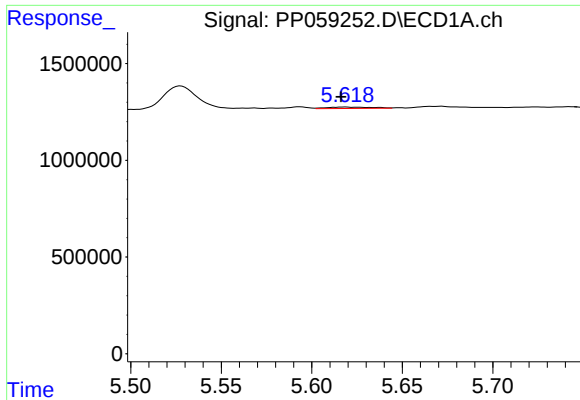

#13 AR-1232-3


R.T.: 5.619 min
Delta R.T.: 0.003 min
Response: 134772
Conc: 5.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

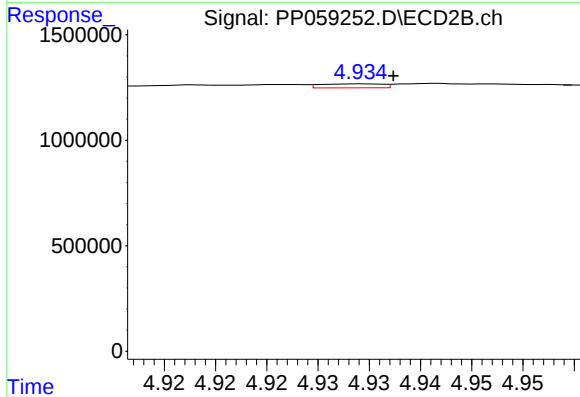


#13 AR-1232-3

R.T.: 4.934 min
Delta R.T.: -0.003 min
Response: 78294
Conc: 3.53 ng/ml

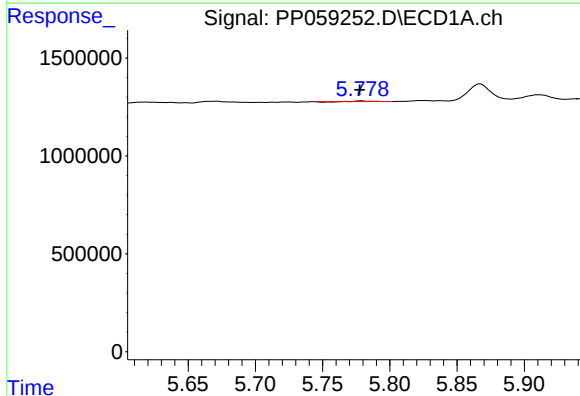


#14 AR-1232-4

R.T.: 5.778 min
Delta R.T.: 0.000 min
Response: 9351
Conc: 0.71 ng/ml

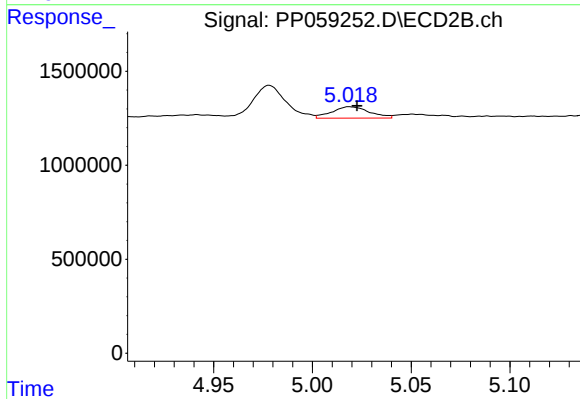

#14 AR-1232-4


R.T.: 5.019 min
Delta R.T.: -0.004 min
Response: 798211
Conc: 37.80 ng/ml

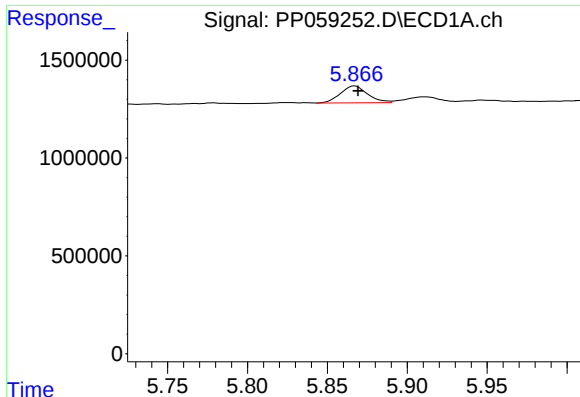

#15 AR-1232-5


R.T.: 5.867 min
Delta R.T.: -0.002 min
Response: 1011823
Conc: 88.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

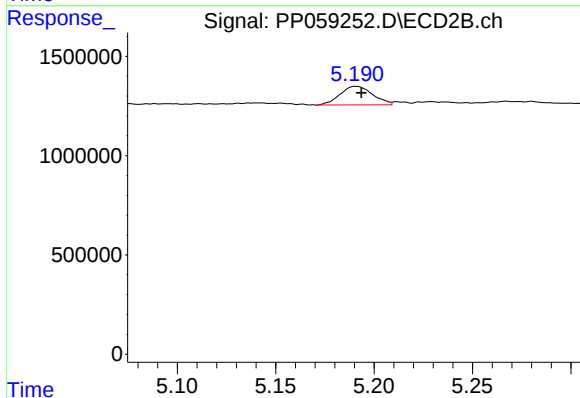


#15 AR-1232-5

R.T.: 5.190 min
Delta R.T.: -0.003 min
Response: 1087856
Conc: 47.46 ng/ml

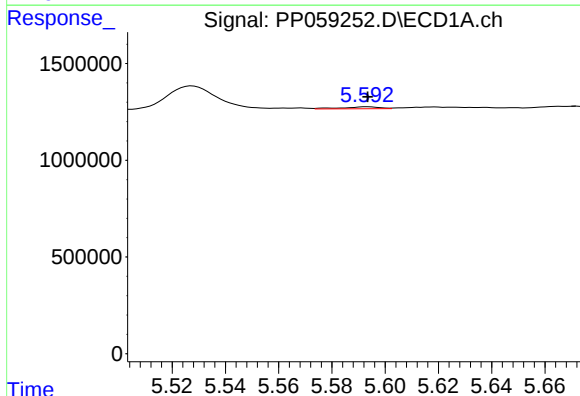


#16 AR-1242-1

R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 104777
Conc: 3.06 ng/ml

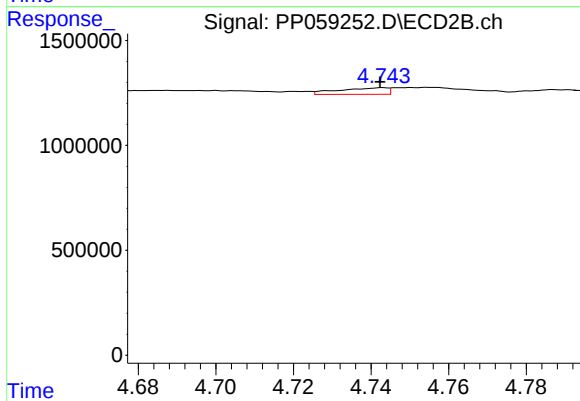

#16 AR-1242-1


R.T.: 4.743 min
Delta R.T.: 0.000 min
Response: 275255
Conc: 4.92 ng/ml

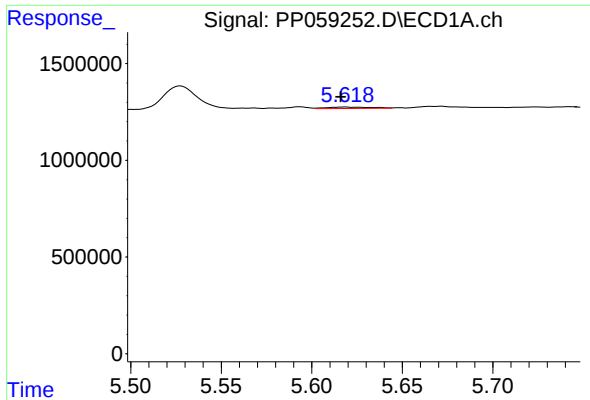

#17 AR-1242-2


R.T.: 5.619 min
Delta R.T.: 0.003 min
Response: 134772
Conc: 2.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

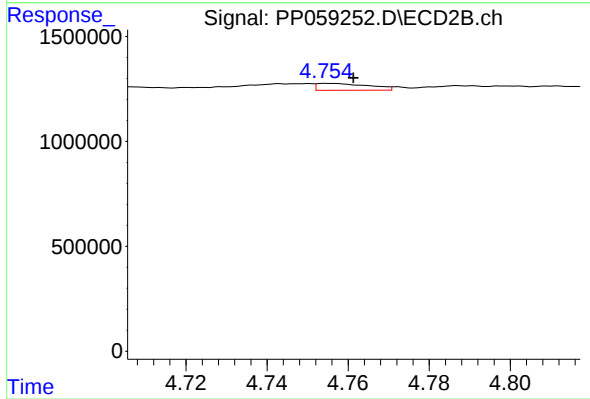


#17 AR-1242-2

R.T.: 4.754 min
Delta R.T.: -0.007 min
Response: 293124
Conc: 3.68 ng/ml

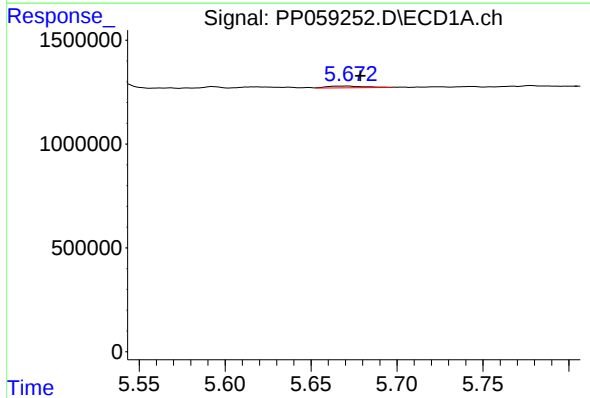


#18 AR-1242-3

R.T.: 5.671 min
Delta R.T.: -0.007 min
Response: 131560
Conc: 4.19 ng/ml

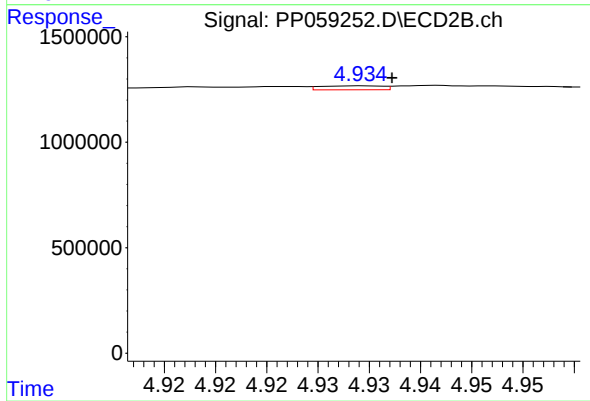

#18 AR-1242-3


R.T.: 4.934 min
Delta R.T.: -0.003 min
Response: 78294
Conc: 1.84 ng/ml

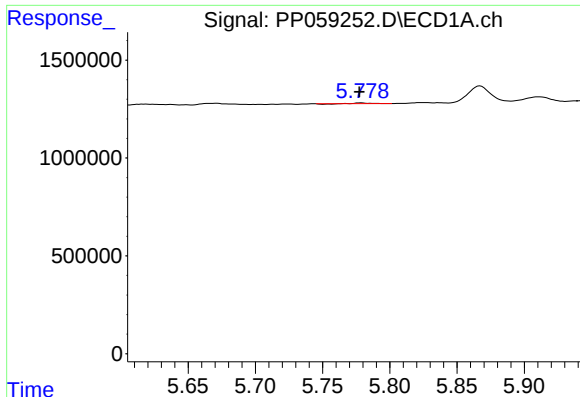

#19 AR-1242-4


R.T.: 5.778 min
Delta R.T.: 0.000 min
Response: 9351
Conc: 0.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

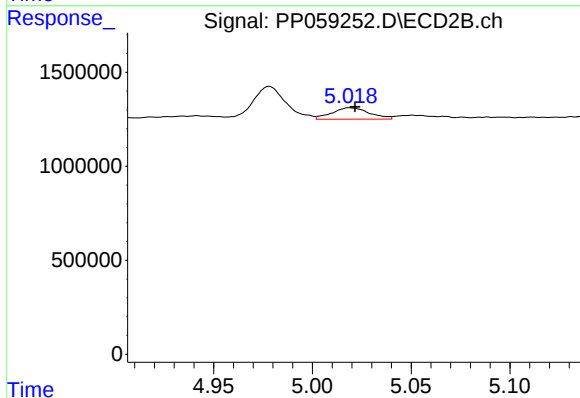


#19 AR-1242-4

R.T.: 5.019 min
Delta R.T.: -0.003 min
Response: 798211
Conc: 18.28 ng/ml

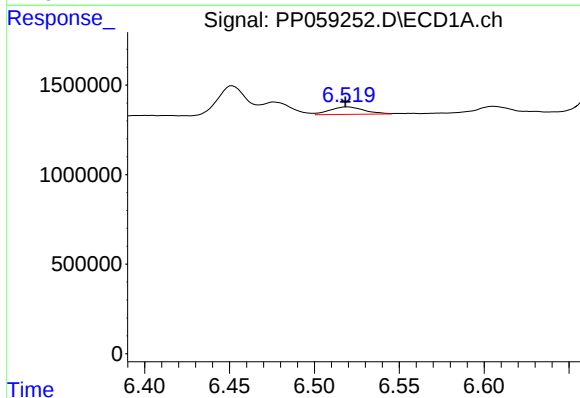


#20 AR-1242-5

R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 586165
Conc: 22.69 ng/ml

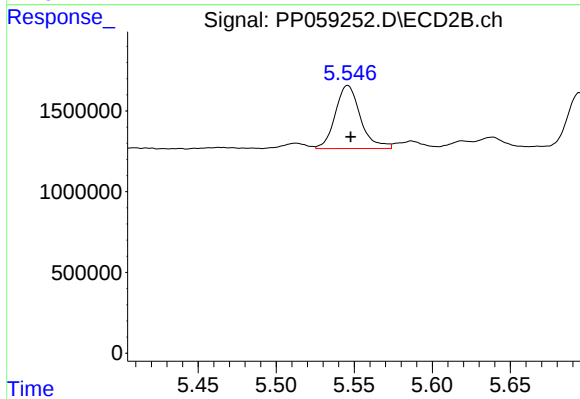

#20 AR-1242-5


R.T.: 5.546 min
Delta R.T.: -0.002 min
Response: 4385827
Conc: 88.29 ng/ml

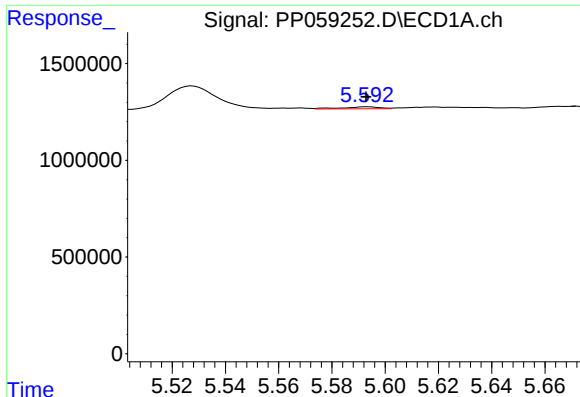

#21 AR-1248-1


R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 104777
Conc: 4.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

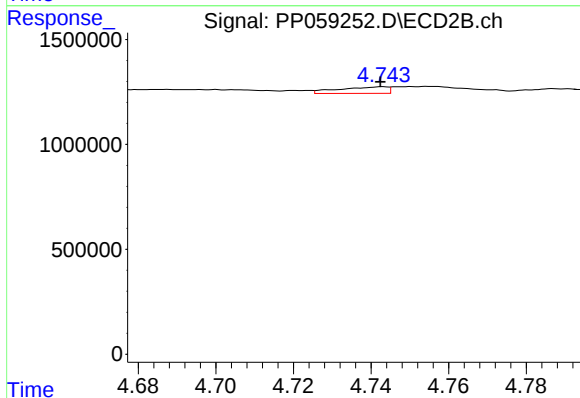


#21 AR-1248-1

R.T.: 4.743 min
Delta R.T.: 0.000 min
Response: 275255
Conc: 6.69 ng/ml

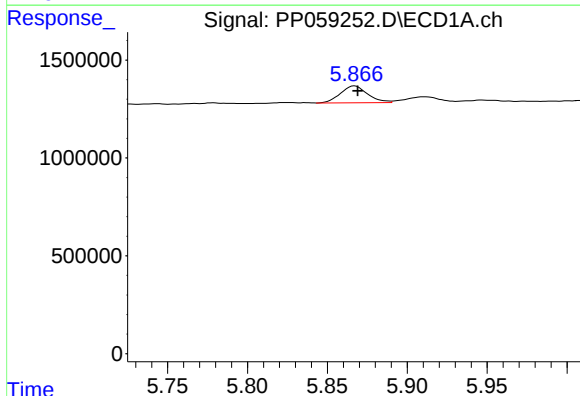


#22 AR-1248-2

R.T.: 5.867 min
Delta R.T.: -0.002 min
Response: 1011823
Conc: 26.14 ng/ml

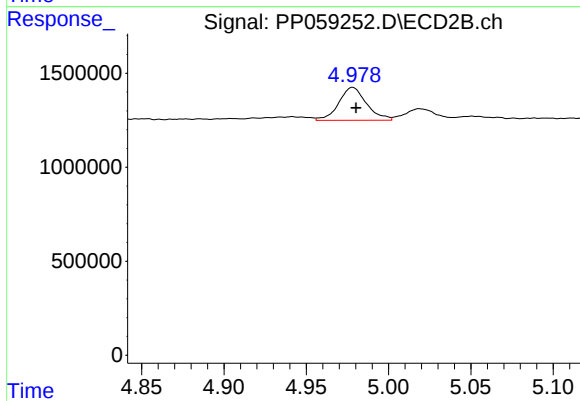

#22 AR-1248-2


R.T.: 4.978 min
Delta R.T.: -0.002 min
Response: 2061028
Conc: 34.23 ng/ml

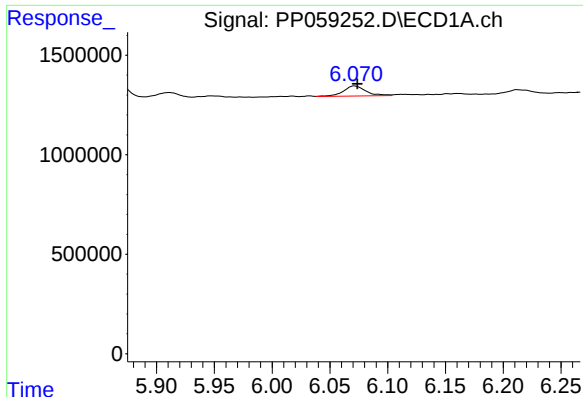

#23 AR-1248-3


R.T.: 6.071 min
Delta R.T.: -0.003 min
Response: 672429
Conc: 15.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

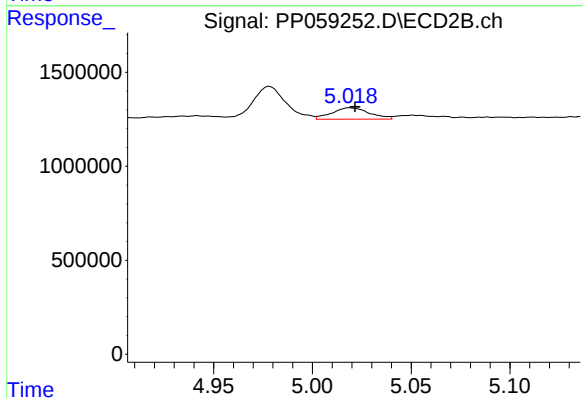


#23 AR-1248-3

R.T.: 5.019 min
Delta R.T.: -0.003 min
Response: 798211
Conc: 12.96 ng/ml

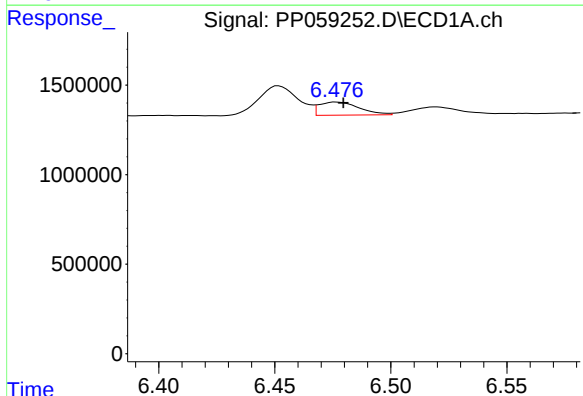


#24 AR-1248-4

R.T.: 6.477 min
Delta R.T.: -0.003 min
Response: 874782
Conc: 21.01 ng/ml

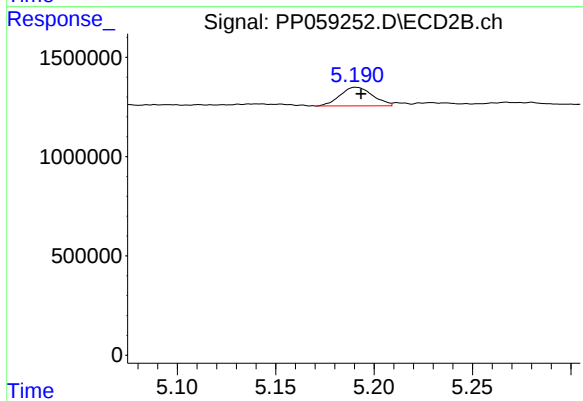

#24 AR-1248-4


R.T.: 5.190 min
Delta R.T.: -0.003 min
Response: 1087856
Conc: 15.11 ng/ml

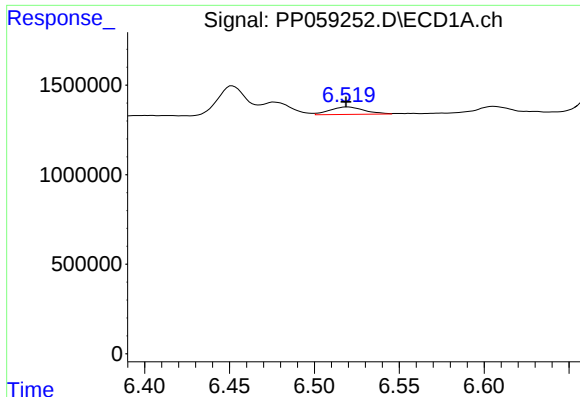

#25 AR-1248-5


R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 586165
Conc: 14.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

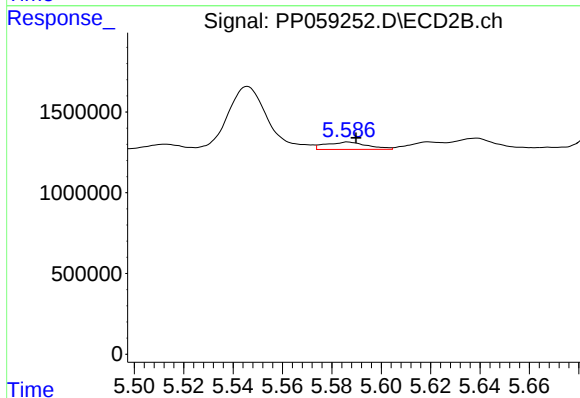


#25 AR-1248-5

R.T.: 5.586 min
Delta R.T.: -0.003 min
Response: 531569
Conc: 8.06 ng/ml

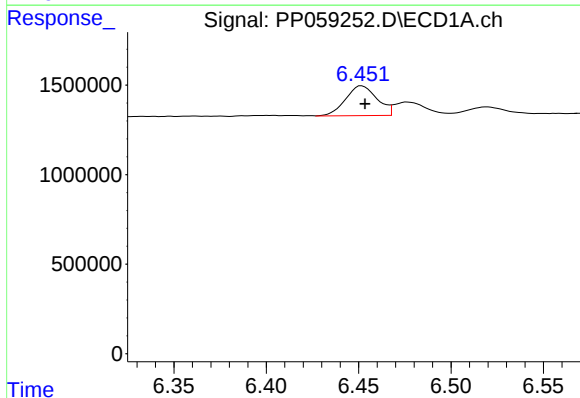


#26 AR-1254-1

R.T.: 6.452 min
Delta R.T.: -0.002 min
Response: 1970388
Conc: 42.18 ng/ml

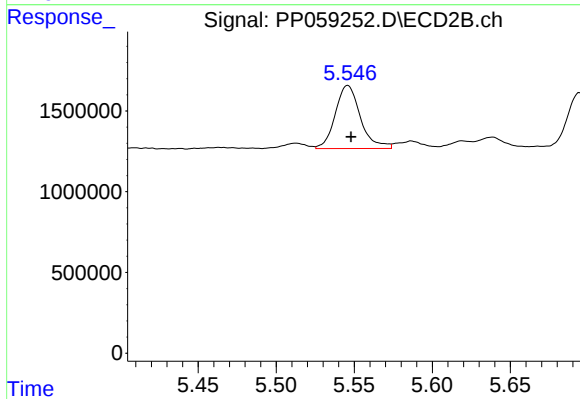

#26 AR-1254-1


R.T.: 5.546 min
Delta R.T.: -0.002 min
Response: 4385827
Conc: 43.29 ng/ml

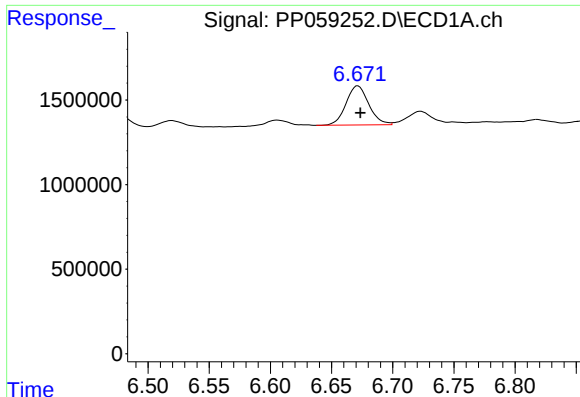

#27 AR-1254-2


R.T.: 6.672 min
Delta R.T.: -0.002 min
Response: 2990970
Conc: 43.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

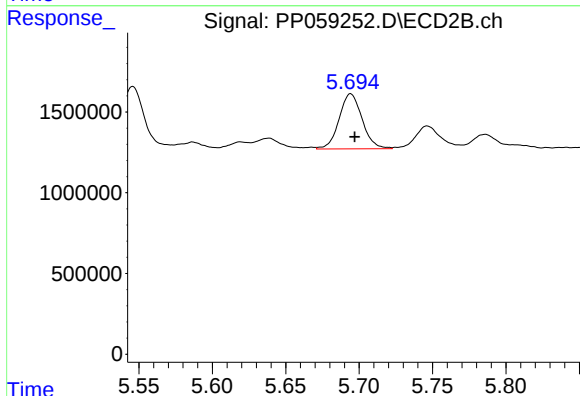


#27 AR-1254-2

R.T.: 5.694 min
Delta R.T.: -0.003 min
Response: 3717642
Conc: 42.11 ng/ml

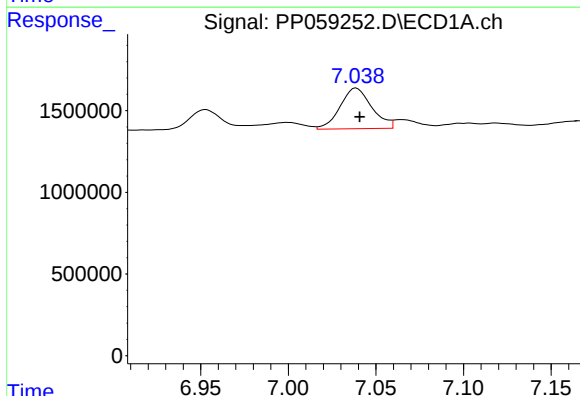


#28 AR-1254-3

R.T.: 7.039 min
Delta R.T.: -0.002 min
Response: 3141409
Conc: 45.51 ng/ml

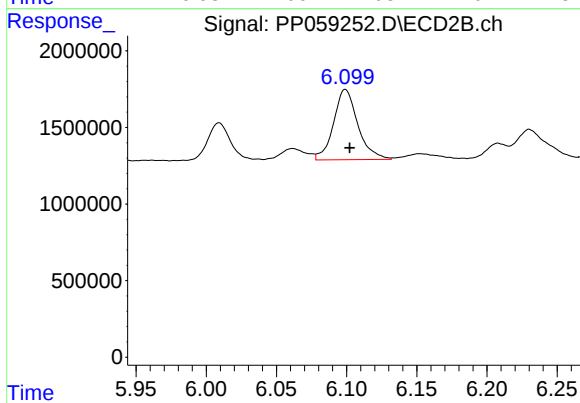

#28 AR-1254-3


R.T.: 6.099 min
Delta R.T.: -0.003 min
Response: 5535366
Conc: 40.04 ng/ml

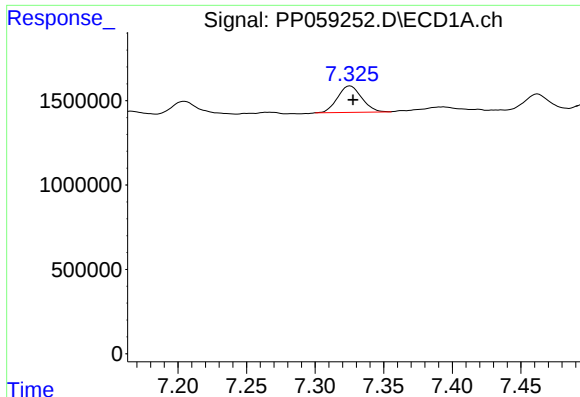

#29 AR-1254-4


R.T.: 7.326 min
Delta R.T.: -0.002 min
Response: 1917697
Conc: 42.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

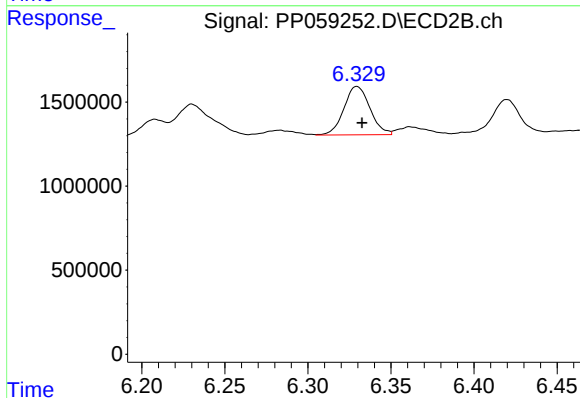


#29 AR-1254-4

R.T.: 6.329 min
Delta R.T.: -0.003 min
Response: 3142060
Conc: 39.09 ng/ml

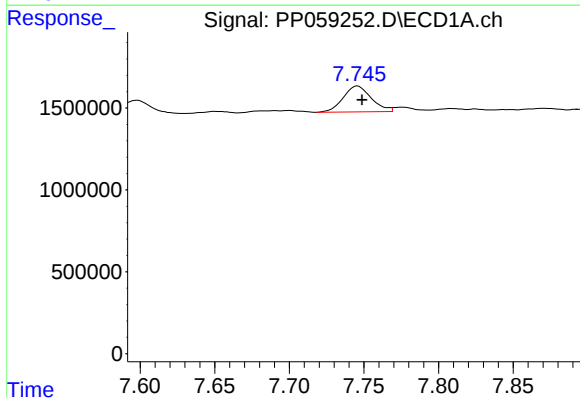


#30 AR-1254-5

R.T.: 7.746 min
Delta R.T.: -0.003 min
Response: 2070968
Conc: 44.08 ng/ml

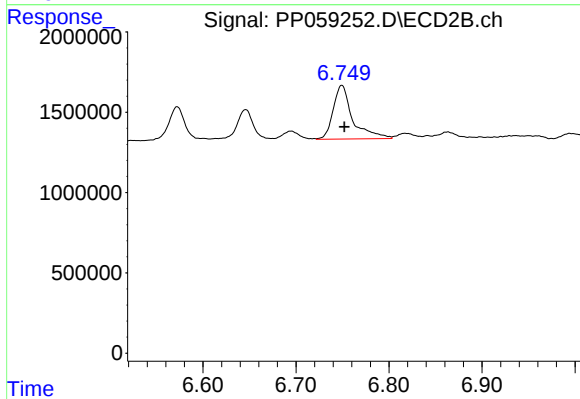

#30 AR-1254-5


R.T.: 6.749 min
Delta R.T.: -0.003 min
Response: 4873070
Conc: 40.75 ng/ml

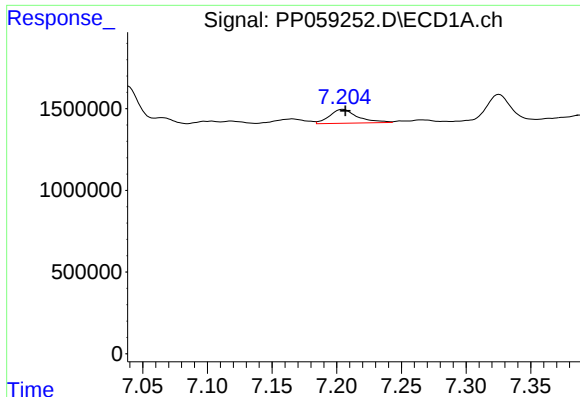

#31 AR-1260-1


R.T.: 7.205 min
Delta R.T.: -0.002 min
Response: 1274993
Conc: 23.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

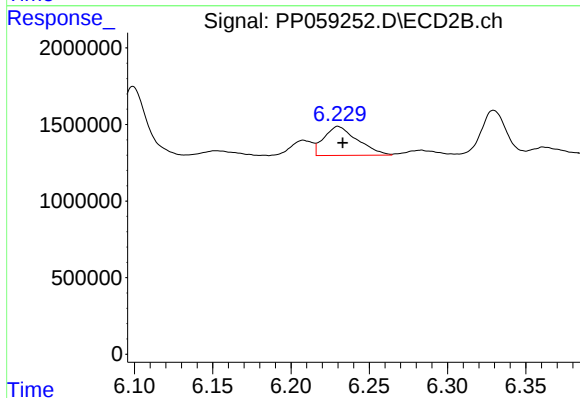


#31 AR-1260-1

R.T.: 6.230 min
Delta R.T.: -0.003 min
Response: 2810706
Conc: 28.38 ng/ml

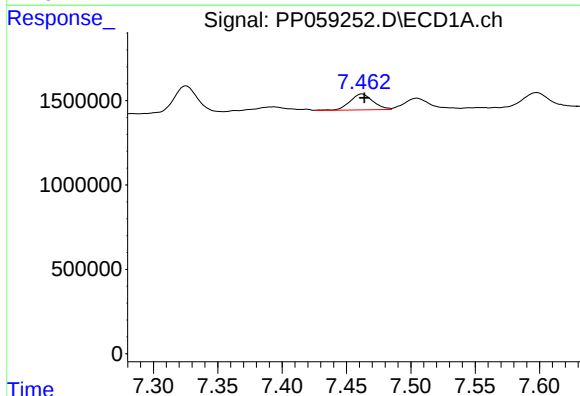


#32 AR-1260-2

R.T.: 7.462 min
Delta R.T.: -0.002 min
Response: 1167895
Conc: 19.62 ng/ml

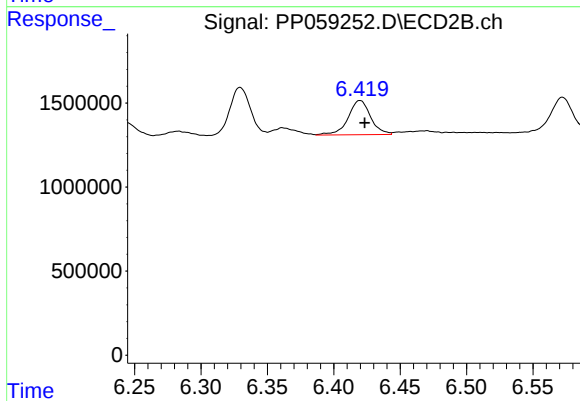

#32 AR-1260-2


R.T.: 6.420 min
Delta R.T.: -0.003 min
Response: 2414818
Conc: 20.87 ng/ml

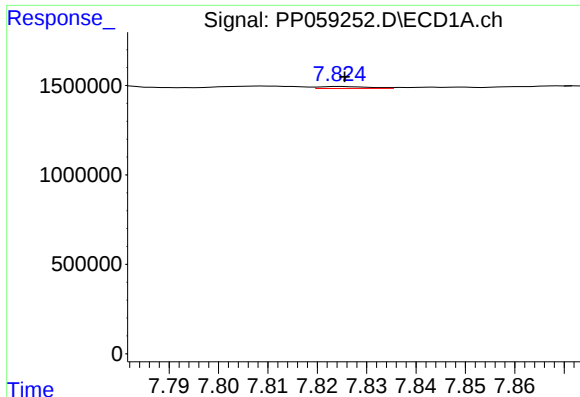

#33 AR-1260-3


R.T.: 7.825 min
Delta R.T.: 0.000 min
Response: 76814
Conc: 1.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

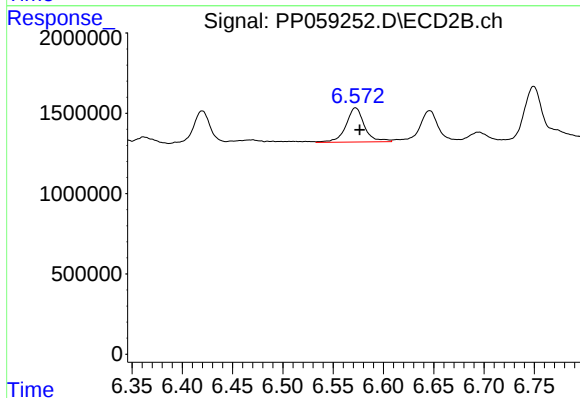


#33 AR-1260-3

R.T.: 6.572 min
Delta R.T.: -0.004 min
Response: 2741452
Conc: 24.65 ng/ml

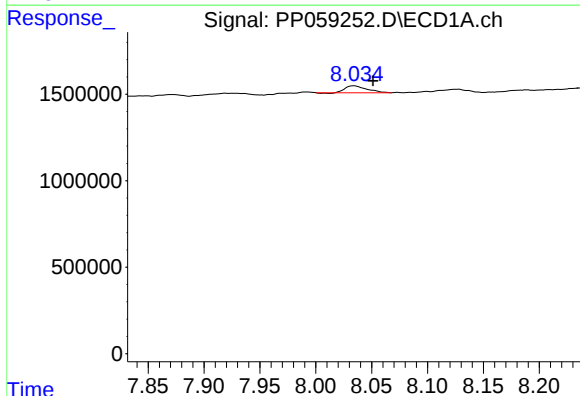


#34 AR-1260-4

R.T.: 8.035 min
Delta R.T.: -0.017 min
Response: 543544
Conc: 12.24 ng/ml

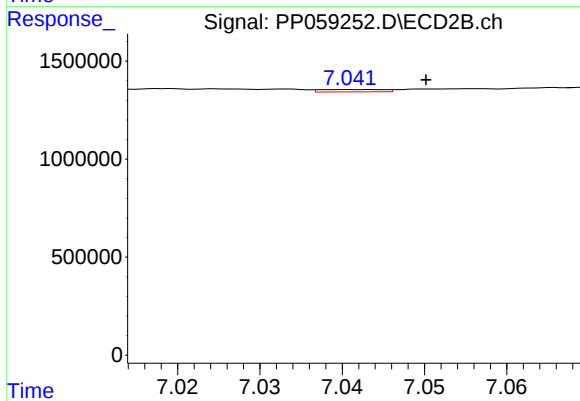

#34 AR-1260-4


R.T.: 7.041 min
Delta R.T.: -0.009 min
Response: 65946
Conc: 0.76 ng/ml

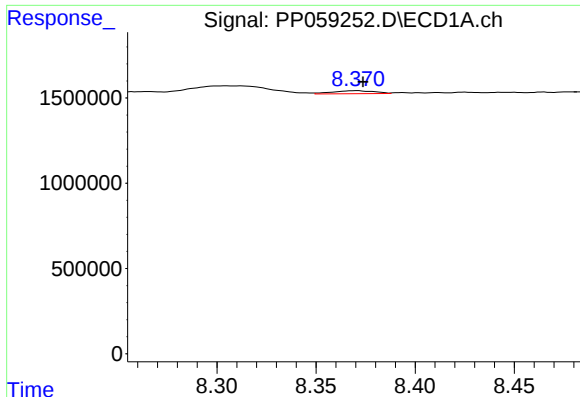

#35 AR-1260-5


R.T.: 8.370 min
Delta R.T.: -0.003 min
Response: 257781
Conc: 3.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

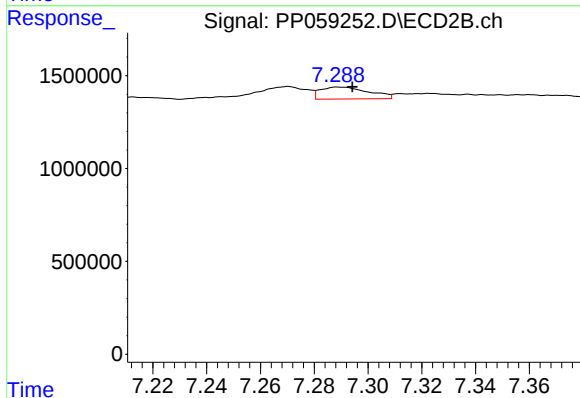


#35 AR-1260-5

R.T.: 7.288 min
Delta R.T.: -0.006 min
Response: 806273
Conc: 4.37 ng/ml

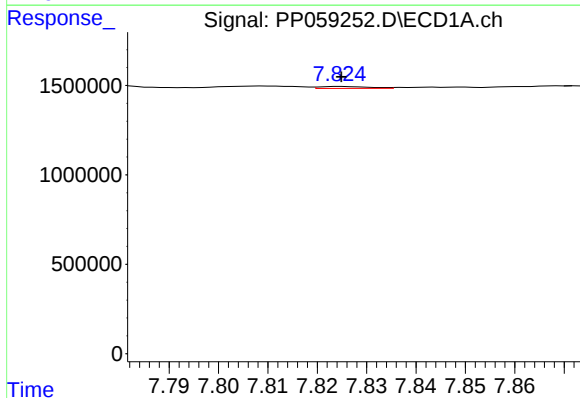


#36 AR-1262-1

R.T.: 7.825 min
Delta R.T.: 0.000 min
Response: 76814
Conc: 1.21 ng/ml

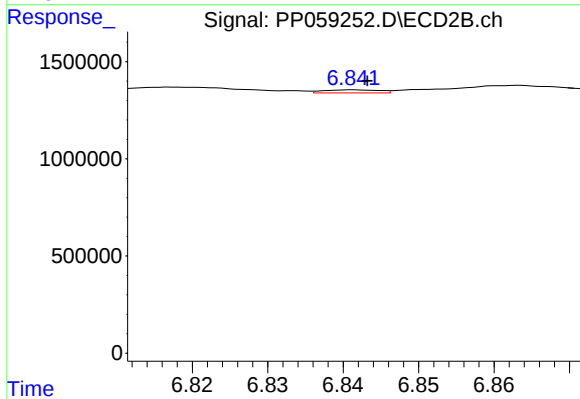

#36 AR-1262-1


R.T.: 6.841 min
Delta R.T.: -0.002 min
Response: 82156
Conc: 1.43 ng/ml

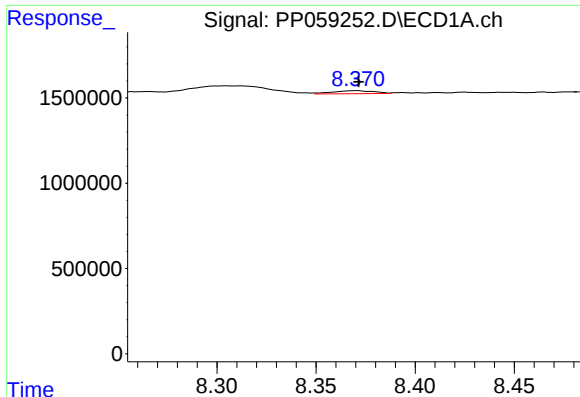

#37 AR-1262-2


R.T.: 8.370 min
Delta R.T.: -0.001 min
Response: 257781
Conc: 2.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

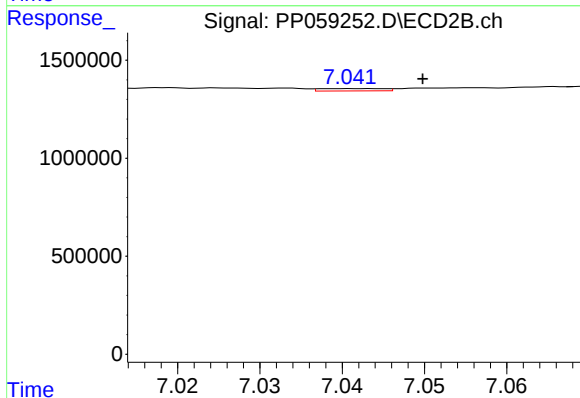


#37 AR-1262-2

R.T.: 7.041 min
Delta R.T.: -0.009 min
Response: 65946
Conc: 0.56 ng/ml

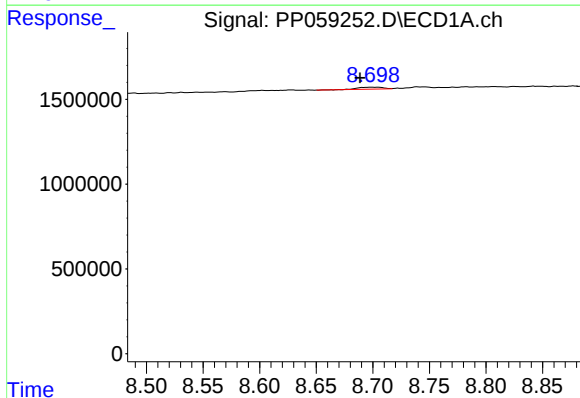


#38 AR-1262-3

R.T.: 8.699 min
Delta R.T.: 0.010 min
Response: 194848
Conc: 3.03 ng/ml

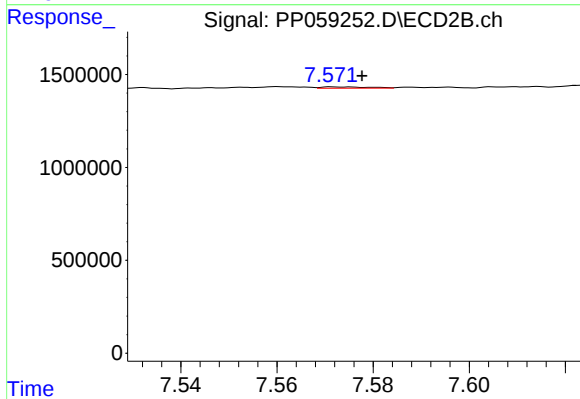

#38 AR-1262-3


R.T.: 7.571 min
Delta R.T.: -0.006 min
Response: 51200
Conc: 0.60 ng/ml

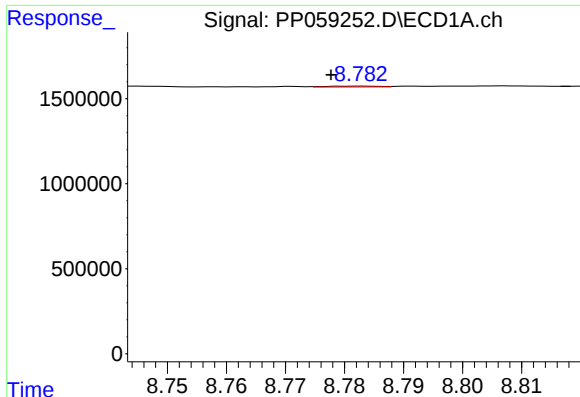

#39 AR-1262-4


R.T.: 8.783 min
Delta R.T.: 0.005 min
Response: 31610
Conc: 0.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

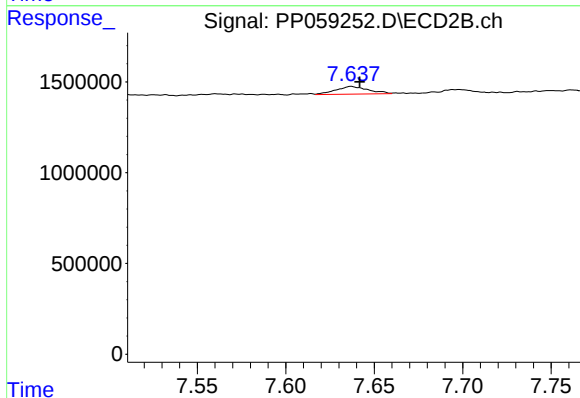


#39 AR-1262-4

R.T.: 7.637 min
Delta R.T.: -0.005 min
Response: 543382
Conc: 3.60 ng/ml

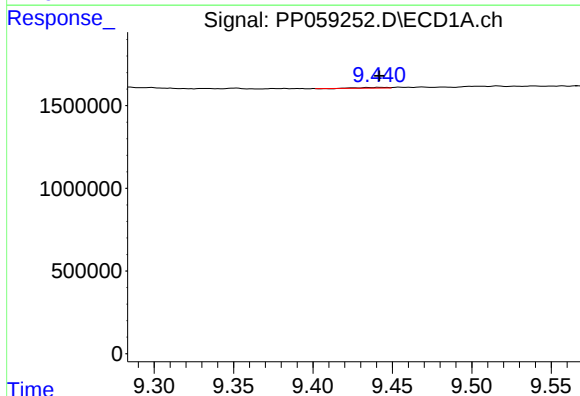


#40 AR-1262-5

R.T.: 9.442 min
Delta R.T.: 0.000 min
Response: 43945
Conc: 1.47 ng/ml

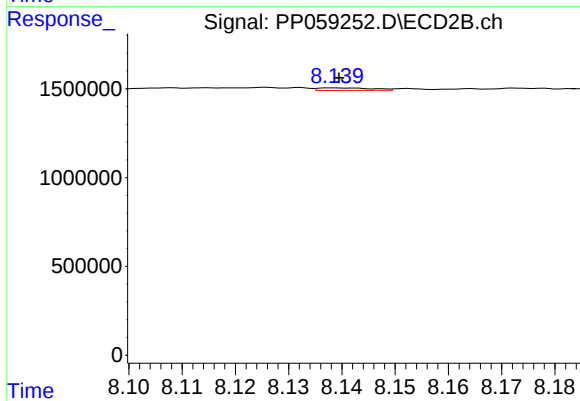

#40 AR-1262-5


R.T.: 8.138 min
Delta R.T.: -0.001 min
Response: 101549
Conc: 1.59 ng/ml

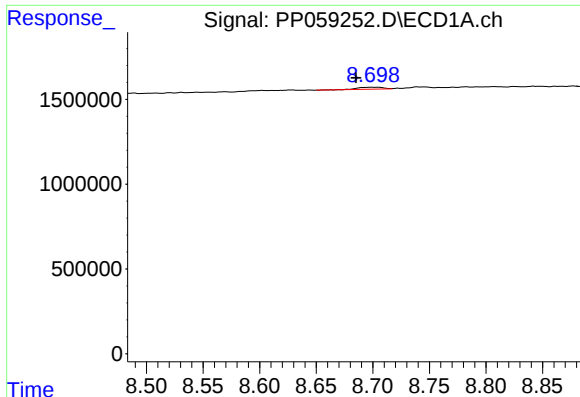

#41 AR-1268-1


R.T.: 8.699 min
Delta R.T.: 0.013 min
Response: 194848
Conc: 1.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

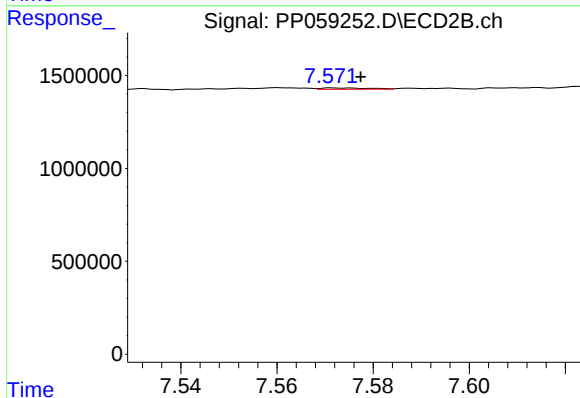


#41 AR-1268-1

R.T.: 7.571 min
Delta R.T.: -0.006 min
Response: 51200
Conc: 0.21 ng/ml

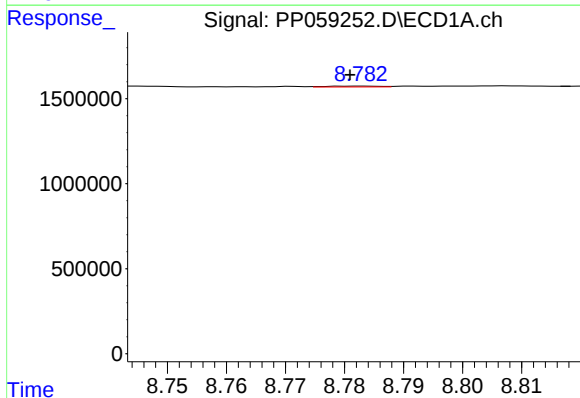


#42 AR-1268-2

R.T.: 8.783 min
Delta R.T.: 0.002 min
Response: 31610
Conc: 0.32 ng/ml

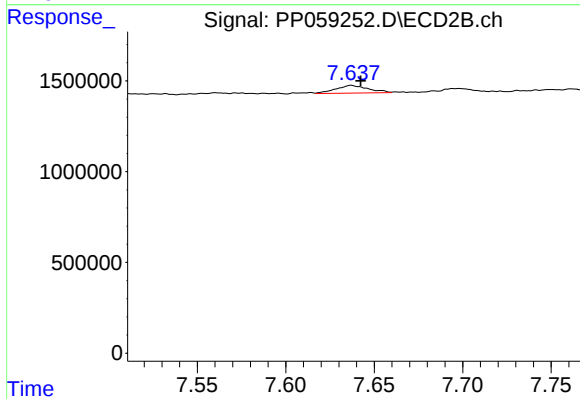

#42 AR-1268-2


R.T.: 7.637 min
Delta R.T.: -0.005 min
Response: 543382
Conc: 2.48 ng/ml

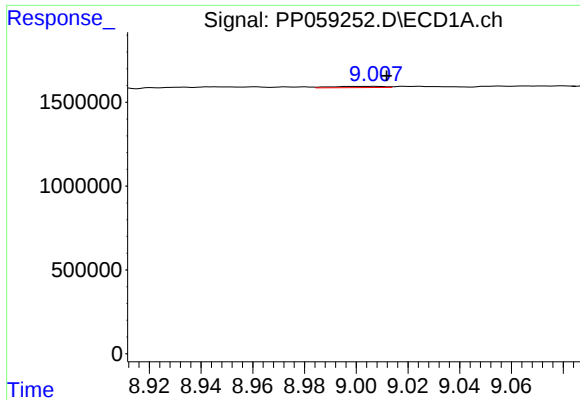

#43 AR-1268-3


R.T.: 9.008 min
Delta R.T.: -0.004 min
Response: 105094
Conc: 1.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

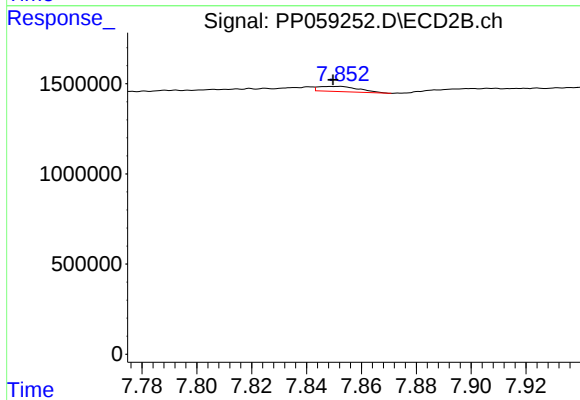


#43 AR-1268-3

R.T.: 7.852 min
Delta R.T.: 0.003 min
Response: 294258
Conc: 1.50 ng/ml

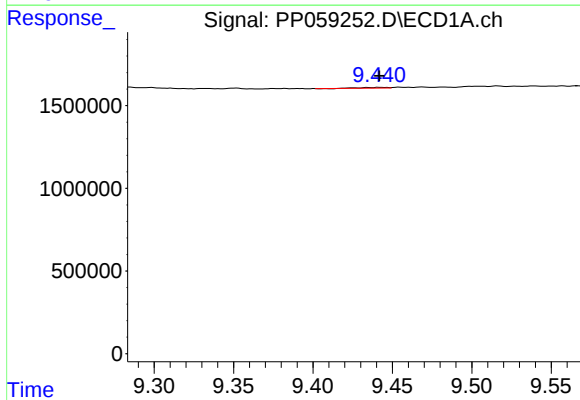


#44 AR-1268-4

R.T.: 9.442 min
Delta R.T.: 0.000 min
Response: 43945
Conc: 1.38 ng/ml

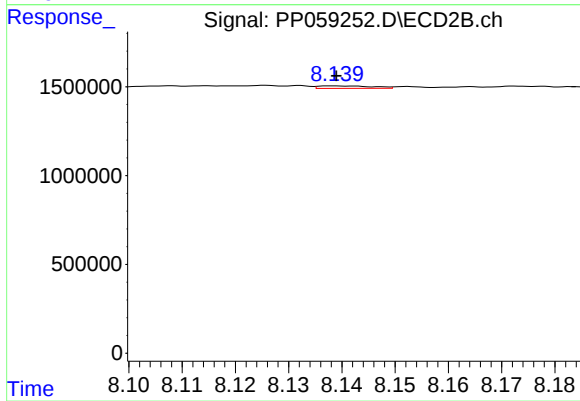

#44 AR-1268-4


R.T.: 8.138 min
Delta R.T.: 0.000 min
Response: 101549
Conc: 1.46 ng/ml

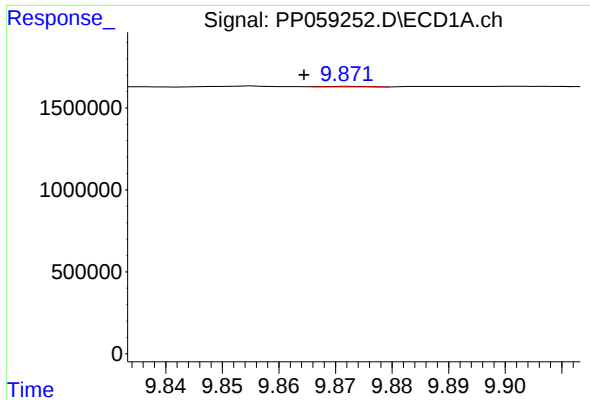

#45 AR-1268-5

R.T.: 9.872 min
Delta R.T.: 0.008 min
Response: 20497
Conc: 0.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

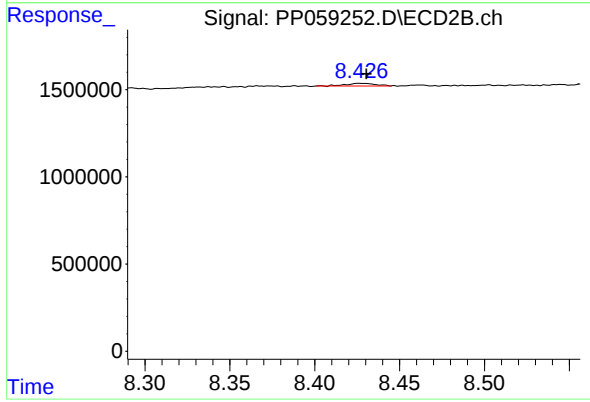

#45 AR-1268-5

R.T.: 8.426 min
Delta R.T.: -0.004 min
Response: 181248
Conc: 0.35 ng/ml