

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
 Data File : PP059253.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2023 09:29
 Operator : YP\AJ
 Sample : 03572-07
 Misc : AR1262 LOD 40 PPB
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 11:02:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.415	3.647	23199088	39684924	18.907	19.586
2)	SA Decachlor...	10.206	8.683	17774303	32761470	23.288	23.288
Target Compounds							
3)	L1 AR-1016-1	5.593	4.738	87873	194972	2.237	3.040 #
4)	L1 AR-1016-2	5.617	4.756	115069	494360	2.030	5.442 #
5)	L1 AR-1016-3	5.680	4.938	47572	110509	1.326	2.300 #
6)	L1 AR-1016-4	5.776	4.980	64011	44247	2.210	1.072 #
7)	L1 AR-1016-5	6.074	5.194	96199	164823	3.179	3.168
8)	L2 AR-1221-1	4.623	3.865	49131	28856	3.119	1.063 #
9)	L2 AR-1221-2	4.726	3.950	534377	798695	45.252	40.116
10)	L2 AR-1221-3	4.785	4.026	314927	72426	8.943	1.217 #
11)	L3 AR-1232-1	4.785	4.026	314927	72426	10.713	1.526 #
12)	L3 AR-1232-2	5.322	4.756	45738	494360	2.934	11.654 #
13)	L3 AR-1232-3	5.617	4.938	115069	110509	4.358	4.981
14)	L3 AR-1232-4	5.776	5.021	64011	167191	4.837	7.918 #
15)	L3 AR-1232-5	5.867	5.194	88134	164823	7.721	7.190
16)	L4 AR-1242-1	5.593	4.738	87873	194972	2.567	3.484 #
17)	L4 AR-1242-2	5.617	4.756	115069	494360	2.345	6.200 #
18)	L4 AR-1242-3	5.680	4.938	47572	110509	1.514	2.593 #
19)	L4 AR-1242-4	5.776	5.021	64011	167191	2.496	3.829 #
20)	L4 AR-1242-5	6.514	5.546	133556	898429	5.170	18.087 #
21)	L5 AR-1248-1	5.593	4.738	87873	194972	3.462	4.739 #
22)	L5 AR-1248-2	5.867	4.980	88134	44247	2.277	0.735 #
23)	L5 AR-1248-3	6.074	5.021	96199	167191	2.277	2.714
24)	L5 AR-1248-4	6.478	5.194	162136	164823	3.894	2.289 #
25)	L5 AR-1248-5	6.514	5.587	133556	179038	3.274	2.713
26)	L6 AR-1254-1	6.453	5.546	440262	898429	9.424	8.868
27)	L6 AR-1254-2	6.671	5.695	461663	1068825	6.709	12.107 #
28)	L6 AR-1254-3	7.040	6.115	340972	2605338	4.940	18.846 #
29)	L6 AR-1254-4	7.329	6.327	151193	316641	3.359	3.939
30)	L6 AR-1254-5	7.743	6.748	1630352	2639599	34.698	22.073 #
31)	L7 AR-1260-1	7.205	6.229	2229863	3741041	40.758	37.774
32)	L7 AR-1260-2	7.462	6.420	1978702	4005840	33.234	34.620
33)	L7 AR-1260-3	7.823	6.575	2625090	4216081	66.703	37.903 #
34)	L7 AR-1260-4	8.050	7.047	2036266	4473369	45.848	51.599
35)	L7 AR-1260-5	8.370	7.290	3637851	8814870	45.490	47.823
36)	L8 AR-1262-1	7.823	6.841	2625090	2543658	41.216	44.211
37)	L8 AR-1262-2	8.370	7.047	3637851	4473369	39.612	37.911
38)	L8 AR-1262-3	8.686	7.574	2642210	3596699	41.058	42.265
39)	L8 AR-1262-4	8.775	7.638	2092595	6153756	63.017	40.737 #
40)	L8 AR-1262-5	9.440	8.136	1147886	2757987	38.466	43.245
41)	L9 AR-1268-1	8.686	7.574	2642210	3596699	23.265	14.750 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
 Data File : PP059253.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2023 09:29
 Operator : YP\AJ
 Sample : 03572-07
 Misc : AR1262 LOD 40 PPB
 ALS Vial : 48 Sample Multiplier: 1


Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 11:02:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.775	7.638	2092595	6153756	21.263	28.097 #
43) L9	AR-1268-3	9.015	7.846	97117	629978	1.048	3.222 #
44) L9	AR-1268-4	9.440	8.136	1147886	2757987	35.983	39.632
45) L9	AR-1268-5	9.861	8.427	526334	1053411	1.939	2.032


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

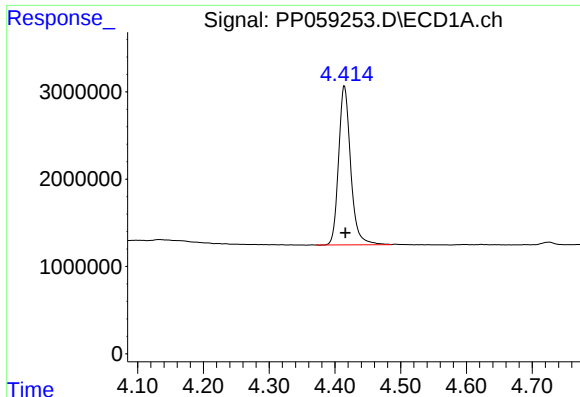

#1 Tetrachloro-m-xylene


R.T.: 4.415 min
Delta R.T.: -0.001 min
Response: 23199088
Conc: 18.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

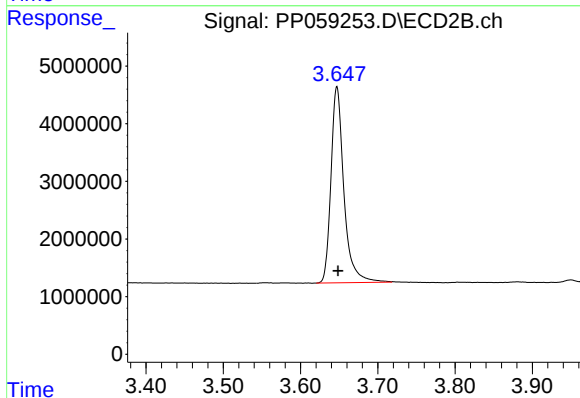


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: -0.002 min
Response: 39684924
Conc: 19.59 ng/ml

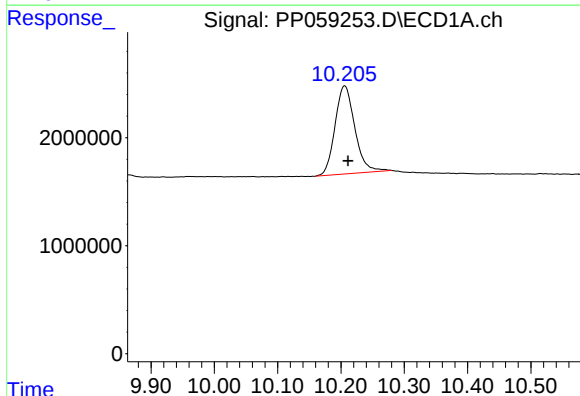


#2 Decachlorobiphenyl

R.T.: 10.206 min
Delta R.T.: -0.005 min
Response: 17774303
Conc: 23.29 ng/ml

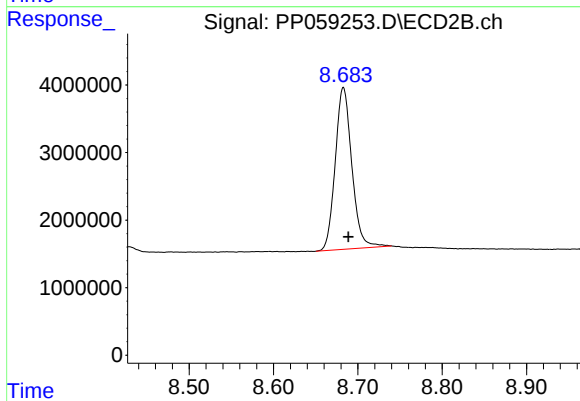

#2 Decachlorobiphenyl


R.T.: 8.683 min
Delta R.T.: -0.006 min
Response: 32761470
Conc: 23.29 ng/ml

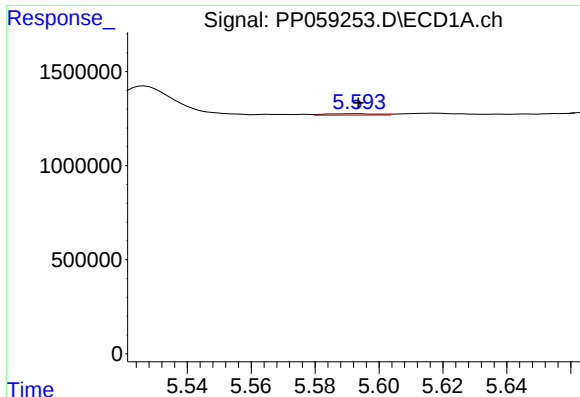

#3 AR-1016-1


R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 87873
Conc: 2.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

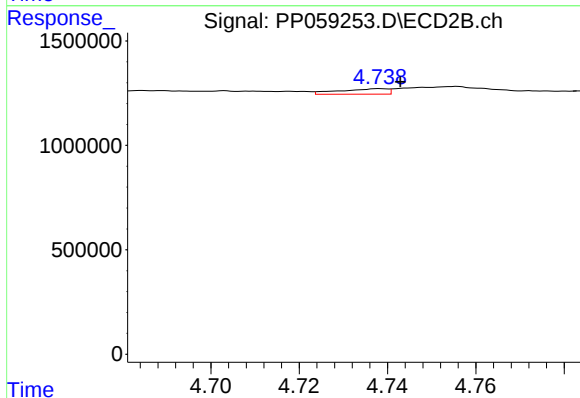


#3 AR-1016-1

R.T.: 4.738 min
Delta R.T.: -0.005 min
Response: 194972
Conc: 3.04 ng/ml

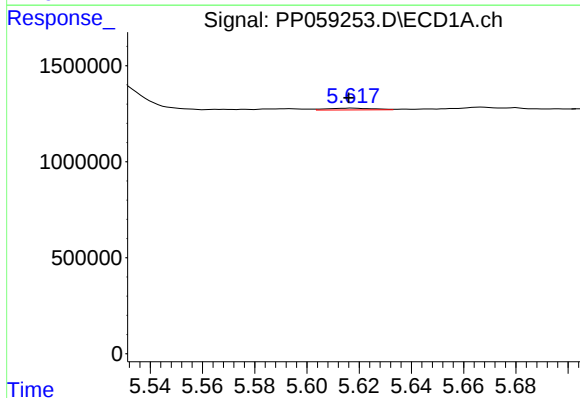


#4 AR-1016-2

R.T.: 5.617 min
Delta R.T.: 0.002 min
Response: 115069
Conc: 2.03 ng/ml

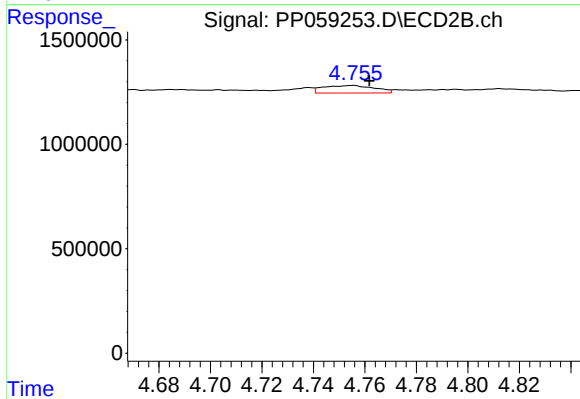

#4 AR-1016-2


R.T.: 4.756 min
Delta R.T.: -0.006 min
Response: 494360
Conc: 5.44 ng/ml

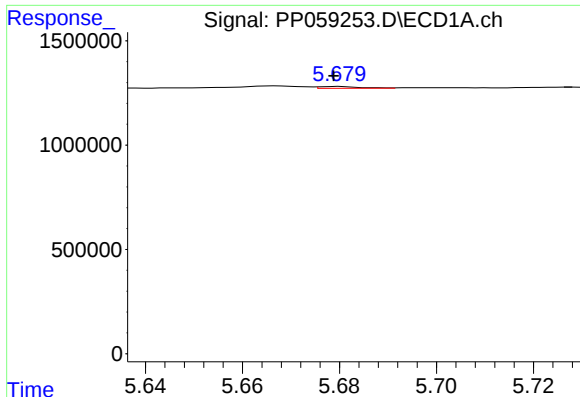

#5 AR-1016-3


R.T.: 5.680 min
Delta R.T.: 0.001 min
Response: 47572
Conc: 1.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

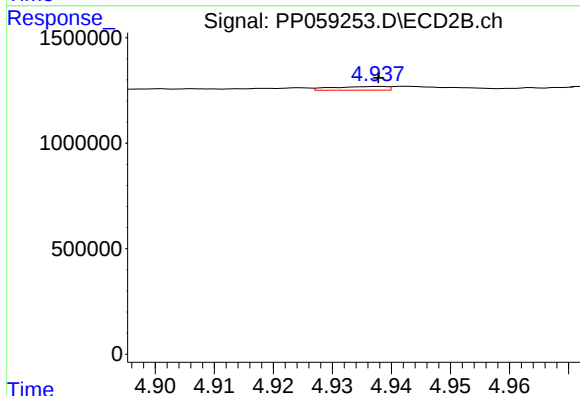


#5 AR-1016-3

R.T.: 4.938 min
Delta R.T.: 0.000 min
Response: 110509
Conc: 2.30 ng/ml

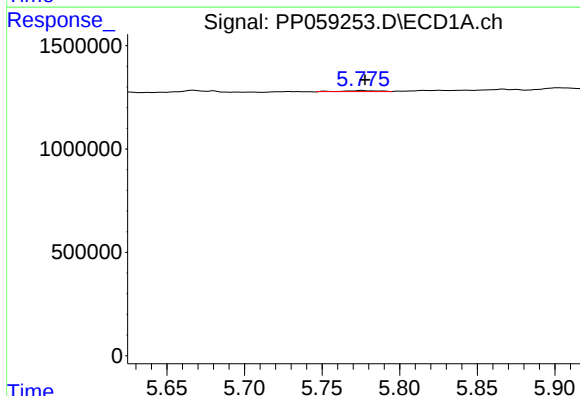


#6 AR-1016-4

R.T.: 5.776 min
Delta R.T.: -0.002 min
Response: 64011
Conc: 2.21 ng/ml

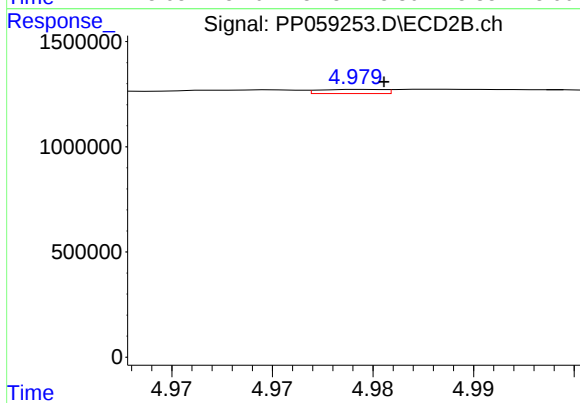

#6 AR-1016-4


R.T.: 4.980 min
Delta R.T.: 0.000 min
Response: 44247
Conc: 1.07 ng/ml

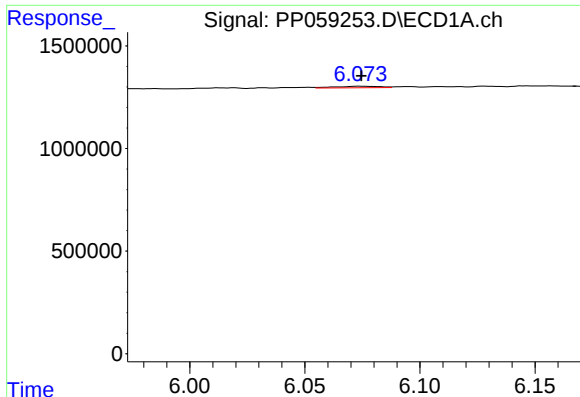

#7 AR-1016-5


R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 96199
Conc: 3.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

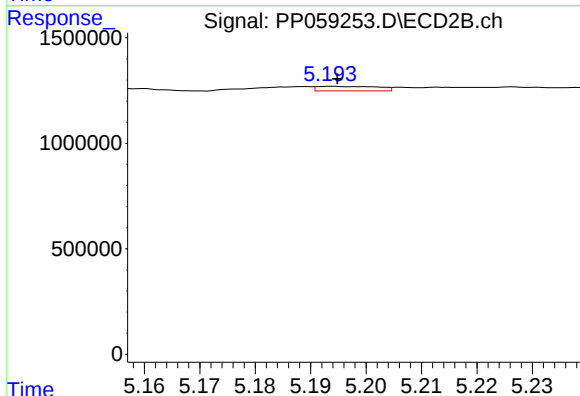


#7 AR-1016-5

R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 164823
Conc: 3.17 ng/ml

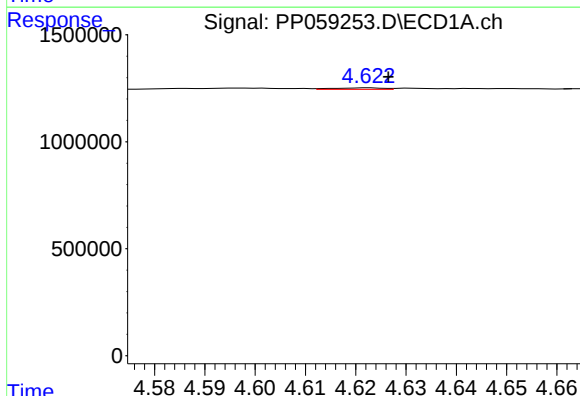


#8 AR-1221-1

R.T.: 4.623 min
Delta R.T.: -0.004 min
Response: 49131
Conc: 3.12 ng/ml

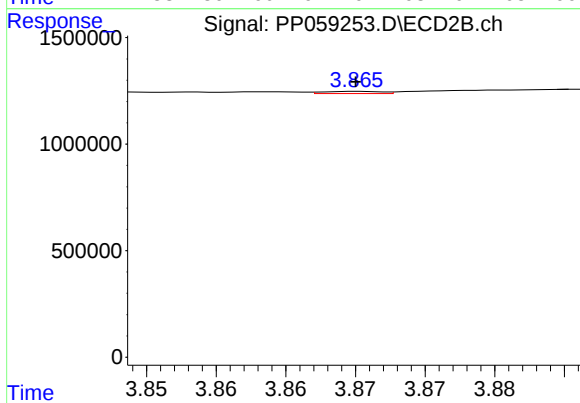

#8 AR-1221-1


R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 28856
Conc: 1.06 ng/ml

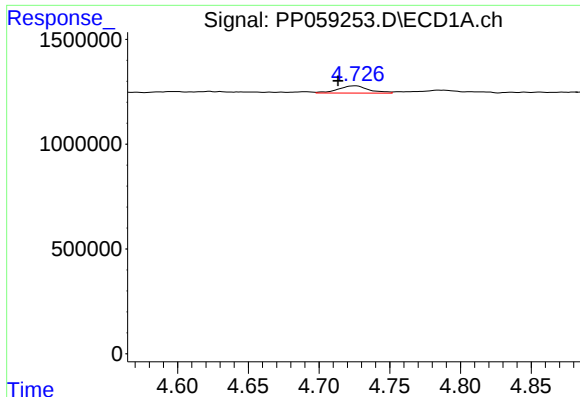

#9 AR-1221-2


R.T.: 4.726 min
Delta R.T.: 0.012 min
Response: 534377
Conc: 45.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

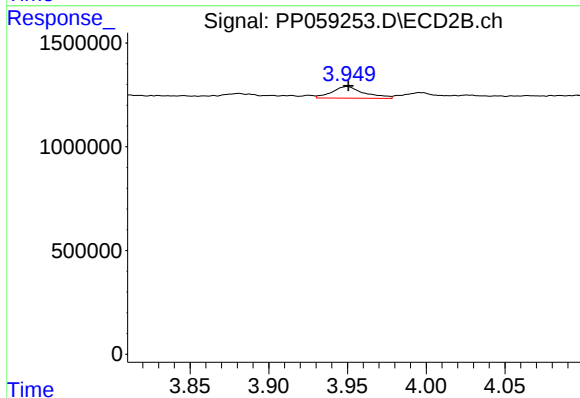


#9 AR-1221-2

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 798695
Conc: 40.12 ng/ml

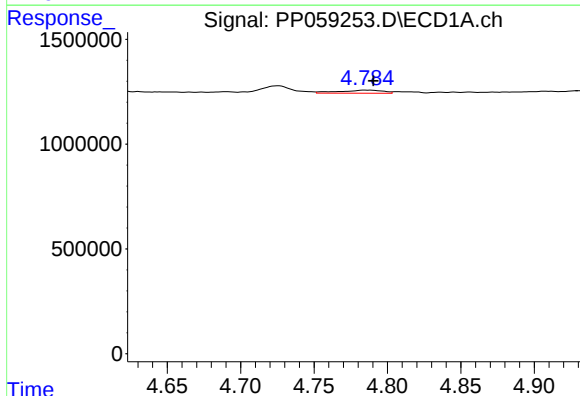


#10 AR-1221-3

R.T.: 4.785 min
Delta R.T.: -0.005 min
Response: 314927
Conc: 8.94 ng/ml

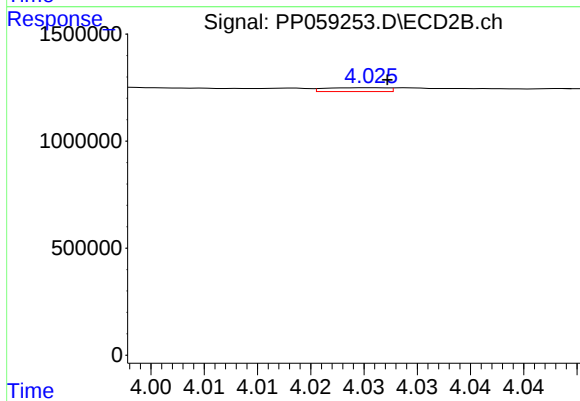

#10 AR-1221-3


R.T.: 4.026 min
Delta R.T.: -0.001 min
Response: 72426
Conc: 1.22 ng/ml

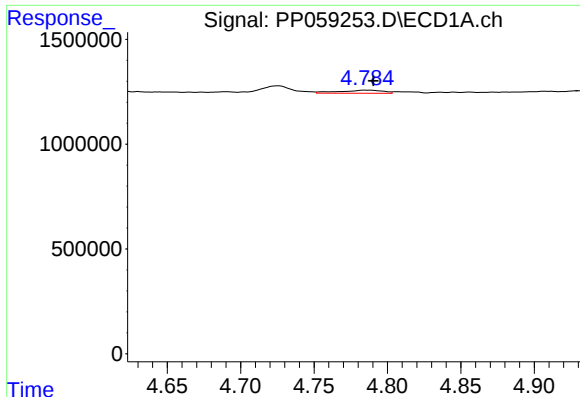

#11 AR-1232-1


R.T.: 4.785 min
Delta R.T.: -0.005 min
Response: 314927
Conc: 10.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

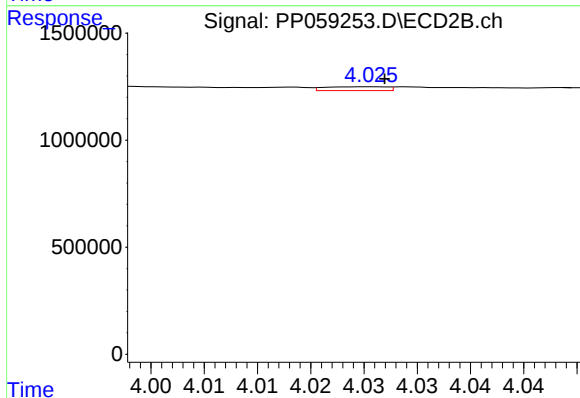


#11 AR-1232-1

R.T.: 4.026 min
Delta R.T.: -0.001 min
Response: 72426
Conc: 1.53 ng/ml

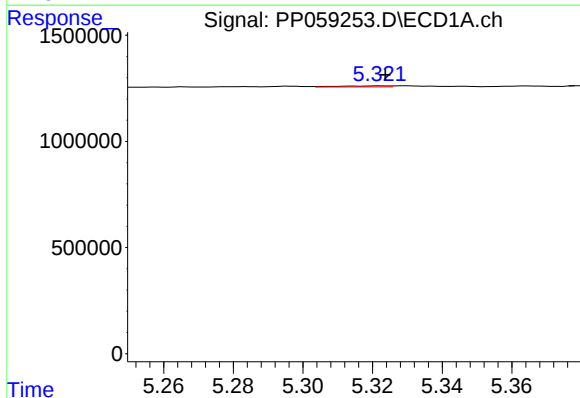


#12 AR-1232-2

R.T.: 5.322 min
Delta R.T.: -0.002 min
Response: 45738
Conc: 2.93 ng/ml

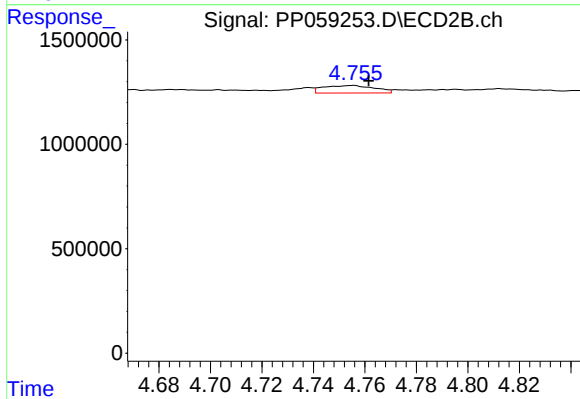

#12 AR-1232-2


R.T.: 4.756 min
Delta R.T.: -0.006 min
Response: 494360
Conc: 11.65 ng/ml

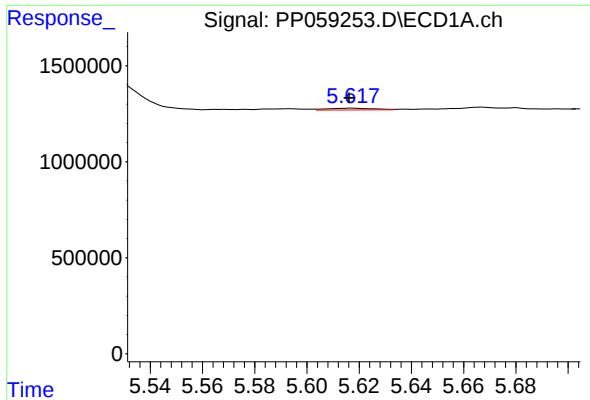

#13 AR-1232-3


R.T.: 5.617 min
Delta R.T.: 0.001 min
Response: 115069
Conc: 4.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

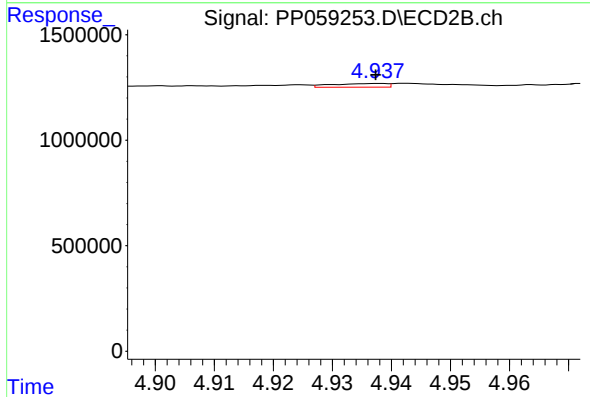


#13 AR-1232-3

R.T.: 4.938 min
Delta R.T.: 0.000 min
Response: 110509
Conc: 4.98 ng/ml

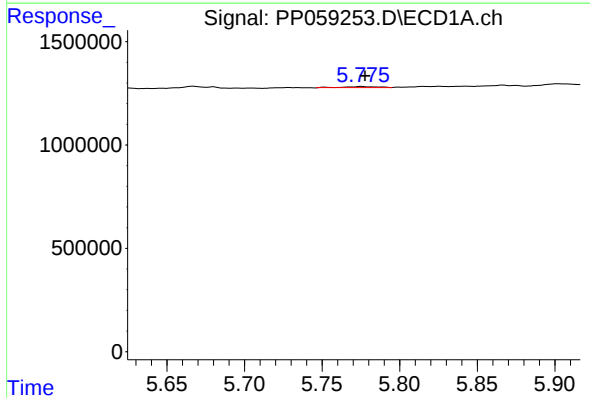


#14 AR-1232-4

R.T.: 5.776 min
Delta R.T.: -0.002 min
Response: 64011
Conc: 4.84 ng/ml

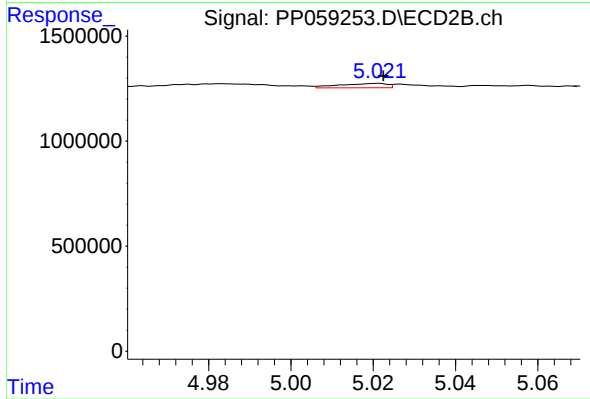

#14 AR-1232-4


R.T.: 5.021 min
Delta R.T.: -0.001 min
Response: 167191
Conc: 7.92 ng/ml

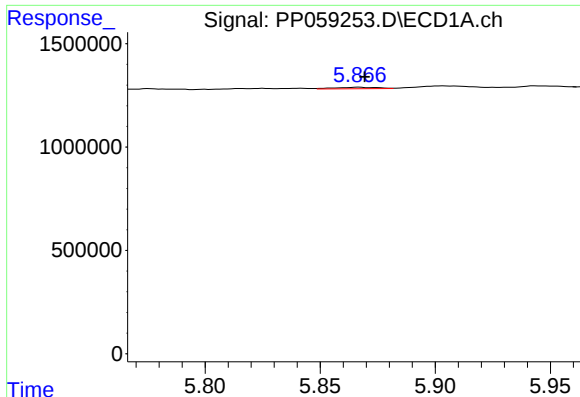

#15 AR-1232-5


R.T.: 5.867 min
Delta R.T.: -0.003 min
Response: 88134
Conc: 7.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

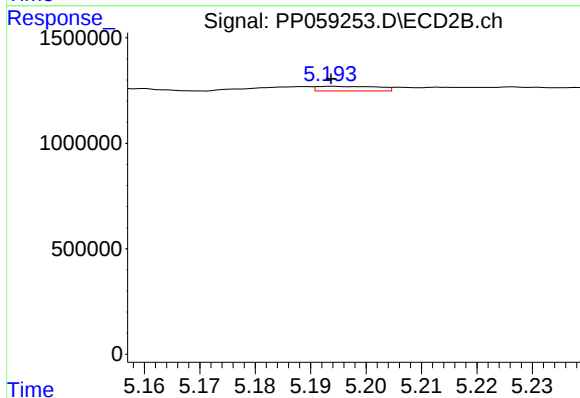


#15 AR-1232-5

R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 164823
Conc: 7.19 ng/ml

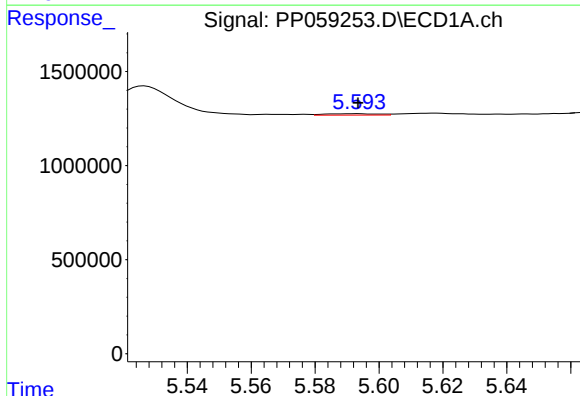


#16 AR-1242-1

R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 87873
Conc: 2.57 ng/ml

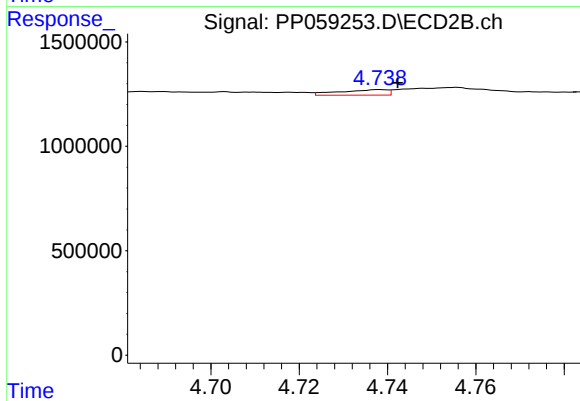

#16 AR-1242-1


R.T.: 4.738 min
Delta R.T.: -0.004 min
Response: 194972
Conc: 3.48 ng/ml

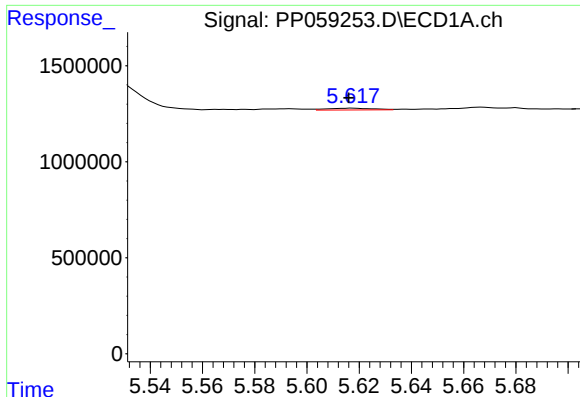

#17 AR-1242-2


R.T.: 5.617 min
Delta R.T.: 0.002 min
Response: 115069
Conc: 2.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

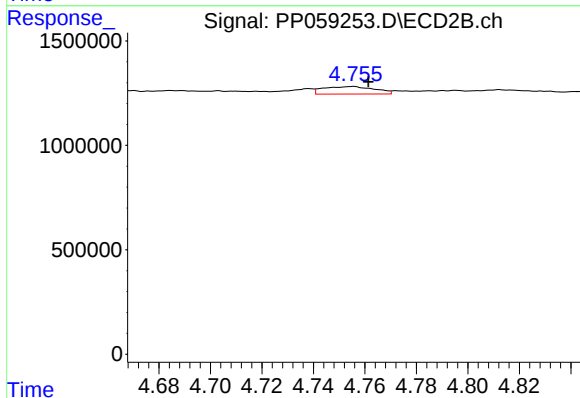


#17 AR-1242-2

R.T.: 4.756 min
Delta R.T.: -0.006 min
Response: 494360
Conc: 6.20 ng/ml

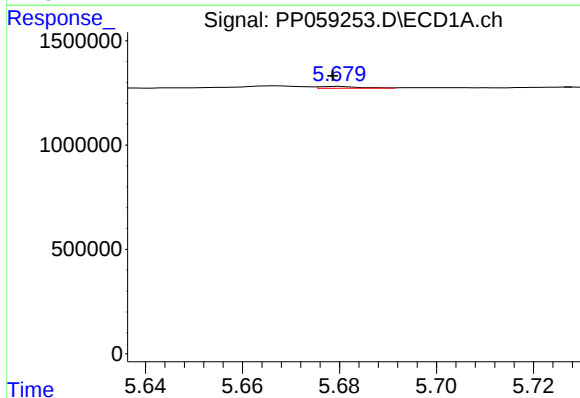


#18 AR-1242-3

R.T.: 5.680 min
Delta R.T.: 0.001 min
Response: 47572
Conc: 1.51 ng/ml

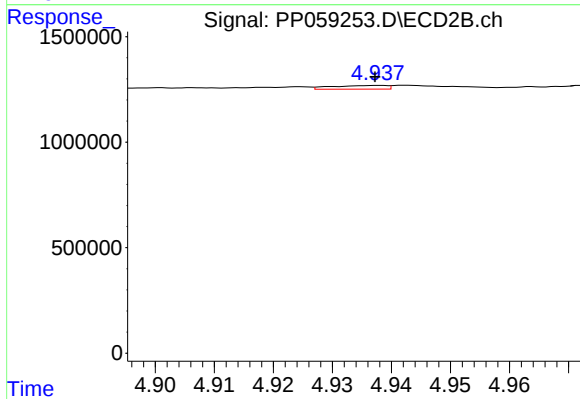

#18 AR-1242-3


R.T.: 4.938 min
Delta R.T.: 0.000 min
Response: 110509
Conc: 2.59 ng/ml

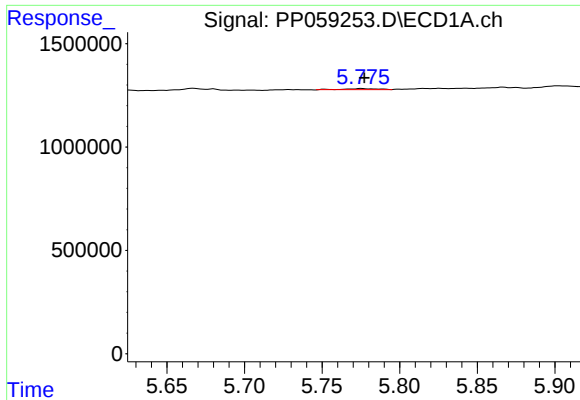

#19 AR-1242-4


R.T.: 5.776 min
Delta R.T.: -0.002 min
Response: 64011
Conc: 2.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

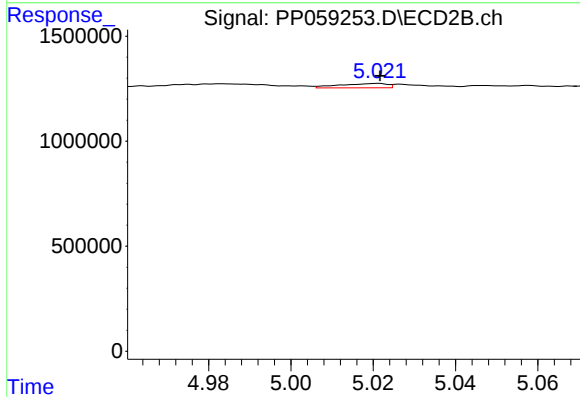


#19 AR-1242-4

R.T.: 5.021 min
Delta R.T.: 0.000 min
Response: 167191
Conc: 3.83 ng/ml

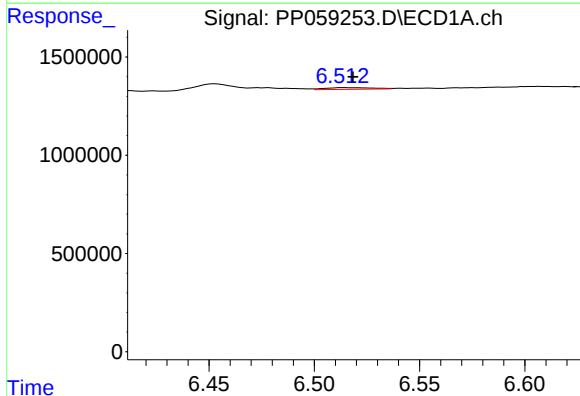


#20 AR-1242-5

R.T.: 6.514 min
Delta R.T.: -0.005 min
Response: 133556
Conc: 5.17 ng/ml

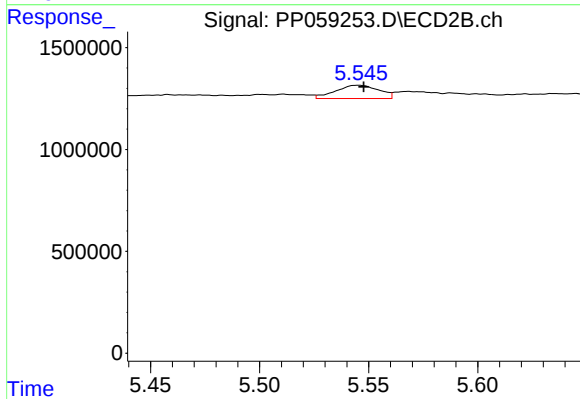

#20 AR-1242-5


R.T.: 5.546 min
Delta R.T.: -0.002 min
Response: 898429
Conc: 18.09 ng/ml

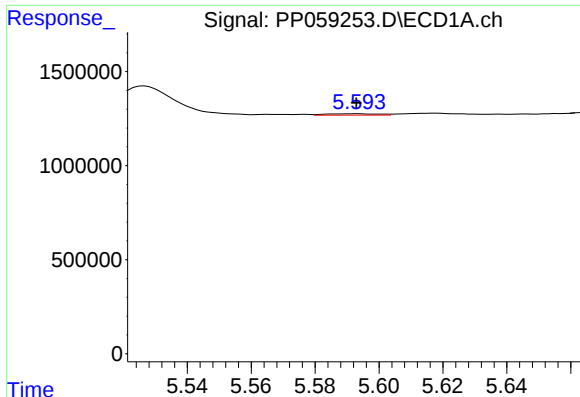

#21 AR-1248-1


R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 87873
Conc: 3.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

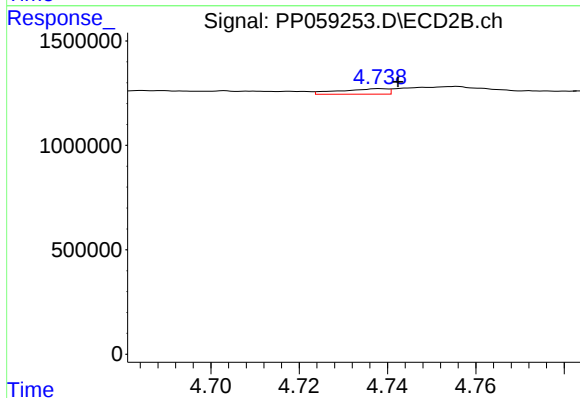


#21 AR-1248-1

R.T.: 4.738 min
Delta R.T.: -0.004 min
Response: 194972
Conc: 4.74 ng/ml

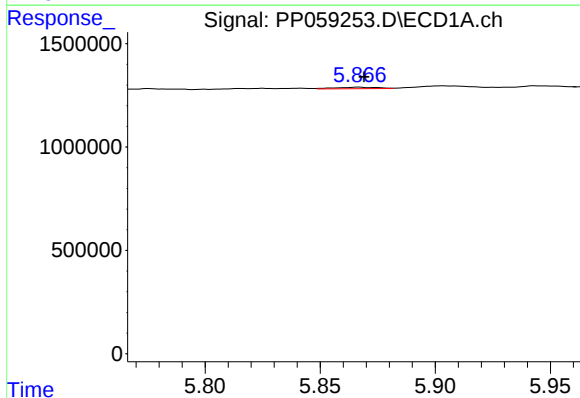


#22 AR-1248-2

R.T.: 5.867 min
Delta R.T.: -0.002 min
Response: 88134
Conc: 2.28 ng/ml

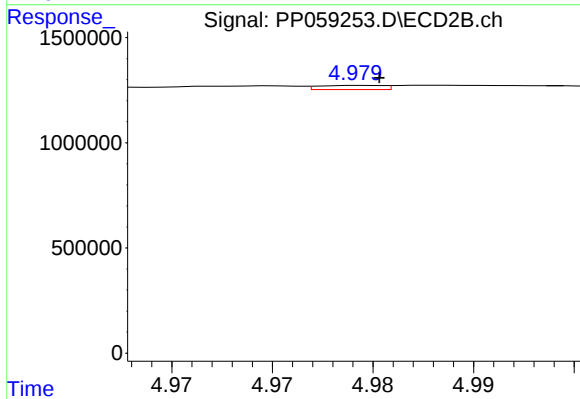

#22 AR-1248-2


R.T.: 4.980 min
Delta R.T.: 0.000 min
Response: 44247
Conc: 0.73 ng/ml

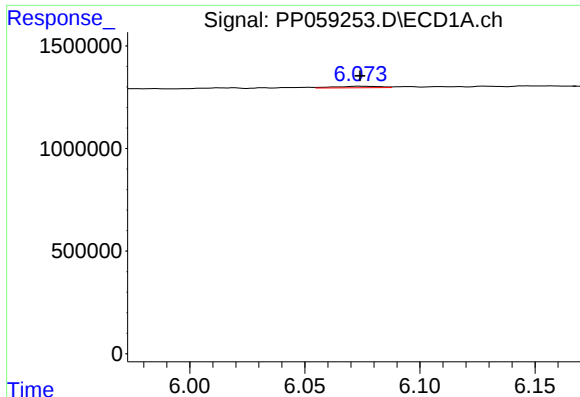

#23 AR-1248-3


R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 96199
Conc: 2.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

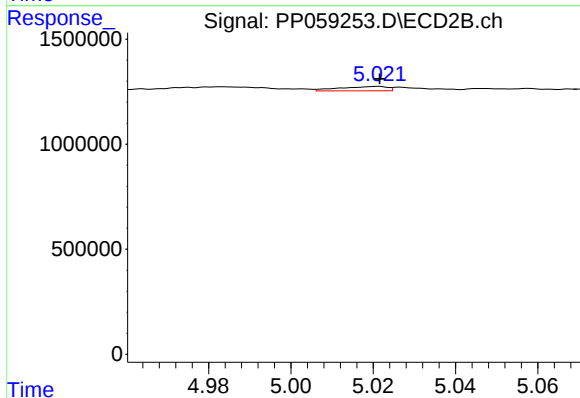


#23 AR-1248-3

R.T.: 5.021 min
Delta R.T.: 0.000 min
Response: 167191
Conc: 2.71 ng/ml

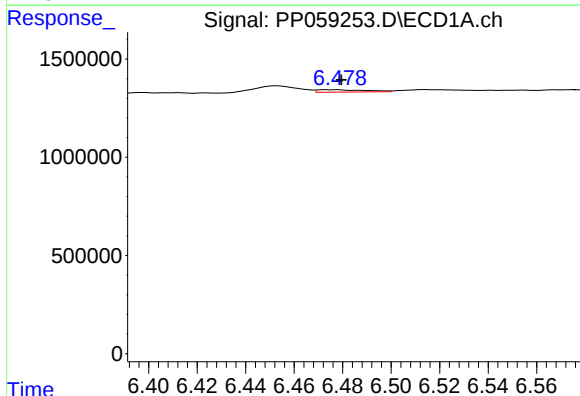


#24 AR-1248-4

R.T.: 6.478 min
Delta R.T.: -0.001 min
Response: 162136
Conc: 3.89 ng/ml

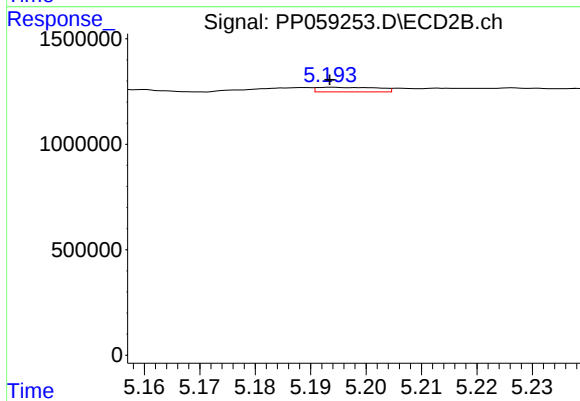

#24 AR-1248-4


R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 164823
Conc: 2.29 ng/ml

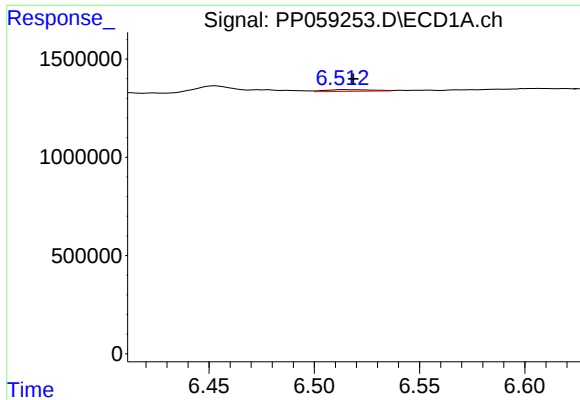

#25 AR-1248-5


R.T.: 6.514 min
Delta R.T.: -0.005 min
Response: 133556
Conc: 3.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

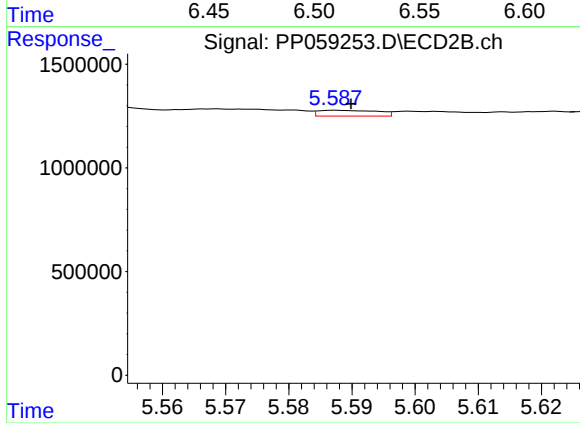


#25 AR-1248-5

R.T.: 5.587 min
Delta R.T.: -0.002 min
Response: 179038
Conc: 2.71 ng/ml

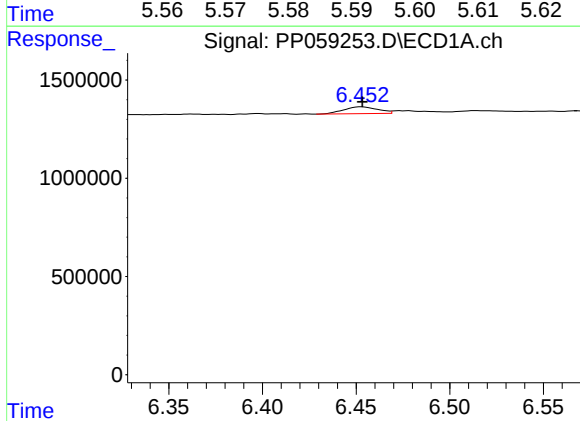


#26 AR-1254-1

R.T.: 6.453 min
Delta R.T.: 0.000 min
Response: 440262
Conc: 9.42 ng/ml

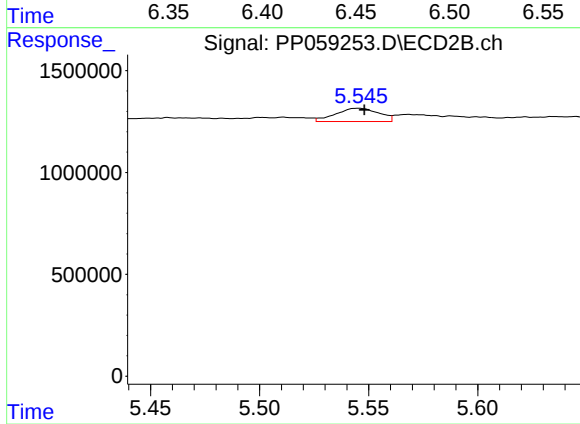

#26 AR-1254-1


R.T.: 5.546 min
Delta R.T.: -0.002 min
Response: 898429
Conc: 8.87 ng/ml

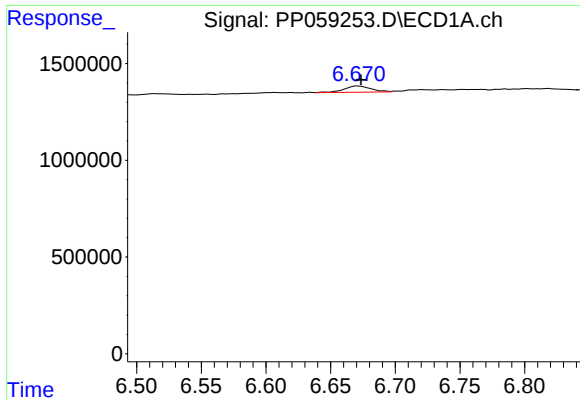

#27 AR-1254-2


R.T.: 6.671 min
Delta R.T.: -0.003 min
Response: 461663
Conc: 6.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

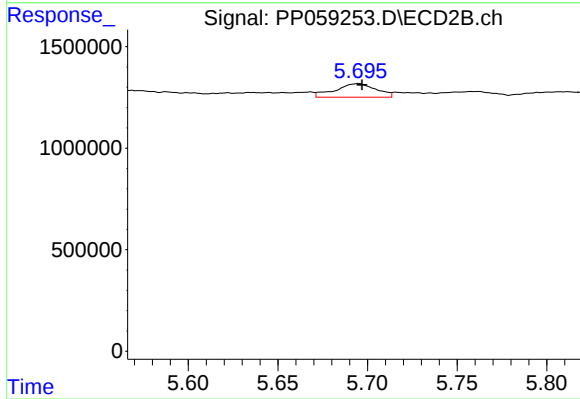


#27 AR-1254-2

R.T.: 5.695 min
Delta R.T.: -0.002 min
Response: 1068825
Conc: 12.11 ng/ml

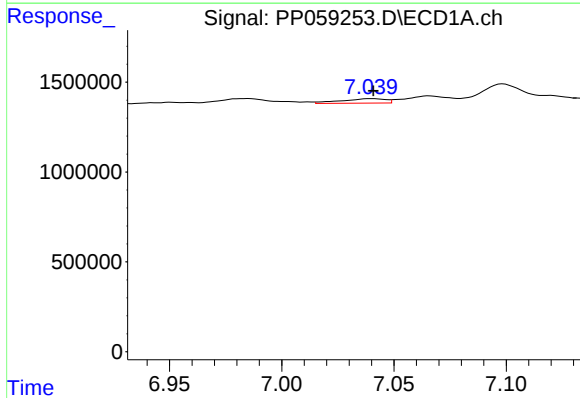


#28 AR-1254-3

R.T.: 7.040 min
Delta R.T.: 0.000 min
Response: 340972
Conc: 4.94 ng/ml

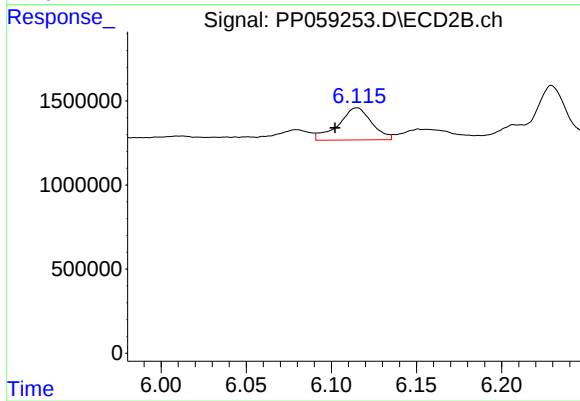

#28 AR-1254-3


R.T.: 6.115 min
Delta R.T.: 0.013 min
Response: 2605338
Conc: 18.85 ng/ml

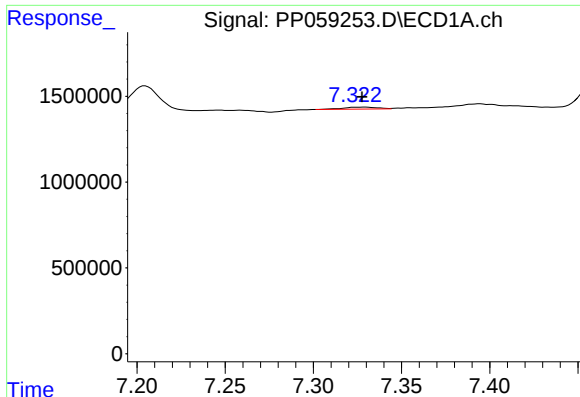

#29 AR-1254-4


R.T.: 7.329 min
Delta R.T.: 0.002 min
Response: 151193
Conc: 3.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

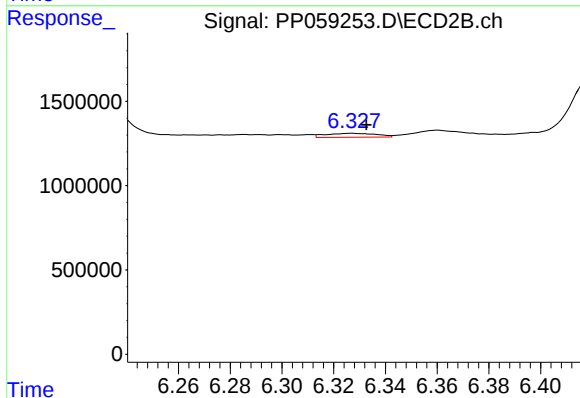


#29 AR-1254-4

R.T.: 6.327 min
Delta R.T.: -0.005 min
Response: 316641
Conc: 3.94 ng/ml

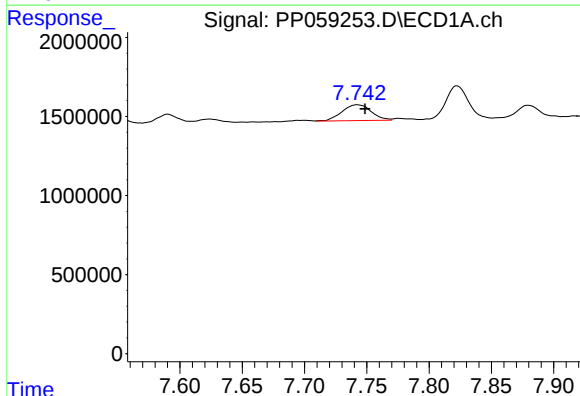


#30 AR-1254-5

R.T.: 7.743 min
Delta R.T.: -0.006 min
Response: 1630352
Conc: 34.70 ng/ml

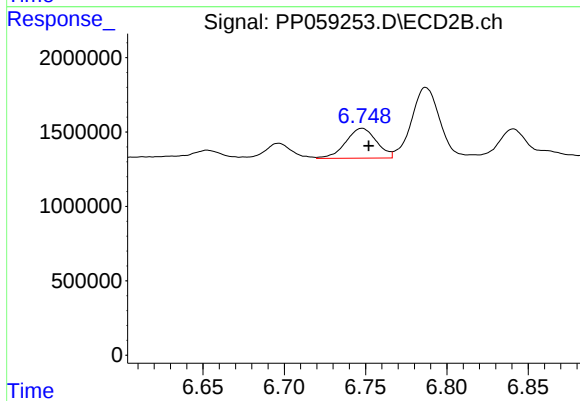

#30 AR-1254-5


R.T.: 6.748 min
Delta R.T.: -0.004 min
Response: 2639599
Conc: 22.07 ng/ml

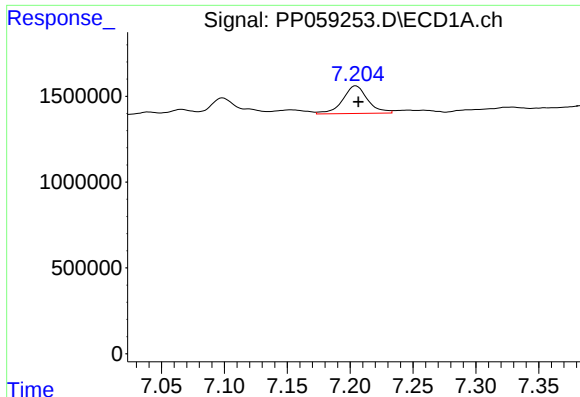

#31 AR-1260-1


R.T.: 7.205 min
Delta R.T.: -0.002 min
Response: 2229863
Conc: 40.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

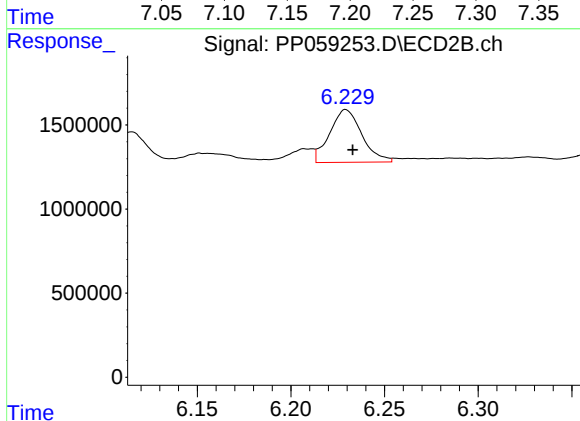


#31 AR-1260-1

R.T.: 6.229 min
Delta R.T.: -0.004 min
Response: 3741041
Conc: 37.77 ng/ml

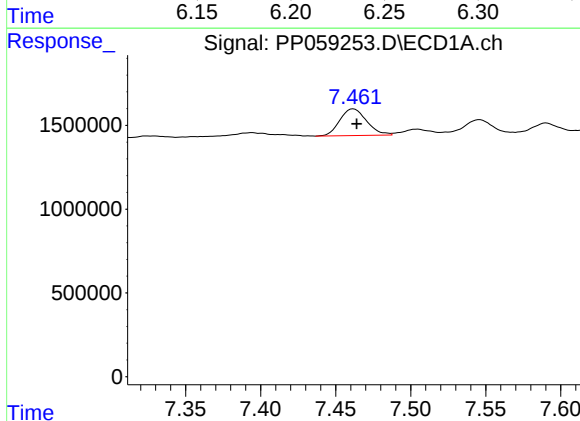


#32 AR-1260-2

R.T.: 7.462 min
Delta R.T.: -0.002 min
Response: 1978702
Conc: 33.23 ng/ml

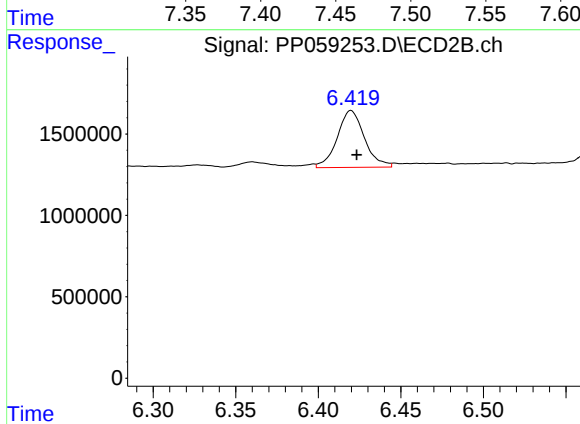

#32 AR-1260-2


R.T.: 6.420 min
Delta R.T.: -0.003 min
Response: 4005840
Conc: 34.62 ng/ml

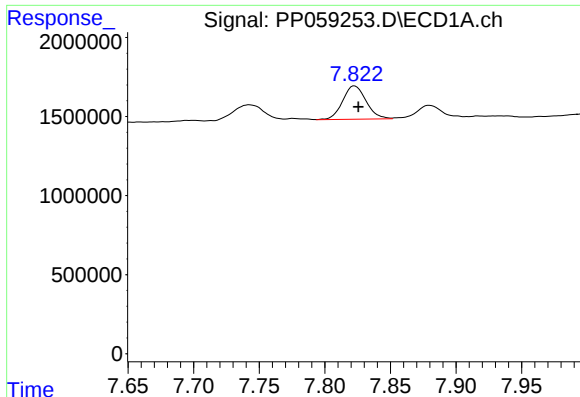

#33 AR-1260-3


R.T.: 7.823 min
Delta R.T.: -0.003 min
Response: 2625090
Conc: 66.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

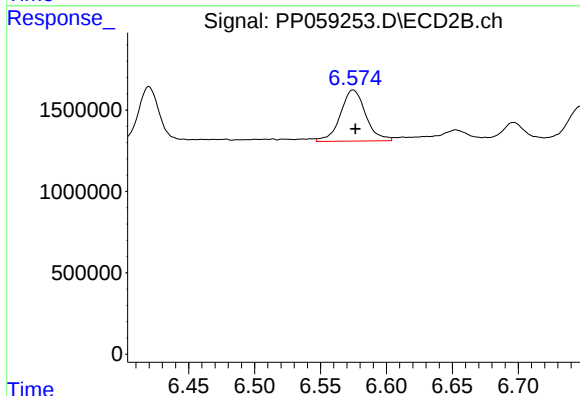


#33 AR-1260-3

R.T.: 6.575 min
Delta R.T.: -0.002 min
Response: 4216081
Conc: 37.90 ng/ml

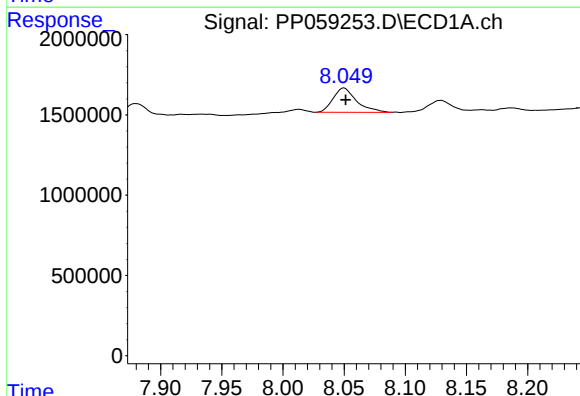


#34 AR-1260-4

R.T.: 8.050 min
Delta R.T.: -0.001 min
Response: 2036266
Conc: 45.85 ng/ml

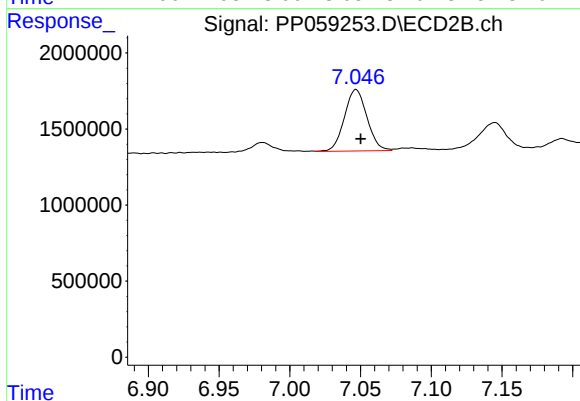

#34 AR-1260-4


R.T.: 7.047 min
Delta R.T.: -0.003 min
Response: 4473369
Conc: 51.60 ng/ml

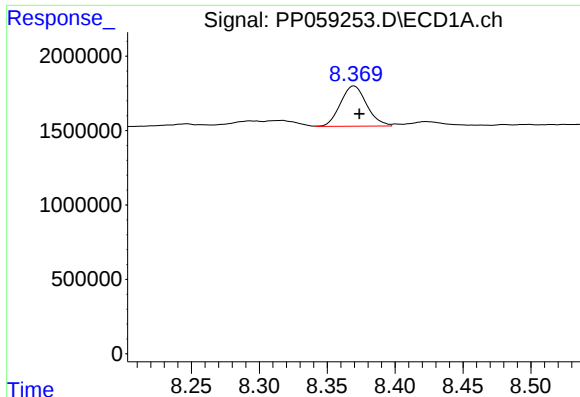

#35 AR-1260-5


R.T.: 8.370 min
Delta R.T.: -0.004 min
Response: 3637851
Conc: 45.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

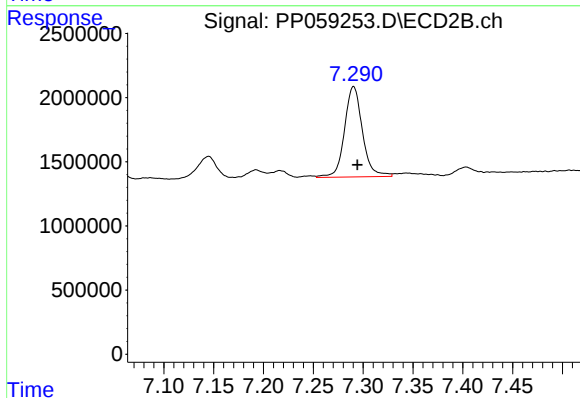


#35 AR-1260-5

R.T.: 7.290 min
Delta R.T.: -0.004 min
Response: 8814870
Conc: 47.82 ng/ml

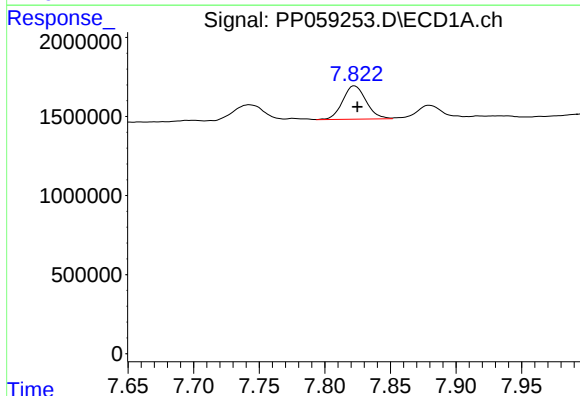


#36 AR-1262-1

R.T.: 7.823 min
Delta R.T.: -0.002 min
Response: 2625090
Conc: 41.22 ng/ml

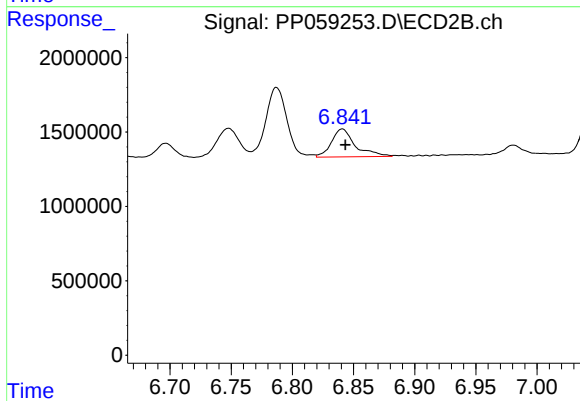

#36 AR-1262-1


R.T.: 6.841 min
Delta R.T.: -0.002 min
Response: 2543658
Conc: 44.21 ng/ml

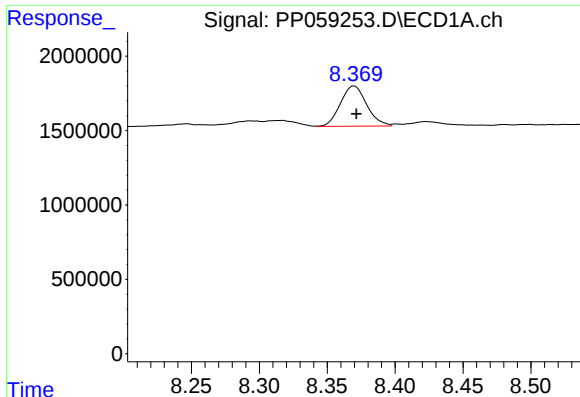

#37 AR-1262-2


R.T.: 8.370 min
Delta R.T.: -0.002 min
Response: 3637851
Conc: 39.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

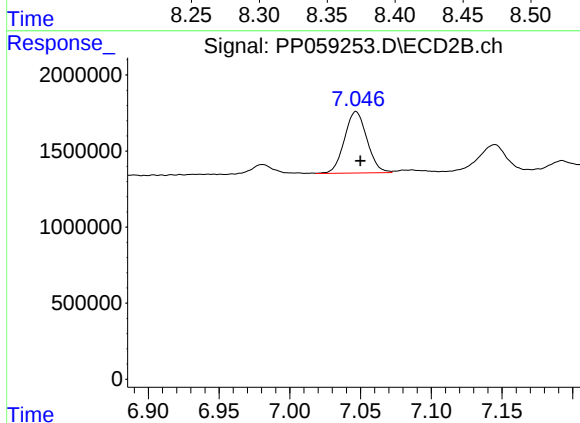


#37 AR-1262-2

R.T.: 7.047 min
Delta R.T.: -0.003 min
Response: 4473369
Conc: 37.91 ng/ml

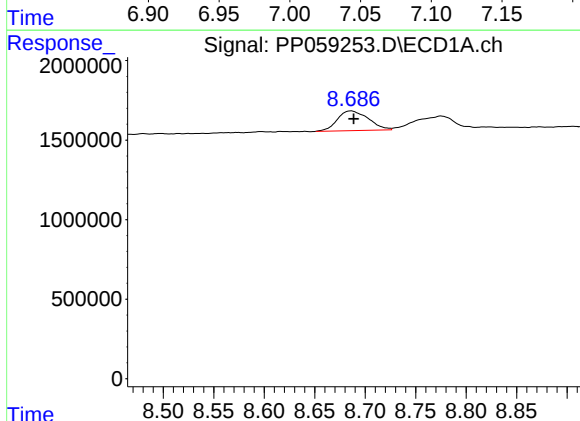


#38 AR-1262-3

R.T.: 8.686 min
Delta R.T.: -0.003 min
Response: 2642210
Conc: 41.06 ng/ml

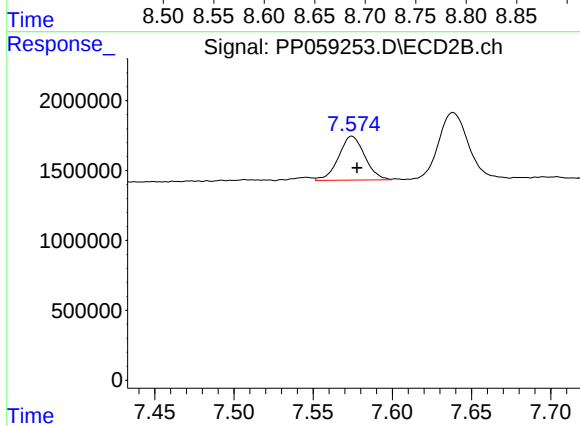

#38 AR-1262-3


R.T.: 7.574 min
Delta R.T.: -0.003 min
Response: 3596699
Conc: 42.26 ng/ml

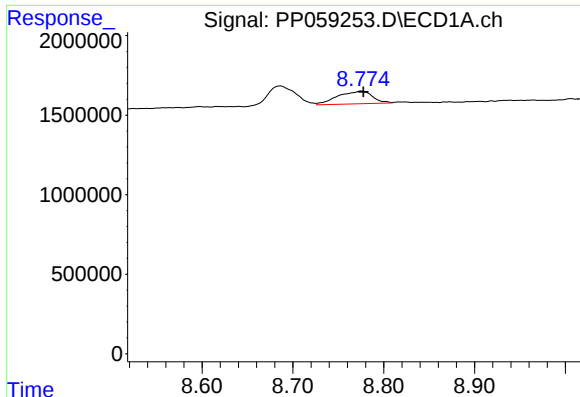

#39 AR-1262-4


R.T.: 8.775 min
Delta R.T.: -0.003 min
Response: 2092595
Conc: 63.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

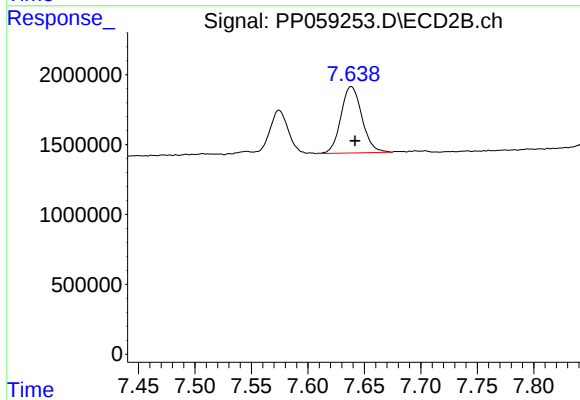


#39 AR-1262-4

R.T.: 7.638 min
Delta R.T.: -0.003 min
Response: 6153756
Conc: 40.74 ng/ml

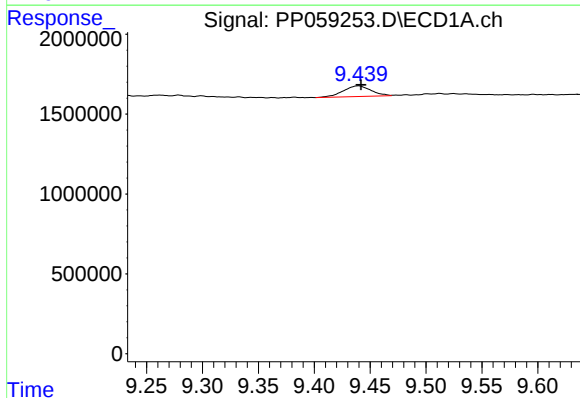


#40 AR-1262-5

R.T.: 9.440 min
Delta R.T.: -0.002 min
Response: 1147886
Conc: 38.47 ng/ml

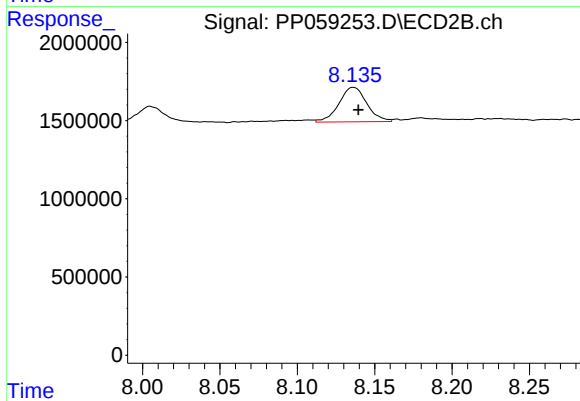

#40 AR-1262-5


R.T.: 8.136 min
Delta R.T.: -0.003 min
Response: 2757987
Conc: 43.25 ng/ml

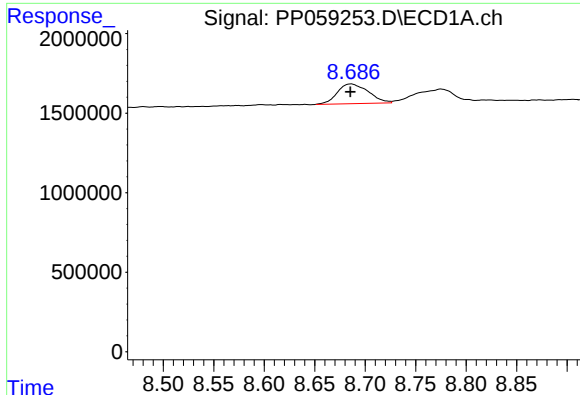

#41 AR-1268-1


R.T.: 8.686 min
Delta R.T.: 0.000 min
Response: 2642210
Conc: 23.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

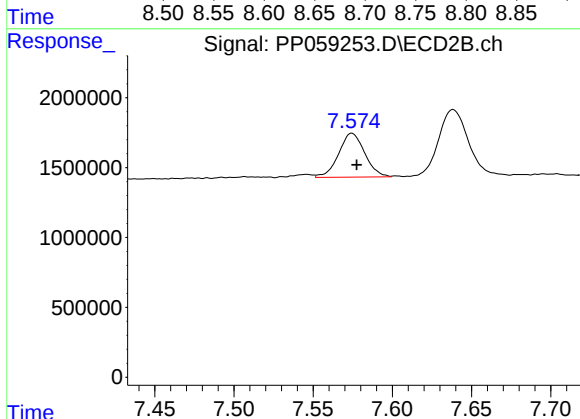


#41 AR-1268-1

R.T.: 7.574 min
Delta R.T.: -0.003 min
Response: 3596699
Conc: 14.75 ng/ml

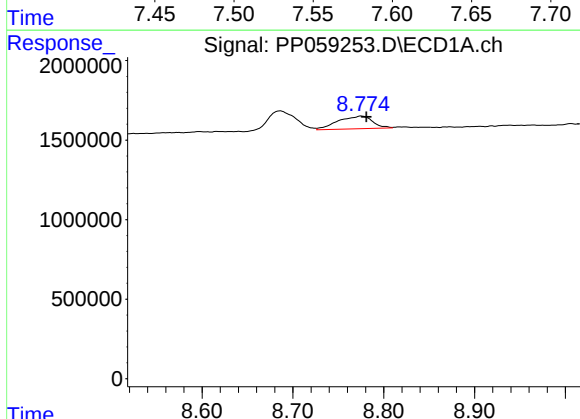


#42 AR-1268-2

R.T.: 8.775 min
Delta R.T.: -0.006 min
Response: 2092595
Conc: 21.26 ng/ml

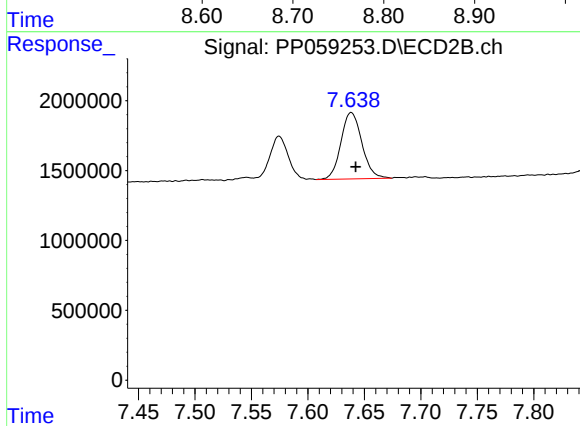

#42 AR-1268-2


R.T.: 7.638 min
Delta R.T.: -0.004 min
Response: 6153756
Conc: 28.10 ng/ml

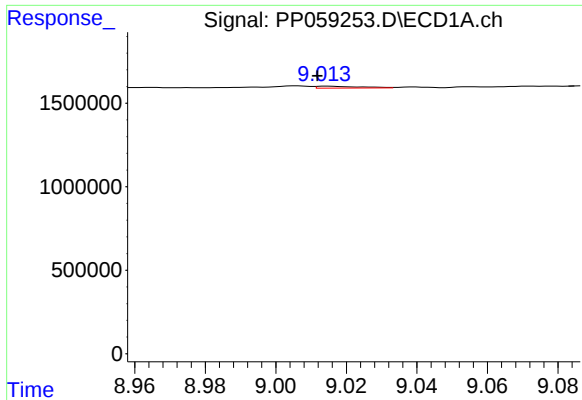

#43 AR-1268-3


R.T.: 9.015 min
Delta R.T.: 0.003 min
Response: 97117
Conc: 1.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

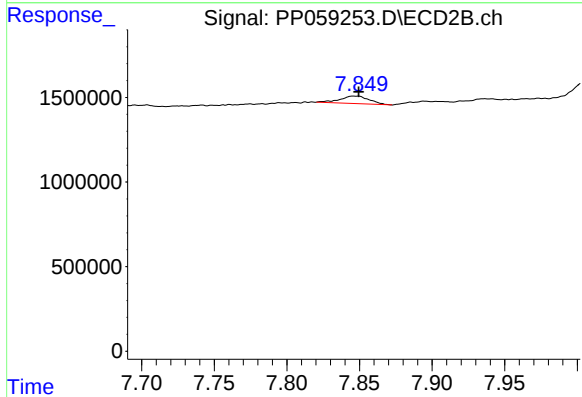


#43 AR-1268-3

R.T.: 7.846 min
Delta R.T.: -0.004 min
Response: 629978
Conc: 3.22 ng/ml

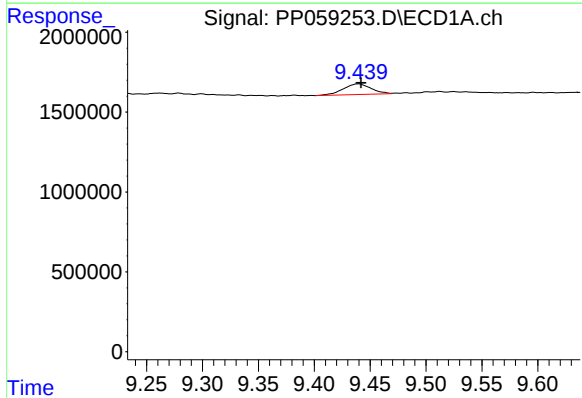


#44 AR-1268-4

R.T.: 9.440 min
Delta R.T.: -0.002 min
Response: 1147886
Conc: 35.98 ng/ml

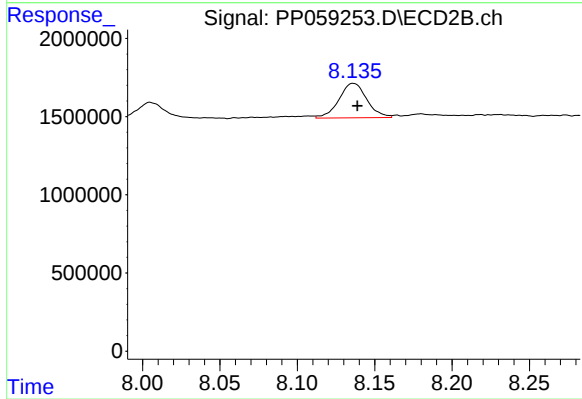

#44 AR-1268-4


R.T.: 8.136 min
Delta R.T.: -0.003 min
Response: 2757987
Conc: 39.63 ng/ml

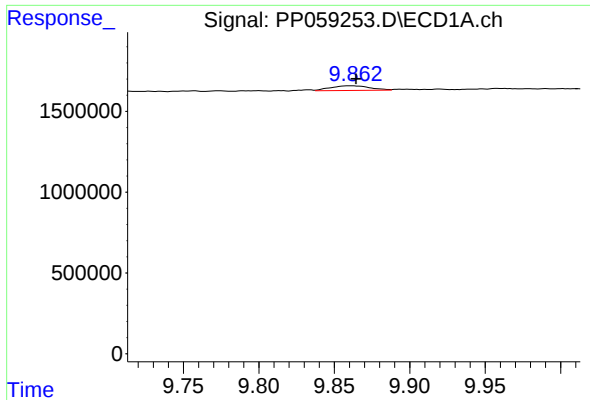

#45 AR-1268-5

R.T.: 9.861 min
Delta R.T.: -0.003 min
Response: 526334
Conc: 1.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

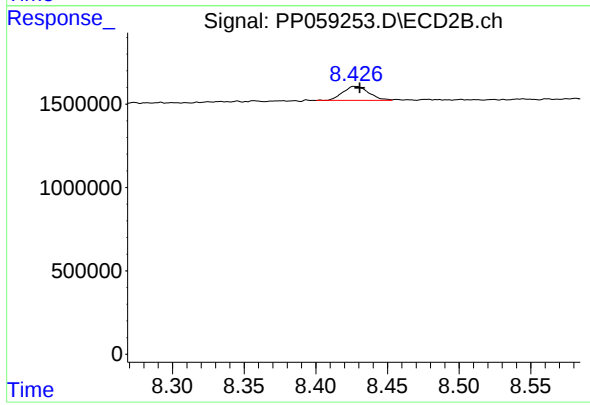

#45 AR-1268-5

R.T.: 8.427 min
Delta R.T.: -0.004 min
Response: 1053411
Conc: 2.03 ng/ml