

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
 Data File : PP059254.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2023 09:45
 Operator : YP\AJ
 Sample : 03572-07
 Misc : AR1268 LOD 40 PPB
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 11:03:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.415	3.648	23801686	40619902	19.398	20.048
2)	SA Decachlor...	10.207	8.684	20226972	37344208	26.502	26.545
Target Compounds							
3)	L1 AR-1016-1	5.593	4.740	99198	190349	2.525	2.968
4)	L1 AR-1016-2	5.619	4.756	149570	319438	2.638	3.517 #
5)	L1 AR-1016-3	5.670	4.940	153290	116729	4.273	2.429 #
6)	L1 AR-1016-4	5.780	4.983	14034	389329	0.484	9.429 #
7)	L1 AR-1016-5	6.076	5.192	165130	65308	5.456	1.255 #
8)	L2 AR-1221-1	4.627	3.860	61237	35715	3.887	1.316 #
9)	L2 AR-1221-2	4.724	3.950	774539	775921	65.589	38.972 #
10)	L2 AR-1221-3	4.791	4.025	559119	89992	15.878	1.512 #
11)	L3 AR-1232-1	4.791	4.025	559119	89992	19.020	1.897 #
12)	L3 AR-1232-2	5.329	4.756	67035	319438	4.301	7.531 #
13)	L3 AR-1232-3	5.619	4.940	149570	116729	5.664	5.261
14)	L3 AR-1232-4	5.780	5.024	14034	189079	1.060	8.955 #
15)	L3 AR-1232-5	5.868	5.192	82458	65308	7.224	2.849 #
16)	L4 AR-1242-1	5.593	4.740	99198	190349	2.898	3.401
17)	L4 AR-1242-2	5.619	4.756	149570	319438	3.048	4.006 #
18)	L4 AR-1242-3	5.670	4.940	153290	116729	4.879	2.739 #
19)	L4 AR-1242-4	5.780	5.020	14034	175258	0.547	4.014 #
20)	L4 AR-1242-5	6.521	5.546	101942	482170	3.946	9.707 #
21)	L5 AR-1248-1	5.593	4.740	99198	190349	3.908	4.627
22)	L5 AR-1248-2	5.868	4.983	82458	389329	2.130	6.465 #
23)	L5 AR-1248-3	6.076	5.020	165130	175258	3.909	2.845 #
24)	L5 AR-1248-4	6.478	5.192	142772	65308	3.429	0.907 #
25)	L5 AR-1248-5	6.521	5.590	101942	167914	2.499	2.545
26)	L6 AR-1254-1	6.453	5.546	316183	482170	6.768	4.759 #
27)	L6 AR-1254-2	6.677	5.701	227476	224625	3.306	2.545
28)	L6 AR-1254-3	7.066f	6.104	1336464	79518	19.363	0.575 #
29)	L6 AR-1254-4	7.333	6.333	89248	93325	1.983	1.161 #
30)	L6 AR-1254-5	7.749	6.753	156728	27676	3.336	0.231 #
31)	L7 AR-1260-1	7.219	6.234	152238	69421	2.783	0.701 #
32)	L7 AR-1260-2	7.477	6.420	786180	111690	13.205	0.965 #
33)	L7 AR-1260-3	7.824	6.559	1228029	2238970	31.204	20.129 #
34)	L7 AR-1260-4	8.070f	7.045	1203923	2981834	27.107	34.394 #
35)	L7 AR-1260-5	8.370	7.290	431408	1509135	5.395	8.187 #
36)	L8 AR-1262-1	7.824	6.844	1228029	37129	19.281	0.645 #
37)	L8 AR-1262-2	8.370	7.045	431408	2981834	4.698	25.270 #
38)	L8 AR-1262-3	8.684	7.576	4713066	10109821	73.238	118.800 #
39)	L8 AR-1262-4	8.779	7.640	4313021	8861216	129.884	58.660 #
40)	L8 AR-1262-5	9.440	8.137	1300456	3109672	43.579	48.759
41)	L9 AR-1268-1	8.684	7.576	4713066	10109821	41.500	41.459

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080823\
Data File : PP059254.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2023 09:45
Operator : YP\AJ
Sample : 03572-07
Misc : AR1268 LOD 40 PPB
ALS Vial : 49 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 11:03:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.779	7.640	4313021	8861216	43.824	40.458
43)	L9 AR-1268-3	9.010	7.847	3856402	8360680	41.598	42.758
44)	L9 AR-1268-4	9.440	8.137	1300456	3109672	40.766	44.686
45)	L9 AR-1268-5	9.862	8.428	11013323	20311690	40.570	39.181


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

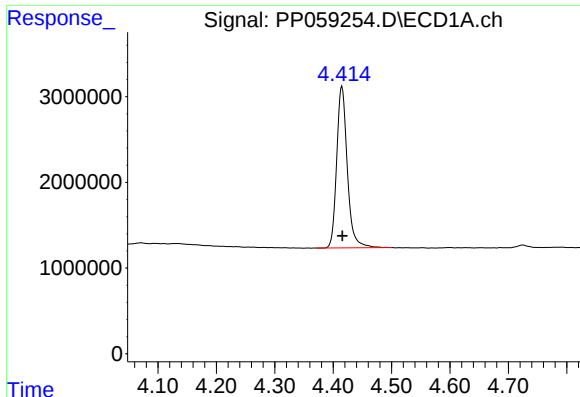

#1 Tetrachloro-m-xylene


R.T.: 4.415 min
Delta R.T.: -0.001 min
Response: 23801686
Conc: 19.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

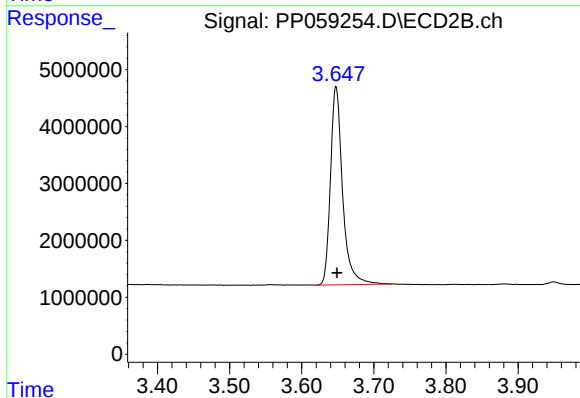


#1 Tetrachloro-m-xylene

R.T.: 3.648 min
Delta R.T.: -0.001 min
Response: 40619902
Conc: 20.05 ng/ml

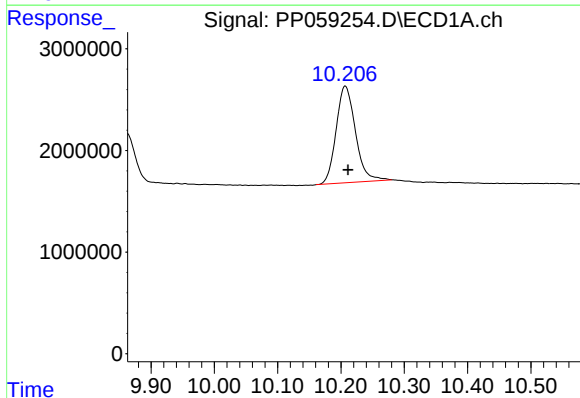


#2 Decachlorobiphenyl

R.T.: 10.207 min
Delta R.T.: -0.004 min
Response: 20226972
Conc: 26.50 ng/ml

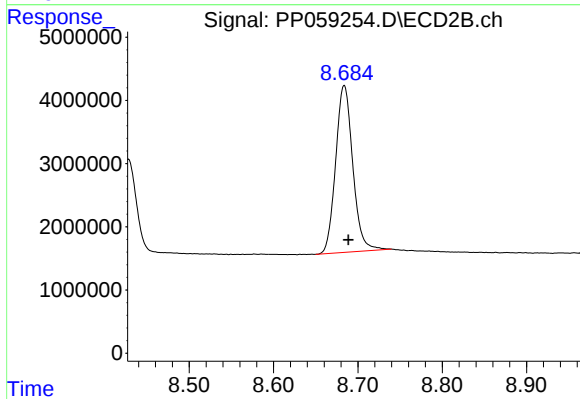

#2 Decachlorobiphenyl


R.T.: 8.684 min
Delta R.T.: -0.005 min
Response: 37344208
Conc: 26.55 ng/ml

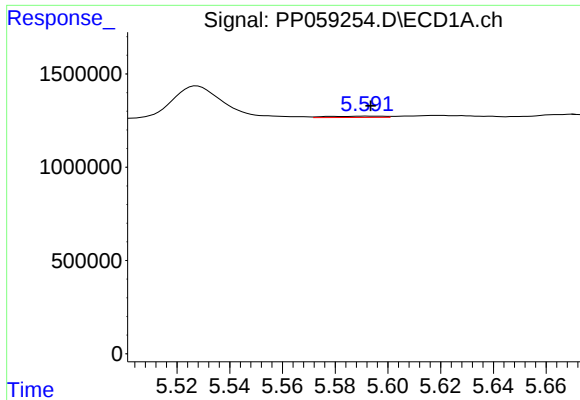

#3 AR-1016-1


R.T.: 5.593 min
Delta R.T.: -0.001 min
Response: 99198
Conc: 2.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

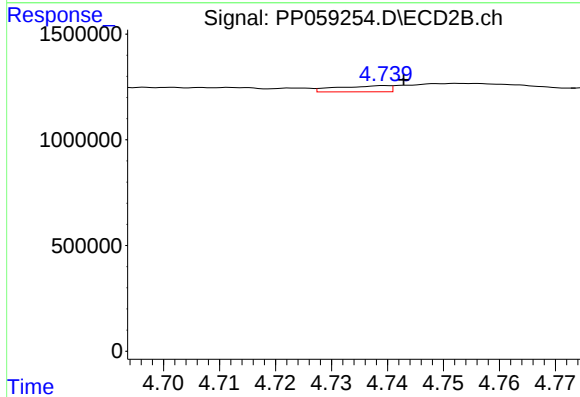


#3 AR-1016-1

R.T.: 4.740 min
Delta R.T.: -0.003 min
Response: 190349
Conc: 2.97 ng/ml

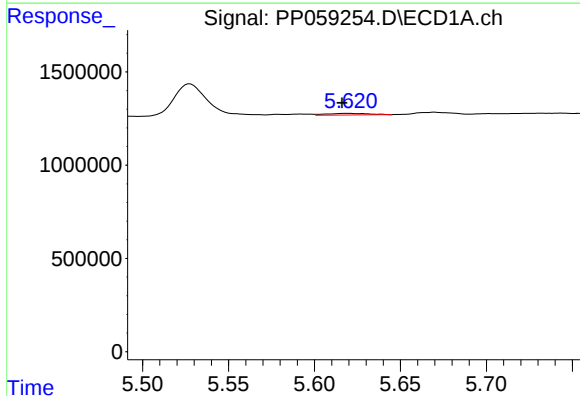


#4 AR-1016-2

R.T.: 5.619 min
Delta R.T.: 0.003 min
Response: 149570
Conc: 2.64 ng/ml

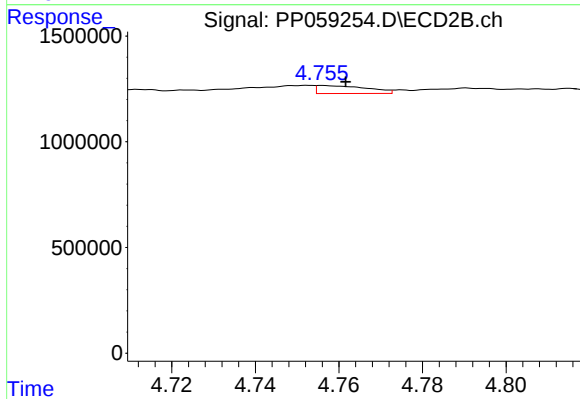

#4 AR-1016-2


R.T.: 4.756 min
Delta R.T.: -0.006 min
Response: 319438
Conc: 3.52 ng/ml

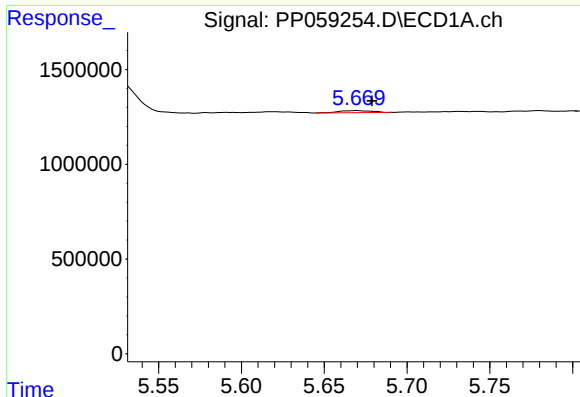

#5 AR-1016-3


R.T.: 5.670 min
Delta R.T.: -0.009 min
Response: 153290
Conc: 4.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

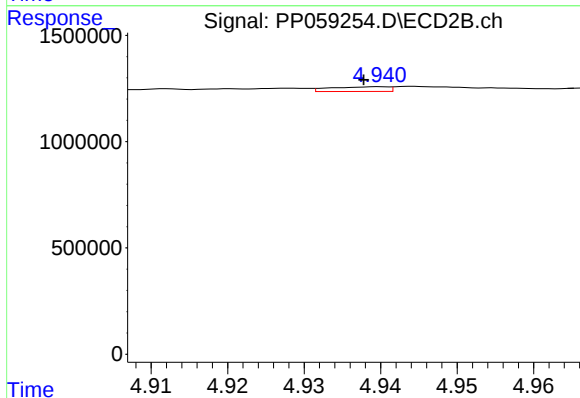


#5 AR-1016-3

R.T.: 4.940 min
Delta R.T.: 0.002 min
Response: 116729
Conc: 2.43 ng/ml

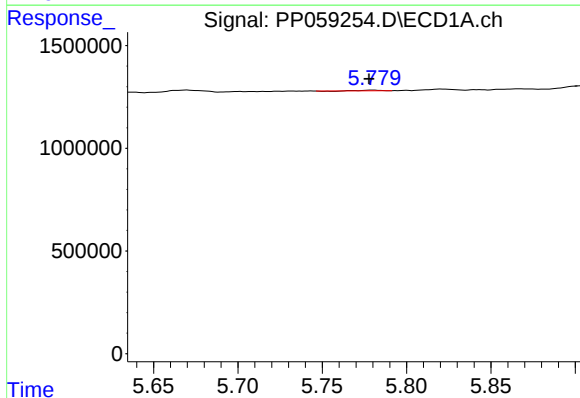


#6 AR-1016-4

R.T.: 5.780 min
Delta R.T.: 0.002 min
Response: 14034
Conc: 0.48 ng/ml

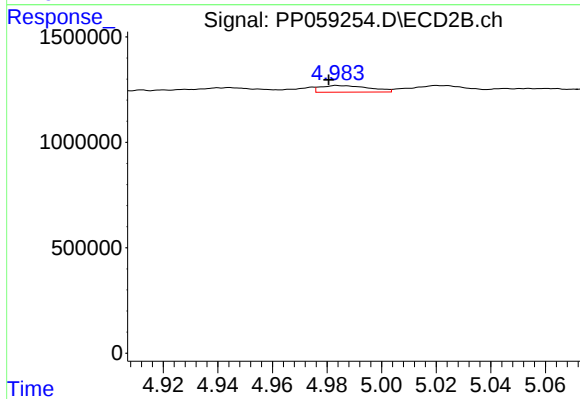

#6 AR-1016-4


R.T.: 4.983 min
Delta R.T.: 0.003 min
Response: 389329
Conc: 9.43 ng/ml

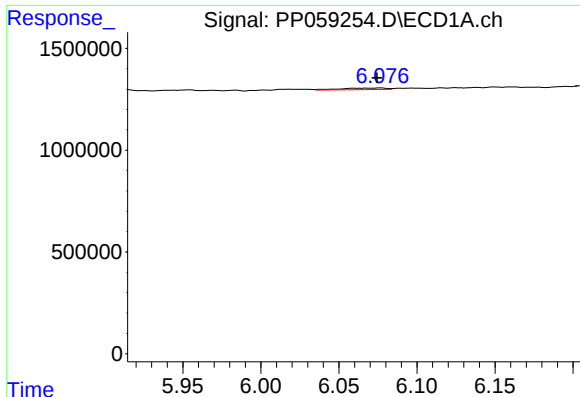

#7 AR-1016-5


R.T.: 6.076 min
Delta R.T.: 0.002 min
Response: 165130
Conc: 5.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

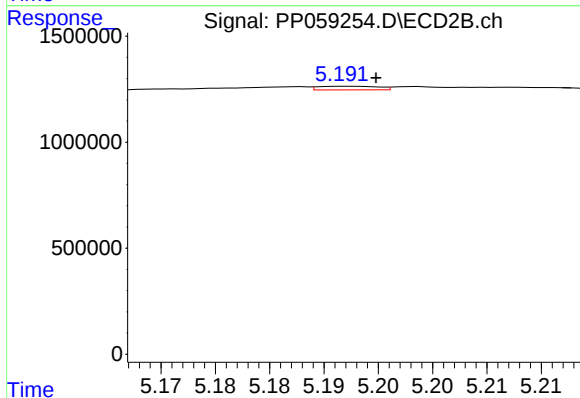


#7 AR-1016-5

R.T.: 5.192 min
Delta R.T.: -0.003 min
Response: 65308
Conc: 1.26 ng/ml

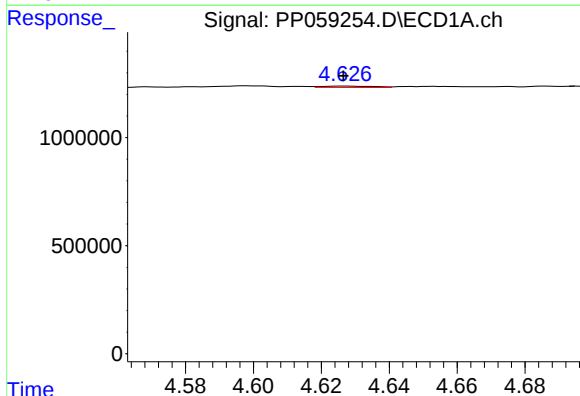


#8 AR-1221-1

R.T.: 4.627 min
Delta R.T.: 0.000 min
Response: 61237
Conc: 3.89 ng/ml

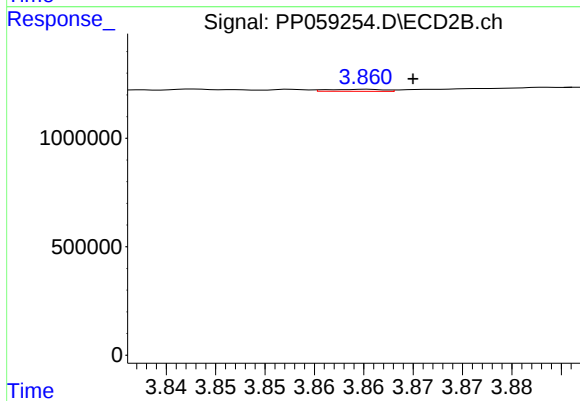

#8 AR-1221-1


R.T.: 3.860 min
Delta R.T.: -0.005 min
Response: 35715
Conc: 1.32 ng/ml

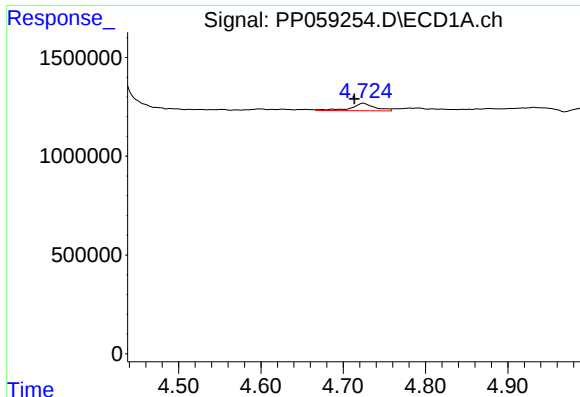

#9 AR-1221-2


R.T.: 4.724 min
Delta R.T.: 0.011 min
Response: 774539
Conc: 65.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

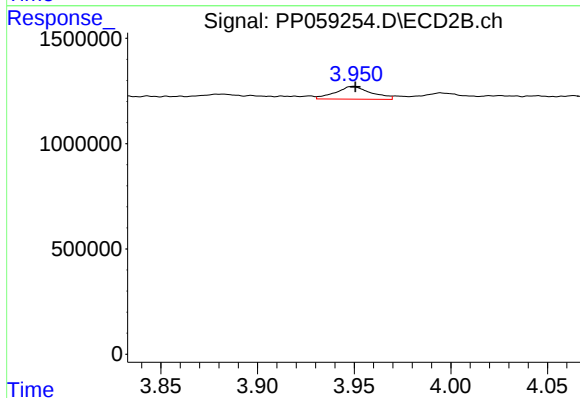


#9 AR-1221-2

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 775921
Conc: 38.97 ng/ml

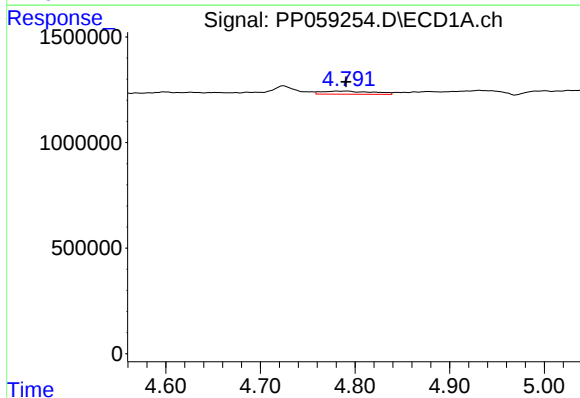


#10 AR-1221-3

R.T.: 4.791 min
Delta R.T.: 0.000 min
Response: 559119
Conc: 15.88 ng/ml

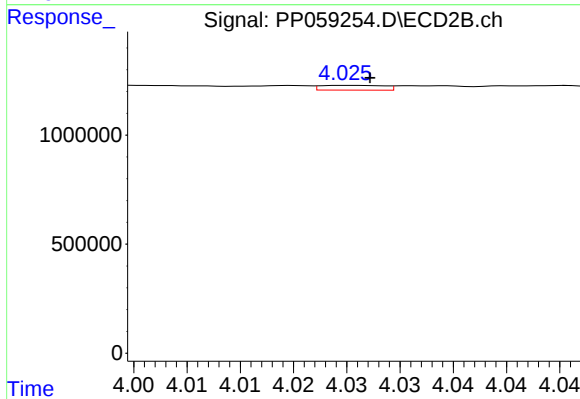

#10 AR-1221-3


R.T.: 4.025 min
Delta R.T.: -0.002 min
Response: 89992
Conc: 1.51 ng/ml

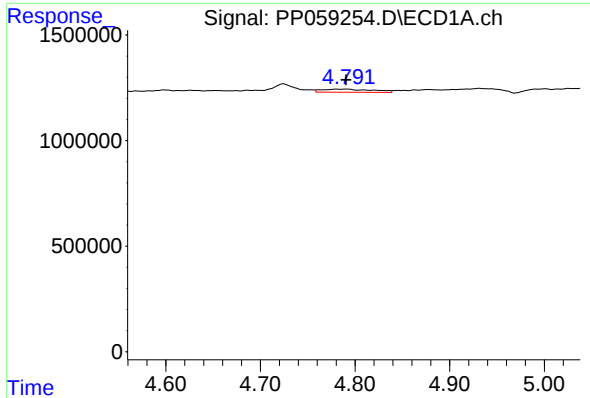

#11 AR-1232-1


R.T.: 4.791 min
Delta R.T.: 0.000 min
Response: 559119
Conc: 19.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

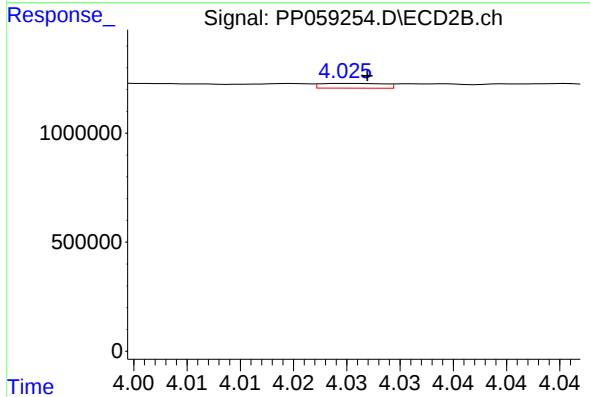


#11 AR-1232-1

R.T.: 4.025 min
Delta R.T.: -0.002 min
Response: 89992
Conc: 1.90 ng/ml

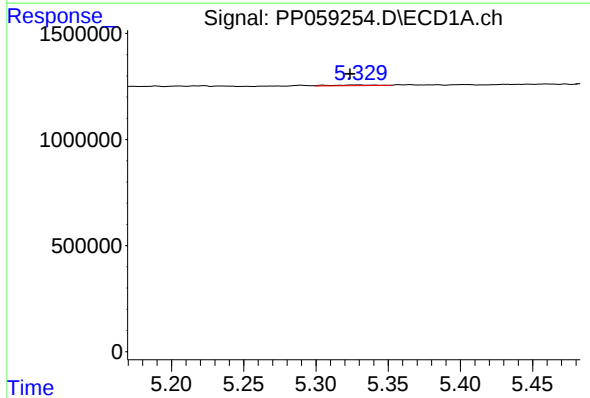


#12 AR-1232-2

R.T.: 5.329 min
Delta R.T.: 0.005 min
Response: 67035
Conc: 4.30 ng/ml

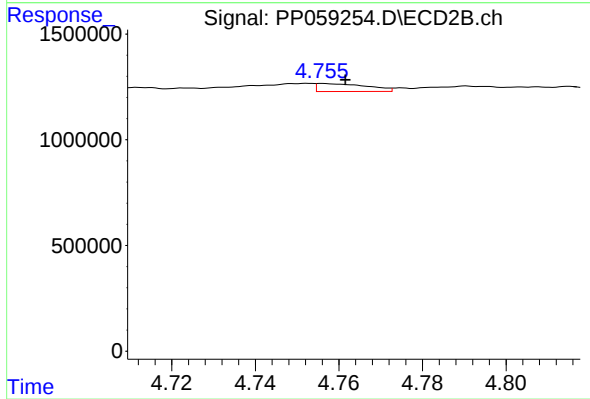

#12 AR-1232-2


R.T.: 4.756 min
Delta R.T.: -0.005 min
Response: 319438
Conc: 7.53 ng/ml

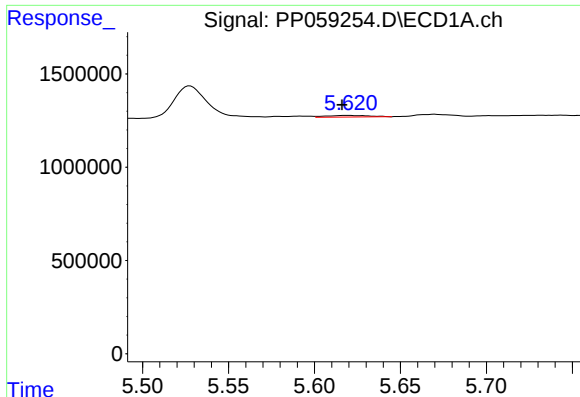

#13 AR-1232-3


R.T.: 5.619 min
Delta R.T.: 0.003 min
Response: 149570
Conc: 5.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

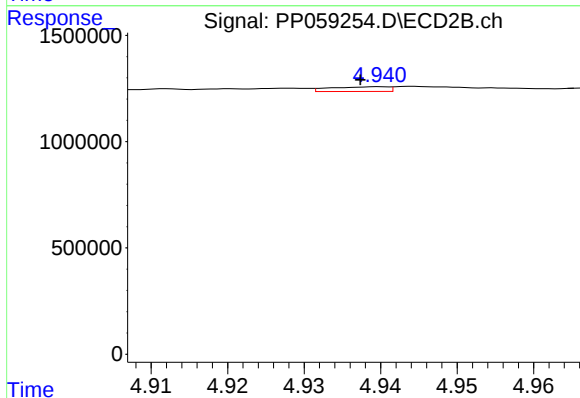


#13 AR-1232-3

R.T.: 4.940 min
Delta R.T.: 0.003 min
Response: 116729
Conc: 5.26 ng/ml

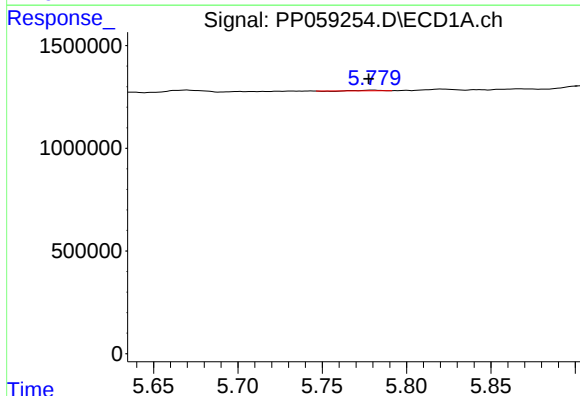


#14 AR-1232-4

R.T.: 5.780 min
Delta R.T.: 0.002 min
Response: 14034
Conc: 1.06 ng/ml

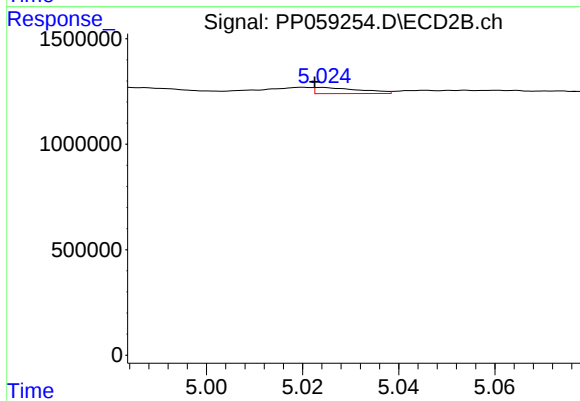

#14 AR-1232-4


R.T.: 5.024 min
Delta R.T.: 0.002 min
Response: 189079
Conc: 8.96 ng/ml

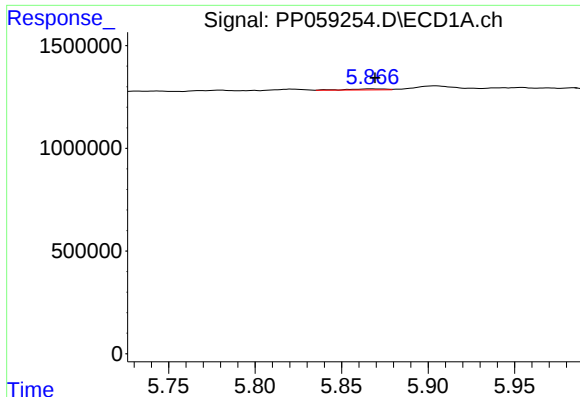

#15 AR-1232-5


R.T.: 5.868 min
Delta R.T.: -0.002 min
Response: 82458
Conc: 7.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

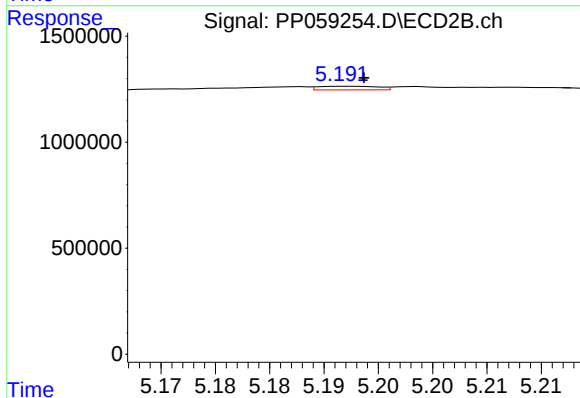


#15 AR-1232-5

R.T.: 5.192 min
Delta R.T.: -0.002 min
Response: 65308
Conc: 2.85 ng/ml

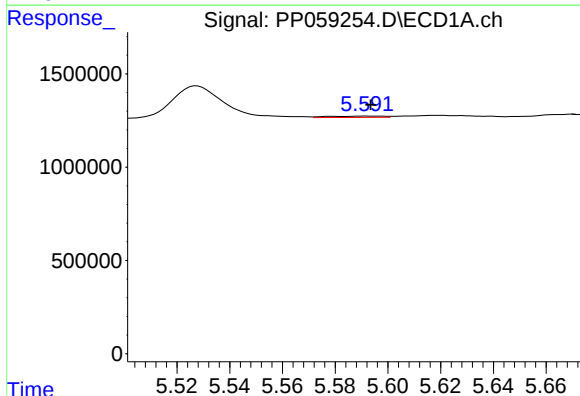


#16 AR-1242-1

R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 99198
Conc: 2.90 ng/ml

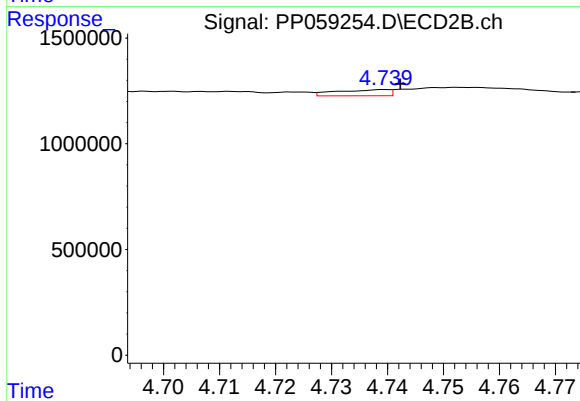

#16 AR-1242-1


R.T.: 4.740 min
Delta R.T.: -0.003 min
Response: 190349
Conc: 3.40 ng/ml

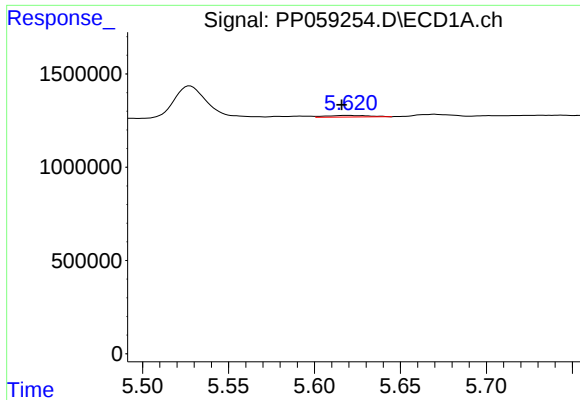

#17 AR-1242-2


R.T.: 5.619 min
Delta R.T.: 0.003 min
Response: 149570
Conc: 3.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

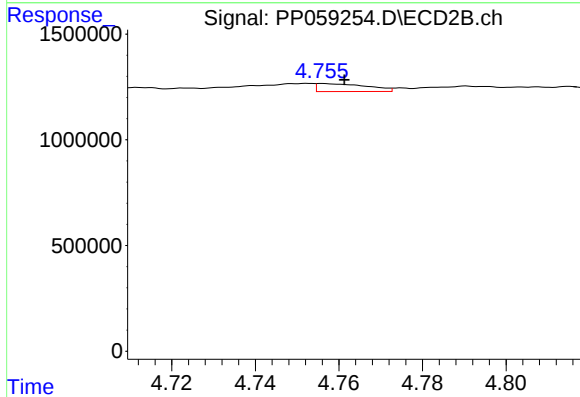


#17 AR-1242-2

R.T.: 4.756 min
Delta R.T.: -0.005 min
Response: 319438
Conc: 4.01 ng/ml

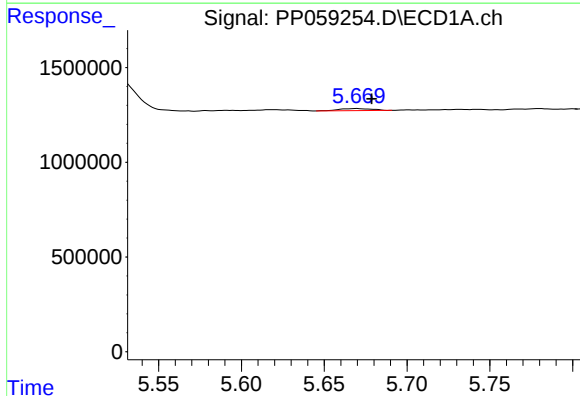


#18 AR-1242-3

R.T.: 5.670 min
Delta R.T.: -0.009 min
Response: 153290
Conc: 4.88 ng/ml

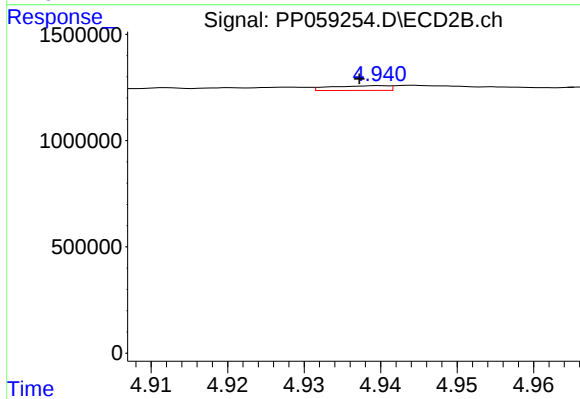

#18 AR-1242-3


R.T.: 4.940 min
Delta R.T.: 0.003 min
Response: 116729
Conc: 2.74 ng/ml

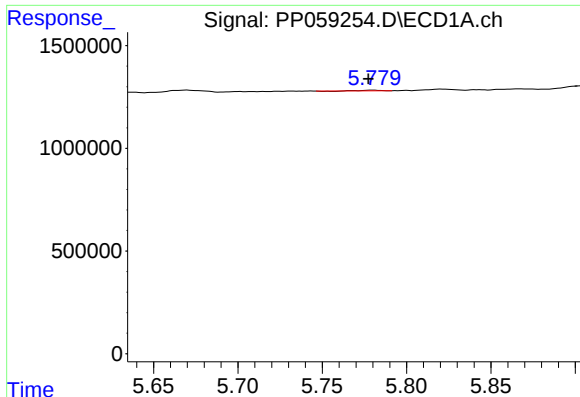

#19 AR-1242-4


R.T.: 5.780 min
Delta R.T.: 0.003 min
Response: 14034
Conc: 0.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

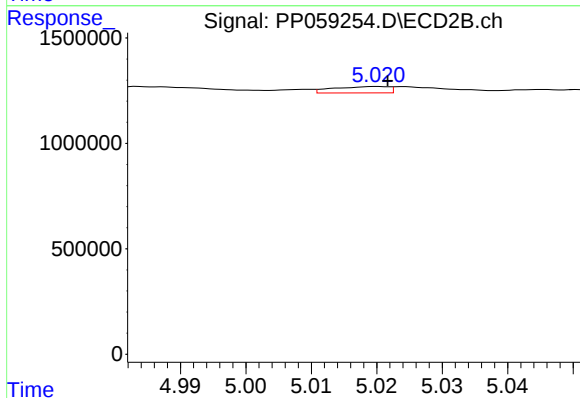


#19 AR-1242-4

R.T.: 5.020 min
Delta R.T.: -0.002 min
Response: 175258
Conc: 4.01 ng/ml

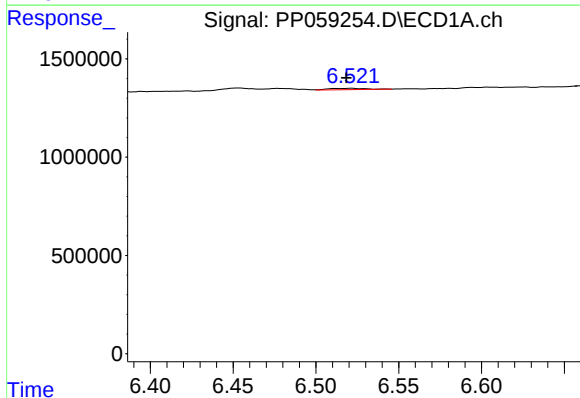


#20 AR-1242-5

R.T.: 6.521 min
Delta R.T.: 0.003 min
Response: 101942
Conc: 3.95 ng/ml

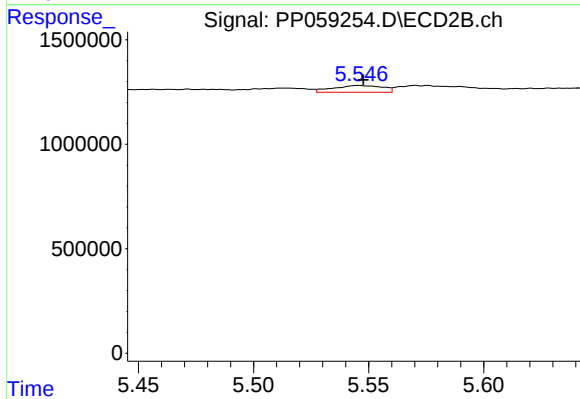

#20 AR-1242-5


R.T.: 5.546 min
Delta R.T.: -0.002 min
Response: 482170
Conc: 9.71 ng/ml

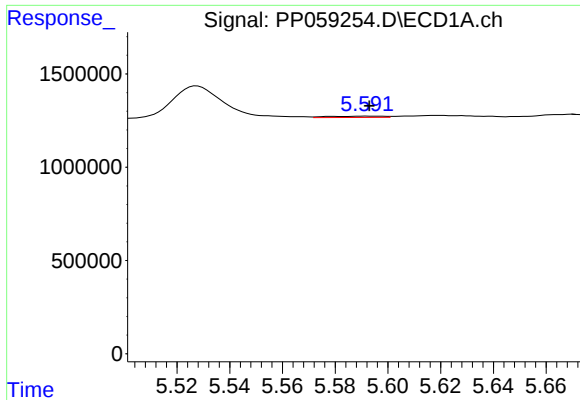

#21 AR-1248-1


R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 99198
Conc: 3.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

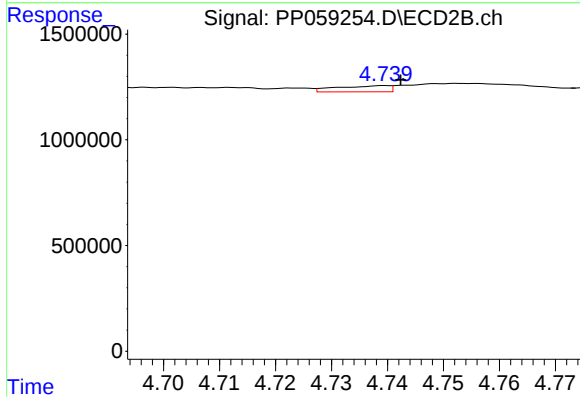


#21 AR-1248-1

R.T.: 4.740 min
Delta R.T.: -0.003 min
Response: 190349
Conc: 4.63 ng/ml

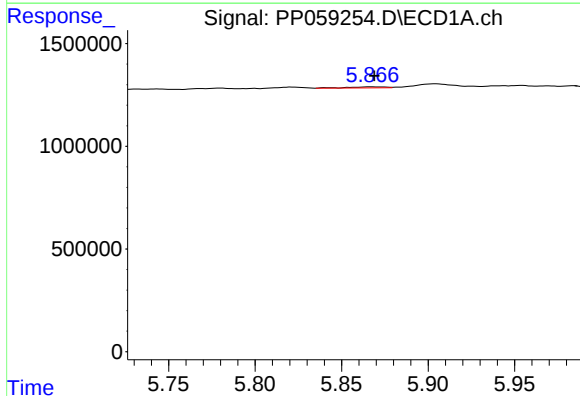


#22 AR-1248-2

R.T.: 5.868 min
Delta R.T.: -0.001 min
Response: 82458
Conc: 2.13 ng/ml

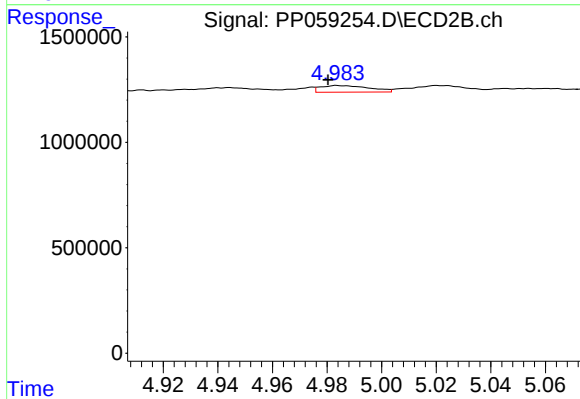

#22 AR-1248-2


R.T.: 4.983 min
Delta R.T.: 0.003 min
Response: 389329
Conc: 6.47 ng/ml

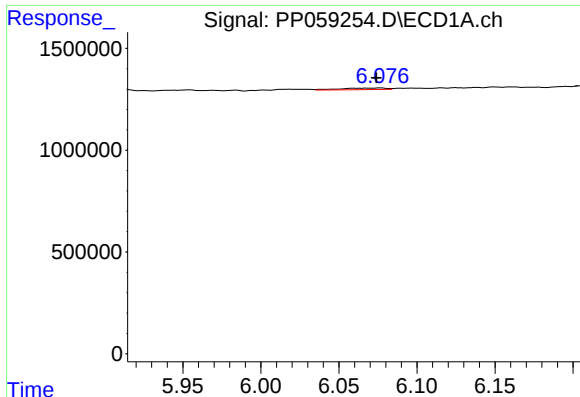

#23 AR-1248-3


R.T.: 6.076 min
Delta R.T.: 0.002 min
Response: 165130
Conc: 3.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

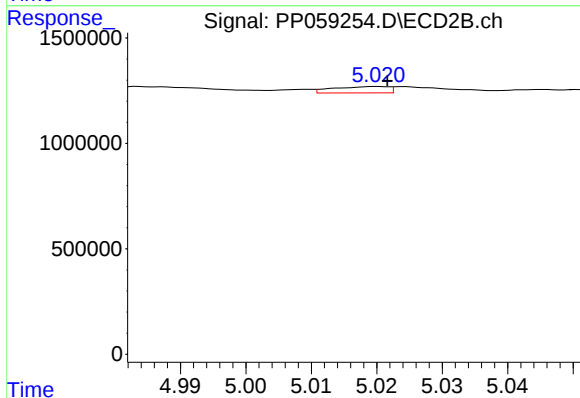


#23 AR-1248-3

R.T.: 5.020 min
Delta R.T.: -0.002 min
Response: 175258
Conc: 2.84 ng/ml

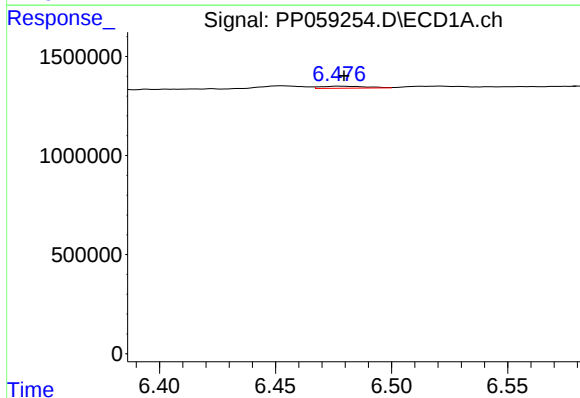


#24 AR-1248-4

R.T.: 6.478 min
Delta R.T.: -0.001 min
Response: 142772
Conc: 3.43 ng/ml

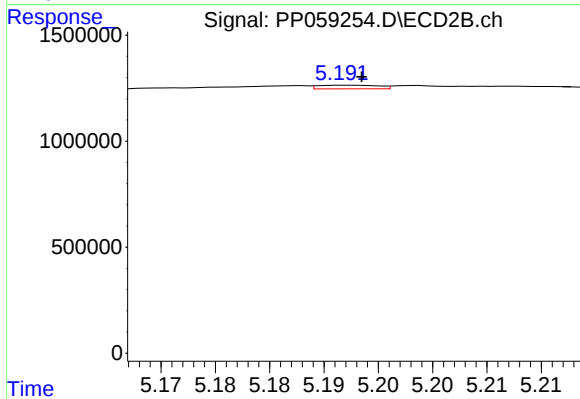

#24 AR-1248-4


R.T.: 5.192 min
Delta R.T.: -0.001 min
Response: 65308
Conc: 0.91 ng/ml

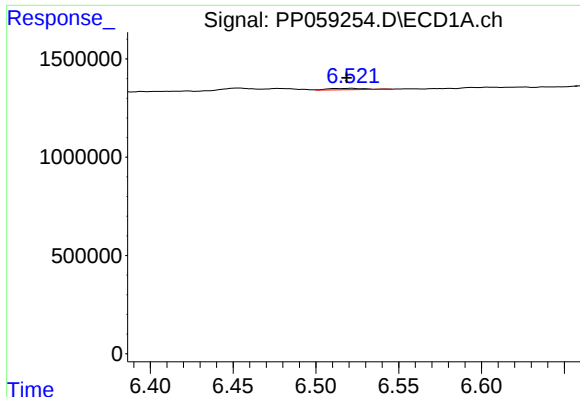

#25 AR-1248-5


R.T.: 6.521 min
Delta R.T.: 0.002 min
Response: 101942
Conc: 2.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

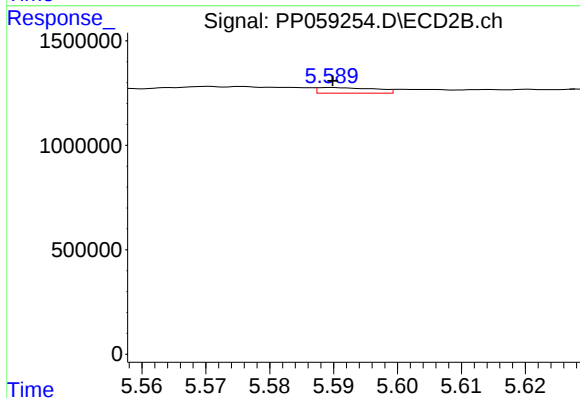


#25 AR-1248-5

R.T.: 5.590 min
Delta R.T.: 0.000 min
Response: 167914
Conc: 2.54 ng/ml

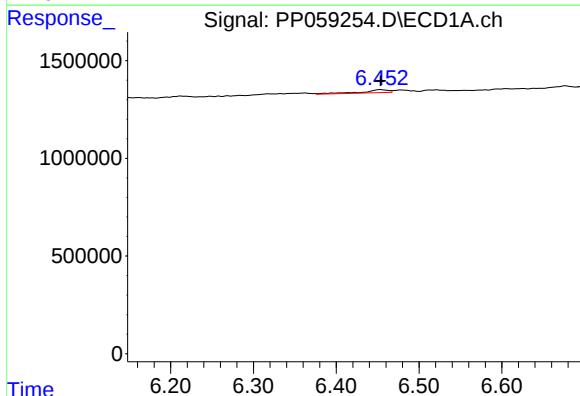


#26 AR-1254-1

R.T.: 6.453 min
Delta R.T.: 0.000 min
Response: 316183
Conc: 6.77 ng/ml

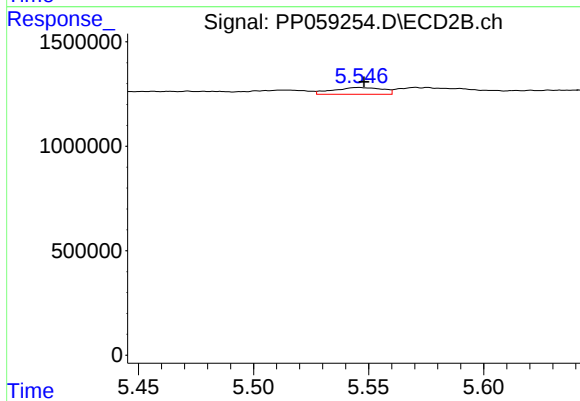

#26 AR-1254-1


R.T.: 5.546 min
Delta R.T.: -0.002 min
Response: 482170
Conc: 4.76 ng/ml

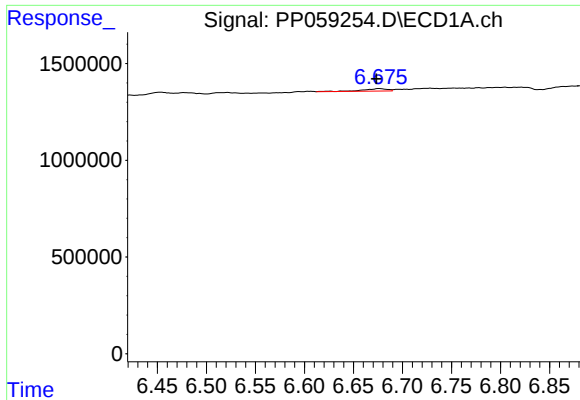

#27 AR-1254-2


R.T.: 6.677 min
Delta R.T.: 0.003 min
Response: 227476
Conc: 3.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

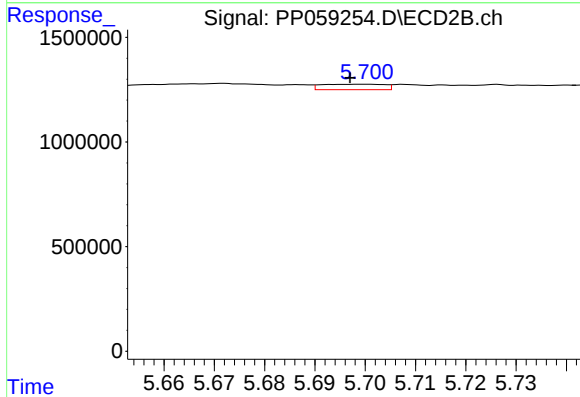


#27 AR-1254-2

R.T.: 5.701 min
Delta R.T.: 0.004 min
Response: 224625
Conc: 2.54 ng/ml

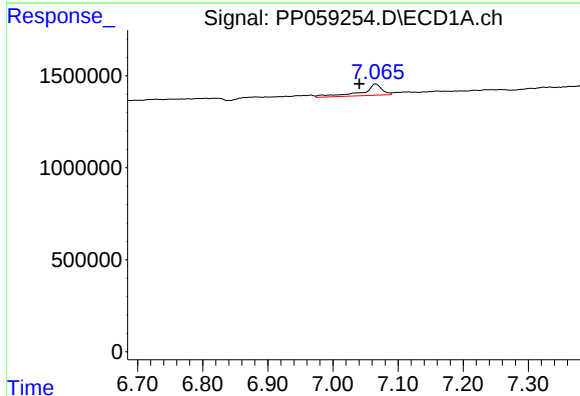


#28 AR-1254-3

R.T.: 7.066 min
Delta R.T.: 0.025 min
Response: 1336464
Conc: 19.36 ng/ml

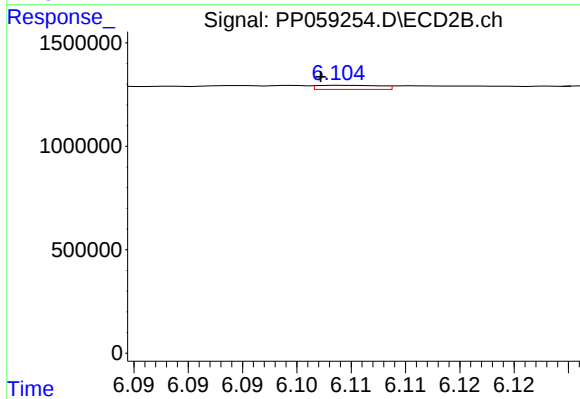

#28 AR-1254-3


R.T.: 6.104 min
Delta R.T.: 0.002 min
Response: 79518
Conc: 0.58 ng/ml

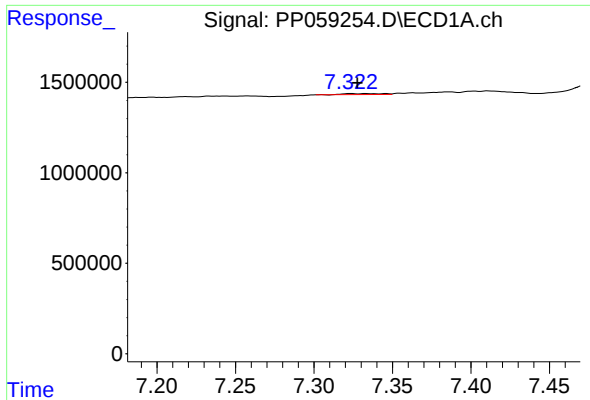

#29 AR-1254-4


R.T.: 7.333 min
Delta R.T.: 0.006 min
Response: 89248
Conc: 1.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

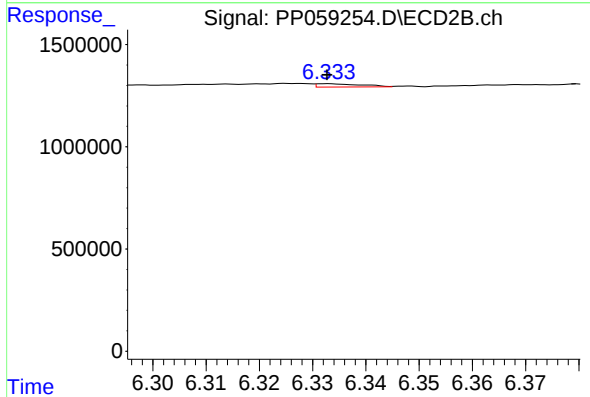


#29 AR-1254-4

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 93325
Conc: 1.16 ng/ml

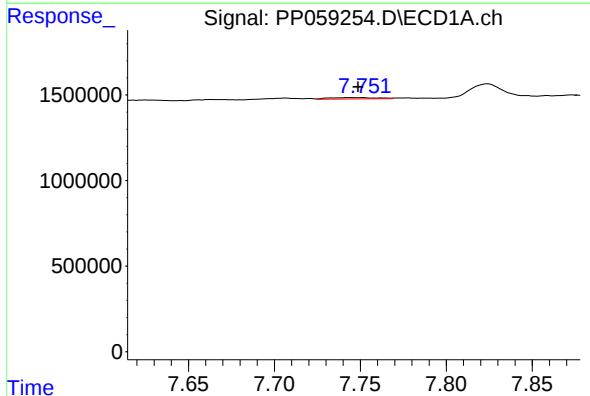


#30 AR-1254-5

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 156728
Conc: 3.34 ng/ml

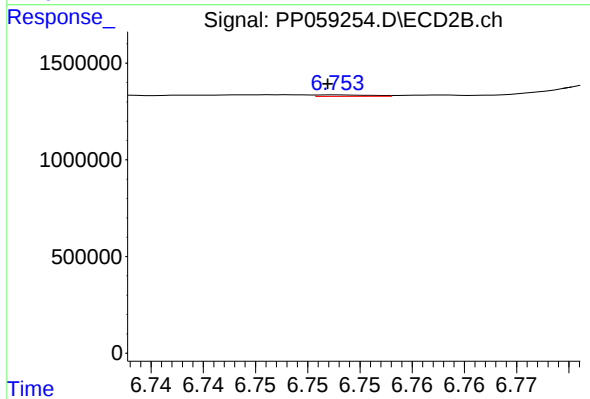

#30 AR-1254-5


R.T.: 6.753 min
Delta R.T.: 0.000 min
Response: 27676
Conc: 0.23 ng/ml

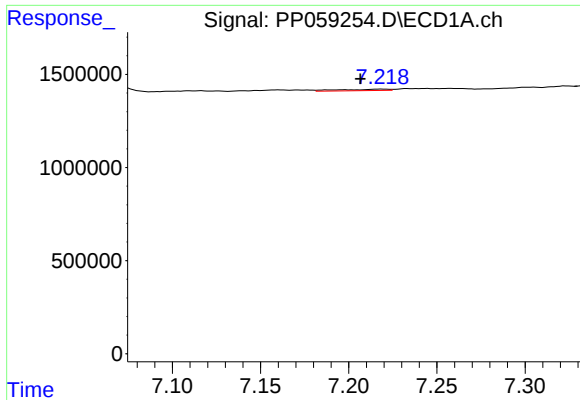

#31 AR-1260-1


R.T.: 7.219 min
Delta R.T.: 0.012 min
Response: 152238
Conc: 2.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

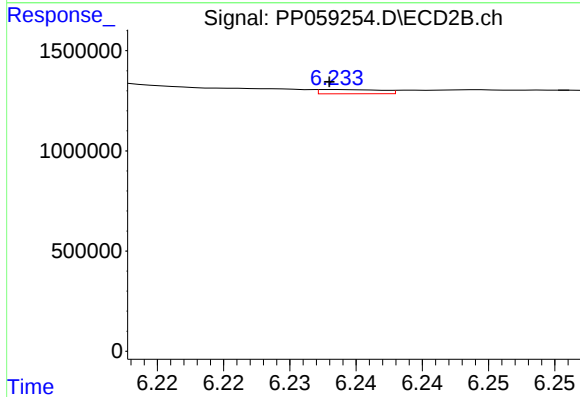


#31 AR-1260-1

R.T.: 6.234 min
Delta R.T.: 0.000 min
Response: 69421
Conc: 0.70 ng/ml

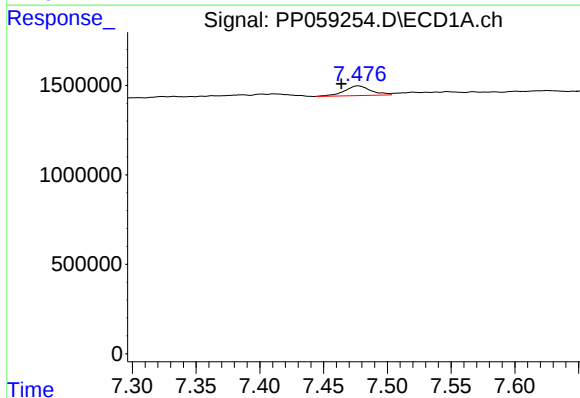


#32 AR-1260-2

R.T.: 7.477 min
Delta R.T.: 0.013 min
Response: 786180
Conc: 13.20 ng/ml

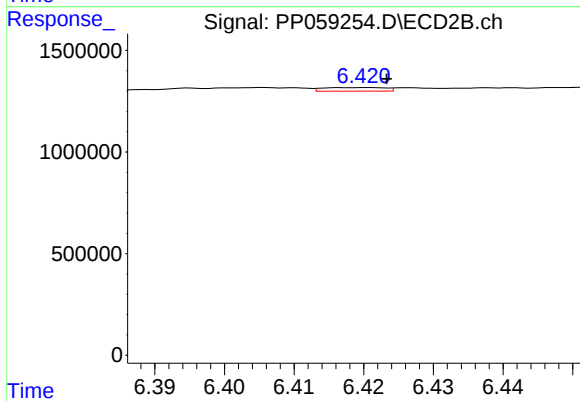

#32 AR-1260-2


R.T.: 6.420 min
Delta R.T.: -0.003 min
Response: 111690
Conc: 0.97 ng/ml

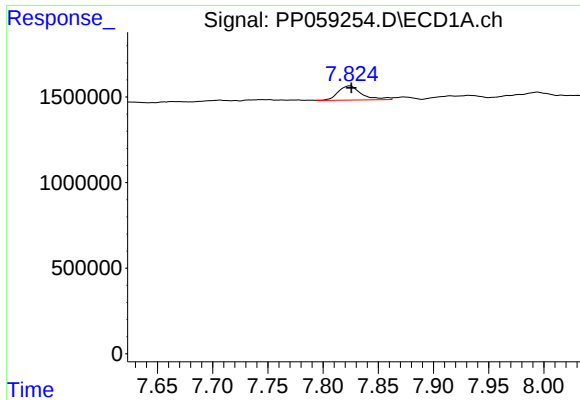

#33 AR-1260-3


R.T.: 7.824 min
Delta R.T.: -0.002 min
Response: 1228029
Conc: 31.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

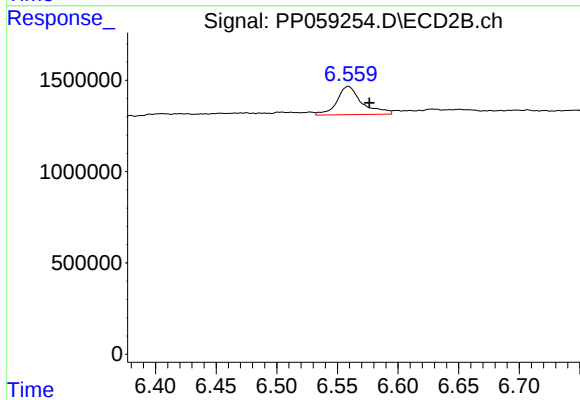


#33 AR-1260-3

R.T.: 6.559 min
Delta R.T.: -0.017 min
Response: 2238970
Conc: 20.13 ng/ml

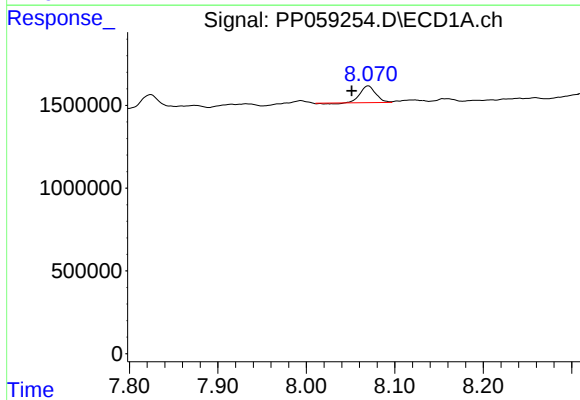


#34 AR-1260-4

R.T.: 8.070 min
Delta R.T.: 0.019 min
Response: 1203923
Conc: 27.11 ng/ml

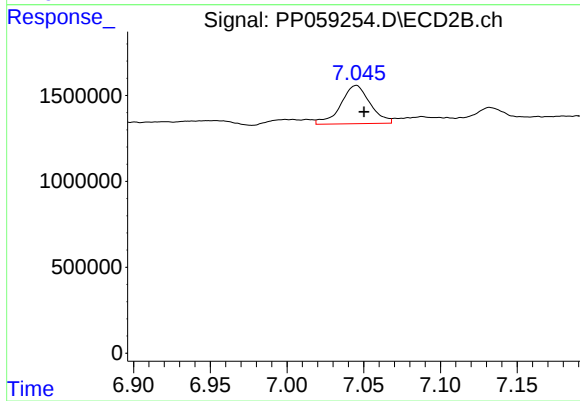

#34 AR-1260-4


R.T.: 7.045 min
Delta R.T.: -0.005 min
Response: 2981834
Conc: 34.39 ng/ml

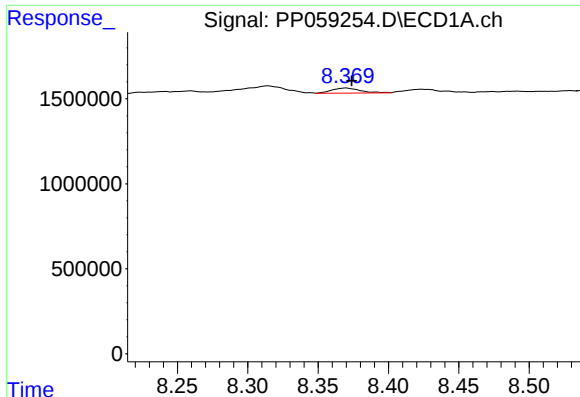

#35 AR-1260-5


R.T.: 8.370 min
Delta R.T.: -0.004 min
Response: 431408
Conc: 5.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

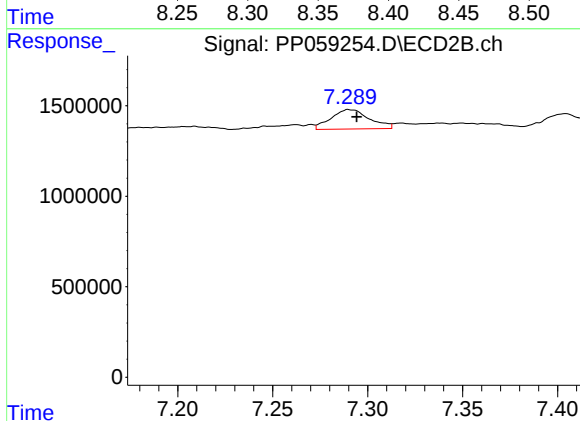


#35 AR-1260-5

R.T.: 7.290 min
Delta R.T.: -0.004 min
Response: 1509135
Conc: 8.19 ng/ml

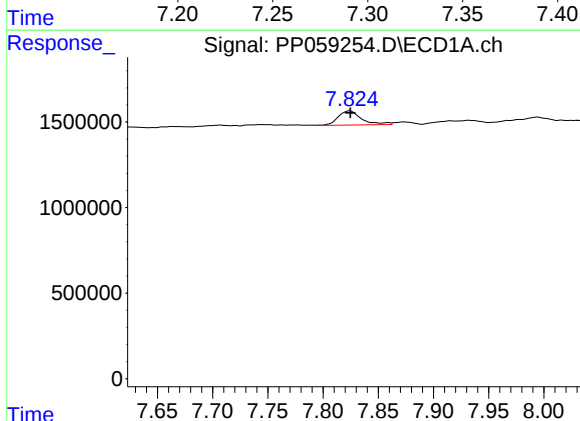


#36 AR-1262-1

R.T.: 7.824 min
Delta R.T.: 0.000 min
Response: 1228029
Conc: 19.28 ng/ml

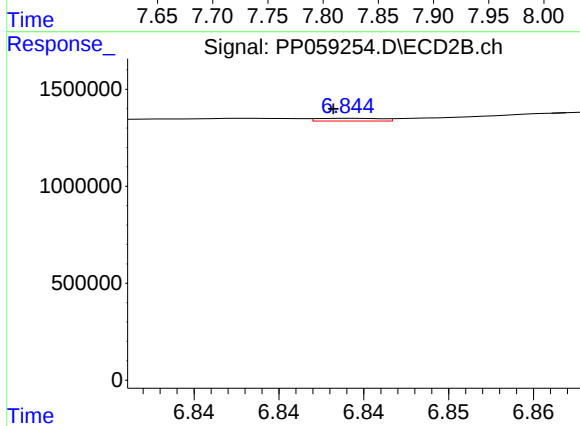

#36 AR-1262-1


R.T.: 6.844 min
Delta R.T.: 0.001 min
Response: 37129
Conc: 0.65 ng/ml

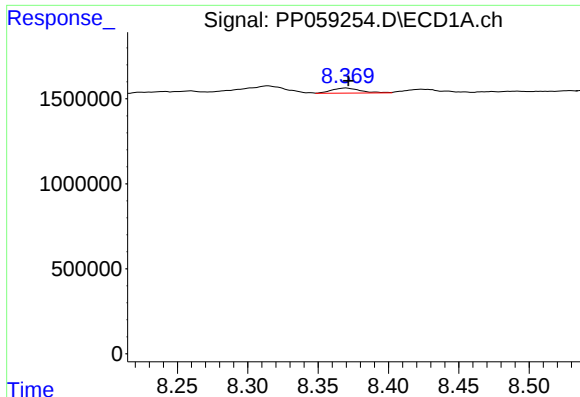

#37 AR-1262-2


R.T.: 8.370 min
Delta R.T.: -0.002 min
Response: 431408
Conc: 4.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

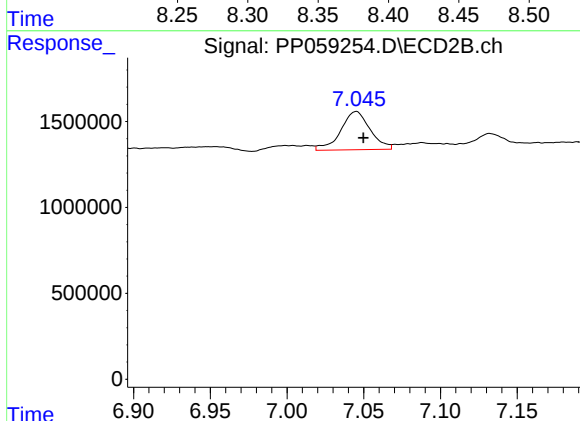


#37 AR-1262-2

R.T.: 7.045 min
Delta R.T.: -0.004 min
Response: 2981834
Conc: 25.27 ng/ml

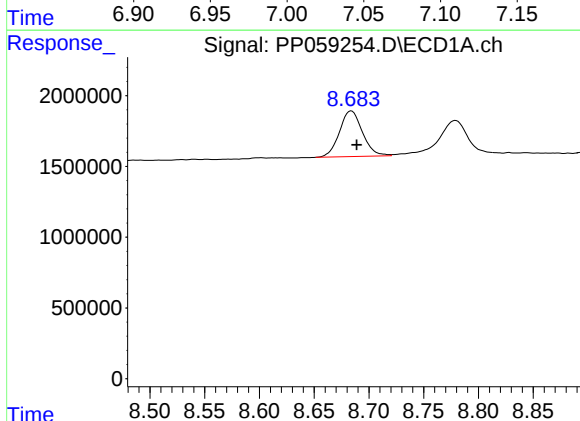


#38 AR-1262-3

R.T.: 8.684 min
Delta R.T.: -0.005 min
Response: 4713066
Conc: 73.24 ng/ml

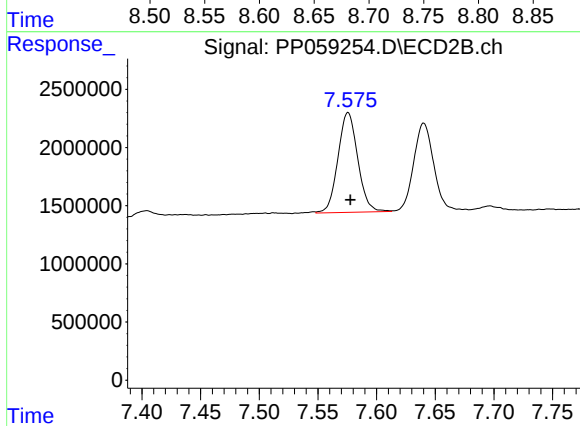

#38 AR-1262-3


R.T.: 7.576 min
Delta R.T.: -0.002 min
Response: 10109821
Conc: 118.80 ng/ml

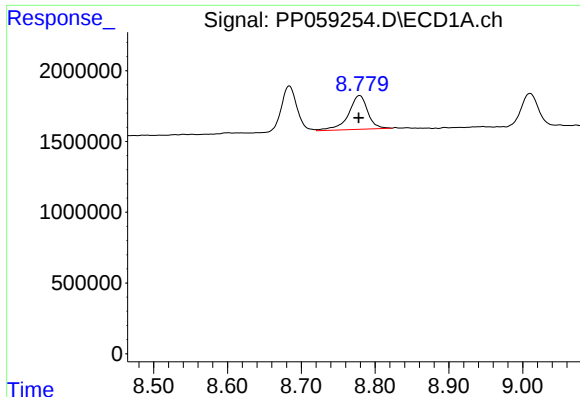

#39 AR-1262-4


R.T.: 8.779 min
Delta R.T.: 0.001 min
Response: 4313021
Conc: 129.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

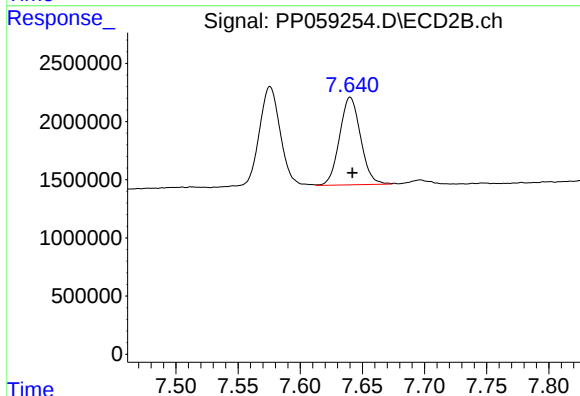


#39 AR-1262-4

R.T.: 7.640 min
Delta R.T.: -0.002 min
Response: 8861216
Conc: 58.66 ng/ml

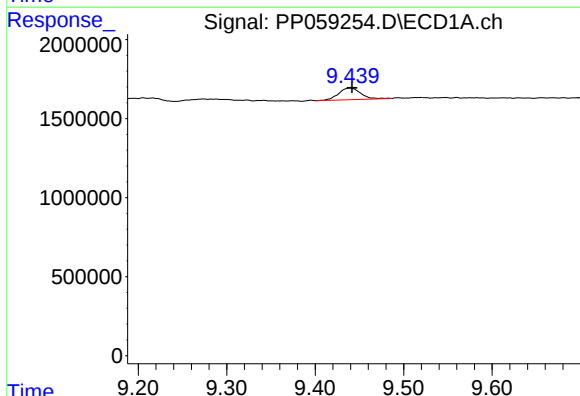


#40 AR-1262-5

R.T.: 9.440 min
Delta R.T.: -0.002 min
Response: 1300456
Conc: 43.58 ng/ml

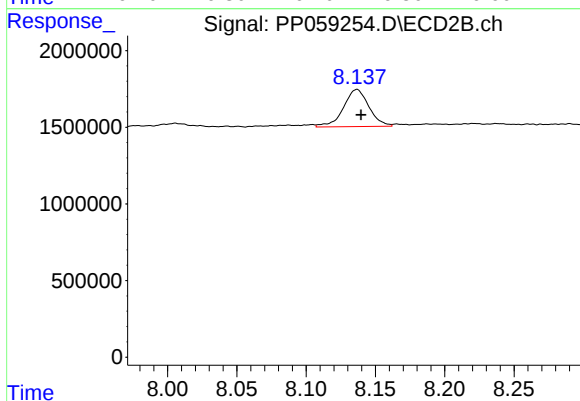

#40 AR-1262-5


R.T.: 8.137 min
Delta R.T.: -0.003 min
Response: 3109672
Conc: 48.76 ng/ml

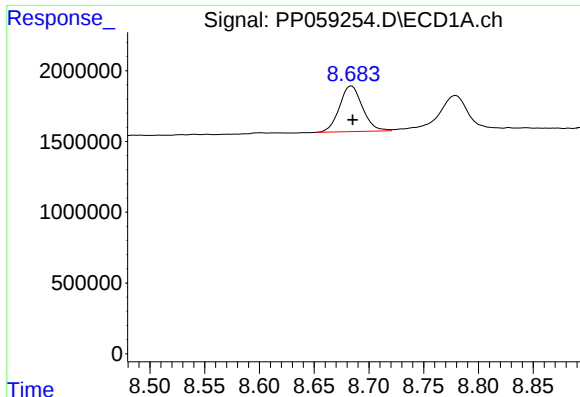

#41 AR-1268-1


R.T.: 8.684 min
Delta R.T.: -0.001 min
Response: 4713066
Conc: 41.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

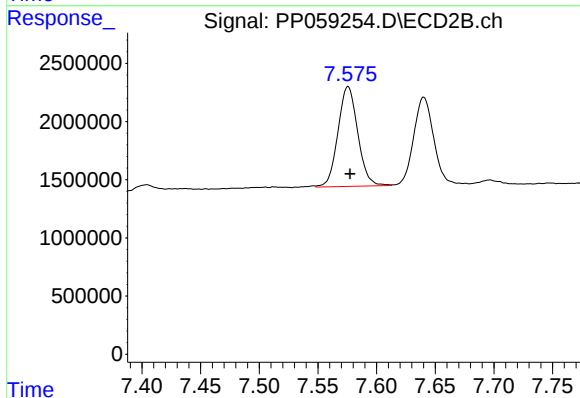


#41 AR-1268-1

R.T.: 7.576 min
Delta R.T.: -0.002 min
Response: 10109821
Conc: 41.46 ng/ml

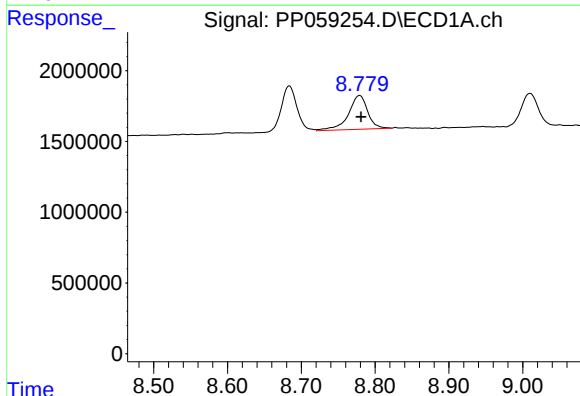


#42 AR-1268-2

R.T.: 8.779 min
Delta R.T.: -0.002 min
Response: 4313021
Conc: 43.82 ng/ml

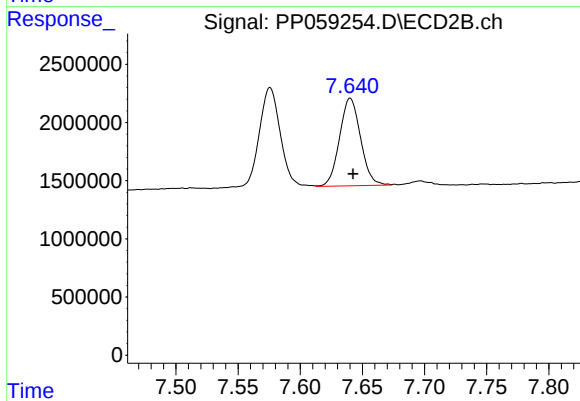

#42 AR-1268-2


R.T.: 7.640 min
Delta R.T.: -0.002 min
Response: 8861216
Conc: 40.46 ng/ml

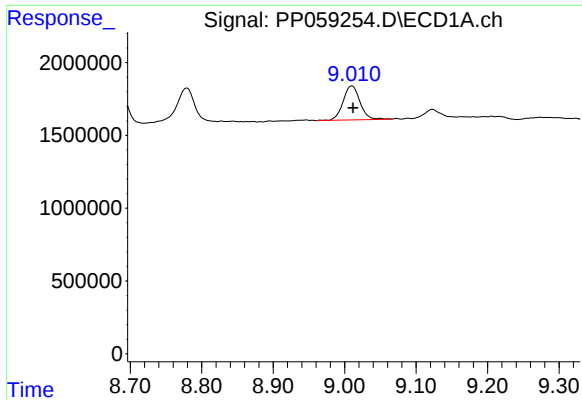

#43 AR-1268-3


R.T.: 9.010 min
Delta R.T.: -0.002 min
Response: 3856402
Conc: 41.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

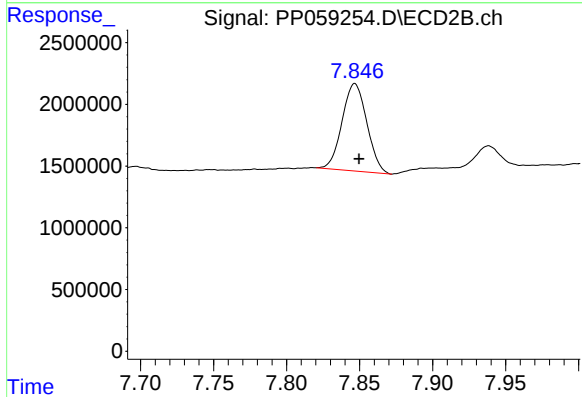


#43 AR-1268-3

R.T.: 7.847 min
Delta R.T.: -0.003 min
Response: 8360680
Conc: 42.76 ng/ml

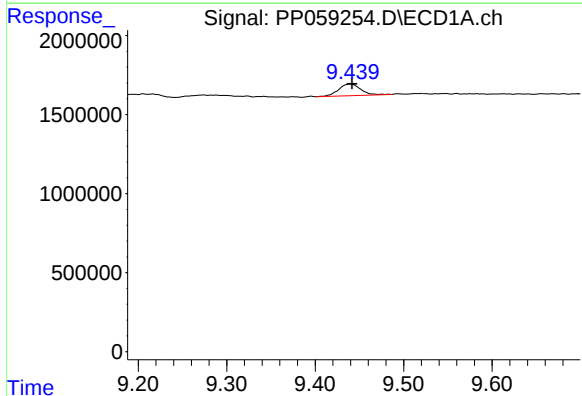


#44 AR-1268-4

R.T.: 9.440 min
Delta R.T.: -0.002 min
Response: 1300456
Conc: 40.77 ng/ml

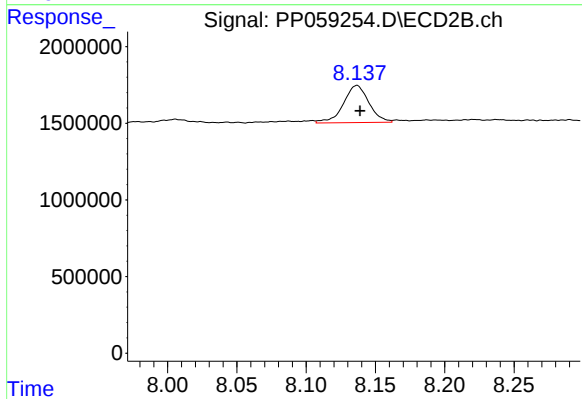

#44 AR-1268-4


R.T.: 8.137 min
Delta R.T.: -0.002 min
Response: 3109672
Conc: 44.69 ng/ml

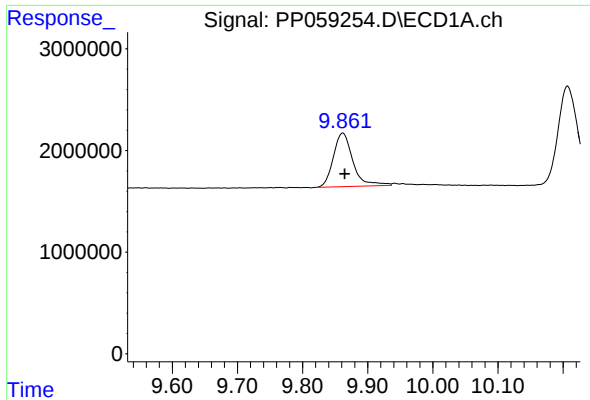

#45 AR-1268-5

R.T.: 9.862 min
Delta R.T.: -0.003 min
Response: 11013323
Conc: 40.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2023

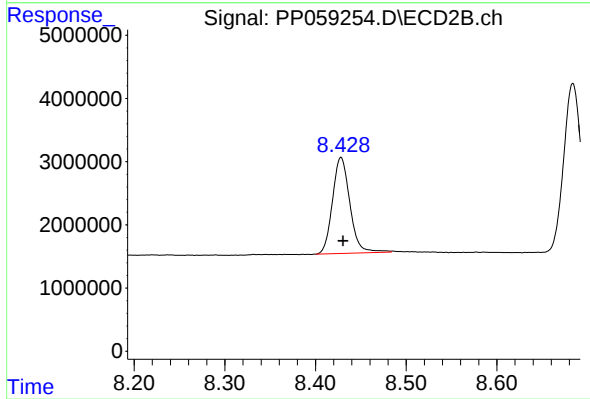

#45 AR-1268-5

R.T.: 8.428 min
Delta R.T.: -0.002 min
Response: 20311690
Conc: 39.18 ng/ml