

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080921\
 Data File : PP038125.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Aug 2021 8:49
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 14:41:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.883	0	2100	N.D.	0.082 #
Target Compounds							
6)	L1 AR-1016-4	0.000	5.417f	0	3514	N.D.	6.186 #
8)	L2 AR-1221-1	0.000	4.146	0	2096	N.D.	6.967 #
9)	L2 AR-1221-2	0.000	4.261f	0	771	N.D.	3.276 #
10)	L2 AR-1221-3	0.000	4.318	0	7419	N.D.	10.061 #
11)	L3 AR-1232-1	0.000	4.318	0	7419	N.D.	10.944 #
14)	L3 AR-1232-4	0.000	5.417f	0	3514	N.D.	11.895 #
19)	L4 AR-1242-4	0.000	5.417f	0	3514	N.D.	6.689 #
22)	L5 AR-1248-2	0.000	5.417f	0	3514	N.D.	4.731 #
23)	L5 AR-1248-3	0.000	5.417f	0	3514	N.D.	4.466 #
43)	L9 AR-1268-3	0.000	8.372f	0	3200	N.D.	1.123 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080921\
Data File : PP038125.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Aug 2021 8:49
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 14:41:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

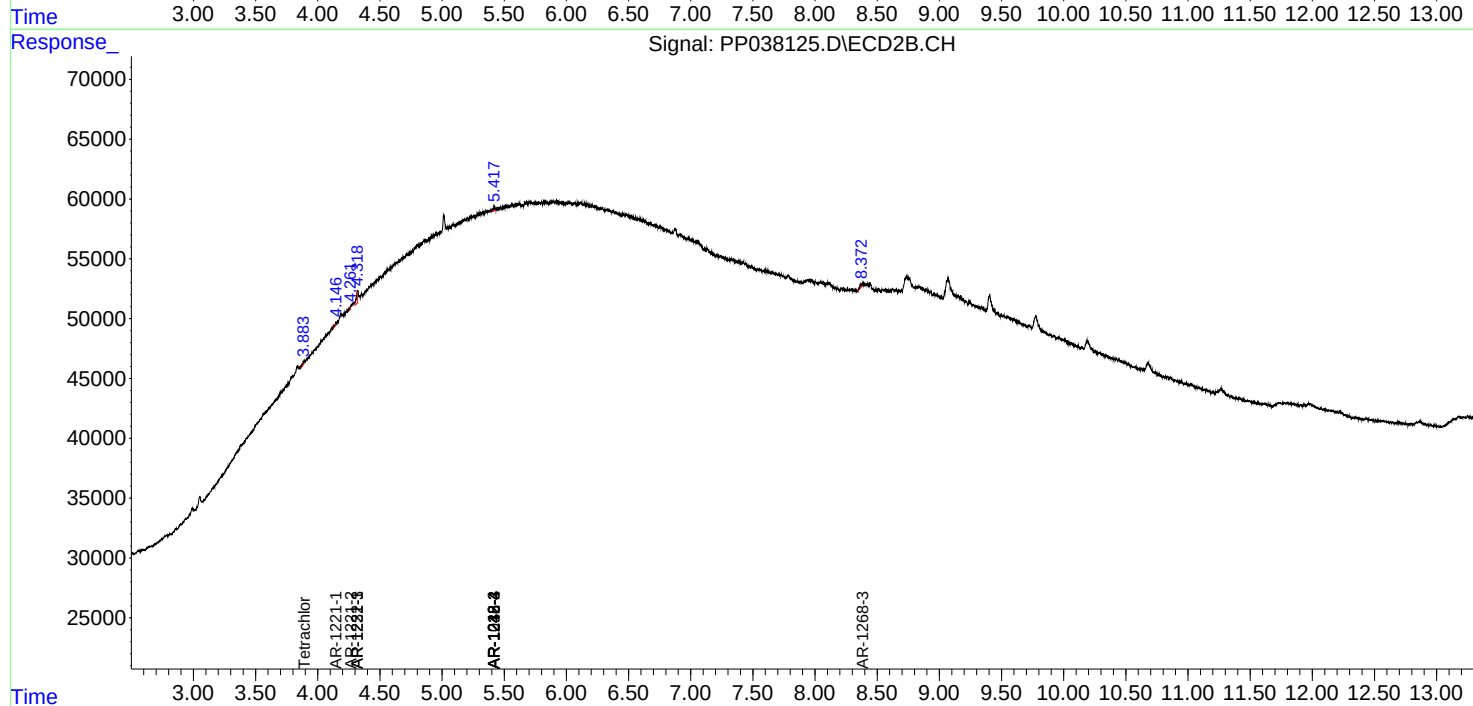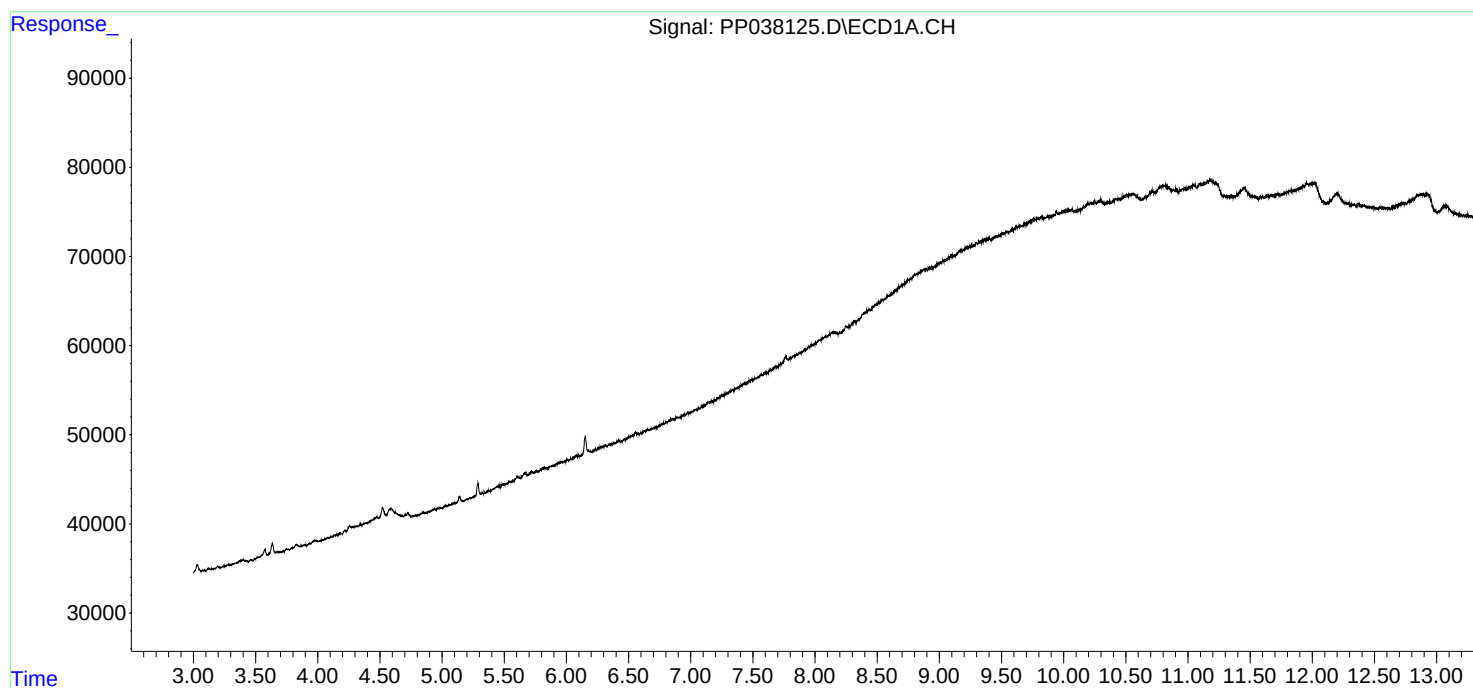


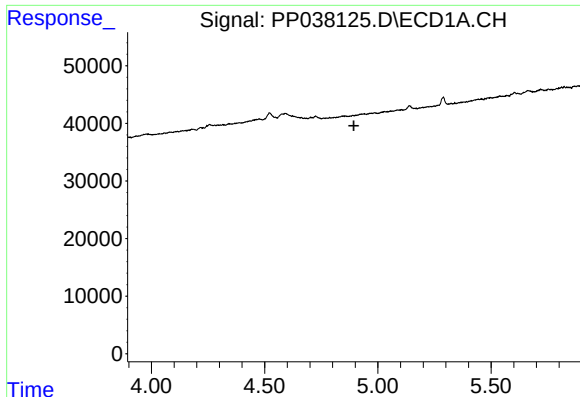

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.894 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

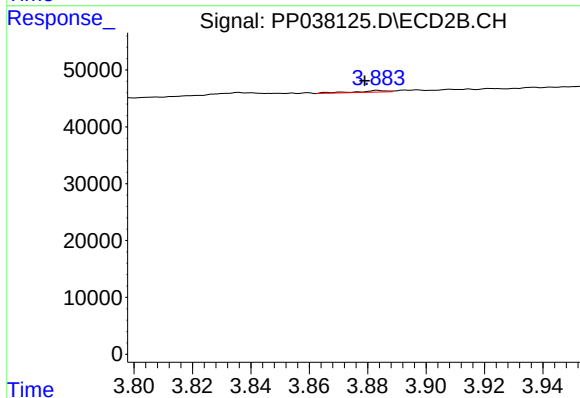


#1 Tetrachloro-m-xylene

R.T.: 3.883 min
Delta R.T.: 0.004 min
Response: 2100
Conc: 0.08 ng/ml

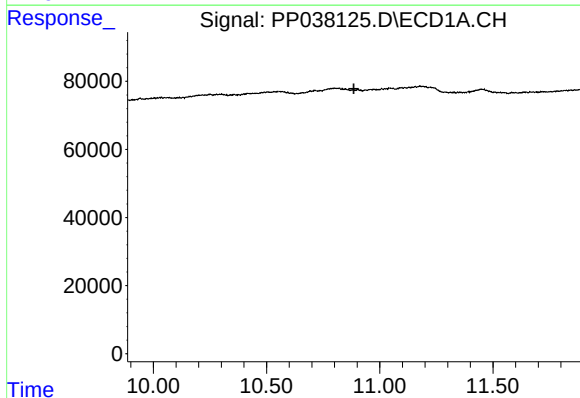


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.886 min
Response: 0
Conc: N.D.

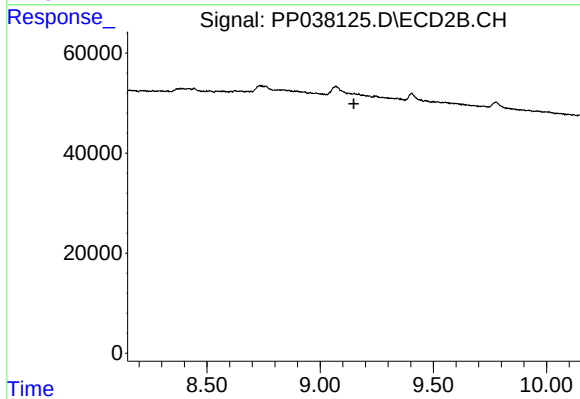

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.149 min
Response: 0
Conc: N.D.

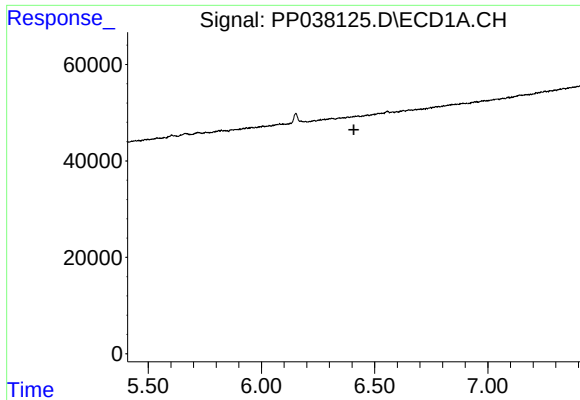

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 6.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

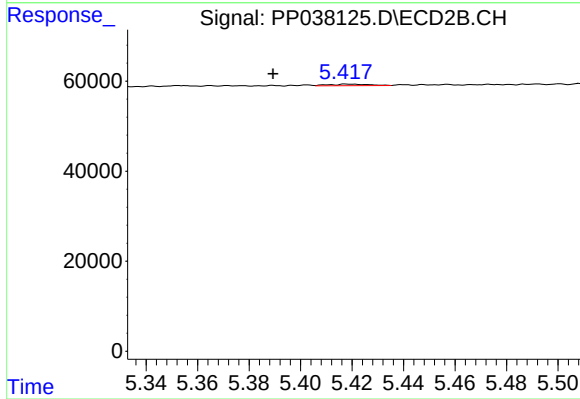


#6 AR-1016-4

R.T.: 5.417 min
Delta R.T.: 0.028 min
Response: 3514
Conc: 6.19 ng/ml

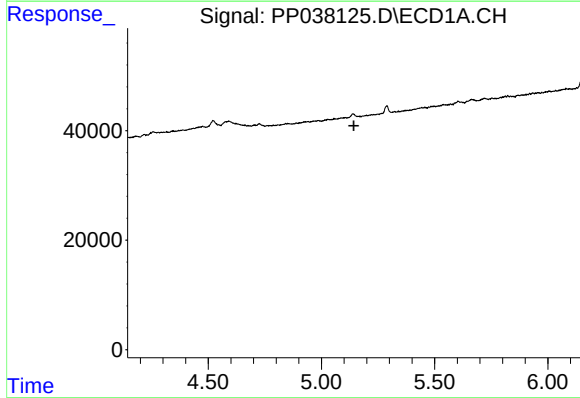


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 5.143 min
Response: 0
Conc: N.D.

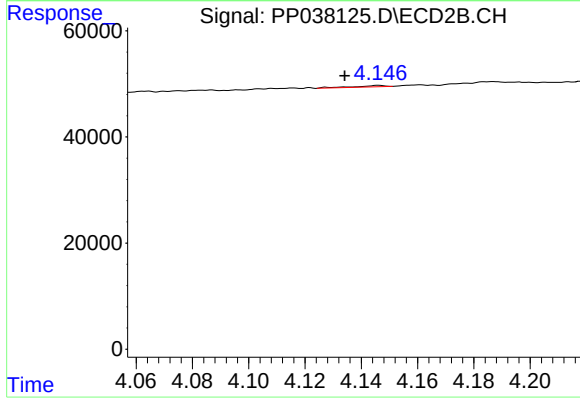

#8 AR-1221-1


R.T.: 4.146 min
Delta R.T.: 0.012 min
Response: 2096
Conc: 6.97 ng/ml

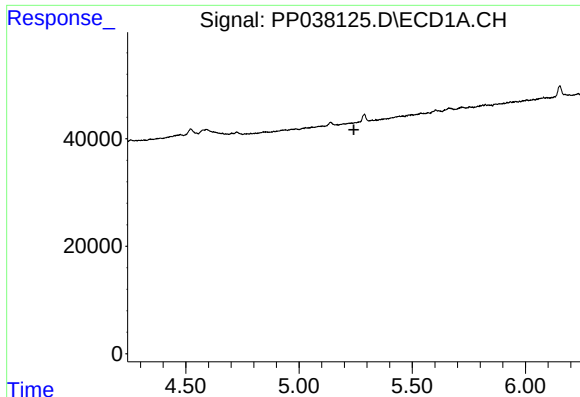

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.242 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

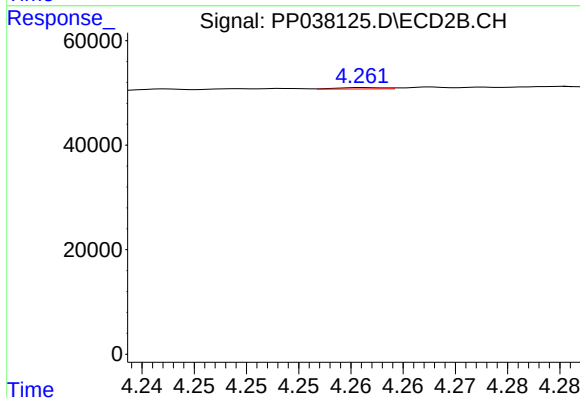


#9 AR-1221-2

R.T.: 4.261 min
Delta R.T.: 0.029 min
Response: 771
Conc: 3.28 ng/ml

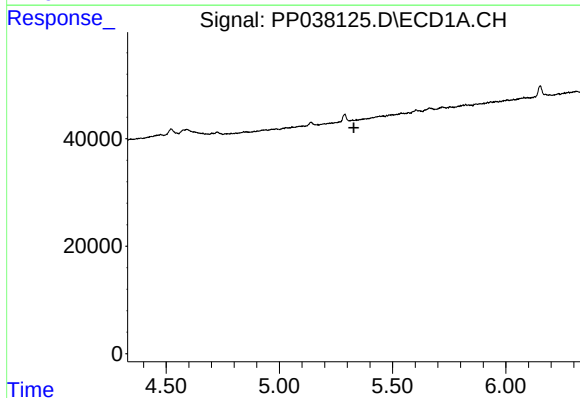


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T.: 5.329 min
Response: 0
Conc: N.D.

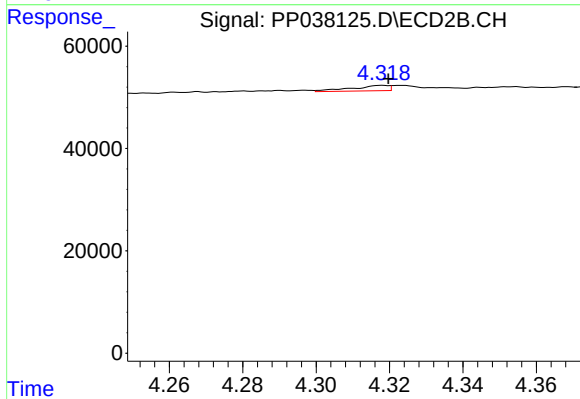

#10 AR-1221-3


R.T.: 4.318 min
Delta R.T.: -0.002 min
Response: 7419
Conc: 10.06 ng/ml

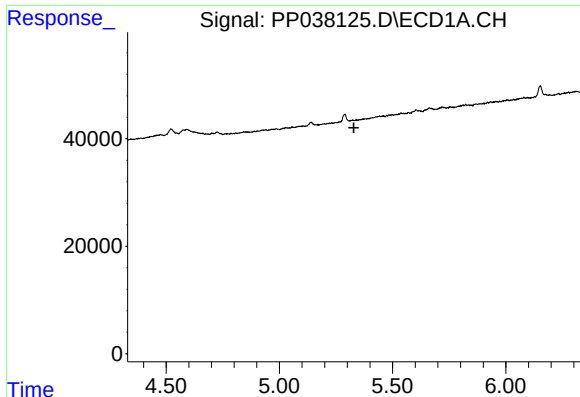

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 5.329 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

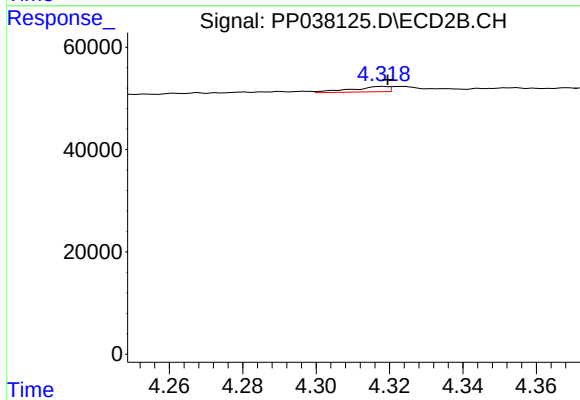


#11 AR-1232-1

R.T.: 4.318 min
Delta R.T.: -0.001 min
Response: 7419
Conc: 10.94 ng/ml

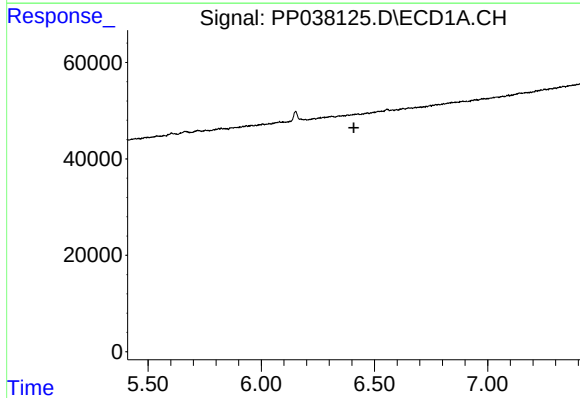


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

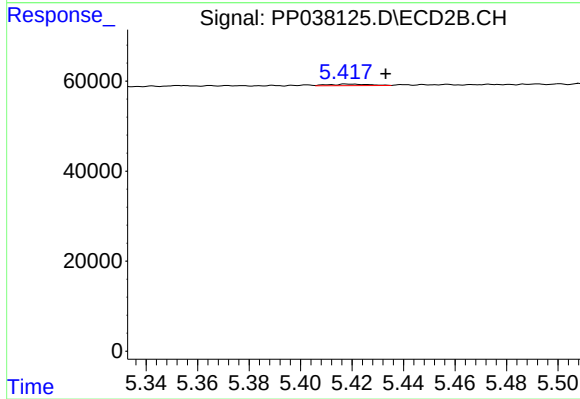

#14 AR-1232-4


R.T.: 5.417 min
Delta R.T.: -0.016 min
Response: 3514
Conc: 11.89 ng/ml

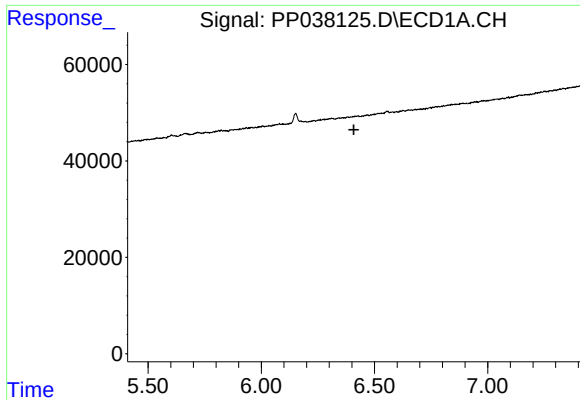

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

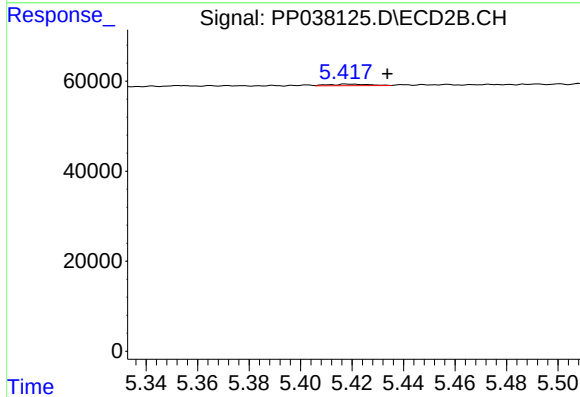


#19 AR-1242-4

R.T.: 5.417 min
Delta R.T.: -0.016 min
Response: 3514
Conc: 6.69 ng/ml

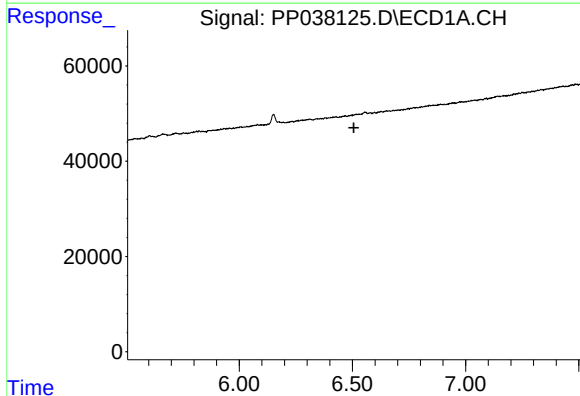


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 6.506 min
Response: 0
Conc: N.D.

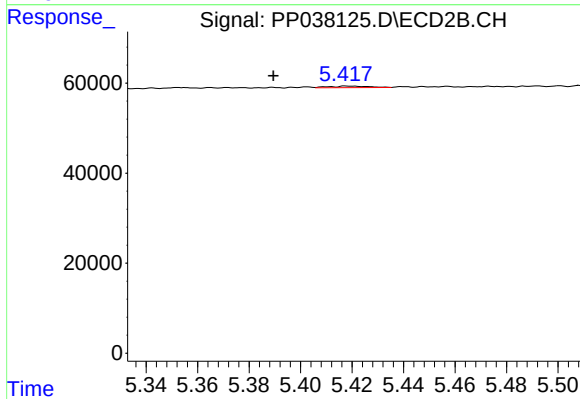

#22 AR-1248-2


R.T.: 5.417 min
Delta R.T.: 0.028 min
Response: 3514
Conc: 4.73 ng/ml

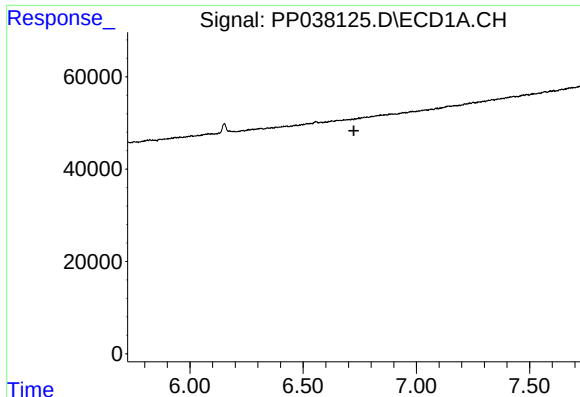

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 6.724 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

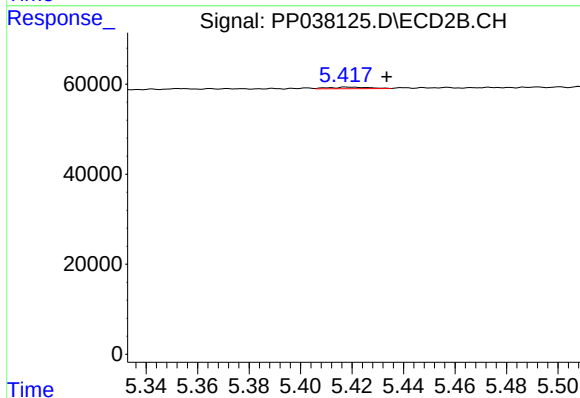


#23 AR-1248-3

R.T.: 5.417 min
Delta R.T.: -0.016 min
Response: 3514
Conc: 4.47 ng/ml

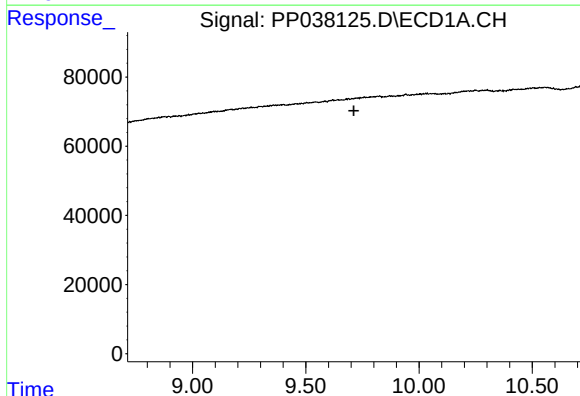

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.713 min
Response: 0
Conc: N.D.

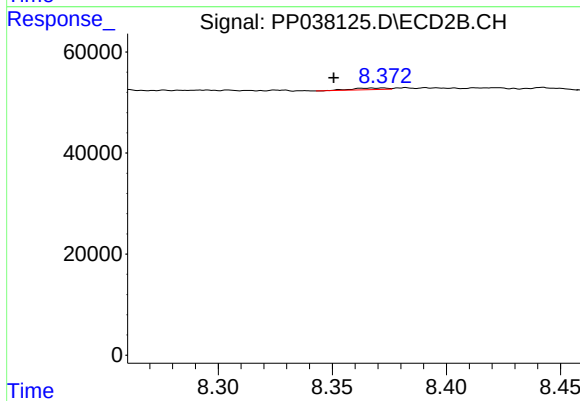

#43 AR-1268-3

R.T.: 8.372 min
Delta R.T.: 0.022 min
Response: 3200
Conc: 1.12 ng/ml