

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080921\
 Data File : PP038160.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Aug 2021 19:53
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 00:58:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.892	3.879	876565	535999	19.724	20.811
2)	SA Decachlor...	10.882	9.145	459862	545917	20.215	21.100
Target Compounds							
9)	L2 AR-1221-2	0.000	4.227	0	7344	N.D.	31.205 #
20)	L4 AR-1242-5	0.000	6.013f	0	6893	N.D.	10.667 #
25)	L5 AR-1248-5	0.000	6.013f	0	6893	N.D.	7.321 #
26)	L6 AR-1254-1	0.000	6.013f	0	6893	N.D.	5.152 #
28)	L6 AR-1254-3	7.751f	0.000	13630	0	6.870	N.D. #
32)	L7 AR-1260-2	8.138f	0.000	22321	0	12.965	N.D. #
33)	L7 AR-1260-3	0.000	7.064	0	7468	N.D.	4.906 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080921\
Data File : PP038160.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Aug 2021 19:53
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 00:58:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

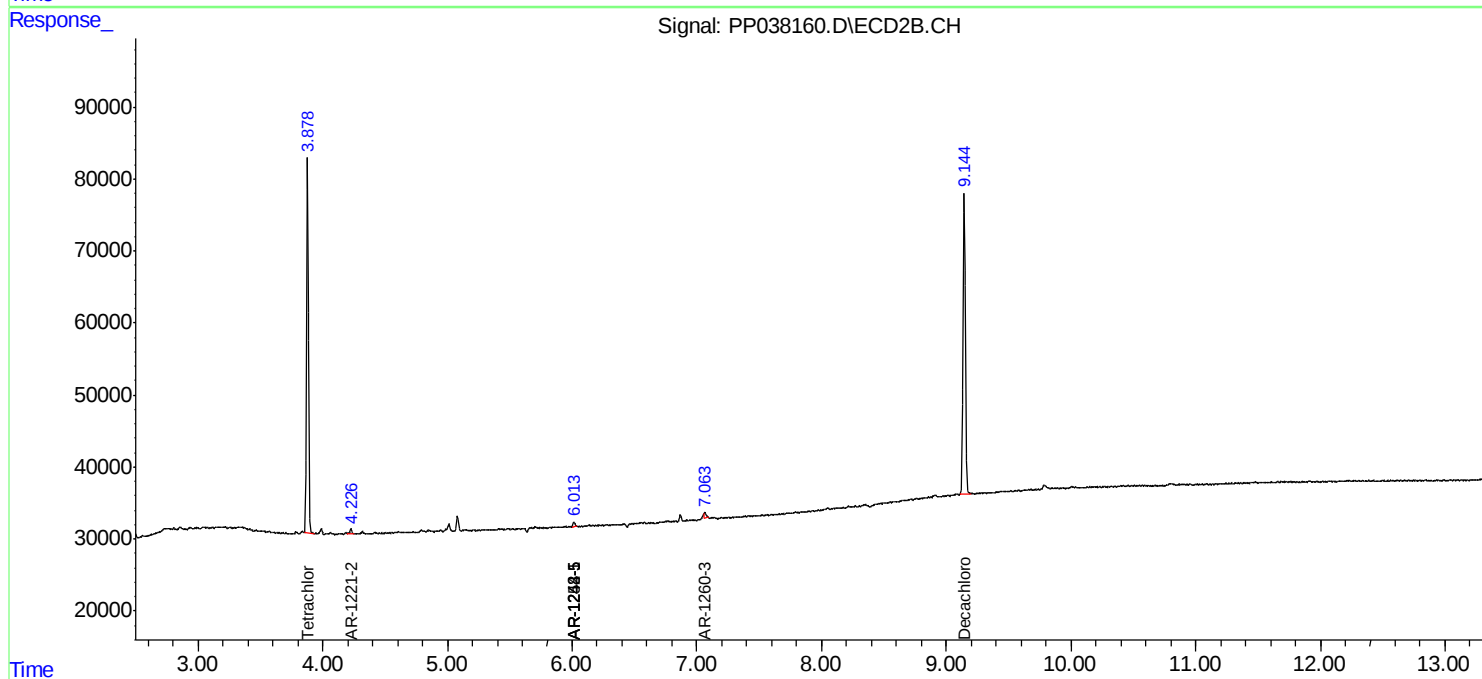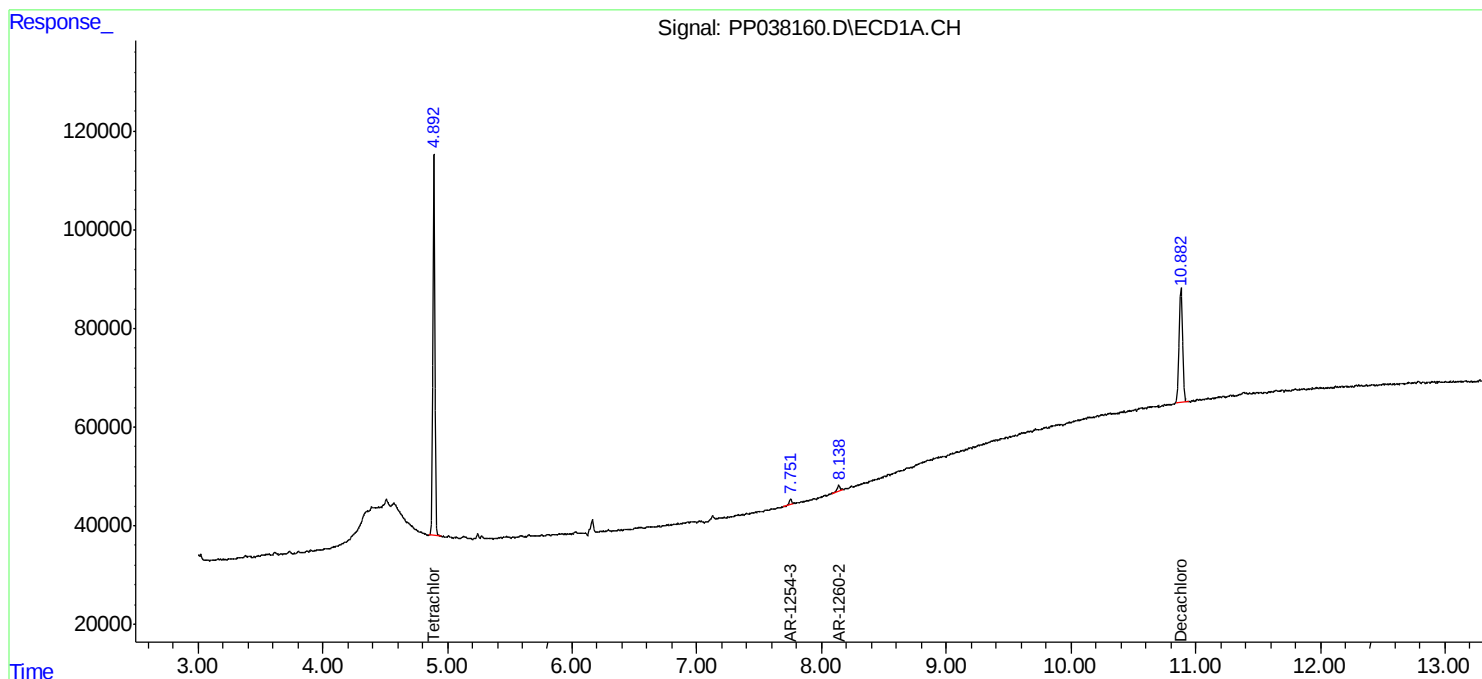


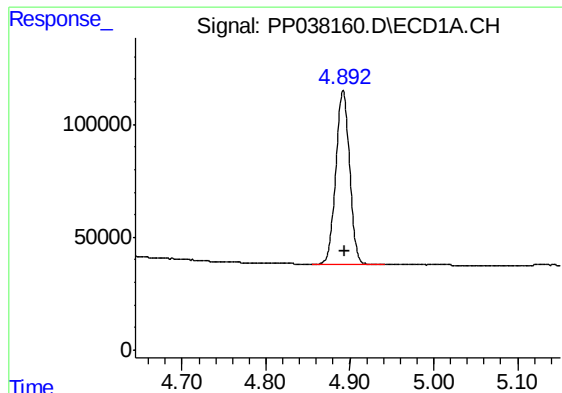

#1 Tetrachloro-m-xylene


R.T.: 4.892 min
Delta R.T.: -0.002 min
Response: 876565
Conc: 19.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

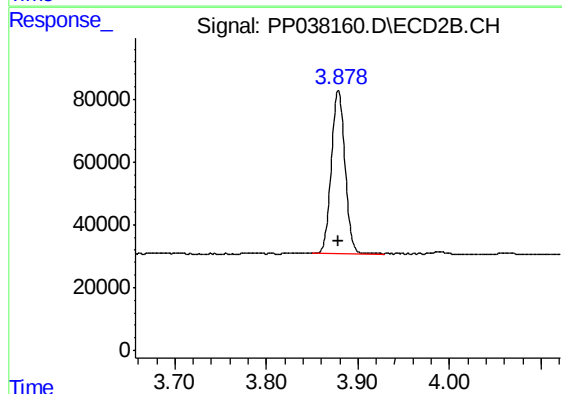


#1 Tetrachloro-m-xylene

R.T.: 3.879 min
Delta R.T.: 0.000 min
Response: 535999
Conc: 20.81 ng/ml

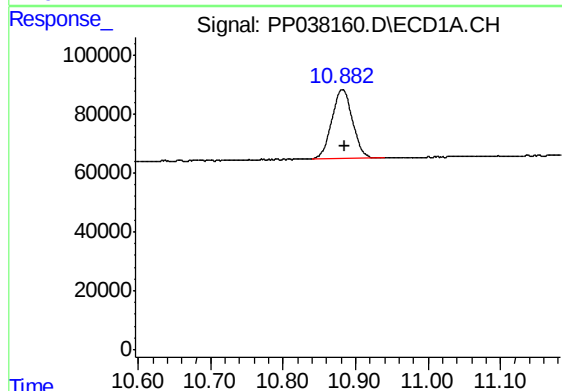


#2 Decachlorobiphenyl

R.T.: 10.882 min
Delta R.T.: -0.004 min
Response: 459862
Conc: 20.22 ng/ml

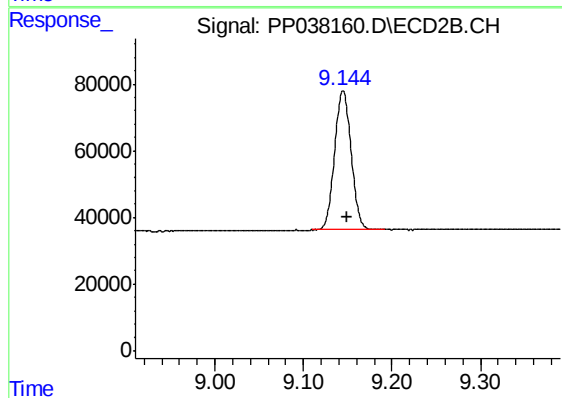

#2 Decachlorobiphenyl


R.T.: 9.145 min
Delta R.T.: -0.004 min
Response: 545917
Conc: 21.10 ng/ml

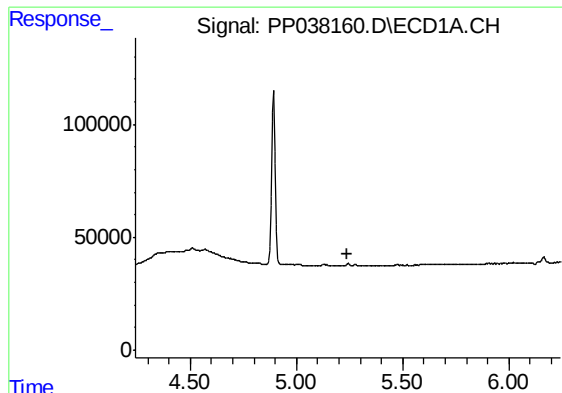

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 5.242 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

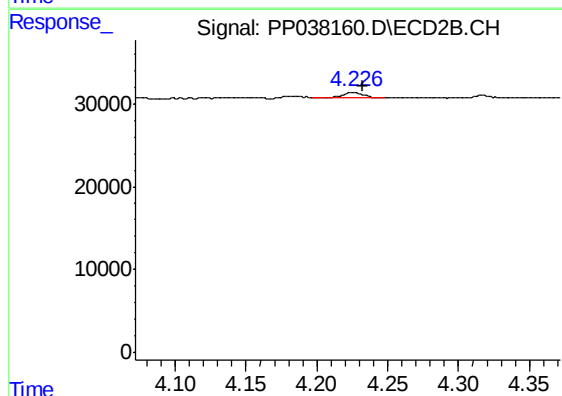


#9 AR-1221-2

R.T.: 4.227 min
Delta R.T.: -0.006 min
Response: 7344
Conc: 31.20 ng/ml

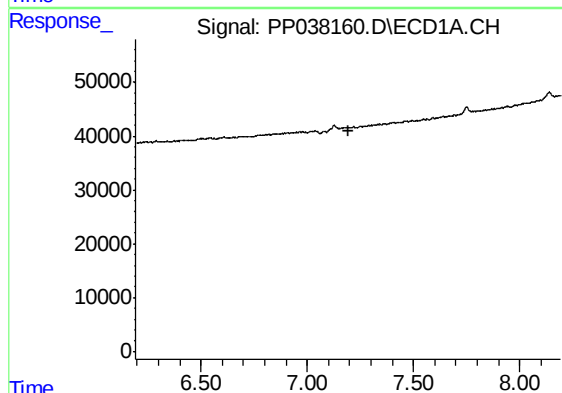


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 7.192 min
Response: 0
Conc: N.D.

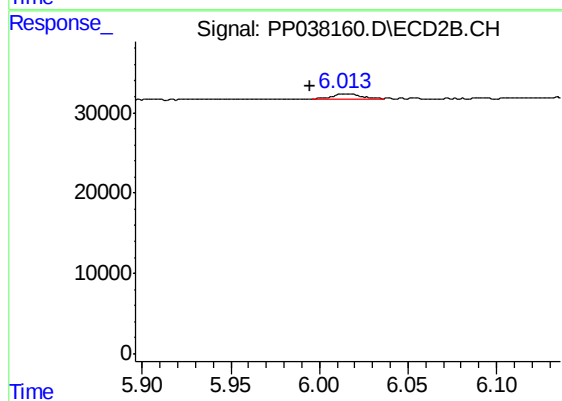

#20 AR-1242-5


R.T.: 6.013 min
Delta R.T.: 0.019 min
Response: 6893
Conc: 10.67 ng/ml

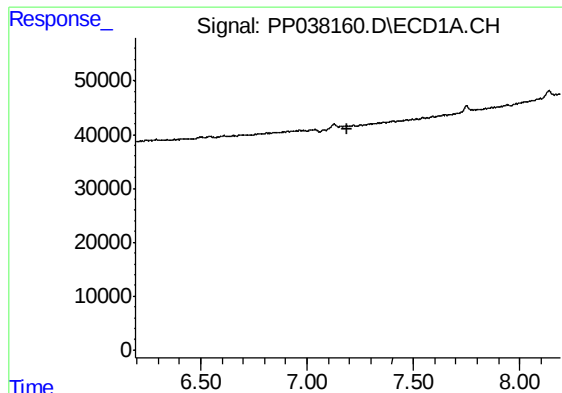

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 7.192 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

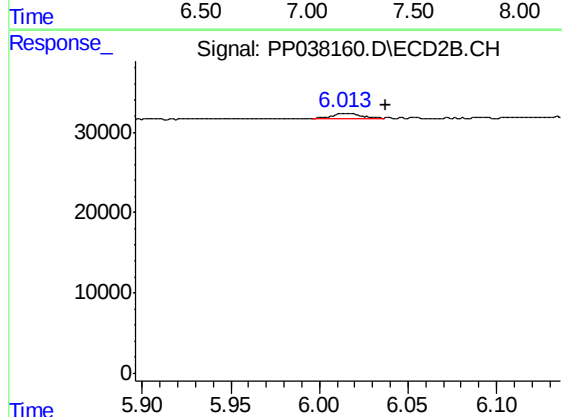


#25 AR-1248-5

R.T.: 6.013 min
Delta R.T.: -0.024 min
Response: 6893
Conc: 7.32 ng/ml

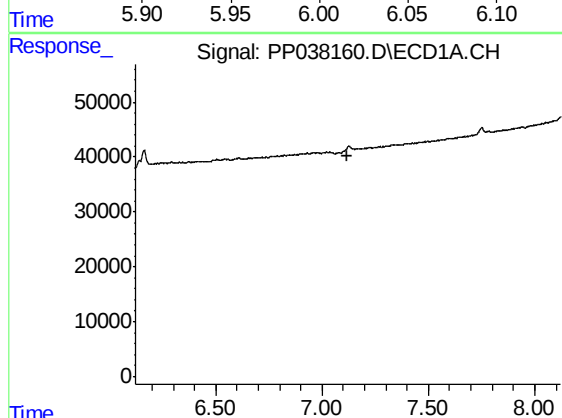


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 7.121 min
Response: 0
Conc: N.D.

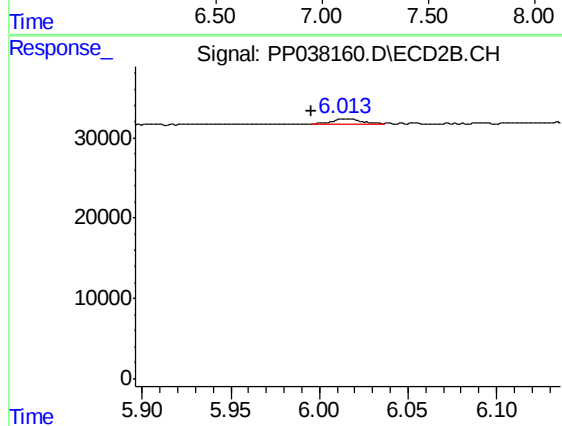

#26 AR-1254-1


R.T.: 6.013 min
Delta R.T.: 0.018 min
Response: 6893
Conc: 5.15 ng/ml

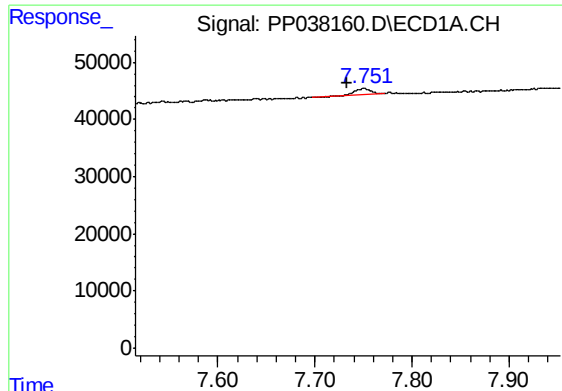

#28 AR-1254-3


R.T.: 7.751 min
Delta R.T.: 0.018 min
Response: 13630
Conc: 6.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

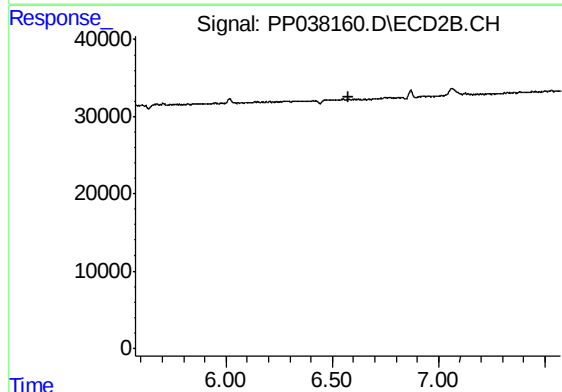


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.573 min
Response: 0
Conc: N.D.

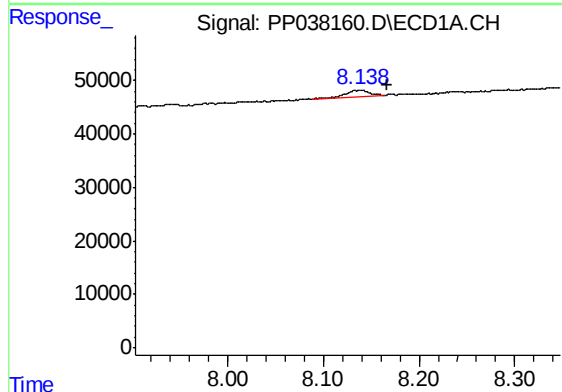


#32 AR-1260-2

R.T.: 8.138 min
Delta R.T.: -0.027 min
Response: 22321
Conc: 12.97 ng/ml

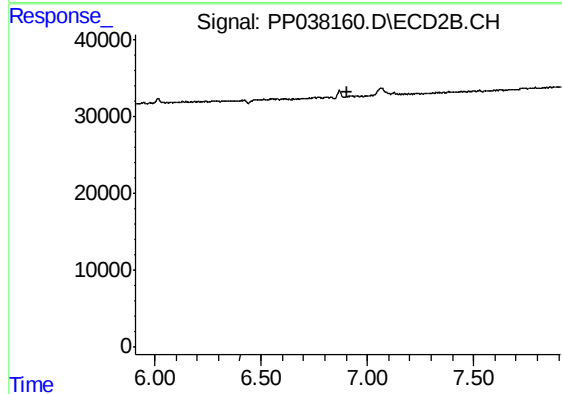

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.909 min
Response: 0
Conc: N.D.

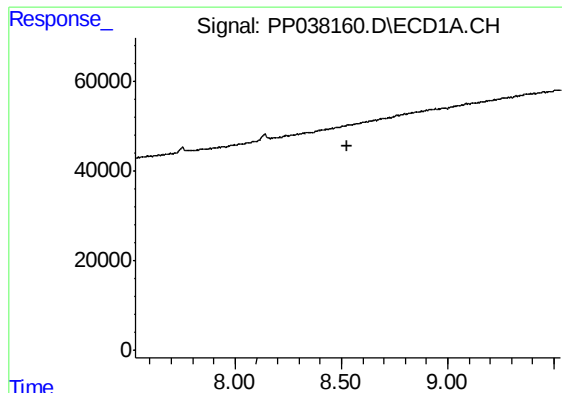

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.530 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

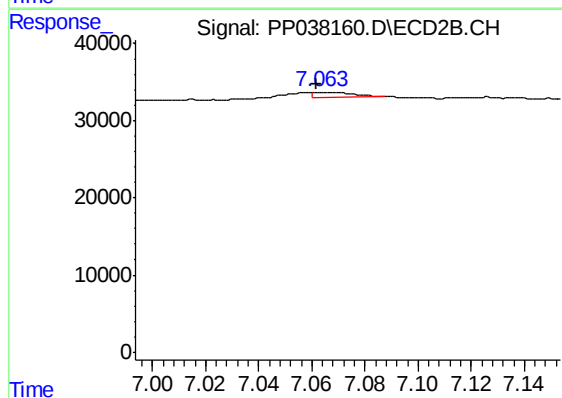

#33 AR-1260-3

R.T.: 7.064 min
Delta R.T.: 0.002 min
Response: 7468
Conc: 4.91 ng/ml