

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080921\
 Data File : PP038164.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Aug 2021 21:01
 Operator : AJ\MA
 Sample : M3321-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CARLSTADT

Manual Integrations
 APPROVED

mohammad
 8/10/2021 4:39:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 01:00:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.892	3.879	889069	563942	20.006	21.896
2) SA Decachlor...	10.880	9.144	399617	436873	17.567	16.885m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080921\
Data File : PP038164.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Aug 2021 21:01
Operator : AJ\MA
Sample : M3321-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CARLSTADT


Manual Integrations
APPROVED

mohammad
8/10/2021 4:39:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 01:00:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

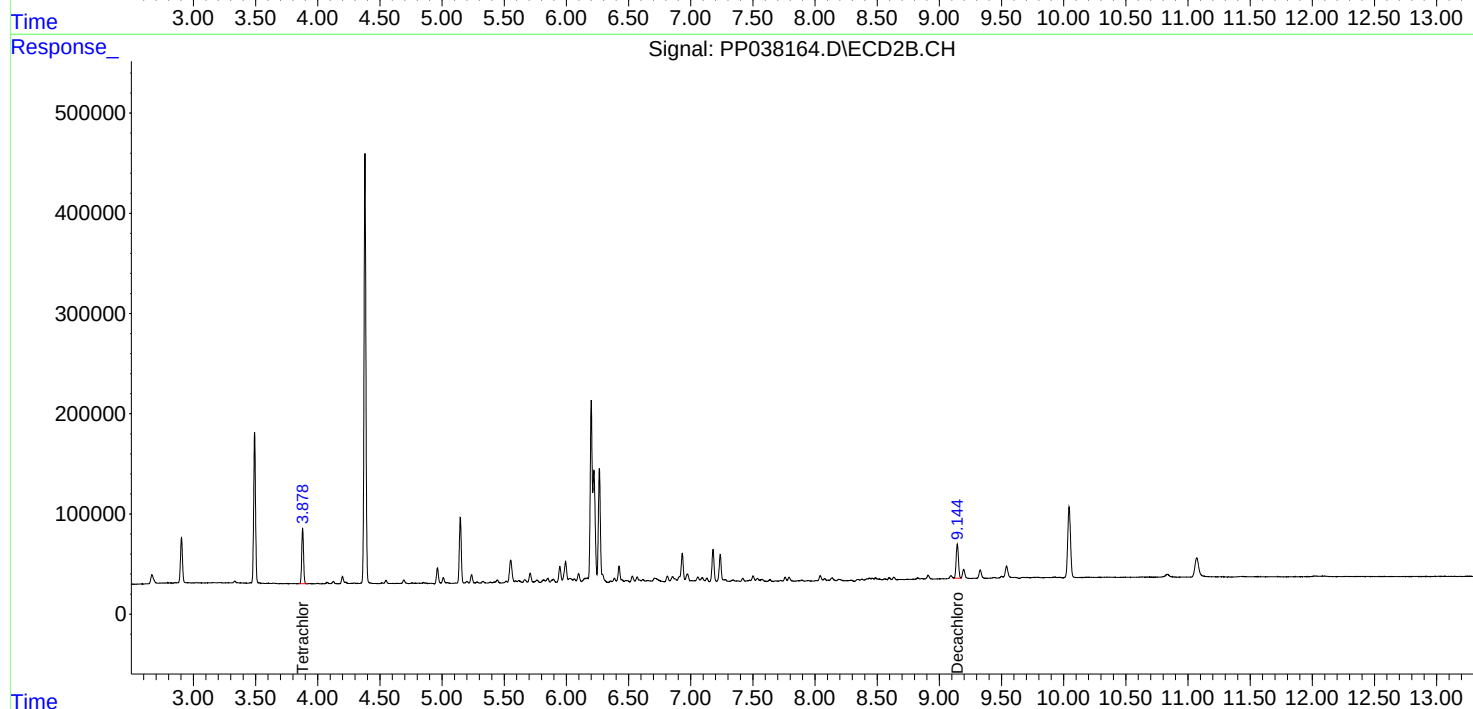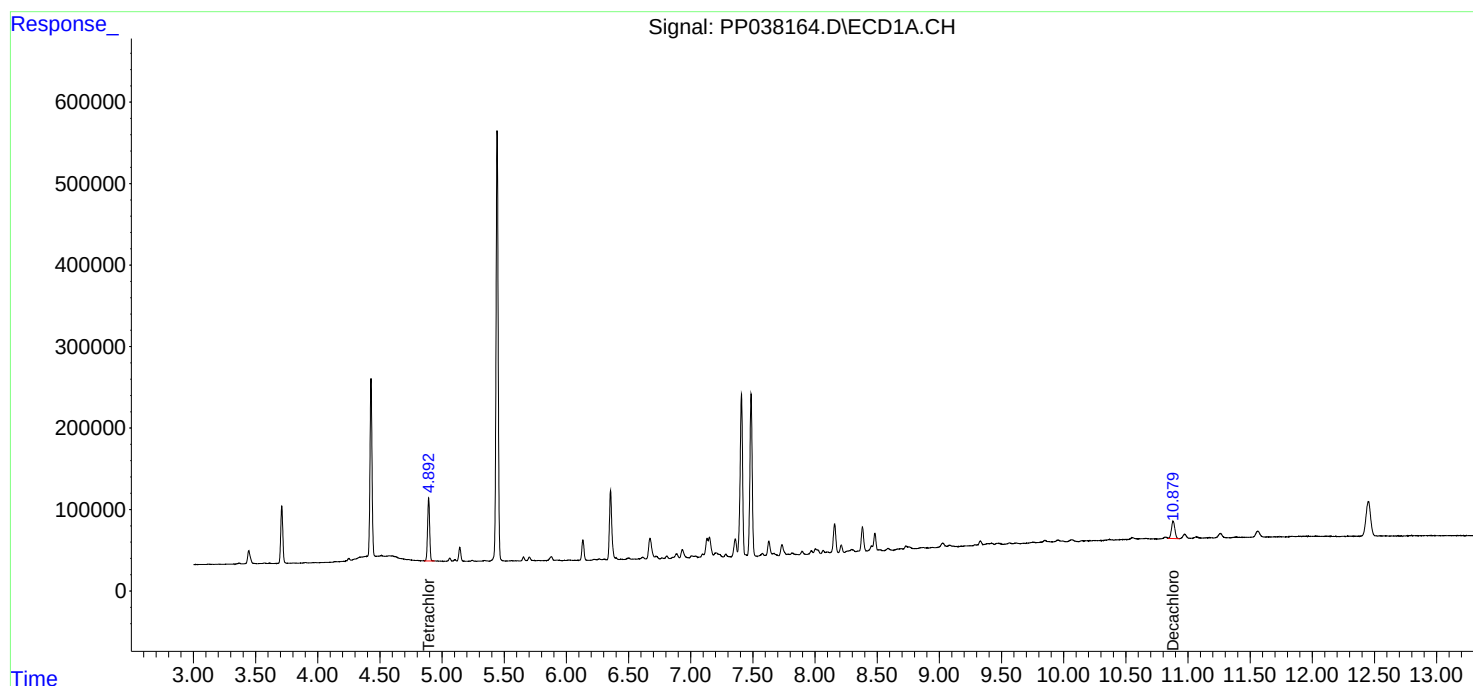

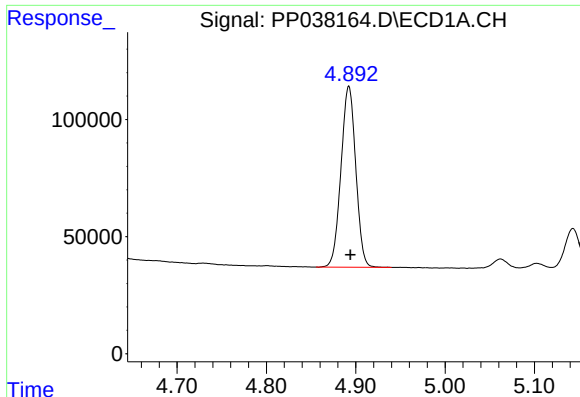


#1 Tetrachloro-m-xylene

R.T.: 4.892 min
Delta R.T.: -0.002 min
Response: 889069
Conc: 20.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
CARLSTADT


Manual Integrations
APPROVED

mohammad
8/10/2021 4:39:03 PM

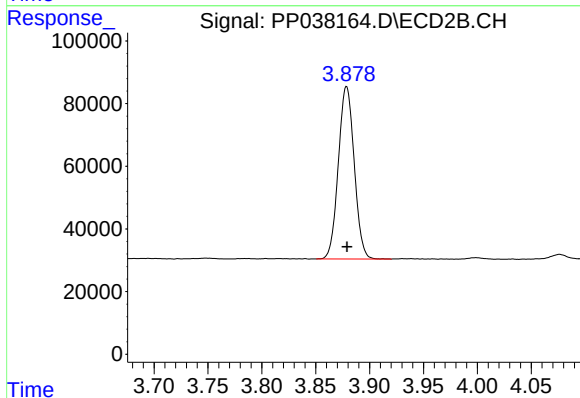


#1 Tetrachloro-m-xylene

R.T.: 3.879 min
Delta R.T.: 0.000 min
Response: 563942
Conc: 21.90 ng/ml

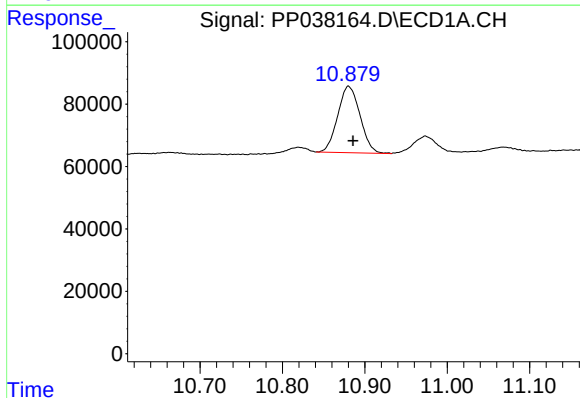

#2 Decachlorobiphenyl

R.T.: 10.880 min
Delta R.T.: -0.006 min
Response: 399617
Conc: 17.57 ng/ml

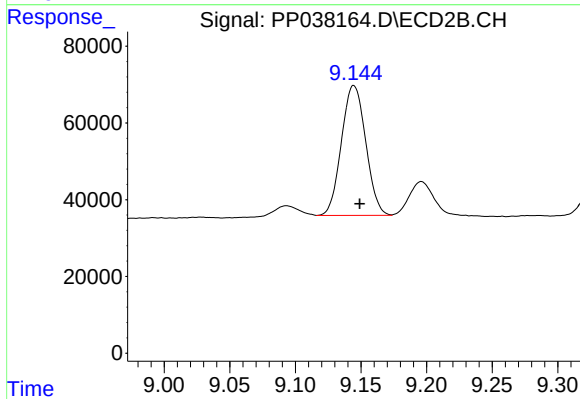

#2 Decachlorobiphenyl

R.T.: 9.144 min
Delta R.T.: -0.005 min
Response: 436873
Conc: 16.89 ng/ml m