

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080921\
 Data File : PP038170.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Aug 2021 22:43
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

mohammad
 8/10/2021 4:39:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 01:04:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.893	3.879	880409	532571	19.811	20.678m
2) SA Decachlor...	10.882	9.146	445068	514131	19.565	19.871

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080921\
Data File : PP038170.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Aug 2021 22:43
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

mohammad
8/10/2021 4:39:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 01:04:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

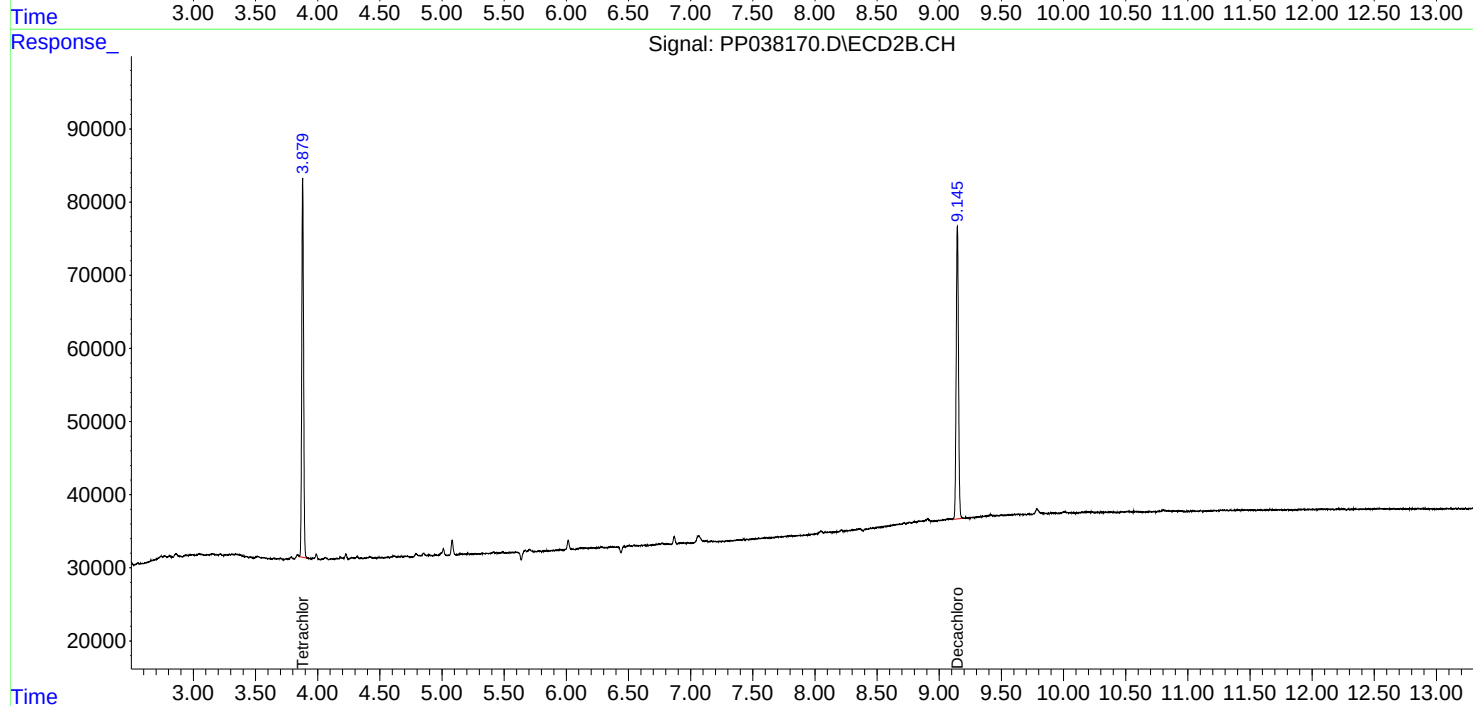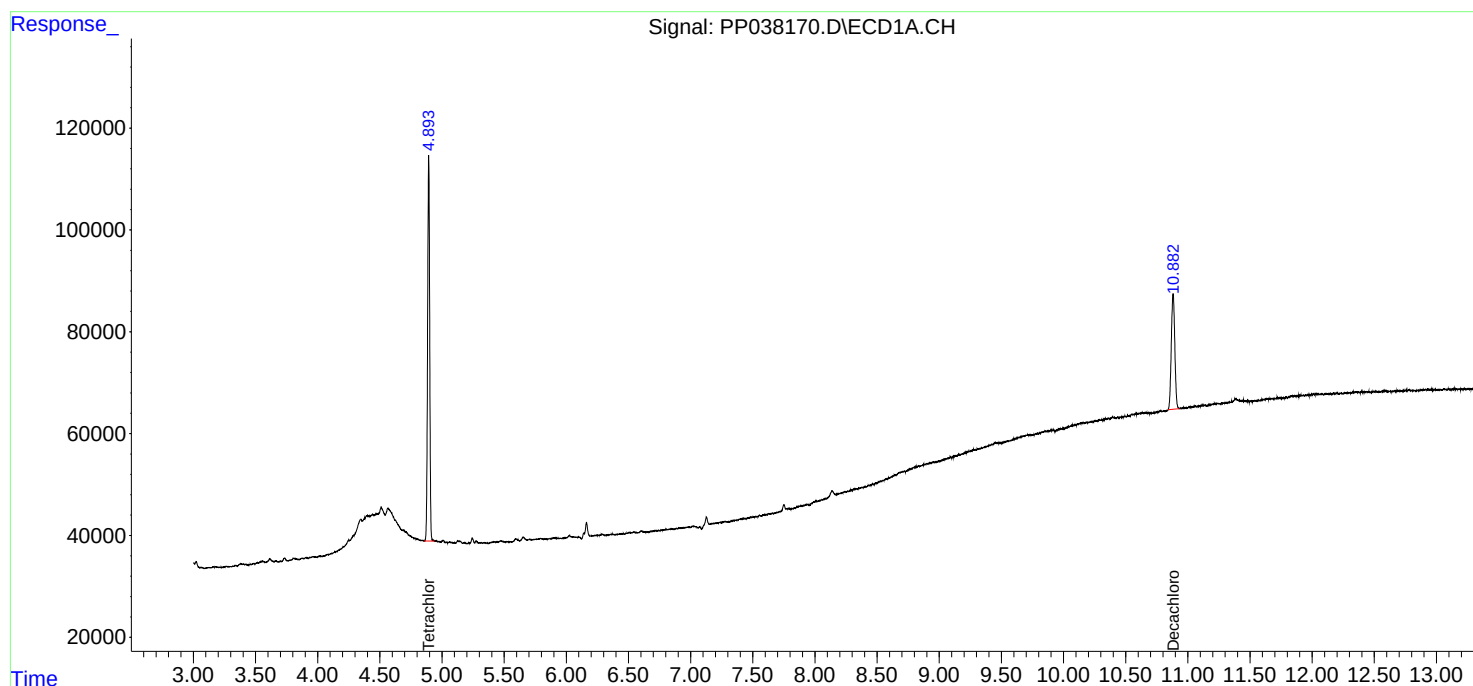

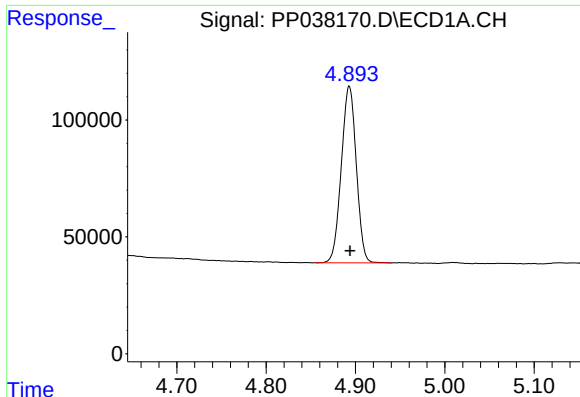


#1 Tetrachloro-m-xylene

R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 880409
Conc: 19.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

mohammad
8/10/2021 4:39:12 PM

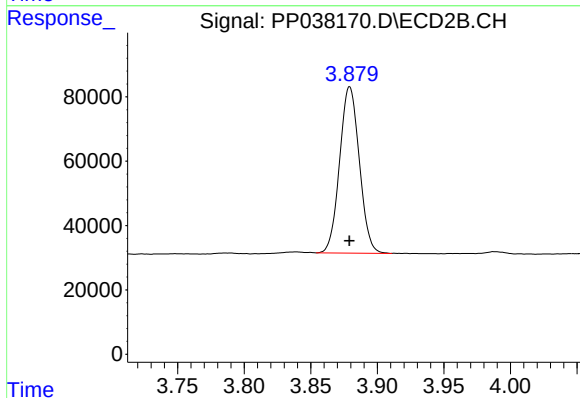


#1 Tetrachloro-m-xylene

R.T.: 3.879 min
Delta R.T.: 0.000 min
Response: 532571
Conc: 20.68 ng/ml m

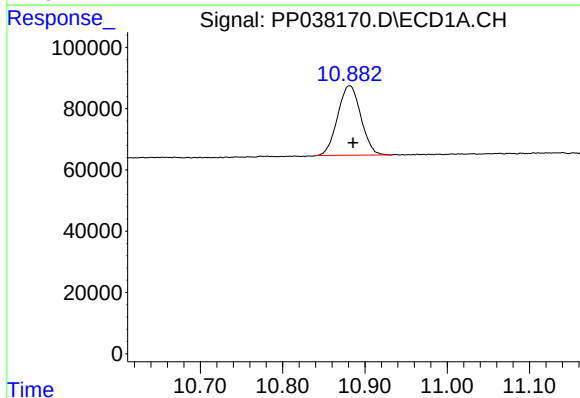

#2 Decachlorobiphenyl

R.T.: 10.882 min
Delta R.T.: -0.004 min
Response: 445068
Conc: 19.56 ng/ml

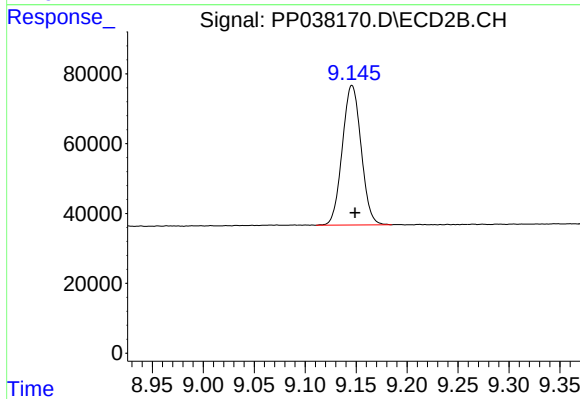

#2 Decachlorobiphenyl

R.T.: 9.146 min
Delta R.T.: -0.003 min
Response: 514131
Conc: 19.87 ng/ml